

InTouch® Critical Care Bed

REF FL27 (2131/2141)

***UPGRADED
2.x - 3 to 3.1***

stryker®

Maintenance Manual



Table of Contents

Symbols and Definitions	9
Warning / Caution / Note Definition.	10
Introduction	11
Intended Use	11
Brief Product Description and Intended Use Statement	11
Introduction	12
Product Illustration	12
Specifications	13
Summary of Safety Precautions	15
Optional Zoom® Drive System (Model 2141 Only)	17
Static Discharge Precautions	18
Setup Procedures.	19
Optional XPRT™ Therapy Mattress	20
Optional PositionPRO™ Repositioning Mattress option	20
Optional Zoom® Drive System (Model 2141 Only).	21
Maintenance Menu Guide	22
Configuration Screen	23
A. Bed Calibration	23
B. Full Diagnostic	34
C. Touch Screen Calibration	35
D. Wi-Fi Calibration	36
E. Bed Options Configuration.	38
F. Serial Number Configuration	39
Preventative Maintenance.	40
Checklist	40
Cleaning.	41
Troubleshooting Guide	43
Scale Troubleshooting	48
Maintenance Error Messages	49
Error Handling	49
Error Messages	49
Quick Reference Replacement Parts List	52
CPU/Power Board - QDF75-0440	54
Fuse Specification	55
Bed Electrical Diagram	56
Service Information.	75

Table of Contents

Service Information (Continued)

Bed lift Actuator (Head) Removal and Replacement - (Base)	75
Bed lift Actuator (Foot) Removal and Replacement - (Base)	76
Fowler Actuator Removal and Replacement - (Litter)	77
Gatch Actuator Removal and Replacement - (Litter)	78
Foot Actuator Removal and Replacement - (Litter)	79
Zoom® Drive Actuator Removal and Replacement (2141 Model Only) - (Base)	80
CPU / Power Board Removal and Replacement - (Litter)	81
Load Cell (Head End) Removal and Replacement - (Litter)	82
Load Cell (Foot End) Removal and Replacement - (Litter)	83
Display Removal and Replacement - (Footboard)	84
Brake Control Board Removal and Replacement - (Footboard)	85
Function Selection/LED Board Removal and Replacement - (Footboard)	86
Touch Screen Removal and Replacement - (Footboard)	87
Battery Removal and Replacement - (Footboard)	88
Brake / Neutral / Drive Potentiometer Removal and Replacement - QDF27-2024	89
Battery Removal and Replacement - (Litter)	90
Fowler Angle Sensor Removal and Replacement - (Litter)	91
Gatch Angle Sensor Removal and Replacement - (Litter)	92
Foot Angle Sensor Removal and Replacement - (Litter)	93
Base Angle Sensor Removal and Replacement - (Base)	94
Trend Angle Sensor Removal and Replacement - (Litter)	95
Headwall Communication Board Removal and Replacement - (Litter)	96
IR Module Removal and Replacement - (Litter) (Optional)	97
Wi-Fi Board Removal and Replacement - (Footboard) (Optional)	98
Base Assembly, Hood (Applies to beds with Serial Numbers U01001 - U51437)	100
Base Assembly, Hood (Applies to beds with Serial Numbers U51438 - Current)	102
Base Assembly, Brake (Applies to beds with Serial Numbers U01001 - U02817)	104
Base Assembly, Brake (Applies to beds with Serial Numbers U02818 - Current)	107
Base Assembly, Caster Lock (Model 2131 Only) (Applies to beds with Serial Numbers U01001 - U51437)	110
Base Assembly, Caster Non-Lock (Model 2141 Only) (Applies to beds with Serial Numbers U01001 - U51437)	111
Base Assembly, Caster Lock (Model 2131 Only) (Applies to beds with Serial Numbers U51438 - Current)	112
Base Assembly, Caster Non-Lock (Model 2141 Only) (Applies to beds with Serial Numbers U51438 - Current)	113
Angle Sensor Assembly	114
Base Assembly, Electrical	115

Table of Contents

Assembly Drawings (Continued)	
Base Assembly, Zoom® (Applies to beds with Serial Numbers U03319 - Current)	
(Including U03258 and U03259)	121
Base Assembly, Zoom® Drive (Model 2141 Only) (Applies to beds with Serial Numbers U01001 - U03318)	
(Excluding U03258 and U03259).	123
Base Assembly, Zoom® Drive (Model 2141 Only)	125
Bed Labeling	127
Lift Assembly (Applies to beds with Serial Numbers U01001 - U02817).	131
Lift Assembly (Applies to beds with Serial Numbers U02818 - Current).	135
Spring Assembly.	139
Litter Assembly (Applies to beds with Serial Numbers U01001 - U02817)	140
Litter Assembly (Applies to beds with Serial Numbers U02818 - U04982)	144
Litter Assembly (Applies to beds with Serial Numbers U04983 - U50240).	148
Litter Assembly (Applies to beds with Serial Numbers U50241 - Current)	152
Litter Assembly, Interior Frame	156
Litter Assembly with Serial Port.	159
Litter Assembly, Upper Frame (Applies to beds with Serial Numbers U01001 - U02817)	160
Litter Assembly, Upper Frame (Applies to beds with Serial Numbers U02818 - Current).	162
Litter Assembly, Foot End (Applies to beds with Serial Numbers U01001 - U02817).	164
Litter Assembly, Foot End (Applies to beds with Serial Numbers U02818 - U04982)	168
Litter Assembly, Foot End (Applies to beds with Serial Numbers U04983 - U50240)	172
Litter Assembly, Foot End (Applies to beds with Serial Numbers U50241 - Current).	176
Litter Assembly, Standard Cabling (Applies to beds with Serial Numbers U01001 - U03318)	
(Excluding U03258 and U03259).	180
Litter Assembly, Standard Cabling (Applies to beds with Serial Numbers U03319 - U04982)	
(Including U03258 and U03259)	181
Litter Assembly, Standard Cabling (Applies to beds with Serial Numbers U04983 - Current)	182
Litter Assembly, Electrical (Applies to beds with Serial Numbers U01001 - U03318)	
(Excluding U03258 and U03259).	183
Litter Assembly, Electrical (Applies to beds with Serial Numbers U03319 - U04982)	
(Including U03258 and U03259)	189
Litter Assembly, Electrical (Applies to beds with Serial Numbers U04983 - U50240)	195
Litter Assembly, Electrical (Applies to beds with Serial Numbers U50241 - Current)	201
120V Electric System	207
Coiled Power Cord (Applies to beds with Serial Numbers U51438 - Current).	208

Table of Contents

Assembly Drawings (Continued)	
120V Straight Plug (Applies to beds with Serial Numbers U01001 - U51437)	209
Optional 120V 90 Degree Plug	210
Litter Assembly, Foot End, without Mattress Connector	211
Litter Assembly, Foot End, with Mattress Connector	212
Standard Outlet	213
Litter Assembly, Optional Dual 120V Outlet	214
Optional 100V Electric System	216
Optional 110V Electric System	217
Optional 200V Electric System	218
Optional 220V Electric System	219
Optional 240V Electric System	220
CPR Assembly, Mechanical	221
Handle Assembly (Model 2131 Only) (Applies to beds with Serial Numbers U01001 - U51437)	226
Handle Assembly (Model 2131 Only) (Applies to beds with Serial Numbers U51438 - Current)	227
Zoom® Handle Assembly (Model 2141 Only) (Applies to beds with Serial Numbers U01001 - U04982) (Excluding U03258 and U03259)	228
Zoom® Handle Assembly (Model 2141 Only) (Applies to beds with Serial Numbers U04983 - U51437) (Including U03258 and U03259)	230
Zoom® Handle Assembly (Model 2141 Only) (Applies to beds with Serial Numbers U51438 - Current)	232
Zoom® Assembly (Applies to beds with Serial Numbers U01001 - U51437)	234
Zoom® Assembly (Applies to beds with Serial Numbers U51438 - Current)	235
Optional No Head End Control Panel	236
Optional Head End Control Panel Assembly	237
Siderail Mounting Assembly, Head End (Applies to beds with Serial Numbers U01001 - U02817)	239
Siderail Mounting Assembly, Head End (Applies to beds with Serial Numbers U02818 - Current)	240
Standard Siderail Assembly, Head End, Right (Applies to beds with Serial Numbers U01001 - U02817)	241
Standard Siderail Assembly, Head End, Right (Applies to beds with Serial Numbers U02818 - Current)	245
Standard Siderail Assembly, Head End, Left (Applies to beds with Serial Numbers U01001 - U02817)	249
Standard Siderail Assembly, Head End, Left (Applies to beds with Serial Numbers U02818 - Current)	253
Standard Siderail Assembly, Labeling	257
Optional Siderail Assembly, Head End, without Speaker/without NC	258
Optional Siderail Assembly, Head End, with Speaker/without NC	259
Optional Siderail Assembly, Head End, with Speaker/iAudio	260
Optional Siderail Assembly, Head End, with Speaker/with NC	261














Table of Contents

Optional Siderail Assembly, Head End, with <i>i</i> Audio - OL270164	262
Optional Siderail Assembly, Head End, with Speaker/with NC/with <i>i</i> Audio	263
Optional Siderail Assembly, Head End, with Speaker/with NC/with <i>i</i> Audio/with <i>i</i> Bed® Wireless.	265
Siderail Mounting Assembly, Foot End (Applies to beds with Serial Numbers U01001 - U02817)	269
Siderail Mounting Assembly, Foot End (Applies to beds with Serial Numbers U02818 - Current)	270
Standard Siderail Assembly, Foot End, Right (Applies to beds with Serial Numbers U01001 - U02817).	271
Standard Siderail Assembly, Foot End, Right (Applies to beds with Serial Numbers U02818 - Current).	274
Standard Siderail Assembly, Foot End, Left (Applies to beds with Serial Numbers U01001 - U02817)	277
Standard Siderail Assembly, Foot End, Left (Applies to beds with Serial Numbers U02818 - Current).	280
Standard Siderail Assembly without <i>i</i> Bed.	283
Optional Siderail Assembly with <i>i</i> Bed	284
Headboard and Footboard Assembly.	285
Standard Footboard Assembly	286
Footboard Assembly with <i>i</i> Bed and WI-FI.	288
Optional Bed Accessories.	291
Bed Extender - FA64234-XXX.	292
Bed Extender Pad with Position Pro Mattress - DM64196.	293
Bed Extender Pad with XPRT™ Mattress - DM64197	293
Line Management System Assembly - FA64210-XXX	294
I.V. Pole Assembly, Permanent - FA64221-XXX/FA64238-XXX	295
I.V. Pole Ass'y, Dual Head End, Permanent - FA64202-XXX	296
Monitor Tray Assembly - FA64214-XXX	298
Upright Oxygen Bottle Holder Assembly - FA64187-XXX.	299
Right-Fit Oxygen Bottle Holder Assembly - FA64203	300
Pendant Assembly with Motion Control - FA64228-XXX	301
Pendant Assembly with Motion Control/NC - FA64226	302
Pendant Assembly with Motion Control/Smart TV - FA64227.	303
Pendant Assembly with Motion Control/NC/Smart TV - FA64225.	304
Pendant Clip Assembly - FA64186-XXX	304
Roller Bumpers.	305
Traction Sleeve Assembly, 4" x 1/2" - FA64215-XXX	306
Traction Sleeve Assembly, 4" x 3/4" - FA64216-XXX	307
Traction Sleeve Assembly, 8" x 1/2" - FA64217-XXX	308
Traction Sleeve Assembly, 8" x 3/4" - FA64218-XXX	309
Traction Sleeve Assembly, 6-1/2" x 3/4" - FA64219-XXX	310





Table of Contents

Wall Saver Cable Assembly - FA64208	311
X-Ray Cassette Holder Assembly - FA64205-XXX	312
Standard Mattress Retainer	314
Tube Support	315
Recycling Passports	316
Warranty	332
Limited Warranty	332
To Obtain Parts and Service	332
Service Contract Coverage	332
Return Authorization.	333
Damaged Merchandise	333
International Warranty Clause.	333

Symbols and Definitions

	Warning, consult accompanying documentation
	Safe Working Load Symbol
~	Alternating Current
	Dangerous Voltage Symbol
	Fuse Rating for Beds with the 100V~ or 120V~ Electric System
	Fuse Rating for Beds with the 200V~ or 220V~ or 240V~ Electric System
	Protective Earth Terminal
	Potential Equalization
	Type B Applied Part
IPX4	Protection from liquid splash
	Medical Equipment approved by the Canadian Standards Association with Respect to Electric Shock, Fire, Mechanical and Other Specified Hazards.
	In accordance with European Directive 2002/96/EC on Waste Electrical and Electronic Equipment, this symbol indicates that the product must not be disposed of as unsorted municipal waste, but should be collected separately. Refer to your local distributor for return and/or collection systems available in your country.
	Model Number
	Manufacturer
	Non-ionizing radiation; i.e. RF transmitter (WiFi)

Symbols and Definitions

	This icon means the iBed Locator is connected.
	This icon means the iBed Locator is not connected.
	This icon means the Network is connected.
	This icon means the Network is not connected.

WARNING / CAUTION / NOTE DEFINITION

The words WARNING, CAUTION, and NOTE carry special meanings and should be carefully reviewed.

WARNING

Alerts the reader about a situation, which if not avoided, could result in death or serious injury. It may also describe potential serious adverse reactions and safety hazards.

CAUTION

Alerts the reader of a potentially hazardous situation, which if not avoided, may result in minor or moderate injury to the user or patient or damage to the equipment or other property. This includes special care necessary for the safe and effective use of the device and the care necessary to avoid damage to a device that may occur as a result of use or misuse.

Note

This provides special information to make maintenance easier or important instructions clearer.

Introduction

INTENDED USE

This manual is designed to assist you with the maintenance of the Stryker *InTouch*® Critical Care Bed, Model FL27 (2131/2141). Carefully read this manual thoroughly before using the equipment or beginning maintenance on it. To ensure safe operation of this equipment, it is recommended that methods and procedures be established for educating and training staff on the safe operation of this bed.

This Maintenance Manual is an integral part of the bed and should be included if the bed is sold or transferred.

BRIEF PRODUCT DESCRIPTION AND INTENDED USE STATEMENT

INTENDED MEDICAL INDICATIONS: InTouch is an AC-powered adjustable hospital bed designed to position patients for procedures, therapy, and recovery in healthcare environment, transport patients between bays and procedural rooms, provide patient security, measure and display patient weight, allow patients to alert caregiver when the patient requires emergency assistance or any assistance to improve comfort levels, and monitor patient position to alert caregiver of a deliberate exit or potential fall. The bed has thirty-nine prerecorded clinical phrases in 24 languages and offers music therapy.

INTENDED PATIENT POPULATION: The intended patient population is acute-care human patients. The safe working load (i.e. the sum of the patient, the mattress, and accessory weight) for InTouch is 550 lbs (249 kg). This bed is not intended for use with patients 35 inches or less and/or patients that weigh less than 50 pounds.

INTENDED PART OF THE BODY: InTouch is intended to support a patient. It is intended to be used with a sleep surface. The Frame can come in contact with human skin but a patient should never be on the frame without a support surface.


INTENDED USER PROFILE: InTouch is intended for use in Acute Care settings. These settings may include critical care, step down, progressive care, med/surg, sub-acute care, and post anesthesia care unit (PACU) or other locations as prescribed. Intended operators are health care professionals (nurses, nurse aids, doctors) which can use all bed operations (e.g., bed motion functions, nurse call, siderail communications, bed exit, therapy options), patient and bystander, which can use bed motion functions, nurse call & siderail communications, and trained professionals for installation, service, and calibration.

INTENDED CONDITION OF USE AND EXPECTED LIFE: Stryker Medical Bed products are designed for a 10 year expected service life under normal use, conditions, and with appropriate periodic maintenance as described in the maintenance manual for each device. Stryker warrants to the original purchaser that the welds on its Bed products will be free from structural defects for the expected 10 year life of the Bed product as long as the original purchaser owns the products.

The product is intended to be used in a healthcare environment, including hospitals, surgery centers, long term acute care centers, and rehabilitation centers. The intended environmental conditions are 10 to 40 degrees Celsius and 30 to 75% RH. The product is compatible with 35" x 84" surfaces, the facility nurse call system, standard Med-Surg equipment, and the facility infrastructure. InTouch is intended to be used with a 6"-8.5" sleep surface. A sleep surface or overlay greater than 6" that offers therapeutic value may be used with patient supervision.


Introduction

PRODUCT ILLUSTRATION

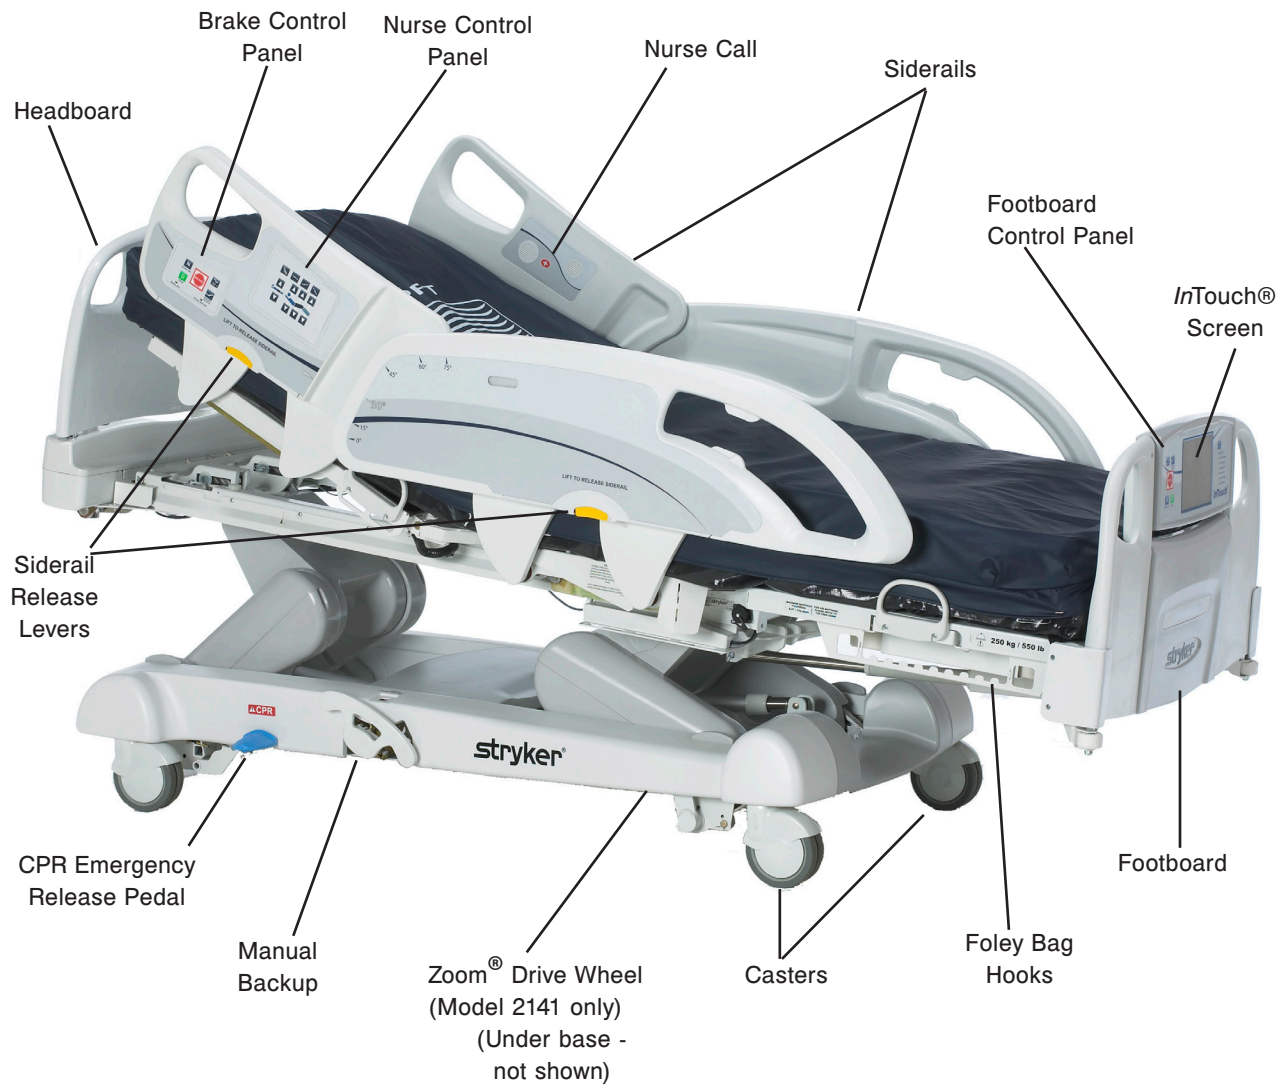

Introduction

SPECIFICATIONS

	Safe Working Load		
	Note: Safe Working Load indicates the sum of the patient, mattress and accessory weight.		
Bed Weight		550 lbs	249 kg
Overall Bed Length		750 lbs	340.2 kg
Overall Bed Width		90"	228,6 cm
Overall Bed Width	Siderails Up	42"	106,7 cm
	Siderails Down	40"	102,9 cm
Base	Underbed Clearance	5"	12,7 cm
Litter	Patient Surface <ul style="list-style-type: none"> Width Length Length (with Optional Bed Extender) 	35" 84" 90"	88,9 cm 213,4 cm 228,6 cm
	Seat Section <ul style="list-style-type: none"> Depth 	18.5"	47 cm
	Foot Section <ul style="list-style-type: none"> Length Angle 	29" 0° to 50°	73,7 cm 0° to 50°
	Fowler Section <ul style="list-style-type: none"> Length Width Angle 	36" 34" to 35" 0° to 70°	91,4 cm 86,4 cm - 88,9 cm 0° to 70°
	Gatch Section <ul style="list-style-type: none"> Length Width Angle 	18" 34" to 35" 0° to 15°	45,7 cm 86,4 cm - 88,9 cm 0° to 15°
	Cardiac Chair <ul style="list-style-type: none"> Standard Cardiac Chair Position Enhanced Cardiac Chair Position 	Head: 65°, Seat: 17°, Foot: 30°, Trend: 3° Head: 70°, Seat: 19°, Foot: 47°, Trend: 3°	
Fowler	Length	36.5"	92,7 cm
Bed Lift System	Height (high) to top of litter	33"	83,8 cm
	Height (low) to top of litter	16"	40,6 cm
	Trendelenburg/Reverse Trendelenburg	12°	
	Bed Lift Time	35 seconds maximum from lowest to highest position	
Scale System	Capacity	550 lbs	249 kg
	Accuracy: <ul style="list-style-type: none"> For weight from 100 lb to 550 lb For weight from 100 lb to 550 lb For weight under 100 lb For weight under 100 lb 	+/- 2% when in Trendelenburg or Reverse Trendelenburg +/- 2% when Flat +/- 2 lb when in Trendelenburg or Reverse Trendelenburg +/- 2 lb when Flat	
CPR System	Speed to level bed from any position <ul style="list-style-type: none"> Fowler Foot and Seat 	15 seconds 60 seconds	
Drive System	Speed (Optional Zoom® Drive)		
	<ul style="list-style-type: none"> Forward Backwards 	3.6 mph 2.5 mph	5.8 km/h 4.0 km/h

Introduction

SPECIFICATIONS (CONTINUED)

Mattress	Recommended Mattress Size • With Bed Extender DM64196 (PositionPRO) (35" x 6" x 4") • With Bed Extender DM64197 (XPRT™) (35" x 6" x 5.5")	35" x 84" x 6"	88,9 cm x 213,4 cm x 15,2 cm	
		35" x 90" x 4"	88,9 cm x 228,6 cm x 10,1 cm	
		35" x 90" x 5.5"	88,9 cm x 228,6 cm x 13,9 cm	
	Recommended Air Mattress Size • With Bed Extender DM64196 (PositionPRO) (35" x 6" x 4") • With Bed Extender DM64197 (XPRT™) (35" x 6" x 5.5")	35" x 84" x 6" - 8.5"	88,9 cm x 213,4 cm x 15,2 cm - 21,6 cm	
		35" x 90" x 4"	88,9 cm x 228,6 cm x 10,1 cm	
		35" x 90" x 5.5"	88,9 cm x 228,6 cm x 13,9 cm	
Maximum Current Consumption	Without Optional Auxiliary Outlet (120VAC Only)	4.8 Amps		
	With Optional Auxiliary Outlet(s) (120VAC Only)	9.8 Amps		
Environmental Conditions	Storage • Ambient Temperature • Relative Humidity • Atmospheric Pressure	-40°F to 158°F 10 to 100% 500 to 1060 hPa	-40°C to 70°C	
	Operating • Ambient Temperature • Relative Humidity • Atmospheric Pressure • Scale Accuracy	50°F to 104°F 30 to 75% 700 to 1060 hPa 64 °F to 77 °F	10°C to 40°C 18 °C to 25 °C	
Electrical Requirements	All electrical requirements meet CSA C22.2 No. 601.1, UL 60601-1 and IEC 60601-1.60601-2-38 specifications.	100V~, 50-60Hz, 7.5A - Two 250V, 10A Fuses 120 ± 10% Vac, 50/60Hz - Two 250V, 10A Fuses 120V~, 50-60Hz, 4.0A (9.8A with 120V Optional Auxiliary Outlet) - Two 250V, 10A Fuses 200V~, 50-60Hz, 3.2A -Two 250V, 10A Fuses 220V~, 50-60Hz, 2.9A -Two 250V, 10A Fuses 240V~, 50-60Hz, 2.7A -Two 250V, 10A Fuses		
Wireless Radio (iBed® Wireless Option)	802.11 b/g, 2.4 GHz • Minimum Operational Signal Strength: -65 dB • Supported Securities: WEP WPA-PSK (TKIP) WPA2-PSK (CCMP/AES) • Supports IPv4 and DHCPv4 802.1x • MS-CHAPv2			
Battery	12 V, 17.6 Ahr, Sealed Lead-Acid Battery (Part Number QDF9188) 3.0 V 220mAh Lithium Battery, Size 20mm - Varta Int. CR2032 Coin Cell PC Battery Holder, Size 20mm - MDP Int. BA2032			

Stryker reserves the right to change specifications without notice.

Specifications listed are approximate and may vary slightly from unit to unit or by power supply fluctuations.

Summary of Safety Precautions

Before operating the bed, it is important to read and understand all information in this manual. Carefully read and strictly follow the safety guidelines listed below.

Note

To ensure safe operations of the bed, methods and procedures must be established for educating and training hospital staff on the intrinsic risks associated with the usage of electric beds.

WARNING

- To prevent permanent damage to this unit, the unit must reach room temperature prior to conducting any setup and/or unit operations.
- The Weigh system is intended to assist in the monitoring of the patient's weight variation. Under no circumstances should its reading be used as sole reference for medical treatment.
- Preventative maintenance should be performed at least once a year to ensure all bed features are functioning properly.
- This bed is not intended for pediatric use, i.e., for any patient measuring 35 inches (88,9 cm) or less.
- This bed is equipped with a hospital grade plug for protection against shock hazard. It must be plugged directly into a properly grounded receptacle. Grounding reliability can be achieved only when a hospital grade receptacle is used.
- Shock Hazard - Improper handling of the power cord may result in damage to the power cord and potential shock hazards. If damage has occurred to the power cord, immediately remove the bed from service and contact the appropriate maintenance personnel. Failure to do so could result in serious injury or death.
- Serious injury can result if caution is not used when operating the bed. Operate the bed only when all people and equipment are clear of the electrical and mechanical systems.
- Always apply the brakes when a patient is on the bed or entering/exiting the bed. Serious injury could result if the bed moves while a patient is getting on or off the bed. Once the brake pedal is engaged, push on the bed to ensure the brakes are securely applied. Do the same test when using the electrical brake.
- To help reduce the number and severity of a potential fall when the patient is unattended, keep the siderails in the fully raised position and the sleep surface horizontal in its lowest position, unless his/her medical condition dictates otherwise. When raising the siderails, be sure that you hear the "click" that signals the locked condition. Pull firmly on the siderail to ensure it is locked into position.
- When the sleep surface sections are articulated, ensure that all the patient's limbs are within the raised siderails to avoid patient injury.
- When a patient's condition requires greater safety measures for his/her security, use the lockout controls in the footboard control panel to inhibit the siderail functions or remove any optional pendant control and install protective pads on the siderails.
- Siderails, with or without their padded covers, are not intended to serve as restraint devices to keep a patient from exiting the bed. Siderails are designed to keep a patient from inadvertently rolling off the bed. It is the responsibility of the attending medical personnel to determine the degree of restraint necessary to ensure a patient will remain safely in bed. Failure to use the siderails properly could result in serious patient injury.
- To reduce the risk of injury, ensure the sleep surface is horizontal and in the lowest position with the siderails fully raised and locked when moving the bed with a patient in it.
- To avoid injury to the patient and/or user, do not attempt to move the bed laterally with the steer mode engaged. The steer wheel cannot swivel.
- The CPR emergency pedal is for emergency use only. When activating the CPR pedal, all people and equipment must be removed from the area below and around the head, thigh and foot sections of the bed or serious personal injury and/or equipment damage could occur.
- To stop the fowler from moving down, the CPR pedal can be released at anytime during activation.
- The manual backup brake is for emergency use only. It should not be used for any other situation than an emergency or it might get overused when the time comes to use it for an emergency.
- Possible fire hazard exists when this bed is used with oxygen administering equipment other than nasal, mask type or half bed-length tent type. Unplug the bed power cord from the wall when oxygen administering equipment is used.
- When using a half bed-length tent type, ensure that the siderails are outside the oxygen tent and that the tent does not extend below the mattress support level. Do not route the power cord between the mattress and the bed frame.
- Do not attach the power cord to any moving parts of the bed frame.
- The power cord could be pinched and may cause electrical shock if a bed extender is used (mattress only).
- The Bed Exit system is not designed to be used with patients weighing less than 50 lbs (23 kg).

Summary of Safety Precautions

WARNING (CONTINUED)

- The Bed Exit system is intended only to aid in the detection of a patient exiting the bed. It is not intended to replace patient monitoring protocol. The Bed Exit system signals when a patient is about to exit the bed.
 - Do not steam clean, hose off or ultrasonically clean the bed. Do not immerse any part of the bed. The internal electrical parts may be damaged by exposure to water. Hand wash regularly all surfaces of the bed with warm water and a mild detergent. Wipe cleaned surfaces dry to avoid build-up of cleaning substances. Inspect the mattress after each use. Discontinue use if any cracks or rips, which may allow fluid to enter the mattress, are found in the mattress cover. Failure to properly clean the mattress, or dispose of it if defective, may increase the risk of exposure to pathogenic substances and may bring about diseases to the patient and user.
 - Always unplug the bed power cord from the wall socket when servicing or cleaning the bed. When working under the bed with the bed in the high position, always apply the brakes and place blocks under the Bed Lift levers to prevent injury in case the Bed Down switch is accidentally pressed.
 - Please ensure patient is not in the bed prior to starting bed calibration. In calibration mode, the software does not control the interferences between the mechanical parts of the bed. Mechanical damage could occur without supervision. Only qualified personnel should perform the calibration.
 - Battery posts, terminals and related accessories contain lead and lead compounds - chemicals known to the state of California to cause cancer and birth defects or other reproductive harm. Wash hands after handling.
 - Do not modify the *InTouch®* bed. Modifying the unit can cause unpredictable operation resulting in injury to the patient or user. Modifying the unit will also void this warranty.
-

CAUTION

- The mattress thickness should not exceed 6 inches (15,24 cm).
 - When using a mattress thicker than 6 inches (15,24 cm) or a mattress overlay, extra caution and/or patient supervision may be required to reduce the likelihood of occurrence of a patient fall.
 - Preventative maintenance should be performed at least once a year to ensure all bed features are functioning properly. Ensure that any bed malfunction is promptly reported to your service personnel for immediate attention.
 - When large fluid spills occur in the area of the circuit boards, cables and motors, immediately unplug the bed power cord from the wall socket, remove the patient from the bed and clean up the fluid. Have maintenance completely check the bed. Fluids can have an adverse effect on operational capabilities of any electrical product. DO NOT put the bed back into service until it is completely dried and has been thoroughly tested for safe operation. Ensure, among other things, that the plastic components being used as covers for the siderail mechanism arms and the foot end casing are removed and that the parts they cover are thoroughly dried.
 - To avoid damage to the siderail mechanisms, do not move the bed using the raised siderails. Move the bed using the handles integrated to the boards.
 - Because individual beds may have different options, footboards should not be moved from one bed to another. Mixing footboards could result in unpredictable bed operation.
 - When servicing, use only identical replacement parts provided by Stryker.
 - For the batteries to maintain sufficient charge, you must plug the bed into a wall outlet (regulated AC power source) when not in use to maximize bed performance while on battery power.
 - If batteries are observed to have corrosion at the terminals, display cracking, have expanded or are bulging at the sides, or no longer can maintain a full charge, they should be replaced immediately.
 - When replacing the batteries, use only Stryker authorized batteries. Use of non-Stryker batteries may lead to unpredictable system performance.
 - Upon a Battery Low alarm (Battery Low LED on Footboard and/or audible beep), stop using the Zoom® drive and recharge the batteries immediately. Ignoring the Battery Low alarms may cause your batteries to degrade quicker than normal and may decrease battery life.
 - Some cleaning products are corrosive in nature and may cause damage to the product if used improperly. If the products described above are used to clean Stryker patient care equipment, measures must be taken to ensure the beds are wiped with a damp cloth soaked in clean water and thoroughly dried following cleaning. Failure to properly rinse and dry the beds will leave a corrosive residue on the surface of the bed, possibly causing premature corrosion of critical components. Failure to follow the above directions when using these types of cleaners may void this product's warranty.
-

Summary of Safety Precautions

Note

- Throughout this Operations Manual, the words “right” and “left” refer to the right and left sides of a patient lying on his/her back on the bed.
- The addition of accessories affects the motion of the bed.
- The *i*Bed option is only used as an informational feature and is not intended to replace normal patient monitoring protocol.

OPTIONAL ZOOM® DRIVE SYSTEM (MODEL 2141 ONLY)

In addition to the previous warnings and cautions, all of the following warnings and cautions apply to units equipped with the Zoom®.

WARNING

- The 2141 *InTouch*® Bed is intended for use by trained hospital personnel only. Failure to properly train personnel could result in injury.
 - USE CAUTION while maneuvering the unit with the drive wheel activated. Always ensure there are no obstacles near the unit while the drive wheel is activated. Injury to the patient, user or bystanders or damage to the frame or surrounding equipment could occur if the unit collides with an obstacle.
 - Use caution when transporting the unit down halls, through doors, in and out of elevators, etc. Damage to the siderails or other parts of the unit could occur if the unit comes in contact with walls or door frames.
 - Put the drive wheel in the neutral position and release the brake before pushing the unit manually. For 2141 models; push the Brake Off button to disengage drive wheel (Zoom®) before pushing the unit manually. Do not attempt to push the unit manually with the drive wheel engaged. The unit will be difficult to push and injury could result.
 - If unanticipated motion occurs, unplug the power cord from the wall socket, push the battery power on/off switch to the “OFF” (0) position (the LED will not be illuminated), actuate the drive wheel pedal to the neutral position and call maintenance.
 - In the event the batteries become discharged while using the Zoom® drive, press the “N” (Brake Off) button to place the drive wheel in Neutral and proceed to push the bed manually. Recharge the batteries prior to using Zoom® again. Continuing to use the Zoom® drive could lead to battery damage and the drive wheel getting stuck in the down position.
 - The power save mode is activated after one hour on battery power with no motion release switch activation. Functions including Bed Exit, Scale and Motion will cease to operate when the unit enters the power save mode. Injury to the patient could occur if proper patient monitoring protocol is not observed.
 - Always unplug the power cord and push the battery power on/off switch to the “OFF” (0) position before service or cleaning. When working under the frame, always support the litter frame to prevent injury in case the Bed Down switch is accidentally activated.
-

Static Discharge Precautions

The electronic circuits in the *InTouch*® Critical Care Bed are completely protected from static electricity damage only while the bed is assembled. It is extremely important that all service personnel always use adequate static protection when servicing the electronic systems of the *InTouch*® Critical Care Bed. You should be using static protection whenever you are touching wires.

Static Protection Equipment

The necessary equipment for proper static protection is:


- 1 static wrist; 3M part number 2214 or equivalent,
- 1 grounding plug; 3M part number 61038 or equivalent,
- 1 test lead with a banana plug on one end and an alligator clip on the other; Smith part number N132B699 or equivalent.

CAUTION

All electronic service parts will be shipped in static shielding bags. Do not open the bags until you have completed steps 2 and 3 of the following procedure. Do not place unprotected circuit boards on the floor. All circuit boards to be returned to Stryker Medical should be shipped in the static shielding bags the new boards were shipped in.

Static Protection Procedure

1. Unplug the power cord from the power source.
2. Insert the grounding plug into a properly grounded hospital grade wall receptacle. Plug the banana plug of the test lead into the receptacle on the grounding plug. Connect the alligator clip on the other end of the test lead to a ground point on the bed.
3. Place the static control wrist strap on your wrist. Connect the alligator clip at the other end of the wrist strap cord to a ground point on the bed.

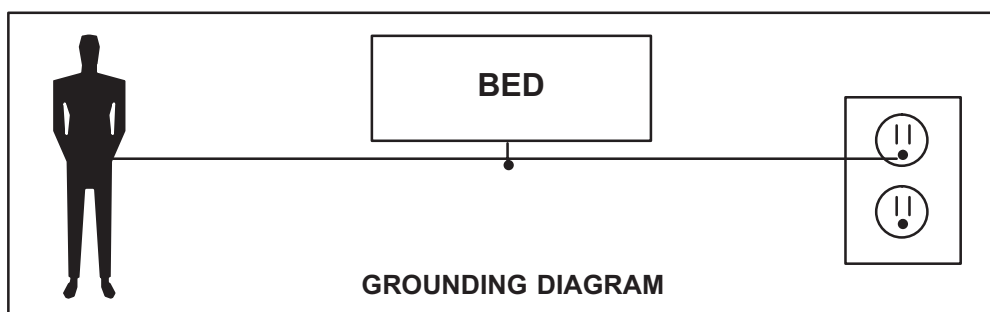

Setup Procedures

To prevent permanent damage to this unit, the unit must reach room temperature prior to conducting any setup and/or unit operations.

It is important to ensure that the bed is working properly before it is put into service. The following list will help ensure that each part of the bed is checked.

- Install the foot and head boards on the bed. Insert the footboard carefully so that the footboard and the casing connectors fit in smoothly.

CAUTION

Because individual beds may have different options, footboards should not be moved from one bed to another. Mixing footboards could result in unpredictable bed operation.

- Plug the power cord to the bed connector at the head end of the bed and into a properly grounded hospital grade wall outlet.
- Turn the battery power switch to the “ON” (1) position (located below the litter surface at patient right side).
- Set the time and date through the touch screen (refer to the *InTouch®* Operations Manual for procedures).

WARNING

This bed is equipped with a hospital grade plug for protection against shock hazard. It must be plugged directly into a properly grounded receptacle. Grounding reliability can be achieved only when a hospital grade receptacle is used.

- To test the manual backup brake (located on the patient’s right side only), flip the manual backup brake pedal outward and depress down fully on the foot end side of the pedal. The word BRAKE in red will be visible in the clear window located on the base next to the pedal and the Brake symbol will illuminate on the footboard control panel. The brakes should now be applied.
- To test the electric brake, engage the brake by pressing the brake button on the siderail or footboard control panel. Try moving the bed to ensure the brakes are applied. Press the Neutral button on the siderail control panel or on the footboard to disengage the brake.
- For Model 2141 Beds only: On the patient’s right side, flip the manual backup brake pedal outward and depress down fully on the head side of the pedal. The letter D in GREEN should be visible in the clear window located on the base next to the pedal. The Zoom® Drive wheel should now be engaged. Depress down fully on the center of the pedal until the letter N in BLUE is visible in the clear window. The Zoom® Drive wheel should now be disengaged.
- Ensure that the siderails raise, lock in the fully raised position and lower smoothly.
- Run through each control on the footboard.
- Verify the scale system and the Bed Exit system for proper operation.
- Run through each control on both inner and outer control panels of the head siderails. If the bed is equipped with the optional Siderail Communication Pendant, plug the provided cable to the 37-pin connector located at the head end of the bed and into the proper wall outlet.
- Raise the bed completely and activate the Trendelenburg function. Ensure the head end lowers to the full down position (refer to the *InTouch®* Operations Manual for procedures). Level the bed using the Bed Lift system controls.
- Raise the bed completely and activate the reverse Trendelenburg function. Ensure the foot end lowers to the full down position (refer to the *InTouch®* Operations Manual for procedures). Level the bed using the Bed Lift system controls.
- Verify functionality of the CPR emergency release: raise the fowler up then depress down on the CPR pedal located on either side of the bed at the head end of the base. The fowler will lower towards a flat position until the pedal is released.
- Ensure the Knee Gatch (if raised) also starts flattening when the Fowler is completely down.
- Verify the following optional equipment for proper operation: 120V Auxiliary Outlet, head end nurse controls, pendant, roller bumpers, Zoom® handles, etc.
- To prevent permanent damage to the bed, ensure the unit reaches room temperature prior to use.

Setup Procedures

OPTIONAL XPRT™ THERAPY MATTRESS

If your bed is equipped with the **XPRT™** Therapy Mattress option, perform the following setup procedures to install the Mattress. For graphic representation of the setup procedures, refer to the **XPRT™** Therapy Mattress Operations Manual.

CAUTION

When using a mattress thicker than 6 inches (15,24 cm) or a mattress overlay, extra caution and/or patient supervision may be required to reduce the likelihood of occurrence of a patient fall.

1. Place mattress over bed litter with printed logo at the foot end of the bed.
2. Fold back foot end section of mattress.
3. Place foot box on foot end of bed litter.
4. Connect the two (2) color coded connectors on the foot box to the corresponding color coded connectors on the mattress. Connect black connection on foot box to cable adapter 2950-001-180 and then to the bed frame.
5. Turn the locking collars clockwise to secure the connections.
6. Connect the other end of the black connector to the bed (left side of litter at foot end behind the accessory outlet).
7. Connect the air line from the mattress to the corresponding fitting on the foot box.
8. Fasten the two (2) retaining clips to the two (2) D-Rings on the foot box.
9. Lower the foot section of mattress over the foot box. Attach the mattress to the bed frame using the mattress tie-downs.
10. Apply linens utilizing the “D” rings for the flat sheet.
11. To secure linens, to mattress, thread four corners through D-Rings attached to mattress.
12. To ensure proper therapy, do not pull linens taut. The linens should remain loose and wrinkly on the surface of the mattress.
13. Plug the mattress power cord into a properly grounded, hospital grade receptacle.

Note

The *InTouch®* bed will detect when the mattress has been connected as well as what type of mattress it is. This will be shown on the *InTouch®* screen.

WARNING

- Do not route the power cord between the mattress and the bed frame.
 - Do not attach the power cord to any moving parts of the bed frame.
 - The power cord could be pinched and may cause electrical shock if a bed extender is used.
-

OPTIONAL POSITIONPRO™ REPOSITIONING MATTRESS OPTION

If your bed is equipped with the PositionPRO™ Patient Repositioning Mattress option, perform the following setup procedures to install the mattress. For graphic representation of the setup procedures, refer to the PositionPRO™ Mattress Operations Manual.

CAUTION

When using a mattress thicker than 6 inches (15,24 cm) or a mattress overlay, extra caution and/or patient supervision may be required to reduce the likelihood of occurrence of a patient fall.

1. Place the mattress onto the bed.
2. Flip the foot section towards the head end.
3. Place the control box (upside down) into the opening in the foot section.

Setup Procedures

OPTIONAL POSITIONPRO™ REPOSITIONING MATTRESS (CONTINUED)

4. Connect outer transparent tubes to manifold, matching the color coding.
5. Connect tilt sensor cables.
 - a. Align the white dots.
 - b. Twist clockwise to fasten.
6. Connect pendant cable.
7. Connect power cord (4') and turn the switch to on.
Note: The switch is hidden under the power cord.
8. Fasten straps over the power cord.
9. Install the power cord in the two (2) retaining clips.
10. Fasten the three (3) retaining straps.
11. Carefully rotate the foot end control box and the mattress into the flat position.

CAUTION

Gently lower the foot end section to not damage the control box.

12. Fasten the retaining straps to secure the mattress to the bed frame (four (4) straps total).
13. Connect the power cord to the 110V outlet on the bed.

Applying the linens

1. Apply the linens using the “D” rings for the flat sheet.
2. To effectively use the “Turn Assist”, do not pull linens taut. Linens should remain loose and wrinkly on surface of the mattress.

WARNING

Ensure that you have always access to the CPR straps.

Note

If any problems are found during bed setup, contact our Technical Service department at USA: 1-800-327-0770 (option 2).

OPTIONAL ZOOM® DRIVE SYSTEM (MODEL 2141 ONLY)

If your bed is equipped with the Zoom® drive, run through the preceding setup procedures and continue with the procedures listed below.

- Run through the operation of the drive wheel (refer to *InTouch®* Operations Manual for procedures) to ensure it is operating properly.
- On the patient's right side of the bed, flip the manual backup brake pedal outward and depress down fully on the head side of the pedal. The letter D in GREEN should be visible in the clear window located on the base next to the pedal. The Zoom® drive (2141 Model only) should now be engaged. Depress down fully on the center of the pedal until the letter N in BLUE is visible in the clear window. The Zoom® drive should now be disengaged.

Maintenance Menu Guide

The Maintenance Menu is accessed through the Touch Screen and contains additional features of the product. This menu provides an interface to the user and/or service personnel in order to provide the ability to control and access maintenance features.

ACCESSING CONFIGURATION SCREEN

WARNING

Please ensure patient is not in the bed prior to starting bed calibration. In calibration mode, the software does not control the interferences between the mechanical parts of the bed. Mechanical damage could occur without supervision. Only qualified personnel should perform the calibration.

Note

Verify that the bed is on a level surface which does not have any slopes or inclines prior to entering into the calibration mode.

1. Unseat and reseat the footboard and wait until the main control screen is displayed.
2. Push and hold the Main Menu button located in the upper right corner of the footboard control panel (see Figure 1 below). Continue pressing on the Main Menu button while executing steps 3-5.
3. Push and hold the **Brake** button for 5 seconds and then release.
4. Push the **HOB 30°+** button once and release.
5. Push the **Drive** button once and release.
6. Release the Main Menu button and you will be taken into the Configuration Screen shown in Figure 2.



Figure 1: Footboard Control Panel

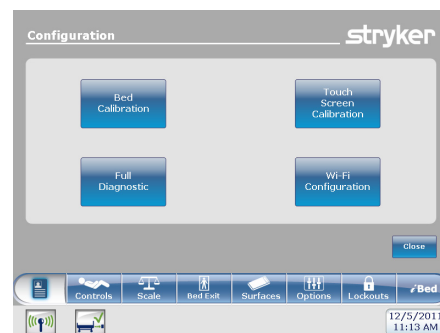


Figure 2: Configuration Screen

Maintenance Menu Guide

CONFIGURATION SCREEN

The following items A, B, and C are configuration buttons available and displayed on the Configuration screen (Figure 3).

- A. Bed Calibration
- B. Full Diagnostic ([see page 34](#))
- C. Touch Screen Calibration ([see page 35](#))
- D. Wi-Fi Configuration ([see page 36](#))

The following items D and E are configuration options available but are **not displayed** on the Configuration screen. To access these configuration options, follow the procedures identified on page listed below.

- E. Bed Options Configuration ([see page 38](#))
- F. Serial Number Configuration ([see page 39](#))

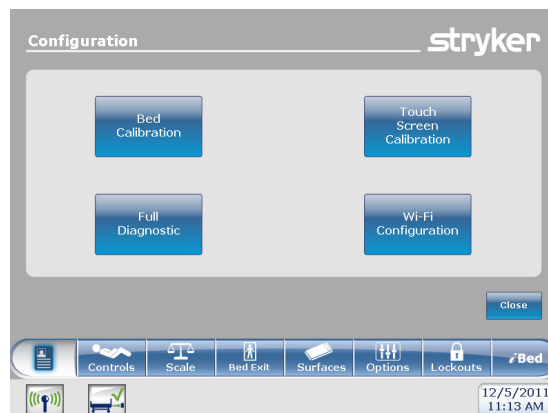


Figure 3: Configuration Screen Menu Items

A. Bed Calibration

CAUTION

Prior to calibration, connect the bed to an A/C outlet.

Note: During calibration, if the backlight shuts off touch the screen to continue.

WARNING

Refer to Figure 4 for WARNING details.

1. To start the bed calibration, press the Bed Calibration button on the Configuration Screen (refer to Figure 3).
2. After pressing the Bed Calibration button, Figure 4 will be displayed. Press "NEXT" to continue with calibration.

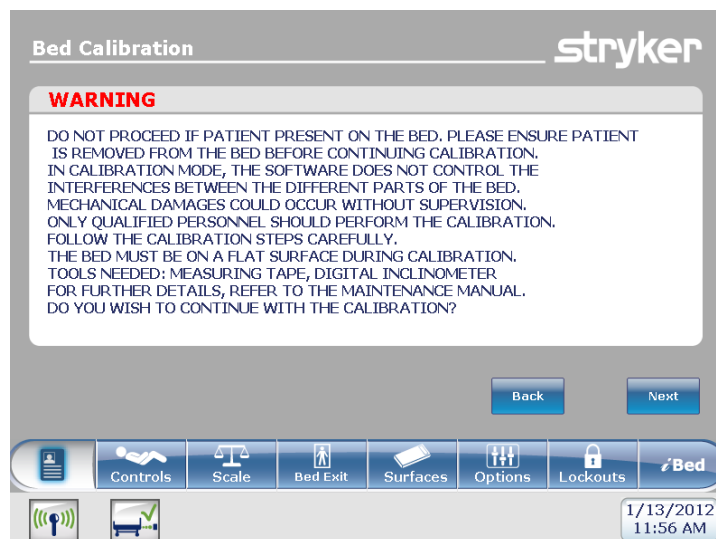


Figure 4: Bed Calibration - WARNING

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

3. After pressing **Next** to continue calibration, Figure 5 will appear.



Figure 5: Bed Calibration - Step #1 of 6

4. Place the Litter surface to a flat position by pressing simultaneously the **Foot Up**, **Fowler Down** and **Gatch Down** buttons as shown in Figure 6.

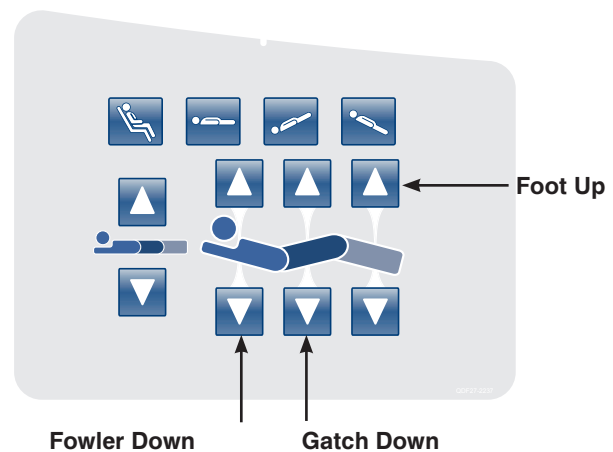


Figure 6: HE Siderail Control Panel - (Right Side Shown)

5. Lower the bed to the lowest position. Press the **Bed Height Down (Head Lift Down)** and **Reverse Trendelenburg (Foot Lift Down)** buttons simultaneously as shown in Figure 7.

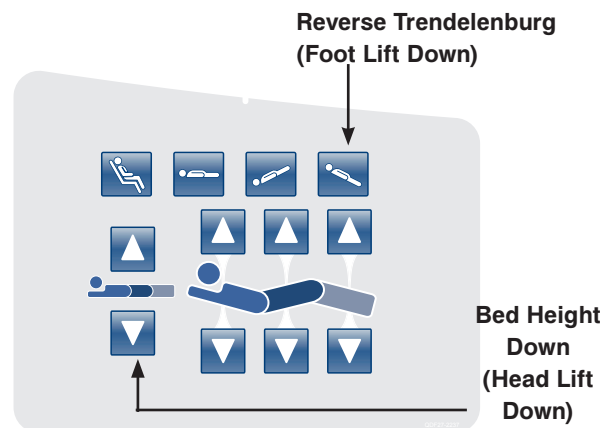


Figure 7: HE Siderail Control Panel - (Right Side Shown)

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

6. Press the **Next** button when done. The “Do Not Touch Bed” screen will appear as shown in Figure 8.

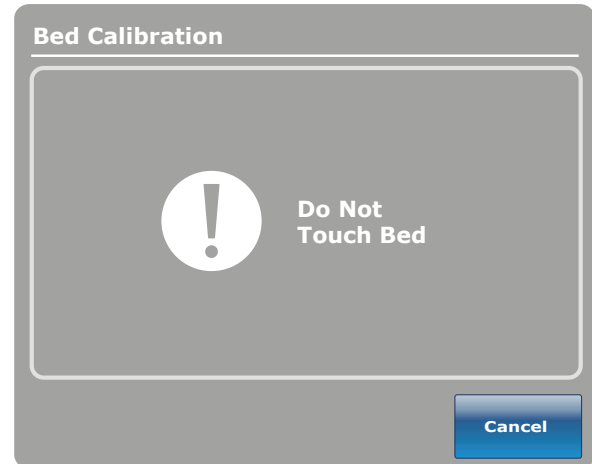


Figure 8

7. When step 1 of the calibration procedure has completed, step 2 of the calibration procedure will begin and Figure 9 will be displayed.



Figure 9: Bed Calibration - Step 2

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

8. Raise the bed height to 20 inches measuring from the top of the seat section to the floor. Press the **Bed Height Up (Head Lift Up)** and **Trendelenburg (Foot Lift Up)** buttons as shown in Figure 10.

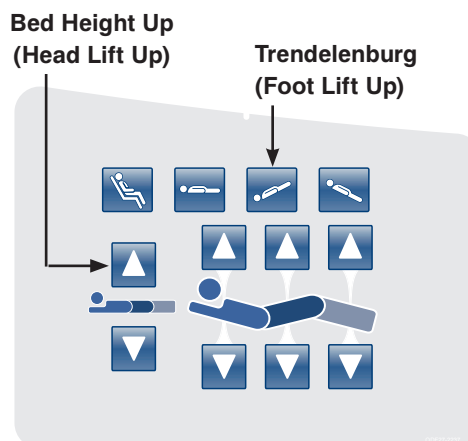


Figure 10: Head Siderail Control Panel (Right Side Shown)

9. Standing on either side of the bed at the fowler section, raise the foot siderail and then position the digital level/inclinometer on the bottom of the litter below the mattress retainer (refer to Figure 11). Using the digital level/inclinometer, verify the bed is level (0.0 ± 0.1).

Note: Cycle power on the digital level/inclinometer prior to placing it on the bottom of the litter frame and do not zero/calibrate the digital level/inclinometer.



Placement
on Litter

Figure 11: Inclinometer placement

10. Press the **Next** button when done. The “Do Not Touch Bed” screen will appear as shown in Figure 12.

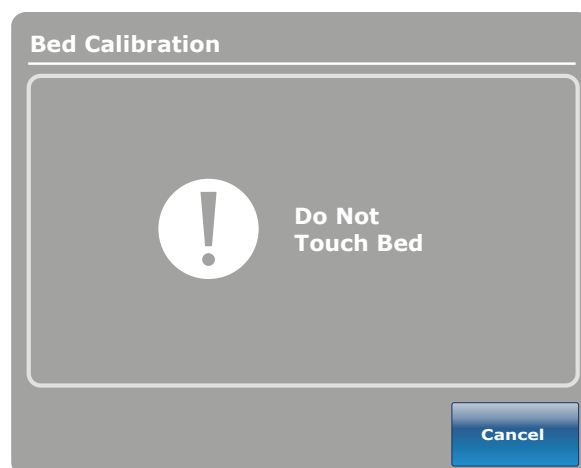


Figure 12: Do Not Touch Bed Screen

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

11. When step 2 of the calibration procedure has completed, step 3 of the calibration procedure will begin and Figure 13 as shown below will appear on the screen.



Figure 13: Bed Calibration - Step 3

12. Place the bed at +12 degrees Trendelenburg by pressing the **Trendelenburg (Foot Lift Up)** button as shown in Figure 14. Verify +12 degrees +/- 0.1 with the inclinometer you previously placed on the litter frame in step 9.

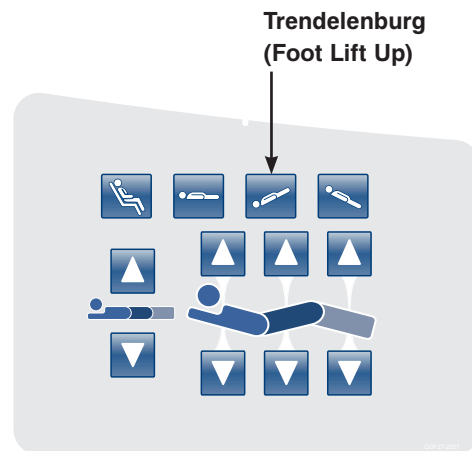


Figure 14: Head Siderail Control Panel

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

13. Press the **Next** button when done.
14. The “Do Not Touch Bed” screen will appear as shown in Figure 15.

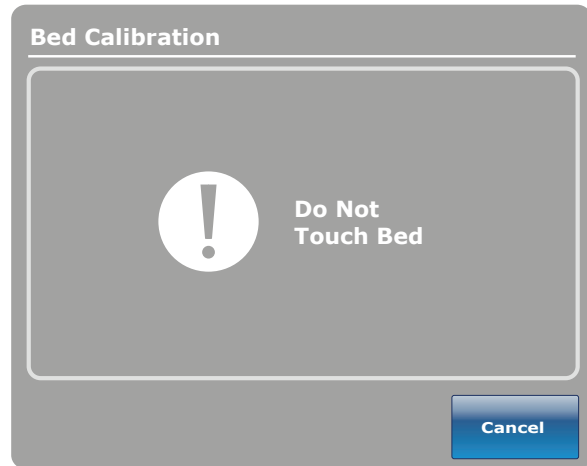


Figure 15: Do Not Touch Bed Screen

15. When step 3 of the calibration procedure has completed, step 4 of the calibration procedure will begin and Figure 16 will be displayed as shown below.



Figure 16: Bed Calibration - Step 4

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

16. Level the bed back out to zero degrees by pushing the Reverse Trendelenburg button until the litter is level while referencing the inclinometer. Note: Confirm inclinometer reads zero degrees.
17. Place the bed at -12 degrees Reverse Trendelenburg by pressing the **Bed Height Up (Head Lift Up)** button as shown in Figure 17 below. Verify -12 degrees \pm 0.1 with the inclinometer you previously placed on the bottom of the litter frame in step 9.

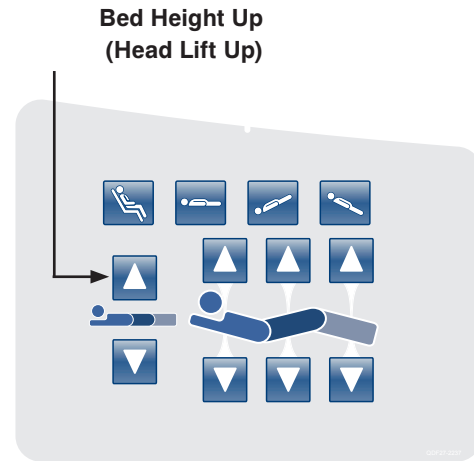


Figure 17: Head Siderail Control Panel - (Right Side Shown)

18. Press the **Next** button when done.

19. The "Do Not Touch Bed" screen will appear as shown in Figure 18.

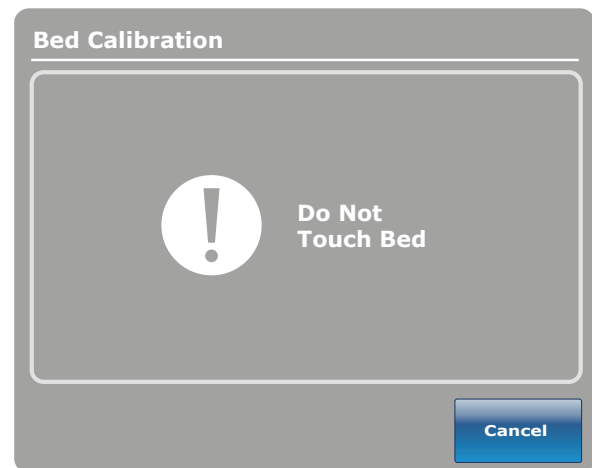


Figure 18: Do Not Touch Bed Screen

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

20. When step 4 of the calibration procedure has completed, step 5 of the calibration procedure will begin and Figure 19 will appear on the screen as shown below.



Figure 19: Bed Calibration - Step 5

21. Place the bed at the highest height by pressing simultaneously the **Trendelenburg (Foot Lift Up)** button and **Bed Height Up (Head Lift Up)** button as shown in Figure 20.

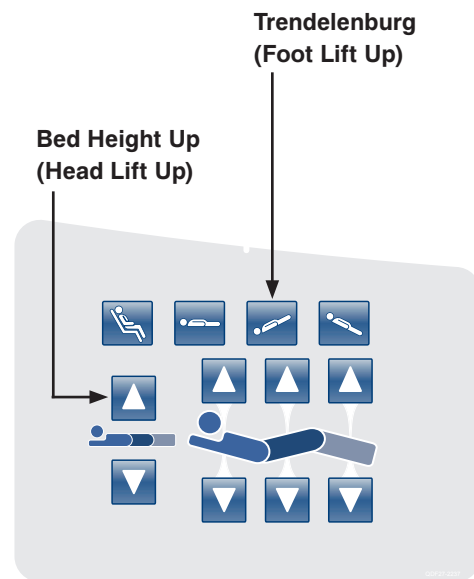


Figure 20: Head Siderail Control Panel - (Right Side Shown)

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

22. Press the **Fowler Up** button until the Fowler reaches the highest height, next press the **Gatch Up** button until the Gatch reaches its highest height, lastly press the **Foot Up** button until the foot section reaches its highest height (refer to Figure 21 below). The foot section should be at a flat position.

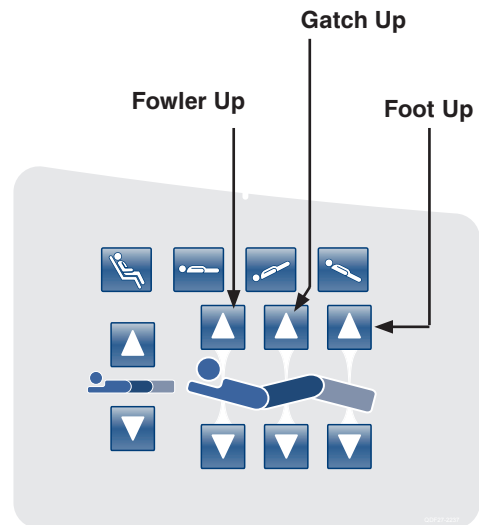


Figure 21: Head Siderail Control Panel - (Right Side Shown)

23. Press the **Next** button when done.

24. The “Do Not Touch Bed” screen will appear as shown in Figure 22.

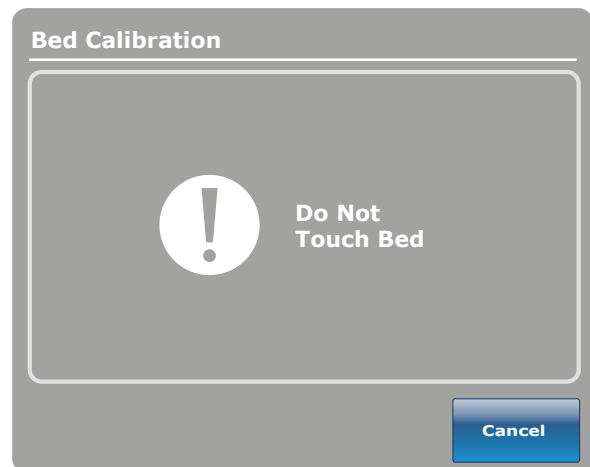


Figure 22: Do Not Touch Bed Screen

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

25. When step 5 of the calibration procedure has completed, step 6 of the calibration procedure will begin and Figure 23 will be displayed as shown below.



Figure 23: Bed Calibration - Step 6

26. Place the bed at the highest height by pressing simultaneously the **Trendelenburg (Foot Lift Up)** button and **Bed Height Up (Head Lift Up)** button (see Figure 24).
27. Place the Fowler and Gatch section of the bed at the highest height by first pressing the **Fowler Up** button then the **Gatch Up** button (See Figure 24).
28. Place the foot at the lowest position by pushing the **Foot Down** button until limit is met (see Figure 24) . **CAUTION: The Gatch must be raised to the highest height prior to running the Foot Down or damage could occur.**

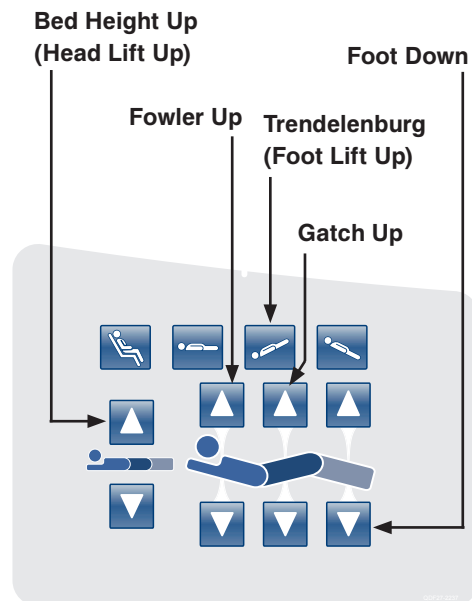


Figure 24: Calibration Complete

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

A. Bed Calibration (Continued)

29. When the calibration procedure is completed, Figure 25 will be displayed as shown below.
30. Press the Close button to exit the Calibration Procedure Menu.
31. Level the litter flat using the CPR pedal. Verify all display readings are zero degrees while the bed is at 33" (84 cm) (highest height). Lower the bed to 16" (41 cm) (lowest height) and verify the display readings maintain a constant reading of zero degrees with no fluctuations. When the bed reaches it lowest height at 16", verify the display readings are still at zero degrees.

Note: If readings are not all zero, you will need to recalibrate the bed by repeating steps 1-30.

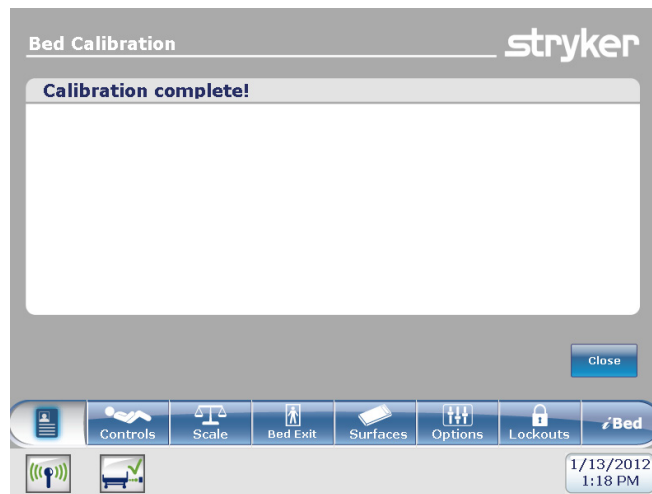


Figure 25: Calibration Complete

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

B. Full Diagnostic

- From the Configuration Screen, press the Full Diagnostic button. Figure 26 will appear.
- The following menu items may be selected by pressing their button.
 - BOARDS** (Figure 27a)
Provides information on the switch boards and the touch screen's software version.
 - ERROR CODES** (Figure 27b)
Provides information on errors which the CPU board has identified.
 - INPUT STATES** (Figure 27c)
Provides information on the status of all switches and jumpers on the bed.
 - MOTORS** (Figure 27d)
Provides information on what a motor is doing when a function button is pushed.
Note: This requires assistance to press the buttons on the head siderails or at the head end control.
 - BUTTONS PRESSED** (Figure 27e)
Provides information on when the CPU has detected a button being pressed.
Note: This requires assistance to press the buttons on the head siderails or at the head end control.
 - SIGNAL VALUES** (Figure 27f)
Provides information on CPU voltages, load cell values, and angle sensor values.

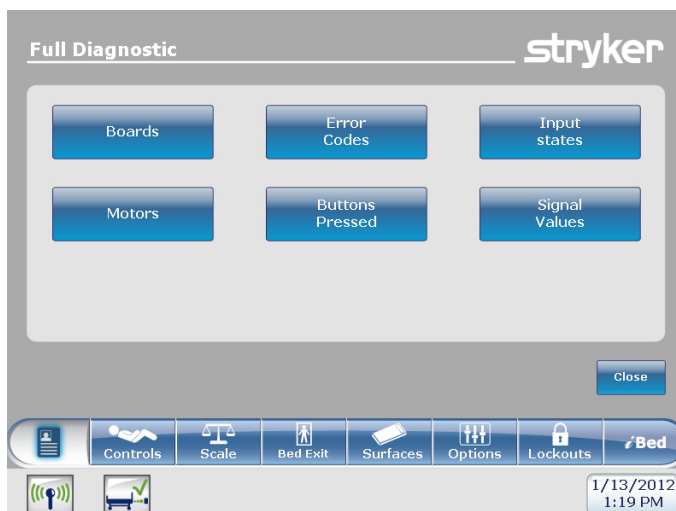


Figure 26: Full Diagnostic Screen

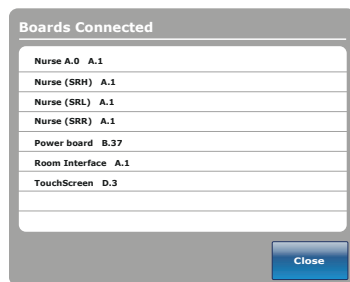


Figure 27a: Board

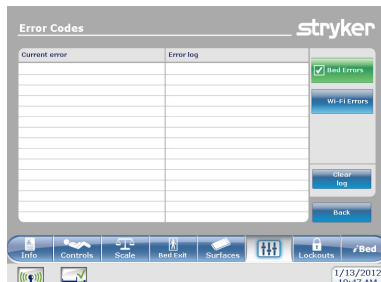


Figure 27b: Error Codes

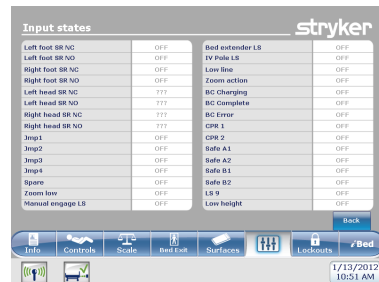


Figure 27c: Input States

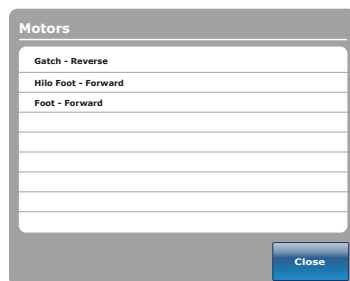


Figure 27d: Motor

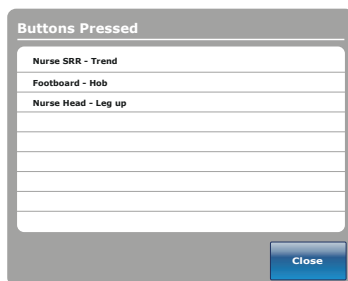


Figure 27e: Pressed Buttons

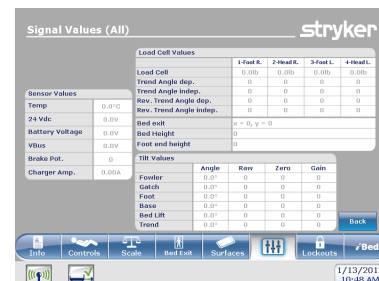


Figure 27f: Signal Values

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

C. Touch Screen Calibration

Ensure patient is not present on the bed before performing the Touch Screen Calibration.

1. From the Configuration Screen, press the Touch Screen Calibration button. Figure 28 will appear.
NOTE: If the touch screen will not respond, you will need to push the HOB 30⁰+, Brake and Drive buttons on the footboard at the same time (this will enable you to get directly into the touch screen calibration).
CAUTION: When pushing the buttons above the fowler, brakes, or drive, actuators may activate.
2. Carefully press and briefly hold a stylus or your finger on the center of the cross hair shown on the screen.
3. Repeat as the target moves around the screen. There will be five different locations to press: center, lower right, upper right, upper left, and lower left.
4. When the last cross hair has been touched, Figure 29 displays 'New calibration settings have been measured'.
5. Tap the screen to register saved data.
6. If you do not want to save the new data, wait for 30 seconds to cancel saved data and keep the current setting.

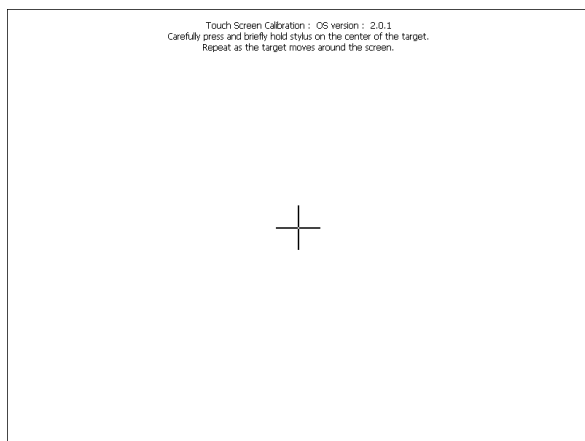


Figure 28: Touch Screen Calibration: Start

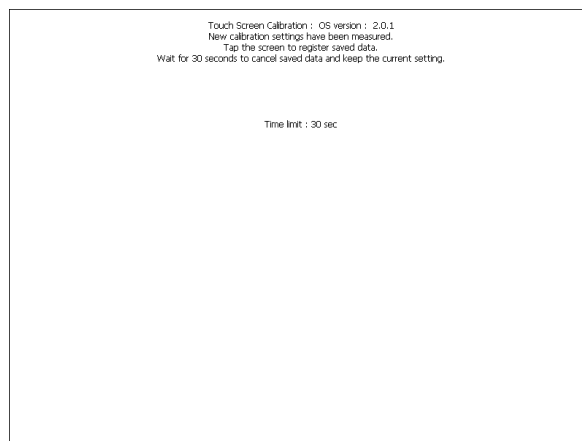


Figure 29: Touch Screen Calibration: Completed

NOTE: The TOUCH SCREEN CALIBRATION SCREEN is a validation of the touch screen's calibration. When the user presses anywhere on the screen, the coordinates x and y are displayed on the lower part of the screen.

CONFIGURATION SCREEN (CONTINUED)

D. Wi-Fi Calibration

CAUTION

These settings should only be modified by trained personnel. Changing these settings may disable the wireless feature. These settings should only be changed or updated with the aid of the hospital's IT department or Stryker Medical Technical Support.

1. From the Configuration Screen, press the “Wi-Fi Configuration” button to configure wireless settings for the bed. Figure (1) will appear.
2. Press the “Wi-Fi ON” / “Wi-Fi OFF” button to toggle the wireless network.
3. To configure the network settings, tap on the **Network Parameters** tab (Figure 30).
 - a. Connection Type: Select either DHCP or Static IP. The selected option will display a checkmark.
 - b. Static IP: The static IP address will be displayed (static IP only). Press the pencil icon to modify the IP address.
 - c. Subnet Mask: The subnet address will be displayed (static IP only). Press the pencil icon to modify the address.
 - d. Default Gateway: The gateway address will be displayed (static IP only). Press the pencil icon to modify the address.
 - e. Network Name (SSID): The name of the selected wireless network will be displayed. Press the pencil icon to manually enter an SSID. Press the hand icon to select from detected wireless networks.
4. To configure the network logon information, tap on the **User Authentication** tab (Figure 31).
 - a. User Name: The user name to access the wireless network will be displayed. Press the pencil icon to modify the user name.
 - b. Password: The password to access the wireless will be shown as asterisks (*). This field will not display the actual password in plain text. Press the pencil icon to enter the password.
 - c. Domain: The domain for the user name is displayed here. Press the pencil icon to modify the domain.

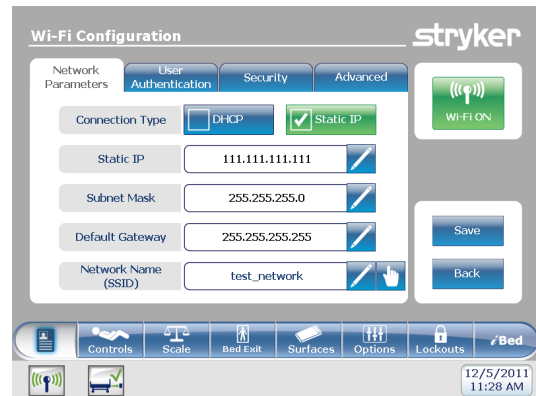


Figure 30: Network Parameters

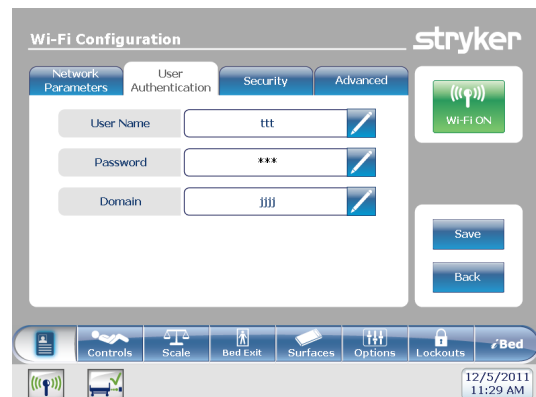


Figure 31: User Authentication

CONFIGURATION SCREEN (CONTINUED)

D. Wi-Fi Calibration (Continued)

5. To configure the wireless network security settings, tap the **Security** tab (Figure 32).
 - a. Authentication: The current security option will be displayed. Press the up and down arrows to cycle through the supported security options.
 - b. Network Key: The network key will be shown as asterisks (*). This field will not display the actual network key in plain text. Press the pencil icon to enter the network key.
 - c. Key Index: The network key index will be displayed (when appropriate). Press the up and down arrows to change the key index.
 - d. Encryption: The current encryption will be displayed. Press the up and down arrows to cycle through the supported encryption types (determined by the authentication type).
 - e. EAP Type: The current EAP will be displayed (when appropriate). Press the up and down arrows to cycle through the supported protocols (determined by the encryption type and authentication type).
6. The following options are available on the **Advanced** tab (Figure 33):
 - a. MAC Address: The MAC address for the iBed Locator will be displayed here. This is a read-only field and cannot be modified.
 - b. IP Address: The current iBed Locator IP address will be displayed here. Press the **Renew IP** button to force the IP address to refresh using the current wireless network configuration.
 - c. If necessary, the **Reset** button can be pressed to reset the iBed Locator to factory default values.

Note

All current wireless configuration settings will be erased and cannot be retrieved.



Figure 32: Security

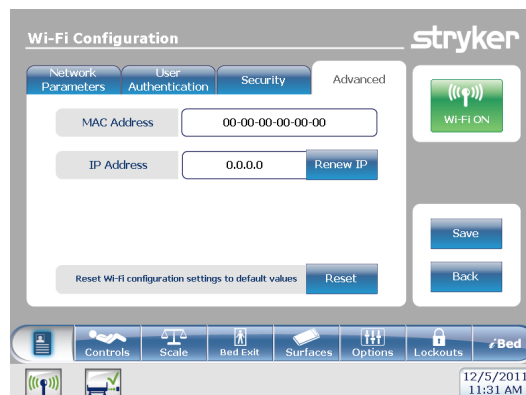


Figure 33: Advanced

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

E. Bed Options Configuration

Access the configuration screen as shown on [page 22](#). Once in the configuration screen, follow the steps below to access the options screen or the serial number screen.

To access the Bed Options screen:

1. Press and hold the **HOB 30** button and the **BRAKE** button at the same time for 5 seconds, then release both buttons. The Bed Options screen (Figure 34) will be displayed.

NOTE: When the European Community message window displays, push the Close button to close out of the message. That is not applicable in this configuration.

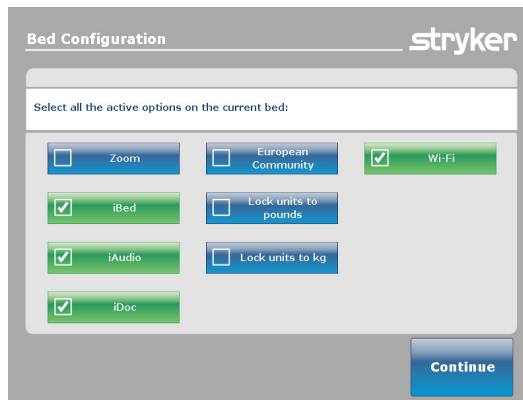


Figure 34: Bed Options screen

2. Select all of the options shown on the Bed Options screen that apply to the bed configuration then, press **Continue**.
NOTE: In Figure 34, the options selected are iBed, iAudio, iDoc and Wi-Fi. All of the options selected will turn green.
3. After pressing **Continue** in step 2, a confirmation screen as shown in Figure 35 will be displayed verifying the options you selected.
 - a. If the options on the confirmation screen do not match the options on the bed, press the **Back** button.
 - b. If the options on the confirmation screen match the options on the bed, press the **OK** button.
4. After pressing the **OK** button, the options will be saved and the screen will return to the configuration screen. Press the **Close** button to close the configuration screen.
5. After pressing the **Close** button, a cycle power screen (Figure 38) will be displayed stating to cycle power on the bed.
6. To cycle power on the bed, turn the battery disconnect switch to **OFF** (O) then unplug the power cord from the wall outlet. Plug the power cord back into the wall outlet then turn the battery disconnect switch back **ON** (I).
7. Test bed functionality prior to returning the bed into service.

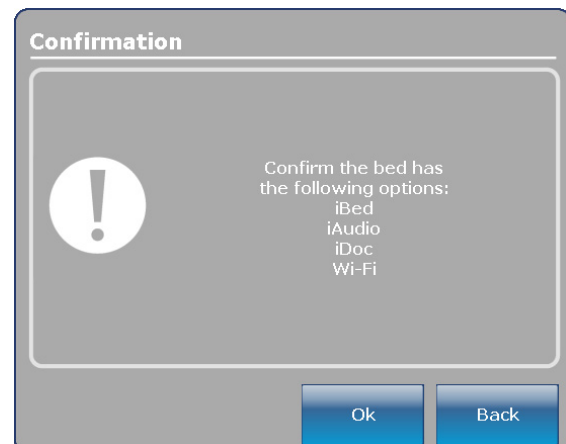


Figure 35: Bed Options Confirmation Screen

Maintenance Menu Guide

CONFIGURATION SCREEN (CONTINUED)

F. Serial Number Configuration

To access the Serial Number screen:

1. Press and hold the **HOB 30** button and the **Vascular Position** button at the same time for 5 seconds then release both buttons. The Bed Configuration - Serial Number screen (Figure 36) will be displayed.

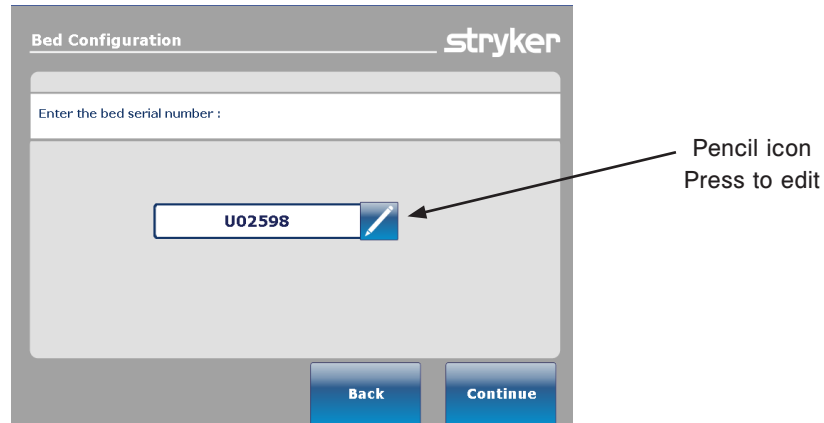


Figure 36: Bed Configuration Serial Number Screen

2. Enter or confirm the serial number of the bed (Figure 36).
 - a. **To enter the serial number:**
 - i. Press the pencil button located to the right of the serial number field. The Edit screen will be displayed.
 - ii. Enter the serial number of the bed in the serial number field, then press the **OK** button. You will be returned to the serial number main screen as shown in Figure 36.
 - iii. Press the **Continue** button and proceed to step 3.
 - b. **To confirm the serial number:**
 - i. Review the serial number displayed in the serial number field.
 - ii. If serial number is correct, press the **Back** button and proceed to step 6.
 - iii. If the serial number is incorrect, press the pencil icon button to open the Edit screen then enter the correct serial number.
 - iv. Press the **OK** button and you will be returned to the serial number main screen.
 - v. Press the **Continue** button and proceed to step 3.
3. After pressing the **Continue** button, the serial number will be saved and the serial number confirmation screen (Figure 37) will be displayed. Press the **OK** button.
4. After pressing the **OK** button, a cycle power screen (Figure 38) will be displayed stating to cycle power on the bed.
5. To cycle power on the bed, turn the battery disconnect switch to **OFF** (O) then unplug the power cord from the wall outlet. Plug the power cord back into the wall outlet then turn the battery disconnect switch back **ON** (I).
6. Test bed functionality prior to returning the bed into service.

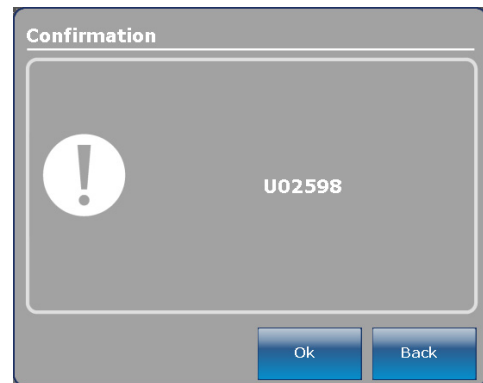


Figure 37: Serial Number Confirmation Screen

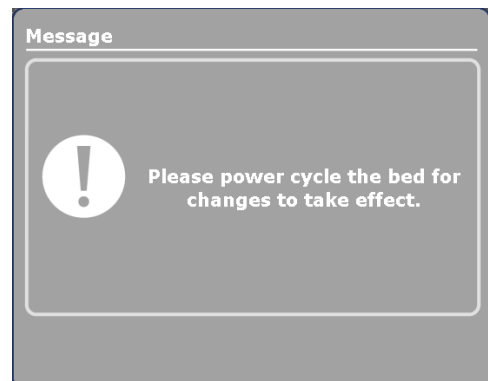


Figure 38: Cycle Power Screen

Preventative Maintenance

Beds require an effective maintenance program, we recommend checking these items annually. Use this sheet for your records. Keep on file.

CHECKLIST

- _____ All fasteners secure (reference all assembly prints).
- _____ Engage brake pedal and push on the bed to ensure all casters lock securely.
- _____ “Brake Not Set” LED on the footboard and head end siderails when brakes are not engaged.
- _____ Locking steer caster engages and disengages properly (2131 Model only).
- _____ Siderails move, latch and stow properly.
- _____ CPR release working properly.
- _____ I.V. pole working properly (if on bed).
- _____ No cracks or splits in head or footboards.
- _____ No rips or cracks in mattress cover.
- _____ All functions on head end siderails working properly (including LEDs).
- _____ All functions on footboard working properly (including LEDs).
- _____ Scale and bed exit system working properly.
- _____ Night light working properly.
- _____ Power cord not frayed.
- _____ No cables worn or pinched.
- _____ All electrical connections tight.
- _____ All grounds secure to the frame.
- _____ Ground impedance not more than 100 milliohms.
- _____ Current leakage not more than 300 microamps.
- _____ Engage drive wheel and ensure it is operating properly (Zoom® option - 2141 model only).
- _____ Motion release switches working properly (Zoom® option - 2141 model only).
- _____ Confirm head end Zoom® handle functionality (2141 model only).
- _____ Replace batteries every two years.
- _____ Replace batteries immediately if batteries are observed to have corrosion at the terminals, display cracking, have expanded or are bulging at the sides, or no longer can maintain a full charge. Use only QDF9188 for battery replacement.
- _____ Ensure ground chains are clean, intact, and have at least two links touching the floor.
- _____ Check fowler angle for accuracy 0° - 70°.
- _____ Check gatch angle for accuracy 0° - 15°.
- _____ Check foot section angle for accuracy 0° - 50°.
- _____ Siderail switches working properly (iBed Awareness option).
- _____ iBED Awareness Light Bar LEDs on footboard and siderails working properly (iBed Awareness option).
- _____ Inspect footboard control labeling for signs of degradation.
- _____ Ensure calibration of the touch screen is accurate.
- _____ Ensure calibration of the bed is accurate.
- _____ Check labels as specified in the Operations and Maintenance manuals for legibility, proper adherence and integrity.
- _____ Confirm iBed® Wireless Module and IR Module are intact and footboard icons are displaying (iBed® Wireless Option).

Bed Serial Number:		

Completed by: _____ Date: _____

Cleaning

Hand wash all surfaces of the bed with warm water and mild detergent. Dry thoroughly. Do not steam clean or hose off the *InTouch®* Critical Care Bed. Do not immerse any part of the bed. Some of the internal parts of the bed are electric and may be damaged by exposure to water.

Suggested cleaners for bed surfaces:

Quaternary Cleaners (active ingredients - ammonium chloride)

Phenolic Cleaners (active ingredient - o-phenylphenol)

Chlorinated Bleach Solution (5.25% - less than 1 part bleach to 100 parts water)

Avoid over saturation and ensure the product does not stay wet longer than the chemical manufacturer's guidelines for proper disinfecting.



CAUTION

SOME CLEANING PRODUCTS ARE CORROSIVE IN NATURE AND MAY CAUSE DAMAGE TO THE PRODUCT IF USED IMPROPERLY. If the products described above are used to clean Stryker patient care equipment, measures must be taken to ensure the beds are wiped with a damp cloth soaked in clean water and thoroughly dried following cleaning. Failure to properly rinse and dry the beds will leave a corrosive residue on the surface of the bed, possibly causing premature corrosion of critical components. Failure to follow the above directions when using these types of cleaners may void this product's warranty.

For mattress cleaning instructions, please see the tag on the mattress, or contact the mattress manufacturer.

Clean Velcro® **after each use**. Saturate Velcro® with disinfectant and allow disinfectant to evaporate. (Appropriate disinfectant for nylon Velcro® should be determined by the hospital.)

Troubleshooting Guide

Note

See "Bed Circuit Boards" section for an outline of bed PCB's and voltage test points.

Problem / Failure		Recommended Action
No Power to Bed. (On wall voltage 120VAC)		<div>1. Verify the bed is plugged into a functional wall outlet. A. Check your country voltage option at wall outlet. I. If your country voltage option is present, go to step 2. II. If 1your country voltage option is not present, contact hospital maintenance staff and try another outlet.</div> <div>2. Verify the Bed main power fuses are good, located in drawer where power cord plugs into the bed. A. Check for continuity of each 10A fuse. I. If each fuse (see CV Table) is good, go to step 3. II. If either fuse (see CV Table) does not have continuity, replace the fuse.</div> <div>3. Verify there is power at the transformer connection (J11) on the CPU/Power board at the foot end. A. Check for 24VAC at J11 between the blue and red wires. I. If 24VAC is present, go to step 4. II. If 24VAC is not present, check the 25 Amp fuse in the fuse holder on the red wire from the transformer. If bad, replace the fuse. III. If 24VAC is not present, check the power cable quick connection going to the transformer for (see CV Table) VAC. If no voltage, follow the cable and repair or replace the damaged component. IV. If (see CV Table) VAC is present, replace the transformer assembly.</div> <div>4. A. Check for 30VAC at J11 between the yellow and orange wires for the transformer. I. If 30VAC is present, go to step 5. II. If 30VAC is not present, check the power cable quick connection going to the transformer for (see CV Table) VAC. If no voltage, follow the cable and repair or replace the damaged component. III. If (see CV Table) VAC is present, replace the transformer assembly.</div> <div>5. A. Check fuse F1 on the CPU/Power board. I. If fuse is good, replace CPU/Power board. II. If fuse does not have continuity, replace the fuse (littelfuse 215008.P).</div>
COUNTRY VOLTAGE (CV) TABLE		
VOLTAGE	FUSE	
100V	10A	
110V	10A	
120V	10A	
200V	10A	
220V	10A	
230V	10A	
240V	10A	

Troubleshooting Guide

Problem / Failure		Recommended Action
No Bed Up Motion.	FOOT	<ol style="list-style-type: none"> 1. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the trend button. <ol style="list-style-type: none"> I. If the foot lift motor runs up, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the litter angle sensor and recalibrate. II. If the foot lift motor does not run up, check for 24VDC at connector J6 while pressing the trend button. Black lead to pin 1, red lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.
	HEAD	<ol style="list-style-type: none"> 1. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the bed up button. <ol style="list-style-type: none"> I. If the head lift motor runs up, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the litter angle sensor and recalibrate. II. If the head lift motor does not run up, check for 24VDC at connector J4 while pressing the trend button. Black lead to pin 1, red lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.
No Bed Down Motion.	FOOT	<ol style="list-style-type: none"> 1. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the reverse trend button. <ol style="list-style-type: none"> I. If the foot lift motor runs down, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the litter angle sensor and recalibrate. II. If the foot lift motor does not run down, check for 24VDC at connector J6 while pressing the reverse trend button. Red lead to pin 1, black lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.
	HEAD	<ol style="list-style-type: none"> 1. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the bed down button. <ol style="list-style-type: none"> I. If the head lift motor runs down, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the litter angle sensor and recalibrate. II. If the head lift motor does not run down, check for 24VDC at connector J4 while pressing the trend button. Red lead to pin 1, black lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.

Troubleshooting Guide

Problem / Failure	Recommended Action
No Fowler Up Motion.	<ol style="list-style-type: none"> 1. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the fowler up button. <ol style="list-style-type: none"> I. If the fowler motor runs up, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the fowler angle sensor and recalibrate. II. If the fowler motor does not run up, check for 24VDC at connector J5 while pressing the fowler up button. Black lead to pin 1, red lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.
No Fowler Down Motion.	<ol style="list-style-type: none"> 1. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the fowler down button. <ol style="list-style-type: none"> I. If the fowler motor runs down, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the fowler angle sensor and recalibrate. II. If the fowler motor does not run down, check for 24VDC at connector J5 while pressing the fowler down button. Red lead to pin 1, black lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.
No Gatch Up Motion.	<ol style="list-style-type: none"> 1. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the gatch up button. <ol style="list-style-type: none"> I. If the gatch motor runs up, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the gatch angle sensor and recalibrate. II. If the gatch motor does not run up, check for 24VDC at connector J3 while pressing the gatch up button. Red lead to pin 1, black lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.

Troubleshooting Guide

Problem / Failure	Recommended Action
No Gatch Down Motion.	<ol style="list-style-type: none"> 1. Go to the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the gatch down button. <ol style="list-style-type: none"> I. If the gatch motor runs down, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the gatch angle sensor and recalibrate. II. If the gatch motor does not run down, check for 24VDC at connector J3 while pressing the gatch down button. Black lead to pin 1, red lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.
No Foot Up Motion.	<ol style="list-style-type: none"> 1. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the foot up button. <ol style="list-style-type: none"> I. If the foot motor runs up, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the foot angle sensor and recalibrate. II. If the foot motor does not run up, check for 24VDC at connector J1 while pressing the foot up button. Red lead to pin 1, black lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.
No Foot Down Motion.	<ol style="list-style-type: none"> 1. Ensure there is no debris in the foot end traction sockets. If debris exists, remove it and press the foot down button. If the foot motor still does not run down, proceed to step 2. 2. Put the bed into the Bed Calibration menu. <ol style="list-style-type: none"> A. Using one of the head siderails, push the foot down button. <ol style="list-style-type: none"> I. If the foot motor runs down, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> a. If recalibration does not work, replace the foot angle sensor and recalibrate. II. If the foot motor does not run down, check for 24VDC at connector J1 while pressing the foot down button. Black lead to pin 1, red lead to pin 2. <ol style="list-style-type: none"> a. If voltage is present, replace the motor. b. If voltage is not present, replace the CPU/Power board.

Troubleshooting Guide

Problem / Failure	Recommended Action
No Trendelenburg Motion.	<ol style="list-style-type: none"> Check the touch screen trend angle display for accuracy of the level of the litter. <ol style="list-style-type: none"> If not accurate, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> If recalibration does not work, replace the trend angle sensor and recalibrate. If replacement of the trend angle sensor did not resolve the problem, replace the CPU/Power board.
No Reverse Trendelenburg Motion.	<ol style="list-style-type: none"> Check the touch screen trend angle display for accuracy of the level of the litter. <ol style="list-style-type: none"> If not accurate, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> If recalibration does not work, replace the trend angle sensor and recalibrate. If replacement of the trend angle sensor did not resolve the problem, replace the CPU/Power board.
No Cardiac Chair Motion.	<ol style="list-style-type: none"> Check the touch screen fowler and foot section angle display for accuracy of the angle of the fowler and foot section. <ol style="list-style-type: none"> If not accurate, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> If recalibration does not work, replace the fowler or foot section angle sensor depending on the one which was not accurate, then recalibrate. If replacement of the fowler or foot section angle sensor did not resolve the problem, replace the CPU/Power board.
HOB 30°.	<ol style="list-style-type: none"> Check the touch screen fowler angle display for accuracy of the angle of the fowler. <ol style="list-style-type: none"> If not accurate, recalibrate the bed (refer to the Bed Calibration procedures located on page 23). <ol style="list-style-type: none"> If recalibration does not work, replace the fowler angle sensor and recalibrate. If replacement of the fowler angle sensor did not resolve the problem, replace the CPU/Power board.

Troubleshooting Guide

Problem / Failure	Recommended Action
No Vascular Motion.	<ol style="list-style-type: none">1. Check the touch screen fowler, gatch, foot, and trend/rev. trend display for accuracy of the angle of all.<ol style="list-style-type: none">I. If not accurate, recalibrate the bed (refer to the Bed Calibration procedures located on page 23).<ol style="list-style-type: none">a. If recalibration does not work, replace the angle sensor of the section that is not accurate and then recalibrate the bed (refer to the Bed Calibration procedures located on page 23).b. If replacement of the fowler angle sensor did not resolve the problem, replace the CPU/Power board.
No Electric Brake Motion.	<ol style="list-style-type: none">1. Verify the Brake Not Set LED is flashing and the Brake Set LED is OFF.<ol style="list-style-type: none">I. If the Brake Set LED is ON, check manual brake position.<ol style="list-style-type: none">a. If manual brake pedal is in the brake position, the bed should not move and is okay; go to step 2.b. If manual brake is not in the brake position, check the switch on the patients left side in the middle below the base hood.2. If the brake motor does not run down when the brake button is pushed, check for 24VDC at connector J7 while pressing the brake button. Black lead to pin 1, red lead to pin 2.

Troubleshooting Guide

SCALE TROUBLESHOOTING

When the Scale System is unable to correctly weigh the patient weight due to a problem with the electronics, Figure 39 will be displayed. It also appears when there is a problem with the Trendelenberg angle sensor; thus the value for the weight and the angle cannot be displayed.

When the weight exceeds 550 lbs., Figure 40 will be displayed. If the weight is less than 2 lbs., the screen will display "0 lb."

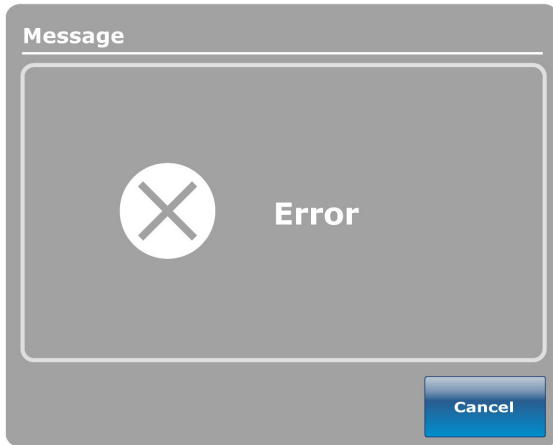


Figure 39

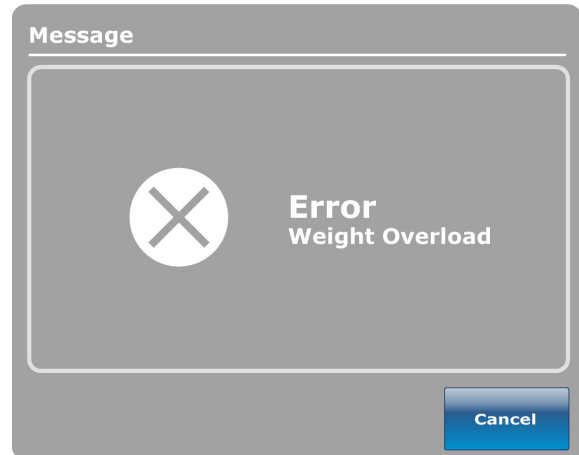


Figure 40

When the Trendelenburg or Reverse Trendelenburg angle is above 12° or below -12° , Figure 41 will be displayed.

When the scale system is unstable due to a problem with scale electronics or excessive patient movement, the weight reading will be orange in color as shown in Figure 42.

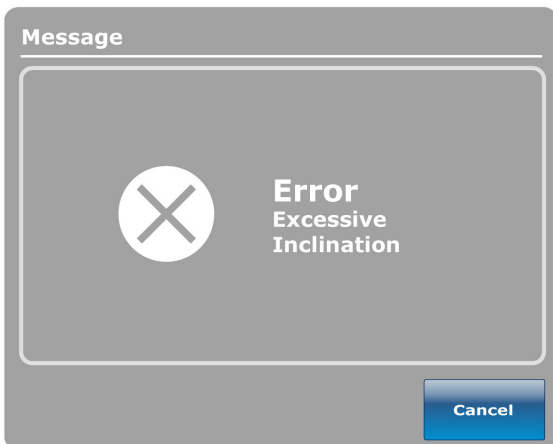


Figure 41



Figure 42

Maintenance Error Messages

ERROR HANDLING

- There are two different CAN networks; each of the networks is divided into two connectors.
- A safe error without command can be obtained when a bad connection is carried out on the Power Sensor Board when the control panel is defective (there is no message sent on the network when a button is pressed) or when the network is defective (short-circuit between the signals, open circuit or defective network circuit).
- A command error without safe is obtained when a bad connection is done on the Power Sensor board, when the control panel is defective (a message is sent over the network but not the safe signal) or when the safe signal is defective (short-circuit panel or open circuit or safe circuit on the Power Sensor board is broken).
- These errors can be present when a button is pressed, or at any time, and will thus cause the Call Maintenance LED to light up.
- There is a LED on the Power Sensor Board (DS2 SAFE) which is active when there is at least one safe signal which is active. There are also four LEDs on the Power Sensor board, which shows the activity of the network. Every time a message is sent on the network, the LEDs will flash. If the network is defective, the LEDs will remain on or remain off. If there is nothing connected to the network, the LEDs will remain on or off.
- A safe error can be obtained if a command button is pressed without having the Power Sensor Board receiving a safe signal or if a safe signal is received by the Power Sensor board without having any command button pressed.
- The control panel for the weighing scale of the Power Sensor board can also send errors to the micro-controller which will display them. An error of the weighing scale control panel will light on the Call Maintenance LED.

ERROR MESSAGES

Touch Screen Error Messages Name	Definition
Atd Invalid Values	Digital to analog converter is damaged (Replace the Control Board).
Brake pot bad range	Verify if potentiometer is still in place.
Brake unable to elec ctl	Verify wiring to Brake motor and limit switch for manual engage.
Brake pot Disconnected or short	Verify wiring to potentiometer and replace potentiometer. Ensure potentiometer is still in place.
Brake motor time out	Verify wiring to brake motor.
Calibration Error	Previous calibration step performed incorrectly, redo calibration procedure.
Cmd WO safe from nurse SRR	Right siderail outside board has a network communication error (Check network connections, dip-switch configuration of board or if a button is stuck).
Cmd WO safe from nurse SRL	Left siderail outside board has a network communication error (Check network connections, dip-switch configuration of board or if a button is stuck).
Cmd WO safe from nurse SRH	Head end board has a network communication error (Check network connections).
Cmd WO safe from pat pend R	Optional pendant control has a network communication error (Check network connections).
Cmd WO safe from pat pend L	Optional pendant control has a network communication error (Check network connections).
Cmd WO safe from pat pend H	Optional pendant control has a network communication error (Check network connections).
Cmd WO safe from TS	Touch screen has a network communication error (Check network connections).

Maintenance Error Messages

ERROR MESSAGES (CONTINUED)

Touch Screen Error Messages Name	Definition
Cmd WO safe from room	Communication board has a network communication error (Check network connections).
Cmd WO safe from room	Communication board has a network communication error (Check network connections).
GPIO Failure Init	Initialization of the PCA9555 (GPIO expansion chip) failed (Replace control board).
GPIO Failure Read	Reading from the PCA9555 (GPIO expansion chip) failed (Replace control board).
GPIO Failure Write	Writing to the PCA9555 (GPIO expansion chip) failed (Replace control board).
Limit switch head side rail right	Verify wiring to limit switch and replace limit switch.
Limit switch head side rail left	Verify wiring to limit switch and replace limit switch.
Limit switch foot side rail right	Verify wiring to limit switch and replace limit switch.
Limit switch foot side rail left	Verify wiring to limit switch and replace limit switch.
Foot Right Load cell over range	Foot Right load cell or cabling is damaged (Replace load cell).
Head Right cell over range	Head Right load cell or cabling is damaged (Replace load cell).
Foot Left Load cell over range	Foot Left load cell or cabling is damaged (Replace load cell).
Head Left Load cell over range	Head Left load cell or cabling is damaged (Replace load cell).
Motor Brake Overheat	Brake motor has ran too long (Leave motor stationary for 54 minutes).
Motor Brake Overload	Brake motor is drawing too many AMPS (remove restriction or replace motor).
Motor Foot Overheat	Foot motor has ran too long (Leave motor stationary for 54 minutes).
Motor Foot Overload	Foot motor is drawing too many AMPS (remove restriction or replace motor).
Motor Gatch Overheat	Gatch motor has ran too long (Leave motor stationary for 54 minutes).
Motor Gatch Overload	Gatch motor is drawing too many AMPS (remove restriction or replace motor).
Motor Head Overheat	Fowler motor has ran too long (Leave motor stationary for 54 minutes).
Motor Head Overload	Fowler motor is drawing too many AMPS (remove restriction or replace motor).
Motor HL Foot Overheat	Foot lift motor has ran too long (Leave motor stationary for 54 minutes).
Motor HL Foot Overload	Foot lift motor is drawing too many AMPS (remove restriction or replace motor).
Motor HL Head Overheat	Head lift motor has ran too long (Leave motor stationary for 54 minutes).
Motor HL Head Overload	Head lift motor is drawing too many AMPS (remove restriction or replace motor).
Motor Zoom® Overheat	Zoom® motor has ran too long (Leave motor stationary for 54 minutes).
Motor Zoom® Overload	Zoom® motor is drawing too many AMPS (remove restriction or replace motor).
No Error	Angle sensor failure or calibration issue.
One Motor Drive Short	Short on drive motor detected.
Safe WO Cmd from A1	Network A1 has a wiring issue (Check cabling).
Safe WO Cmd from A2	Network A2 has a wiring issue (Check cabling).
Safe WO Cmd from B1	Network B1 has a wiring issue (Check cabling).

Maintenance Error Messages

ERROR MESSAGES (CONTINUED)

Touch Screen Error Messages Name	Definition
Safe WO Cmd from B2	Network B2 has a wiring issue (Check cabling).
Scale ADC Error	Scale chip not calibrated. DC Control Board needs to be replaced.
Scale Chip Failure	Control board is bad (Replace Control Board).
Tilt base over range	Verify if tilt sensor is still in place. Inspect for a damaged or improperly assembled tilt sensor or recalibrate bed.
Tilt Error Base	Angle sensor is damaged (Replace sensor).
Tilt Error Foot	Angle sensor is damaged (Replace sensor).
Tilt Error Gatch	Angle sensor is damaged (Replace sensor).
Tilt Error Head	Angle sensor is damaged (Replace sensor).
Tilt Error HiLo Foot	Angle sensor is damaged (Replace sensor).
Tilt Error Trend	Angle sensor is damaged (Replace sensor).
Tilt foot over range	Verify if tilt sensor is still in place. Inspect for a damaged or improperly assembled tilt sensor or recalibrate bed.
Tilt gatch over range	Verify if tilt sensor is still in place. Inspect for a damaged or improperly assembled tilt sensor or recalibrate bed.
Tilt head over range	Verify if tilt sensor is still in place. Inspect for a damaged or improperly assembled tilt sensor or recalibrate bed.
Tilt hiLo foot over range	Verify if tilt sensor is still in place. Inspect for a damaged or improperly assembled tilt sensor or recalibrate bed.
Tilt trend over range	Verify if tilt sensor is still in place. Inspect for a damaged or improperly assembled tilt sensor or recalibrate bed.
Zoom® time out for switch	Verify wiring to Zoom® motor.
Wi-Fi / IR Communication Error	Definition
Wireless Adapter Failure	Unable to detect or communicate with Wi-Fi radio. Check assembly or cabling of Wi-Fi card in footboard or replace Wi-Fi card or footboard.
DHCP Error: Unable to obtain IP Address	Bed is not able to connect to the wireless network. Check wireless network settings and Wi-Fi configuration of bed.
Unable to connect to network	Bed is not able to connect to the wireless network. Check wireless network settings and Wi-Fi configuration of bed.
Fixed IP Address duplication	IP Address conflict with other devices on the network. Make sure Fixed IP address on every bed is unique.
Internal Communication Error	Internal software failure. Software corruption may have occurred. Re-upload software or replace footboard.
Wi-Fi Settings corrupted	Reconfigure Wi-Fi settings in bed.
Bed Serial Number not available	Configure bed serial number.
Left IR Module not detected	Unable to detect IR module. Check cabling or replace the IR module.
Right IR Module not detected	Unable to detect IR module. Check cabling or replace the IR module.
IR Interface Board not detected	Unable to detect the Room interface board. Check cabling or replace the Room interface board.
IR Crosstalk detected	Crosstalk detected with iBed Locator Wall module. Verify placement of IR modules on bed or wall modules.
Internal Media Storage Error	Definition
Internal Media storage not detected	Unable to access internal storage memory. Check assembly or cabling of memory card in footboard or replace footboard.

Quick Reference Replacement Parts List


The parts and accessories listed on this page are all currently available for purchase. Some of the parts identified on the assembly drawing parts in this manual may not be individually available for purchase. Please call Stryker Customer Service USA: 1-800-327-0770 for availability and pricing.

Part Name	Part Number
Electrical Components	
Actuator, Brake	QDF27-1227
Actuator, Foot	QDF27-1216
Actuator, Fowler	QDF27-1214
Actuator, Gatch	QDF27-1215
Actuator, Lift, Foot End	QDF27-1251
Actuator, Lift, Head End	QDF27-1252
Angle Sensor, Foot, Fowler, Base, Gatch, Lift (U01001 - U02817)	27-1209
Angle Sensor, Foot, Fowler, Base, Gatch, Lift (U021818 - Current)	27-2477
Batteries (Replace both at same time)	QDF9188
Board, CPU/Power	QDF75-0440
Board, Drive (2141 Zoom® Only)	QDF27-1430
Board, Headwall	QDF75-0270
Board, Brake Control	QDF27-1097
Board, Footboard, Function Section/LED's	QDF75-0010
Board, Siderail, Outside (Bed Motion)	QDF27-1099
Board, Touch Screen, Foot	QDF2125
Fuse, 8Amp Ceramic	QDF2120
Fuse, 10Amp, Main Power	QDF8078
Fuse, 25Amp Cartridge	QDF2119
Load Cell	QDF27-1372
Motor, Drive (2141 Zoom® Only)	QDF27-1445
Motor, Drive Actuator (2141 Zoom® Only)	27-2593
Position Sensor, Brake/Brake Off/Drive	QDF27-2024
Power Cord	QDF8066
Speaker, Right Siderail	QDF27-2216
Speaker, Left Siderail	QDF27-2175
Touch Screen, Footboard	QDF27-2193
Transformer (120VAC)	QDF27-2038

Quick Reference Replacement Parts List

Part Name	Part Number
Other Components	
Caster (2141 Model - all four casters) (2131 Model - both head end casters)	RD27-1970
Caster, Steer (2131 Model Only - both foot end casters)	RD27-1971
Headboard Assembly	27-2583K
Footboard Assembly without <i>i</i> Bed	27-2760K
Footboard Assembly with <i>i</i> Bed and <i>i</i> Audio	27-2761K
Footboard Assembly with <i>i</i> Bed and Wi-Fi	27-2762K

CPU/Power Board - QDF75-0440

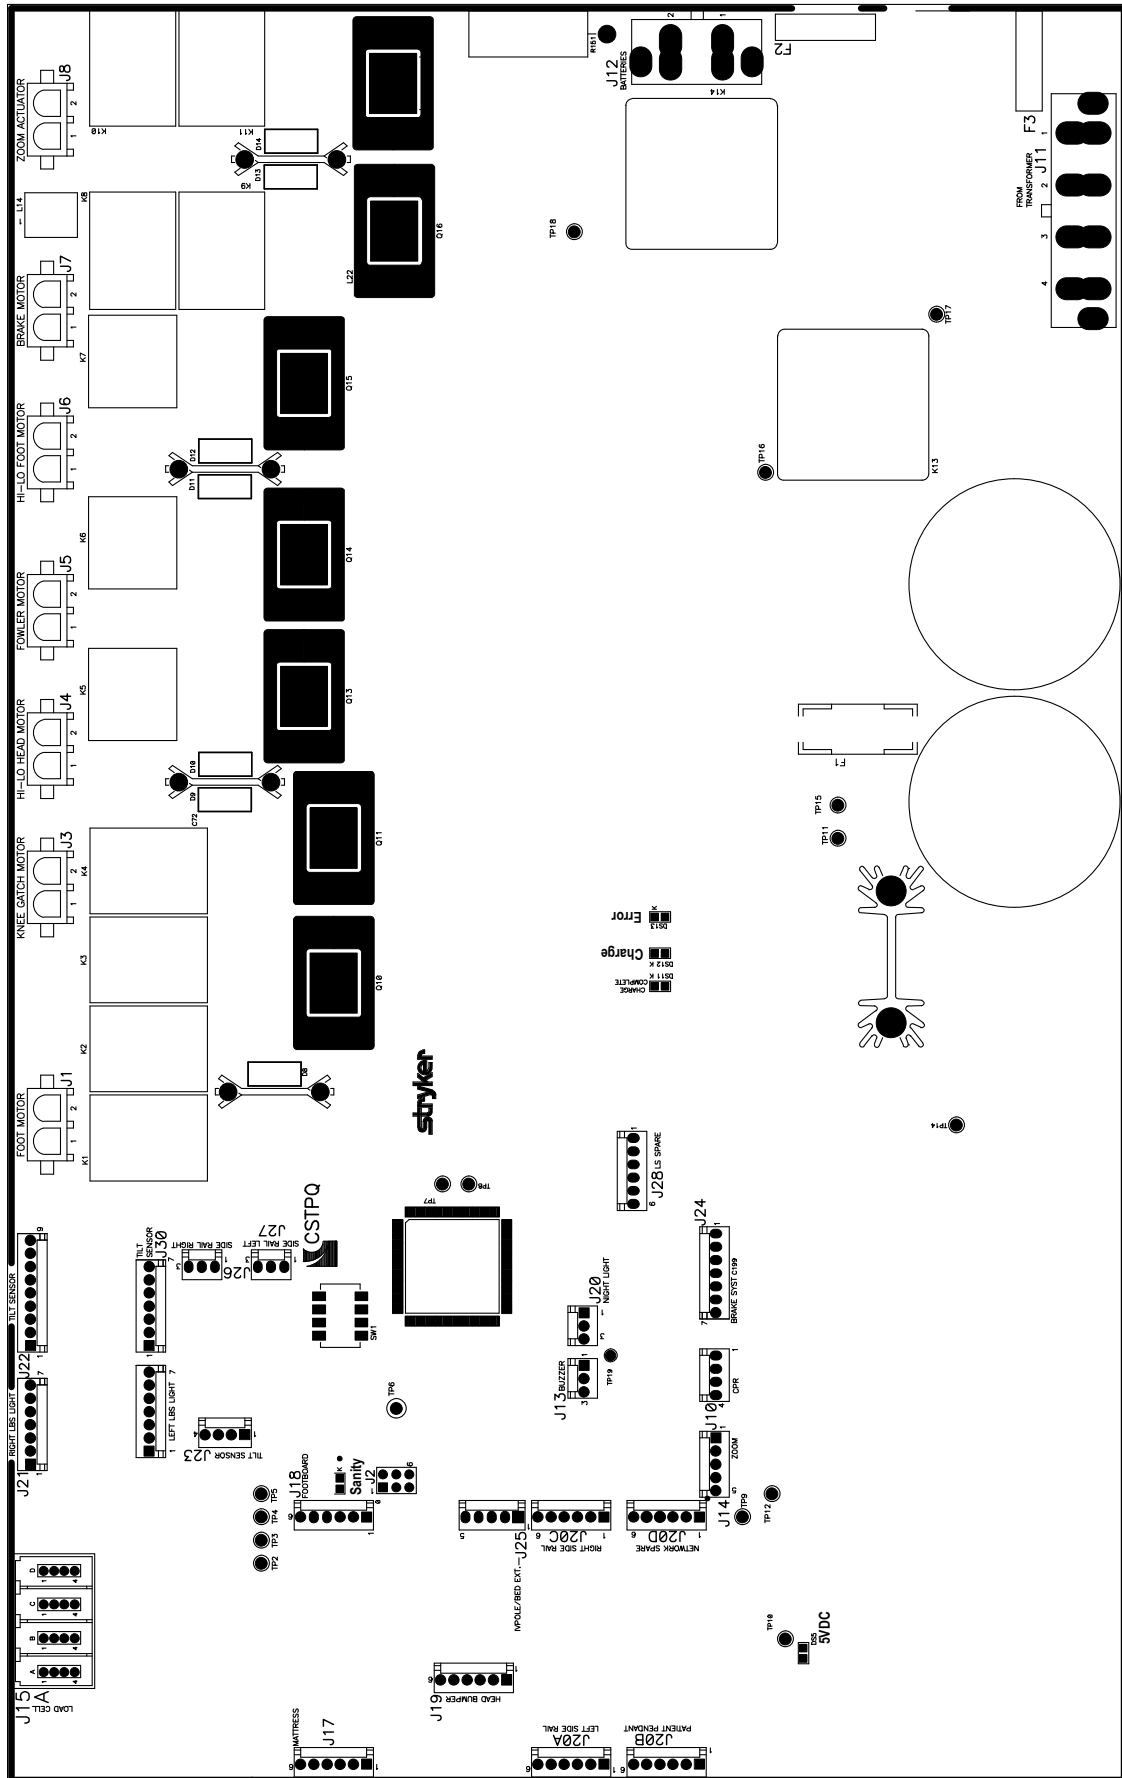

CPU/Power Board - QDF75-0440


FUSE SPECIFICATION

Location	Description	Amp
F1	30VAC from transformer for the battery charger and the 5VDC / 12VDC supply	10 Amp - 215008.P
F2	24 VDC from batteries for power supply	40 Amp - 142.6185.5402
F3	24 VAC from transformer for power supply	40 Amp - 142.6185.5402

Cable Location	Voltage	Positive Lead	Negative Lead	Description
J11	24-31VAC	Blue	Red	Stepped down voltage from transformer for power supply
J11	30-39VAC	Yellow	Orange	Stepped down voltage from transformer for battery charger and power supply
J12	24-29VDC	Pin 1 - Red	Pin 2 - Black	Battery/Charger
J1	24-28VDC	Pin 1 - Black	Pin 2 - Brown	Foot Actuator Up
J1	24-28VDC	Pin 2 - Brown	Pin 1 - Blue	Foot Actuator Down
J3	24-28VDC	Pin 1 - White	Pin 2 - Black	Gatch Actuator Up
J3	24-28VDC	Pin 2 - Black	Pin 1 - White	Gatch Actuator Down
J6	24-28VDC	Pin 2 - White	Pin 1 - Black	Bed Lift-Foot Up
J6	24-28VDC	Pin 1 - Black	Pin 2 - White	Bed Lift-Foot Down
J4	24-28VDC	Pin 2 - White	Pin 1 - Black	Bed Lift-Head Up
J4	24-28VDC	Pin 1 - Black	Pin 2 - White	Bed Lift-Head Down
J5	24-28VDC	Pin 2 - White	Pin 1 - Black	Fowler Actuator Up
J5	24-28VDC	Pin 1 - Black	Pin 2 - White	Fowler Actuator Down
J7	24-28VDC 24-28VDC 24-28VDC	Pin 1 - Black Pin 1 - Black Pin 1 - Black	Pin 2 - White Pin 2 - White Pin 2 - White	Brake/Brake Off/Drive Actuator • Brake • Brake Off • Drive
J8	Bed Unplugged 25VDC 25VDC	Pin 2 - White Pin 1 - Black	Pin 1 - Black Pin 2 - White	Zoom® Drive Actuator (Model 2141 Only)


Bed Electrical Diagram

27-1136 Rev R (Reference Only)

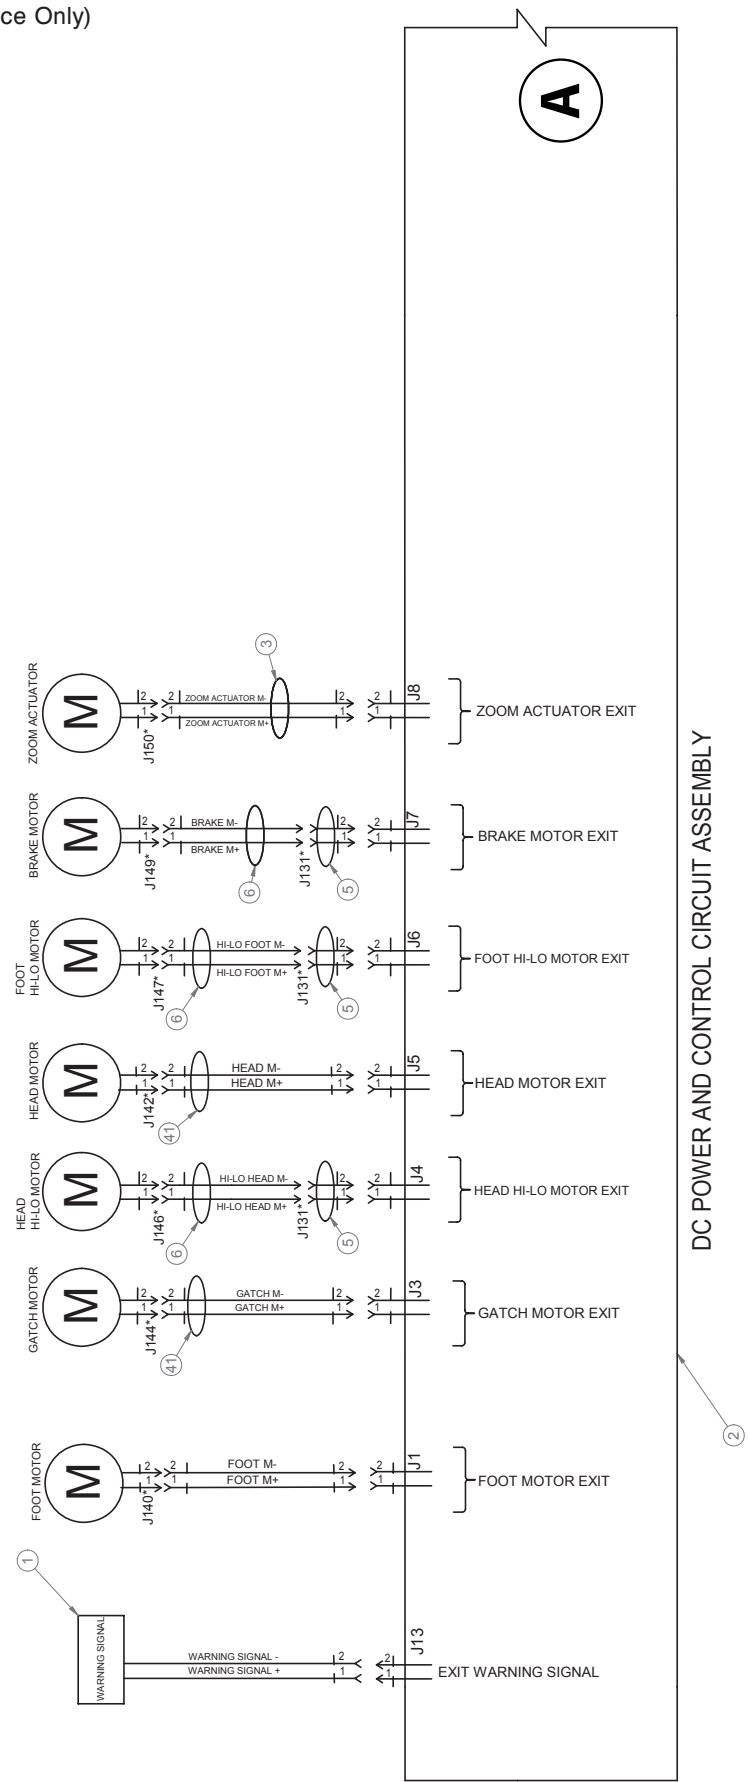


ALL MODELS

Bed Electrical Diagram

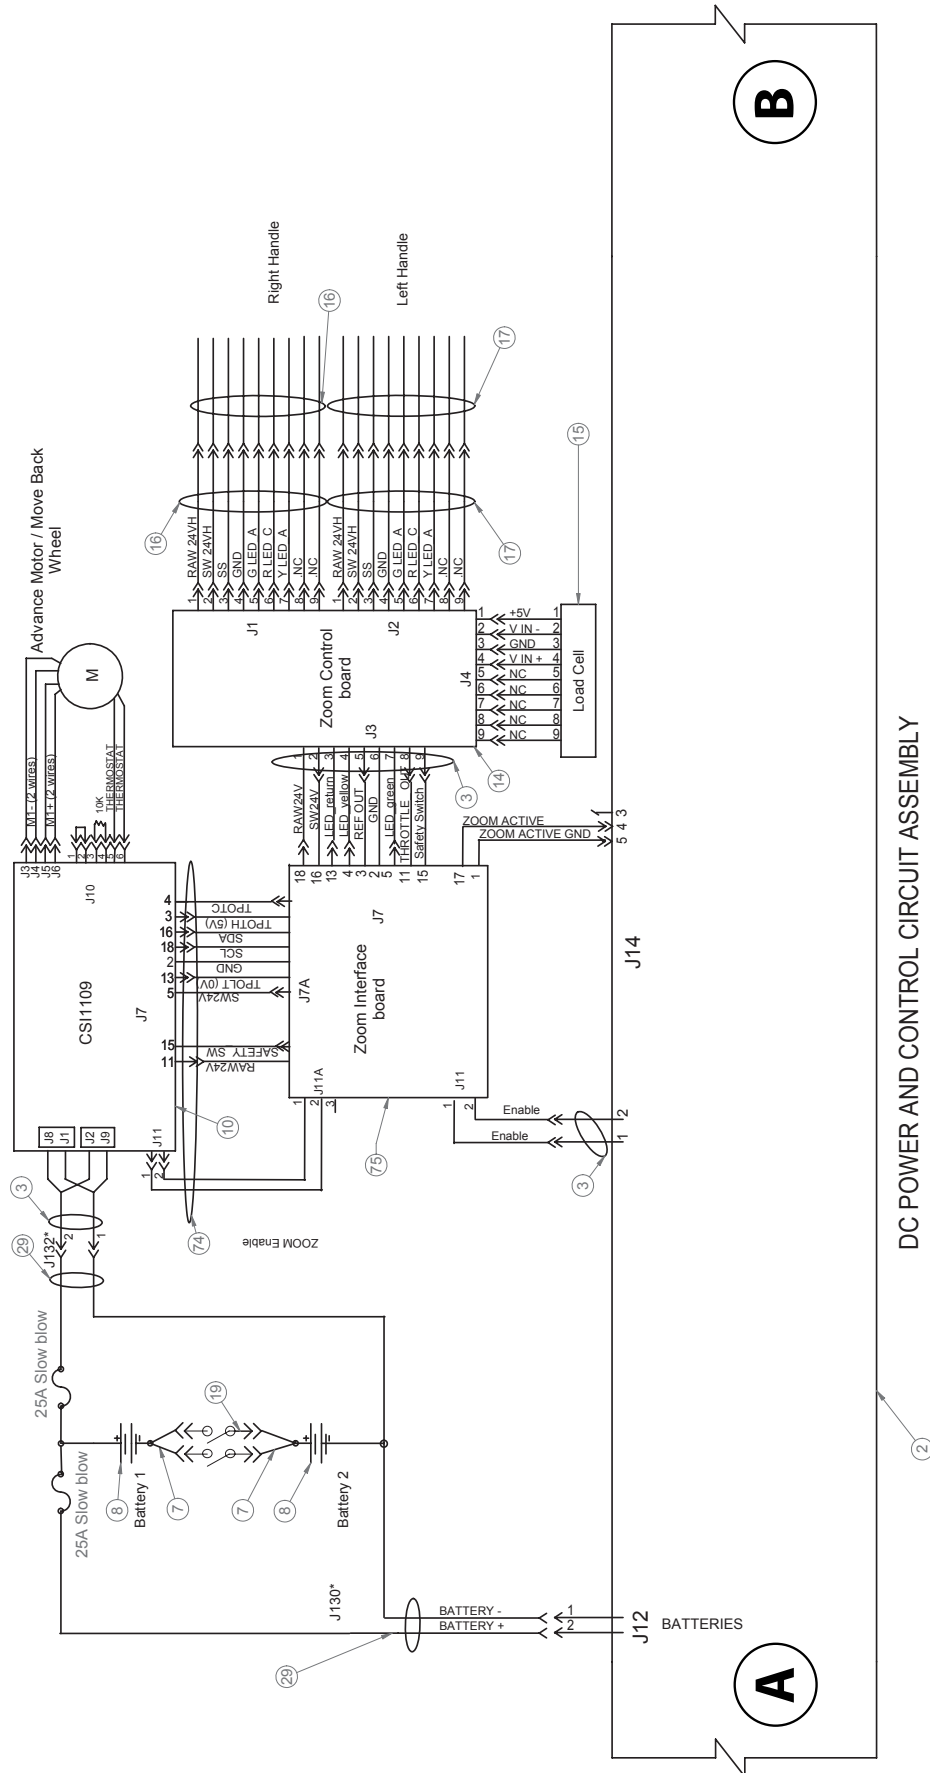


2131 to 2156

Bed Electrical Diagram

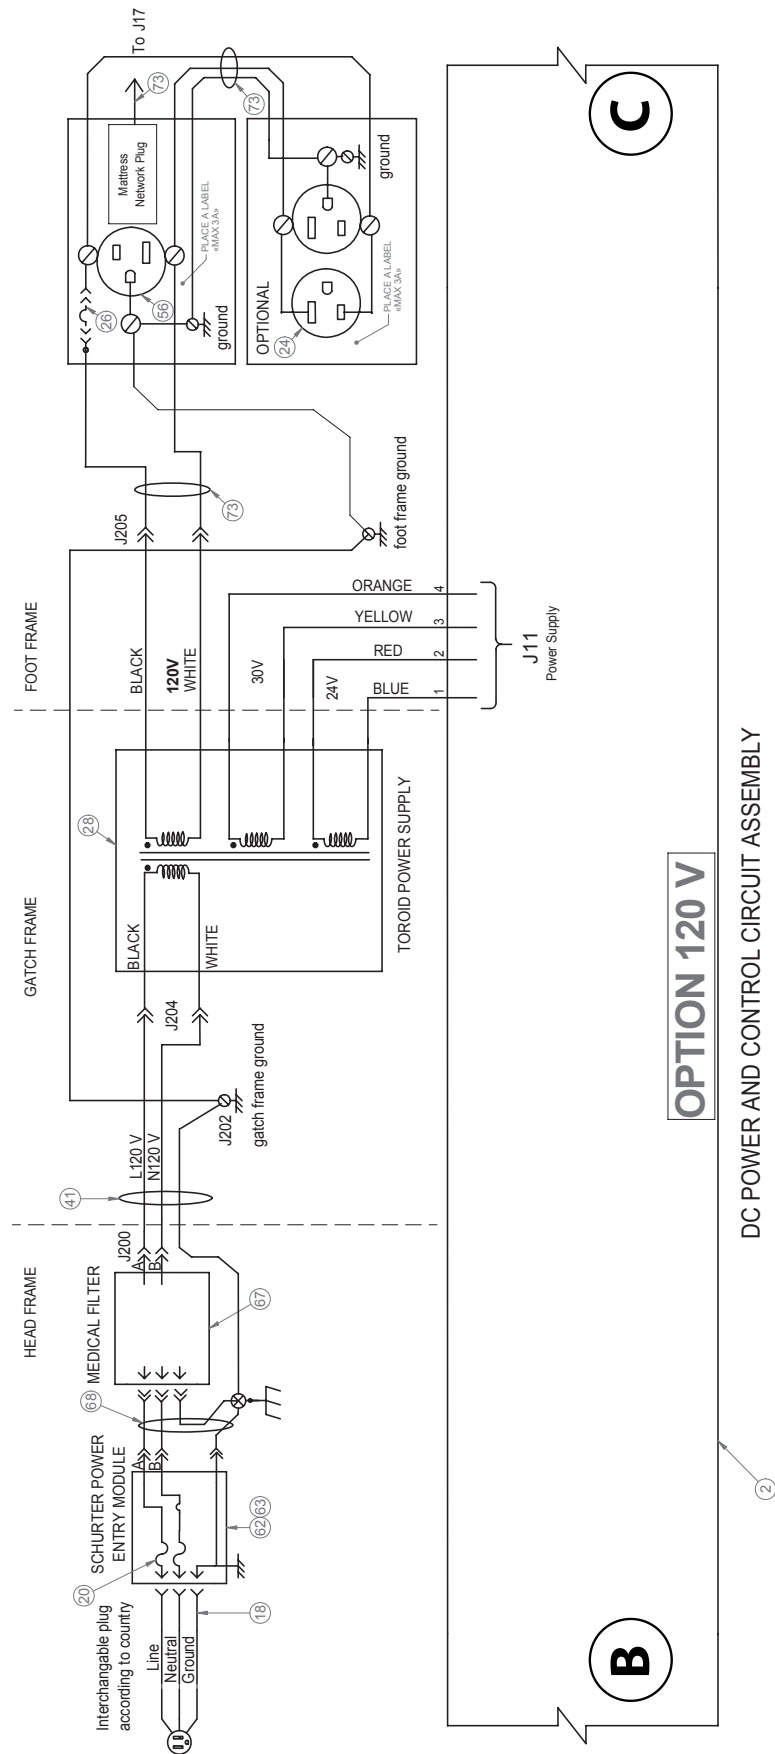


ALL MODELS

Bed Electrical Diagram

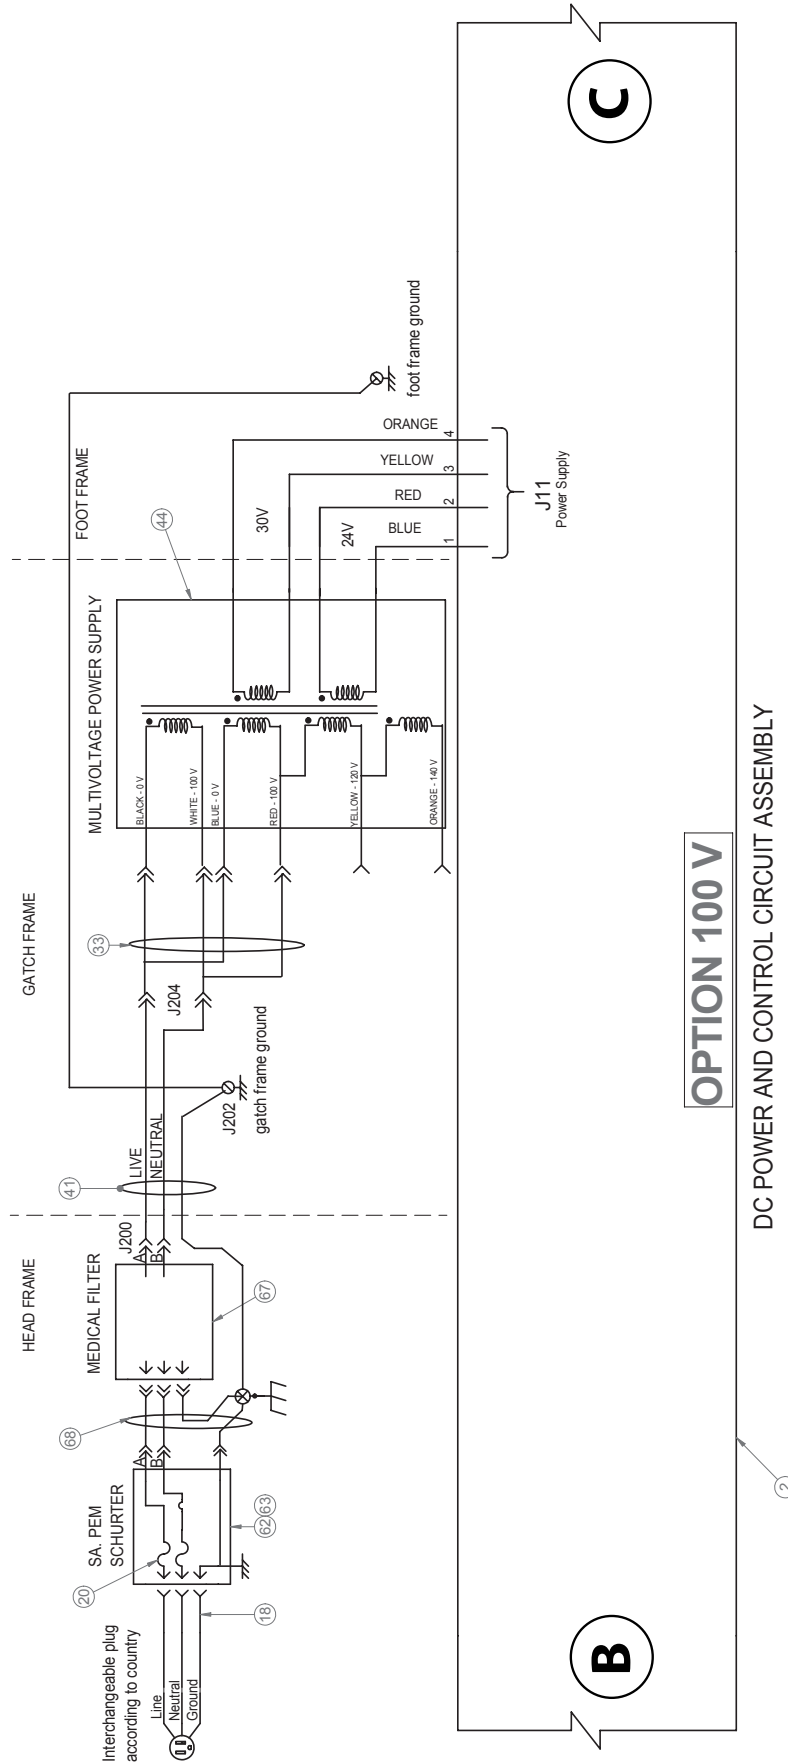


ALL MODELS

Bed Electrical Diagram

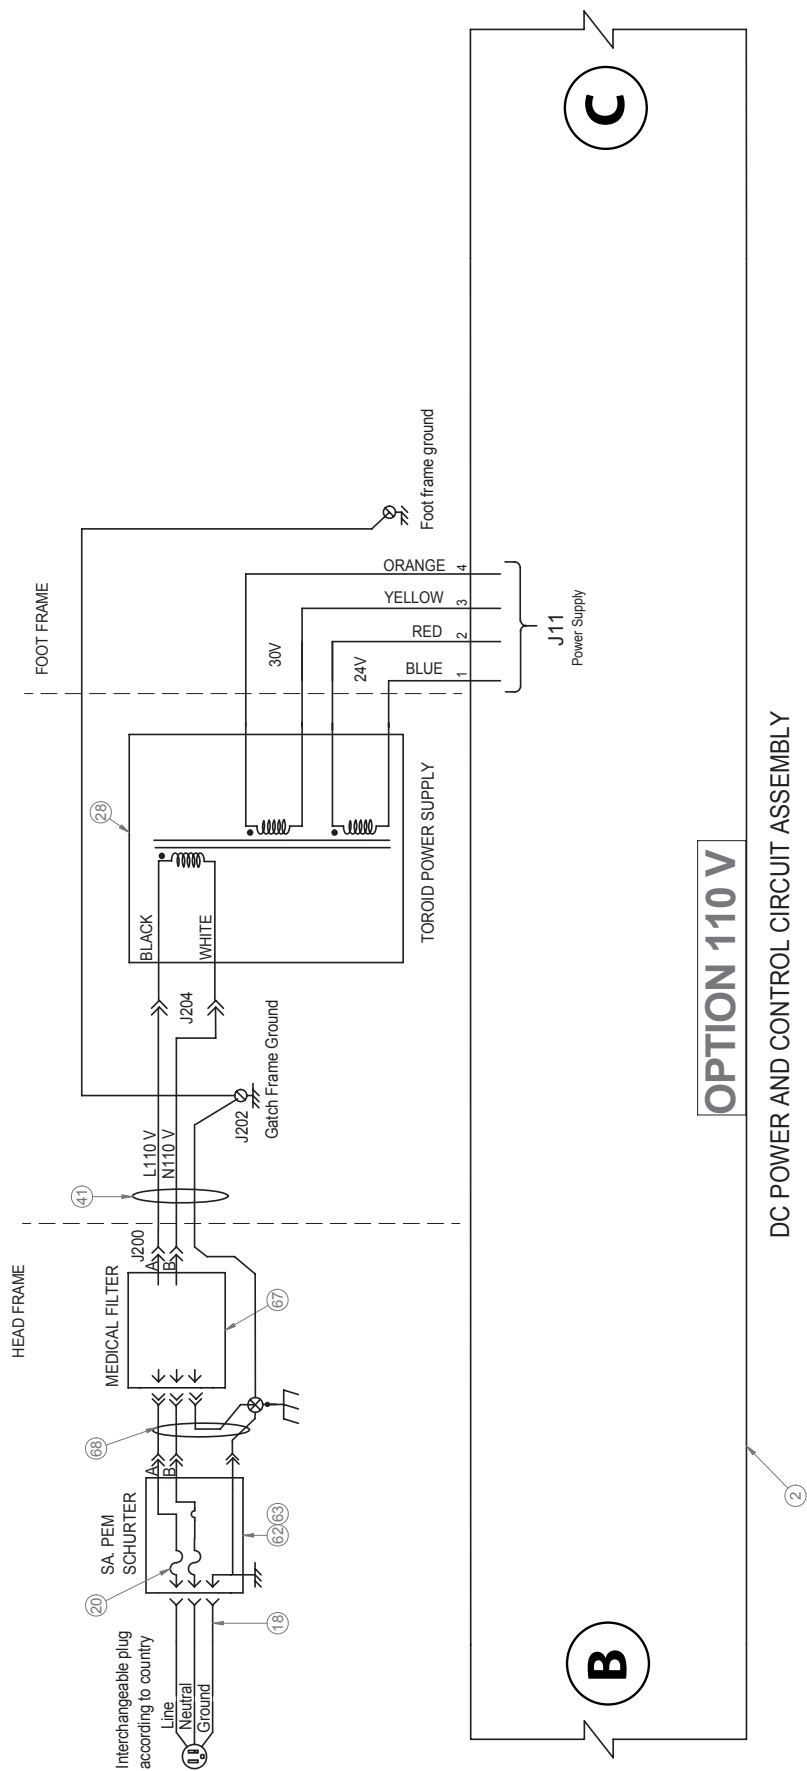


2131 to 2141

Bed Electrical Diagram

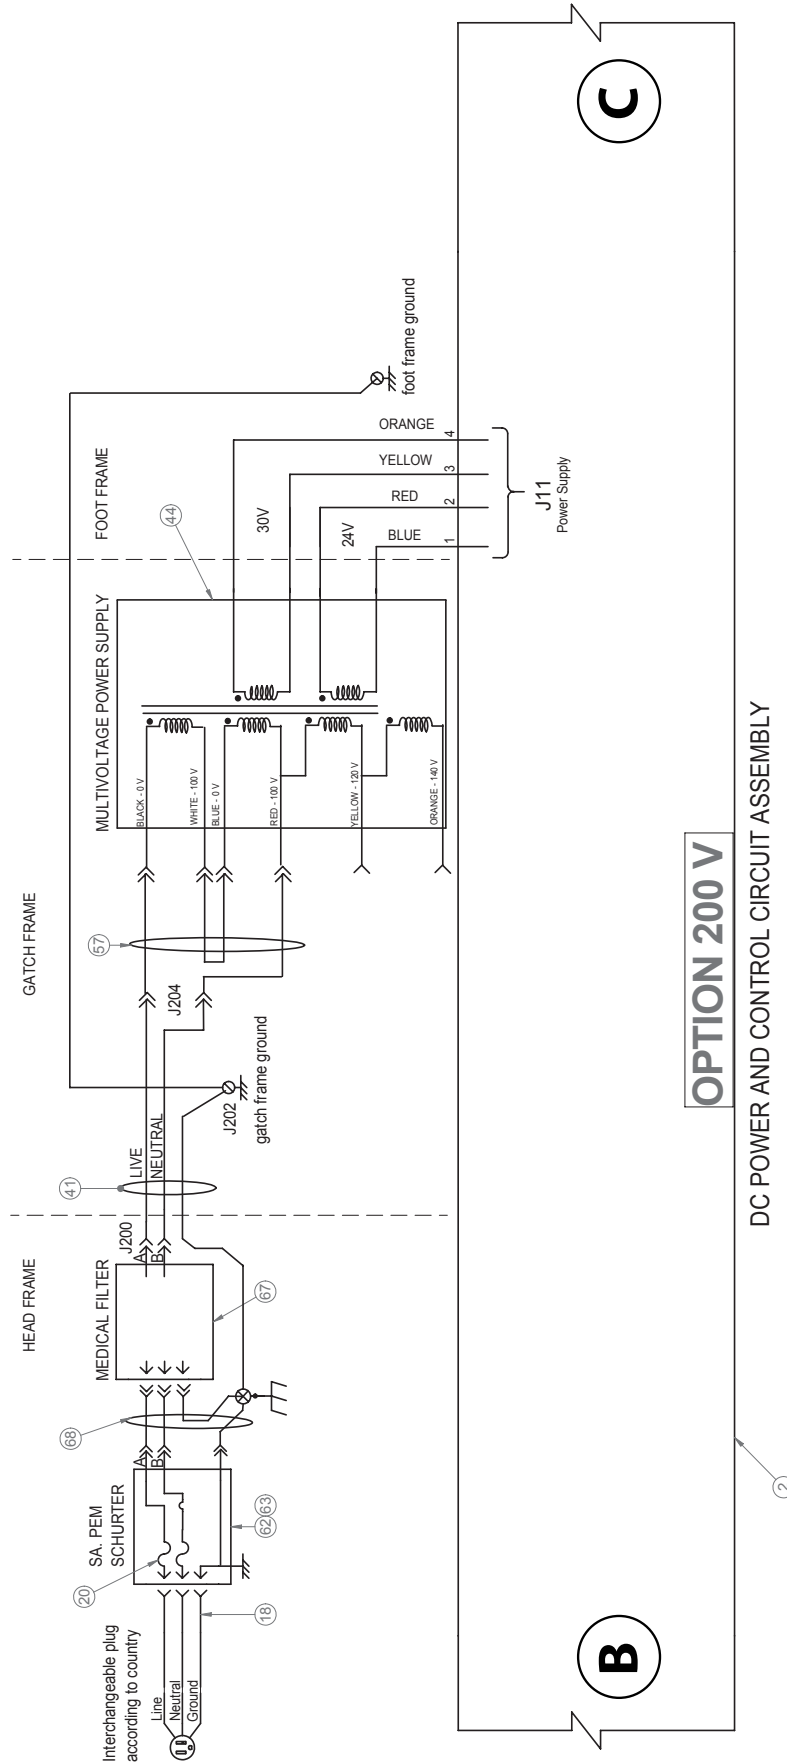


ALL MODELS

Bed Electrical Diagram

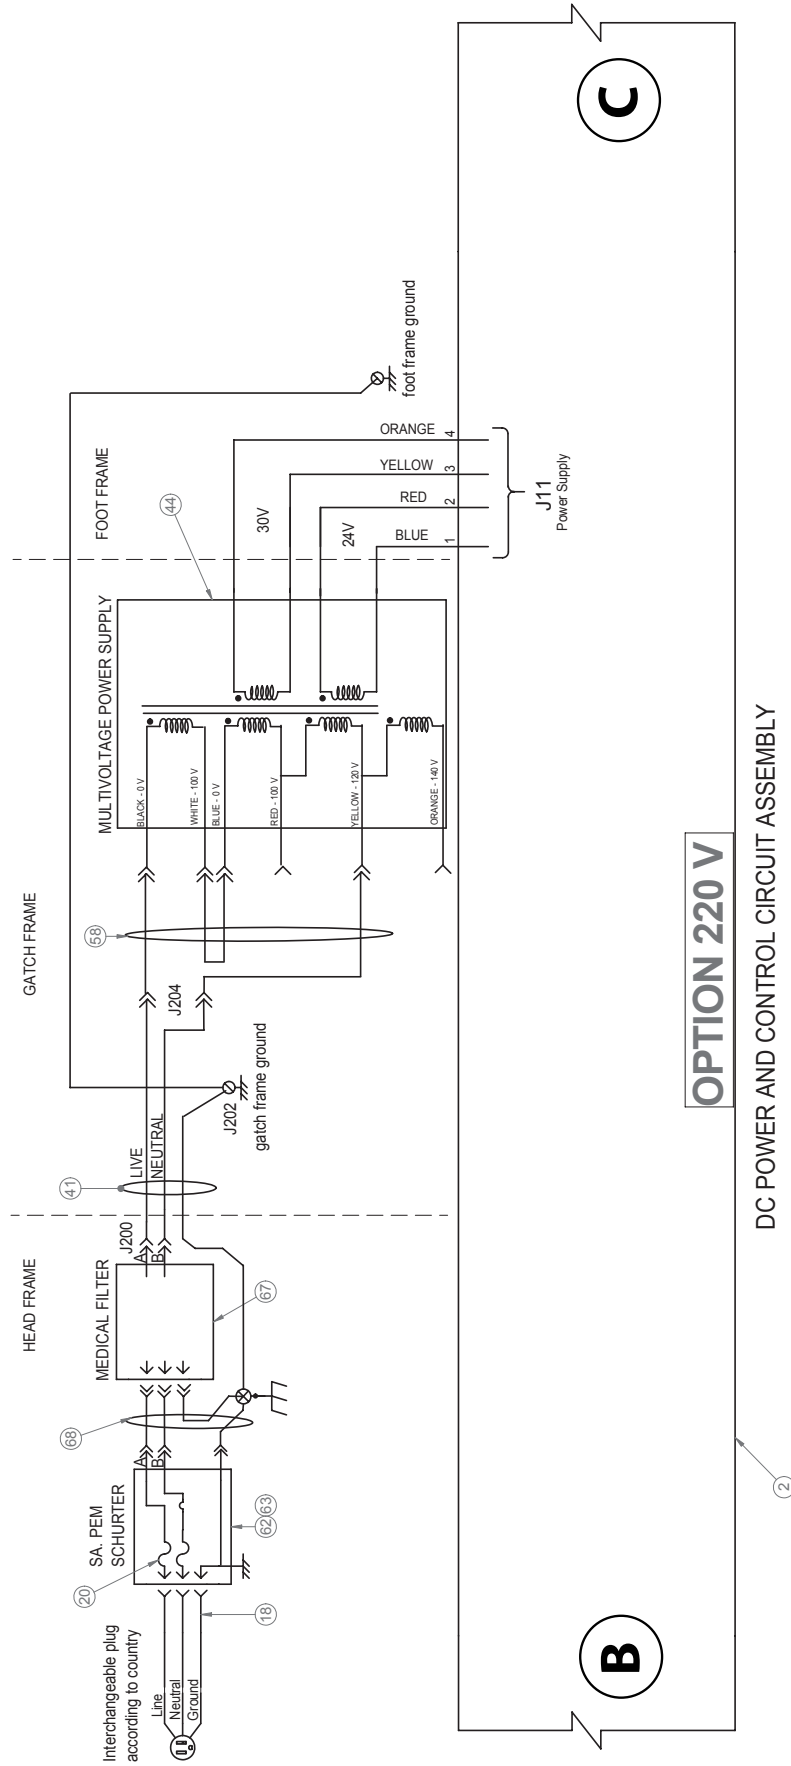


ALL MODELS

Bed Electrical Diagram

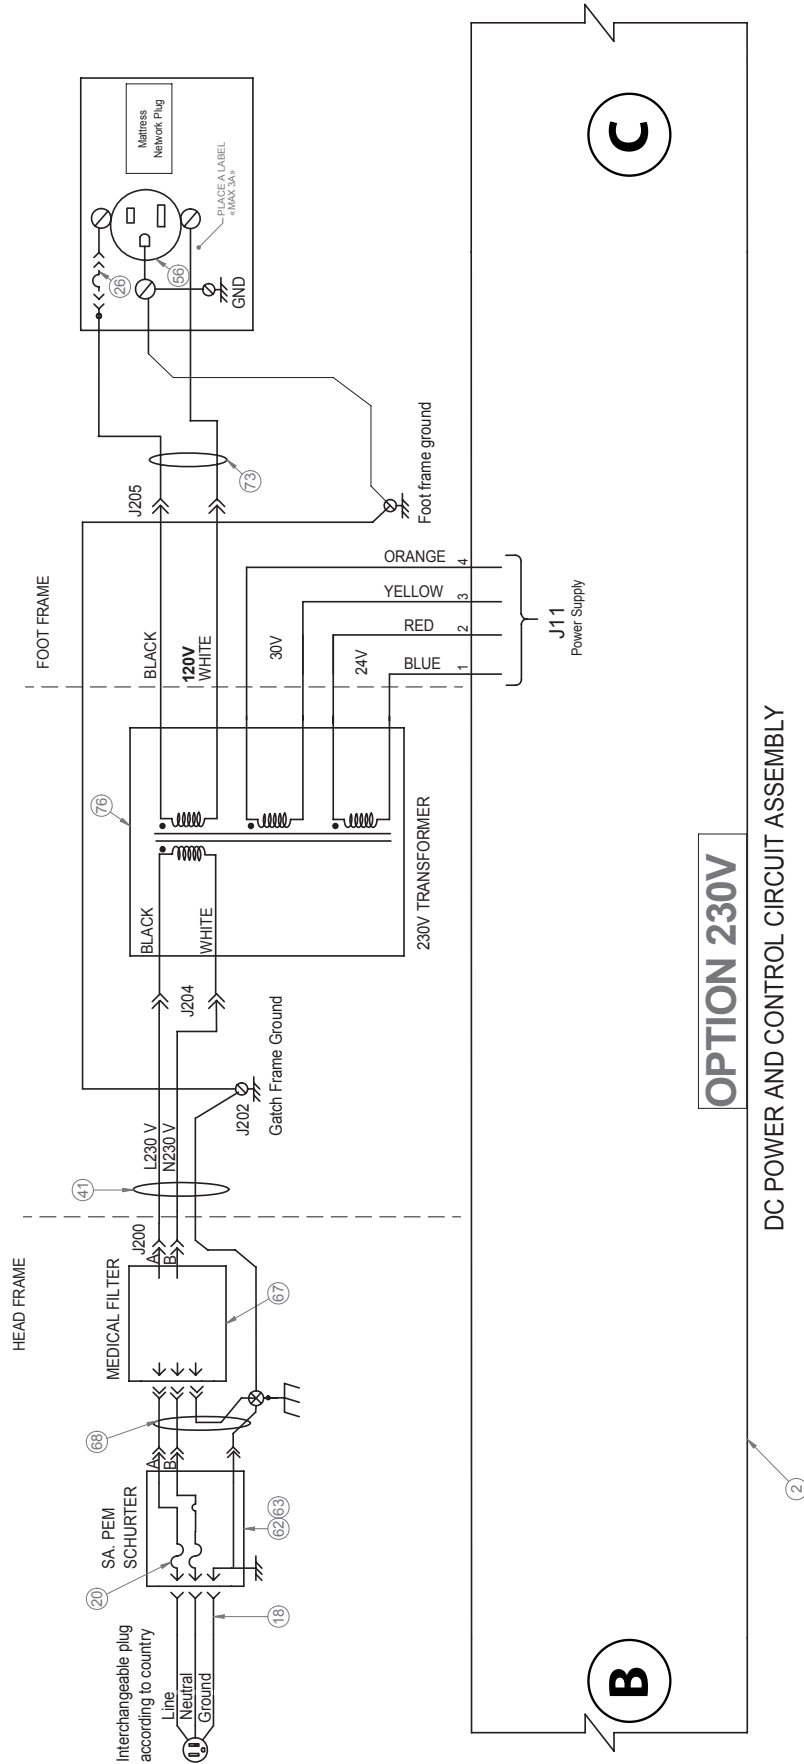


2131 to 2156

Bed Electrical Diagram

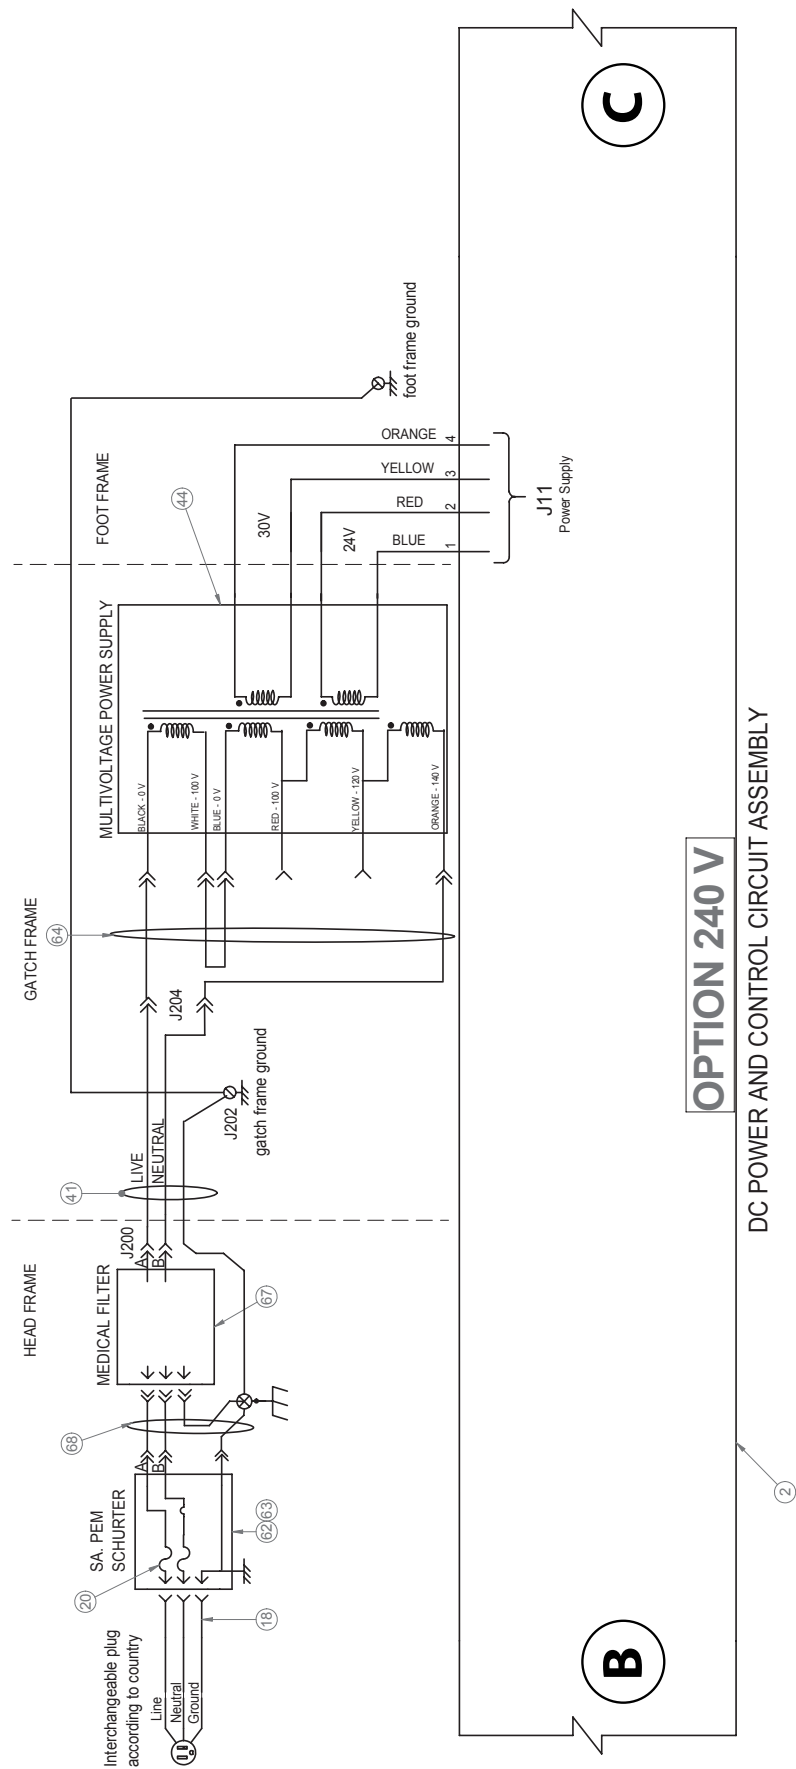


ALL MODELS

Bed Electrical Diagram

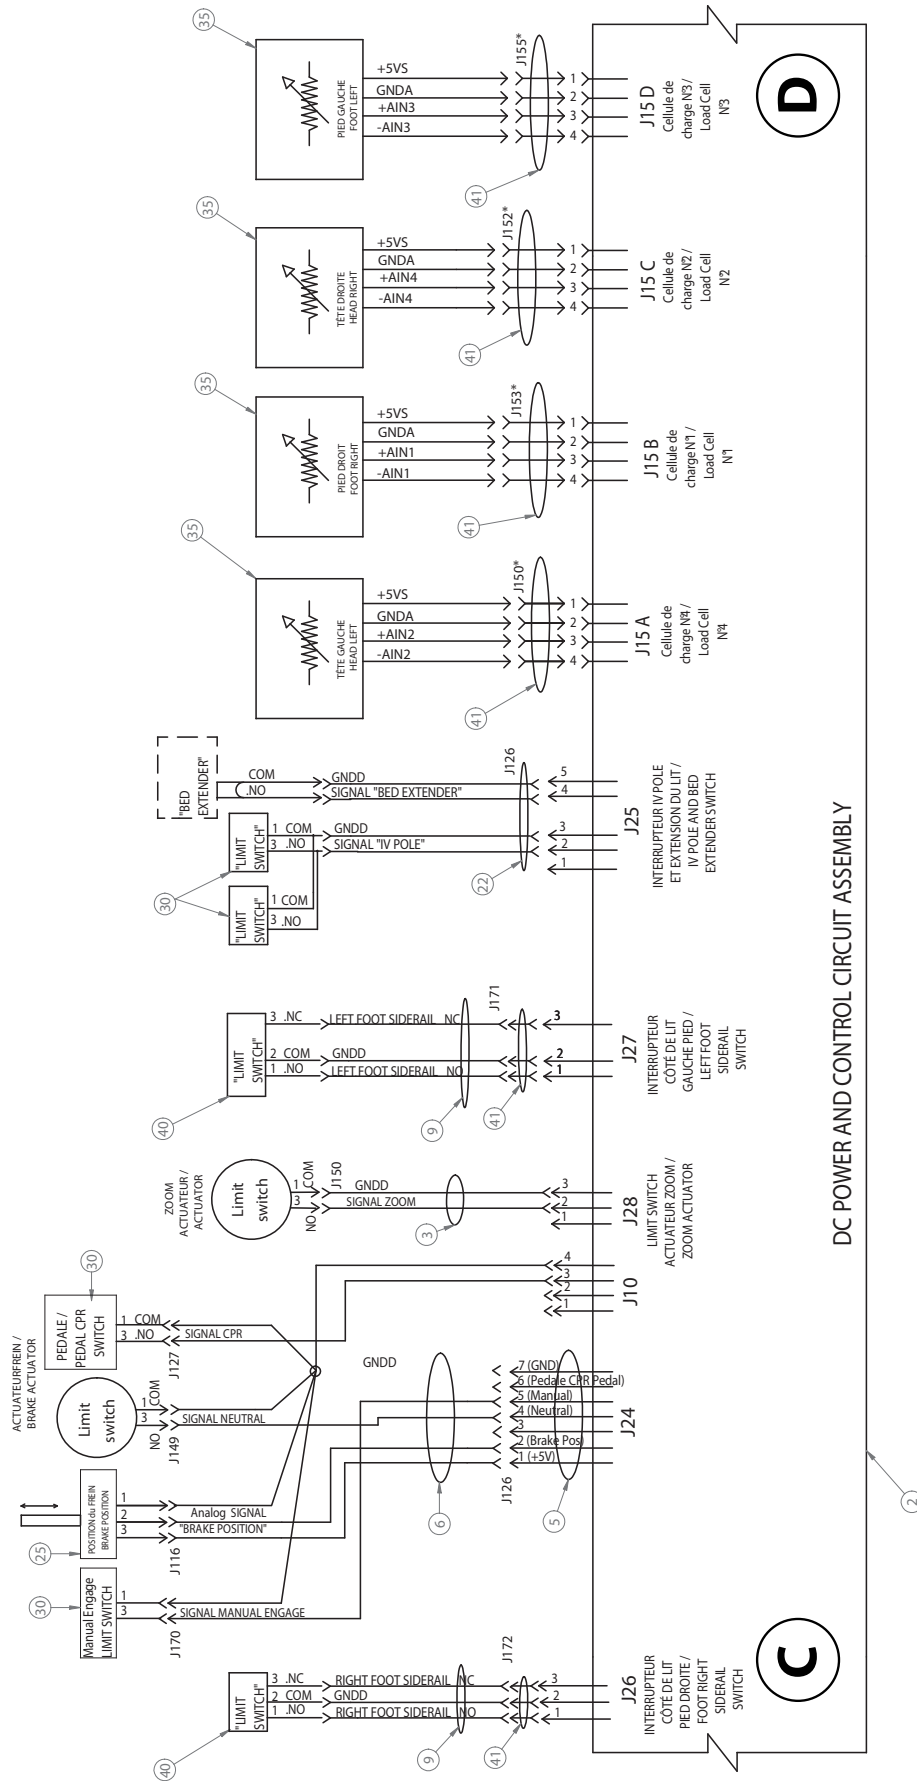


2131 to 2156

Bed Electrical Diagram

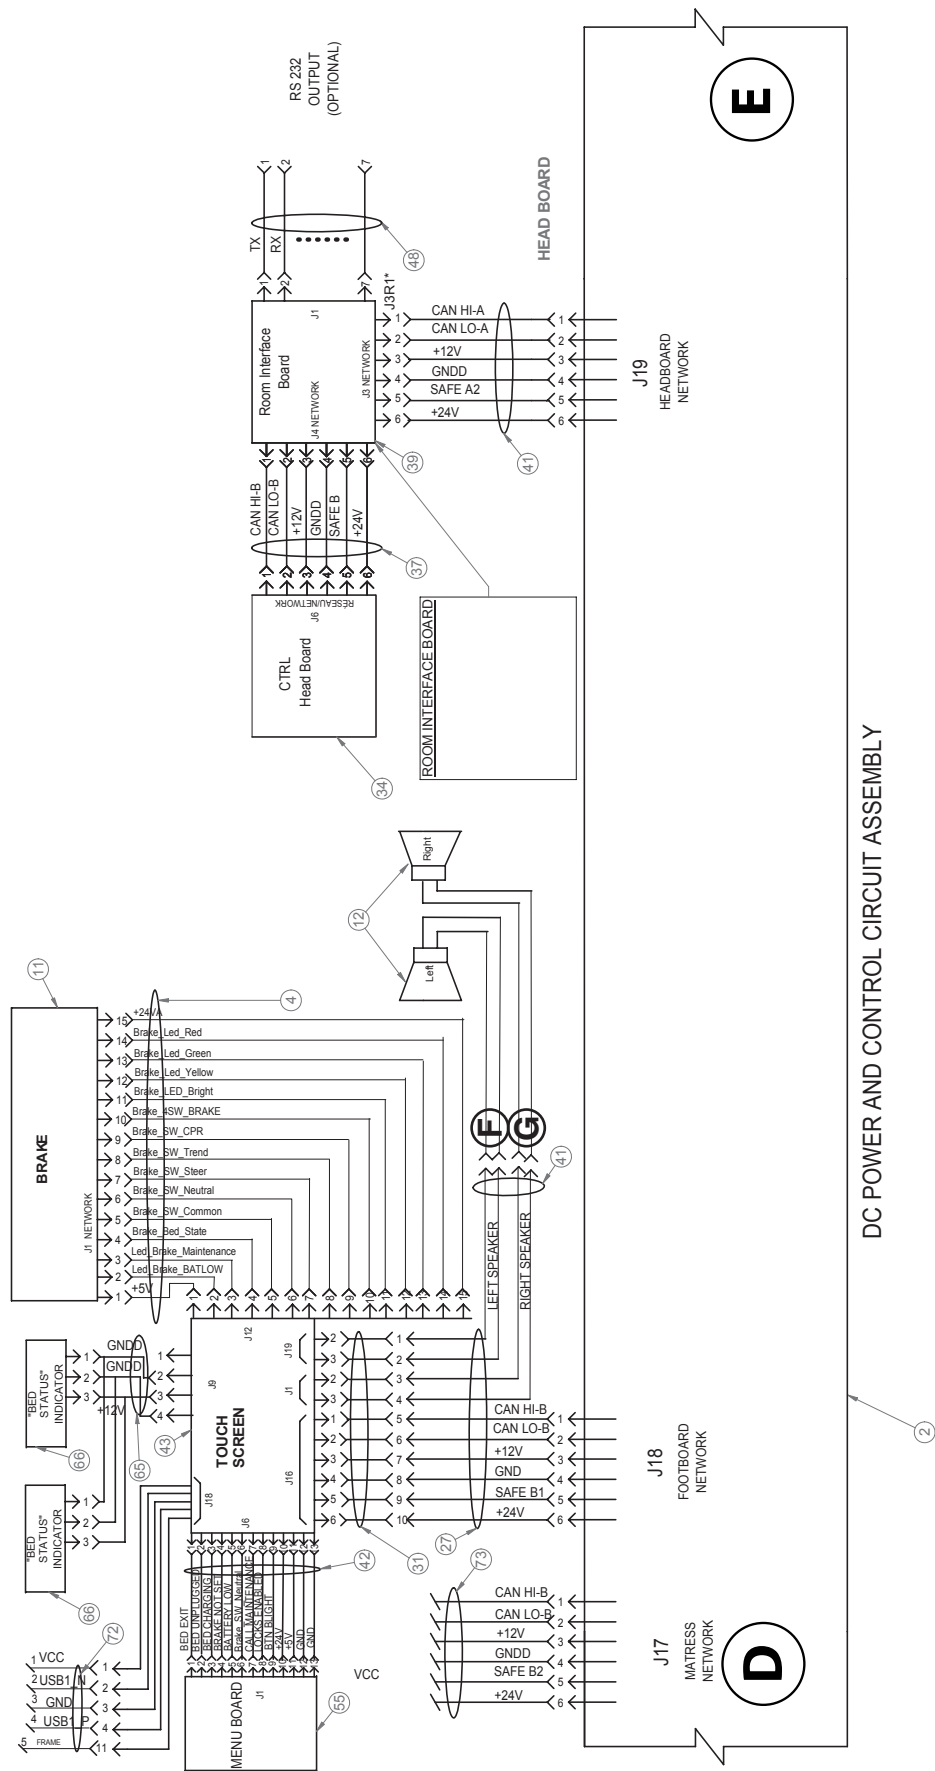


2131 to 2156

Bed Electrical Diagram

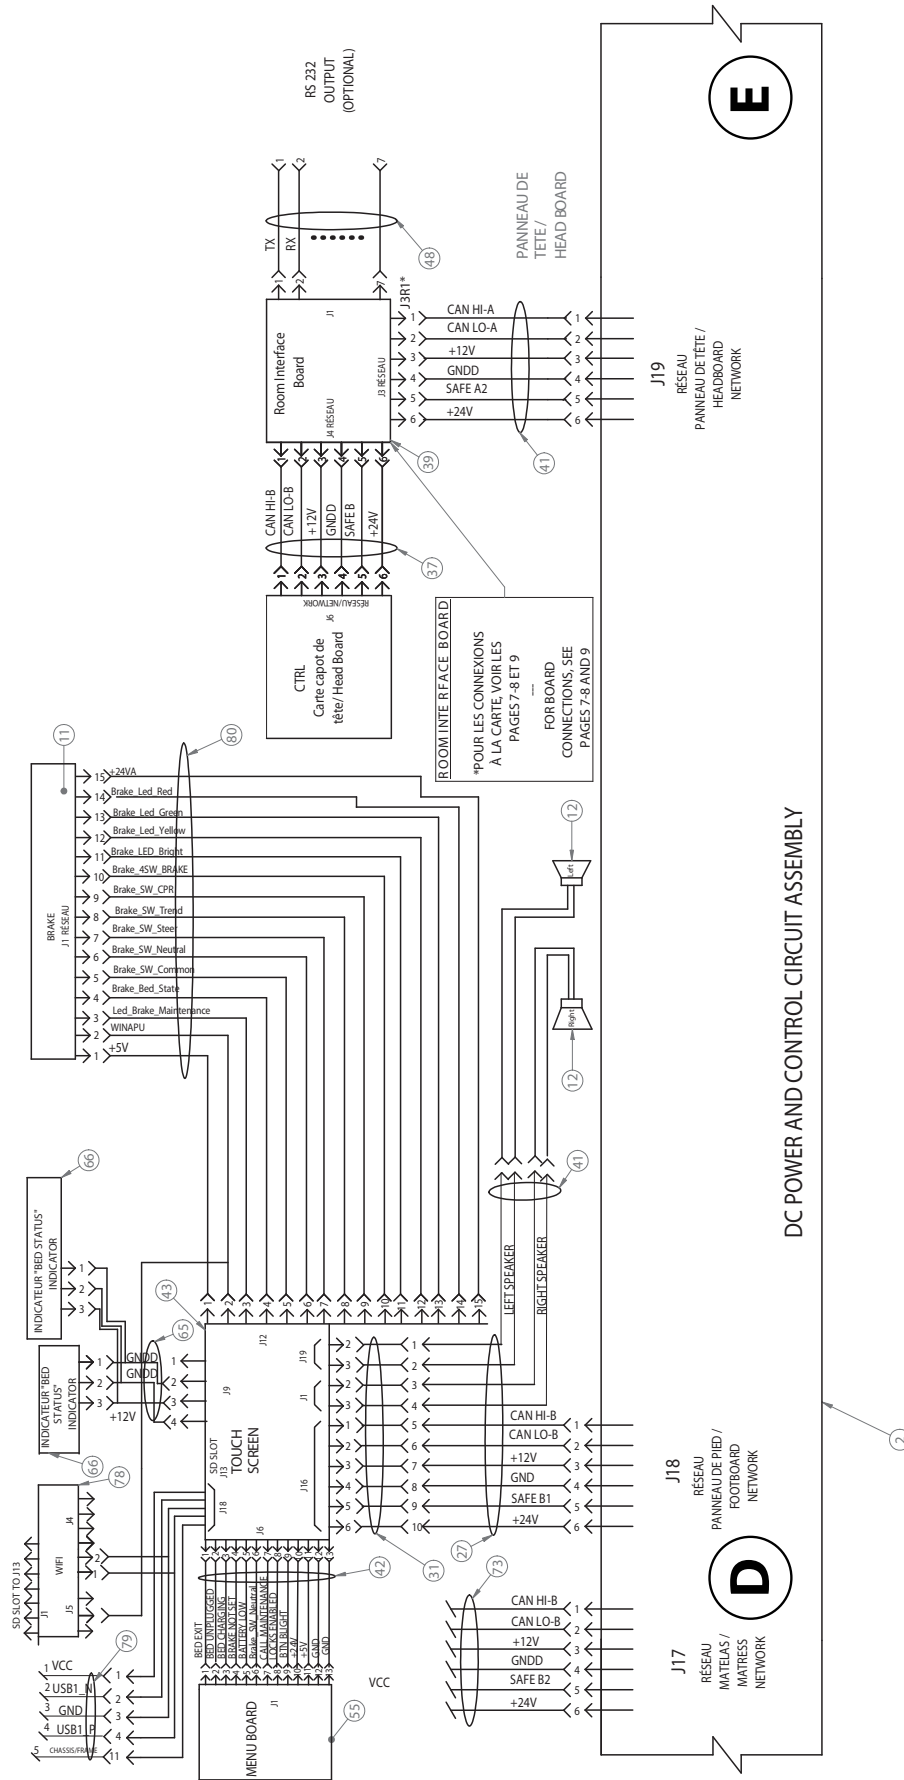

2131 / 2141 WITH WI-FI OPTION


Bed Electrical Diagram

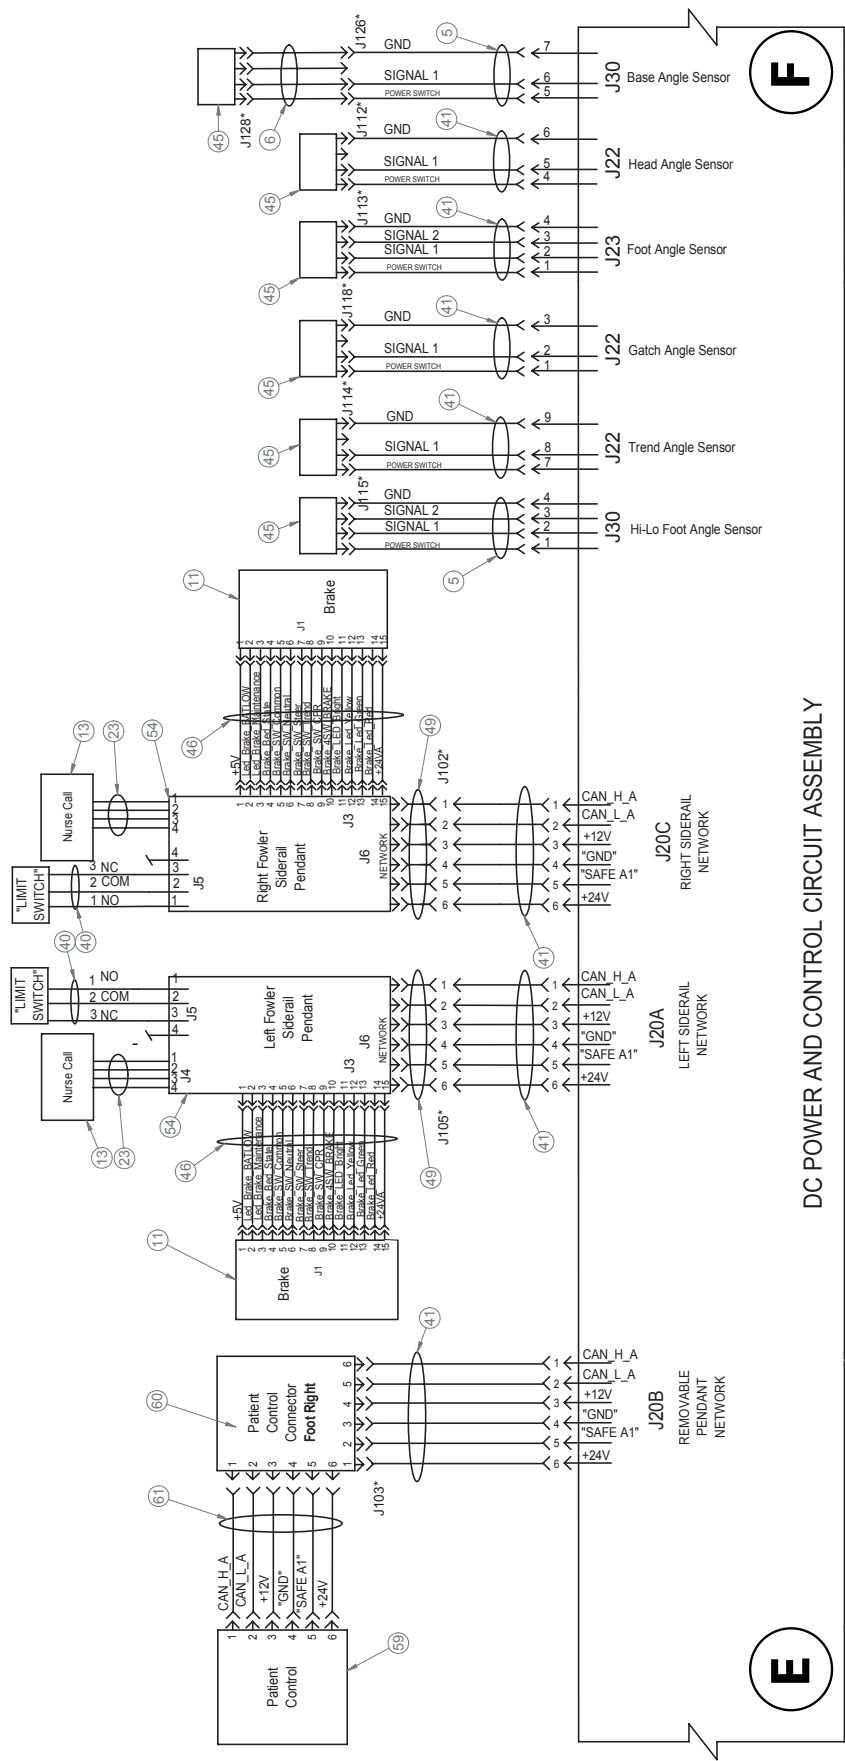

ALL MODELS


DIP SWITCH CONFIGURATION ON SIDERAIL & HEAD NURSE CTRL BOARD			
RIGHT	ON	ON	ON
LEFT	OFF	ON	ON
HEAD	ON	OFF	ON

Bed Electrical Diagram

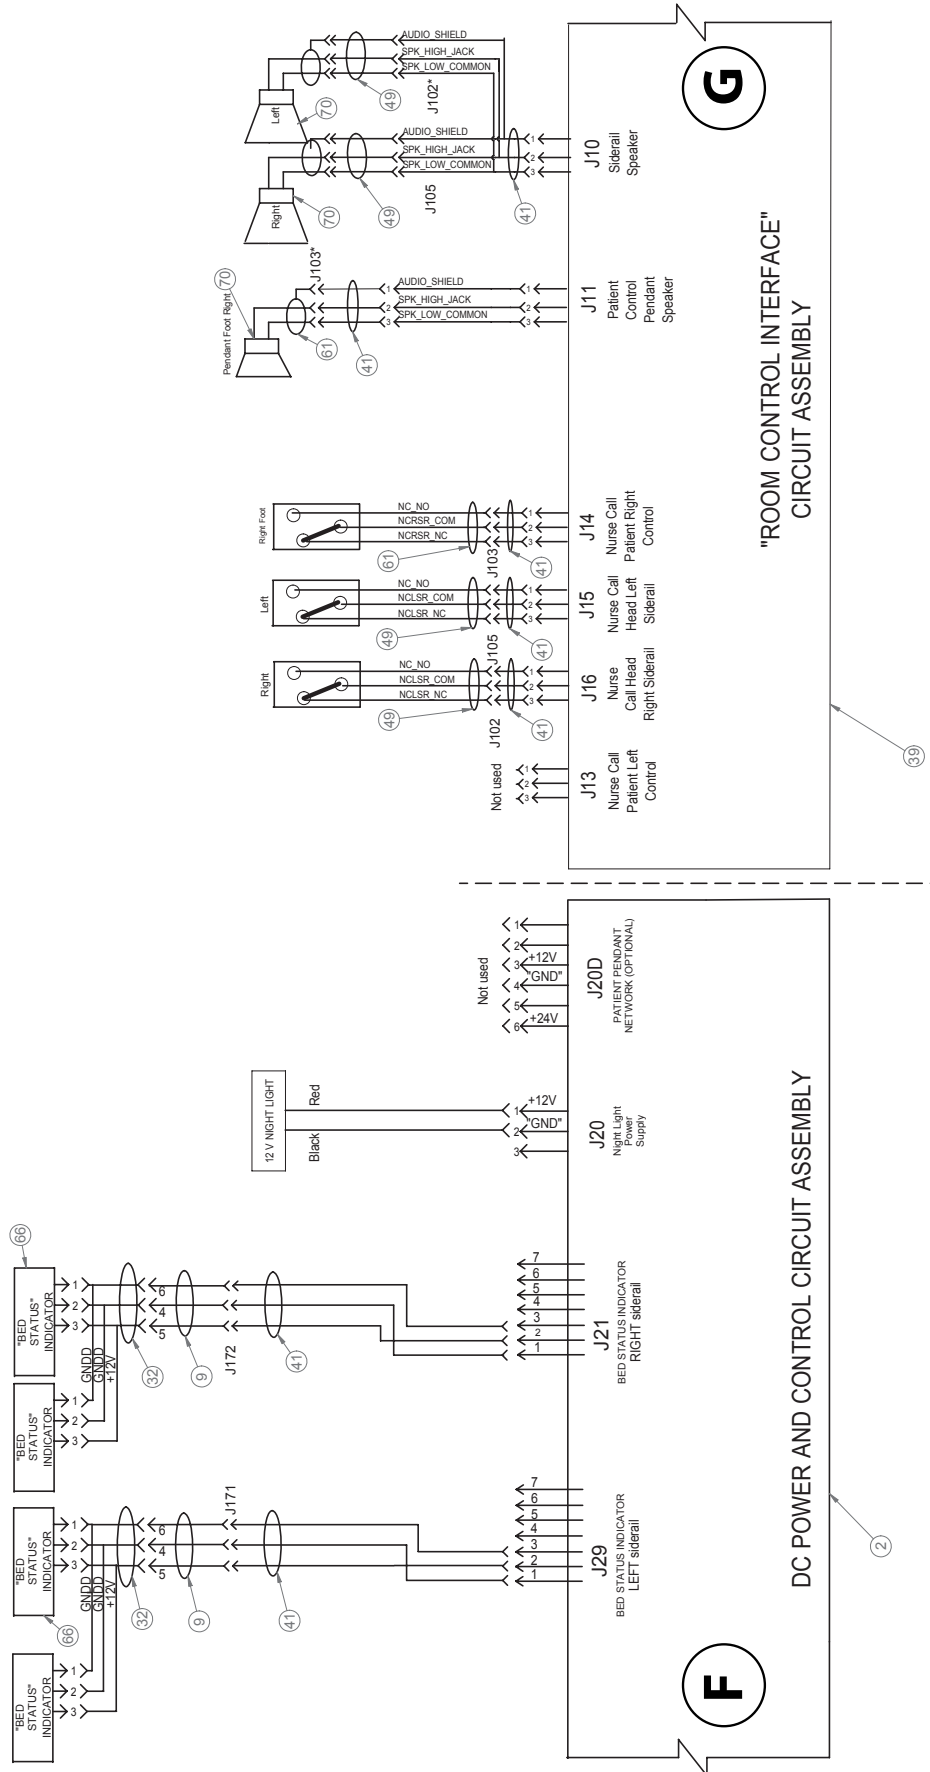


ALL MODELS

Bed Electrical Diagram

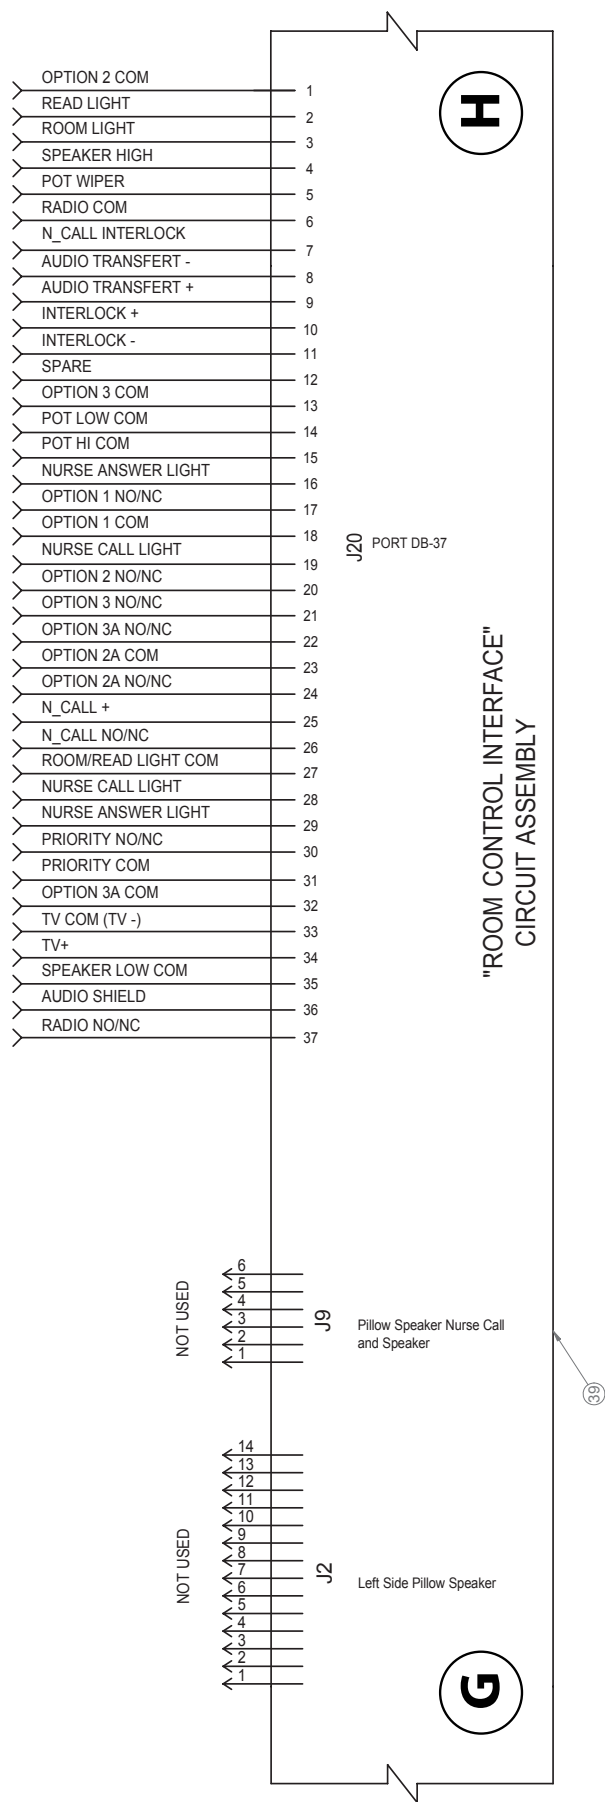


ALL MODELS PRIOR TO 3.1

Bed Electrical Diagram

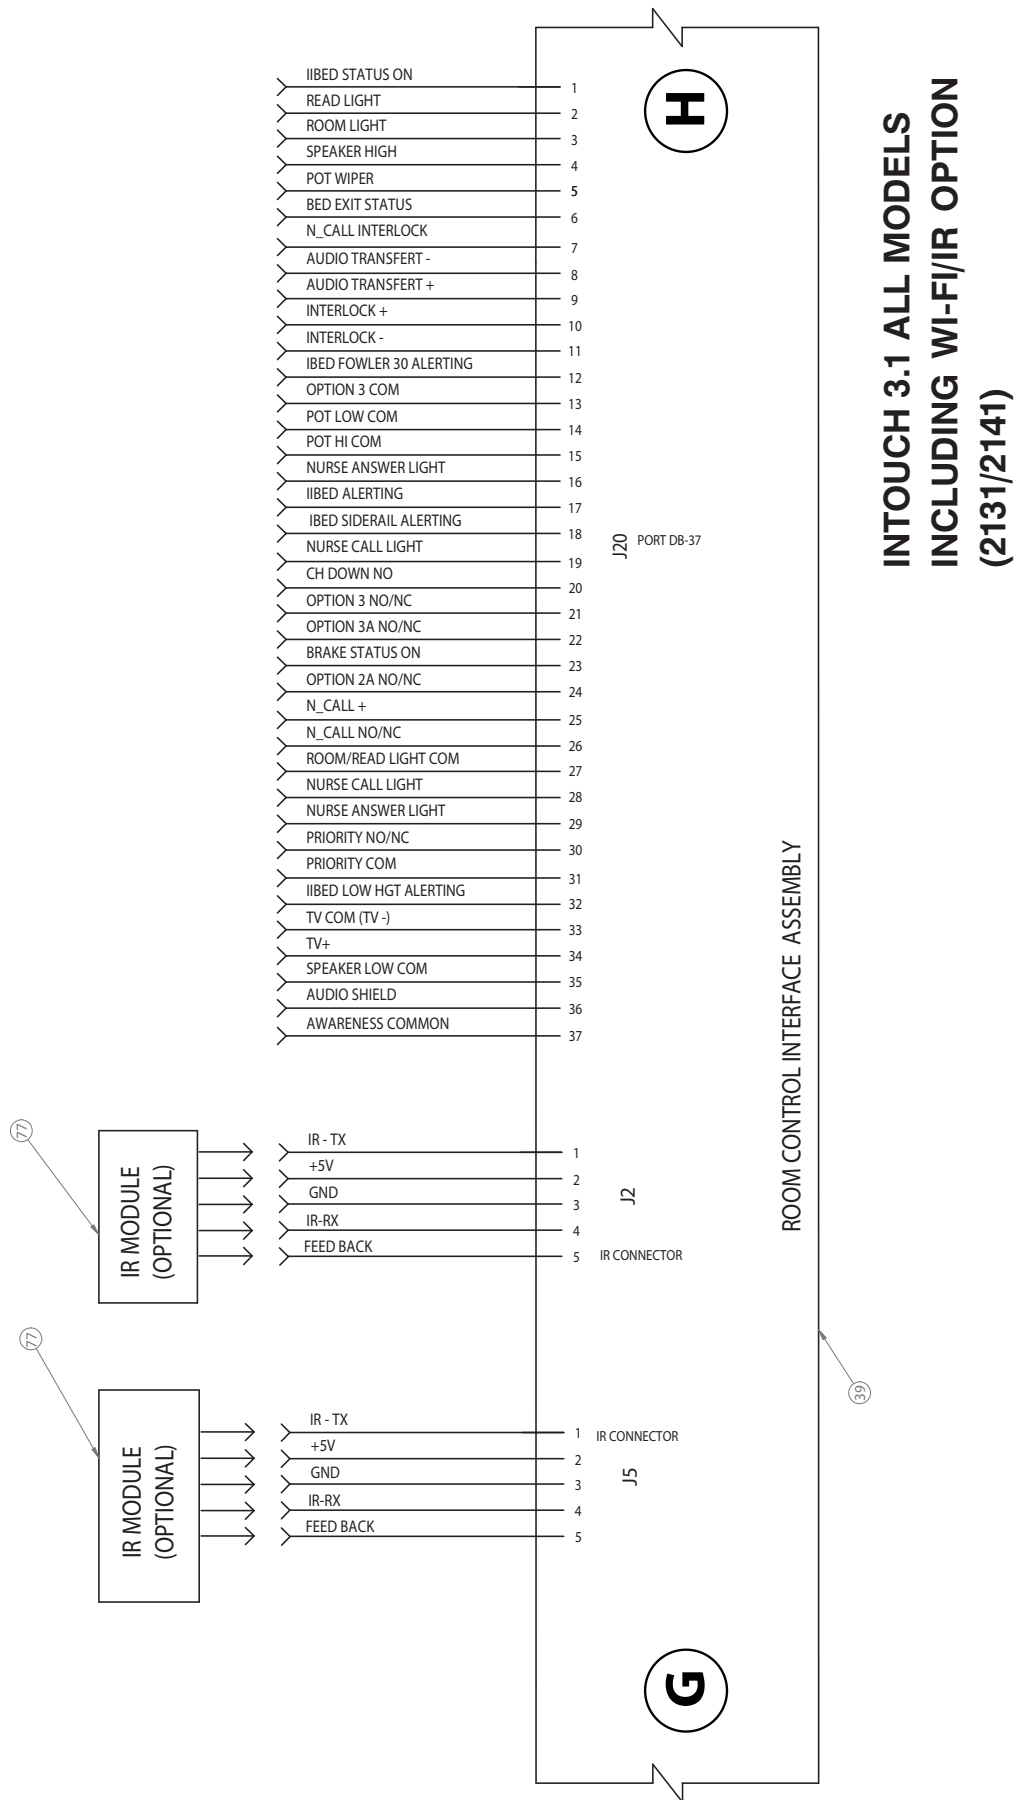

Bed Electrical Diagram

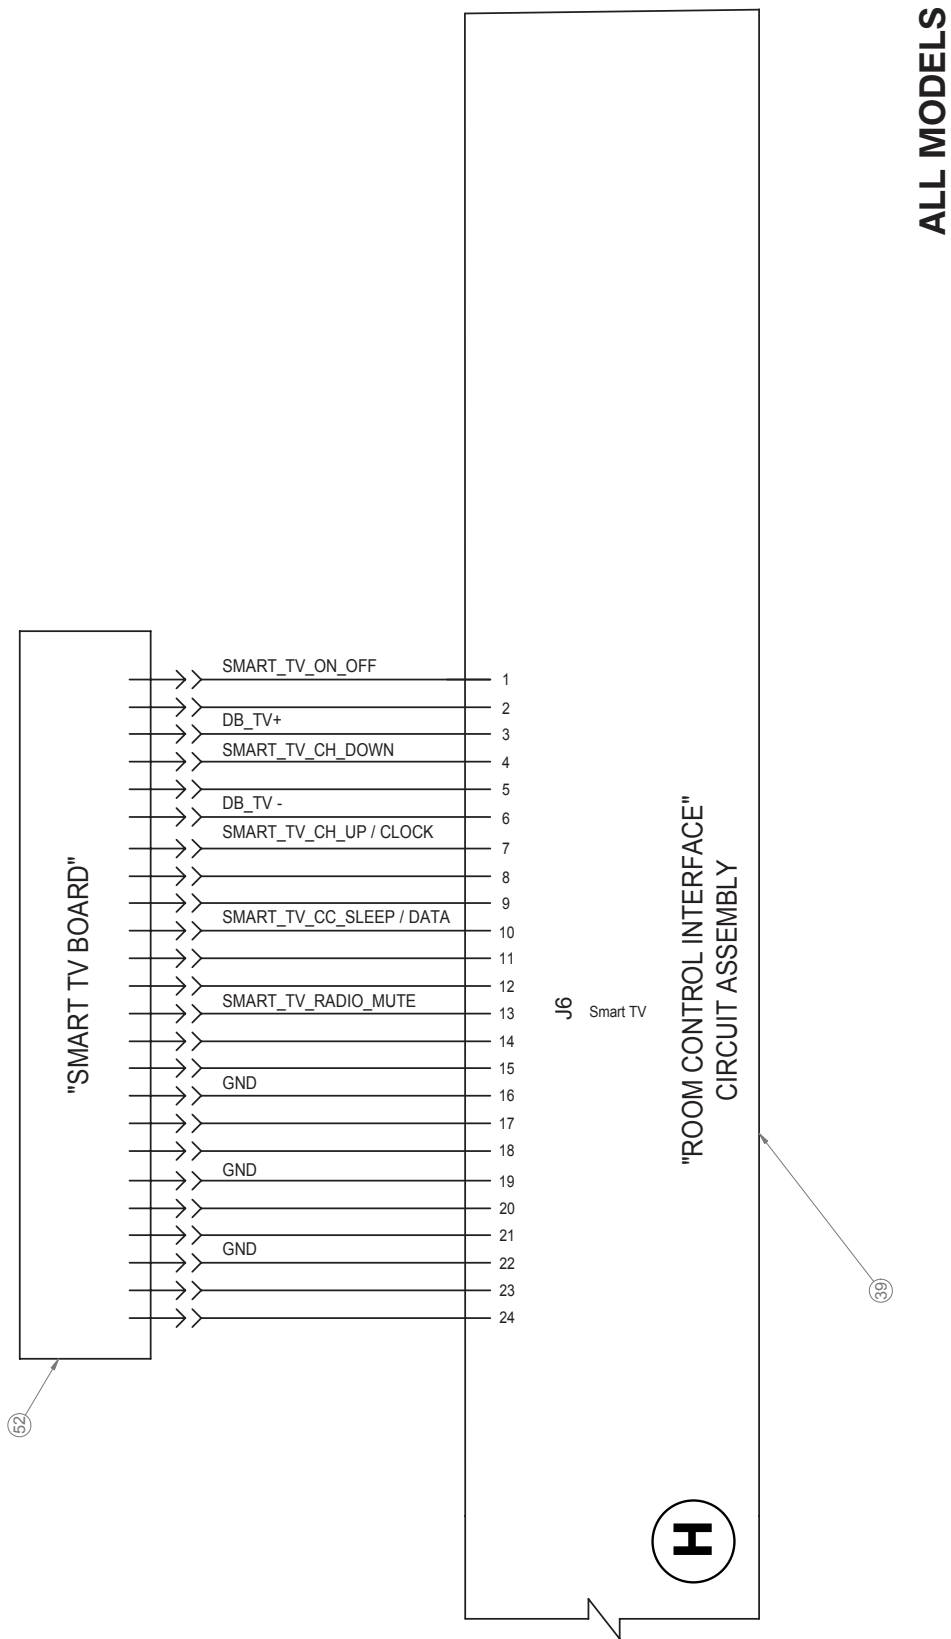

Bed Electrical Diagram

Bed Electrical Diagram - 27-1136 Rev R (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF5095	Sound Alarm	1
2	QDF75-0440	DC Power Control	1
3	QDF27-1185	Number 3 Harness	1
4	QDF27-2229	Footboard Brake Cable	1
5	QDF27-2181	Number 2 Harness	1
6	QDF27-2182	Base Structure Extension	1
7	QDF27-1381	Battery Switch Cable	2
8	QDF9188	12V, 17.9 Ah Battery	2
9	QDF27-1208	Limit Switch Siderail Cable	2
10	QDF27-1430	CSI 1109 Board	1
11	QDF27-1097	Brake / Neutral / Drive Board	3
12	QDF27-2196	Speaker	2
13	QDF27-1429	Nurse Call Board	2
14	QDF75-0230	Zoom® Control Board	1
15	QDF9136	Load Cell Handle	1
16	QDF9130	Right Handle	1
17	QDF9131	Left Handle	1
18	QDF8066	Power Cord	2
19	QDF2087	Toggle Switch	1
20	QDF8078	10A Fuse	2
22	QDF27-1607	I.V. Pole and Bed Extender Cable	1
23	QDF27-1682	Nurse Call Board Cable	2
24	QDF8024	120V Auxiliary Outlet	1
25	QDF27-2024	Linear Position Sensor	1
26	QDF9025	Breaker	1
27	QDF27-2214	Footboard Control Board Cable	1
28	QDF27-2038	Toroid Power Supply	1
29	QDF27-1646	Battery Cable	2
30	QDF9004	Micro-Switch	2
31	QDF27-2232	Footboard Cable	1
32	QDF27-1834	Footboard LBS Cable	2
33	QDF27-1841	100V Adapter	1
35	QDF27-1372	Load Cell	4
36	QDF21-1151	CAN Head Control Board	3
37	QDF21-2895	12" Network Cable	2
39	QDF75-0270	CAN Room Interface Board w/o GEN III	1
40	QDF27-1521	Siderail Limit Switch	2
41	QDF27-2213	Number 1 Harness Wire	1
42	QDF27-2230	Touch Screen Cable	2
43	QDF75-0290	Touch Screen Board	1
44	QDF27-2049	Multivoltage Power Supply	1
45	QDF75-0140	Angle Sensor	6
46	QDF27-1156	Brake Board Cable	2
47	QDF27-2025	12V 3 LEDs Night Light	1
48	QDF27-2432	Serial Interface Connector Cable	1
49	QDF27-2212	Head Siderail Cable	2
52	QDF2060	Smart TV Board	1
53	QDF21-2901	SIP-N-PUFF Cable	2
54	QDF27-1099	Siderail & Head Nurse Control Board	3
55	QDF75-0010	Menu Touch Screen Board	1
56	QDF9573	XPRT™ Mattress Plug	-

Bed Electrical Diagram

Bed Electrical Diagram - 27-1136 Rev R (Reference Only) (Continued)

Item	Part No.	Part Name	Qty.
57	QDF27-1842	200V Adaptor	1
58	QDF27-1843	220V Adaptor	1
59	QDF27-1102	Patient Pendant Control	2
60	—	Patient Pendant Connector	1
61	QDF27-1525	Patient Pendant Cable	2
62	QDF9574	Schurter #4303.0001	1
63	QDF9575	Schurter #4303.2901	1
64	QDF27-1840	240V Adaptor	1
65	QDF27-2253	LBS Cable	1
66	QDF27-1562	Local Bed Status Board	2
67	QDF9571	Medical Filter	1
68	QDF27-1524	Filter and Receptacle Connector	1
69	QDF27-1681	Interior Siderail Cable	2
70	QDF27-1526	Speaker	4
72	QDF27-2231	USB Cable	1
73	QDF27-1976	Auxiliary Plug + Mattress Cable	1
74	QDF27-2542	Zoom® Interface Board Harness	1
75	QDF75-0240	Zoom® Interface Board	1
76	QDF27-2658	230V Transformer	1
77	QDF75-0310	IR Module	2
78	QDF75-0630	Wi-Fi Board	1
79	QDF27-2573	USB Y Cable to Interface Board	1
80	QDF27-2594	Brake Card to Interface Cable	1

Service Information

BED LIFT ACTUATOR (HEAD) REMOVAL AND REPLACEMENT - (BASE)


Tools Required:

- Needle-Nose Pliers
- Diagonal Pliers
- Jack (if needed)
- 2 x 4 (20" recommended)

Step #8:

Locate Jack Stand between floor and underside of Foot Frame.

Floor

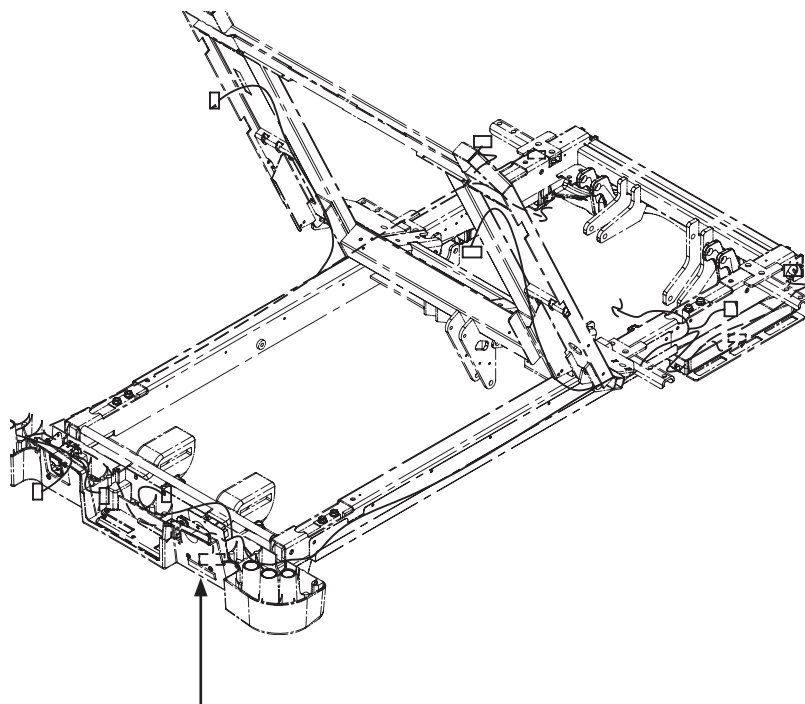

Procedure:

1. Plug bed into wall outlet.
2. Raise the head end siderails to the full up position and set the brakes using one of the brake control locations or by using the manual brake pedal.
3. Remove head end base cover by pulling up and out.
4. Remove center base cover by pulling up and out.
5. Using diagonal pliers, cut the zip tie securing the actuator cable to the base frame.
6. Using Needle-nose pliers, remove the rue clips from the clevis pins securing the actuator.

CAUTION

Do not remove the clevis pins.

7. If the bed will lower down, run it all the way down so the litter is supported by the base litter stop.
8. If the bed will not lower all the way down; using a jack and a 2 x 4, take tension off of the actuator clevis pins by placing the jack and 2 x 4 between the bottom of the right side of the litter and the floor and jack up just enough to take the litter weight off of the base frame (reference picture above).

CAUTION

Make sure that prior to jacking, the 2 x 4 is perpendicular to the floor.

9. Using the bed up/down controls, tap the up or down button to remove tension on the clevis pins and remove clevis pins.
10. Unplug the cable quick connect and remove the actuator.
11. Reverse the steps to install the new actuator.
12. Test all bed functionality prior to putting bed back in service.

[Return To Table of Contents](#)

Service Information

BED LIFT ACTUATOR (FOOT) REMOVAL AND REPLACEMENT - (BASE)

Tools Required:

- Needle-Nose Pliers
- Diagonal Pliers

Procedure:

1. Plug bed into wall outlet.
2. Raise head end siderails to full up position and ensure brakes are activated.
3. Remove head end base cover by pulling up and out.
4. Remove center base cover by pulling up and out.
5. Using diagonal pliers, cut the zip tie securing the actuator cable to the base frame.
6. Using Needle-nose pliers, remove the rue clips from the clevis pins securing the actuator.



CAUTION

Do not remove the clevis pins.

7. Lower the bed all of the way down so the litter is supported by the base litter stops.
8. Using the bed up/down controls, tap the up or down button to remove tension on the clevis pins and remove clevis pins.
9. Unplug the cable quick connect and remove the actuator.
10. Reverse the steps to install the new actuator.
11. Test all bed functionality prior to putting bed back in service.

Service Information


FOWLER ACTUATOR REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Diagonal Pliers
- Regular Screwdriver
- Phillips Screwdriver #2
- 3/8" Combination Wrench

Procedure:

1. Plug bed into wall outlet.
2. Raise bed to the full up position.
3. Raise the head end siderails to the full up position and set the brakes using one of the brake control locations or by using the manual brake pedal.
4. Working from the right side of the bed, step on the CPR pedal to lower the fowler all the way down.
5. Raise the gatch to the full up position.
6. Remove the three center base hoods (head, center, foot), then remove the right base hood.
7. Using Needle-nose pliers, remove the two rue clips from the clevis pins holding the actuator.
8. Using diagonal pliers, cut the zip ties securing the CPR cable to the actuator and the litter frame. Also cut the zip ties securing the actuator cable to the wire harness.
9. Unplug the actuator from the quick connect.
10. Holding the actuator with one hand remove the clevis pins from the actuator and carefully lower the actuator down.
11. Using a Phillips screwdriver and a 3/8" combination wrench, remove the CPR cable retaining screw from the right CPR pedal.
12. Using a regular screwdriver, loosen the CPR cable retainer on the actuator just enough so it will move.
13. Slide the gray cable retainer lock towards the CPR cable retainer and unclip the CPR cable from the red actuator release activator.
14. Remove actuator.
15. Reverse these steps to reinstall.
16. When re-adjusting the cable retainer lock set, set it to 1.00 ± 0.06 as shown (right). When the actuator is back in place, use needle-nose pliers to reattach the spring to the center of the clevis pin.
17. Test all bed functionality prior to putting bed back into service.

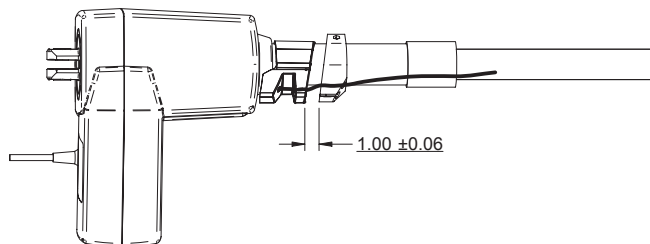

Service Information

GATCH ACTUATOR REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Needle-Nose Pliers

Procedure:


1. Plug bed into wall outlet.
2. Set the brakes using one of the brake control locations or by using the manual brake pedal.
3. Remove the mattress and set aside.
4. Raise bed to the full up position.
5. If the actuator will run, lower the gatch down to take the tension off of the actuator mounting pins. If the actuator will not run, support the gatch section to take tension off of the actuator mounting pins.
6. Unplug the actuator cable from the quick connect near the actuator.
7. Using Needle-nose pliers, remove the two rue clips from the clevis pins holding the actuator in place.
8. Holding the actuator with one hand, remove the clevis pins securing the actuator to the bed then remove the actuator.
9. Reverse these steps to reinstall
Note: If new actuator shaft does not line up with mounting holes, mount the base of the actuator then plug the actuator in and run it electrically in or out until lined up.
10. Test all bed functionality prior to putting bed back in service.

Service Information

FOOT ACTUATOR REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Needle-Nose pliers
- Diagonal Pliers
- Phillips Screwdriver #2
- Jack Stand

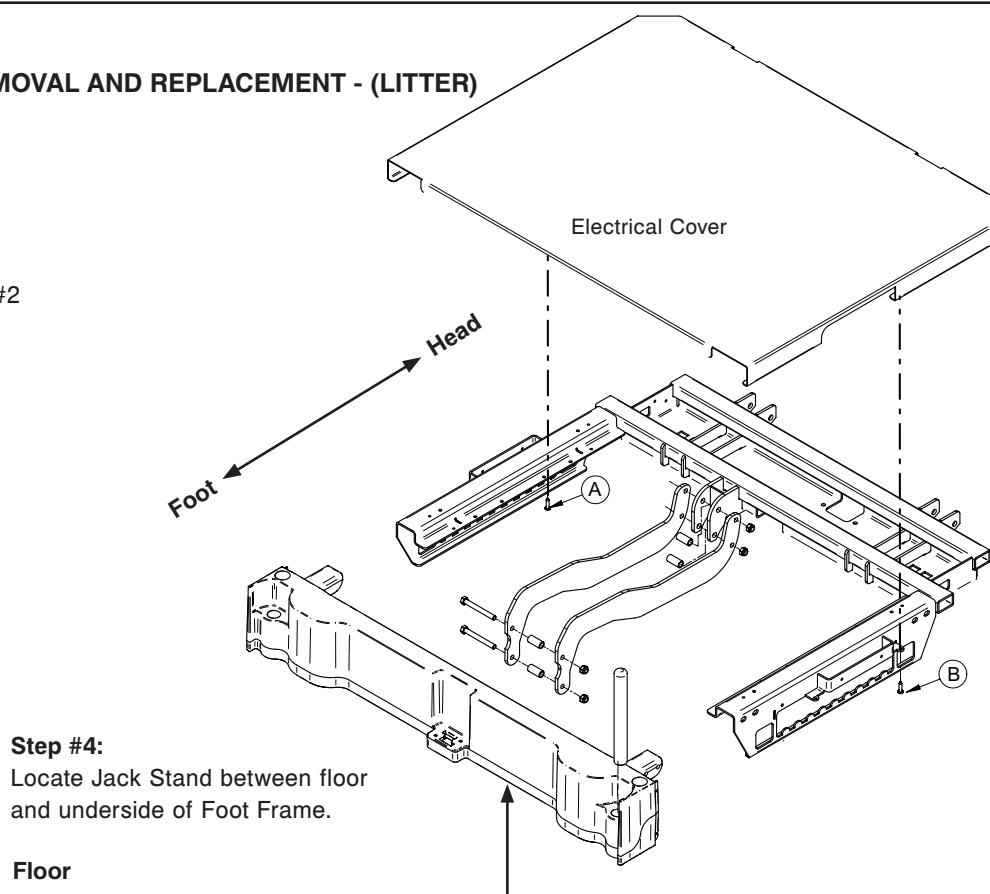

Procedure:

1. Plug bed into wall outlet.
2. Set the brakes by using one of the brake control locations or the manual brake pedal.
3. Remove the mattress and set aside.
4. Using a jack stand, support the foot section by lowering the bed height down enough to take the tension off the actuator mounting pins (reference drawing above).
5. Using diagonal pliers, cut the zip ties securing the actuator cable to the bed.
6. Remove the mattress assembly or fold back to expose the foot section.
7. Using a Phillips screwdriver, remove the two screws (reference drawing above, item A and B) securing the electrical cover from the foot section and remove the cover.

Note: Use caution as the cover is large and heavy.

8. Unplug the actuator from J1 and feed cable down to actuator.
9. Using needle-nose pliers, remove the two rue clips from the clevis pins holding the actuator in place.
10. Holding the actuator with one hand, remove the clevis pins securing the actuator to the bed then remove the actuator.
11. Reverse these steps to reinstall.

Note: If new motor shaft does not line up with mounting holes, mount the base of the actuator then plug the actuator in and run it electrically in or out until lined up.

12. Test all bed functionality prior to putting bed back in service.

Service Information

ZOOM® DRIVE ACTUATOR REMOVAL AND REPLACEMENT (2141 MODEL ONLY) - (BASE)

Tools Required:

- Needle-Nose Pliers
- Pry Bar or 2 x 4
- Diagonal Pliers

Procedure:

1. Plug bed into wall outlet.
2. Position the bed height in the middle range.
3. Remove the center base cover then remove the Zoom® drive actuator cover and set aside.
4. Using Needle-nose pliers, remove the two rue clips from the clevis pins securing the actuator to the base frame.
5. Using diagonal pliers, cut the zip ties securing the actuator cable and then unplug the actuator from the quick connect.
6. Using a pry bar or a 2 x 4, pry upward on the Zoom® drive actuator frame and push the actuator clevis pins out.
7. Remove actuator.
8. Reverse steps to install new actuator.
9. Test all bed functionality prior to putting bed back into service.

Service Information

CPU / POWER BOARD REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:



- Phillips Screwdriver #2
- ESD System
- 3/8" Nutdriver

Procedure:

1. Plug bed into wall outlet.
2. Set the brakes using one of the brake control locations or by using the manual brake pedal.
3. Raise the bed to the full upright position.
4. Remove the mattress assembly or fold back to expose the foot section.
5. Using a Phillips screwdriver, remove the two screws (reference drawing, item A and B) securing the electrical cover and remove the cover.

Note: Use caution as the cover is large and heavy.

6. Unplug the bed from the wall outlet and turn battery switch OFF. The bed should now have no power.
7. Using an ESD system, properly ground yourself.
8. Unplug all cable connections from the CPU/Power board.
9. Using a 3/8" nutdriver and a Phillips screwdriver, unscrew the four screws (C) securing the metal CPU/Power board mounting plate to the electrical tray (reference drawing above).
10. Remove CPU/Power board and discard.
11. Reverse steps 9-4 to install the new CPU/Power board (QDF75-0440).
12. Plug bed back into wall outlet and turn the battery switch back ON.
13. Configure bed options (refer to the Bed Options Configuration procedure on [page 38](#)).
14. Configure the bed serial number (refer to the Serial Number Configuration procedure on [page 39](#)).
15. Recalibrate the bed by referring to the Bed Calibration procedure on [page 23](#).
16. Test all bed functionality prior to putting the bed back into service.

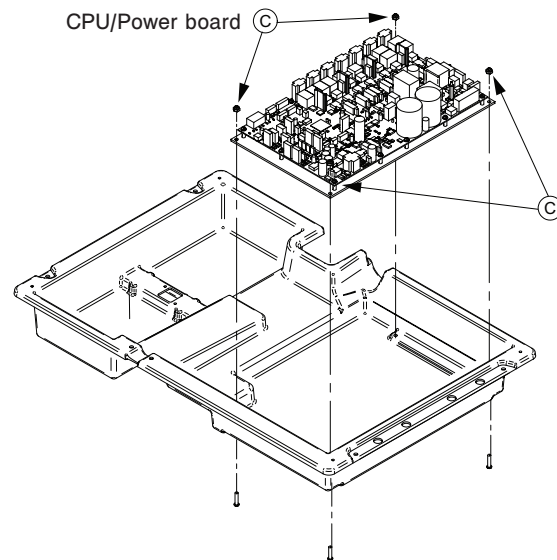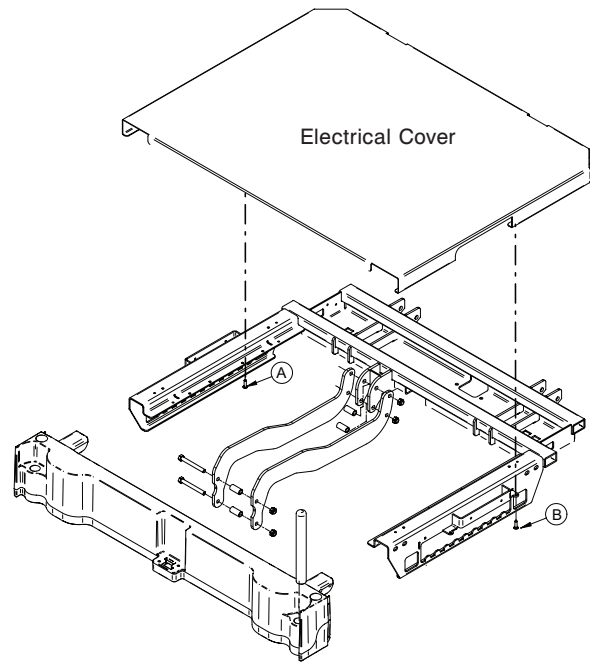

Service Information

LOAD CELL (HEAD END) REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Phillips Screwdriver #2
- Needle-Nose Pliers
- 3/8" Drive Ratchet
- 1/2" Socket
- 1/2" Combination Wrench

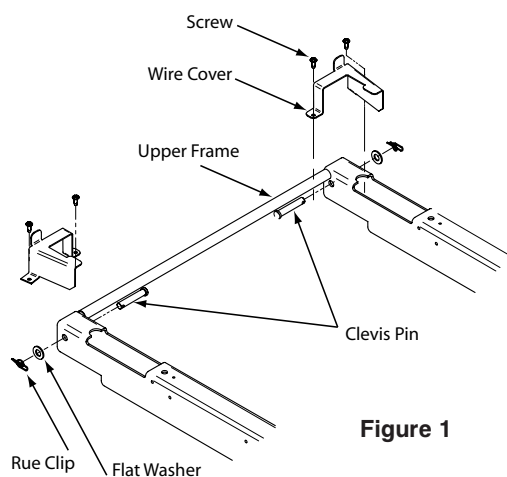


Figure 1

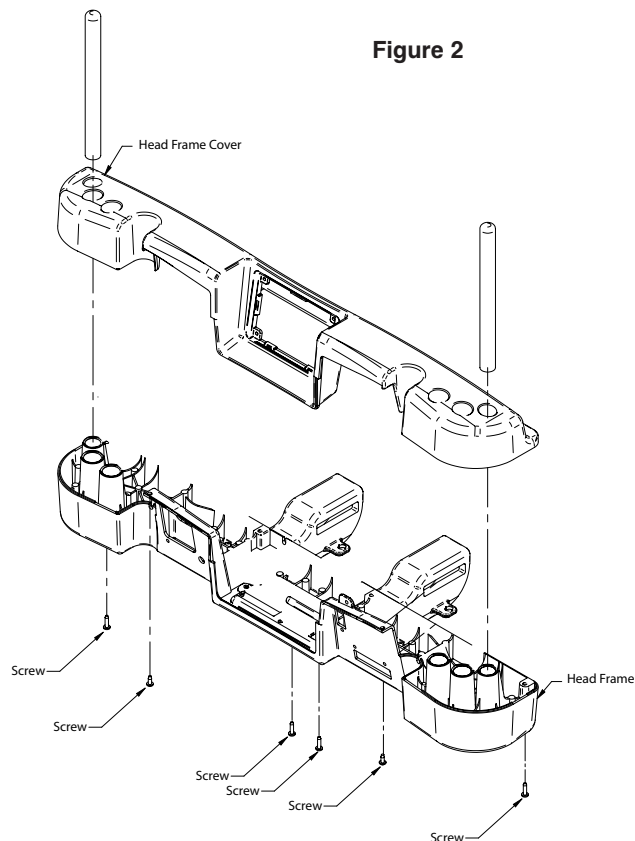


Figure 2

Procedure: (procedure the same for left and right sides)

1. Plug bed into wall outlet.
2. Raise bed and fowler to full up position, gatch down and foot up.
3. Raise head end siderails.
4. Using a Phillips screwdriver, remove the two screws securing the wire cover to the head frame (Figure 1).
5. Using a Phillips screwdriver, remove the six screws from the head frame cover, lift up on the cover and lay it on the litter (Figure 2)
6. Unscrew the load cell connection and feed the connection back towards the cell.
7. Using Needle-nose pliers, remove the rue clip and the flat washer.
8. Using one hand, grab the upper frame cross bar to remove tension on the litter then push the clevis pin out.
9. Using a ratchet with a 1/2" socket and a 1/2 combination wrench, remove the two bolts securing the load cell then remove the load cell.
10. Reverse procedures to install the new load cell.



CAUTION

Ensure cables do not get pinched when securing the head end frame cover together.

11. Recalibrate the bed (refer to Bed Calibration procedures on [page 23](#)).
12. Test all bed functionality prior to putting bed back into service.

Service Information

LOAD CELL (FOOT END) REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Phillips Screwdriver #2
- Needle-Nose Pliers
- 1/2" Combination Wrench
- 3/8" Ratchet
- 1/2" Shallow Well Socket
- Diagonal Pliers
- Jack
- 2 x 4 (20" recommended)

Procedure: (procedure the same for left and right sides)

1. Plug bed into wall outlet.
2. Raise bed to around 24" (reference the footboard display) and gatch to full up position.
3. Remove the mattress assembly.
4. Using a 1/2" combination wrench, remove the four bolts securing the gatch section cover and remove by lifting up on the foot end and then pushing backwards on the cover.
5. Raise the foot end siderails up.
6. Using needle-nose pliers, remove the rue clip and flat washer.
7. Remove the foot end base cover.
8. Using a Phillips screwdriver, remove the four screws securing the foley bag bracket.
9. Using a jack and 2 x 4, take the tension off of the load cells and remove the clevis pins from both foot end load cells.
10. Unscrew load cell cable connector.
11. Using diagonal pliers, cut the two cable ties securing the main wire harness and the siderail cable located just behind the load cell.
12. Using a ratchet and 1/2" socket, remove the two nuts and bolts securing the load cell to the litter frame.
13. Remove the load cell by pulling back and upward towards the middle of the bed while feeding the cable through the litter frame.
14. Reverse procedures to install the new load cell.



CAUTION

Do not pinch the cable when installing the load cell.


15. Recalibrate the bed (refer to Bed Calibration procedures on [page 23](#)).
16. Test all bed functionality prior to putting bed back into service.

Service Information

DISPLAY REMOVAL AND REPLACEMENT - (FOOTBOARD)

Tools Required:

- Phillips Screwdriver #2
- Stubby Phillips Screwdriver #2
- Small Slotted Screwdriver
- Utility Knife
- ESD System

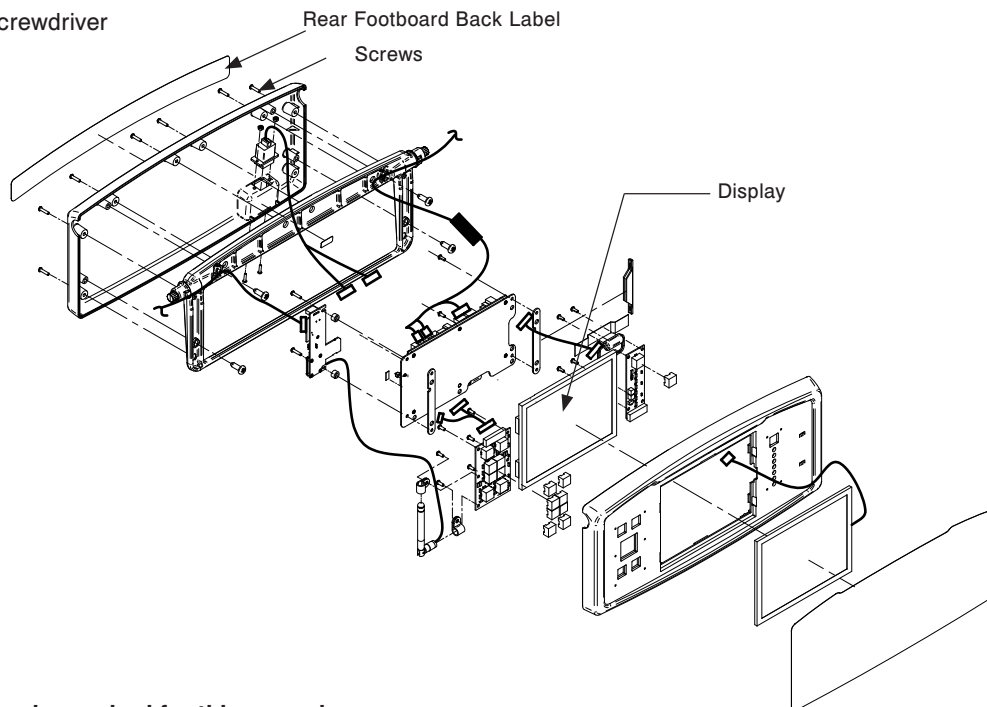

Procedure:

Note: ESD protection is required for this procedure.


1. Remove the footboard assembly and place onto a nearby work surface, face down.
2. Using a small slotted screwdriver or a utility knife, remove the rear footboard label.
Note: This label will need to be replaced with a new label (QDF27-1768).
3. Using a Phillips screwdriver, remove the six screws securing the footboard display panel to the footboard.
4. Pivot the display panel up.
5. Using a stubby Phillips screwdriver, remove the two screws from the bottom of the display panel.
6. Hold the display panel and footboard assembly together and flip the footboard assembly over, with the display panel facing up.
7. Carefully remove the display panel from the footboard assembly. Rotate over to display the circuit boards.
8. Disconnect the two ribbon cables from J3 and J7 by pulling outward on the locking tabs, then pulling the ribbon cable.
9. Disconnect the menu board cable from connector J6.
10. Using a Phillips screwdriver, remove the two screws that secure the Wi-Fi board to the LCD interface board.
11. Using a Phillips screwdriver, remove the two screws that secure the LCD interface board to the display housing.
12. Remove the two spacer shims between the LCD interface board and the display housing.
13. Carefully remove the LCD interface board from the display.
Note: The components are secured together with double-sided foam tape. Slight upward force will be necessary to separate.
14. Using a small slotted screwdriver, separate the locking tabs from the display and remove the display.
15. Reverse the procedure to install the new display.
16. Recalibrate the touch screen, by referencing the Touch Screen Calibration procedure on [page 23](#).
17. Test all bed functionality before returning the bed to service.

Service Information

BRAKE CONTROL BOARD REMOVAL AND REPLACEMENT - (FOOTBOARD)

Tools Required:

- Phillips Screwdriver #2
- Stubby Phillips Screwdriver #2
- Small Slotted Screwdriver
- Utility Knife
- ESD System

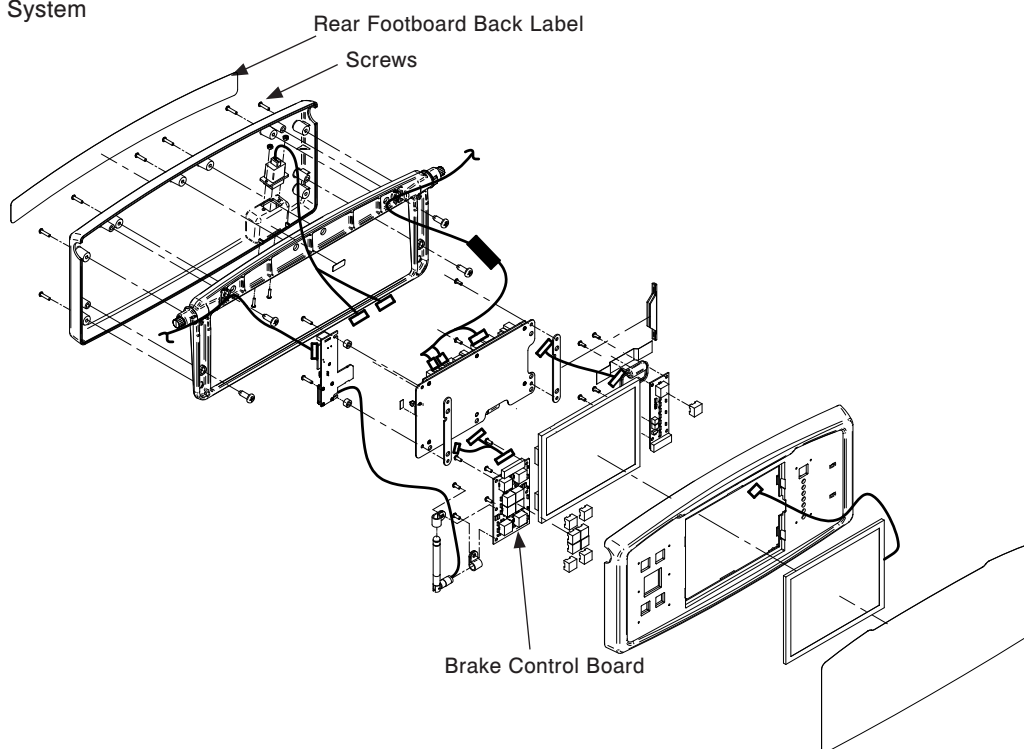

Procedure:

Note: ESD protection is required for this procedure.


1. Remove the footboard assembly and place onto a nearby work surface, face down.
2. Using a small slotted screwdriver or a utility knife, remove the rear footboard label.
Note: This label will need to be replaced with a new label (QDF27-1768).
3. Using a Phillips screwdriver, remove the six screws securing the footboard display panel to the footboard.
4. Pivot the display panel up.
5. Using a stubby Phillips screwdriver, remove the two screws from the bottom of the display panel.
6. Hold the display panel and footboard assembly together and flip the footboard assembly over, with the display panel facing up.
7. Carefully remove the display panel from the footboard assembly. Rotate over to display the circuit boards.
8. Using a Phillips screwdriver, remove the two screws that secure the Wi-Fi antenna P-clamps to the brake control board.
9. Using a Phillips screwdriver, remove the remaining four screws that secure the brake control board to the footboard display housing.
10. Disconnect the brake control cable from the brake control board.
11. Remove the brake control board.
12. Reverse the procedure to install the new brake control board.
13. Test all bed functionality before returning the bed to service.

Service Information

FUNCTION SELECTION/LED BOARD REMOVAL AND REPLACEMENT - (FOOTBOARD)

Tools Required:

- Phillips Screwdriver #2
- Stubby Phillips Screwdriver #2
- Small Slotted Screwdriver
- Utility Knife
- ESD System

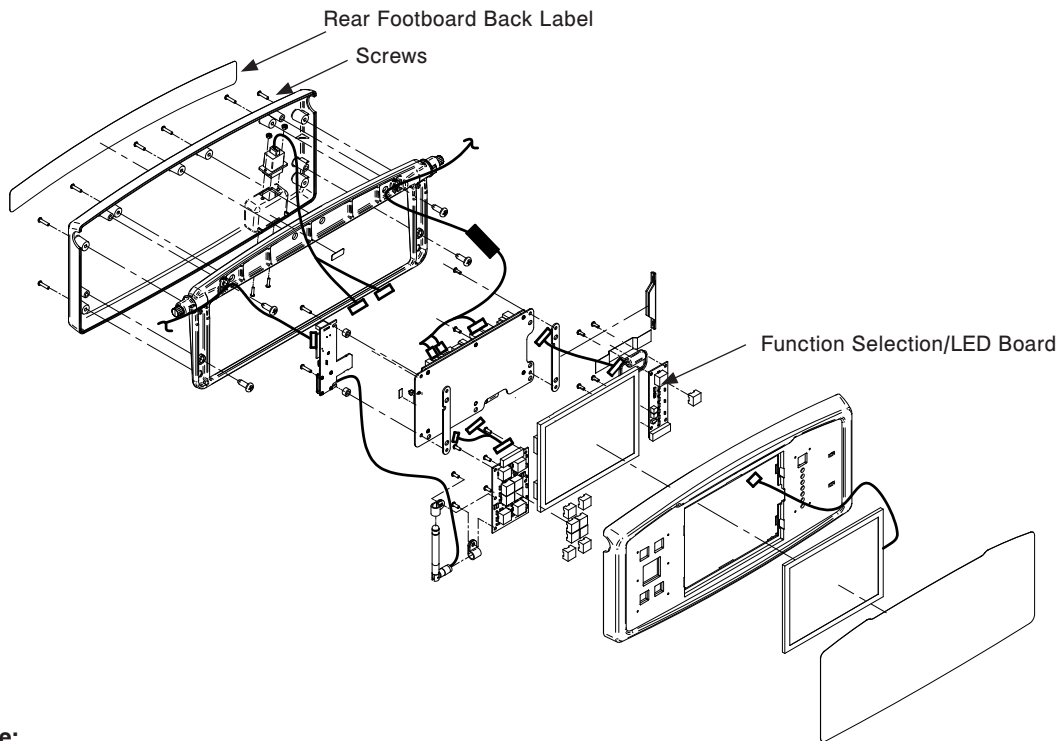

Procedure:


1. Plug the bed into a wall outlet.
2. Raise the bed to the full up position and level.
3. Unplug the bed and turn the battery disconnect "OFF" (0).
4. Using a small slotted screwdriver or a utility knife, remove the rear footboard label.
Note: This label will need to be replaced with a new label (QDF27-1768).
5. Using a Phillips screwdriver, remove the six screws from the top of the control panel which the label was covering.
6. Raise the display up and using a stubby Phillips screwdriver, remove the three screws on the bottom.
7. Remove the display housing and unplug the two cables from the function control board and set the display assembly on a bench to work on.
8. Using a Phillips screwdriver, remove the four screws securing the function selection/LED board.
9. Unplug the cable going to the function selection/LED board.
10. Reverse the procedures to install the new function selection/LED board.
11. Test all bed functionality prior to putting the bed back into service.

Service Information

TOUCH SCREEN REMOVAL AND REPLACEMENT - (FOOTBOARD)

Tools Required:

- Phillips Screwdriver #2
- Stubby Phillips Screwdriver #2
- Small Slotted Screwdriver
- Utility Knife
- ESD System

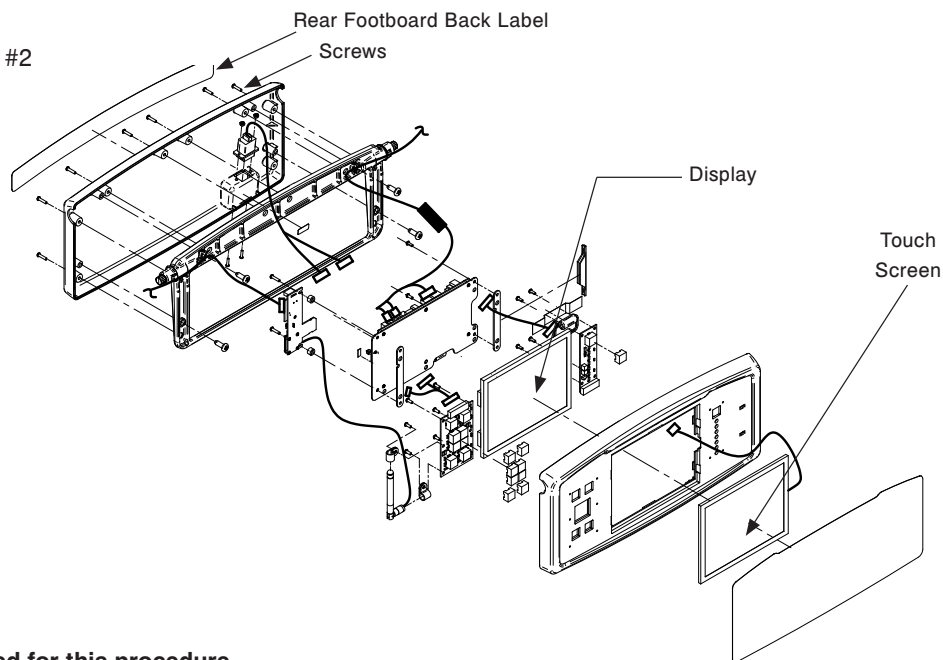

Procedure:

Note: ESD protection is required for this procedure.

1. Remove the footboard assembly and place onto a nearby work surface, face down.
2. Using a small slotted screwdriver or a utility knife, remove the rear footboard label.
Note: This label will need to be replaced with a new label (QDF27-1768).
3. Using a Phillips screwdriver, remove the six screws securing the footboard display panel to the footboard.
4. Pivot the display panel up.
5. Using a stubby Phillips screwdriver, remove the two screws from the bottom of the display panel.
6. Hold the display panel and footboard assembly together and flip the footboard assembly over, with the display panel facing up.
7. Carefully remove the display panel from the footboard assembly and rotate over to display the circuit boards.
8. Disconnect the two ribbon cables from J3 and J7 by pulling outward on the locking tabs, then pulling the ribbon cable.
9. Disconnect the menu board cable from connector J6.
10. Using a Phillips screwdriver, remove the two screws that secure the Wi-Fi board to the LCD interface board.
11. Using a Phillips screwdriver, remove the two screws that secure the LCD interface board to the display housing.
12. Remove the two spacer shims between the LCD interface board and the display housing.
13. Carefully remove the LCD interface board from the display.
Note: The components are secured together with double-sided foam tape. Slight upward force will be necessary to separate.
14. Using a small slotted screwdriver, separate the locking tabs from the display and remove the display.
15. Using a small slotted screwdriver or utility knife, remove the foot control overlay label.
Note: This overlay label will need to be replaced with a new overlay label (QDF27-2188-ENG) and patent pending label (QE71-1094-ENG).
16. Carefully separate the touch screen from the display housing.
17. Reverse the procedure to install the new touch screen.
18. Recalibrate the touch screen, by referencing the Touch Screen Calibration procedure on [page 23](#).
19. Test all bed functionality before returning the bed to service.

Service Information


BATTERY REMOVAL AND REPLACEMENT - (FOOTBOARD)

Tools Required:

- Phillips Screwdriver #2
- Stubby Phillips Screwdriver #2
- Small Slotted screwdriver
- Utility Knife
- ESD System

Procedure:

1. Plug the bed into a wall outlet.
2. Raise the bed to the full up position and level.
3. Unplug the bed and turn the battery disconnect switch to the "OFF" (0) position.
4. Using a small slotted screwdriver or a utility knife, remove the rear footboard label.
Note: This label will need to be replaced with a new label (QDF27-1768).
5. Using a Phillips screwdriver remove the six screws from the top of the control panel which the label was covering.
6. Raise the display up and using a stubby Phillips screwdriver, remove the three screws on the bottom.
7. Remove the display housing and unplug the two cables from the function control board and set the display assembly on a bench to work on.
8. Remove the battery and replace with new battery (see figure below).
9. Reverse the above steps to reassemble.
10. Referencing the operation manual complete the Time / Date Setup procedure.

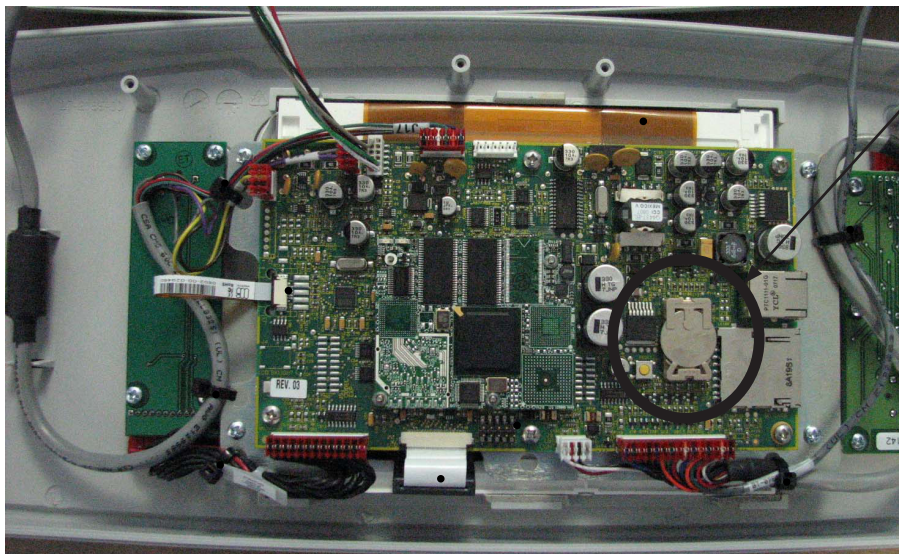


Battery

Service Information

BRAKE / NEUTRAL / DRIVE POTENTIOMETER REMOVAL AND REPLACEMENT - QDF27-2024

Tools Required:

- Diagonal Pliers

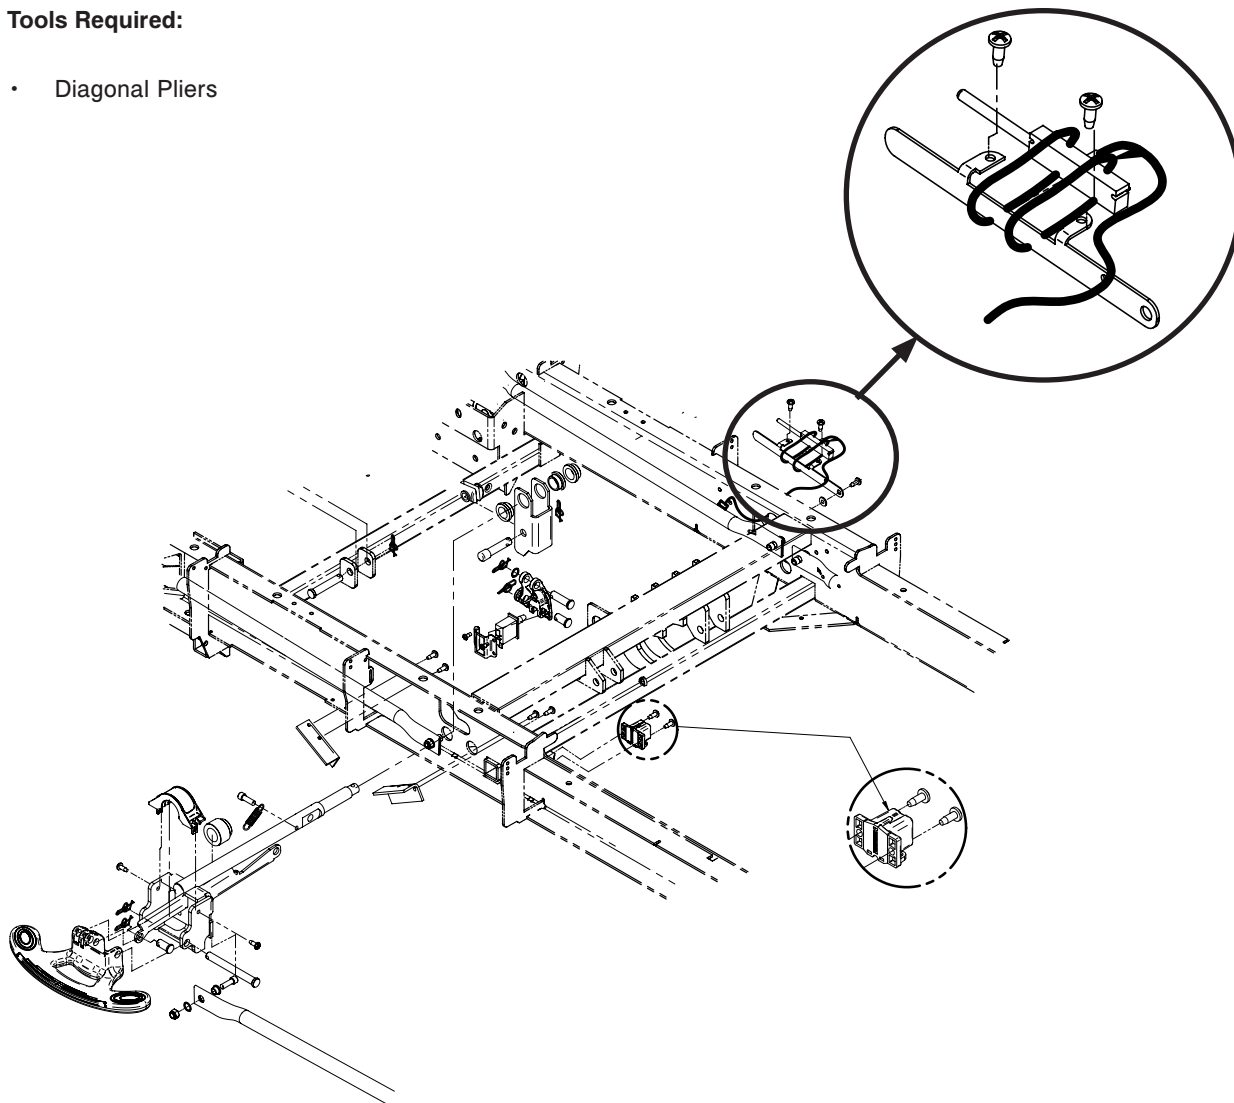

Procedure:

1. Plug bed into wall outlet.
2. Raise the bed lift and patient's left siderails all the way up.
3. Remove the base center covers (foot, center, and head).
4. Remove the patient's left base frame cover.
5. Cut the two wire ties securing the potentiometer to the potentiometer bracket; then cut the two wire ties securing the potentiometer wires to the frame.
6. Remove the electrical tape holding the quick connection together.
7. Reverse the above procedures for installation of the new potentiometer.
Note: Make sure to install new wire ties in the same location.
8. Recalibrate the bed (refer to Bed Calibration procedures on [page 23](#)).
9. Test all bed functionality prior to putting the bed back into service.

Service Information

BATTERY REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Phillips Screwdriver #2
- 5/16" Nutdriver
- 5/16" Combination Wrench

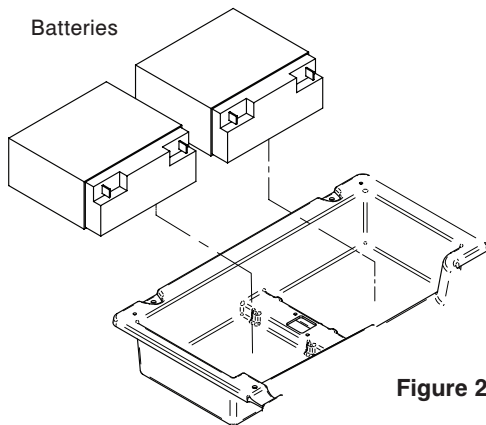


Figure 2

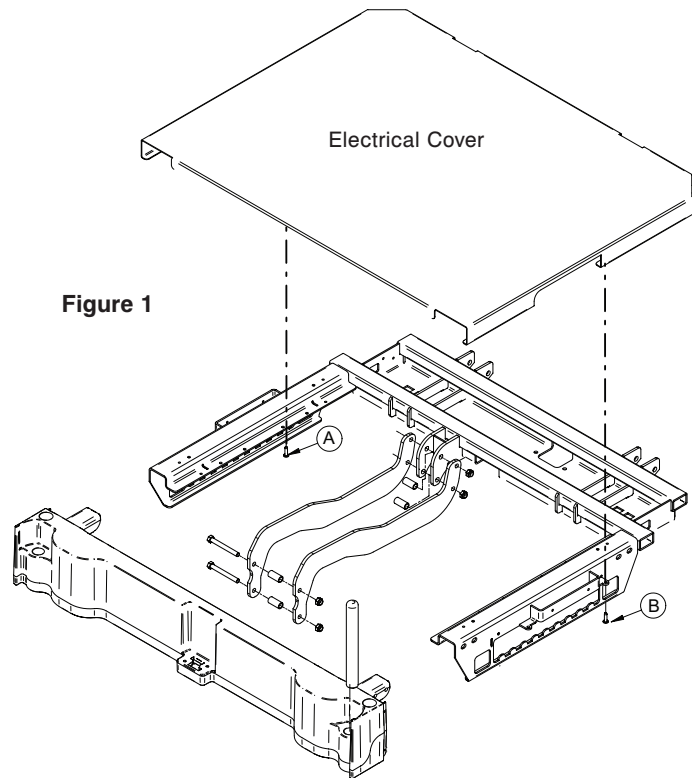


Figure 1

Procedure:

Note

Batteries should always be replaced in pairs.

1. Plug bed into wall outlet.
2. Set the brakes using one of the brake control locations or by using the manual brake pedal.
3. Raise the bed to the full up position.
4. Remove the mattress assembly or fold back to expose the foot section.
5. Using a Phillips screwdriver, remove the two screws securing the electrical cover and remove the cover (reference Figure 1 above, item A and B).

Note: Use caution as the cover is large and heavy.

6. Unplug the bed from the wall outlet and turn battery switch "OFF" (0). The bed should now have no power.
7. Unplug J12 connector from the CPU/Power board.
8. Lift up on both batteries and stand them upright (reference Figure 2 above).
9. Using a 5/16" nutdriver and a 5/16" combination wrench, unbolt the wires from the battery posts.
10. Reverse the steps to install new batteries.

Note: New battery information should be facing the right side when installing and upright when installed.


11. Test all bed functionality while plugged into wall outlet and when unplugged prior to putting back into service.

Service Information

FOWLER ANGLE SENSOR REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Stubby Phillips Screwdriver #2
- ESD System

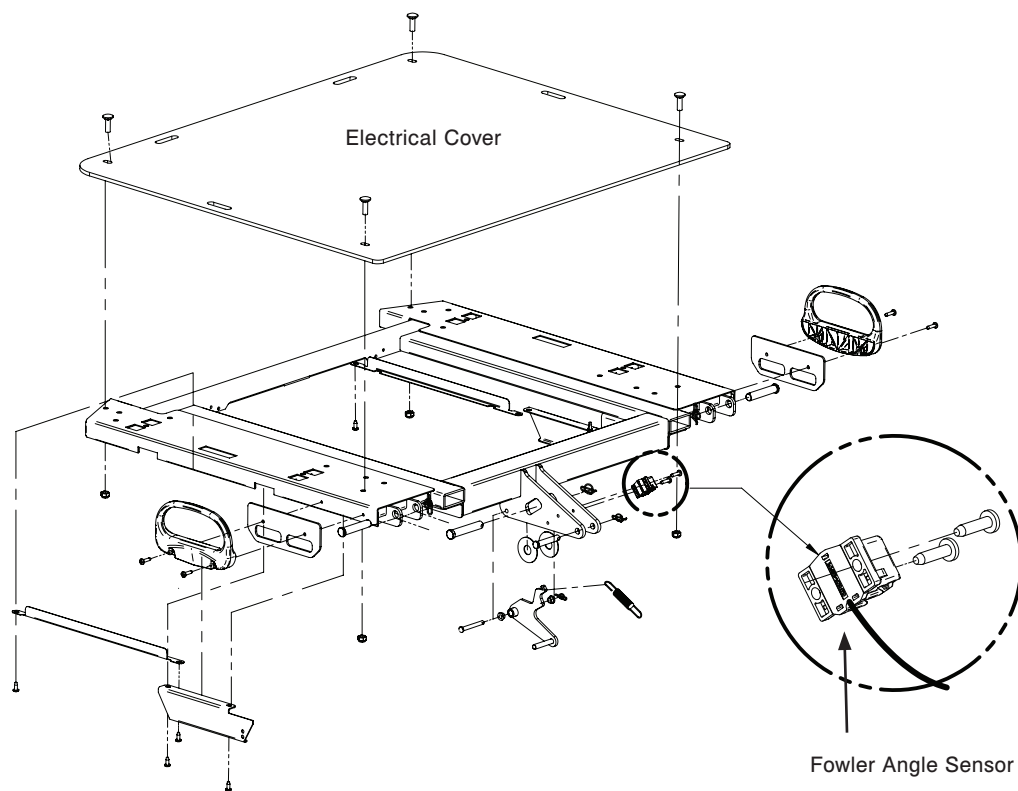

Procedure:


1. Plug bed into wall outlet.
2. Set the brakes using one of the brake control locations or by using the manual brake pedal.
3. Raise the bed to the full up position and raise the patient left siderails (head end and foot end).
4. If fowler motor will run, raise fowler up to approximately 20 degrees. If the fowler motor will not run, put the bed into the calibration mode step one as shown on [page 23](#). Run the Fowler up to approximately 20 degrees.
5. Working from the left side of the bed, use a stubby Phillips screwdriver and remove the two screws securing the fowler angle sensor to the bottom of the fowler frame.
6. Using an ESD system, properly ground yourself.
7. Unclip the three clips holding the board cover on.
8. Unplug the cable from the board.
9. Reverse the steps to install the new fowler angle sensor.
- Note: Do not over-tighten the two screws.**
10. Recalibrate the bed (refer to Bed Calibration procedures on [page 23](#)).
11. Test all bed functionality prior to putting the bed back into service.

Service Information

GATCH ANGLE SENSOR REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Stubby Phillips Screwdriver #2
- ESD System

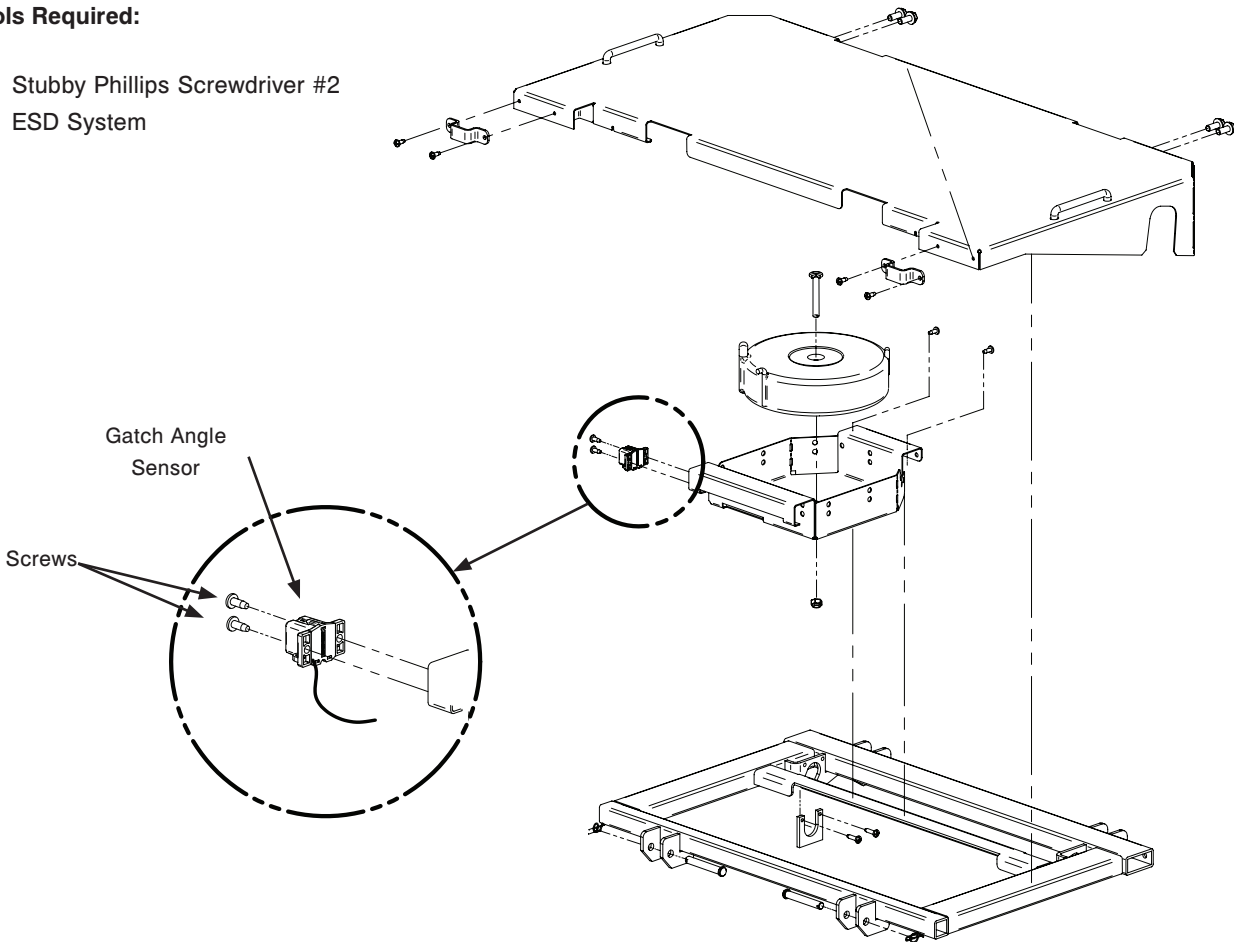

Procedure:


1. Plug bed into wall outlet.
 2. Set the brakes using one of the brake control locations or by using the manual brake pedal.
 3. Raise the bed to the full up position.
 4. If gatch motor will run, raise gatch up to approximately 20 degrees. If the gatch motor will not run, then put the bed into the calibration mode step one as shown on [page 23](#).
 5. Working from the bottom left side of the litter, under the gatch section, use a stubby Phillips screwdriver and remove the two screws securing the gatch angle sensor to the bottom of the gatch frame.
 6. Using an ESD system, properly ground yourself.
 7. Unclip the three clips holding the board cover on.
 8. Unplug the cable from the board.
 9. Reverse the steps to install new gatch angle sensor.
- Note: Do not over tighten the two screws.**
10. Recalibrate the bed (refer to Bed Calibration procedures on [page 23](#)).
 11. Test all bed functionality prior to putting the bed back into service.

Service Information

FOOT ANGLE SENSOR REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Phillips Screwdriver #2
- ESD System

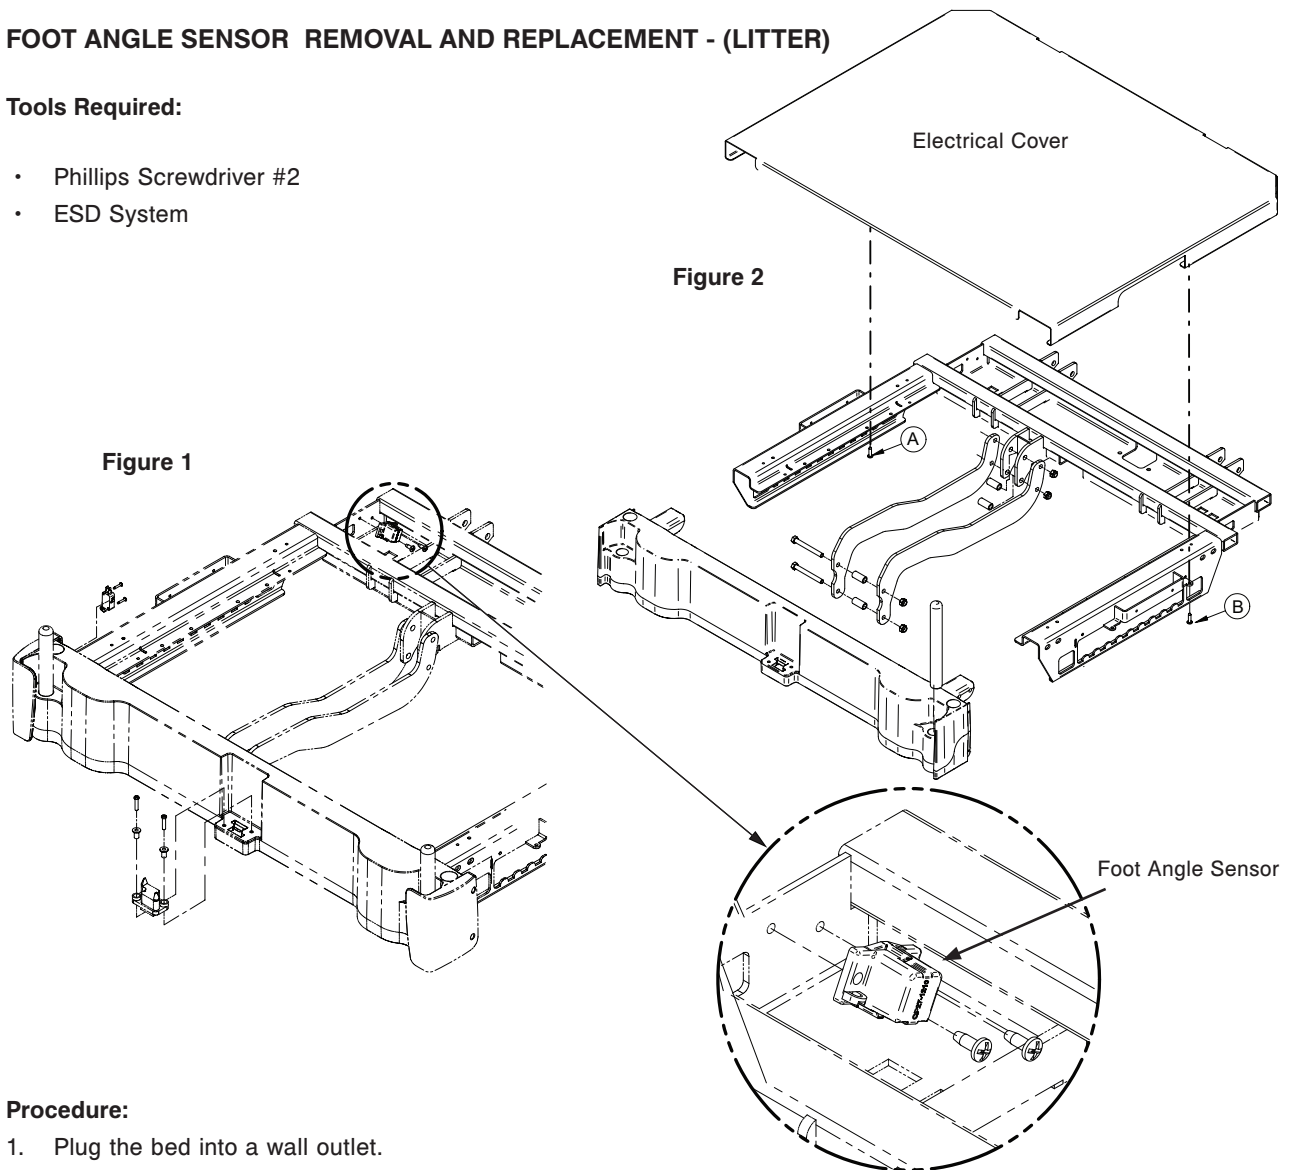

Procedure:


1. Plug the bed into a wall outlet.
 2. Raise the bed to the full up position and level the litter surface.
 3. Remove or fold back the mattress, exposing the foot section.
 4. Using a Phillips screwdriver, remove the two screws securing the electrical cover and then remove the cover (refer to Figure 1 above, item A and B).
 5. Using a Phillips screwdriver, remove the two screws securing the angle sensor to the foot frame (refer to Figure 2 above). **Note: Use caution as the cover is large and heavy.**
 6. Using an ESD system, properly ground yourself.
 7. Unclip the three clips holding the board cover on.
 8. Unplug the cable from the board.
 9. Reverse the steps to install the new foot angle sensor.
- Note: Do not over-tighten the two screws.**
10. Recalibrate the bed (refer to Bed Calibration procedures on [page 23](#)).
 11. Test all bed functionality prior to putting the bed back into service.

Service Information

BASE ANGLE SENSOR REMOVAL AND REPLACEMENT - (BASE)

Tools Required:

- Stubby Phillips Screwdriver
- ESD System

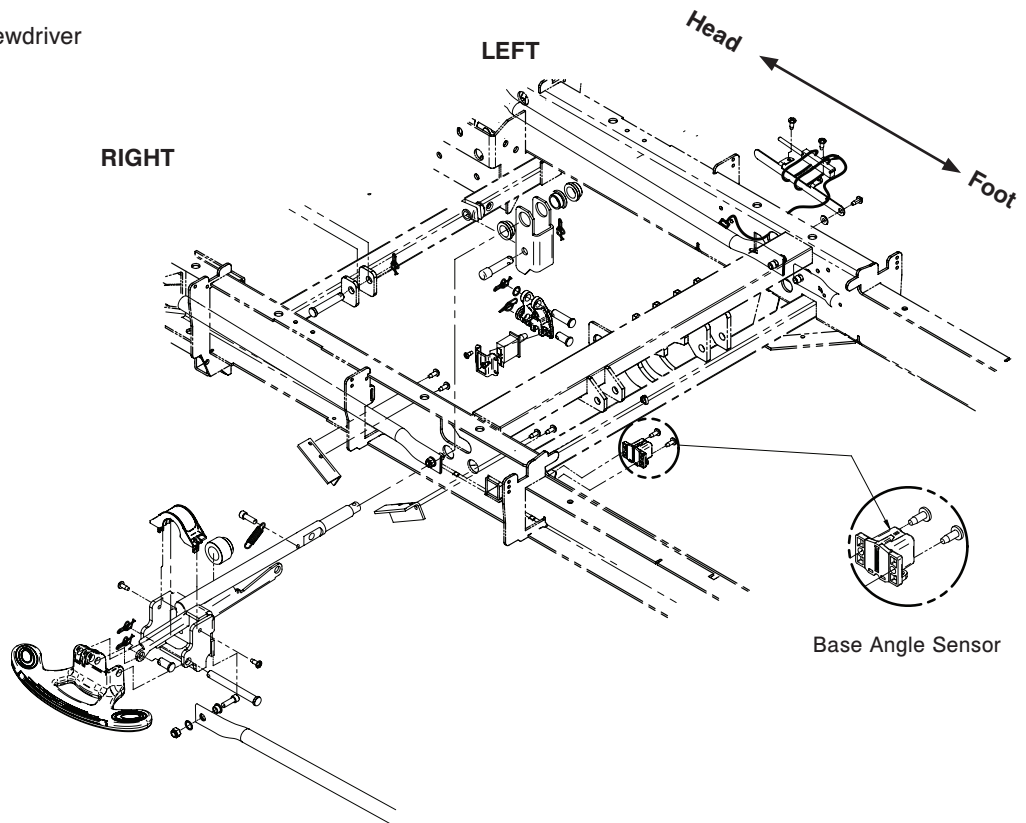

Procedure:


1. Plug the bed into a wall outlet.
 2. Set the brakes using one of the brake control locations or by using the manual brake pedal.
 3. Raise the bed to the full up position and raise the patient right siderails (foot end and head end).
 4. Remove the head end, enter, foot end, and right base cover.
 5. Using a Phillips screwdriver, remove the two screws securing the base angle sensor to the base frame (reference Figure above).
 6. Using an ESD system, properly ground yourself.
 7. Unclip the three clips holding the board cover on.
 8. Unplug the cable from the board.
 9. Reverse the steps to install new base angle sensor.
- Note: Do not over-tighten the two screws.**
10. Recalibrate the bed (refer to Bed Calibration procedures on [page 23](#)).
 11. Test all bed functionality prior to putting the bed back into service.

Service Information

TREND ANGLE SENSOR REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Phillips Screwdriver #2
- ESD System

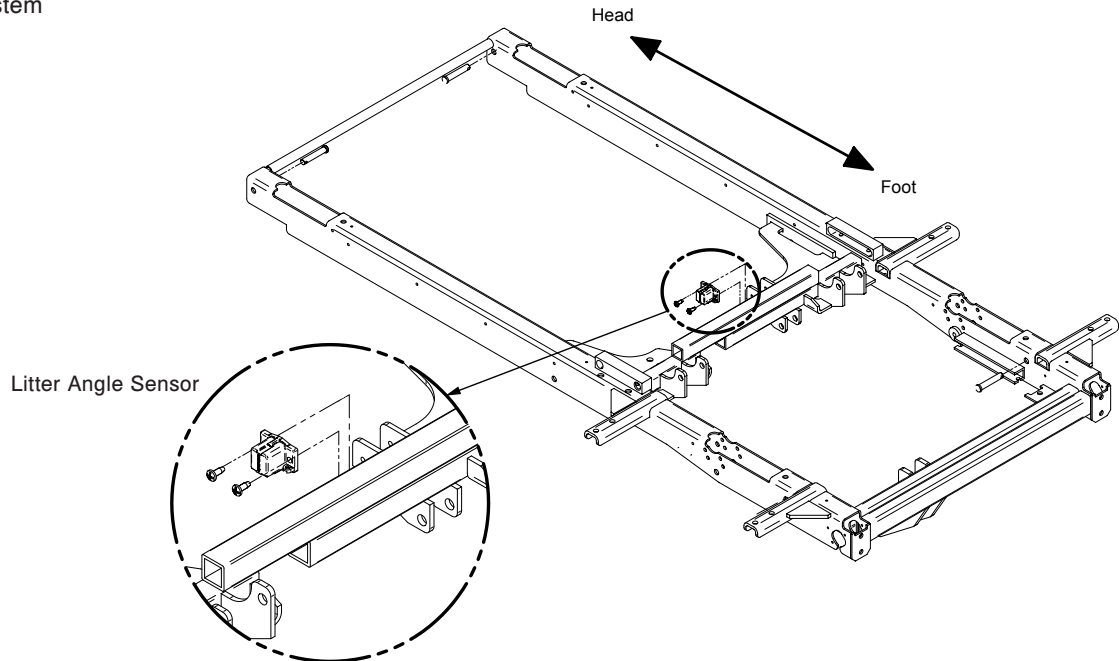

Procedure:

1. Plug the bed into a wall outlet.
2. Raise the bed to the full up position and raise the patient right siderail.
3. Working from the patient's right side, use a Phillips screwdriver and remove the two screws securing the trend angle sensor to the litter frame (refer to Figure above),
4. Using an ESD system, properly ground yourself.
5. Unclip the three clips holding the board cover on.
6. Unplug the cable from the board.
7. Reverse the steps to install new trend angle sensor.

Note: Do not over-tighten the two screws.


8. Recalibrate the bed (refer to Bed Calibration procedures on [page 23](#)).
9. Test all bed functionality prior to putting the bed back into service.

Service Information

HEADWALL COMMUNICATION BOARD REMOVAL AND REPLACEMENT - (LITTER)

Tools Required:

- Phillips Screwdriver #2
- ESD System

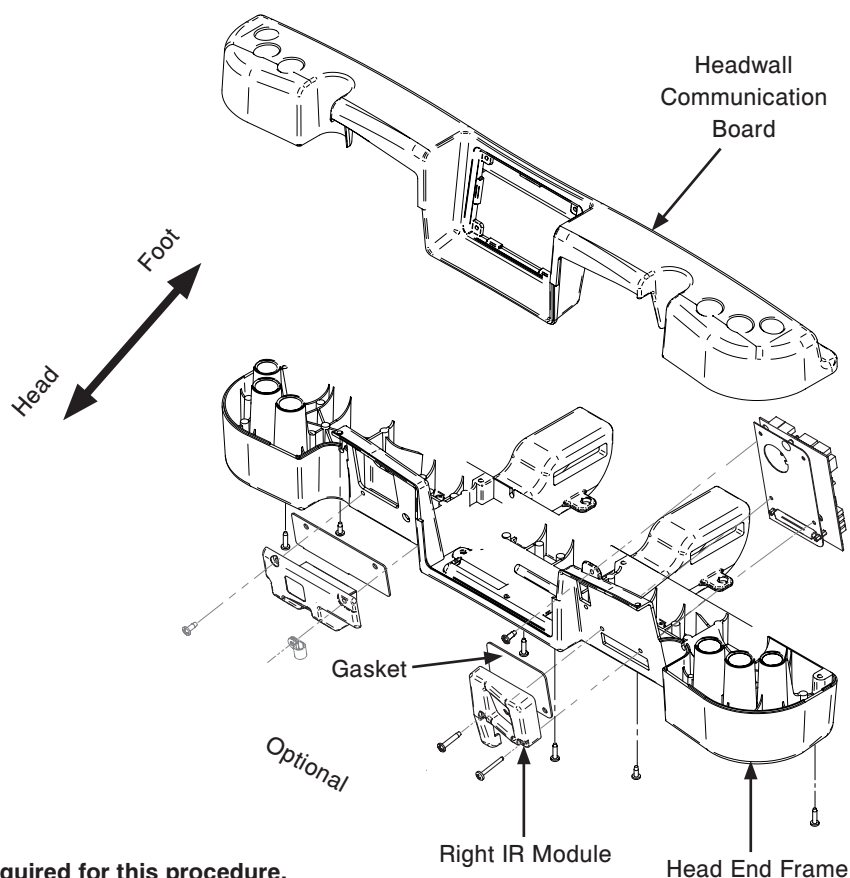

Procedure:

Note: ESD protection is required for this procedure.

1. Plug the bed into a wall outlet.
2. Raise the bed to the full up position.
3. Raise the fowler to the full up position.
4. Unplug the bed power cord from the wall outlet.
5. Turn the battery disconnect switch off.
6. Remove the headboard from the bed.
7. If the optional head end IV pole is present, use a 1/2" socket and 3/8" drive ratchet to remove the IV pole.
8. Using a Phillips screwdriver, remove the six screws that secure the head end frame cover to the head end frame.
9. Remove the head end frame cover and set aside.
10. Using a Phillips screwdriver, remove the two screws that secure the right IR module and gasket to the head end frame.

Note: Ensure the IR module cable is routed in the wire track before reinstallation.

11. Using a Phillips screwdriver, remove the screw that secures the headwall communication board to the head end frame.
12. Disconnect all of the cables going to the headwall communication board.

Note: Make note of all cable connections and dip switch settings on the headwall communication board.


13. Configure the new headwall communication board to match the dip switch settings from the old headwall communication board.
14. If the bed is equipped with the optional Smart TV, transfer the Smart TV board from the old headwall communication board to the new headwall communication board.
15. Reverse steps 12 through 1 to install the new headwall communication board.
16. Test all bed functionality before returning the bed to service.

Service Information

IR MODULE REMOVAL AND REPLACEMENT - (LITTER) (OPTIONAL)

Tools Required:

- Phillips Screwdriver #2
- Diagonal Pliers
- ESD System

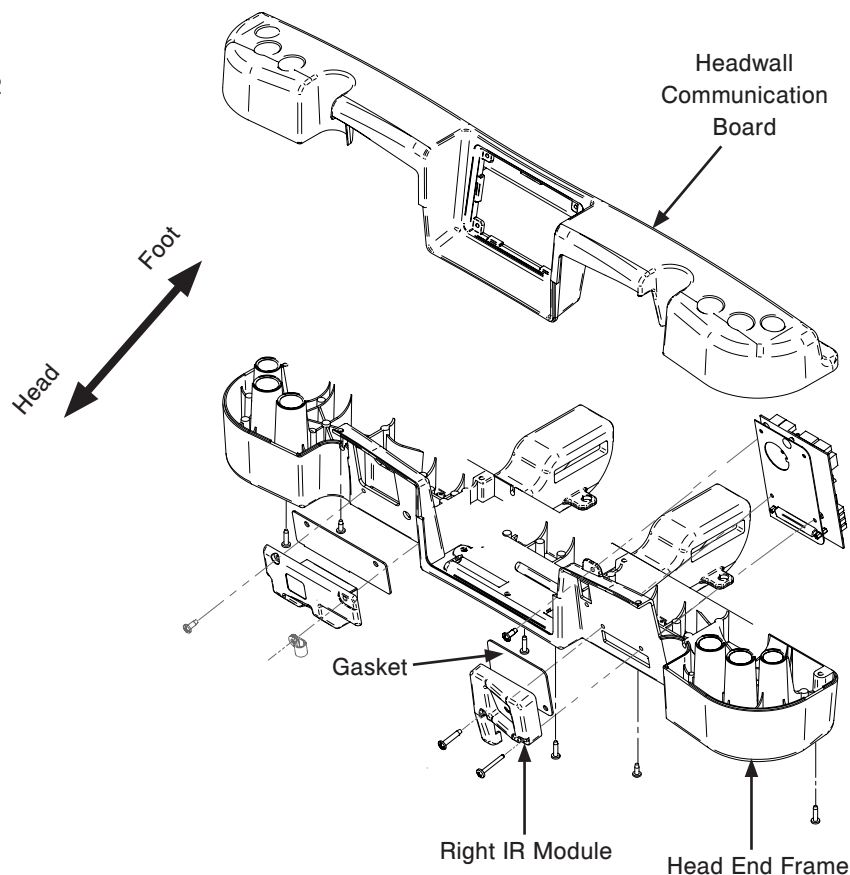

Procedure:

Note: ESD protection is required for this procedure.

1. Plug the bed into a wall outlet.
2. Raise the bed to the full up position.
3. Raise the fowler to the full up position.
4. Unplug the bed power cord from the wall outlet.
5. Turn the battery disconnect switch off.
6. Remove the headboard from the bed.
7. If the optional head end IV pole is present, use a 1/2" socket and 3/8" drive ratchet to remove the IV pole.
8. Using a Phillips screwdriver, remove the six screws that secure the head end frame cover to the head end frame.
9. Remove the head end frame cover and set aside.
10. Using a Phillips screwdriver, remove the two screws that secure the right IR module and gasket to the head end frame.

Note: Ensure the IR module cable is routed in the wire track before reinstallation.

11. Using a Phillips screwdriver, remove the two screws that secure the left IR module and gasket to the head end frame.
12. Using diagonal pliers, cut the cable tie that secures the IR module cables below the head end frame.
13. Disconnect the right IR module cable from connector J5 on the headwall communication board.
14. Disconnect the left IR module cable from connector J2 on the headwall communication board.
15. Reverse the procedure to install the new IR modules.

Note: Route both right and left IR module cables into the head end frame through the matching right and left Zoom® handle cable cutouts in the head end frame.


16. Test all bed functionality before returning the bed to service.

Service Information

WI-FI BOARD REMOVAL AND REPLACEMENT - (FOOTBOARD) (OPTIONAL)

Tools Required:

- Phillips Screwdriver #2
- Stubby Phillips Screwdriver #2
- Small Slotted Screwdriver
- Utility Knife
- ESD System

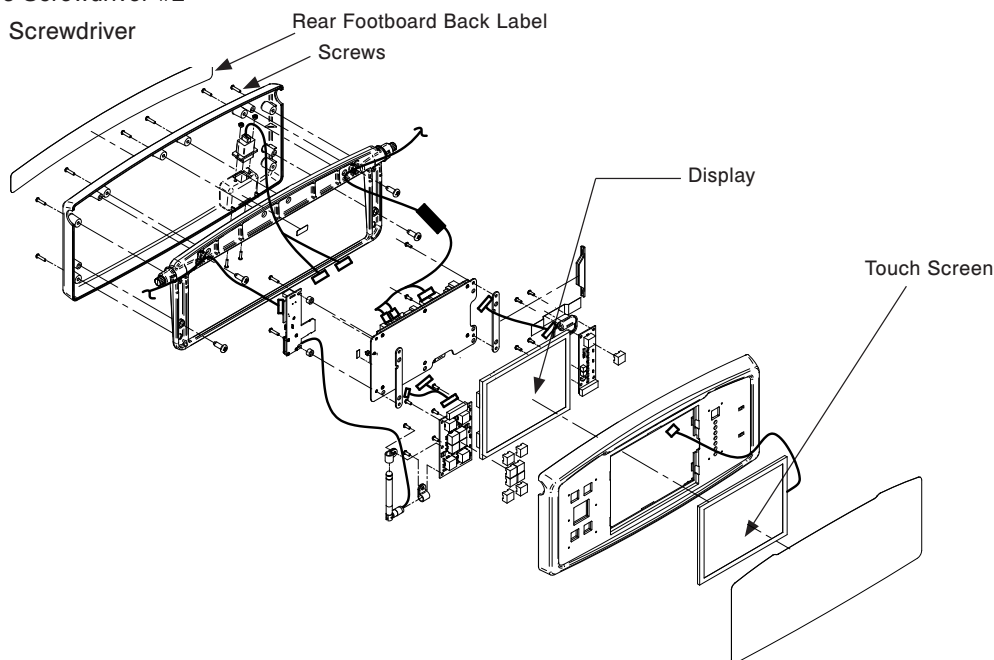

Procedure:

Note: The facility's IT department must be contacted to update the IP/DNS record for the affected product. The MAC address for the record will need to be updated from the old Wi-Fi board MAC address to the new Wi-Fi board MAC address. Failing to do so will prevent the unit from connecting to the facility's wireless network.

Note: ESD protection is required for this procedure.

1. On the footboard display screen, press the Wi-Fi antenna icon located in the lower left corner of the display.
2. Record the MAC address of the current Wi-Fi board.
3. Remove the footboard assembly and place onto a nearby work surface, face down.
4. Using a small slotted screwdriver or a utility knife, remove the rear footboard label.
Note: This label will need to be replaced with a new label (QDF27-1768).
5. Using a Phillips screwdriver, remove the six screws securing the footboard display panel to the footboard.
6. Pivot the display panel up and remove the two screws from the bottom of the display panel using a stubby Phillips screwdriver.
7. Hold the display panel and footboard assembly together and flip the footboard assembly over, with the display panel facing up.
8. Carefully remove the display panel from the footboard assembly and rotate over to display the circuit boards.
9. Using a Phillips screwdriver, remove the two screws that secure the Wi-Fi antenna P-clamps to the brake control board. Set the P-clamps aside for reinstallation.
10. Using a Phillips screwdriver, remove the two screws that secure the Wi-Fi board to the LCD interface board.
11. Unlock the Wi-Fi board from the LCD interface board by pressing in until it clicks.
12. Remove the Wi-Fi board from the LCD interface board.

Service Information

WI-FI BOARD REMOVAL AND REPLACEMENT - (FOOTBOARD) (OPTIONAL) (CONTINUED)

13. Reverse the procedure to install the new display.
14. On the footboard display screen, press the Wi-Fi antenna icon located in the lower left corner of the display.
15. Record the MAC address of the newly installed Wi-Fi board.
16. Provide the MAC addresses of the old Wi-Fi board and the new Wi-Fi board, along with the serial number of the unit, to the facility's IT department.


Note: The MAC address for the record will need to be updated from the old Wi-Fi board MAC address to the new Wi-Fi board MAC address. Failing to do so will prevent the unit from connecting to the facility's wireless network.

17. Configure the bed's Wi-Fi settings with hospital network information.
 - a. Access the Configuration Menu by referencing the procedure on [page 23](#).
 - b. On the Configuration Menu screen, press Wi-Fi Configuration.
 - c. Press the Advanced tab.
 - d. Press Reset.
 - e. Press OK.
 - f. Press Save.
 - g. In the pop-up message screen, press Close.
 - h. Using the Wi-Fi configuration tabs, configure the bed to the hospital network settings.
 - i. Once configured, press Save.
 - j. In the pop-up message screen, press Close.
18. Press the Wi-Fi antenna icon on the bottom left corner of the touch screen.
 - a. Verify the bed has connected to the hospital network by looking for brackets around the antenna in the Wi-Fi icon in the bottom left corner of the touch screen.
 - b. Press the Wi-Fi icon in the bottom left corner of the touch screen and verify the bed received a proper hospital issued IP address.
19. Test all bed functionality before returning the bed to service.

Base Assembly, Hood


(Applies to beds with Serial Numbers U01001 - U51437)

L27-026 Rev-07 (Reference Only)

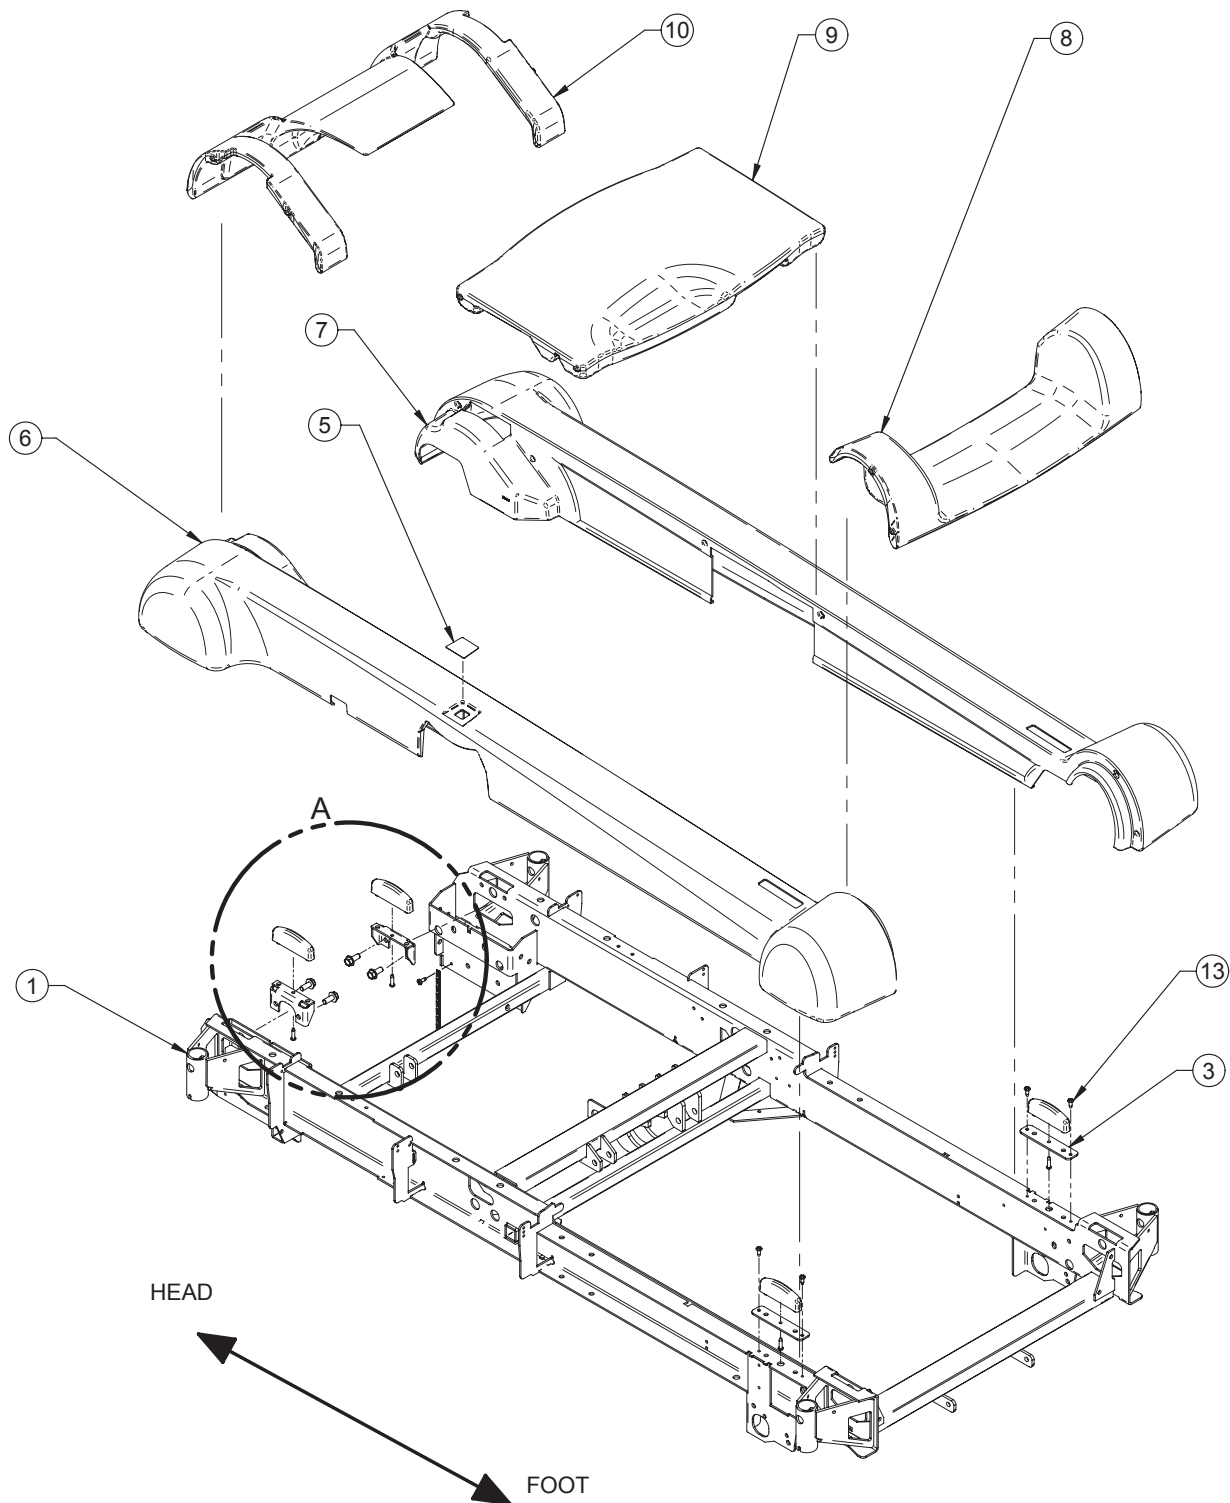

Base Assembly, Hood

(Applies to beds with Serial Numbers U01001 - U51437)

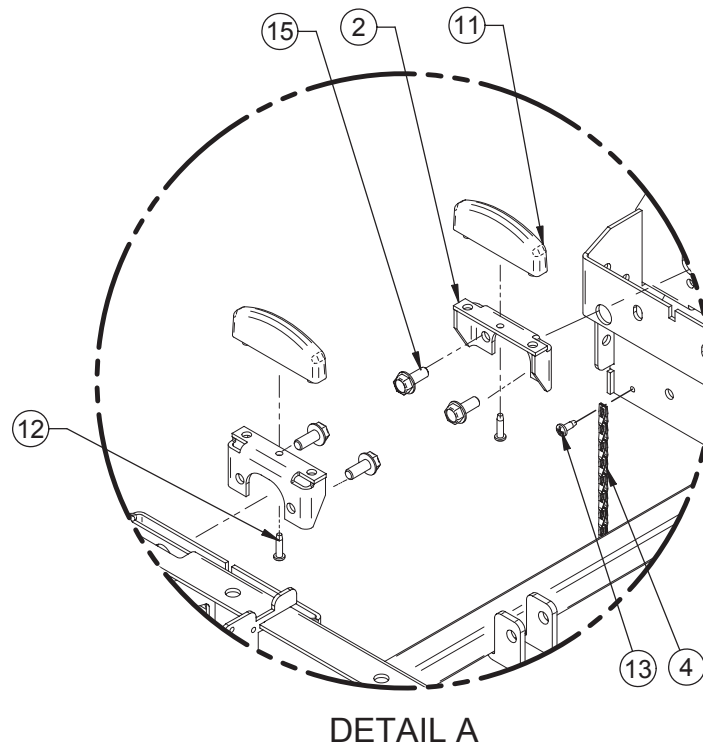


Base Assembly, Hood - L27-026 Rev-07 (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-0758P	Base Assembly	1
2	27-1462P	Support Stopper	2
3	27-1628P	Foot Stopper Support	2
4	27-2123	Ground Chain	1
5	QDF27-1419	Base Transparent Plate	1
6	QP27-1008	Right Base Cover	1
7	QP27-1009	Left Base Cover	1
8	QP27-1087	Foot Base Cover	1
9	QP27-1093	Center Base Cover	1
10	QP27-1105	Head Base Cover	1
11	QP27-1461	Stopper in Base	4
12	VV23A1G24HL	Tapping Screw	4
13	VV83A9G16	Tapping Screw	5
15	VVB4A1O24	Thread Rolling Bolt	4

Base Assembly, Hood


(Applies to beds with Serial Numbers U51438 - Current)

L27-026 Rev J (Reference Only)

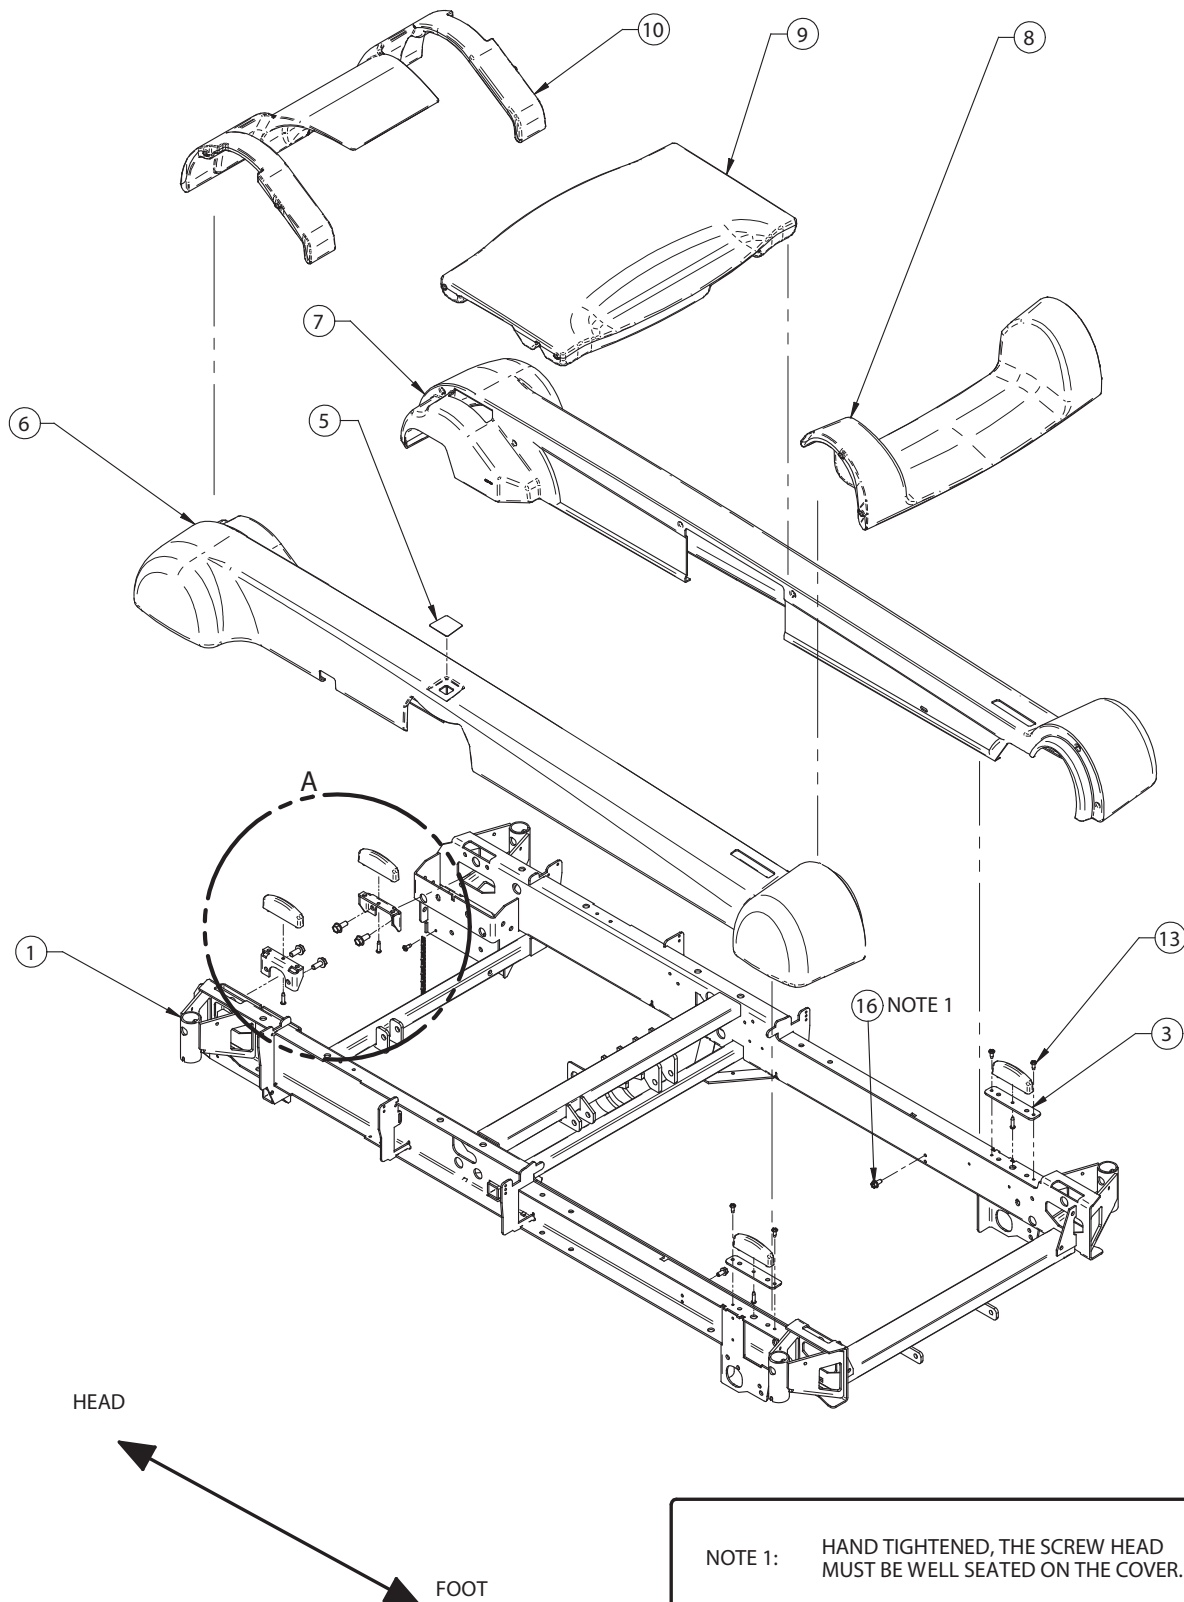

Base Assembly, Hood

(Applies to beds with Serial Numbers U51438 - Current)

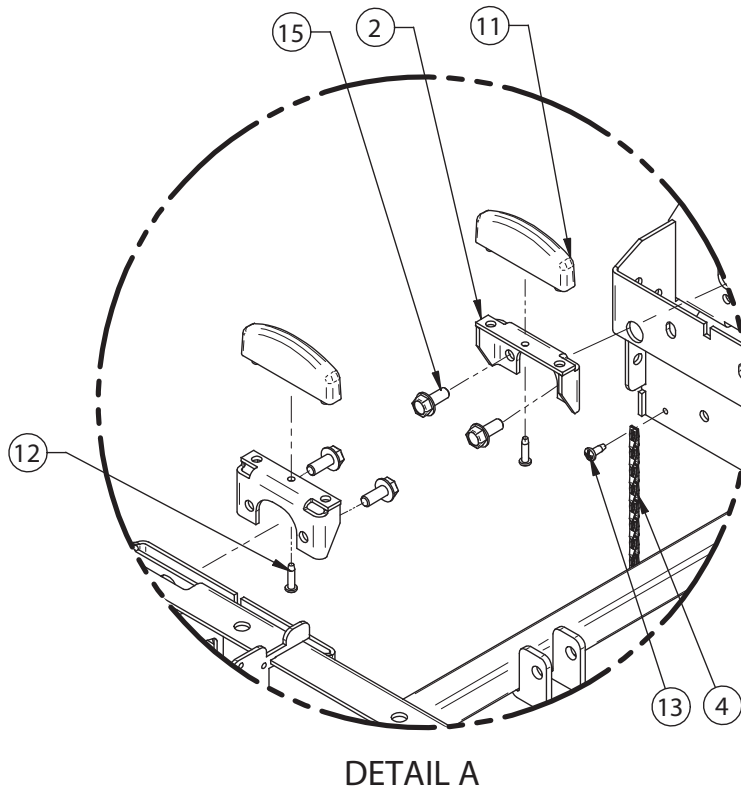


Base Assembly, Hood - L27-026 Rev J (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-0758P	Base Assembly	1
2	27-1462P	Support Stopper	2
3	27-1628P	Foot Stopper Support	2
4	27-2123	Ground Chain	1
5	QDF27-1419	Base Transparent Plate	1
6	QP27-1008	Right Base Cover	1
7	QP27-1009	Left Base Cover	1
8	QP27-1087	Foot Base Cover	1
9	QP27-1093	Center Base Cover	1
10	QP27-1105	Head Base Cover	1
11	QP27-1461	Stopper in Base	4
12	VV23A1G24HL	Tapping Screw	4
13	VV83A9G16	Tapping Screw	5
15	VVB4A1O24	Thread Rolling Bolt	4
16	VV84A1I16	Flanged Hex Head Tapping Screw	2

Base Assembly, Brake

(Applies to beds with Serial Numbers U01001 - U02817)


L27-020 Rev-16 (Reference Only)

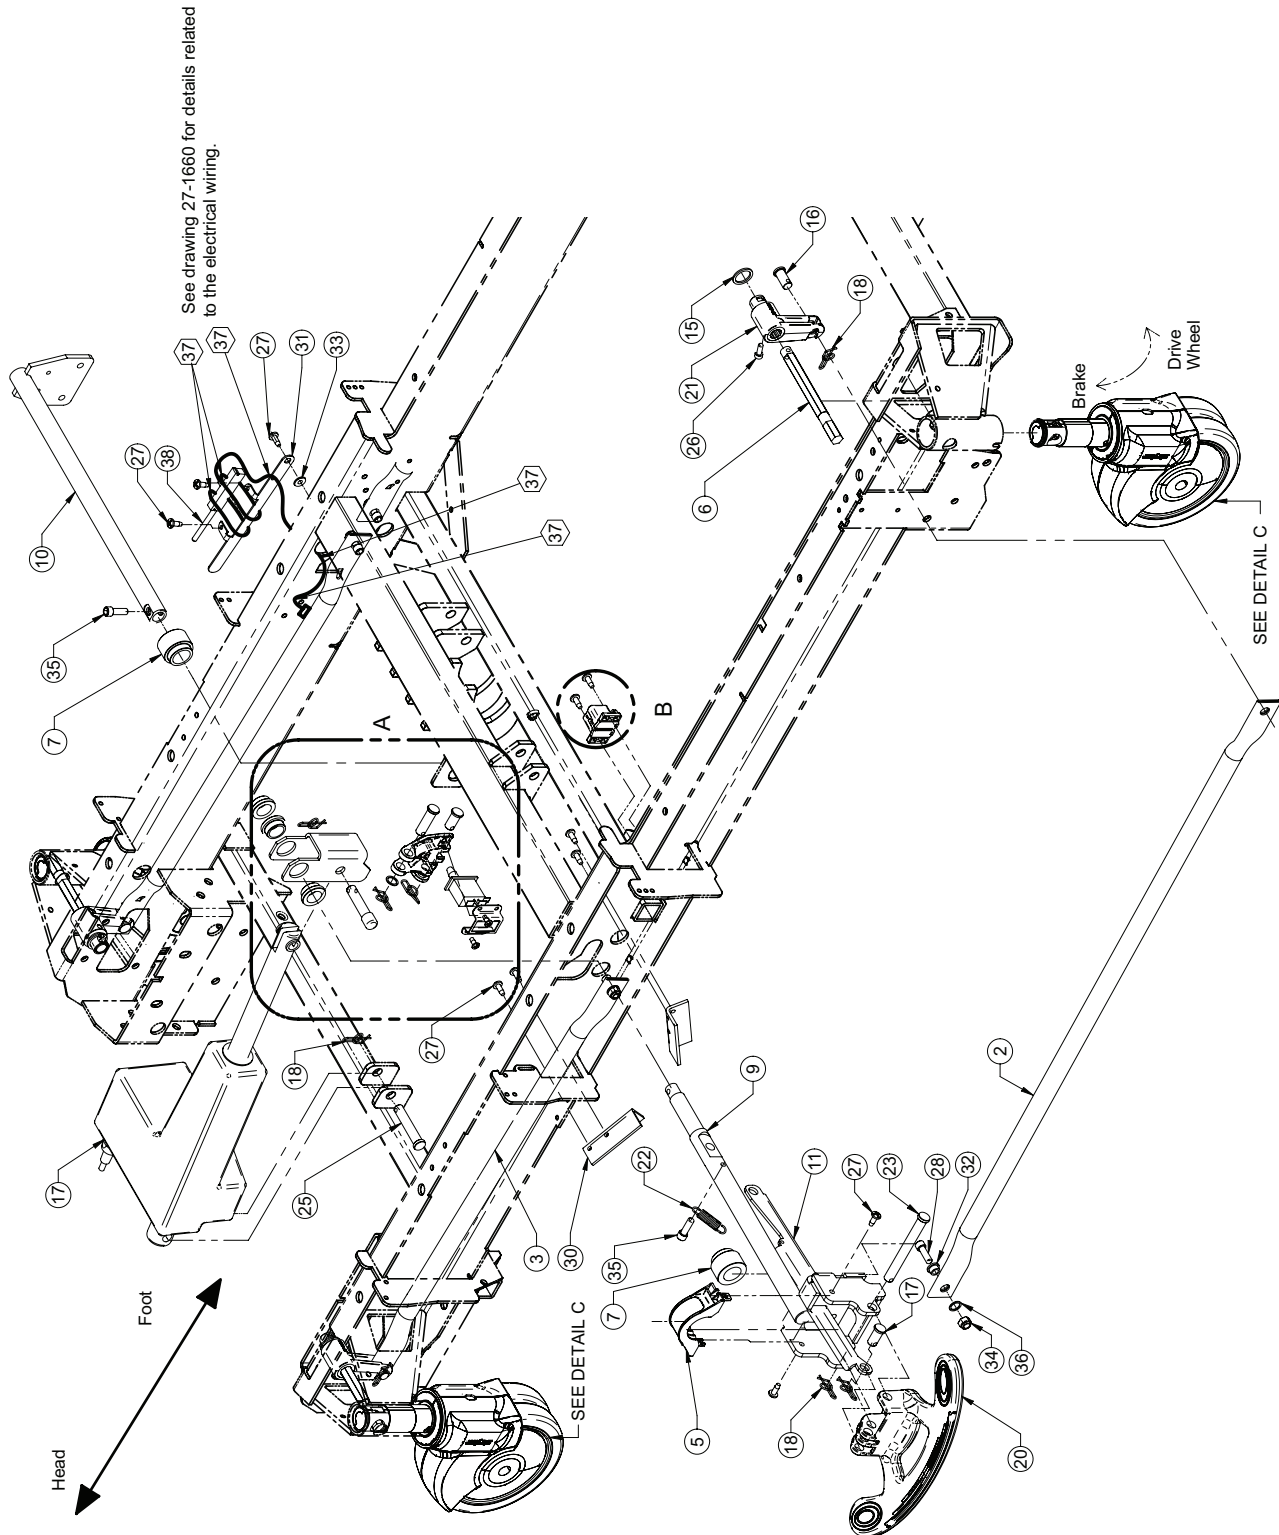


Base Assembly, Brake

(Applies to beds with Serial Numbers U01001 - U02817)


The angle sensor orientation is important. Wire should exit towards the bottom.

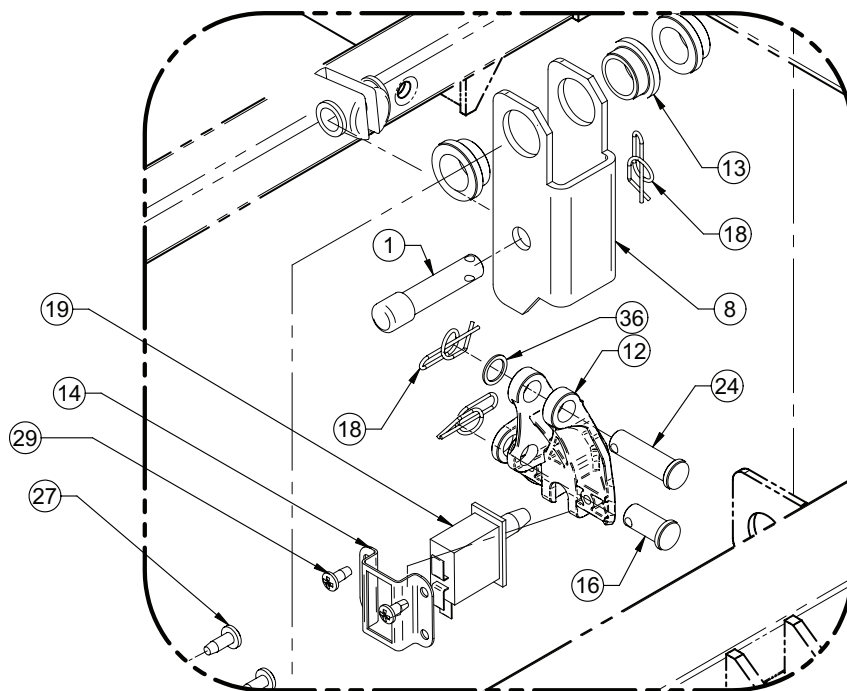

Detail A

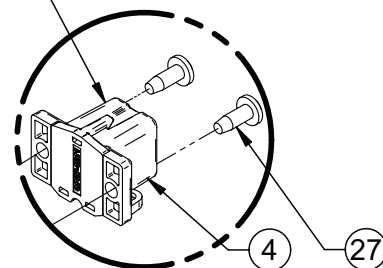


Detail B

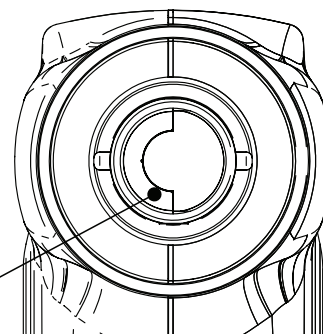

Place wheel axis with biggest hole towards head of bed when the cam is in neutral.

Detail C

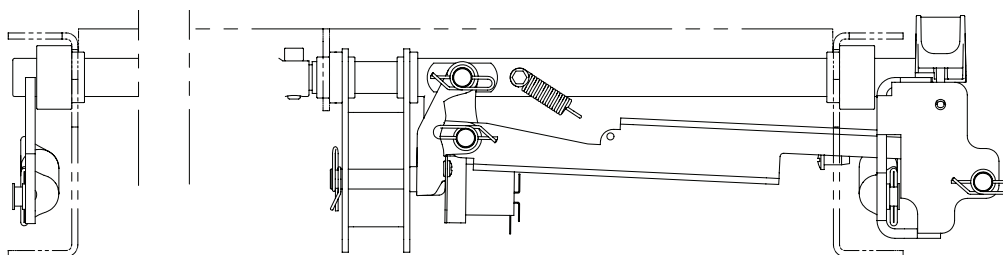

View of Assembled Brake System

Base Assembly, Brake

(Applies to beds with Serial Numbers U01001 - U02817)


Base Assembly, Brake - L27-020 Rev-16 (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-1402Z	Brake Clevis pin	1
2	27-0772Z	Foot Brake Tube	2
3	27-0773Z	Head Brake Tube	2
4	27-1209	Angle Sensor	1
5	27-1255-10	Brake Indicator	1
6	27-1336Z	Casters Activation Roller Strike	4
7	27-1354	Brake Bearing	2
8	27-1391Z	Brake Actuator Pivot	1
9	27-1405Z	Right Brake Cross Member	1
10	27-1406Z	Left Brake Cross Member	1
11	27-1411Z	Brake Shift Control Stem	1
12	27-1448	Brake Trigger	1
13	27-1449	Braking Bearing	3
14	27-1452Z	Microswitch Bracket	1
15	VW10C202802	Washer	4
16	VG50A1224	Clevis Pin	6
17	QDF27-1227	Brake Actuator	1
18	QDF7878	Fastener Pin	10
19	QDF9159	Cherry Limit Switch	1
20	QPA27-1165	Emergency Pedal	1
21	QPA27-1335	Brake Lever	4
22	QRE27-1844	Extension Spring	1
23	VG50A1259	Clevis Pin	1
24	VG50B1236	Clevis Pin	1
25	VG50B1248	Clevis Pin	1
26	VV10A0G16-S	Hexagon Cylinder Head	4
27	VV83A9G16	Tapping Screw	11
28	VV10A1N24	Hexagon Cylinder Head	4
29	VV83A9E12	Tapping Screw	2
30	27-1745Z	Head Brake Microswitch Stop	2
31	27-1946Z	Potentiometer Support	1
33	27-1948	Copper Sleeve Spacer	1
34	VE30A1N	Nylon Locknut	4
35	VV10A1N24-S	Cylinder Head Hex Screw	2
36	VW10C121601	Nylon Washer	5
37	QDF9518	Cable Tie	1
38	M0019	Grease	1
39	QDF27-2024	Position Sensor	1
40	VW10C081602	Nylon Washer	1
41	QB2938T1	Sleeve	4

Base Assembly, Brake

(Applies to beds with Serial Numbers U02818 - Current)


L27-043 Rev-02 (Reference Only)

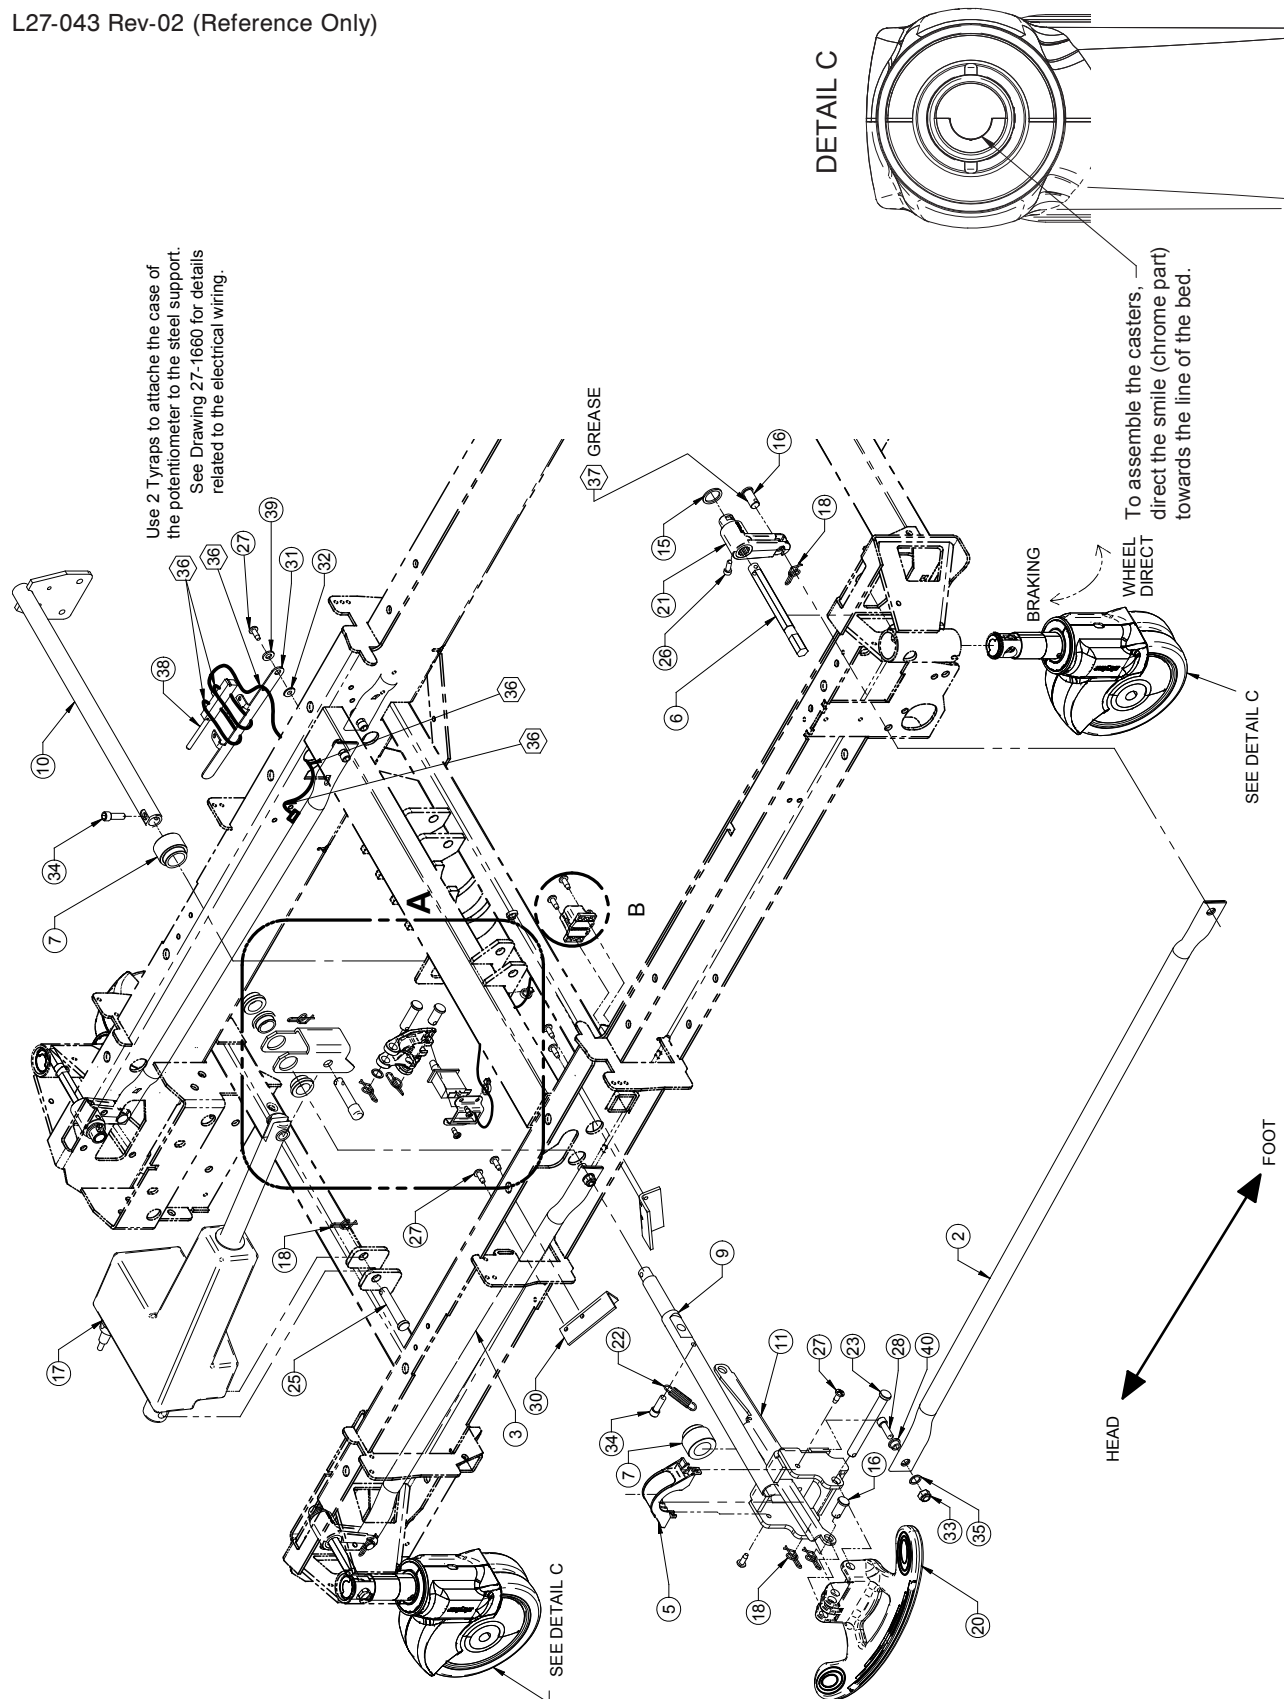

[Return To Table of Contents](#)


Base Assembly, Brake

(Applies to beds with Serial Numbers U02818 - Current)

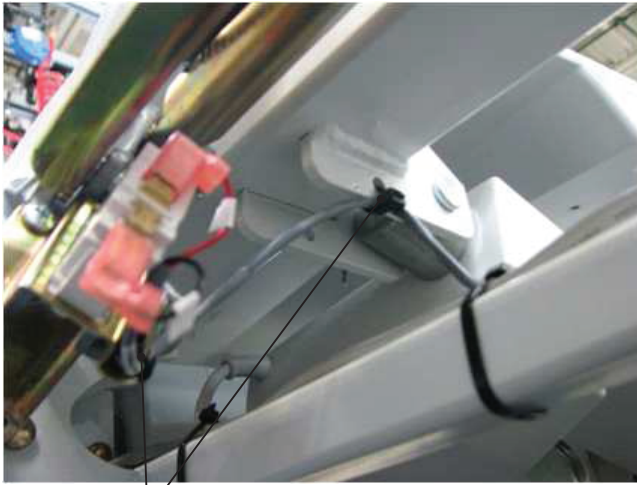


Tyrap positioning


The angle sensor orientation is very important. Wire should exit towards the bottom.

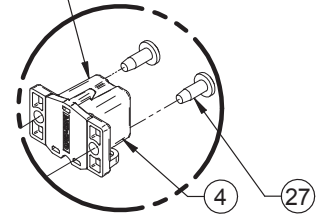

DETAIL B

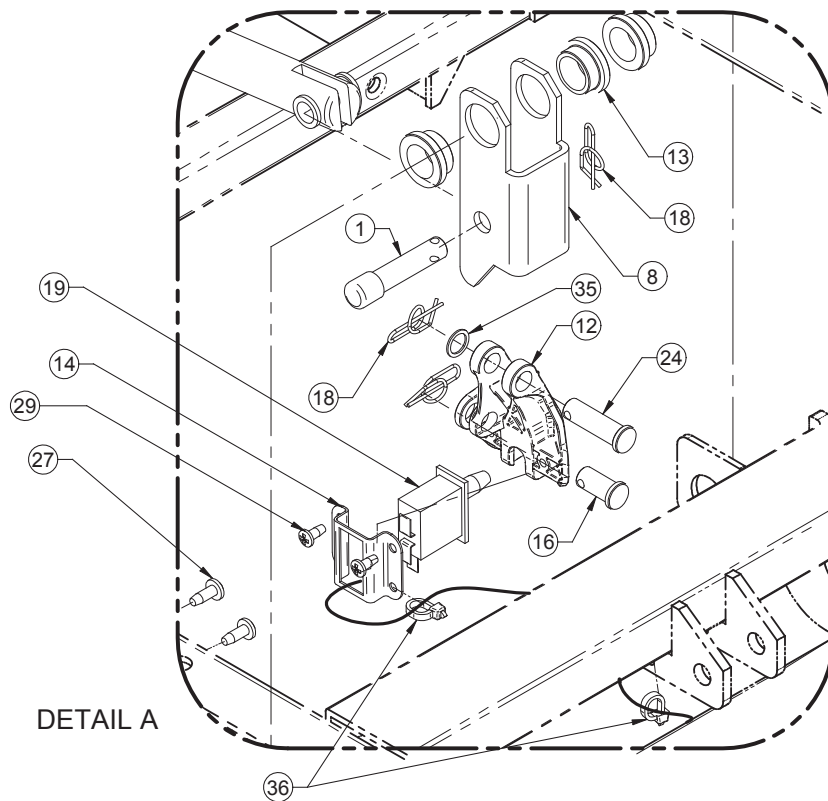

DETAIL A

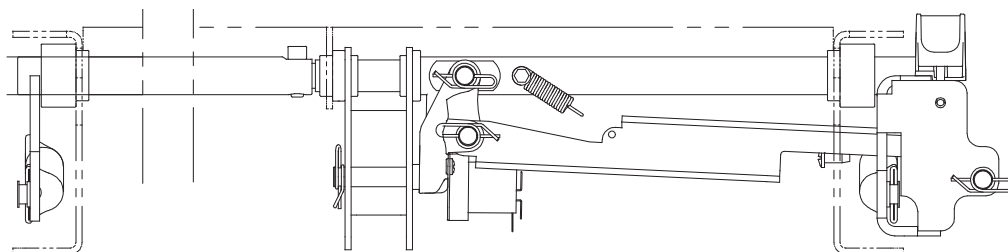

View of Assembled Brake System

Base Assembly, Brake

(Applies to beds with Serial Numbers U02818 - Current)


Base Assembly, Brake - L27-043 Rev-02 (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-1402Z	Brake Clevis pin	1
2	27-0772Z	Foot Brake Tube	2
3	27-0773Z	Head Brake Tube	2
4	27-2477	Angle Sensor Assembly	1
5	QP27-1255	Brake Indicator	1
6	27-1336Z	Casters Activation Roller Strike	4
7	27-1354	Brake Bearing	2
8	27-1391Z	Brake Actuator Pivot	1
9	27-1405Z	Right Brake Cross Member	1
10	27-1406Z	Left Brake Cross Member	1
11	27-1411Z	Brake Shift Control Stem	1
12	QPA27-1448	Brake Trigger	1
13	27-1449	Braking Bearing	3
14	27-1452Z	Microswitch Bracket	1
15	VW10C202802	Washer	4
16	VG50A1224	Clevis Pin	6
17	QDF27-1227	Brake Actuator	1
18	QDF7878	Fastener Pin	10
19	QDF9159	Cherry Limit Switch	1
20	27-2519P	Emergency Pedal	1
21	QPA27-1335	Brake Lever	4
22	QRE27-1844	Extension Spring	1
23	VG50A1259	Clevis Pin	1
24	VG50B1236	Clevis Pin	1
25	VG50B1248	Clevis Pin	1
26	VV10A0G16-S	Hexagon Cylinder Head	4
27	VV83A9G16	Tapping Screw	9
28	VV10A1N24	Hexagon Cylinder Head	4
29	VV83A9E12	Tapping Screw	2
30	27-1745Z	Head Brake Microswitch Stop	2
31	27-1946Z	Potentiometer Support	1
32	27-1948	Copper Sleeve Spacer	1
33	VE30A1N	Nylon Locknut	4
34	VV10A1N24-S	Cylinder Head Hex Screw	2
35	VW10C121601	Nylon Washer	5
36	QDF9518	Cable Tie	3
37	M0019	Grease	1
38	QDF27-2024	Position Sensor	1
39	VW10C081602	Nylon Washer	1
40	QB2938T1	Sleeve	4

Base Assembly, Caster Lock (Model 2131 Only)

(Applies to beds with Serial Numbers U01001 - U51437)

OL270006 Rev-02 (Reference Only)

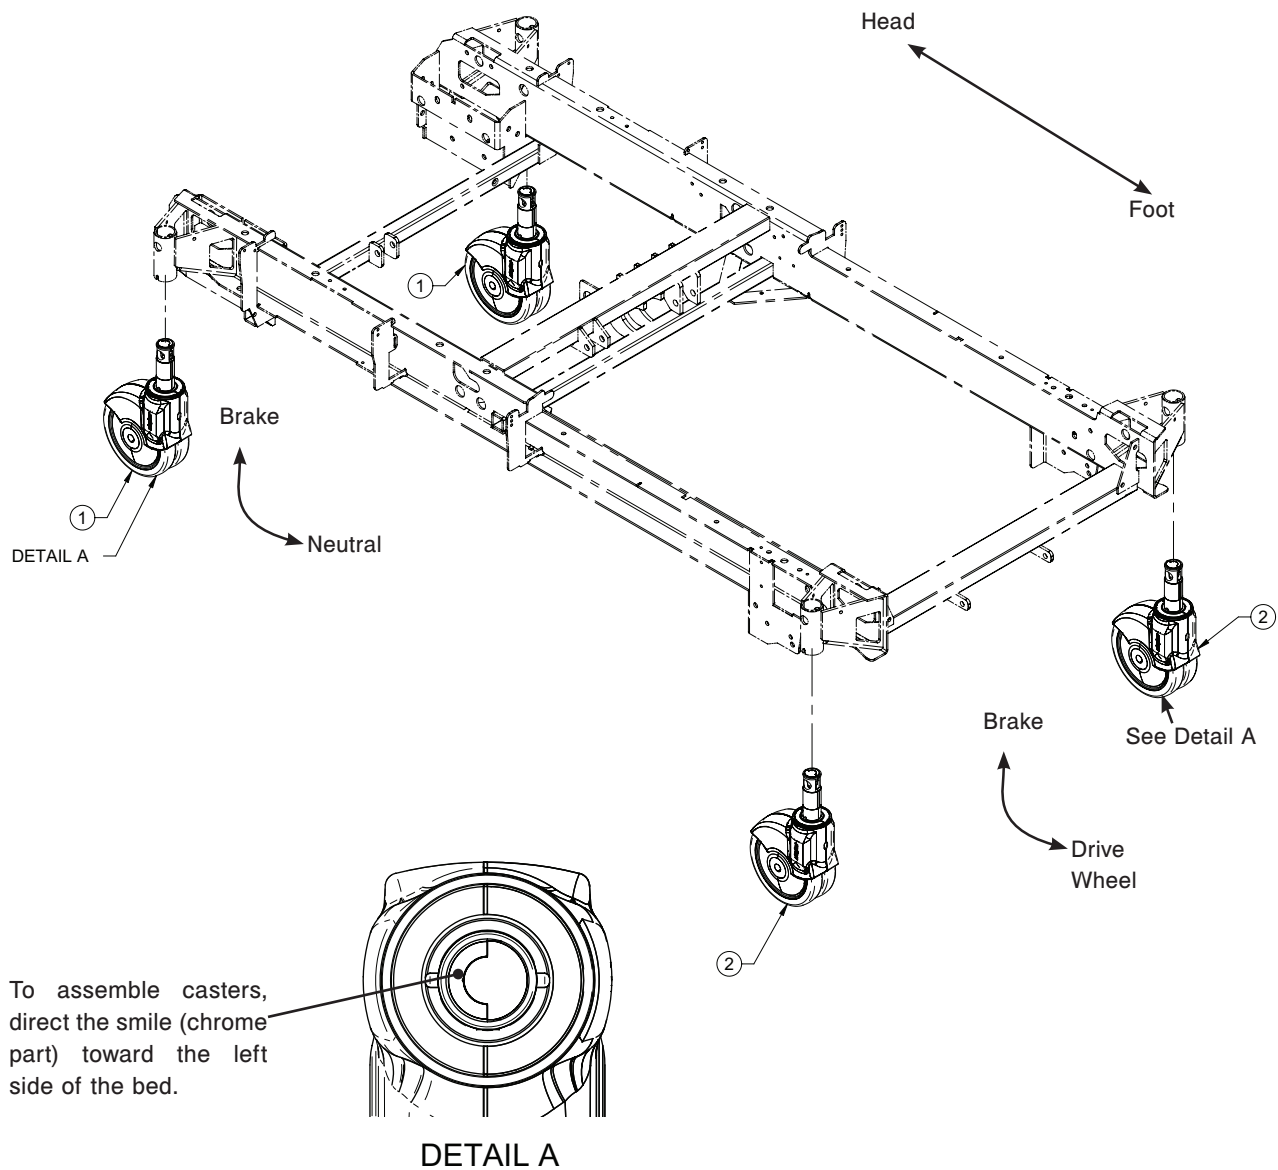


Item	Part No.	Part Name	Qty.
1	RD27-1970	5.5" Caster Brake/Neutral/Neutral	2
2	RD27-1971	5.5" Caster Brake/Neutral/Drive	2

Base Assembly, Caster Non-Lock (Model 2141 Only)

(Applies to beds with Serial Numbers U01001 - U51437)

OL270005 Rev-02 (Reference Only)

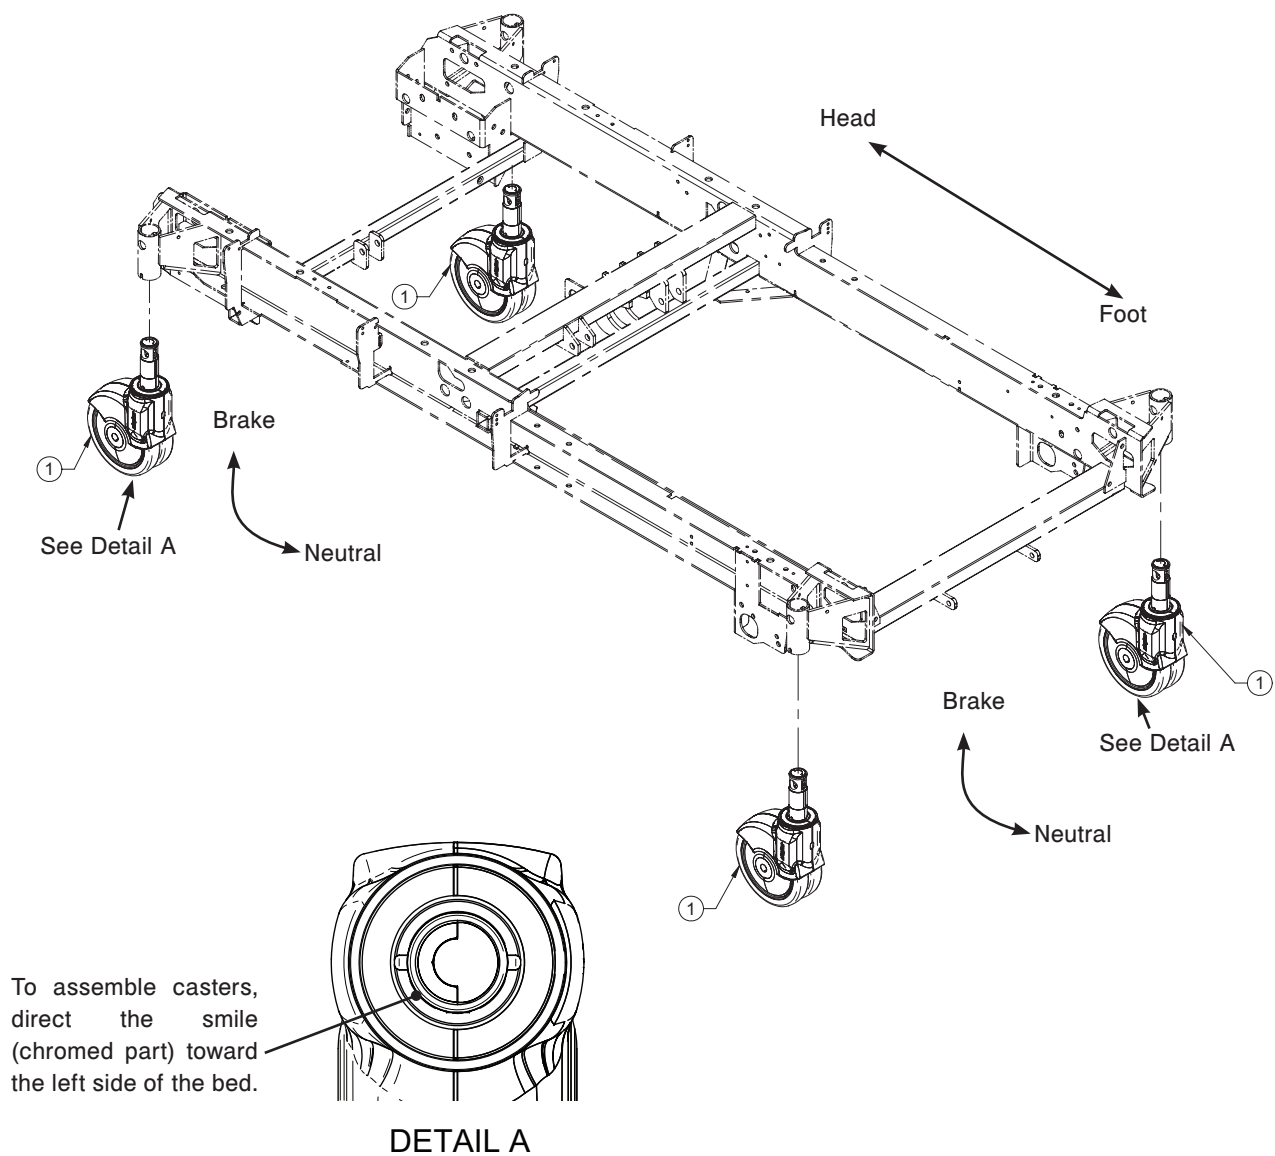


Item	Part No.	Part Name	Qty.
1	RD27-1970	5.5" Caster Brake/Neutral/Neutral	4

Base Assembly, Caster Lock (Model 2131 Only)

(Applies to beds with Serial Numbers U51438 - Current)

OL270006 Rev D (Reference Only)

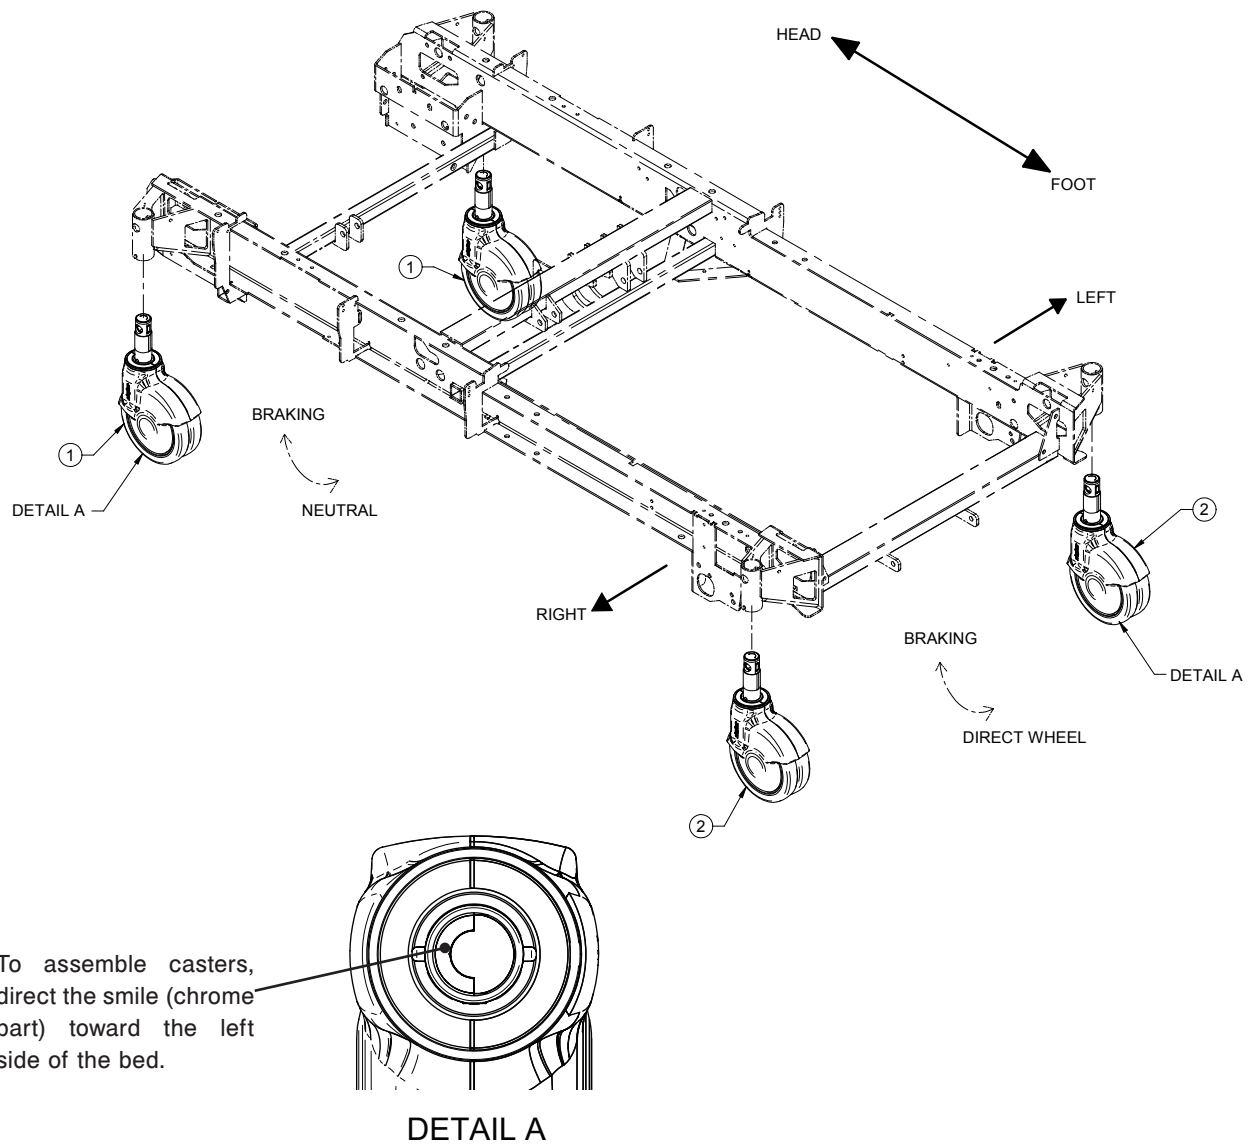


Item	Part No.	Part Name	Qty.
1	RD27-2787	5.5" Caster Brake/Neutral/Neutral	2
2	RD27-2788	5.5" Caster Brake/Neutral/Drive	2

Base Assembly, Caster Non-Lock (Model 2141 Only)

(Applies to beds with Serial Numbers U51438 - Current)

OL270005 Rev D (Reference Only)

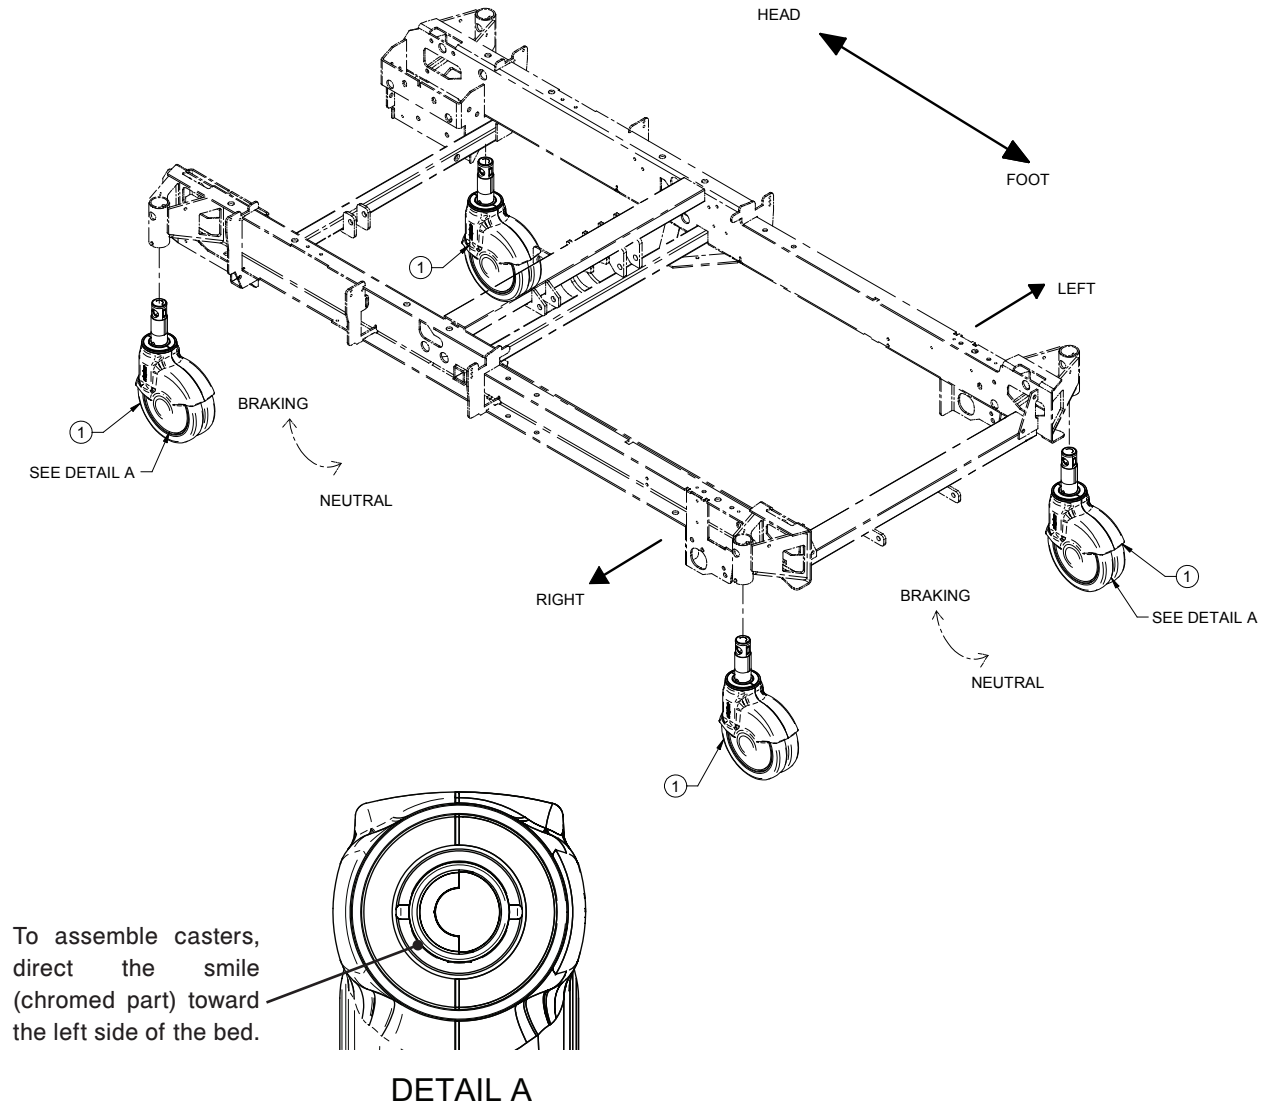


Item	Part No.	Part Name	Qty.
1	RD27-2787	5.5" Caster Brake/Neutral/Neutral	4

Angle Sensor Assembly

27-1209 (Applies to beds with Serial Numbers U01001 - U02817)


27-2477 (Applies to beds with Serial Numbers U02818 - Current)

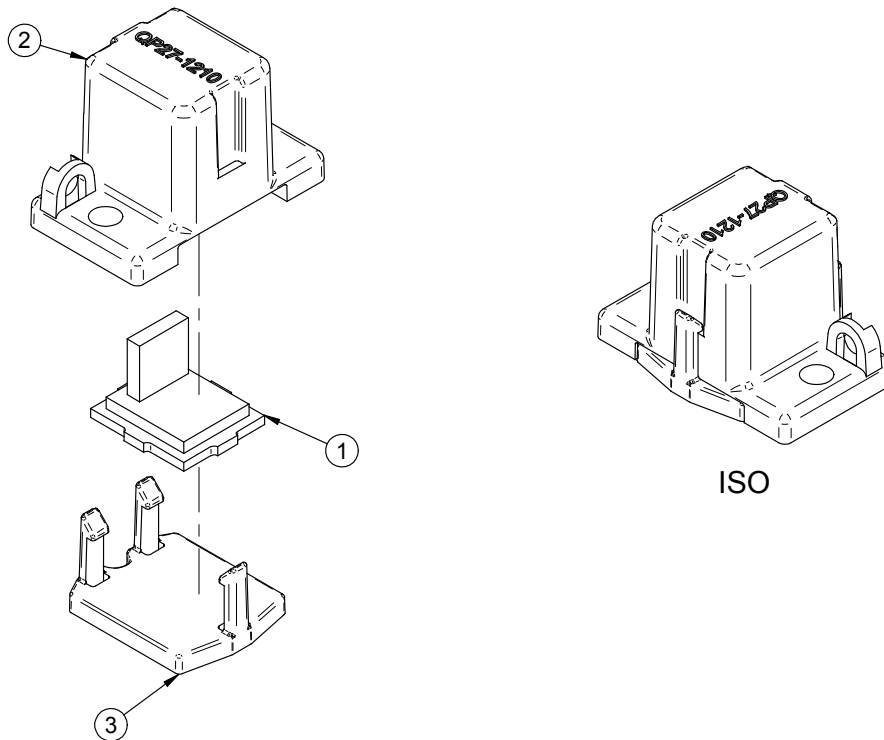

Item	Part No.	Part Name	Qty.
1	QDF27-1551	Angle Sensor	1 (U01001 - U02817)
	QDF75-0140	Angle Sensor	1 (U02818 - Current)
2	QP27-1210	Angle Sensor Case	1
3	QP27-1211	Bottom Lid for Tilt Sensor	1


Base Assembly, Electrical

27-2709 Rev A (Reference Only)

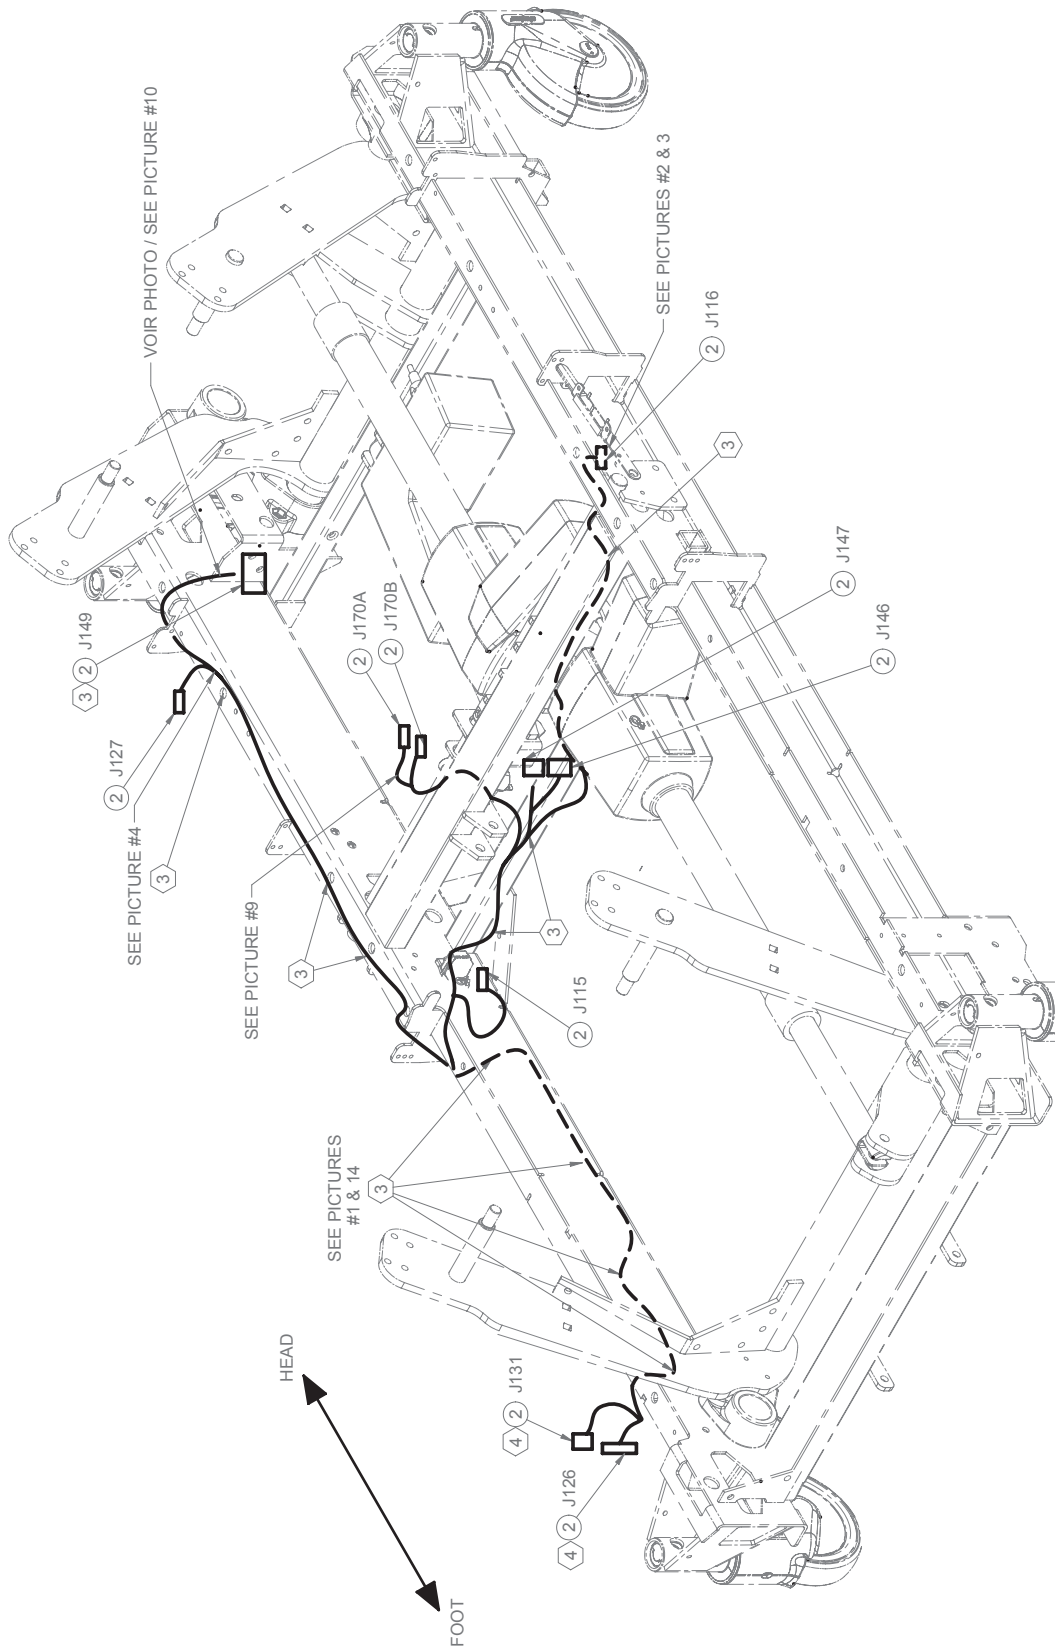

[Return To Table of Contents](#)

Base Assembly, Electrical

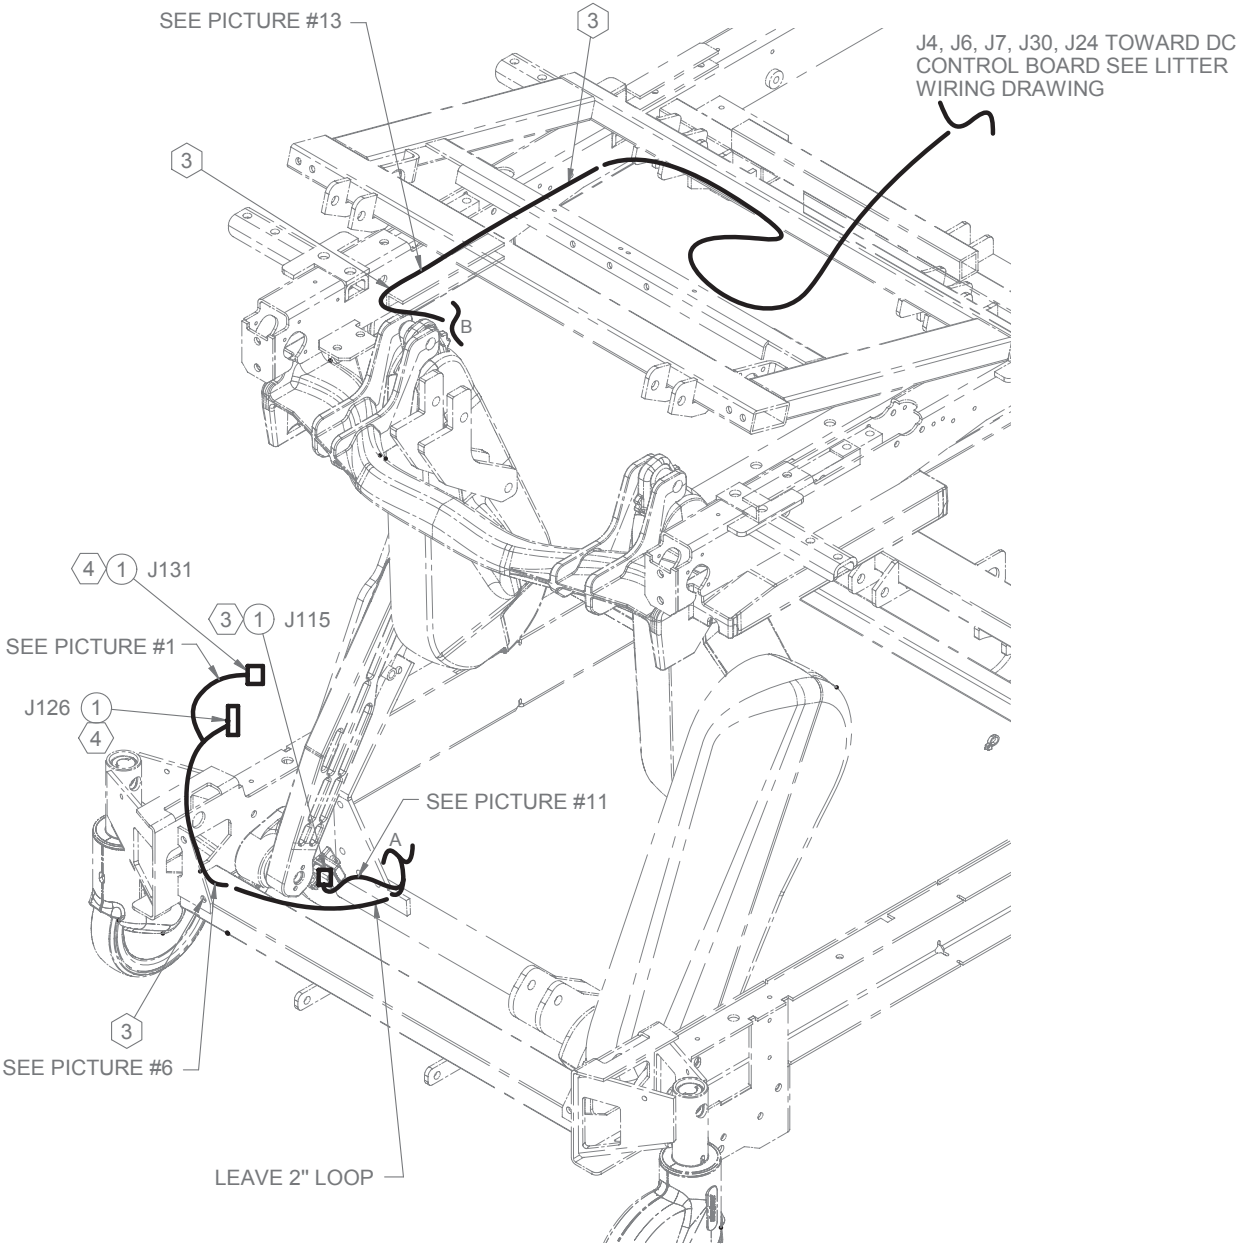


Base Assembly, Electrical

Note

To avoid any risk of pinching when assembling these cables:

- Bed must be in high position
- Gatch must be at 15 degrees
- Foot Litter must be at 45 degrees

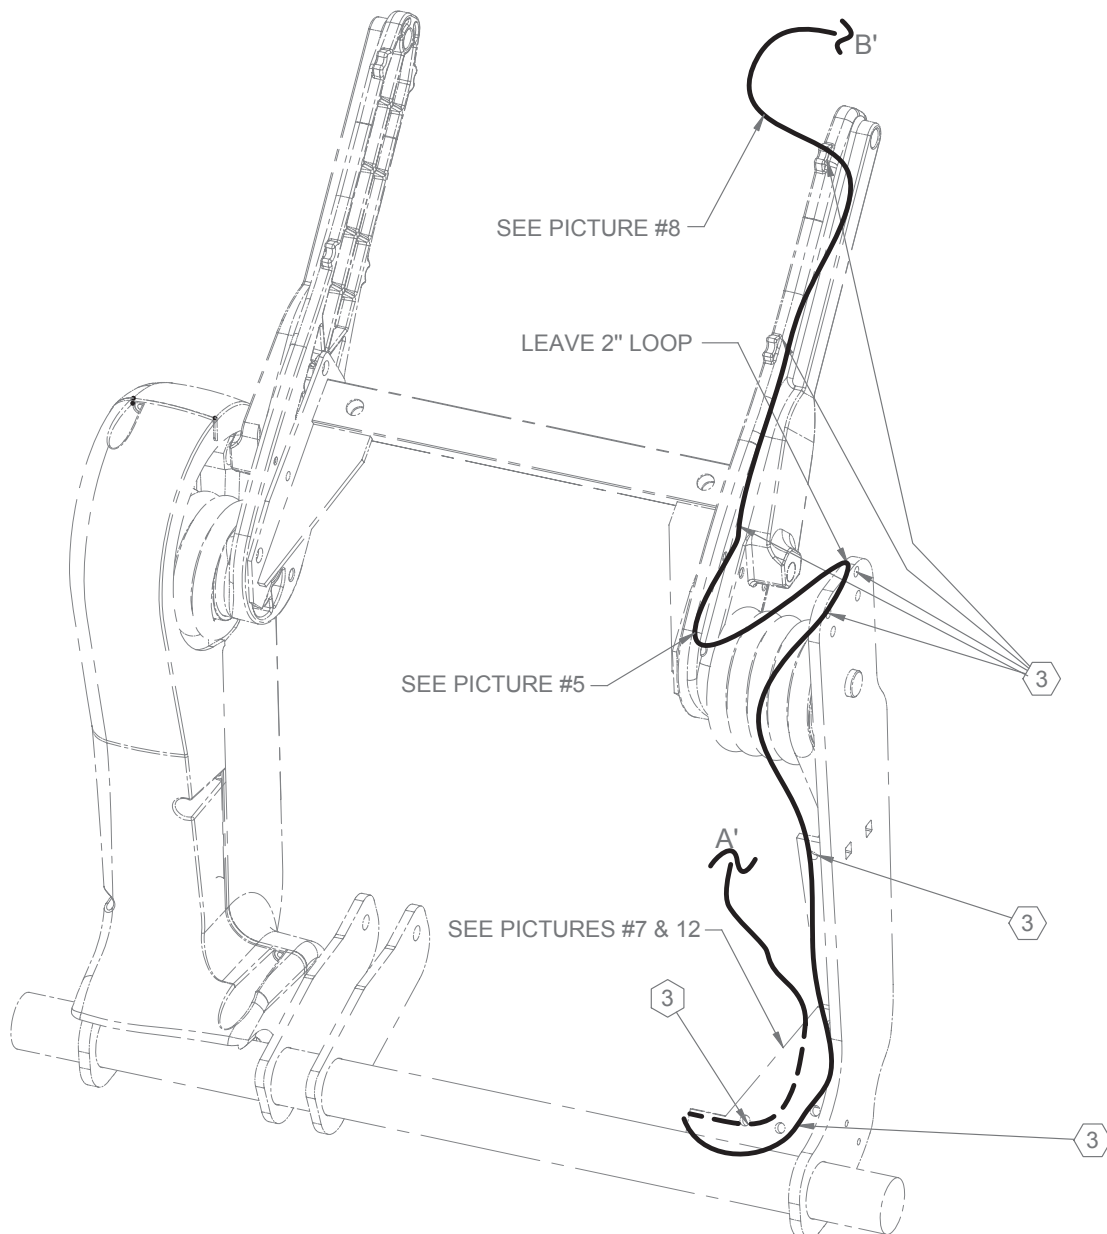

Base Assembly, Electrical

Be sure to place the connectors one beside the other and in a flat position.

PHOTO #1

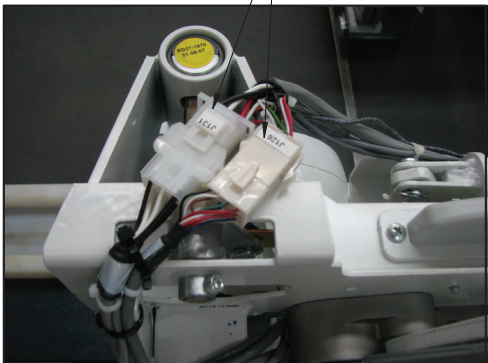


PHOTO #2



PHOTO #3



PHOTO #4

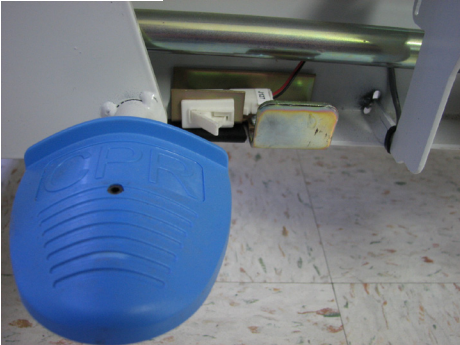


PHOTO #5



PHOTO #6



PHOTO #7



PHOTO #8



PHOTO #9



PHOTO #10



Base Assembly, Electrical

PHOTO #11



PHOTO #12



PHOTO #13



PHOTO #14



CABLE QDF27-2182 CONNECTION TABLE					
Cable No.	Connector No.	To	Cable No.	Connector No.	
QDF27-2182	J126	To	QDF27-1181	J126 Hi-lo Harness	
QDF27-2182	J131	To	QDF27-1181	J131 Hi-lo Harness	
QDF27-2182	J115	To	27-2477	Sensor Base	
QDF27-2182	J127	To	QDF2083	CPR Switch	
QDF27-2182	J116	To	QDF27-2024	Potentiometer	
QDF27-2182	J170A	To	QDF9159	No Manual Switch	
QDF27-2182	J170B	To	QDF9159	COM Manual Switch	
QDF27-2182	J146	To	QDF27-1252	Hi-lo Head Motor	
QDF27-2182	J147	To	QDF27-1251	Hi-lo Foot Motor	
QDF27-2182	J149	To	QDF27-1227	Brake Motor	

Base Assembly, Electrical

CABLE QDF27-2181 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2181	J126	To	QDF27-2182	J126 Hi-lo Harness
QDF27-2181	J131	To	QDF27-2182	J131 Hi-lo Harness
QDF27-2181	J115	To	27-2477	Sensor Base
QDF27-2181	J7	To	QDF75-0440	J7 DC Control Board
QDF27-2181	J6	To	QDF75-0440	J6 DC Control Board
QDF27-2181	J4	To	QDF75-0440	J4 DC Control Board
QDF27-2181	J30	To	QDF75-0440	J30 DC Control Board
QDF27-2181	J24	To	QDF75-0440	J24 DC Control Board


Base Assembly, Electrical 27-2709 Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF27-2181	Wires Harness #2	1
2	QDF27-2182	Base Frame Extender	1
3	QDF9518	Wire Tie	51
4	QDF9523	Wire Tie	2

Base Assembly, Zoom®

**(Applies to beds with Serial Numbers U03319 - Current)
(Including U03258 and U03259)**

OL270232-XXX Rev B (Reference Only)

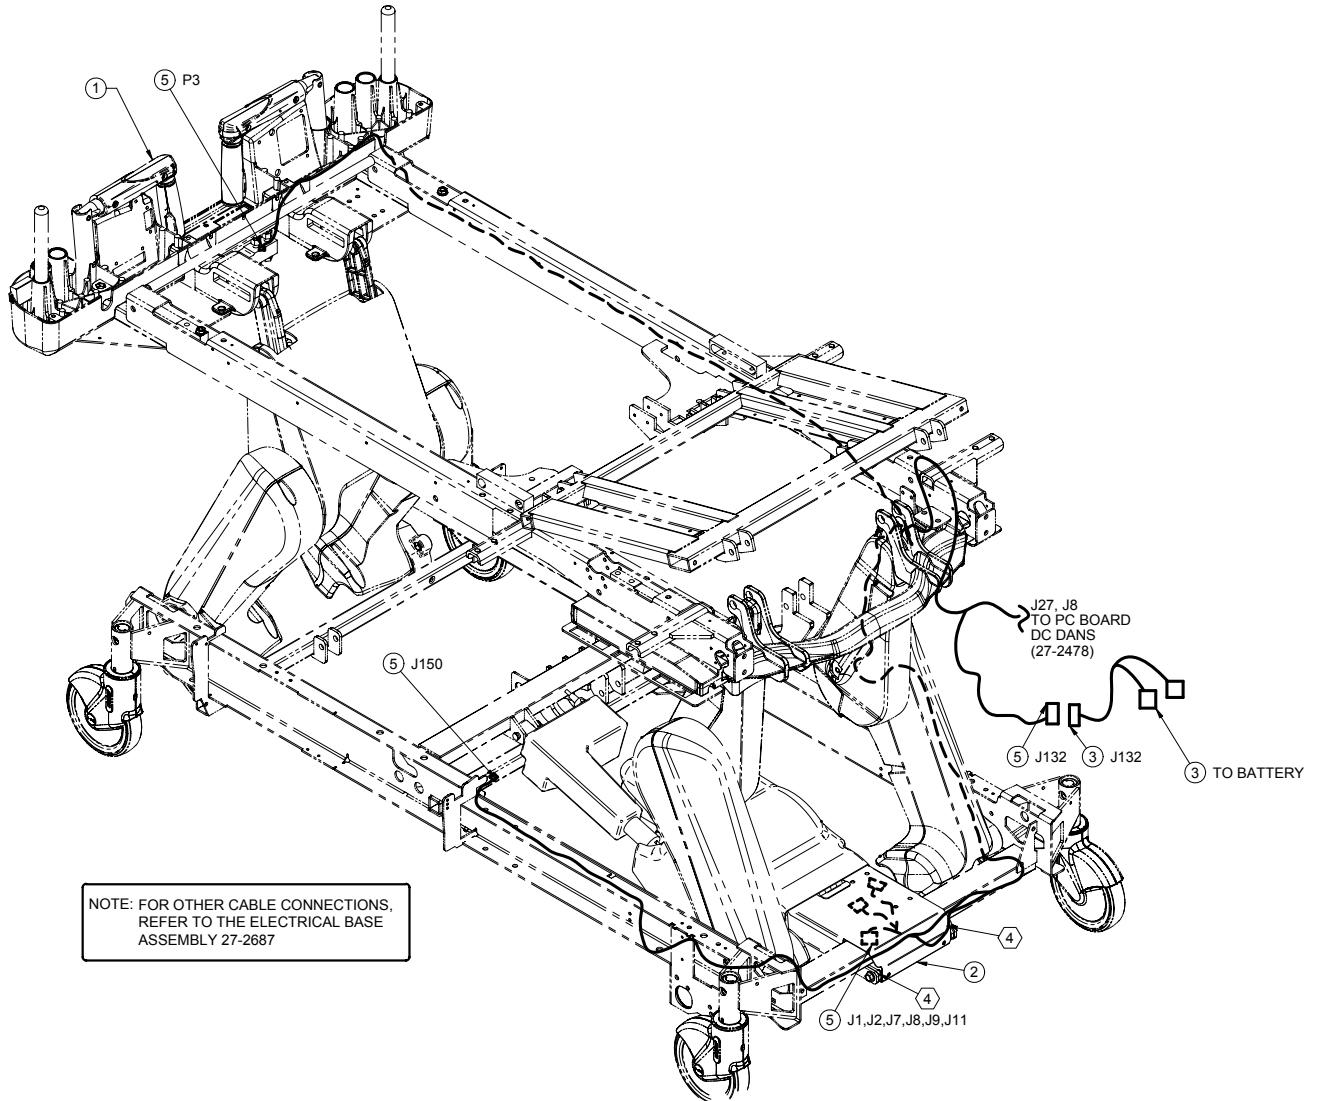

CABLE CONNECTION QDF27-1646 TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1646	Mini Fit	To	QDF27-1185	J132
QDF27-1646	Black Eyelets	To	QDF9188	BAT #2 POLE -
QDF27-1646	White Eyelets	To	QDF9188	BAT #1 POLE +

Base Assembly, Zoom®

**(Applies to beds with Serial Numbers U03319 - Current)
(Including U03258 and U03259)**

QDF27-1185 CONNECTIONS				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1185	J27	To	QDF21-1174	DC Card J27
QDF27-1185	J8	To	QDF21-1174	DC Card J8
QDF27-1185	J132	To	QDF27-1646	Mini Fit
QDF27-1185	P3	To	QDF27-1430	P3 (27-2547-XXX)
QDF27-1185	J150	To	QDF27-1445	Zoom (27-2546)
QDF27-1185	J1	To	QDF27-2548	J1 (27-2546)
QDF27-1185	J9	To	QDF27-2548	J9 (27-2546)
QDF27-1185	J2	To	QDF27-2548	J2 (27-2546)
QDF27-1185	J8	To	QDF27-2548	J8 (27-2546)
QDF27-1185	J7	To	QDF75-0240	J7
QDF27-1185	J11	To	QDF75-0240	J11

NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Base Assembly, Zoom® - OL270232-XXX Rev B (Reference Only)


Item	Part No.	Part Name	Qty.
1	27-2547-XXX	Zoom® Handle Assembly	1
2	27-2546	Zoom® Drive Base Assembly	1
3	QDF27-1646	Battery Wire	1
4	QDF9518	Cable Attachment	1
5	QDF27-1185	Wire Harness	1

Base Assembly, Zoom® Drive (Model 2141 Only)

(Applies to beds with Serial Numbers U01001 - U03318)

(Excluding U03258 and U03259)

27-1700 Rev-08 (Reference Only)

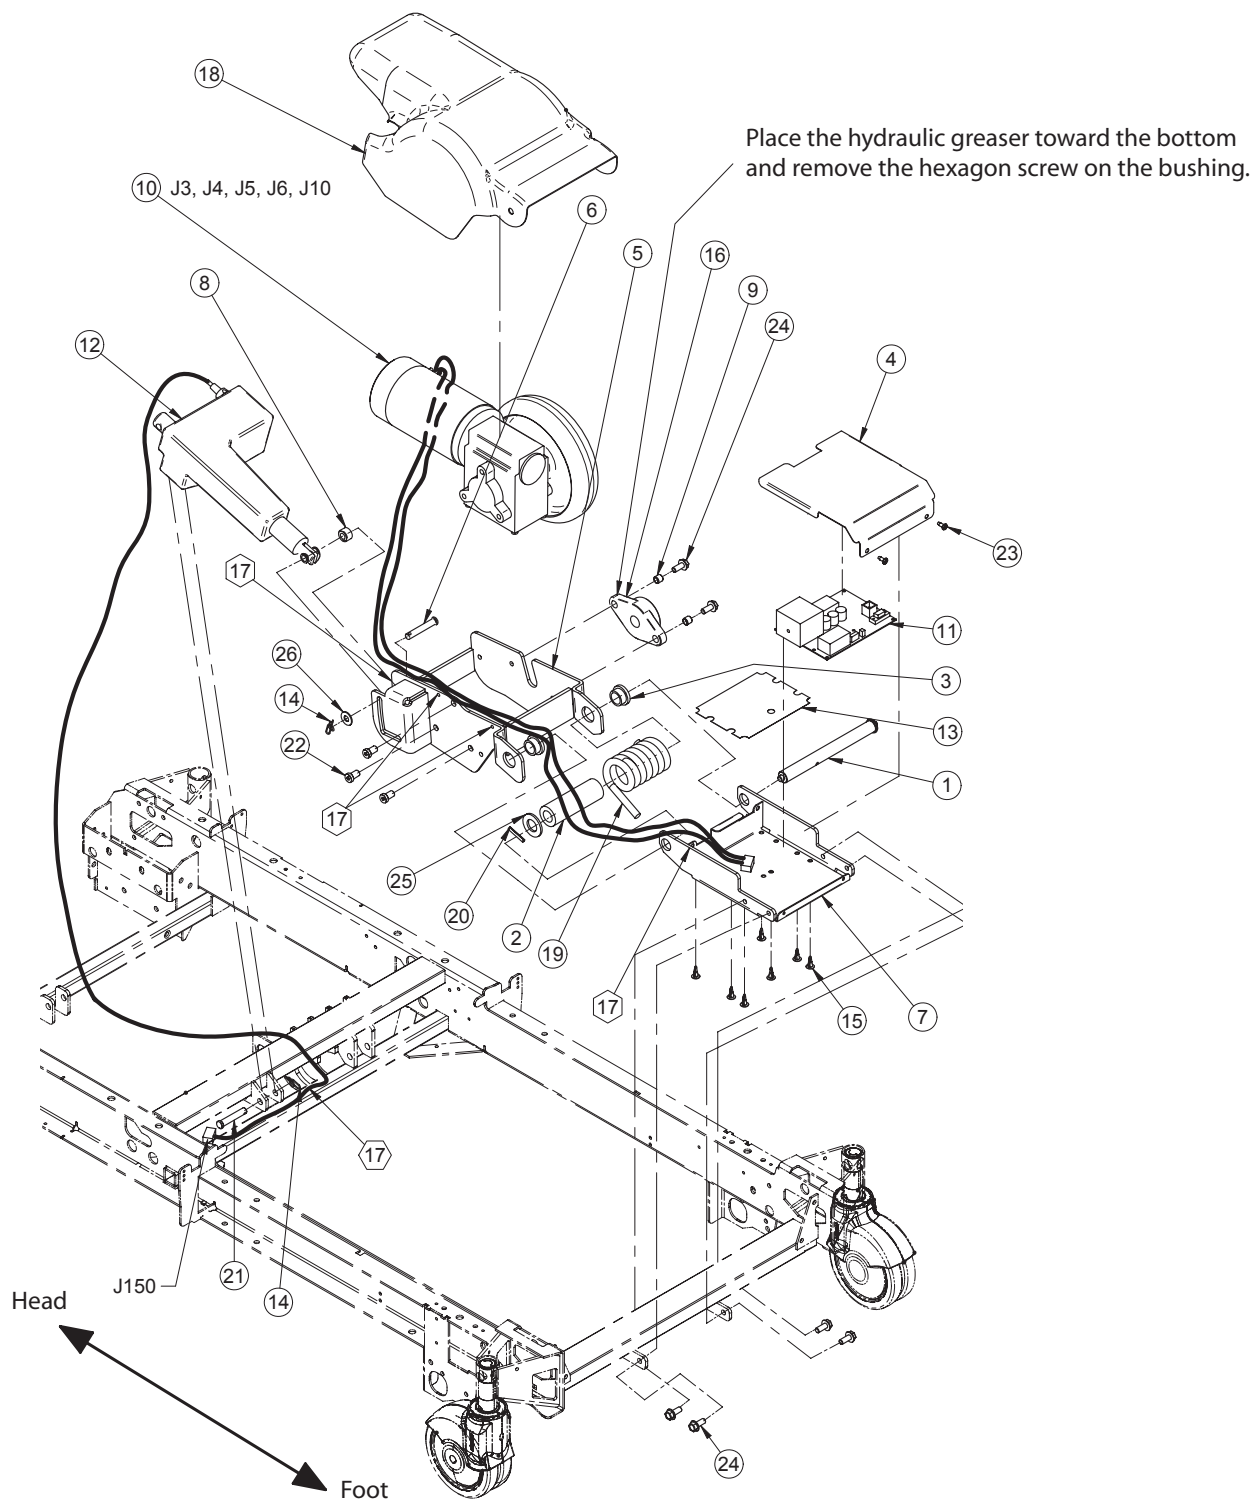

Base Assembly, Zoom® Drive (Model 2141 Only)

(Applies to beds with Serial Numbers U01001 - U03318)

(Excluding U03258 and U03259)


ACTUATOR CONNECTION QDF27-1445 TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1445	2-Positions Con.	To	QDF27-1184	J150 (OL270002)

MOTOR REDUCER CONNECTION 27-1683 TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1010	Red 2-Positions Con.	To	QDF27-1430	J3, J4
QDF27-1010	Black 2-Pos. Con.	To	QDF27-1430	J5, J6 (CSI 1109)
QDF27-1010	4-Positions MTA	To	QDF27-1430	J10 (CSI 1109)

Base Assembly, Zoom® Drive - 27-1700 Rev-08 (Reference only)

Item	Part No.	Part Name	Qty.
1	27-0804Z	Fifth Wheel Long Shaft	1
2	27-0898	Motorized Fifth Wheel Spring Pivot	1
3	27-0915	Fifth Wheel Thread Spacer	2
4	27-0961W	CSI1109 Box Cover	1
5	27-1059W	Motorized Wheel Structure	1
6	27-1138	Fifth Wheel Actuator Axis	1
7	27-1140W	Fifth Wheel Structure Box	1
8	27-1150	Fifth Wheel Actuator Spacer	1
9	27-1636	Motorized Fifth Wheel Sleeve	2
10	27-1683	Fifth Wheel	1
11	QDF27-1430	CSI1109 Zoom® Board	1
12	QDF27-1445	Fifth Wheel Actuator	1
13	QE71-1019	Fifth Wheel Board Protector	1
14	QDF7878	Clevis Pin 3/8" Diameter	2
15	QDF8011	Board Support	7
16	QDF9162	Fifth Wheel 3/4" Flange Bearing	1
17	QDF9518	Cable Tie	5
18	QP27-1916-10	Motorized Wheel Cover	1
19	QRT27-0796	Fifth Wheel Torsion Spring	1
20	VG10B0636	Spring Pin 3/16 x 1 1/4"	1
21	VG50B1248	Clevis Pin Diameter 3/8" x 2"	1
22	VV10A1P20-S	Cylindric Head Screw 3/8-16 UNC x 5/8" LG	3
23	VV83A9G16	Tapping Screw Type B Pan Head Phillips #10 x 1/2"	2
24	VVB4A1024	Bolt 5/16-18 x 3/4" Thread Rolling	6
25	VW10B264004	Steel Washer 13/16 x 1 1/2" x 1/8	1
26	VW10C122802	Nylon Washer 3/8" ins. X 7/8" out. X 1/16" wi.	1

27-2546 Rev-02 (Reference Only)

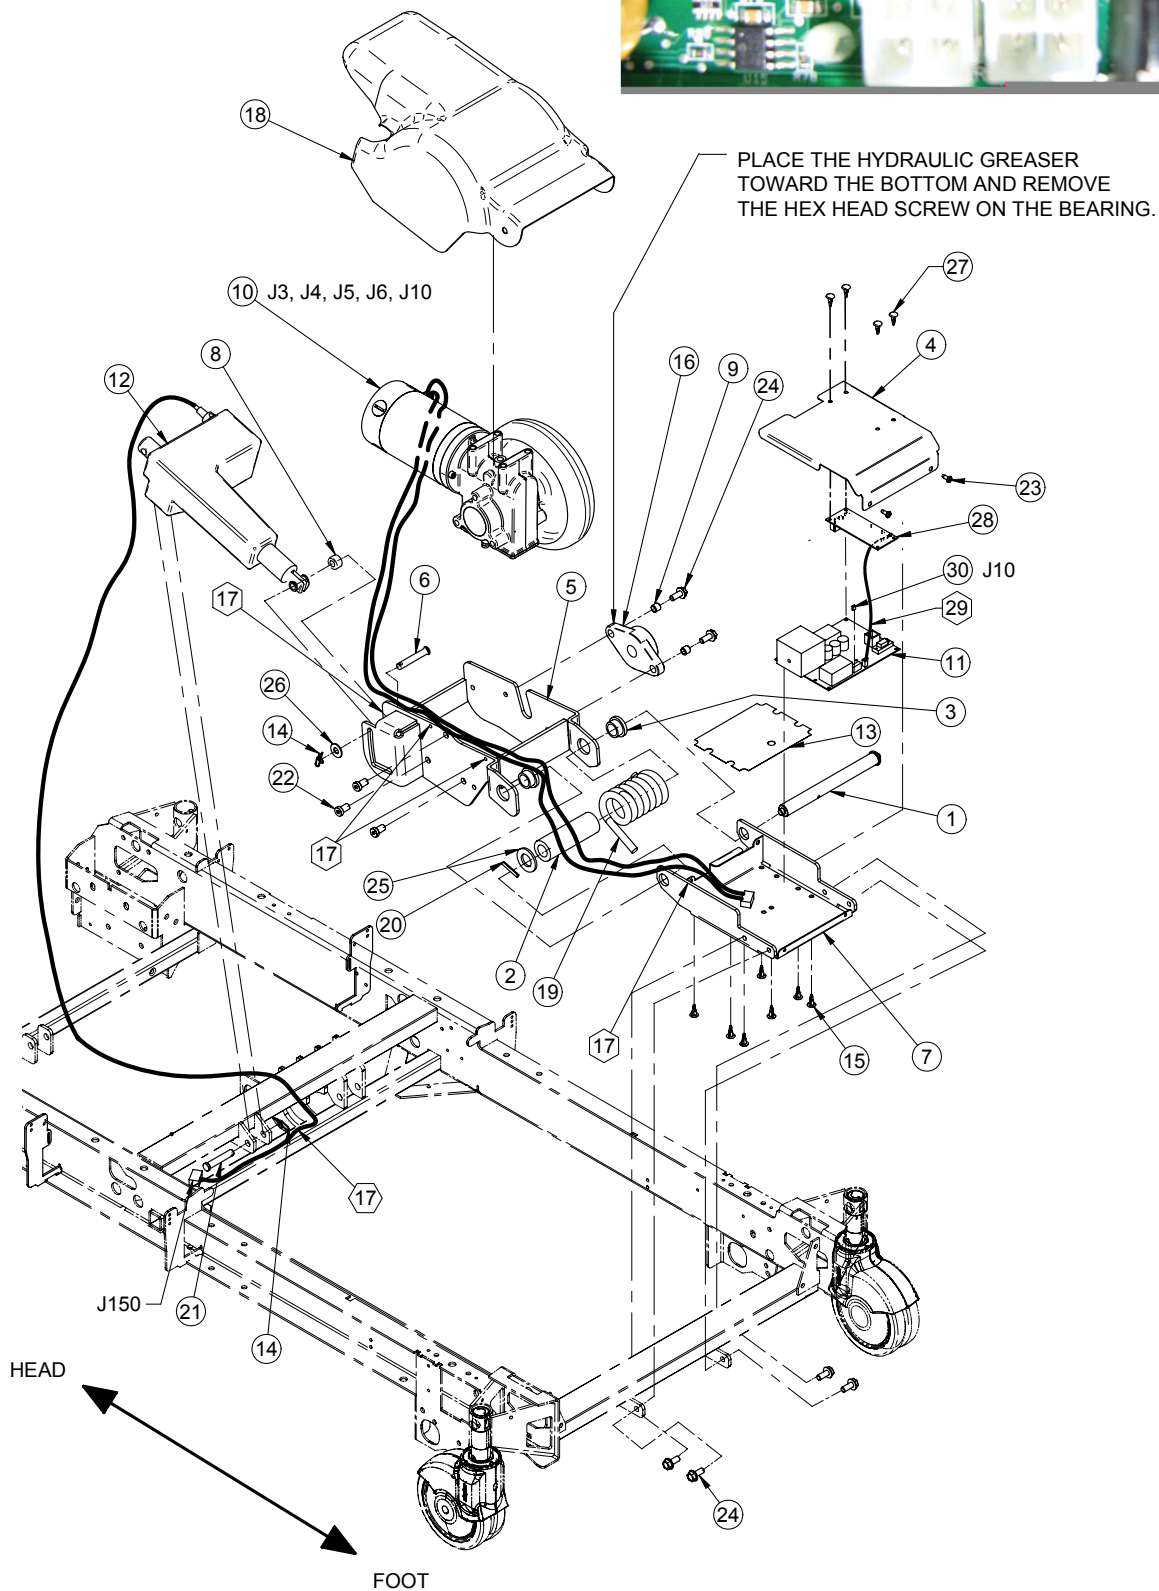

Base Assembly, Zoom® Drive (Model 2141 Only)

ACTUATOR CONNECTION QDF27-1445 TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1445	2-Positions Con.	To	QDF27-1185	J150 (OL270002)

MOTOR REDUCER CONNECTION 27-2593 TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2523	Red 2-Positions Con.	To	QDF27-1430	J3, J4
QDF27-2523	Black 2-Pos. Con.	To	QDF27-1430	J5, J6 (CSI 1109)
QDF27-2523	4-Positions MTA	To	QDF27-1430	J10 (CSI 1109)

CABLE CONNECTIONS 27-2542 TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2542	J7, 18-Position Mini Fit	To	QDF27-1430	J7 (CSI 1109)
QDF27-2542	J11, 2-Positions MTA	To	QDF27-1430	J11 (CSI 1109)
QDF27-2542	J7A, 9-Positions MTA	To	QDF75-0240	J7A, 9-Positions MTA
QDF27-2542	J11A, 3-Positions MTA	To	QDF75-0240	J11A, 3-Positions MTA


Base Assembly, Zoom® Drive (2141 Model Only) - 27-2546 Rev-02 (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-0804Z	Fifth Wheel Long Shaft	1
2	QP27-2556	Motorized Fifth Wheel Spring Pivot	1
3	27-0915	Fifth Wheel Thread Spacer	2
4	27-2545P	CSI1109 Box Cover	1
5	27-1059P	Motorized Wheel Structure	1
6	27-1138	Fifth Wheel Actuator Axis	1
7	27-1140P	Fifth Wheel Structure Box	1
8	27-1150	Fifth Wheel Actuator Spacer	1
9	27-1636	Motorized Fifth Wheel Sleeve	2
10	27-2593	Fifth Wheel	1
11	QDF27-1430	CSI1109 Zoom® Board	1
12	QDF27-1445	Fifth Wheel Actuator	1
13	QE71-1019	Fifth Wheel Board Protector	1
14	QDF7878	Clevis Pin	2
15	QDF8011	Board Support	7
16	QDF9162	Fifth Wheel Flange Bearing	1
17	QDF9518	Cable Tie	5
18	QP27-1916	Motorized Wheel Cover	1
19	QRT27-0796	Fifth Wheel Torsion Spring	1
20	VG10B0636	Spring Pin	1
21	VG50B1248	Clevis Pin Diameter	1
22	VV10A1P20-S	Cylindric Head Screw	3
23	VV83A9G16	Pan Head Tapping Screw	2
24	VVB4A1024	Thread Rolling Bolt	6
25	VW10B264004	Steel Washer	1
26	VW10C122802	Nylon Washer	1
27	QDF2134	Board Support	4
28	QDF75-0240	Zoom® Interface Board	1
29	QDF27-2542	Zoom® Interface Board Harness	1
30	QDF8047	Jumper	1


Bed Labeling

OL270016-XXX Rev P (Reference Only)





RIGHT SIDE OF THE BED

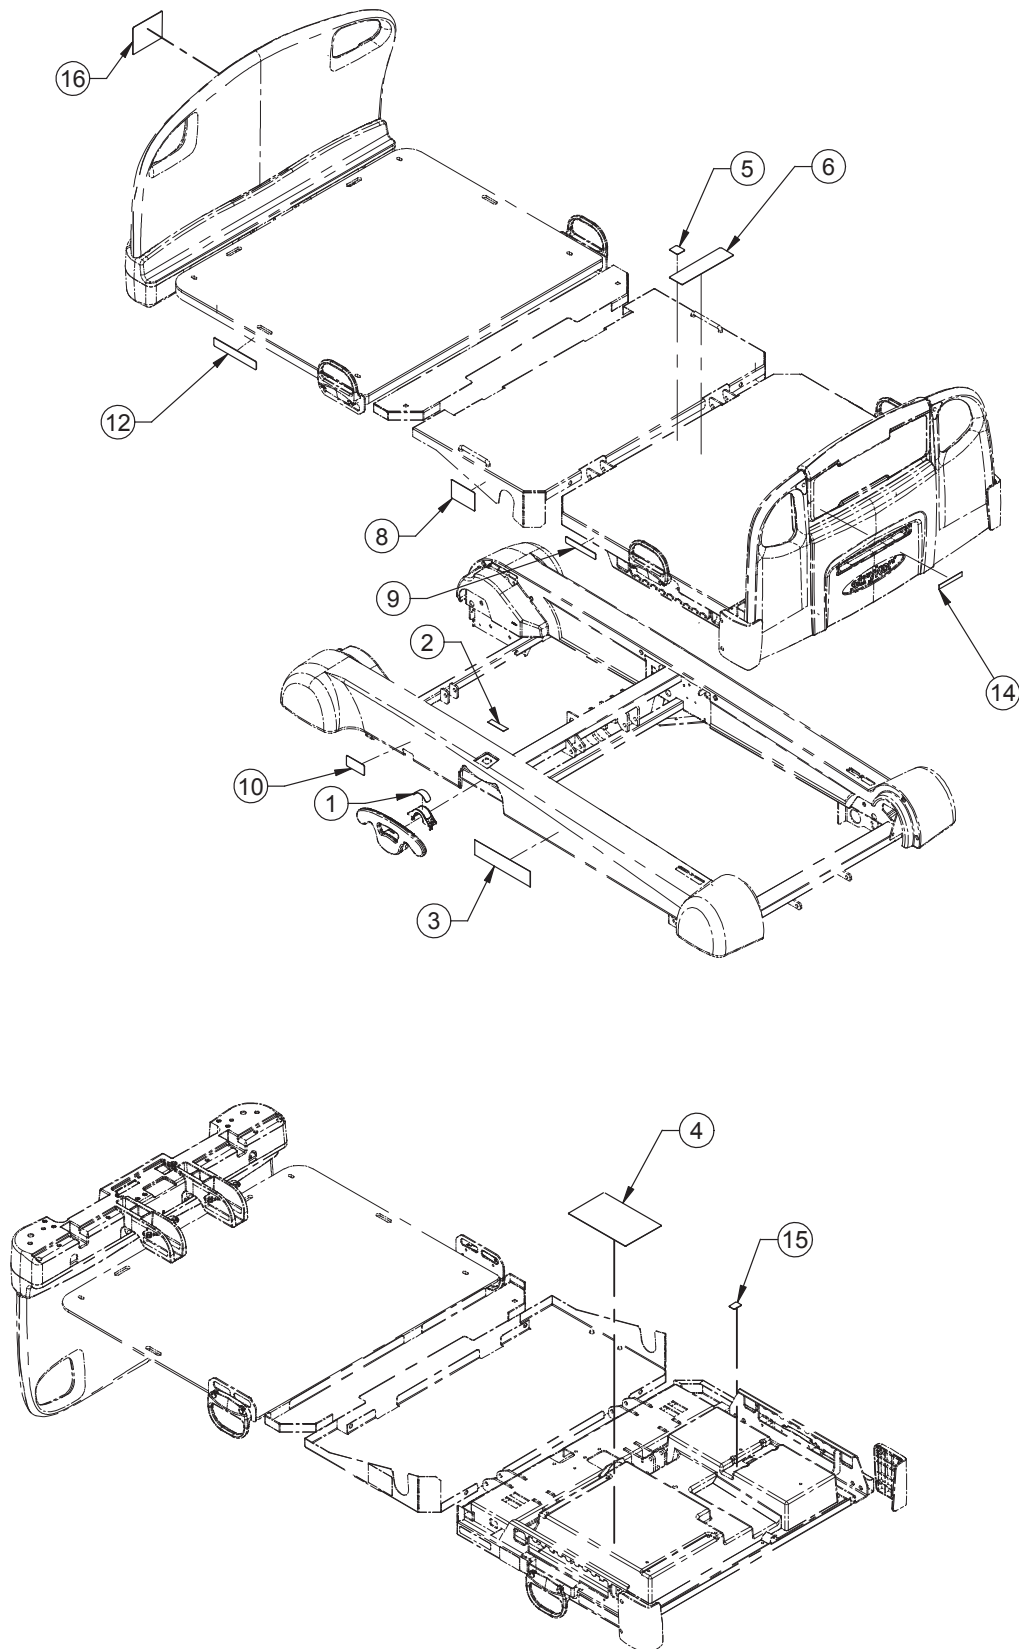

Bed Labeling



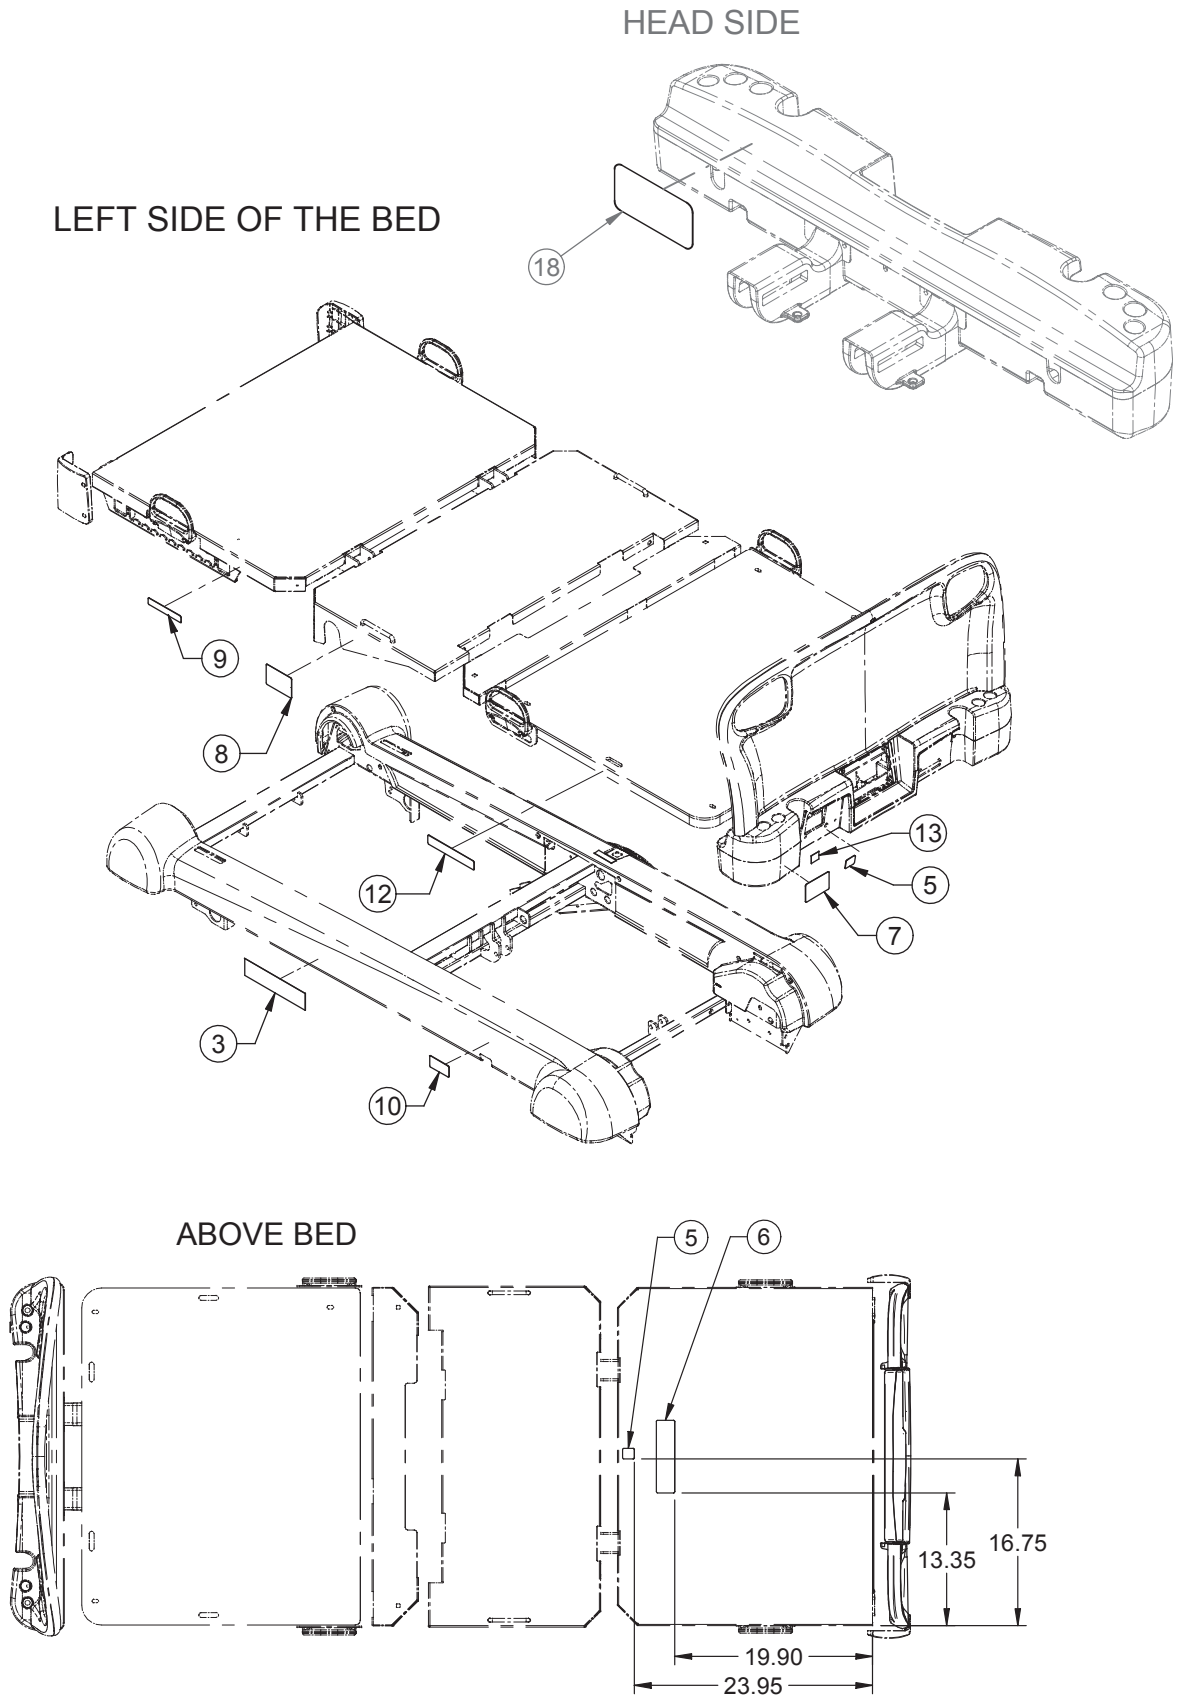


Bed Labeling

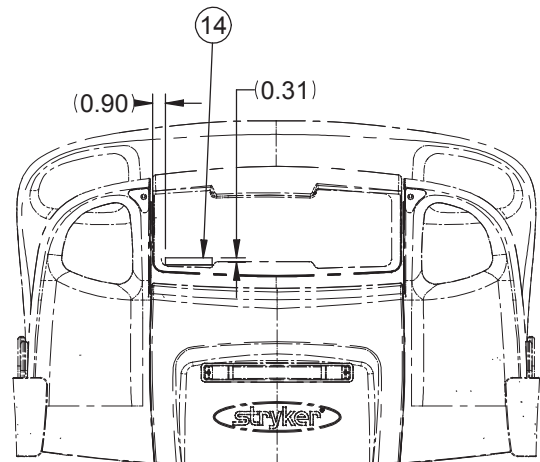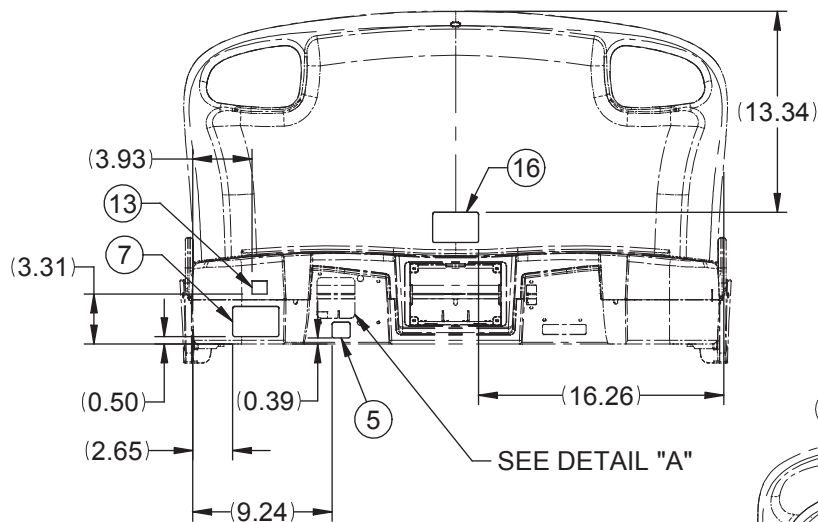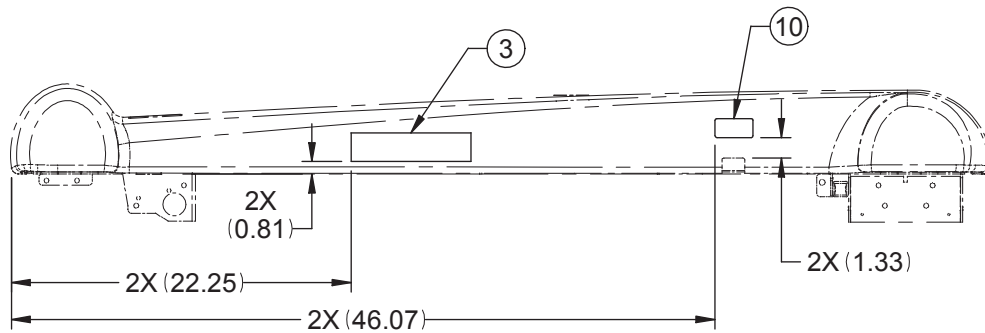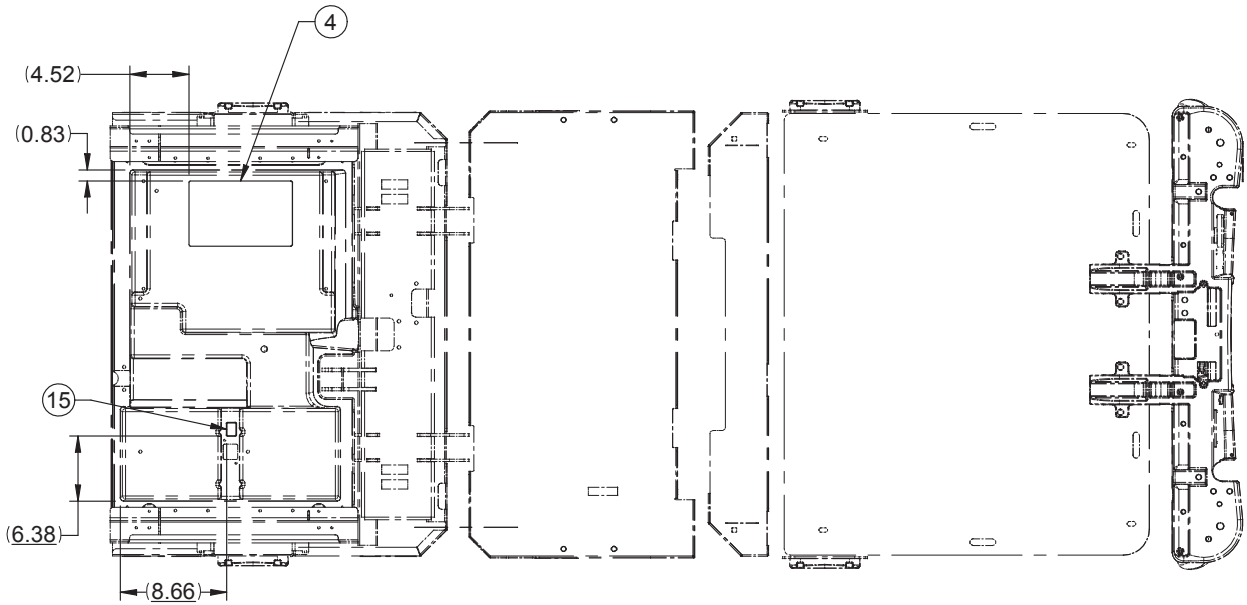

[Return To Table of Contents](#)

Bed Labeling

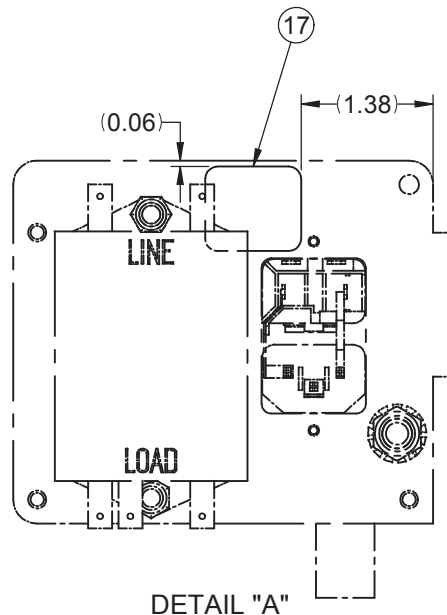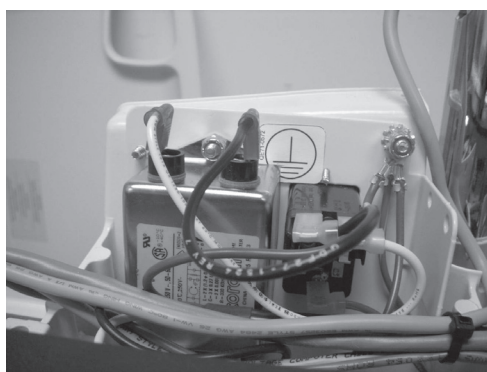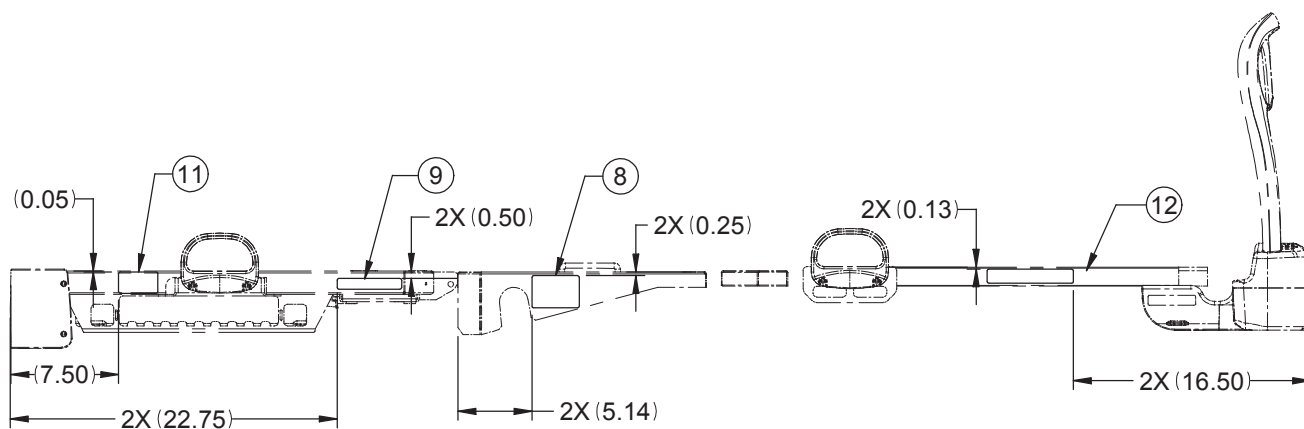

VIEW FROM INSIDE

NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)


Base Labeling - OL270016-XXX Rev P (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF27-1256-XXX	Brake Pedal Label	1
2	QE71-0947-XXX	Manual Backup Label	1
3	QE71-1046	Stryker Label	2
4	QE14400	Result of Isolation Room Label	1
5	QE18545	Reference Customer Manual Label	2
6	QE71-1207-XXX	Electric Shock Hazard Label	1
7	QE71-0943-XXX	Grounding Reliability Label	1
8	QE71-0944-XXX	Oxygen Tent Label	2
9	QE71-0949-XXX	Maximum Mattress Thickness Label	2
10	QE71-0963-XXX	CPR Label	2
12	QE71-1010	550 lbs Safe Working Load label	2
13	QE71-0571	Fuse 10A 250V Label	1
14	QE71-1094-XXX	Patent Pending Label	1
15	QE71-1042-XXX	On-Off Label	1
16	QE71-1257-XXX	Orientation Label	1
17	QE71-0572	Ground Label	1
18	QE71-1368	CSA Label	1

Lift Assembly

(Applies to beds with Serial Numbers U01001 - U02817)

L27-027 Rev-11 (Reference Only)

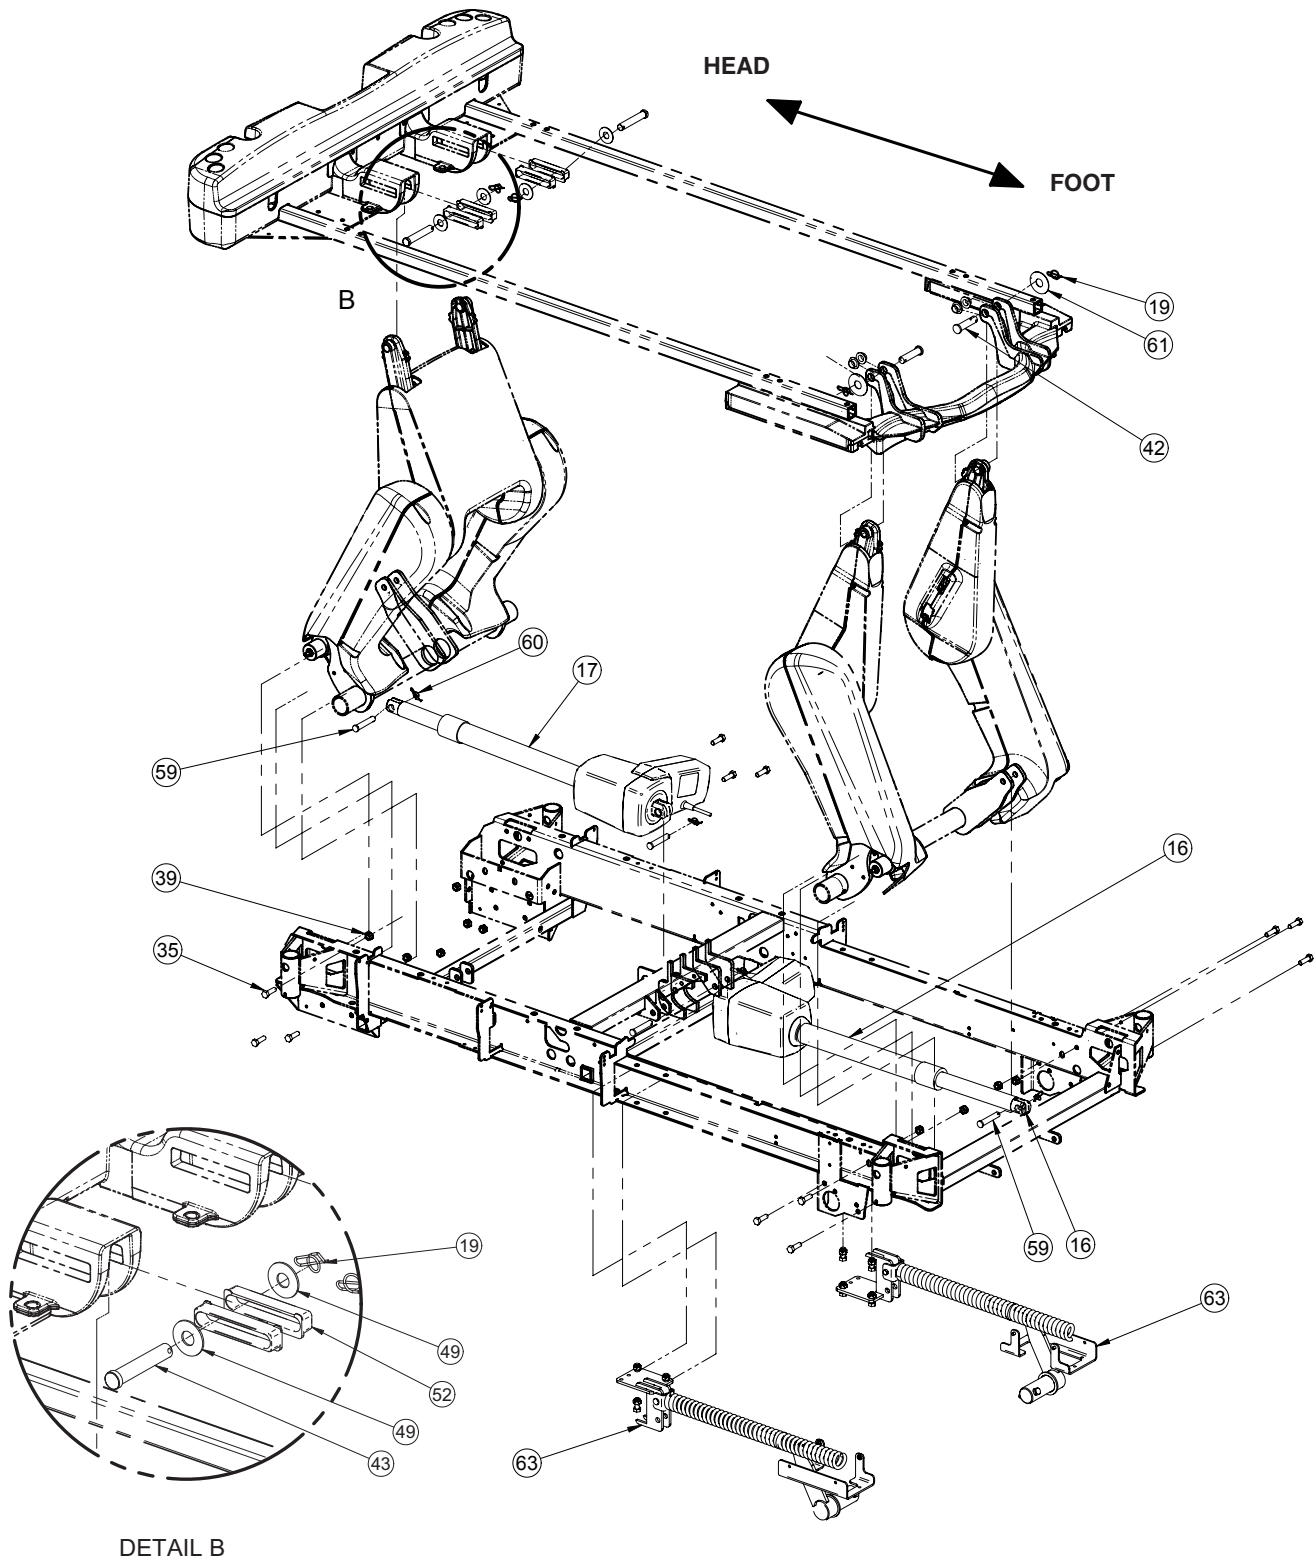


Lift Assembly

(Applies to beds with Serial Numbers U01001 - U02817)

Head End


Assemble this part
with the arrow pointing
toward the head of the
bed.

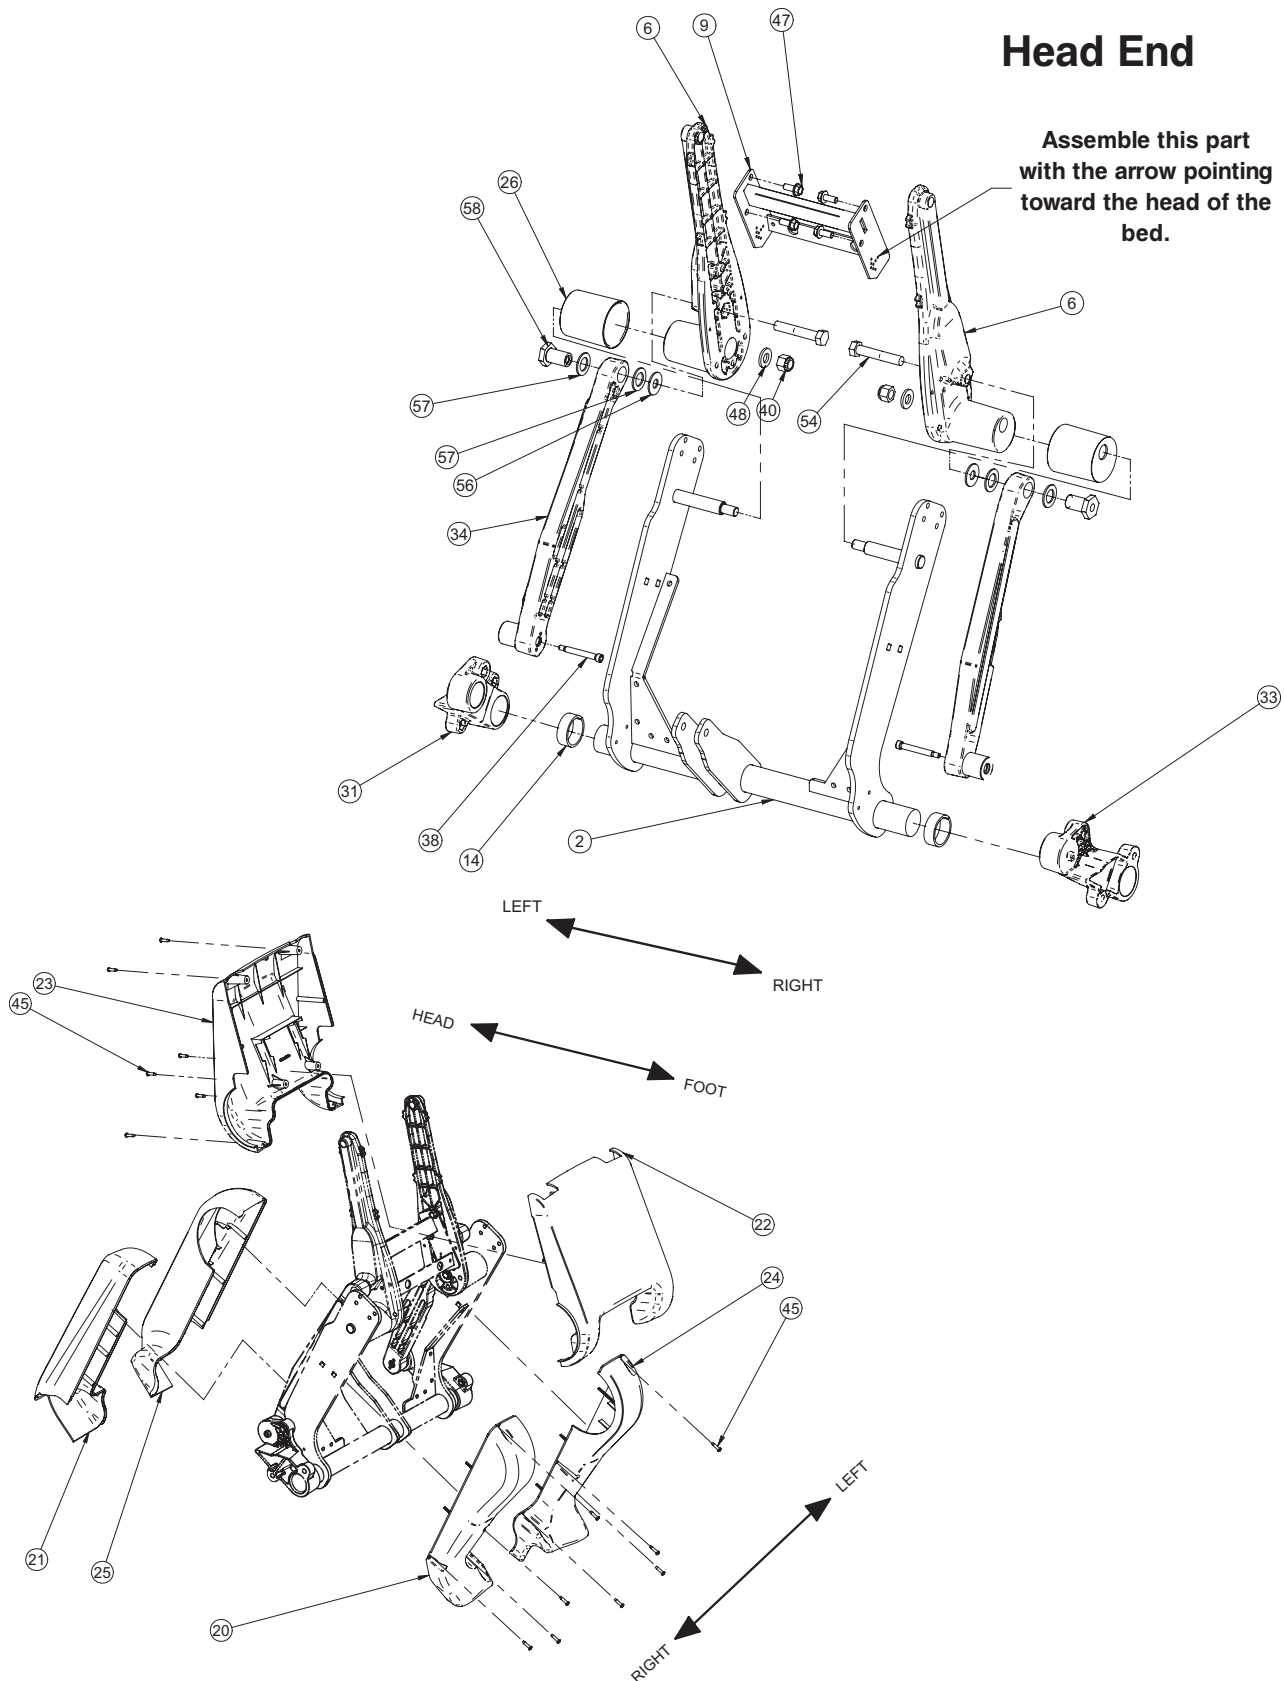

Lift Assembly

(Applies to beds with Serial Numbers U01001 - U02817)

Foot End

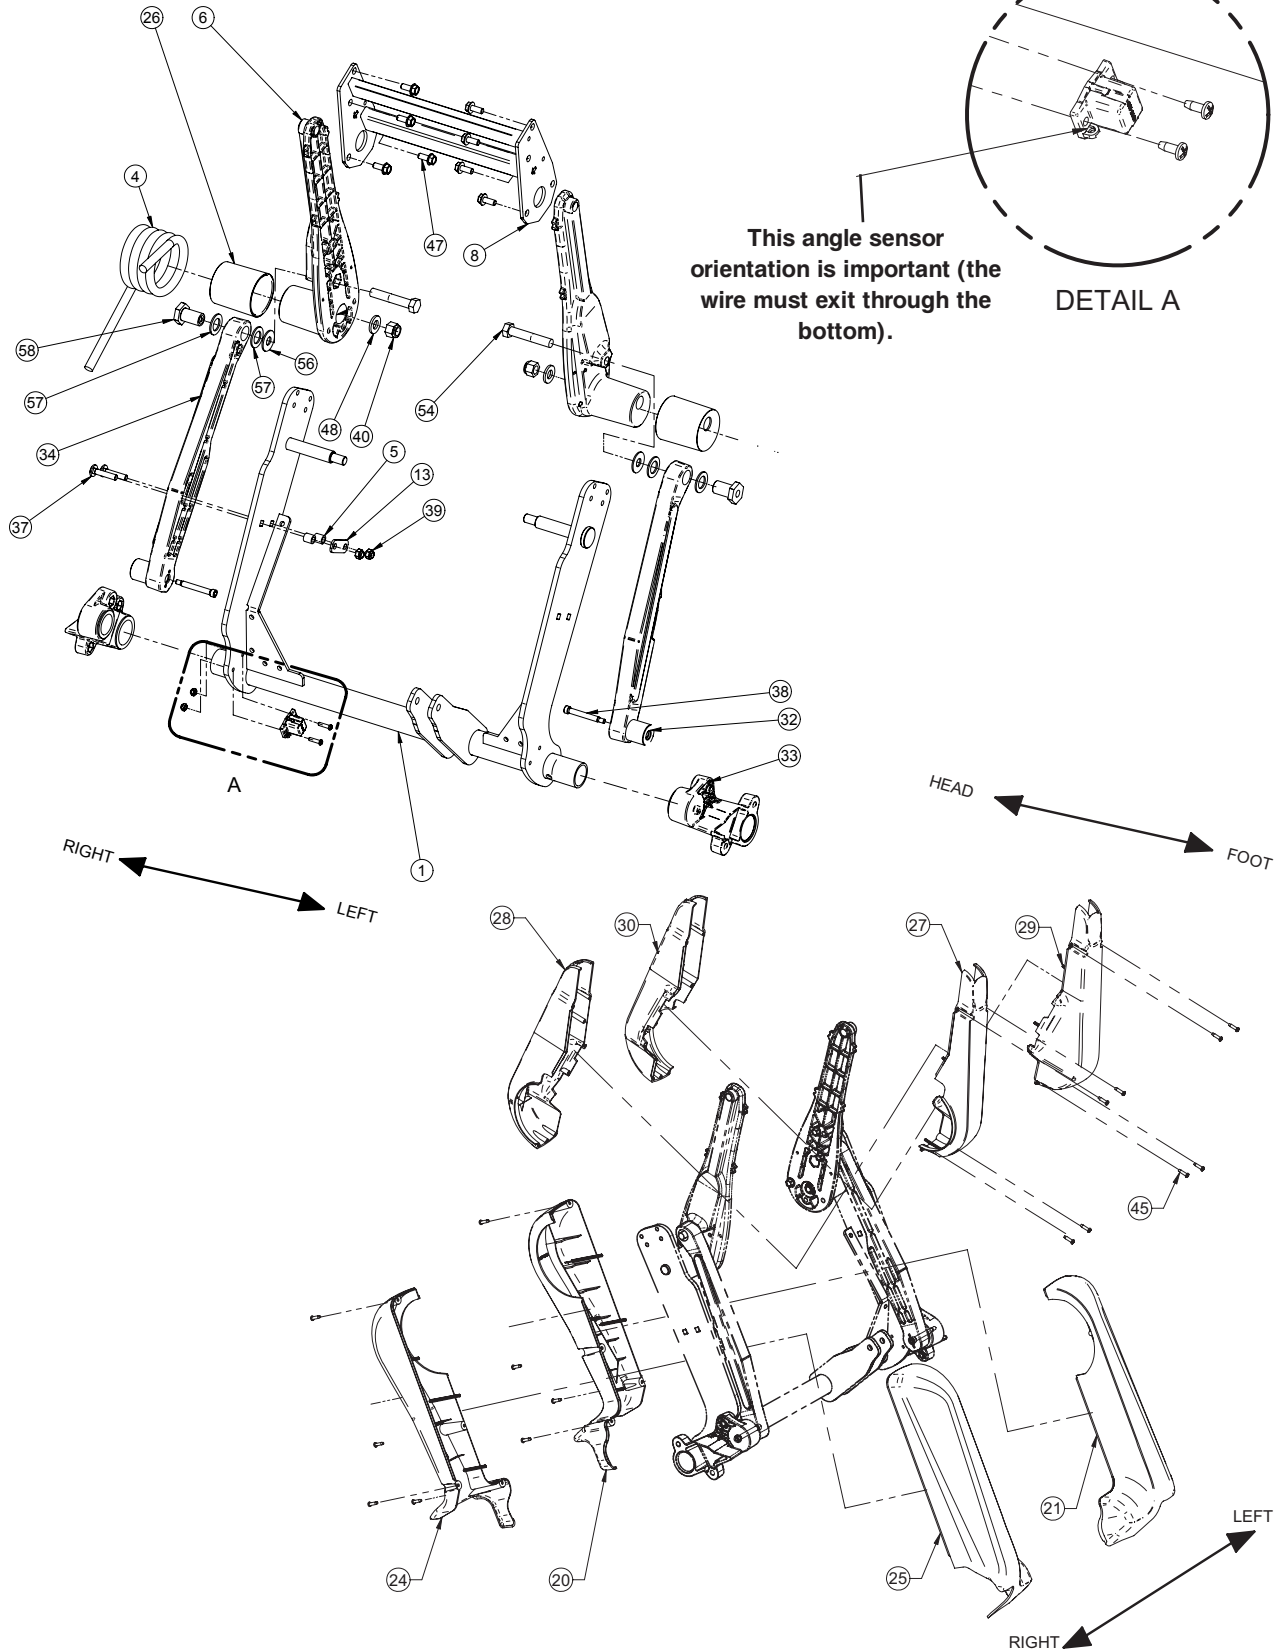

Lift Assembly

(Applies to beds with Serial Numbers U01001 - U02817)


Lift Assembly - L27-027 Rev-11 (Reference only)

Item	Part No.	Part Name	Qty.
1	27-0992W	Foot Main Lift	1
2	27-0993W	Head Main Lift	1
3	QRT27-1002	Bed Lift System Left Spring	1
4	QRT27-1011	Bed Lift System Right Spring	1
5	27-1012	Spring Stop	4
6	QPA27-1013	Molded Bed Lift System Arm	4
8	27-1977W	Foot Reinforcement	1
9	27-1089W	Head Transverse Reinforcement	1
12	27-1209	Angle Sensor	1
13	27-1243Z	Spring Retention Plate	2
14	27-1623	Lift Spacer	4
16	QDF27-1251	Foot Lift Actuator	1
17	QDF27-1252	Head Lift Actuator	1
19	QDF7899	Hitch Pin Diameter 1/2"	4
20	QP27-0982-10	Exterior Right Low Lift Cover	2
21	QP27-0983-10	Interior Right Low Lift Cover	2
22	QP27-098-10	Interior Head High Lift Cover	1
23	QP27-0985-10	Exterior Head High Lift Cover	1
24	QP27-0986-10	Exterior Left Low Lift Cover	2
25	QP27-0987-10	Interior Left Low Lift Cover	2
26	QP27-1065	Spring Sleeve	4
27	QP27-1236-10	Exterior Right Foot High Lift Cover	1
28	QP27-1237-10	Interior Right Foot High Lift Cover	1
29	QP27-1238-10	Exterior Left Foot High Lift Cover	1
30	QP27-1239-10	Interior Left Foot High Lift Cover	1
31	QPA27-1024	Right Lever Support	2
32	QPA27-1030	Right Stiffener Arm	2
33	QPA27-1036	Left Lever Support	2
34	QPA27-1040	Left Stiffener Arm	2
35	VB18A1O32	Bolt	12
37	VB35A1O40	Carriage Bolt	4
38	VD60B1O48	Shoulder Screw	4
39	VE30A1O	Nylon Locknut	16
40	VE30A1R	Nylon Locknut Diameter 1/2-13	4
42	VG50A1648	Clevis Pin Diameter	2
43	VG50A1654	Clevis Pin Diameter	2
45	VV23A1G24HL	Pan Head Tapping Screw	32
46	VV83A9G16	Pan Head Tapping Screw	2
47	VVB4A1024	Bolt 5/16-18 x 3/4 Thread Rolling	12
48	VW10A173308	Flat Washer AA 1/2" P.Z.	4
49	VW10C173602	Nylon Washer	4
52	QP27-1830-00	Glider	4
54	VB18A1R54-S	Hexagon Bolt 1/2-13 UNC x 2 3/4"	4
56	27-2022Z	Stiffener Arm Steel Washer	4
57	27-2019	Stiffener Arm Acetal Washer	8
58	QDF27-2018Z	Stiffener Arm Bearing	4
59	QDF27-2053Z	Clevis Pin Diameter 10 mm x 50 mm	4
60	QDF7878	Hitch Pin Diameter 3/8"	4
61	VW10C432002	Nylon Washer	2
62	VE30A0G	Nylon Locknut #10-32	2
63	27-2117	Spring in Base	1
64	QDF2100	Round	4

Lift Assembly

(Applies to beds with Serial Numbers U02818 - Current)


L27-044 Rev-C (Reference Only)

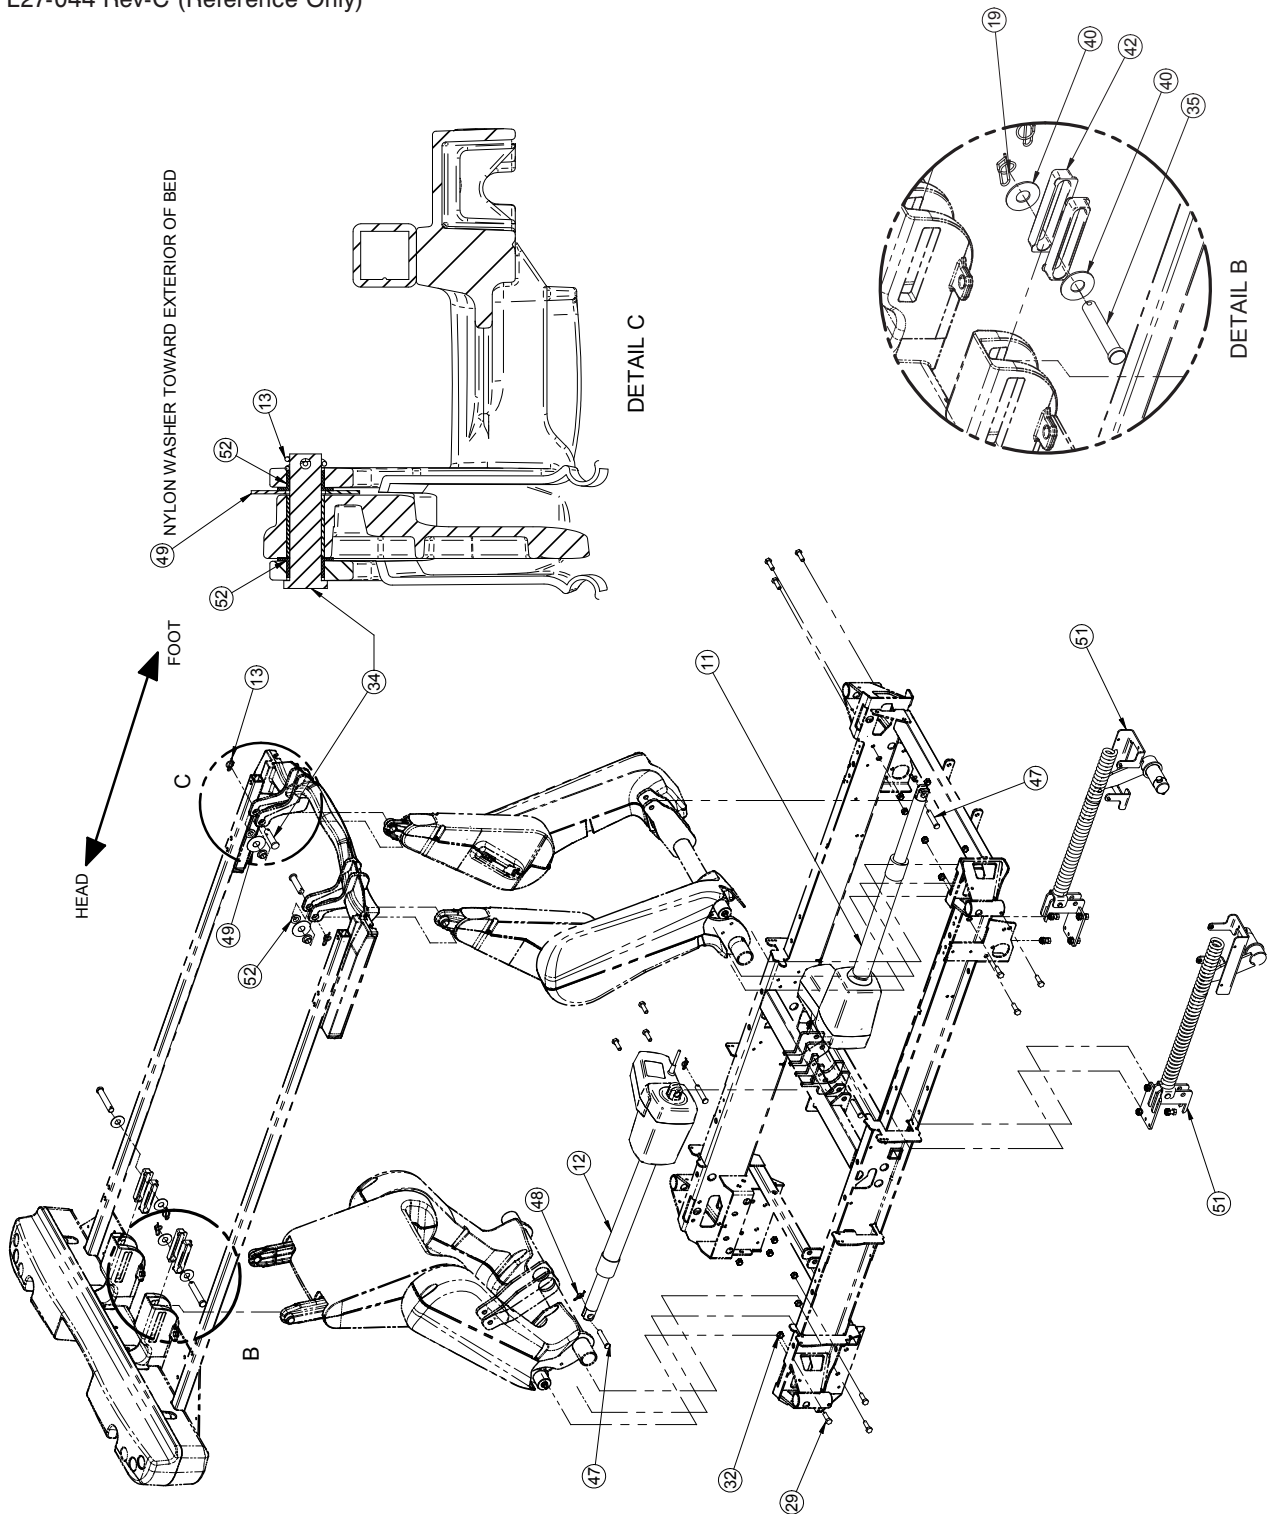

Lift Assembly

(Applies to beds with Serial Numbers U02818 - Current)


Head End

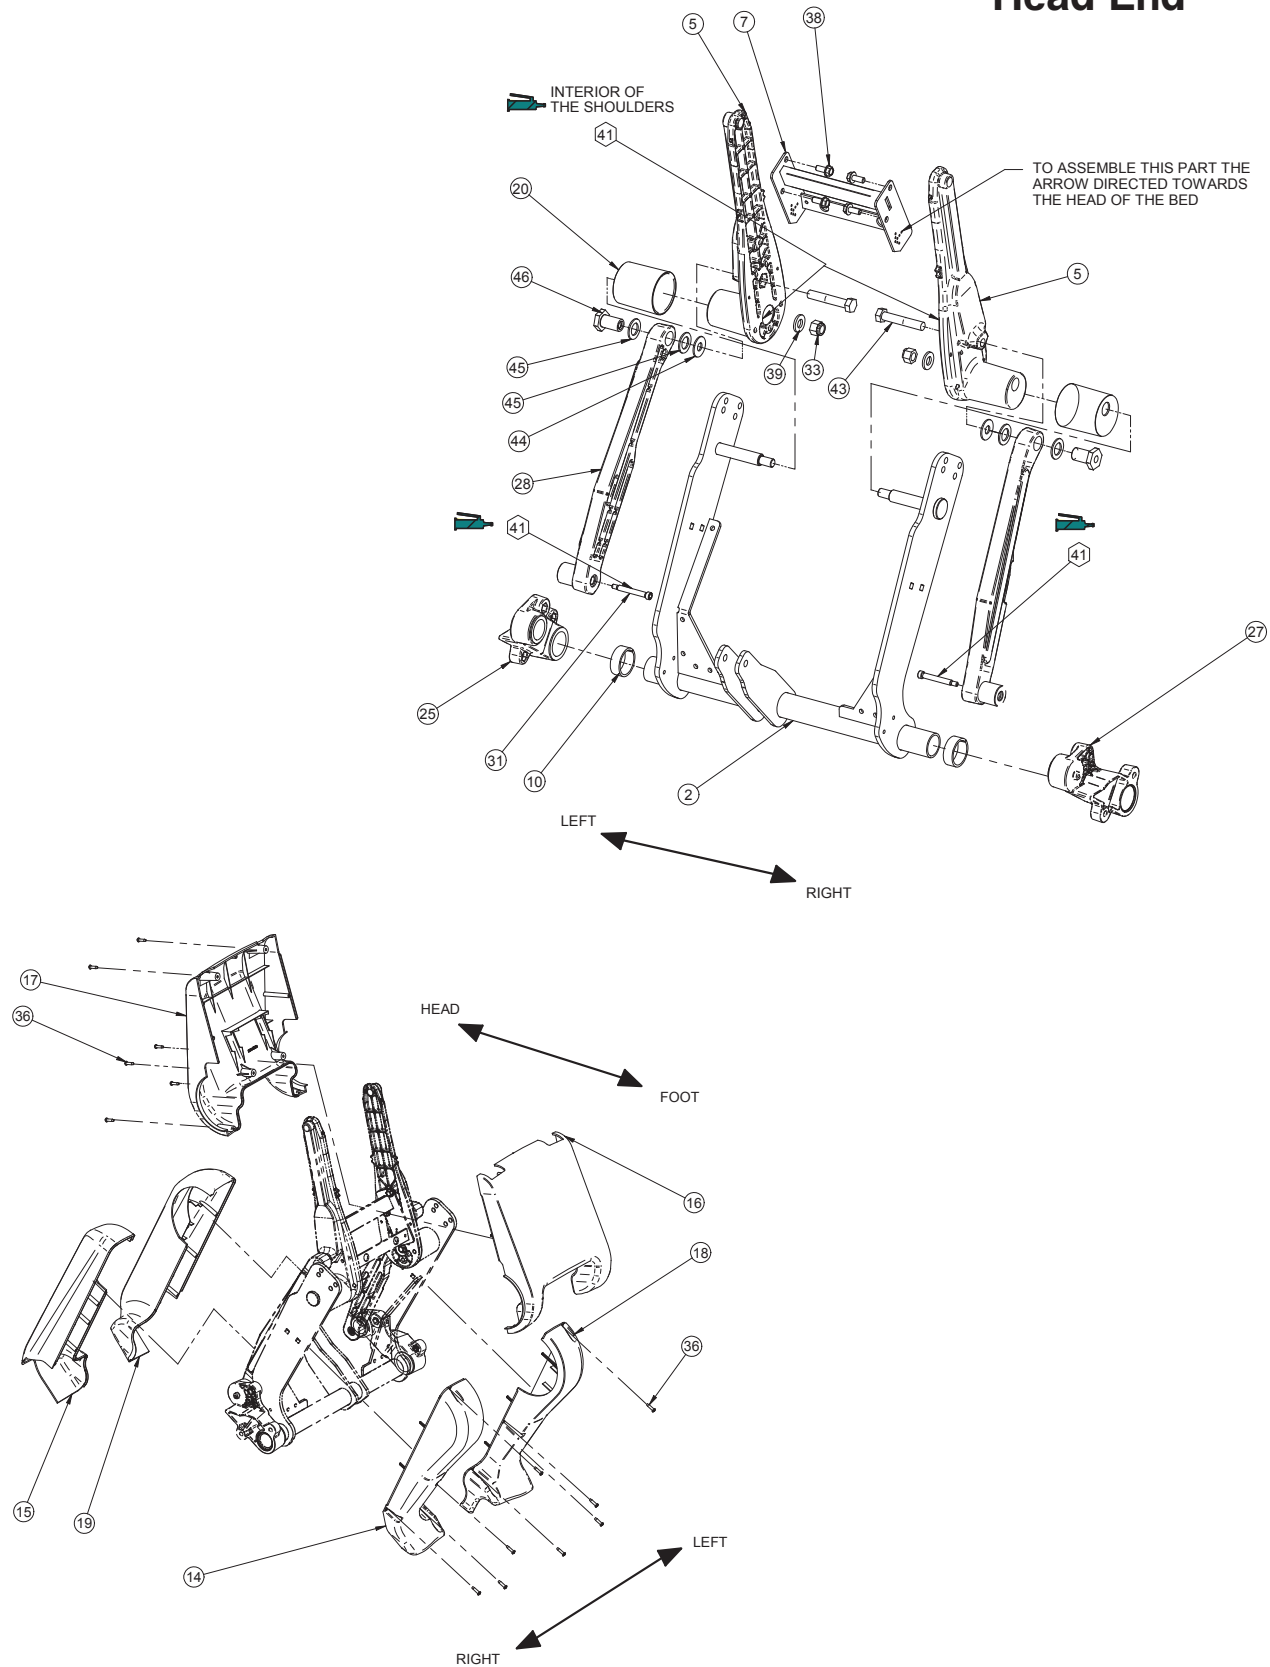

Lift Assembly

(Applies to beds with Serial Numbers U02818 - Current)

Foot End

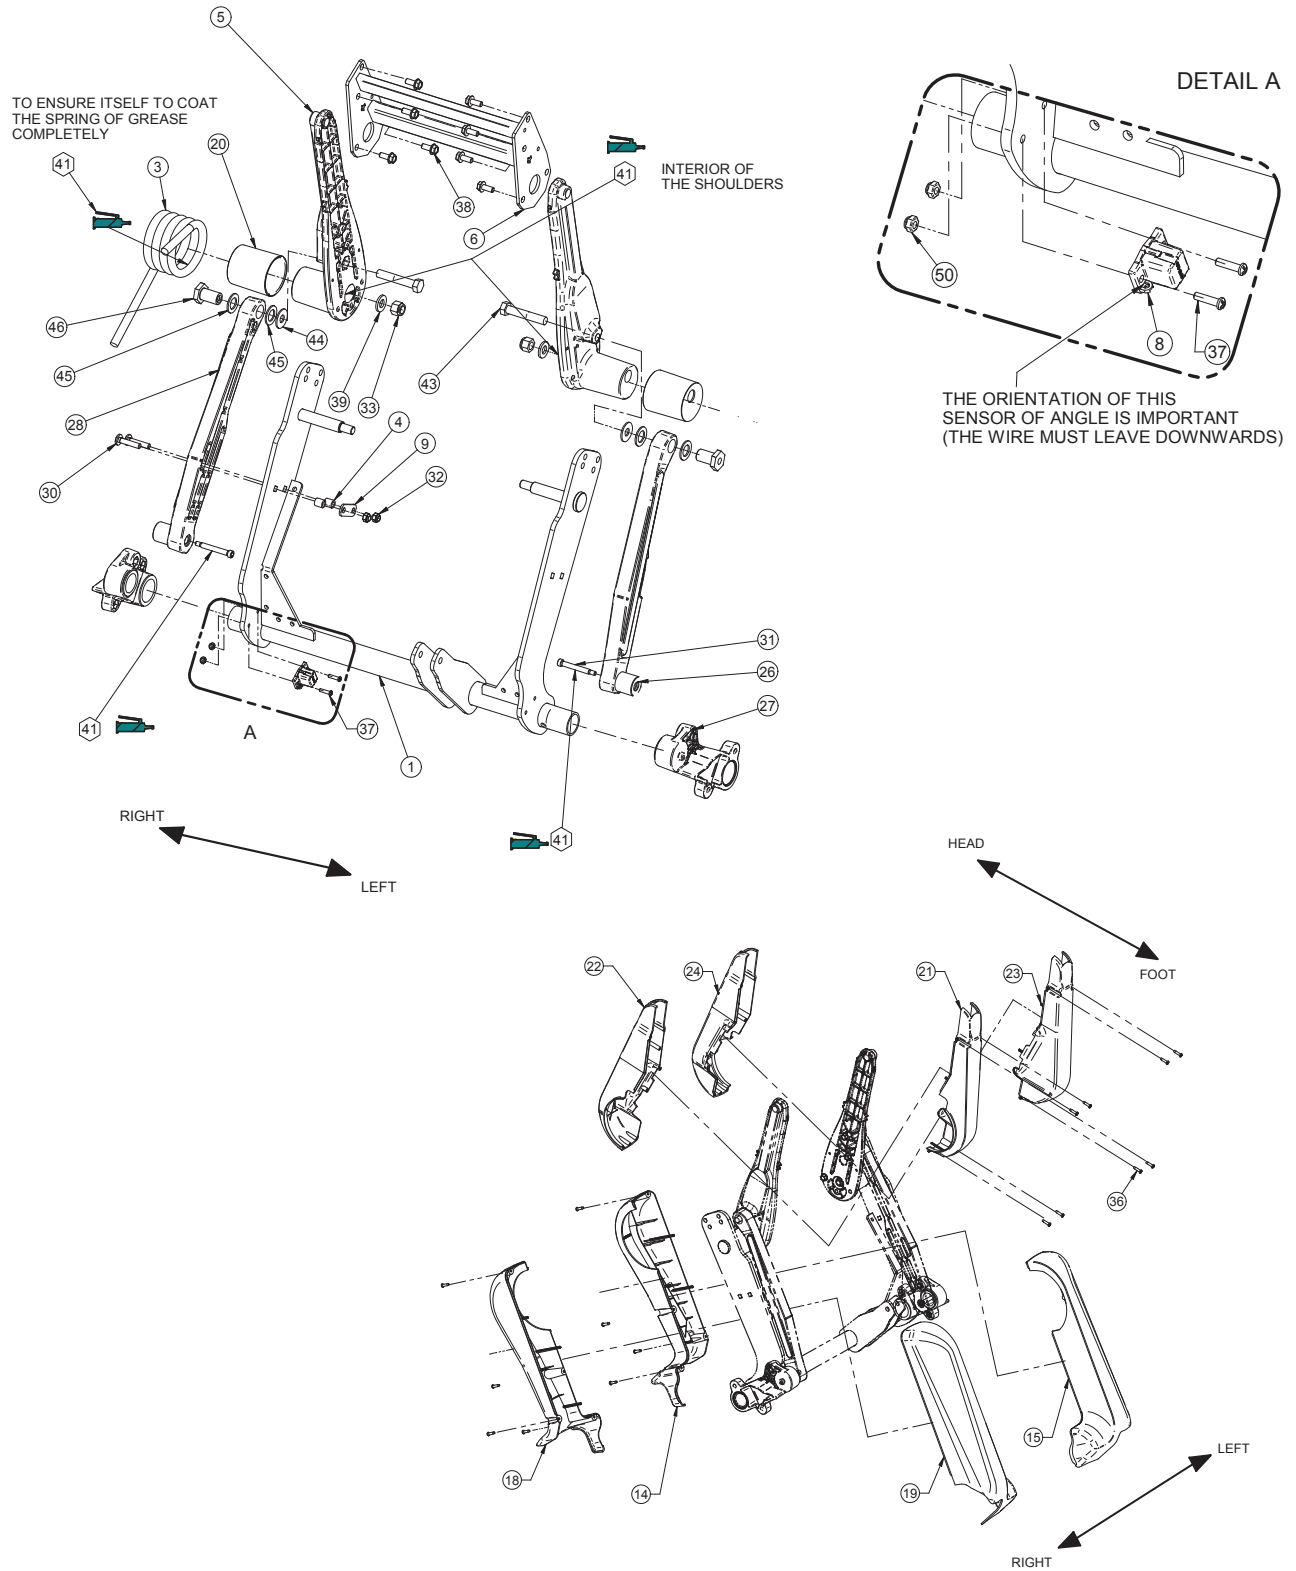

Lift Assembly


(Applies to beds with Serial Numbers U02818 - Current)

Lift Assembly - L27-044 Rev-C (Reference only)

Item	Part No.	Part Name	Qty.
1	27-0992W	Foot Main Lift	1
2	27-0993W	Head Main Lift	1
3	QRT27-1011	Bed Lift System Right Spring	1
4	27-1012	Spring Stop	2
5	QPA27-1013	Molded Bed Lift System Arm	4
6	27-1977W	Foot Reinforcement	1
7	27-1089W	Head Transverse Reinforcement	1
8	27-2477	Angle Sensor Assembly	1
9	27-1243Z	Spring Retention Plate	1
10	27-1623	Lift Spacer	2
11	QDF27-1251	Foot Lift Actuator	1
12	QDF27-1252	Head Lift Actuator	1
13	QDF7899	Hitch Pin Diameter 1/2"	4
14	QP27-0982-10	Exterior Right Low Lift Cover	2
15	QP27-0983-10	Interior Right Low Lift Cover	2
16	QP27-0984-10	Interior Head High Lift Cover	1
17	QP27-0985-10	Exterior Head High Lift Cover	1
18	QP27-0986-10	Exterior Left Low Lift Cover	2
19	QP27-0987-10	Interior Left Low Lift Cover	2
20	QP27-1065	Spring Sleeve	4
21	QP27-1236-10	Exterior Right Foot High Lift Cover	1
22	QP27-1237-10	Interior Right Foot High Lift Cover	1
23	QP27-1238-10	Exterior Left Foot High Lift Cover	1
24	QP27-1239-10	Interior Left Foot High Lift Cover	1
25	QPA27-1024	Right Lever Support	2
26	QPA27-1030	Right Stiffener Arm	2
27	QPA27-1036	Left Lever Support	2
28	QPA27-1040	Left Stiffener Arm	2
29	VB18A1O32	Bolt	12
30	VB35A1O40	Carriage Bolt	2
31	VD60B1O48	Shoulder Screw	4
32	VE30A1O	Nylon Locknut	14
33	VE30A1R	Nylon Locknut Diameter	4
34	VG50A1648	Clevis Pin Diameter	2
35	VG50A1654	Clevis Pin Diameter	2
36	VV23A1G24HL	Pan Head Tapping Screw	32
37	VV33A0G24	Pan Head Tapping Screw	2
38	VVB4A1024	Thread Rolling Bolt	12
39	VW10A173308	Flat Washer	4
40	VW10C173602	Nylon Washer	4
41	M0019	Grease	1
42	QP27-1830-01	Glider	4
43	VB18A1R54-S	Hexagon Bolt	4
44	27-2022Z	Stiffener Arm Steel Washer	4
45	QP27-2019	Stiffener Arm Acetal Washer	8
46	27-2018Z	Stiffener Arm Bearing	4
47	27-2053Z	Clevis Pin Diameter	4
48	QDF7878	Hitch Pin Diameter	4
49	VW10C432002	Nylon Washer	2
50	VE30A0G	Nylon Locknut	2
51	27-2117	Spring in Base	1
52	QDF2100	Round	4

Spring Assembly

27-2117 Rev-06 (Reference Only)

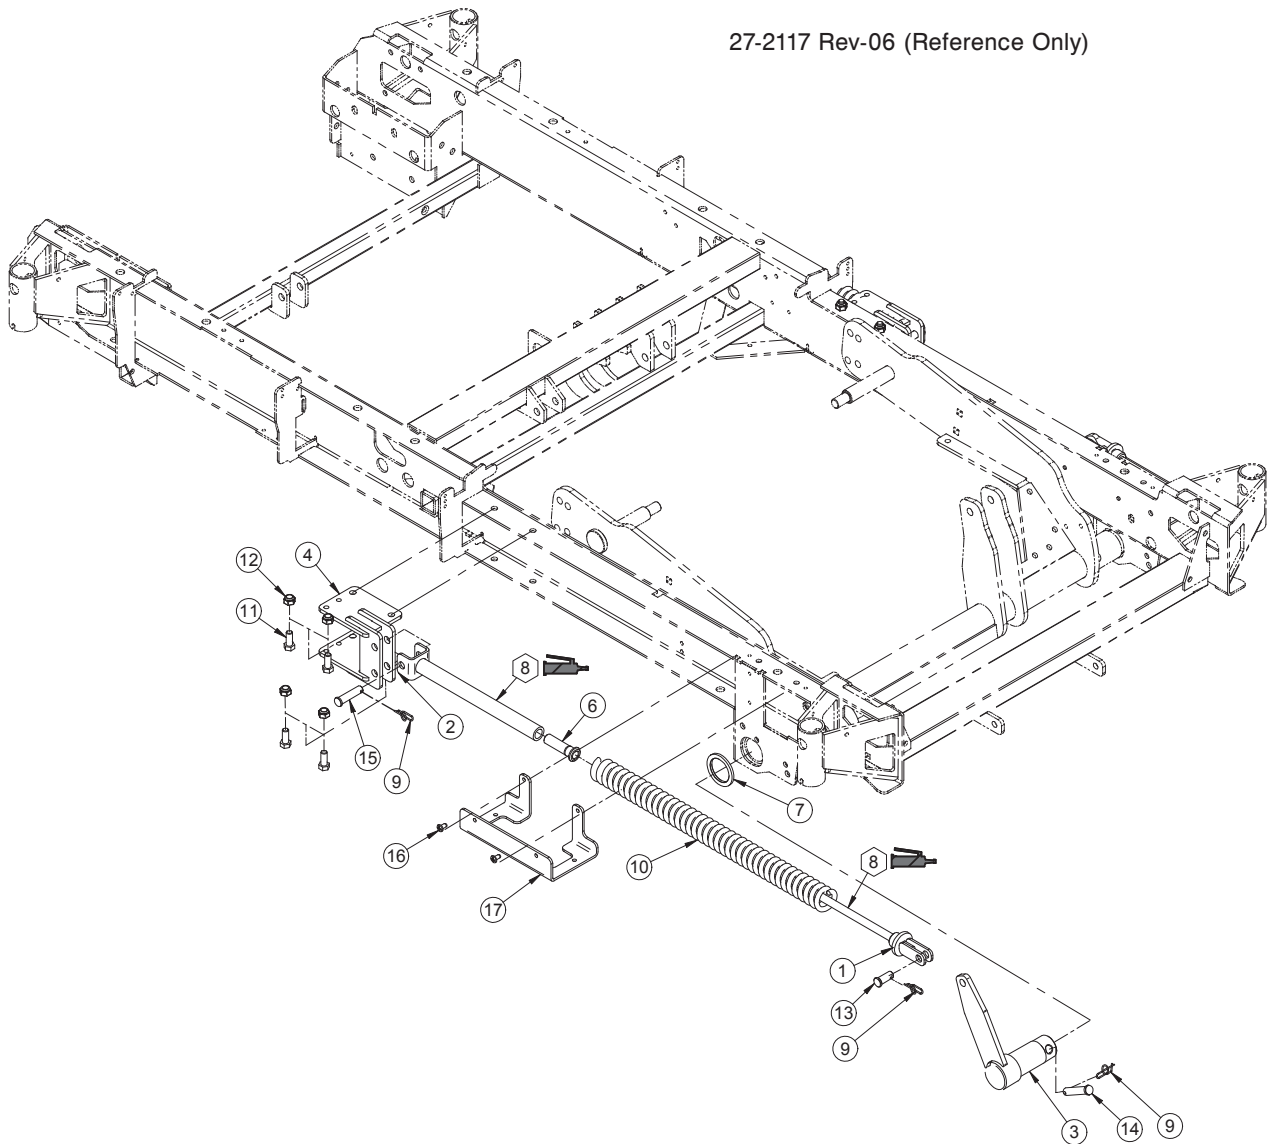

Spring Assembly - 27-2117 Rev-06 (Reference Only)


Item	Part No.	Part Name	Qty.
1	27-2096P	Hi-Lo Spring Support	2
2	27-2099P	Hi-Lo Spring Support Tube	2
3	27-2102P	Spring Tie	2
4	27-2107P	Spring Support Assembly	2
6	27-2115	Hi-Lo Spring Support Glider	2
7	27-2116	Acetal Washer	2
8	M0019	Grease	1
9	QDF7878	Clevis Pin Diameter	6
10	QRC27-2114	Base Compression Spring	2
11	VB15A1O24	Bolt	8
12	VE30A1O	Nylon Locknut	8
13	VG50A1228	Clevis Pin	2
14	VG50A1244	Clevis Pin	2
15	VG50A1240	Clevis Pin	2
16	VV83A9G12	Phillips Head Tapping Screw	4
17	27-2139P	Base Wiring Routing	2

[Return To Table of Contents](#)

Litter Assembly

(Applies to beds with Serial Numbers U01001 - U02817)

L27-038 Rev-01 (Reference Only)

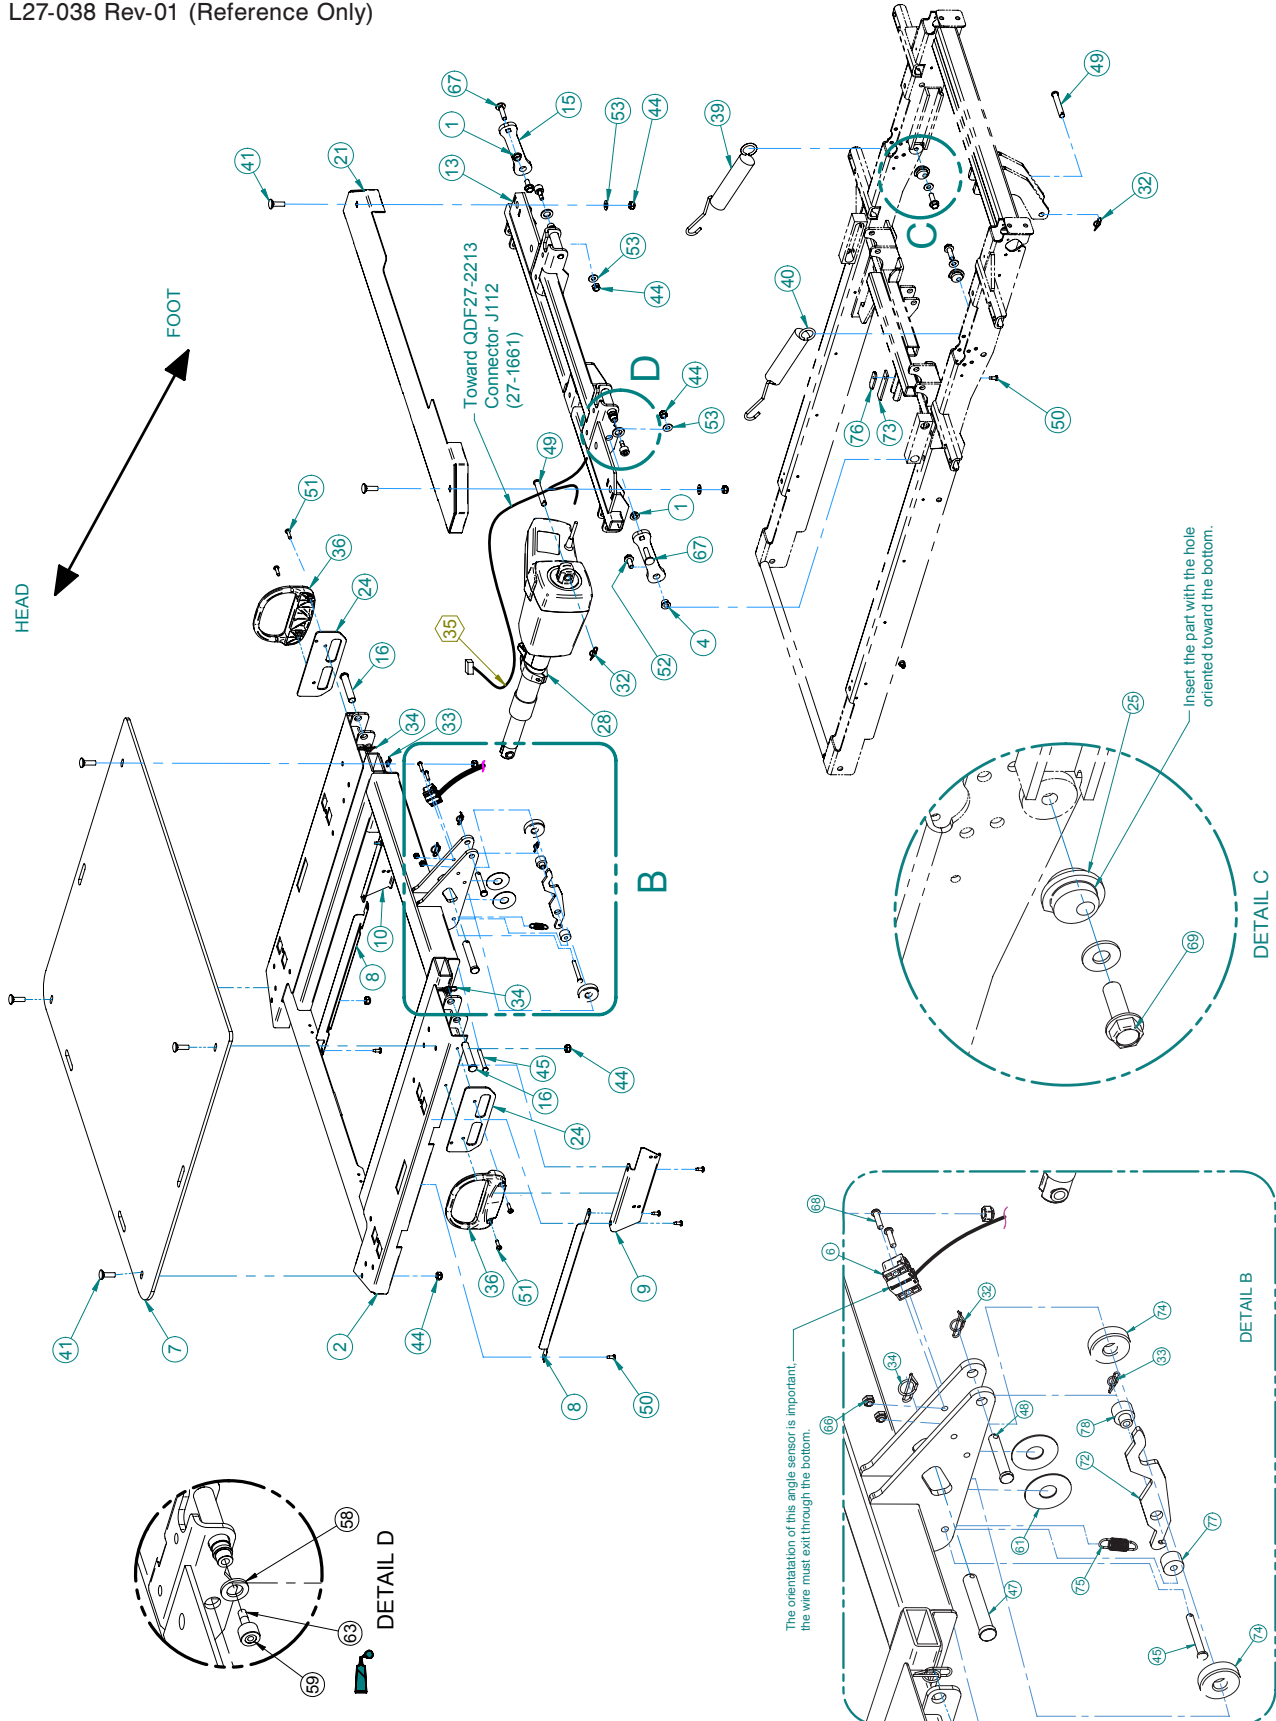

(Applies to beds with Serial Numbers U01001 - U02817)



Litter Assembly

(Applies to beds with Serial Numbers U01001 - U02817)

Litter Assembly - L27-038 Rev-01 (Reference Only)

Item	Part No.	Part Name	Qty.
1	21-3613	5/16" Sleeve for 3/16	2
2	27-0054W	Fowler S.A.	1
3	27-0485	Clevis Pin	4
4	27-0919	5/16" Sleeve for 5/16	2
5	27-2260W	Bolted Foot Litter	1
6	27-1209	Angle Sensor	2
7	QDF27-1397	Fowler	1
8	27-1634W	Cable Protector	2
9	27-1652W	Right Cable Protector	1
10	27-1667W	Left Cable Protector	1
11	27-1825W	Welded Center Section Cover	1
12	27-1862W	Gatch	1
13	27-1888W	Intermediary Fowler	1
15	27-1919Z	Lever Arm	2
16*	27-1920	Clevis Pin	2
17	27-1925	Gatch Bushing	2
18	27-1932Z	Gatch Pivot	1
19	27-1935Z	Upper Pivot Support	1
20	27-1940W	Transformer Box	1
21	27-1973W	Intermediary Section Cover	1
24	27-2015W	Head Restraint Support	2
25	27-2141	Unbalanced Spring Support Rod	2
28	QDF27-1214	Fowler Actuator	1
29	QDF27-1215	Gatch Actuator	1
30	QDF27-1216	Foot Actuator	1
32	QDF7878	Cotter Pin	10
33	QDF7898	Cotter Pin	2
34	QDF7899	Cotter Pin	3
35*	QDF9518	Cable Tie	1
36	QP27-1435-10	Mattress Stopper	2
37	QP27-1958	Gatch Pivot Stopper	1
39	QRT27-2020	Torsion Spring	1
40	QRT27-2026	Right Upper Frame Spring Base Rod	1
41	VB35A1O32	Carriage Bolt	6
42	VB24A1O50	Carriage Bolt	1
44	VE30A1O	Nylon Locknut	9
45	VG50A0848	Clevis Pin Diameter	2
46	VG50A1244	Clevis Pin	2
47	VG50A1654	Clevis	1
48	VG50B1248	Clevis Pin Diameter	2
49	VG50B1250	Clevis Pin	2
50	VV83A9G16	Phillips Screw	14
51	VV83A9G24	Phillips Screw	6
52	VVB4A1024	Thread Rolling Bolt	6
53	VW10A10	Flat Washer	6
56	QDF2098	CAM Follower	2
57	VE39A0P	Nylon Locknut	2
58	27-2063	Intermediary Pivot Washer	2
59	QDF2110	Needle Bearing	2

Litter Assembly

(Applies to beds with Serial Numbers U01001 - U02817)


Litter Assembly - L27-038 Rev-01 (Continued) (Reference Only)

Item	Part No.	Part Name	Qty.
61	VW10C432002	Nylon Washer	2
63*	M0008	Threadlocker (Blue)	.030 ml
66	VE30A0G	Nylon Locknut	2
67	VB35A1O36	Carriage Bolt	2
68	VV33A0G24	Phillips Screw	2
69	VVB4A1032	Hex Head Thread Rolling Bolt	2
72	27-2223Z	Finger	1
73	27-2217	PVC Slide	1
74	27-2227	Bushing Latch Finger	2
75	QRE27-2218	Finger Bracket Spring	1
76	27-2219Z	Plate of Tightening	1
77	27-2221	Male Bushing Latch Finger	1
78	27-2220	Male Bushing Latch Finger	1

Litter Assembly


(Applies to beds with Serial Numbers U02818 - U04982)

L27-045 Rev-00 (Reference Only)

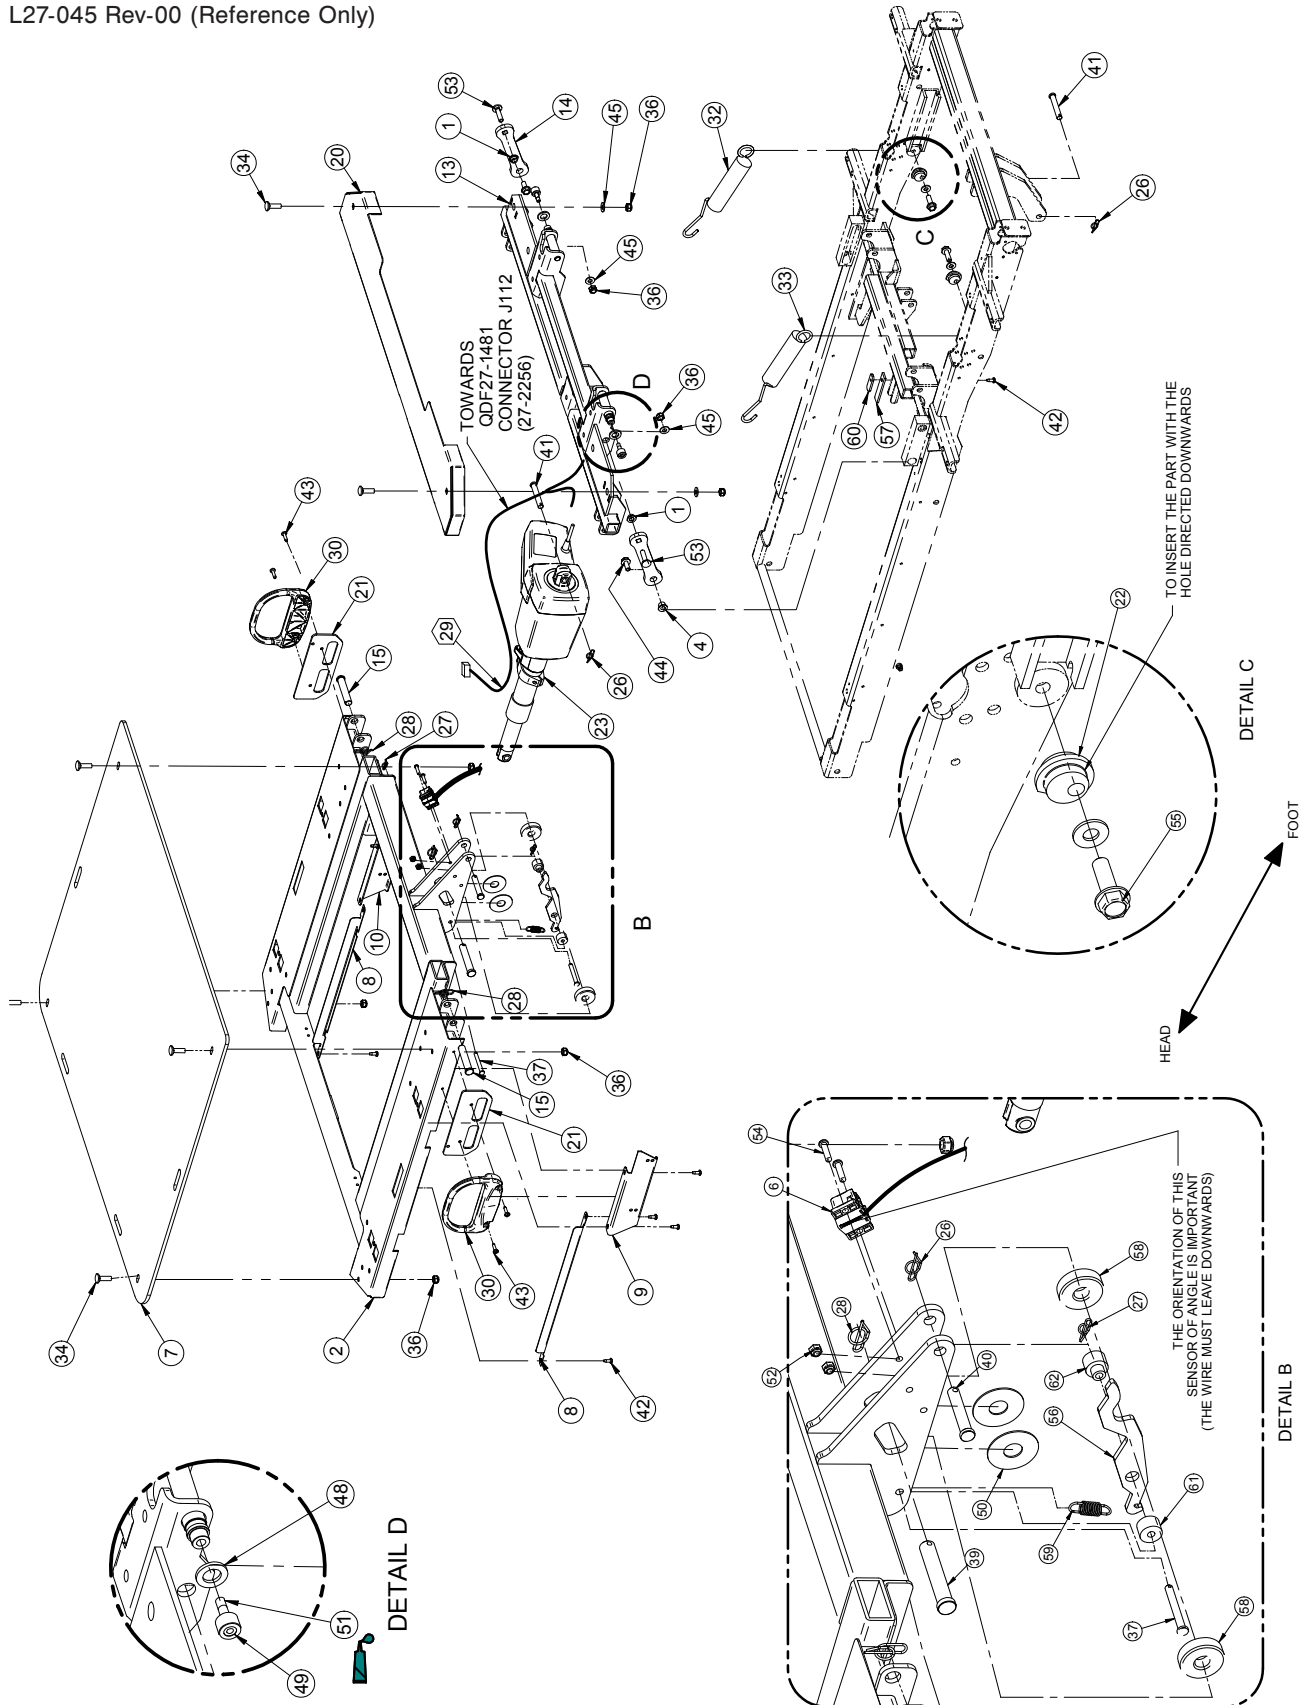

Litter Assembly

(Applies to beds with Serial Numbers U02818 - U04982)

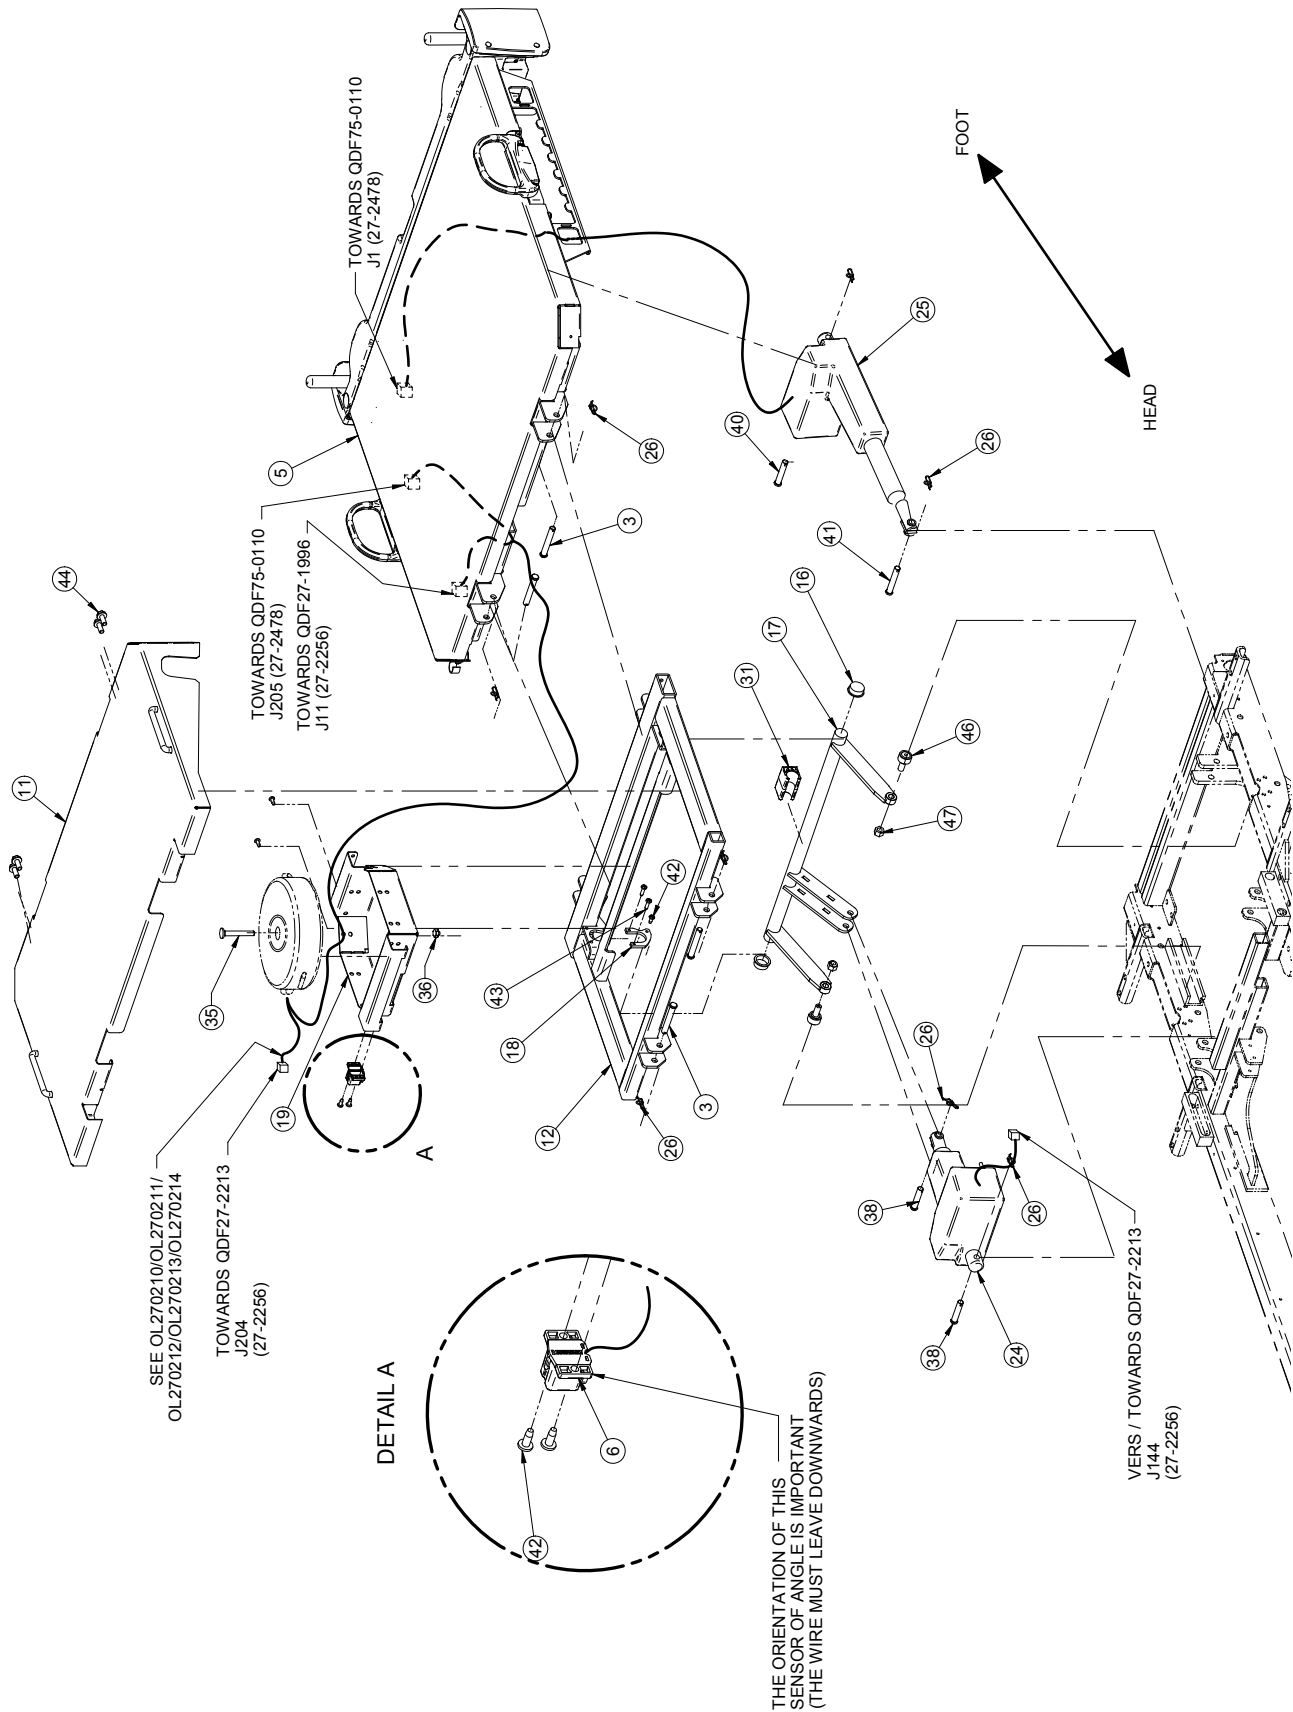

Litter Assembly

(Applies to beds with Serial Numbers U02818 - U04982)

Litter Assembly - L27-045 Rev-00 (Reference Only)

Item	Part No.	Part Name	Qty.
1	21-3613	5/16" Sleeve for 3/16	2
2	27-2269W	Fowler S.A.	1
3	27-0485	Clevis Pin 3/8"	4
4	27-0919	5/16" Sleeve for 5/16	2
5	27-2478	Bolted Foot Litter	1
6	27-2477	Angle Sensor Assembly	2
7	QDF27-1397	Fowler	1
8	27-1634W	Cable Protector	2
9	27-1652W	Right Cable Protector	1
10	27-1667W	Left Cable Protector	1
11	27-1825W	Welded Center Section Cover	1
12	27-1862W	Gatch	1
13	27-1888W	Intermediary Fowler	1
14	27-1919Z	Lever Arm	2
15	27-1920	Clevis Pin	2
16	27-1925	Gatch Bushing	2
17	27-1932Z	Gatch Pivot	1
18	27-1935Z	Upper Pivot Support	1
19	27-1940W	Transformer Box	1
20	27-1973W	Intermediary Section Cover	1
21	27-2015W	Head Restraint Support	2
22	27-2141	Unbalanced Spring Support Rod	2
23	QDF27-1214	Fowler Actuator	1
24	QDF27-1215	Gatch Actuator	1
25	QDF27-1216	Foot Actuator	1
26	QDF7878	Cotter Pin	10
27	QDF7898	Cotter Pin	2
28	QDF7899	Cotter Pin	3
29*	QDF9518	Cable Tie	1
30	QP27-1435-10	Mattress Stopper	2
31	QP27-1958	Gatch Pivot Stopper	1
32	QRT27-2020	Torsion Spring	1
33	QRT27-2026	Right Upper Frame Spring Base Rod	1
34	VB35A1O32	Carriage Bolt	6
35*	VB24A1O50	Carriage Bolt	1
36	VE30A1O	Nylon Locknut	9
37	VG50A0848	Clevis Pin	2
38	VG50A1244	Clevis Pin	2
39	VG50A1654	Clevis Pin	1
40	VG50B1248	Clevis Pin	2
41	VG50B1250	Clevis Pin	2
42	VV83A9G16	Phillips Screw	14
43	VV83A9G24	Phillips Screw	6
44	VVB4A1024	Thread Rolling Bolt	6
45	VW10A10	Flat Washer	6
46	QDF2098	CAM Follower	2
47	VE39A0P	Nylon Locknut	2
48	27-2063	Intermediary Pivot Washer	2
49	QDF2110	Needle Bearing	2

Litter Assembly

(Applies to beds with Serial Numbers U02818 - U04982)


Litter Assembly - L27-045 Rev-00 (Continued) (Reference Only)

Item	Part No.	Part Name	Qty.
50	VW10C432002	Nylon Washer	2
51*	M0008	Threadlocker (Blue)	.030 ml
52	VE30A0G	Nylon Locknut	2
53	VB35A1O36	Carriage Bolt	2
54	VV33A0G24	Phillips Screw	2
55	VVB4A1032	Hex Head Thread Rolling Bolt	2
56	27-2223Z	Finger	1
57	27-2217	PVC Slide	1
58	27-2227	Bushing Latch Finger	2
59	QRE27-2218	Finger Bracket Spring	1
60	27-2219Z	Plate of Tightening	1
61	27-2221	Male Bushing Latch Finger	1
62	27-2220	Male Bushing Latch Finger	1

Litter Assembly


(Applies to beds with Serial Numbers U04983 - U50240)

L27-065 Rev A (Reference Only)

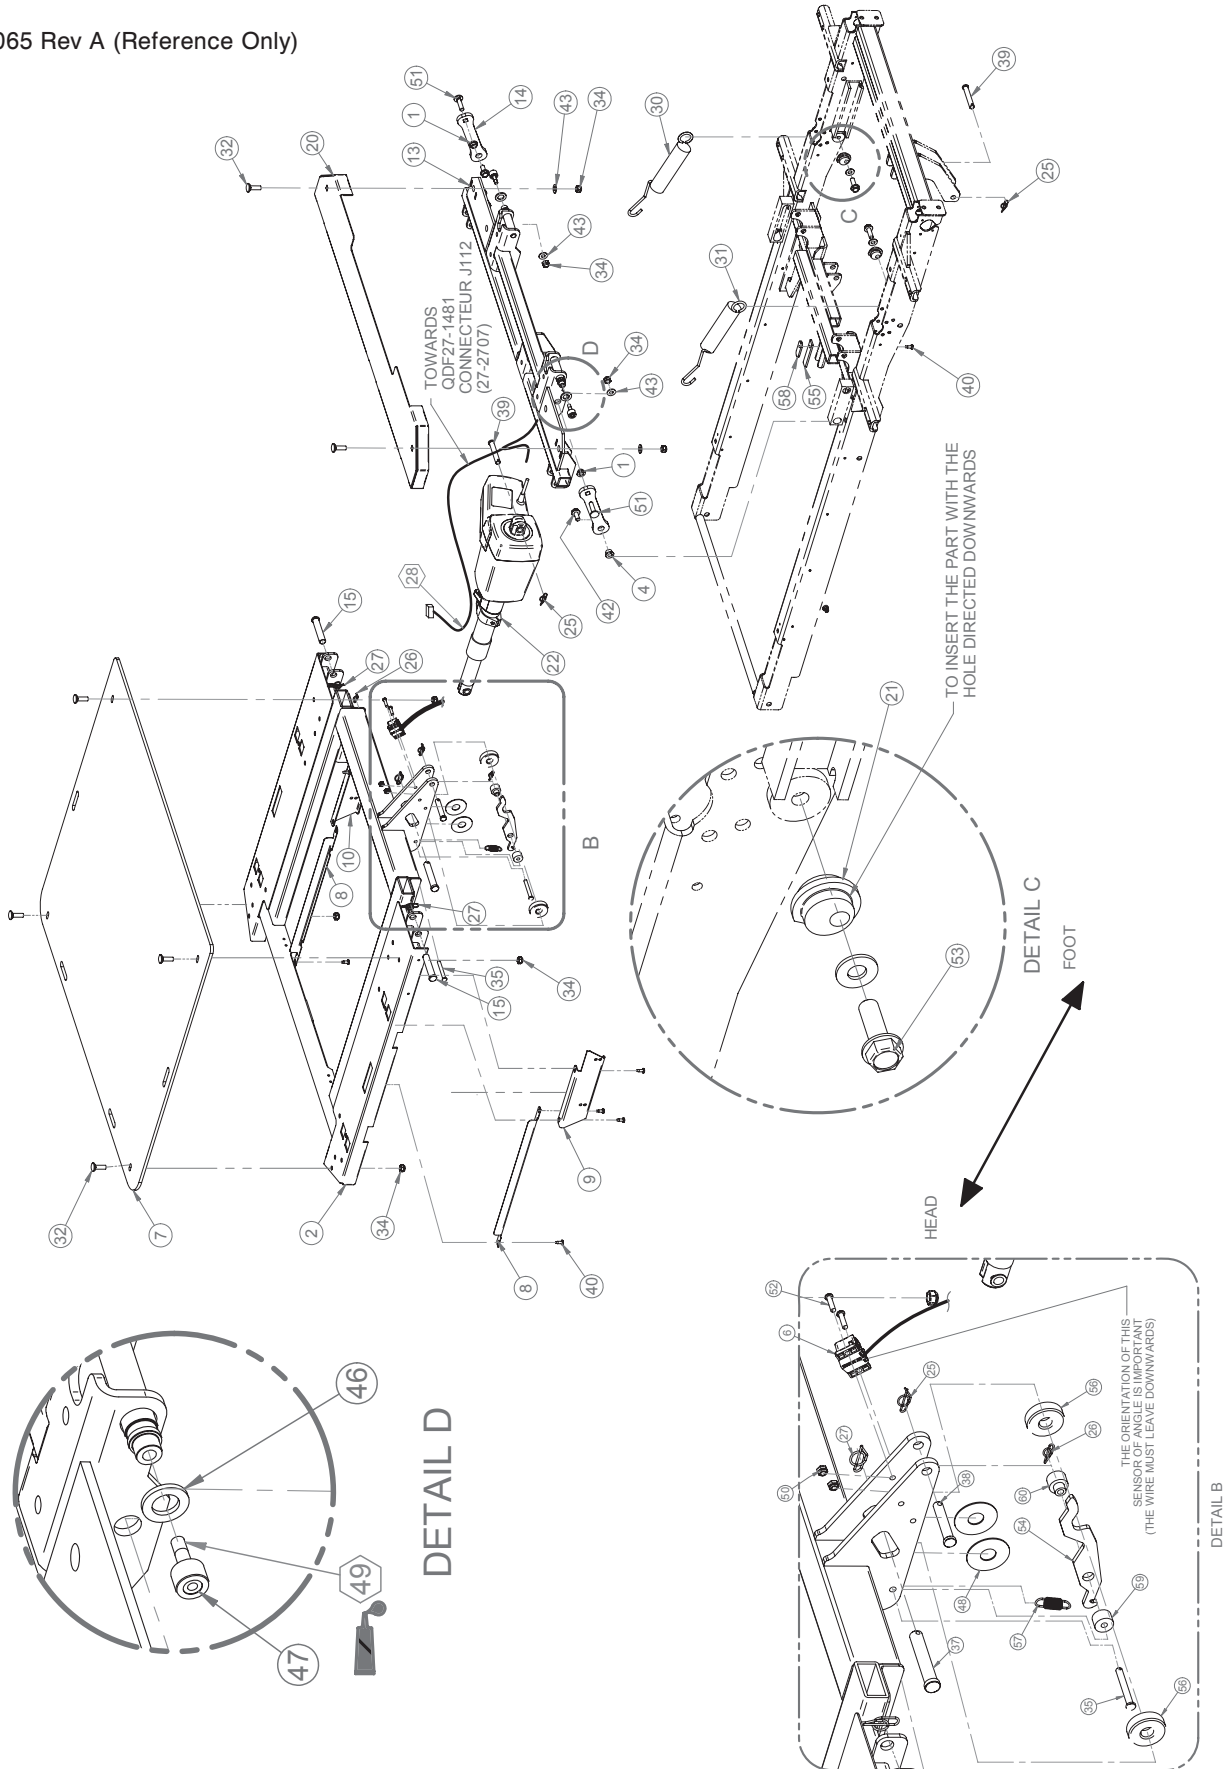

Litter Assembly

(Applies to beds with Serial Numbers U04983 - U50240)

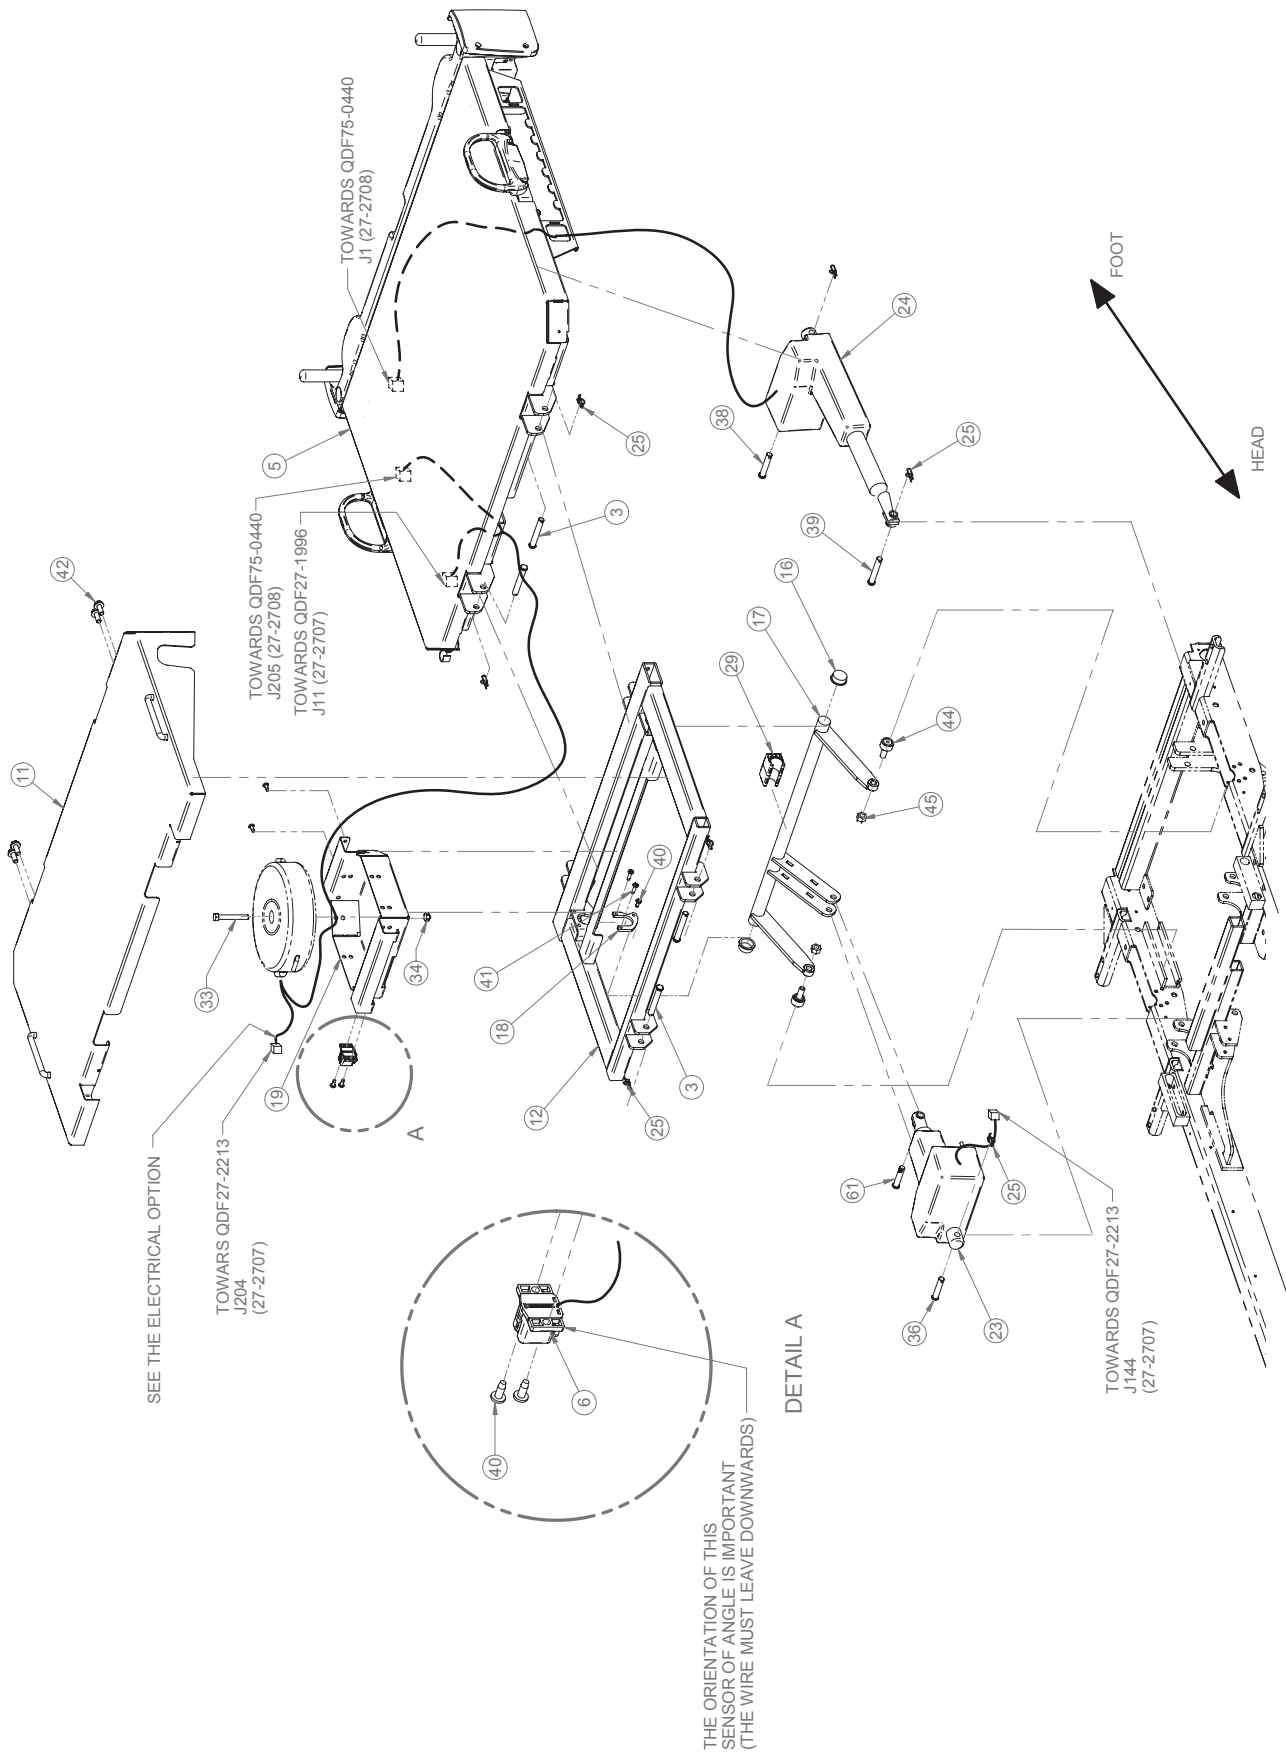

[Return To Table of Contents](#)

Litter Assembly

(Applies to beds with Serial Numbers U04983 - U50240)

Litter Assembly - L27-065 Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	21-3613	5/16" Sleeve for 3/16	2
2	27-2269P	Fowler S.A.	1
3	27-0485	Clevis Pin -	4
4	27-0919	5/16" Sleeve for 5/16	2
5	27-2708	Bolted Foot Litter	1
6	27-2477	Angle Sensor Assembly	2
7	QDF27-1397	Fowler	1
8	27-1634P	Cable Protector	2
9	27-1652P	Right Cable Protector	1
10	27-1667P	Left Cable Protector	1
11	27-1825P	Welded Center Section Cover	1
12	27-1862P	Gatch	1
13	27-1888P	Intermediary Fowler	1
14	27-1919Z	Lever Arm	2
15	27-1920	Clevis Pin	2
16	27-1925	Gatch Bushing	2
17	27-1932Z	Gatch Pivot	1
18	27-1935Z	Upper Pivot Support	1
19	27-1940P	Transformer Box	1
20	27-1973P	Intermediary Section Cover	1
21	27-2141	Unbalanced Spring Support Rod	2
22	QDF27-1214	Fowler Actuator	1
23	QDF27-1215	Gatch Actuator	1
24	QDF27-1216	Foot Actuator	1
25	QDF7878	Cotter Pin	9
26	QDF7898	Cotter Pin	2
27	QDF7899	Cotter Pin	3
28	QDF9518	Cable Tie	1
29	QP27-1958	Gatch Pivot Stopper	1
30	QRT27-2020	Torsion Spring	1
31	QRT27-2026	Right Upper Frame Spring Base Rod	1
32	VB35A1O32	Carriage Bolt	6
33	VB15A1O50	Carriage Bolt	1
34	VE30A1O	Nylon Locknut 5/16-18	9
35	VG50A0848	Clevis Pin	2
36	VG50A1244	Clevis Pin	1
37	VG50A1654	Clevis	1
38	VG50B1248	Clevis Pin	2
39	VG50A1250	Clevis Pin	2
40	VV83A9G16	Phillips Screw	14
41	VV83A9G24	Phillips Screw	2
42	VVB4A1O24	Thread Rolling Bolt	4
43	VW10A10	Flat Washer	6
44	QDF2098	CAM Follower	2
45	VE59A0P	Nylon Locknut 3/8-24	2
46	27-2063	Intermediary Pivot Washer	2
47	QDF2110	Needle Bearing	2
48	VW10C432002	Nylon Washer	2
49	M0008	Threadlocker (Blue)	-

Litter Assembly

(Applies to beds with Serial Numbers U04983 - U50240)


Litter Assembly - L27-065 Rev A (Continued) (Reference Only)

Item	Part No.	Part Name	Qty.
50	VE30A0G	Nylon Locknut	2
51	VB35A1O36	Carriage Bolt	2
52	VV33A0G24	Phillips Screw	2
53	VVB4A1O32	Hex Head Thread Rolling Bolt	2
54	27-2223Z	Finger	1
55	27-2217	PVC Slide	1
56	27-2227	Bushing Latch Finger	2
57	QRE27-2218	Finger Bracket Spring	1
58	27-2219Z	Plate of Tightening	1
59	27-2221	Female Bushing Latch Finger	1
60	27-2220	Male Bushing Latch Finger	1
61	QDF2132	Clevis Pin	1

Litter Assembly

(Applies to beds with Serial Numbers U50241 - Current)

L27-056 Rev E (Reference Only)

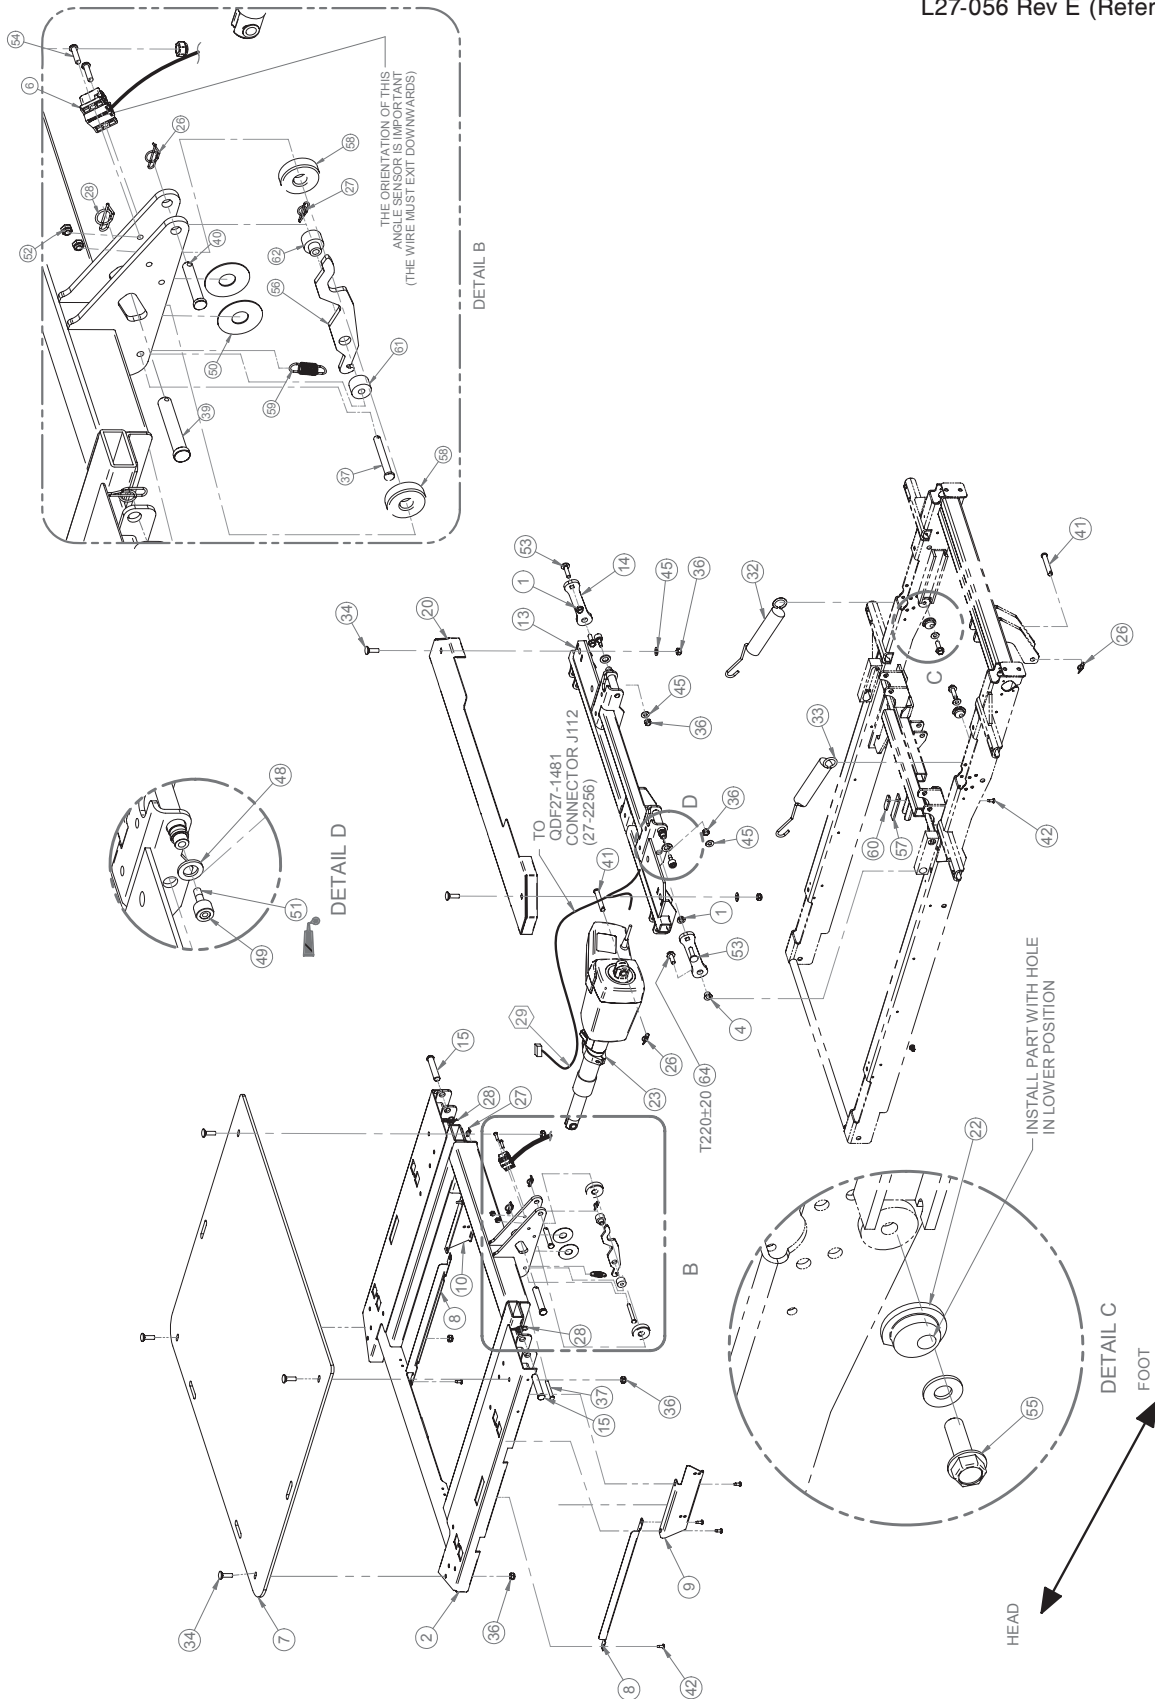

(Applies to beds with Serial Numbers U50241 - Current)



Litter Assembly

(Applies to beds with Serial Numbers U50241 - Current)

Litter Assembly - Common Components - L27-056 Rev E (Reference Only)

Item	Part No.	Part Name	Qty.
1	21-3613	5/16" Sleeve for 3/16	2
2	27-2269P	Fowler S.A.	1
3	27-0485	Clevis Pin -	4
4	27-0919	5/16" Sleeve for 5/16	2
5	27-2688	Bolted Foot Litter	1
6	27-2477	Angle Sensor Assembly	2
7	QDF27-1397	Fowler	1
8	27-1634P	Cable Protector	2
9	27-1652P	Right Cable Protector	1
10	27-1667P	Left Cable Protector	1
11	27-1825P	Welded Center Section Cover	1
12	27-1862P	Gatch	1
13	27-1888P	Intermediary Fowler	1
14	27-1919Z	Lever Arm	2
15	27-1920	Clevis Pin	2
16	27-1925	Gatch Bushing	2
17	27-1932Z	Gatch Pivot	1
18	27-1935Z	Upper Pivot Support	1
19	27-1940P	Transformer Box	1
20	27-1973P	Intermediary Section Cover	1
22	27-2141	Unbalanced Spring Support Rod	2
23	QDF27-1214	Fowler Actuator	1
24	QDF27-1215	Gatch Actuator	1
25	QDF27-1216	Foot Actuator	1
26	QDF7878	Cotter Pin	9
27	QDF7898	Cotter Pin	2
28	QDF7899	Cotter Pin	3
29	QDF9518	Cable Tie	1
31	QP27-1958	Gatch Pivot Stopper	1
32	QRT27-2020	Torsion Spring	1
33	QRT27-2026	Right Upper Frame Spring Base Rod	1
34	VB35A1O32	Carriage Bolt	6
35	VB15A1O50	Carriage Bolt	1
36	VE30A1O	Nylon Locknut 5/16-18	9
37	VG50A0848	Clevis Pin	2
38	VG50A1244	Clevis Pin	1
39	VG50A1654	Clevis	1
40	VG50B1248	Clevis Pin	2
41	VG50A1250	Clevis Pin	2
42	VV83A9G16	Phillips Screw	14
43	VV83A9G24	Phillips Screw	2
44	VVB4A1O24	Thread Rolling Bolt	4
45	VW10A10	Flat Washer	6
46	QDF2098	CAM Follower	2
47	VE59A0P	Nylon Locknut 3/8-24	2
48	27-2063	Intermediary Pivot Washer	2
49	QDF2110	Needle Bearing	2
50	VW10C432002	Nylon Washer	2
51	M0008	Threadlocker (Blue)	-

Litter Assembly


(Applies to beds with Serial Numbers U50241 - Current)

Litter Assembly (Continued) - Common Components - L27-056 Rev E (Reference Only) (Continued)


Item	Part No.	Part Name	Qty.
52	VE30A0G	Nylon Locknut	2
53	VB35A1O36	Carriage Bolt	2
54	VV33A0G24	Phillips Screw	2
55	VVB4A1O32	Hex Head Thread Rolling Bolt	2
56	27-2223Z	Finger	1
57	27-2217	PVC Slide	1
58	27-2227	Bushing Latch Finger	2
59	QRE27-2218	Finger Bracket Spring	1
60	27-2219Z	Plate of Tightening	1
61	27-2221	Female Bushing Latch Finger	1
62	27-2220	Male Bushing Latch Finger	1
63	QDF2132	Clevis Pin	1
64	VVB4A1O28	Thread Rolling Bolt	2

Litter Assembly, Interior Frame

L27-055 Rev C (Reference Only)

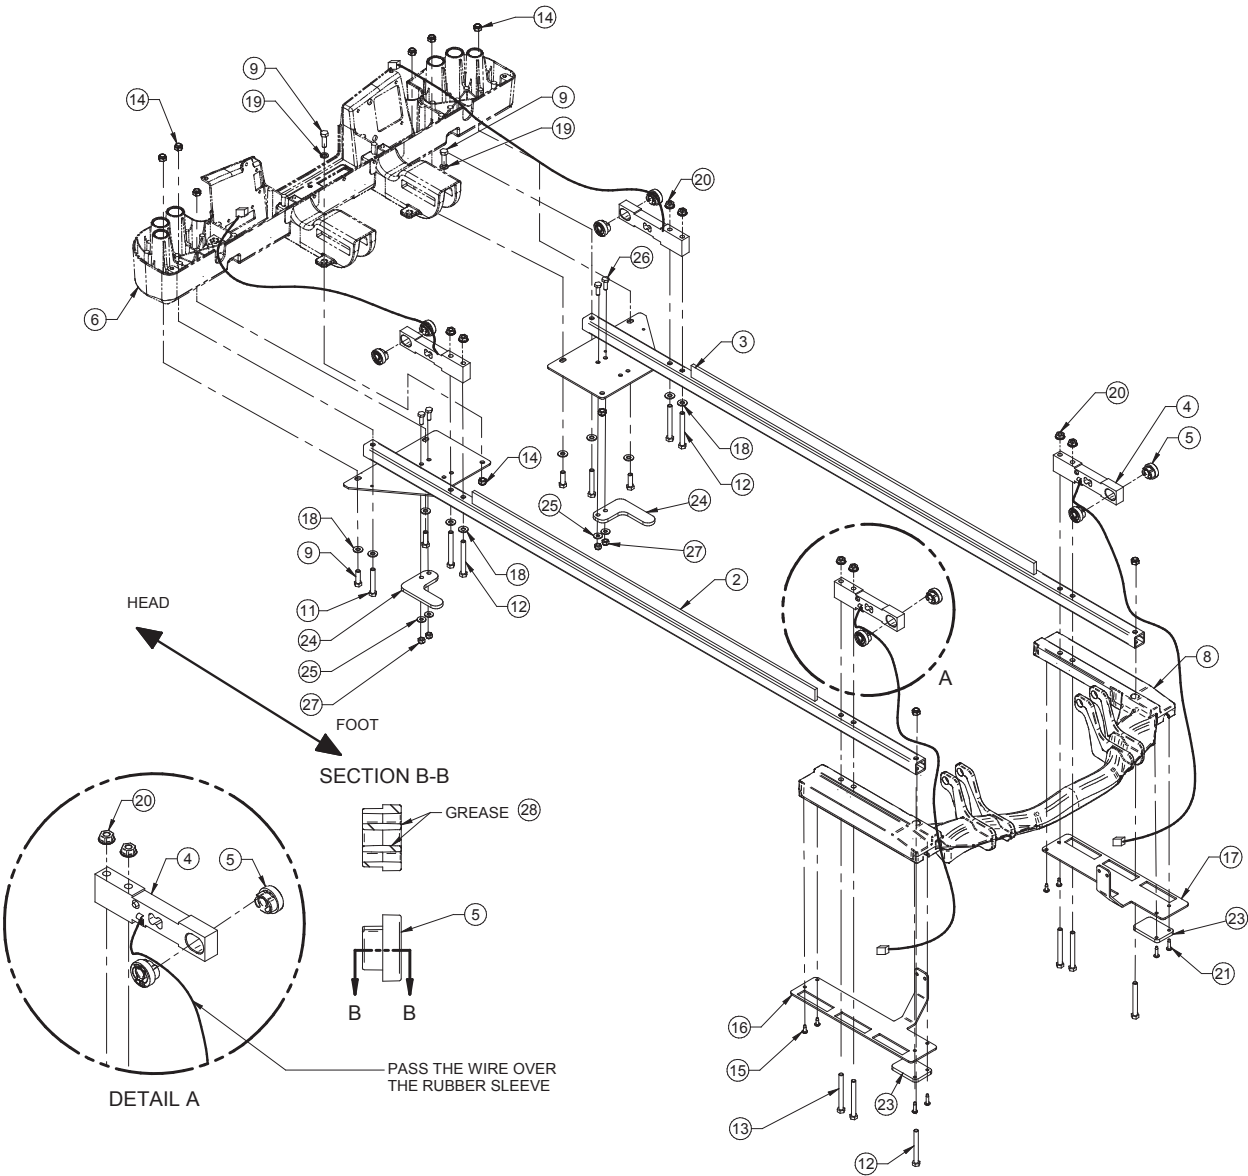

Litter Assembly, Interior Frame

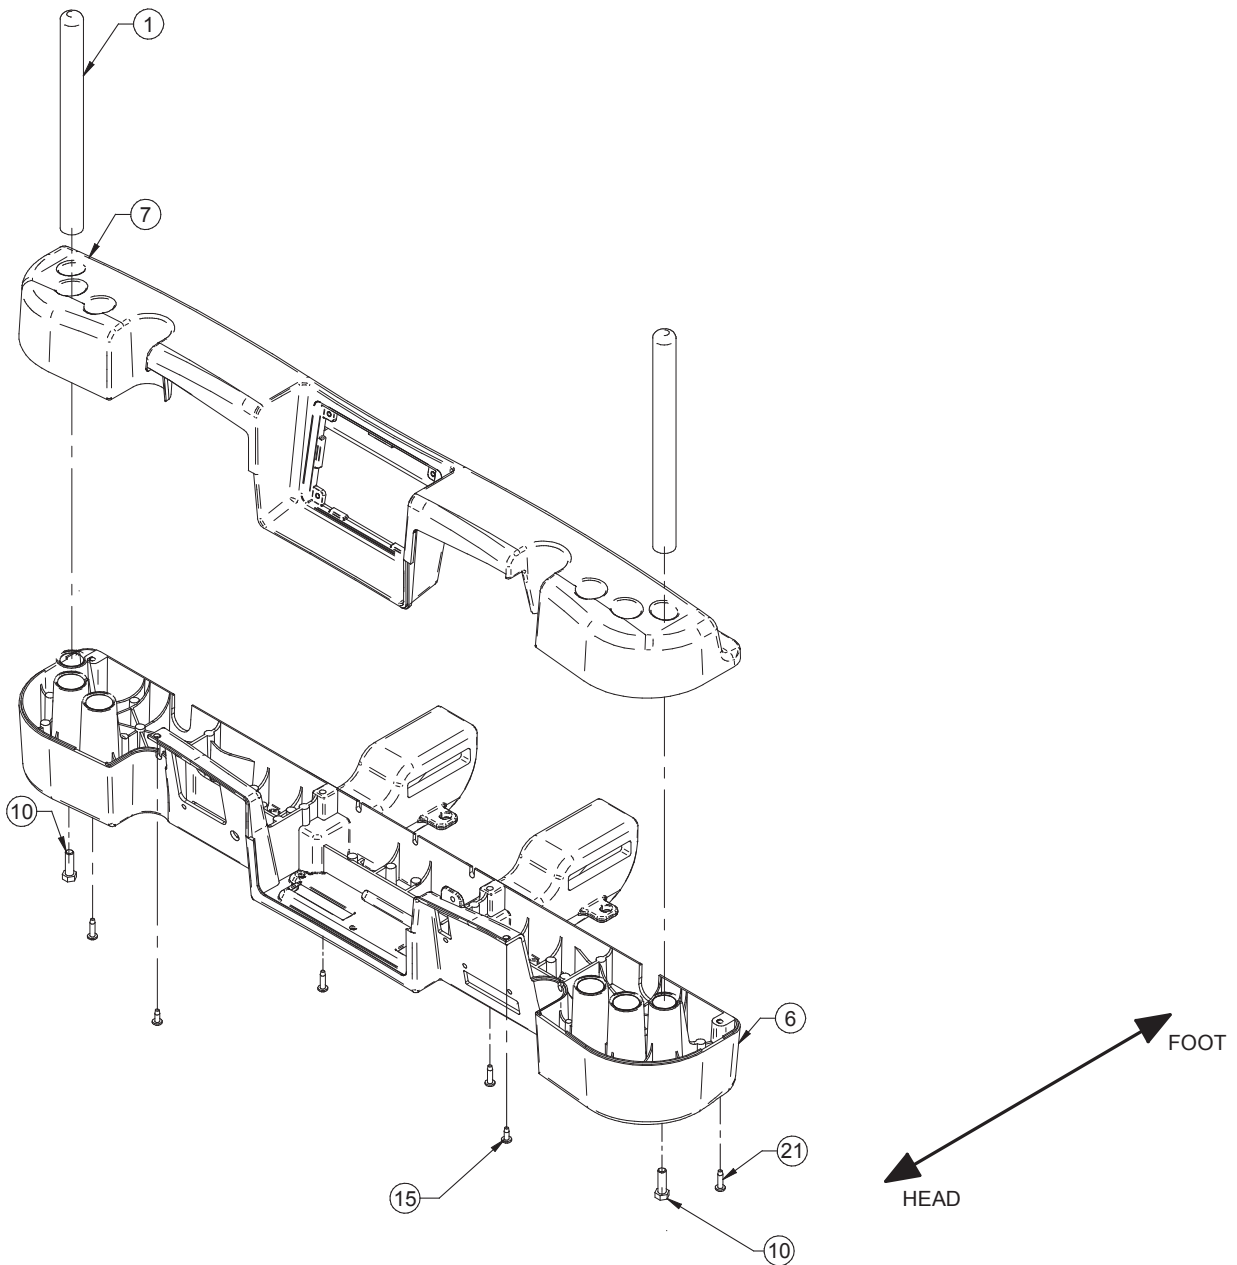


Litter Assembly, Interior Frame

Litter Assembly, Interior Frame - L27-055 Rev C (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-1180C	Head Board Anchoring	2
2	27-1310P	Right Lower Frame Support	1
3	27-1368P	Left Lower Frame Support	1
4	QDF27-1372	Symmetrical Load Cell	4
5	QP27-1469	Elastimer Sleeve	8
6	QPA27-1290	Head Chassis	1
7	QPA27-1291	Frame Head Cover	1
8	27-1426P	Foot Frame Support	1
9	VB15A1O32	Bolt	6
10	VB15A1O32-S	Bolt	2
11	VB15A1O48	Bolt	2
12	VB15A1O54	Bolt	6
13	VB15A1O56	Hex Bolt	4
14	VE30A1O	Nylon Hex Locknut	10
15	VV83A9G16	Pan Head Tapping Screw	6
16	27-1806P	Right Frame Support Cover	1
17	27-1385P	Left Frame Support Cover	1
18	VW10A10	Flat Washer	10
19	VW20A10	Spring Washer	2
20	VE78A1O	Flanged Locknut	8
21	VV83A9G24	Pan Head Tapping Screw	8
23	27-2143P	Spacer Foot	2
24	27-2144P	Spacer Head	2
25	VW10A08	Flat Washer	4
26	VB15A1N24	Bolt	4
27	VE30A1N	Nylon Hex Locknut	4
28	M0019	Grease	1

Litter Assembly with Serial Port

OL270278 Rev A (Reference Only)

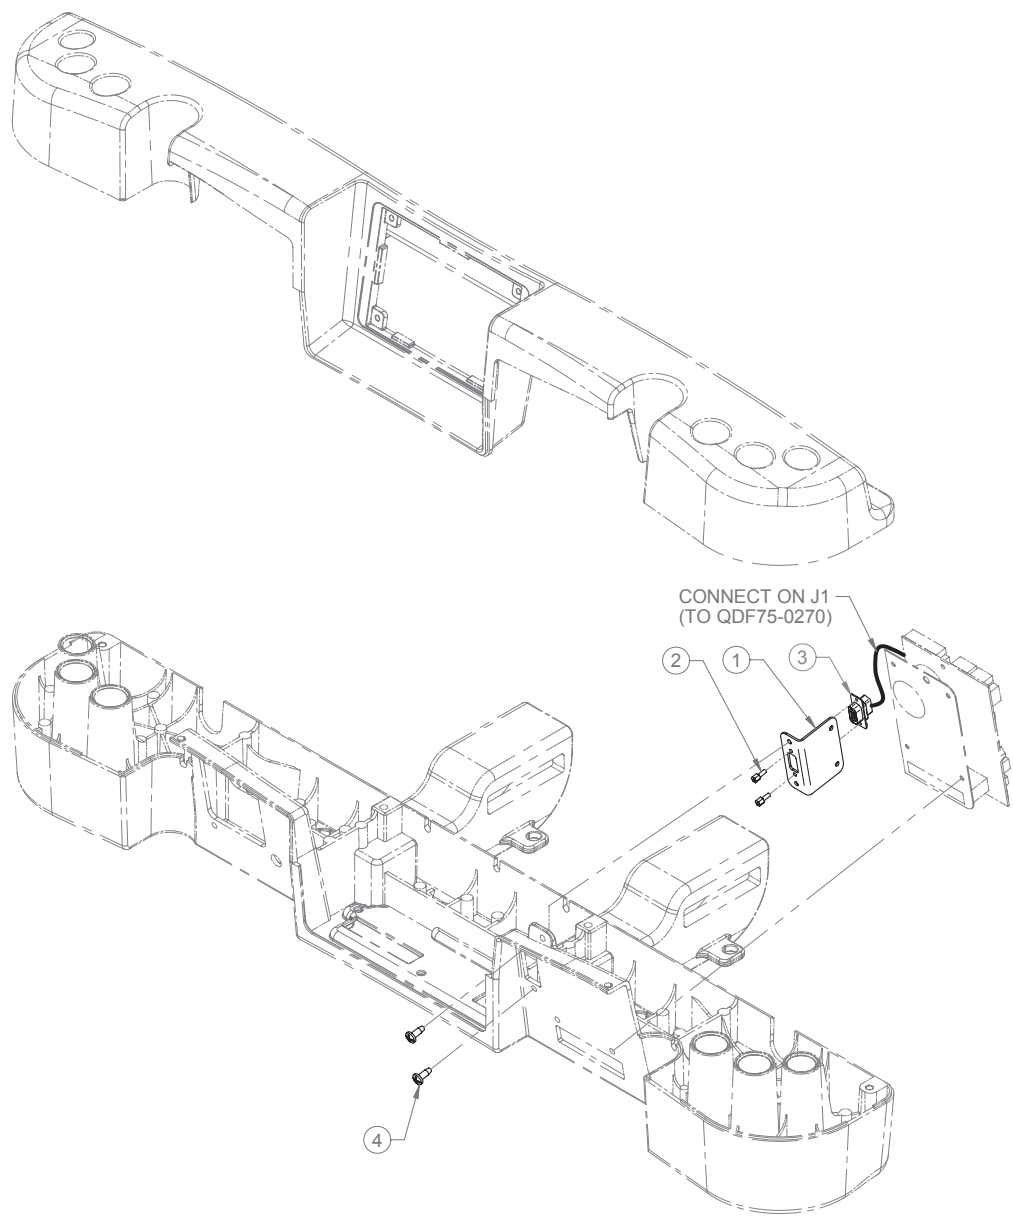


Litter Assembly with Serial Port - OL270278 Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-1520P	Support Connector	1
2	QDF2056	Standoff	2
3	QDF27-2432	Serial Interconnection Cable	1
4	VV83A9G16	Pan Head Phillips Screw	2

Litter Assembly, Upper Frame

(Applies to beds with Serial Numbers U01001 - U02817)


L27-041 Rev-00 (Reference Only)

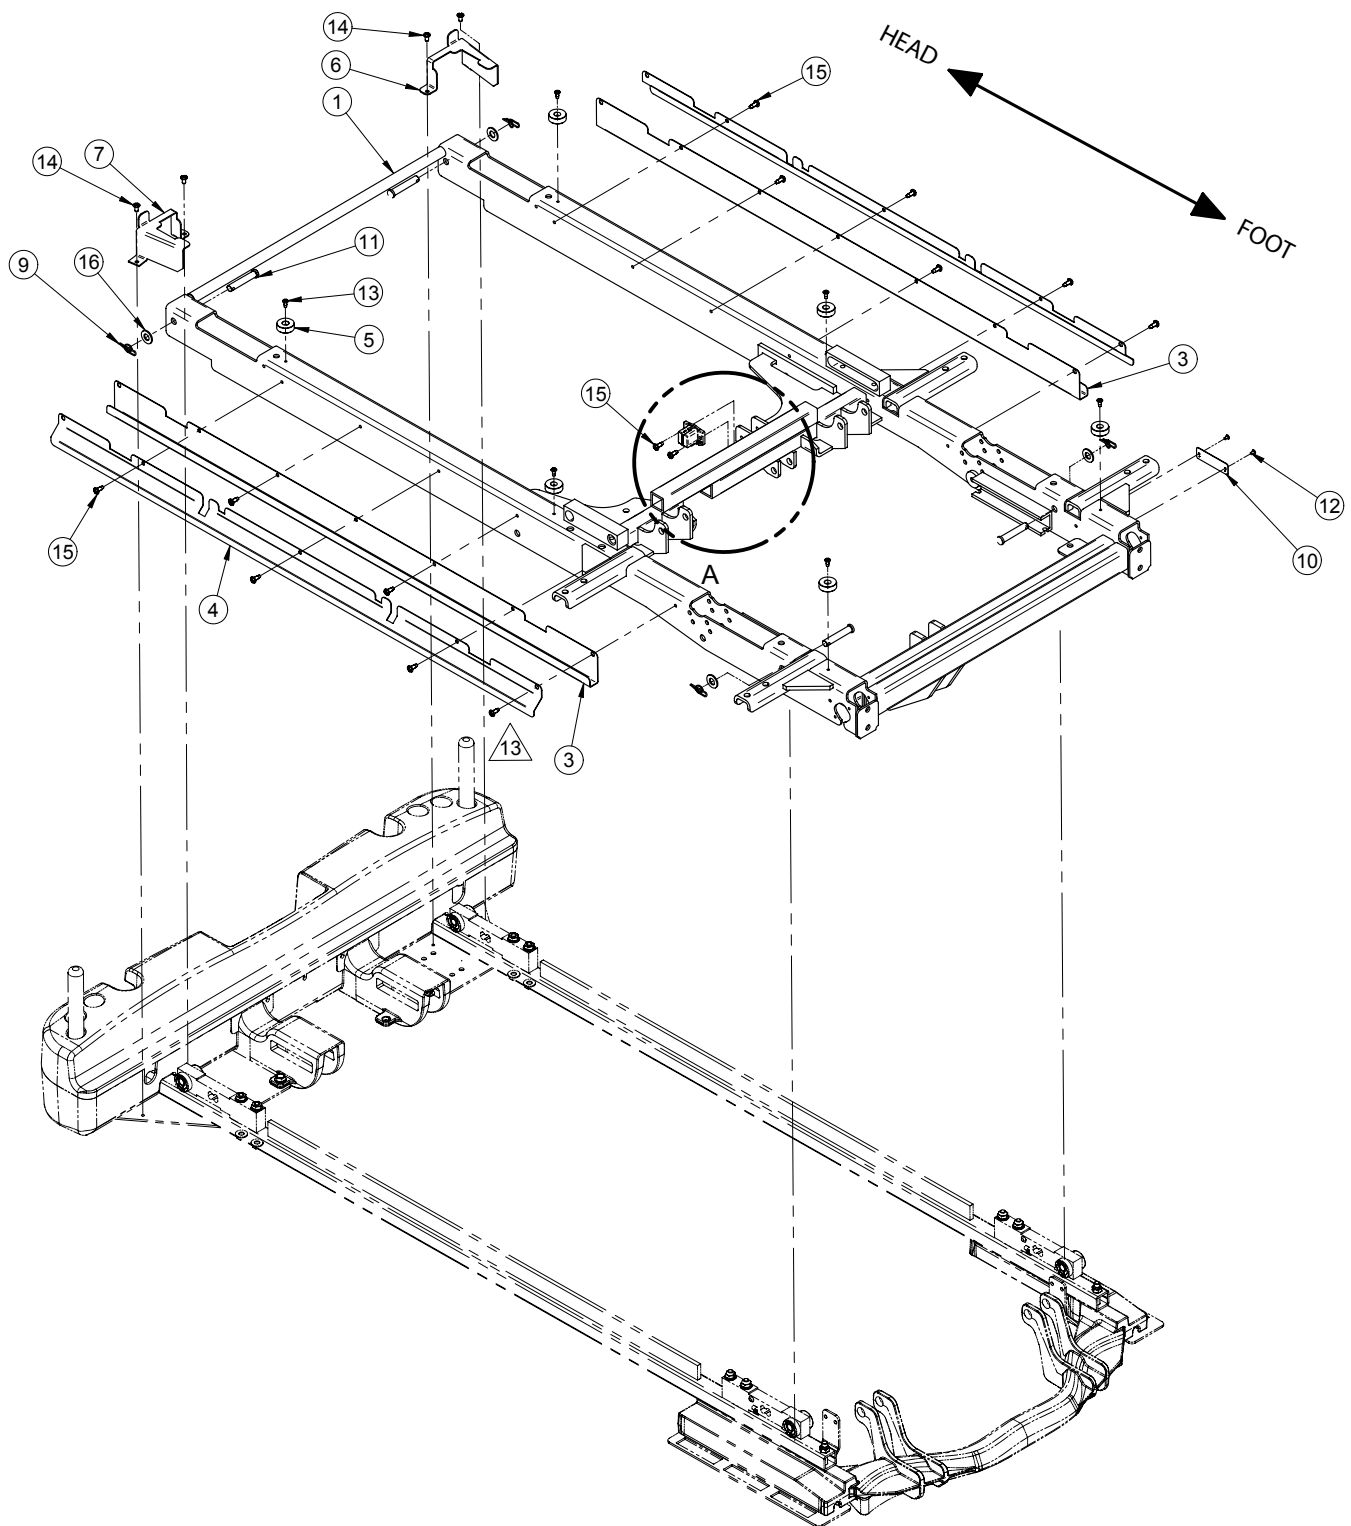

Litter Assembly, Upper Frame

(Applies to beds with Serial Numbers U01001 - U02817)

The orientation of this angle sensor is important. The wire must exit through the bottom.

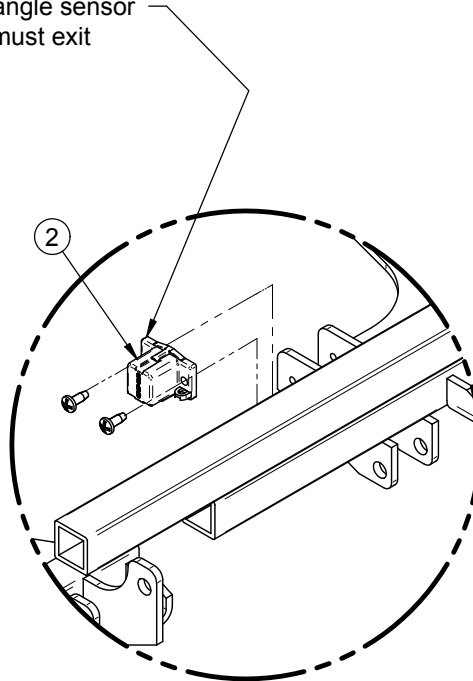

DETAIL A


Litter Assembly, Frame - L27-041 Rev-00 (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-0264W	Upper Frame	1
2	27-1209	Angle Sensor	1
3	27-1433W	Wire Channel	1
4	27-1434W	Wire Cover	2
5	27-1760	Stopper	6
6	27-1850W	Left Head Frame Wire Cover	1
7	27-1851W	Right Head Frame Wire Cover	1
9	QDF7878	Coupling Pin Diameter 3/8"	4
10	QE71-1181	Serial Number Plate	1
11	VG50B1248	Clevis Pin, Diameter 3/8" x 2"	4
12	VR11H43	Pop Rivet	2
13	VV83A9E12	Pan Head Tapping Screw, #8 x 3/8"	7
14	VV83A9G12	Pan Head Tapping Screw, #10 x 3/8"	4
15	VV83A9G16	Pan Head Tapping Screw, #10 x 1/2"	14
16	VW10A12	3/8" Washer	4

Litter Assembly, Upper Frame


(Applies to beds with Serial Numbers U02818 - Current)

L27-046 Rev-01 (Reference Only)

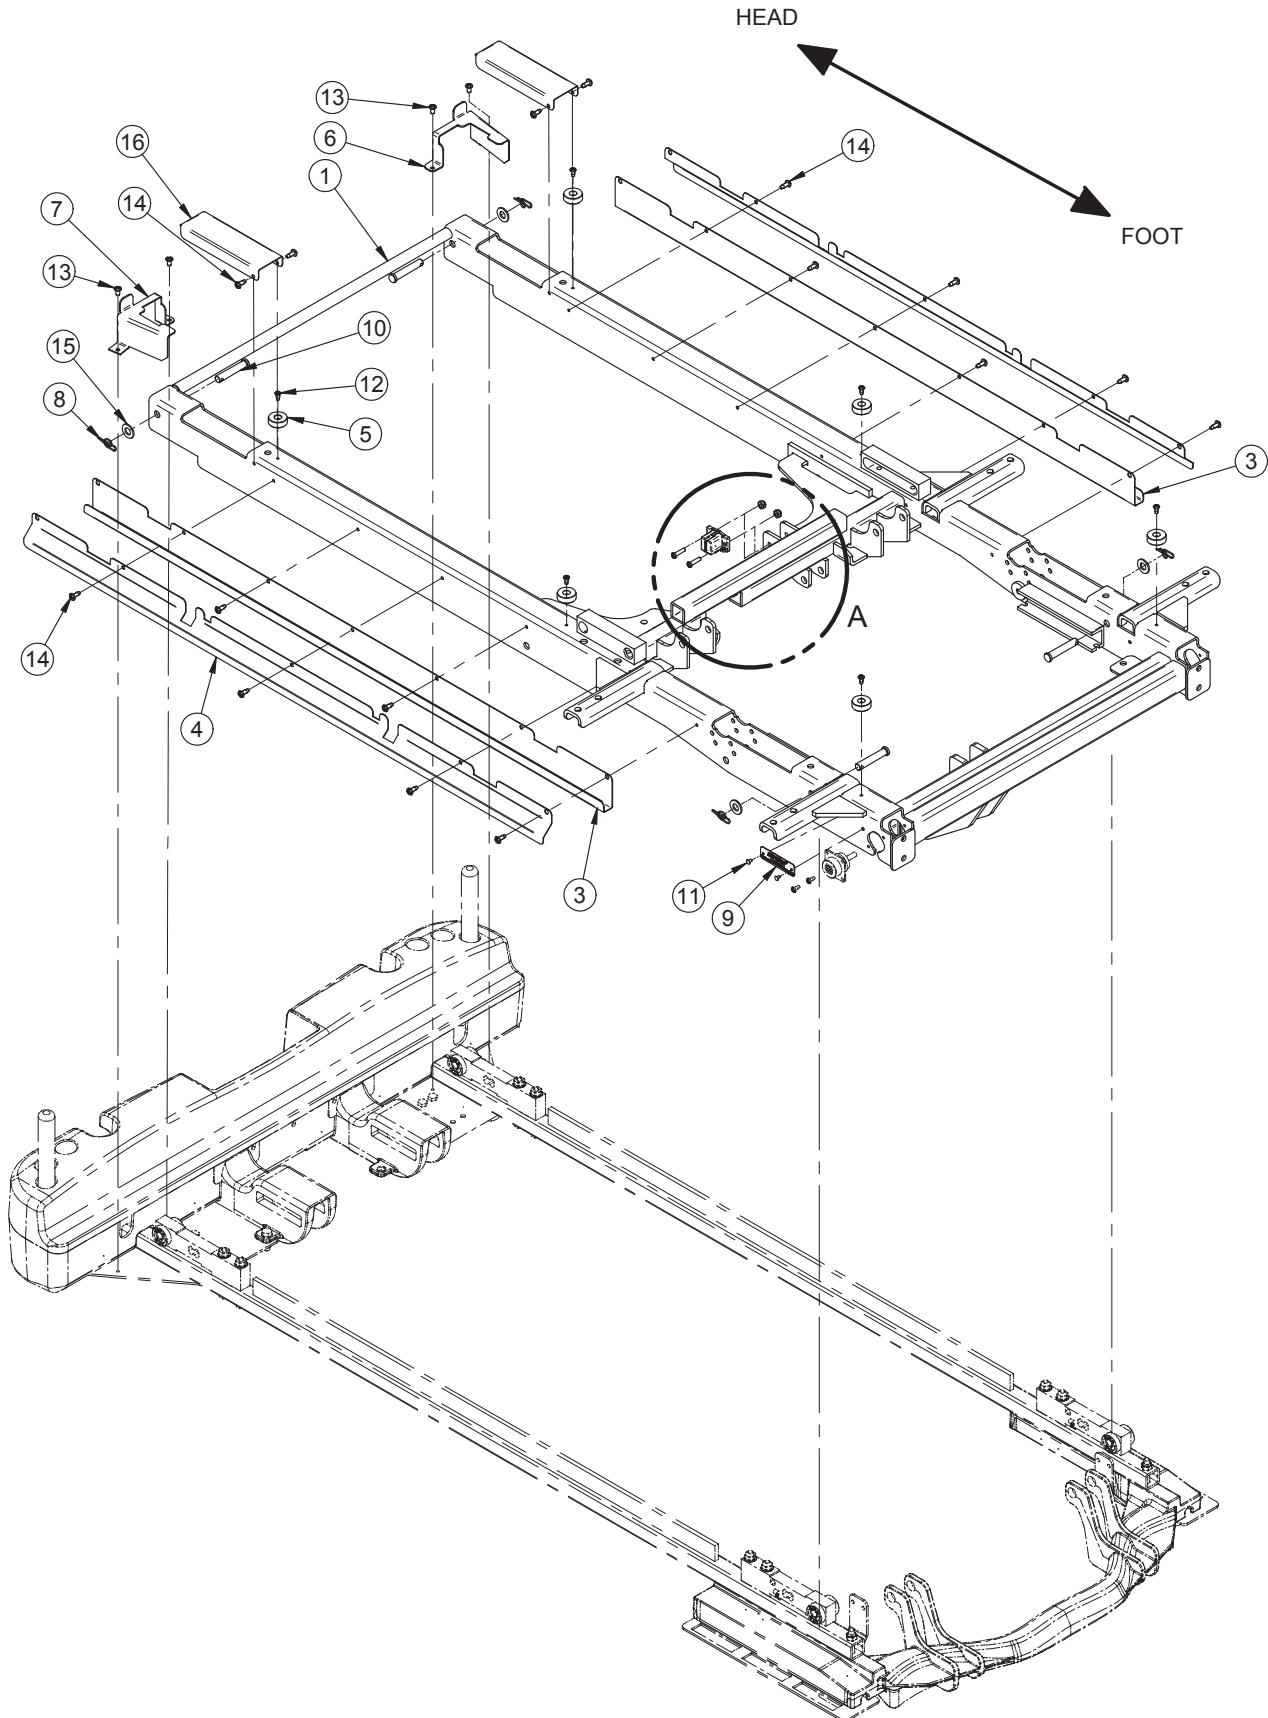

Litter Assembly, Upper Frame

(Applies to beds with Serial Numbers U02818 - Current)

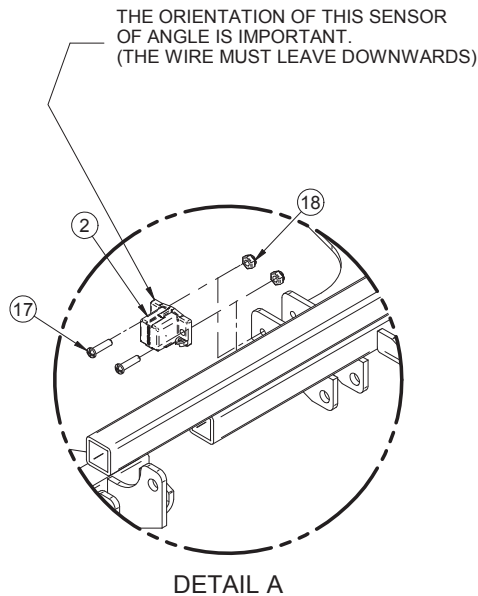


Litter Assembly, Upper Frame - L27-046 Rev-01 (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-2598P	Upper Frame	1
2	27-2477	Angle Sensor Assembly	1
3	27-1433P	Wire Channel	2
4	27-1434P	Wire Cover	2
5	QP27-1760	Stopper	6
6	27-1850P	Left Head Frame Wire Cover	1
7	27-1851P	Right Head Frame Wire Cover	1
8	QDF7878	Coupling Pin	4
9	QE71-1181	Serial Number Plate	1
10	VG50B1248	Clevis Pin	4
11	VR11H43	Pop Rivet	2
12	VV83A9E12	Pan Head Tapping Screw	6
13	VV83A9G12	Pan Head Tapping Screw	4
14	VV83A9G16	Pan Head Tapping Screw	16
15	VW10A12	Washer	4
16	27-2005P	Hiding place cell	2
17	VV33A0G24	Phillips Head Screw	2
18	VE30A0G	Nylon Nut	2

Litter Assembly, Foot End


(Applies to beds with Serial Numbers U01001 - U02817)

27-2260 Rev-00 (Reference Only)

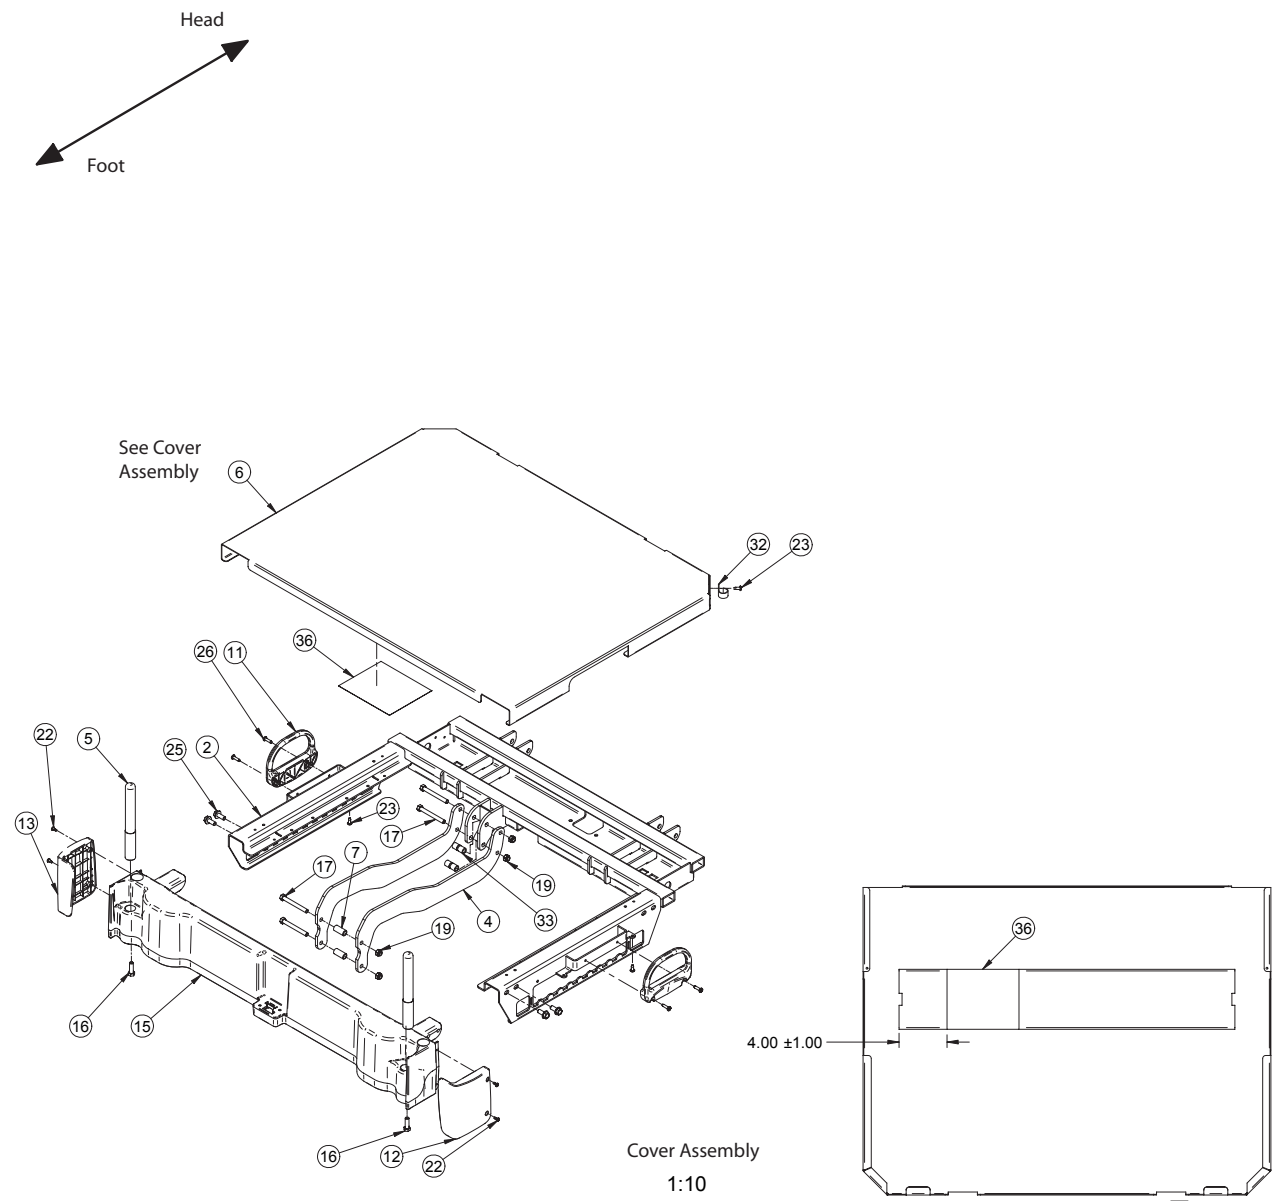


Litter Assembly, Foot End

(Applies to beds with Serial Numbers U01001 - U02817)

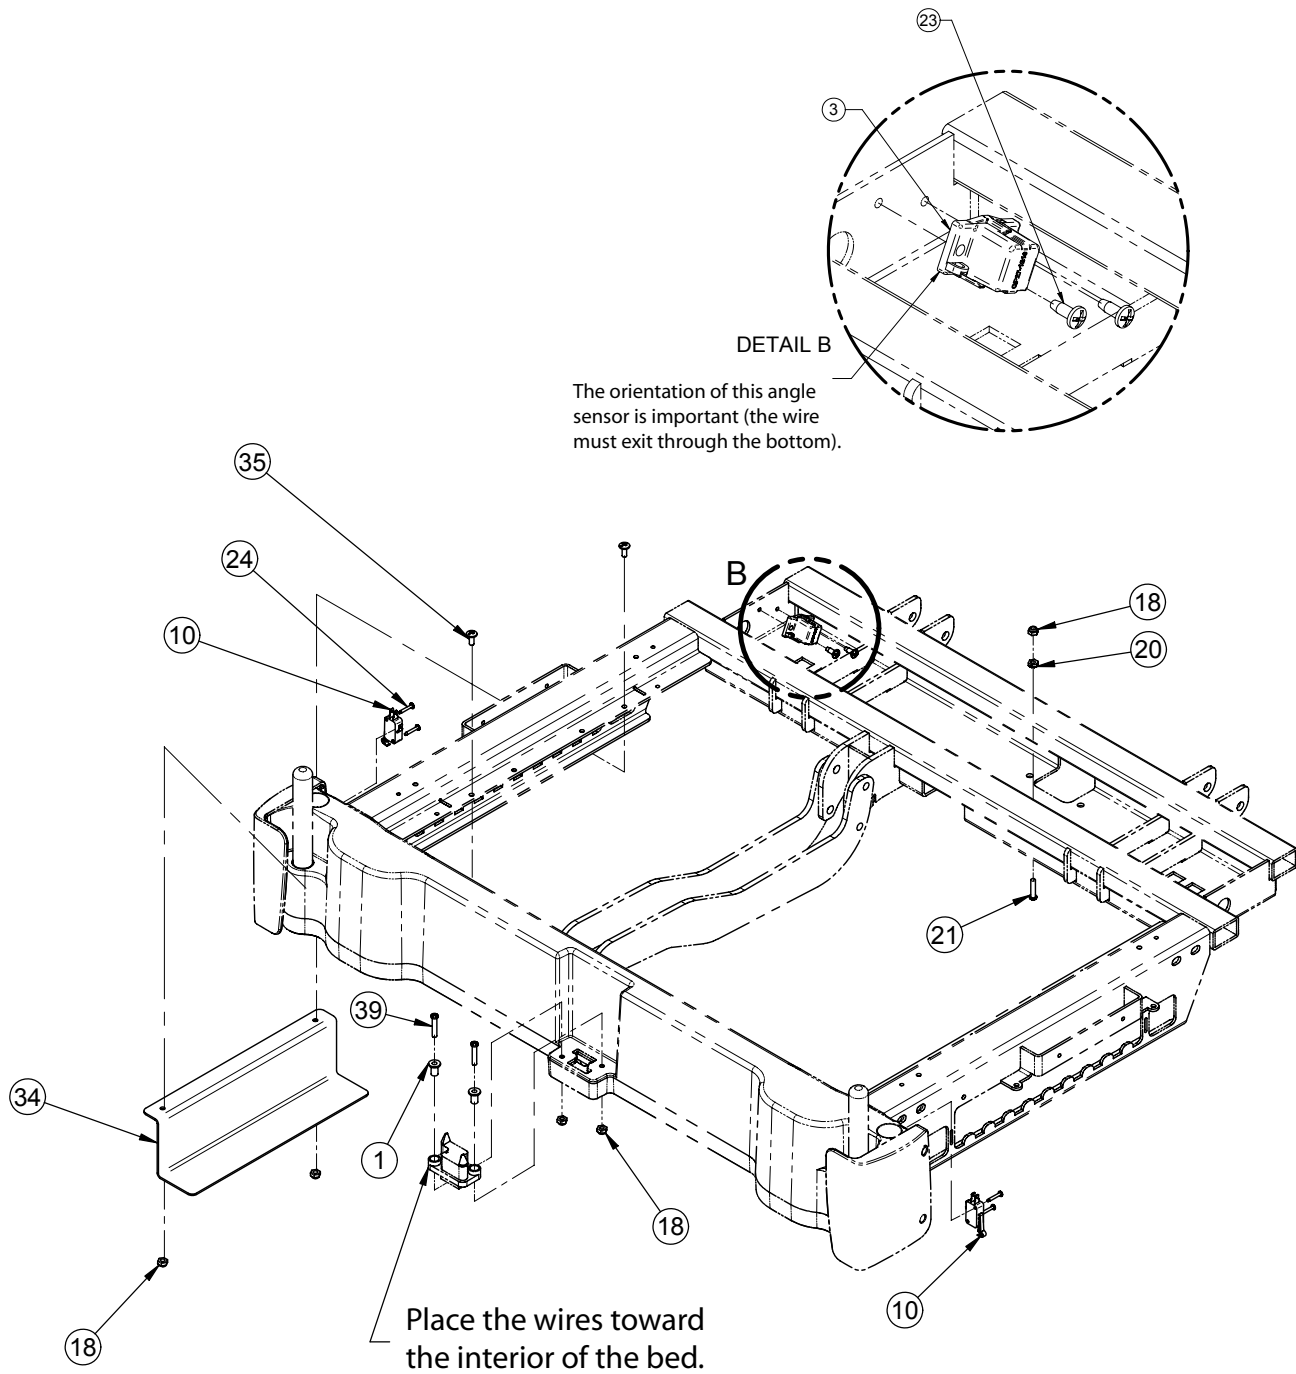


Litter Assembly, Foot End

(Applies to beds with Serial Numbers U01001 - U02817)

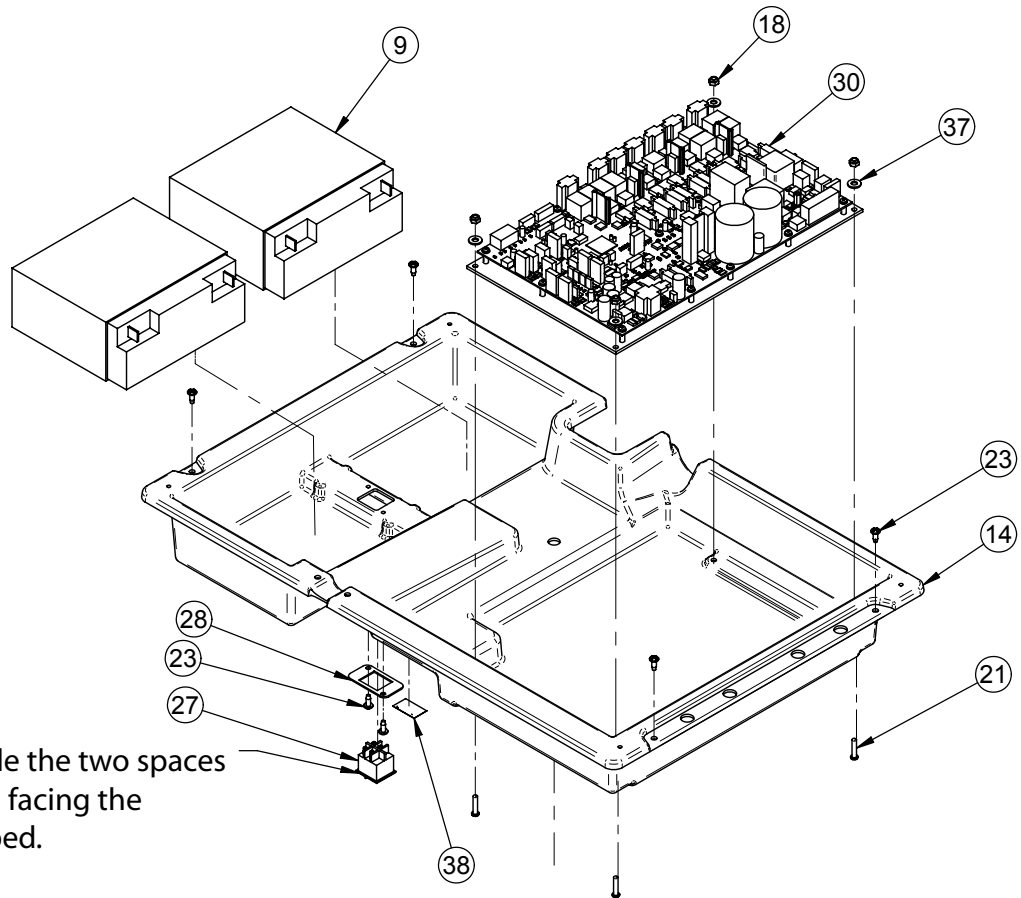

Always assemble the two spaces without the pin facing the interior of the bed.

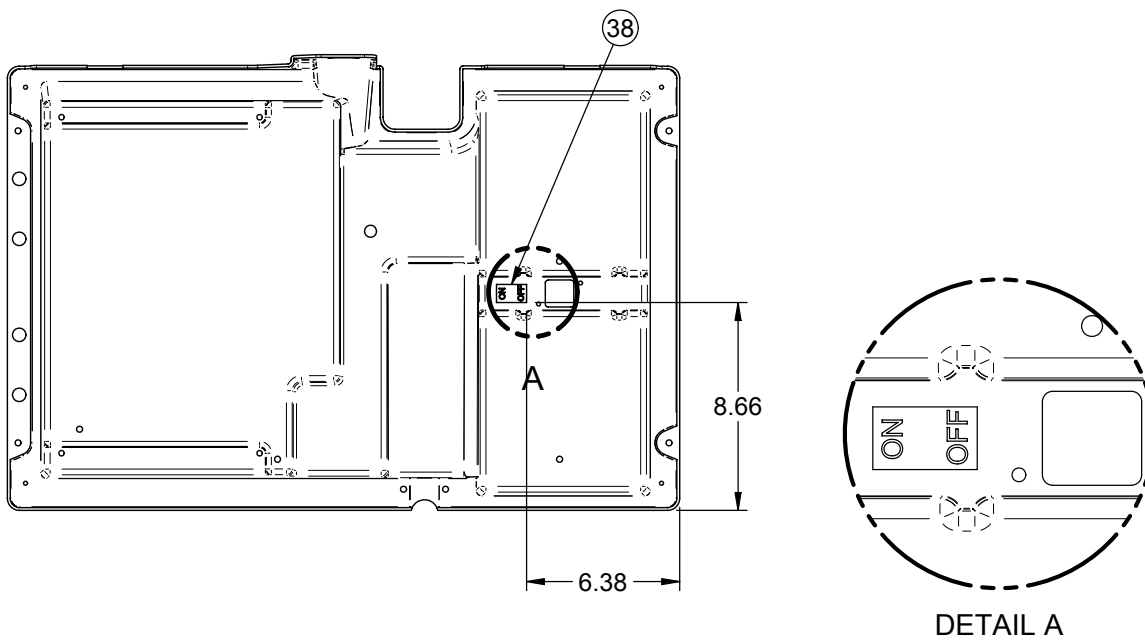

Litter Assembly, Foot End

(Applies to beds with Serial Numbers U01001 - U02817)


Litter Assembly, Foot End - 27-2260 Rev-00 (Reference Only)

Item	Part No.	Part Name	Qty.
1	25-0527Z	Connector's Sleeve	2
2	27-0112W	Foot Section	1
3	27-1209	Angle Sensor	1
4	27-1579W	Foot Litter Center Plate	2
5	27-1833C	Footboard Rod	2
6	27-1606W	Mattress Support	1
7	27-1710Z	Spacer	2
9	QDF9188	12V 18AH Battery	2
10	QDF9535	Micro Switch	2
11	QP27-1435-10	Mattress Stopper	2
12	QP27-1439-05	Left Foot Bumper	1
13	QP27-14405	Right Foot Bumper	1
14	QP27-1597	Molded Electronic Box	1
15	QPA27-1576W	Molded Foot Litter End	1
16	VB15A1O32-S	Scotch Grip Bolt	2
17	VB15A1O54	Full Thread Bolt	4
18	VE30A0G	Nylon Locknut	9
19	VE30A1O	Nylon Locknut	4
20	VE80A0G	Locknut	1
21	VV22A0G28	Phillips Machine Screw	5
22	VV83A9E12	Phillips Screw	4
23	VV83A9G16	Phillips Screw	11
24	VV87A9A24	Phillips Tapping Screw	4
25	VVB4A1024	Thread Rolling Bolt	4
26	VV83A9G24	Phillips Tapping Screw	4
27	QDF2089	Battery Switch	1
28	27-1972Z	Switch Support Plate	1
30	QDF75-0440	DC Control Board	1
32	QDF2091	Wiring Clip	1
33	27-2058Z	Spacer	2
34	27-1858W	Electronic Box Reinforcement	1
35	VV37A0G16	Phillips Machine Screw	2
36	QE71-1061	Battery Protection Sticker	1
37	VW10C081802	Nylon Washer	4
38	QE71-1042	ON-OFF Sticker	1
39	VV31A0G32	Phillips Machine Screw	2

Litter Assembly, Foot End


(Applies to beds with Serial Numbers U02818 - U04982)

27-2478 Rev-00 (Reference Only)

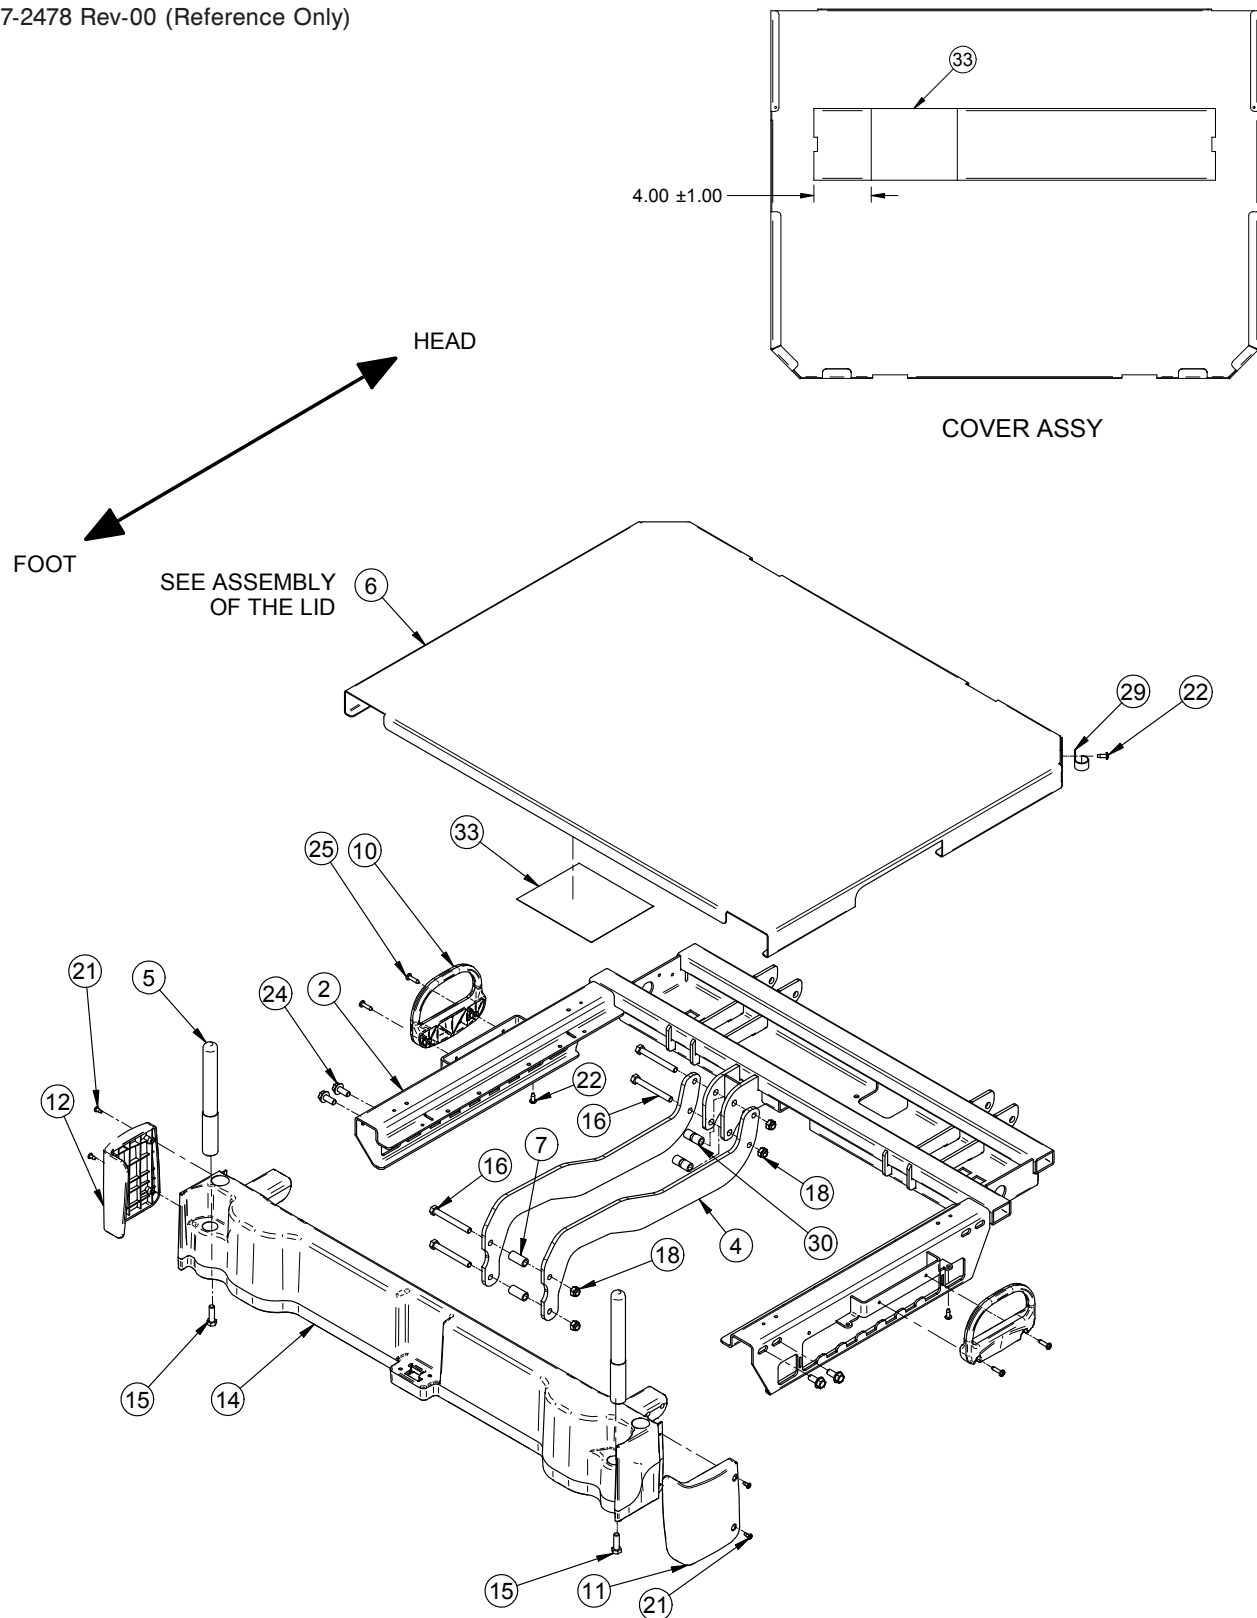


Litter Assembly, Foot End

(Applies to beds with Serial Numbers U02818 - U04982)

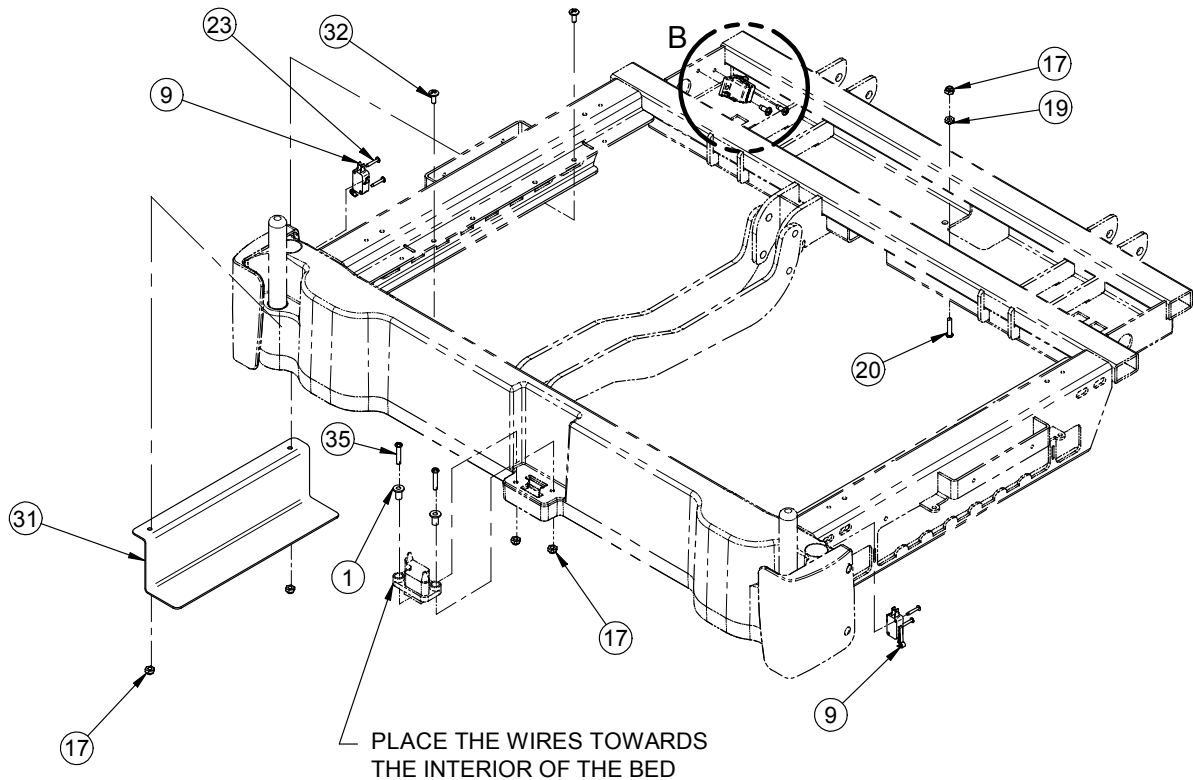


DETAIL B

THE ORIENTATION OF THIS SENSOR OF ANGLE IS IMPORTANT (THE WIRE MUST EXIT THROUGH THE BOTTOM)

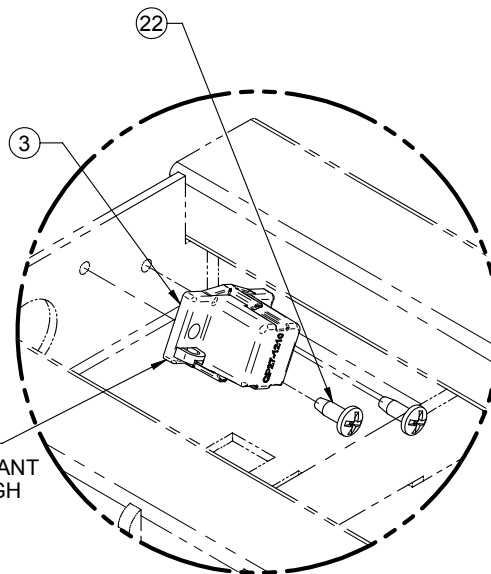

Litter Assembly, Foot End

(Applies to beds with Serial Numbers U02818 - U04982)

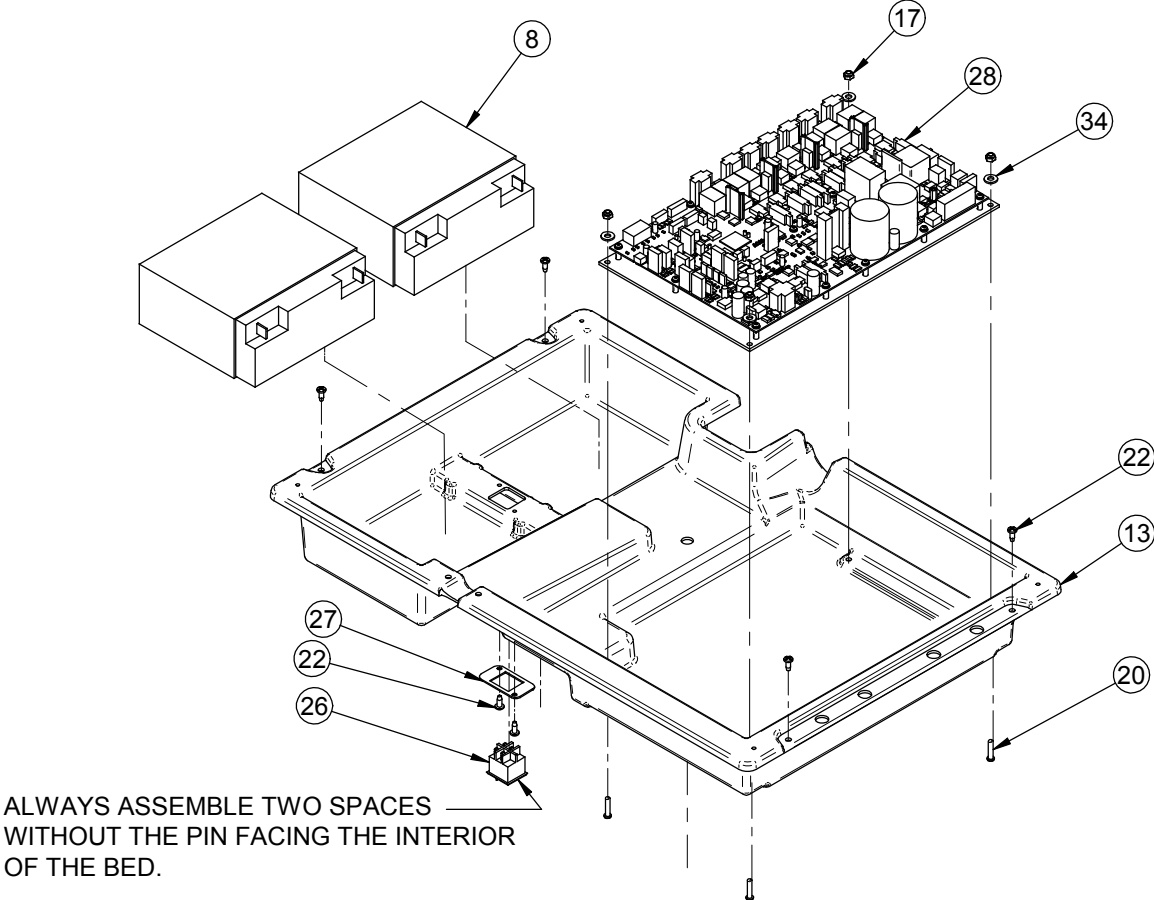

	SW1 ON / ON QDF75-0440			
	1	2	3	4
ON	Option with LBS	Option with <i>i</i> -Audio	Option with Zoom®	Option with <i>i</i> -Doc
OFF	Option without LBS	Option without <i>i</i> -Audio	Option without Zoom®	Option without <i>i</i> -Doc

Litter Assembly, Foot End

(Applies to beds with Serial Numbers U02818 - U04982)


Litter Assembly, Foot End - 27-2478 Rev-00 (Reference Only)

Item	Part No.	Part Name	Qty.
1	25-0527Z	Connector's Sleeve	2
2	27-0112W	Foot Section	1
3	27-2247	Angle Sensor	1
4	27-1579W	Foot Litter Center Plate	2
5	27-1833C	Footboard Rod	2
6	27-1606W	Mattress Support	1
7	27-1710Z	Spacer	2
8	QDF9188	12V 18AH Battery	2
9	QDF9535	Micro Switch	2
10	QP27-1435-10	Mattress Stopper	2
11	QP27-1439-05	Left Foot Bumper	1
12	QP27-1440-05	Right Foot Bumper	1
13	QP27-1597	Molded Electronic Box	1
14	QPA27-1576W	Molded Foot Litter End	1
15	VB15A1O32-S	Scotch Grip Bolt	2
16	VB15A1O54	Full Thread Bolt	4
17	VE30A0G	Nylon Locknut	9
18	VE30A1O	Nylon Locknut	4
19	VE80A0G	Locknut	1
20	VV22A0G28	Phillips Machine Screw	5
21	VV83A9E12	Phillips Screw	4
22	VV83A9G16	Phillips Screw	11
23	VV87A9A24	Phillips Tapping Screw	4
24	VVB4A1024	Thread Rolling Bolt	4
25	VV83A9G24	Phillips Tapping Screw	4
26	QDF2089	Battery Switch	1
27	27-1972Z	Switch Support Plate	1
28	QDF75-0440	DC Control Board	1
29	QDF2091	Wiring Clip	1
30	27-2058Z	Spacer	2
31	27-1858W	Electronic Box Reinforcement	1
32	VV37A0G16	Phillips Machine Screw	2
33	QE71-1061	Battery Protection Sticker	1
34	VW10C081802	Nylon Washer	4
35	VV31A0G32	Phillips Machine Screw	2

Litter Assembly, Foot End



(Applies to beds with Serial Numbers U04983 - U50240)

27-2708 Rev A (Reference Only)

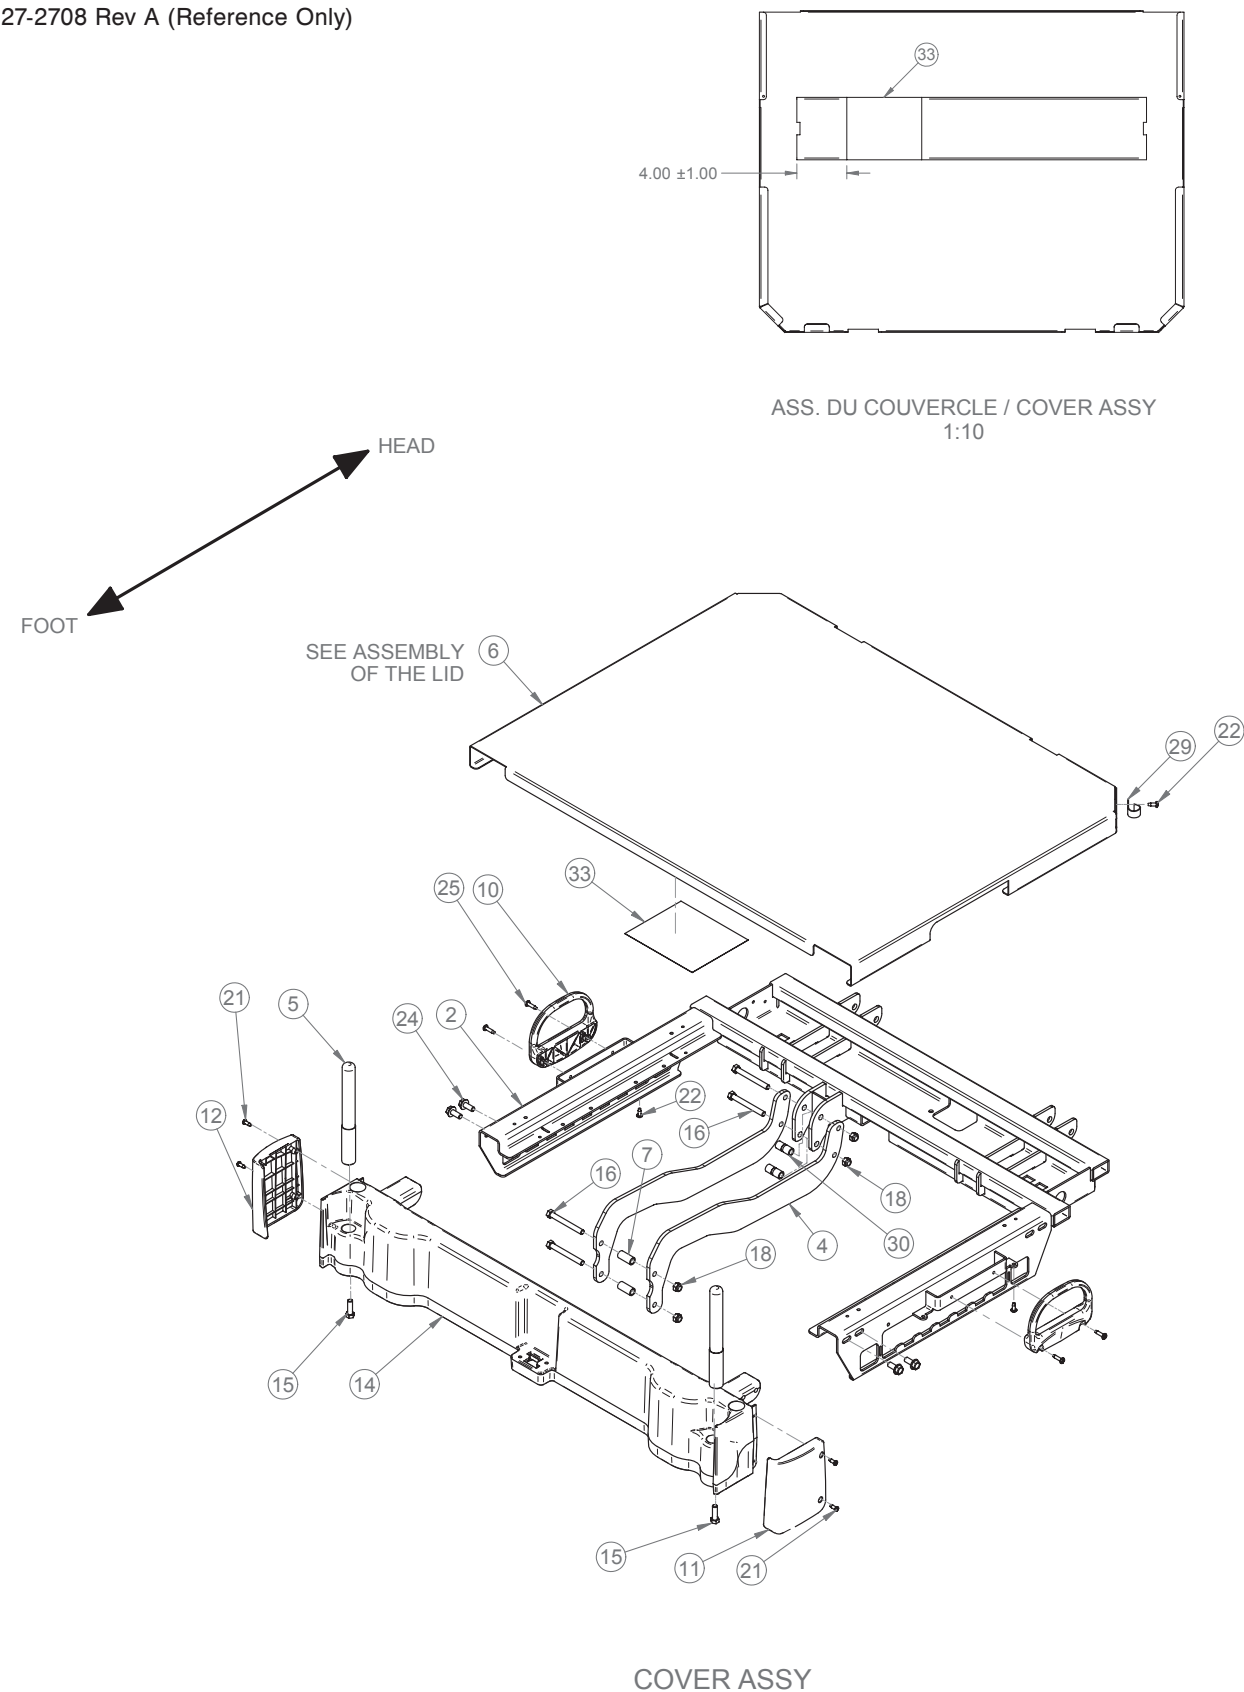


Litter Assembly, Foot End

(Applies to beds with Serial Numbers U04983 - U50240)

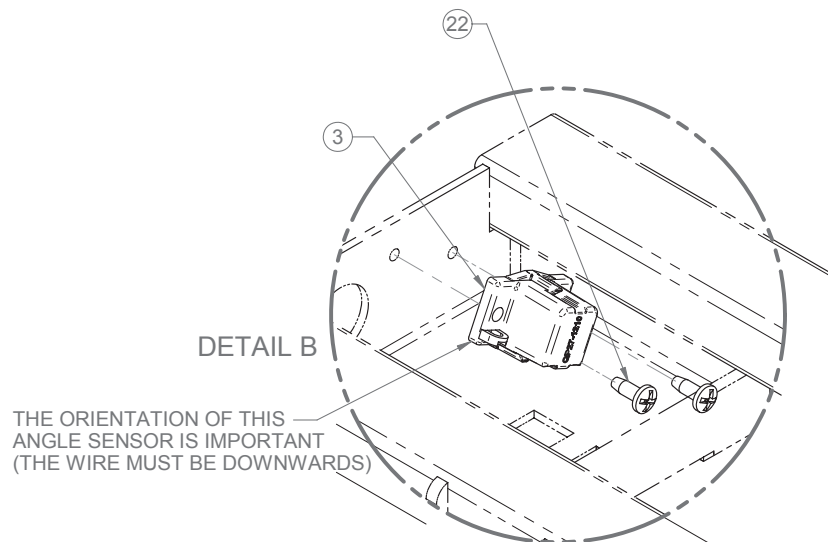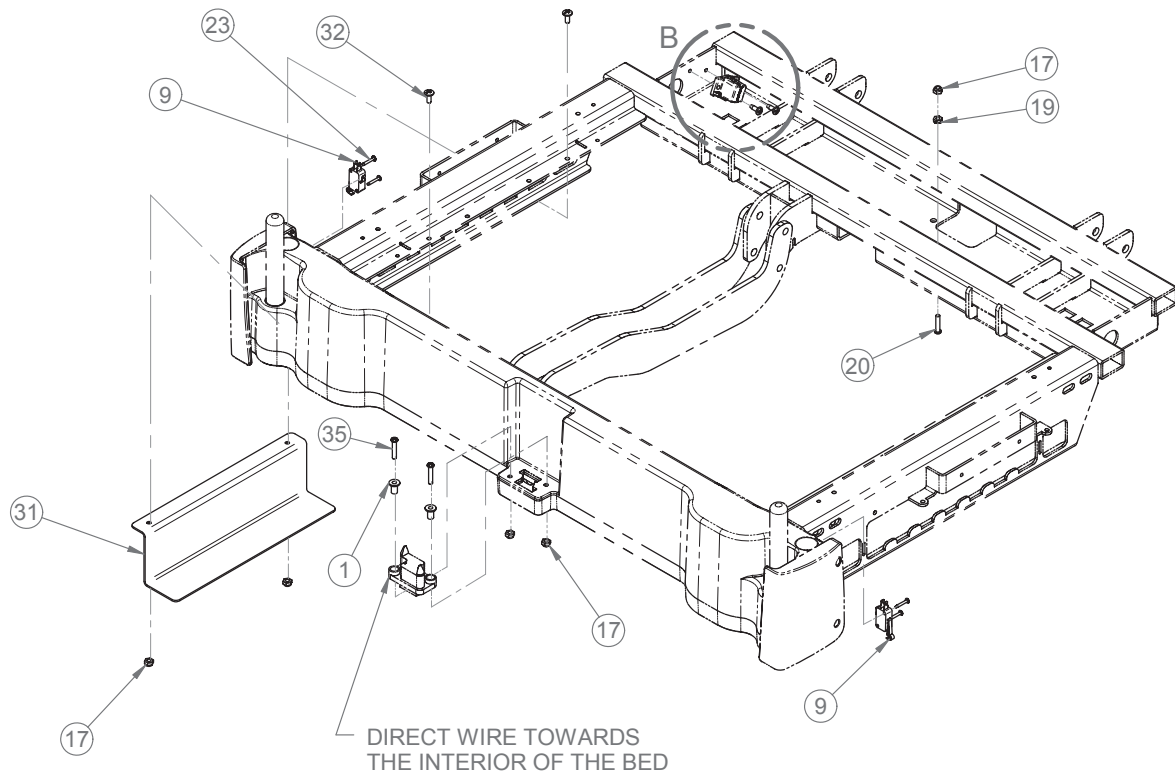

Litter Assembly, Foot End

(Applies to beds with Serial Numbers U04983 - U50240)

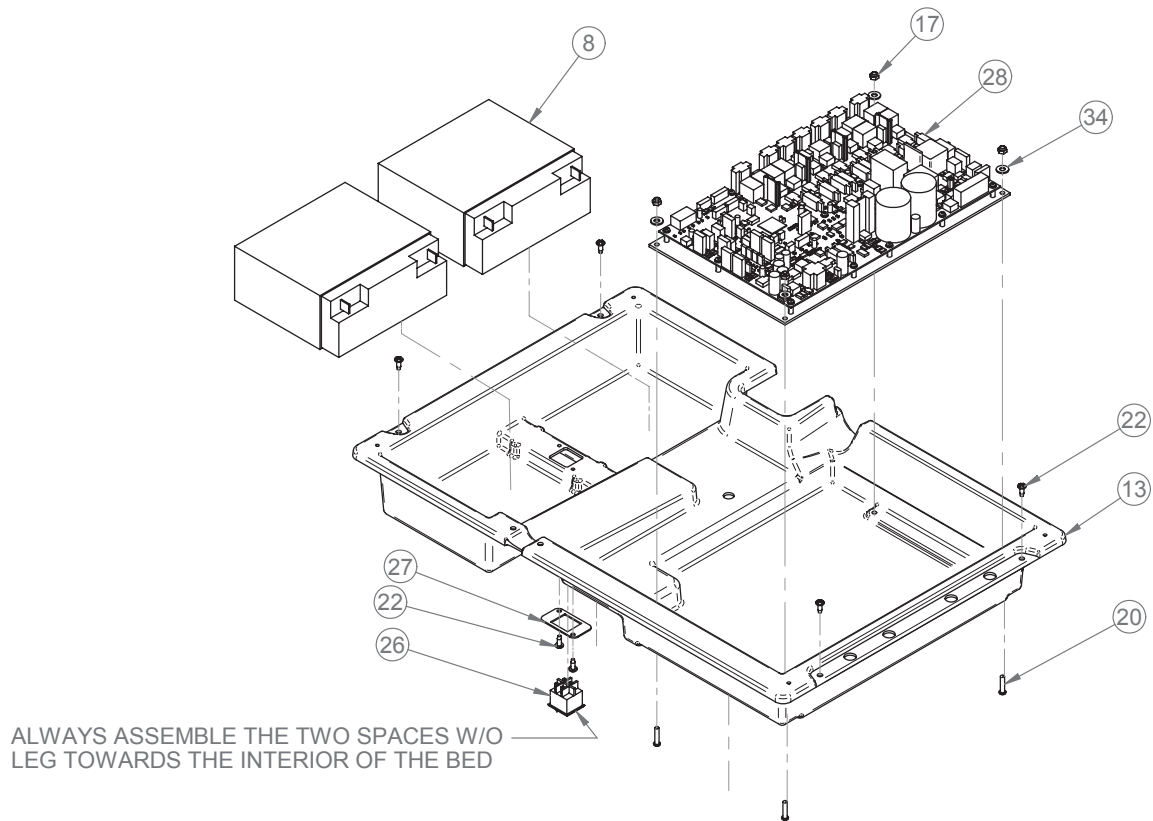

Litter Assembly, Foot End

(Applies to beds with Serial Numbers U04983 - U50240)


Litter Assembly, Foot End - 27-2708 Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	25-0527Z	Connector's Sleeve	2
2	27-0112P	Foot Section	1
3	27-2477	Angle Sensor	1
4	27-1579P	Foot Litter Center Plate	2
5	27-1833C	Footboard Rod	2
6	27-1606P	Mattress Support	1
7	27-1710Z	Spacer	2
8	QDF9188	12V 18AH Battery	2
9	QDF9535	Micro Switch	2
10	QP27-1435	Mattress Stopper	2
11	QP27-2644	Left Foot Bumper	1
12	QP27-2645	Right Foot Bumper	1
13	QP27-1597	Molded Electronic Box	1
14	QPA27-1576P	Molded Foot Litter End	1
15	VB15A1O32-S	Scotch Grip Bolt	2
16	VB15A1O54	Full Thread Bolt	4
17	VE30A0G	Nylon Locknut	9
18	VE30A1O	Nylon Locknut	4
19	VE80A0G	Locknut	1
20	VV33A0G28	Phillips Machine Screw	5
21	VV83A9E16	Phillips Screw	4
22	VV83A9G16	Phillips Screw	11
23	VV87A9A24	Phillips Tapping Screw	4
24	VVB4A1O24	Thread Rolling Bolt	4
25	VV83A9G24	Phillips Tapping Screw	4
26	QDF2089	Battery Switch	1
27	27-1972Z	Switch Support Plate	1
28	QDF75-0440	DC Control Board	1
29	QDF2091	Wiring Clip	1
30	27-2058Z	Spacer	2
31	27-1858P	Electronic Box Reinforcement	1
32	VV37A0G16	Phillips Machine Screw	2
33	QE71-1061	Battery Protection Sticker	1
34	VW10C081802	Nylon Washer	4
35	VV31A0G32	Phillips Machine Screw	2

Litter Assembly, Foot End


(Applies to beds with Serial Numbers U50241 - Current)

27-2688 Rev B (Reference Only)

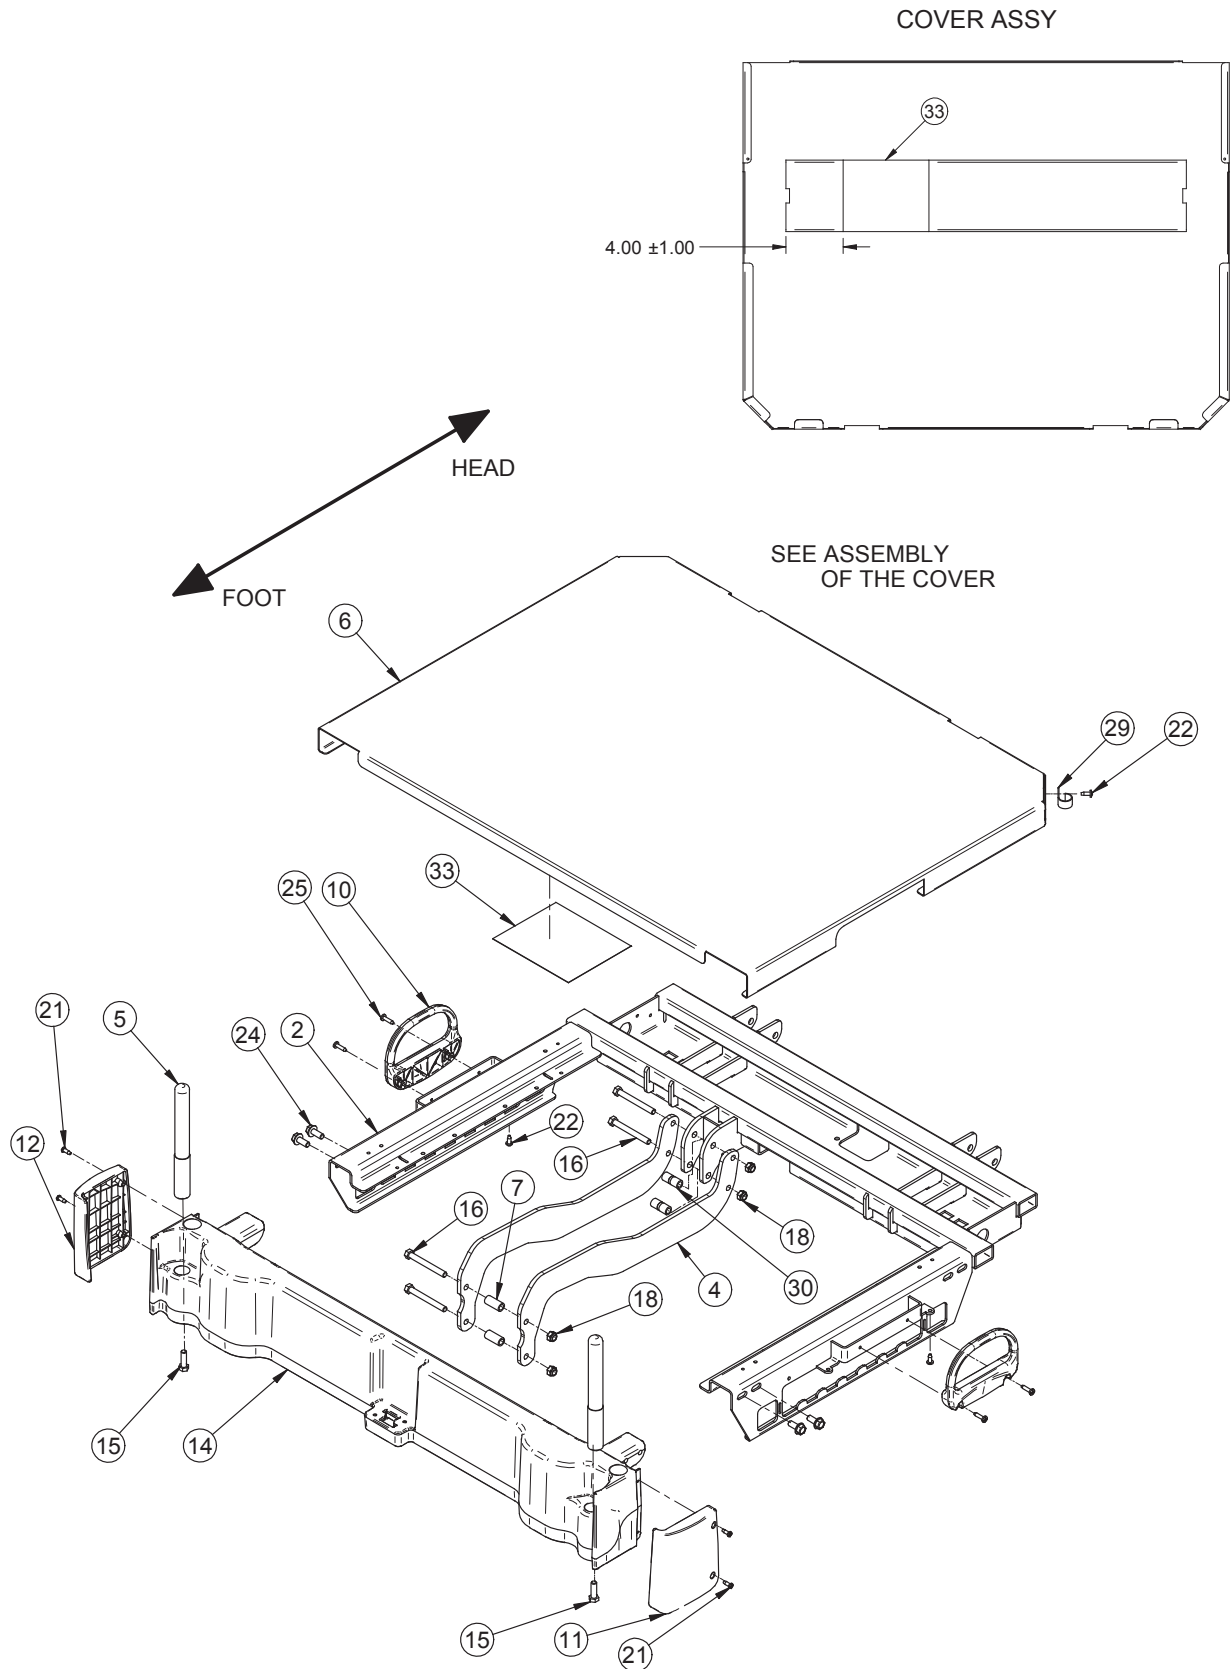


Litter Assembly, Foot End

(Applies to beds with Serial Numbers U50241 - Current)

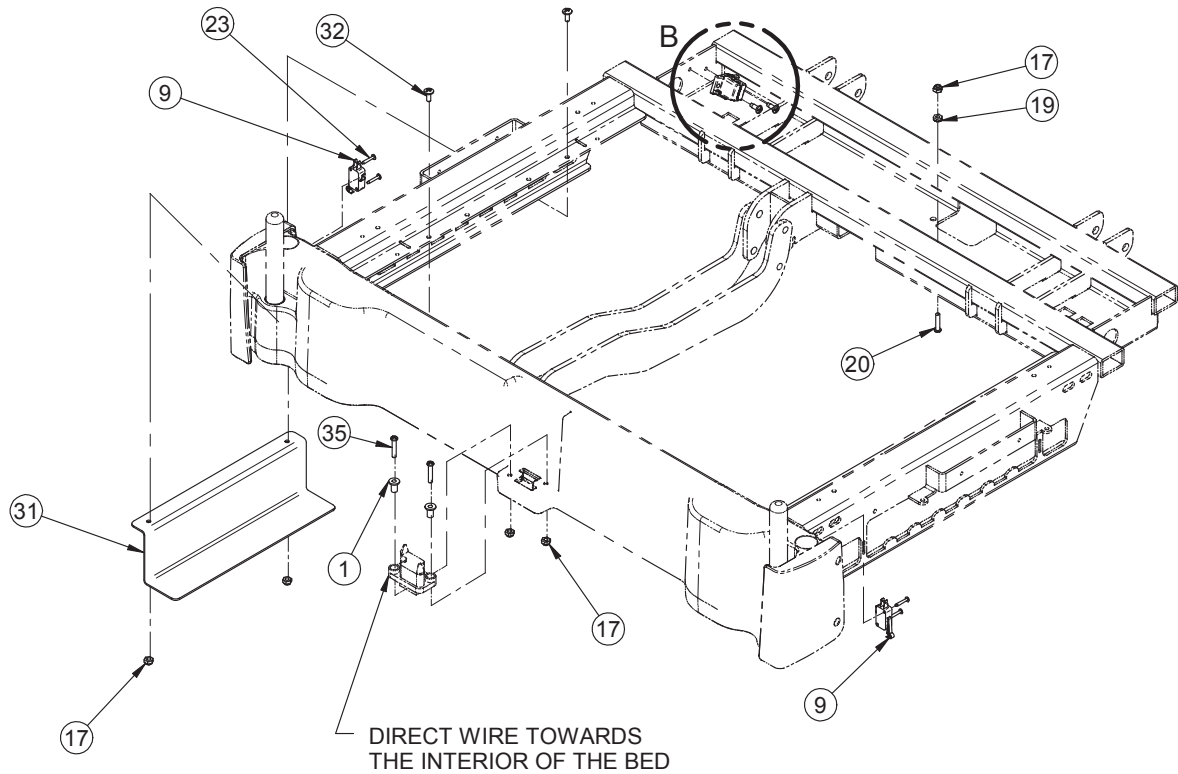


DETAIL B

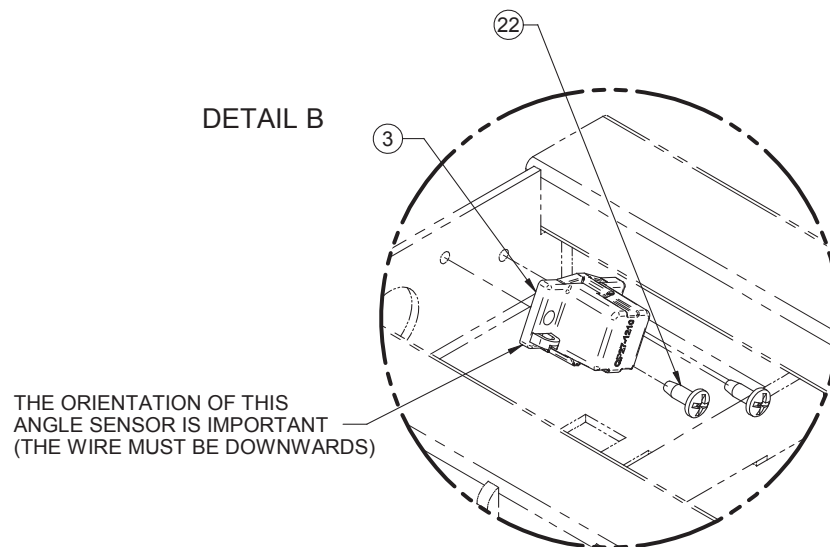

Litter Assembly, Foot End

(Applies to beds with Serial Numbers U50241 - Current)

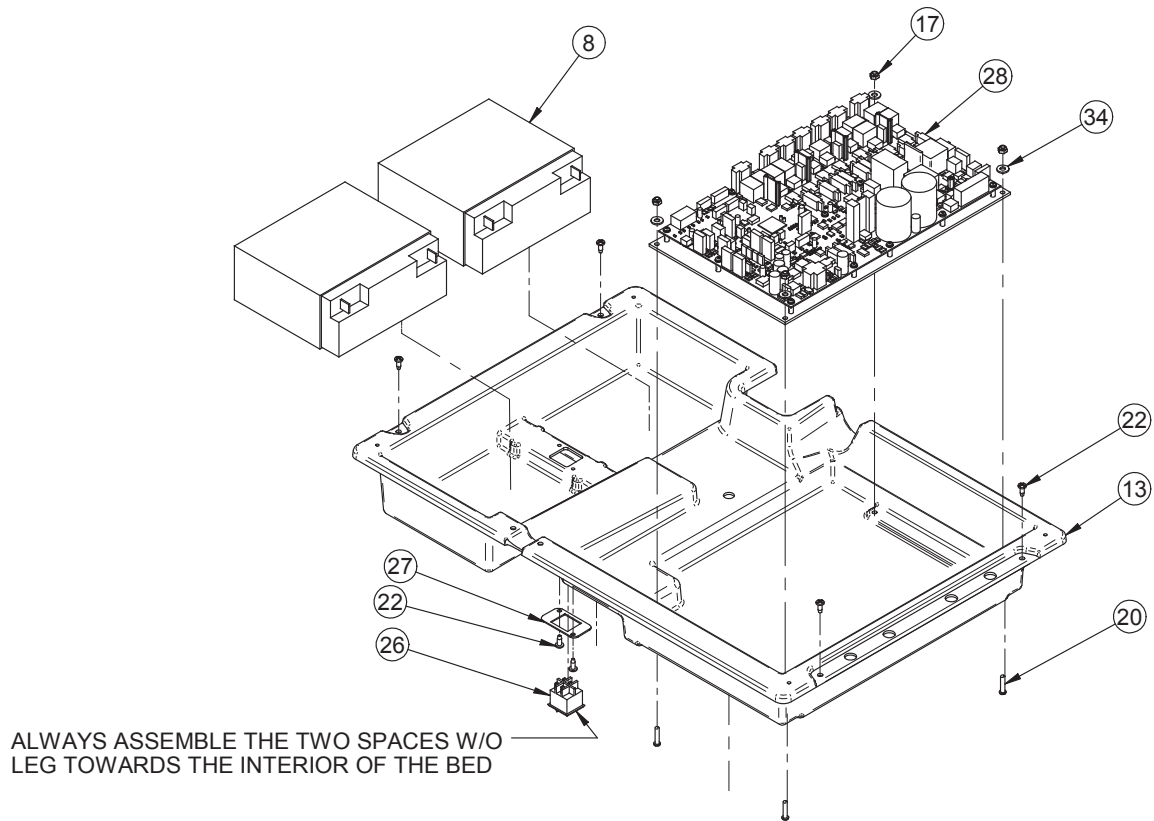

Litter Assembly, Foot End

(Applies to beds with Serial Numbers U50241 - Current)

Litter Assembly, Foot End - Common Components - 27-2688 Rev B (Reference Only)


Item	Part No.	Part Name	Qty.
1	25-0527Z	Connector's Sleeve	2
2	27-0112P	Foot Section	1
3	27-2477	Angle Sensor	1
4	27-1579W	Foot Litter Center Plate	2
5	27-1833C	Footboard Rod	2
6	27-1606W	Mattress Support	1
7	27-1710Z	Spacer	2
8	QDF9188	12V 18AH Battery	2
9	QDF9535	Micro Switch	2
10	QP27-1435-10	Mattress Stopper	2
11	QP27-2644	Left Foot Bumper	1
12	QP27-2645	Right Foot Bumper	1
13	QP27-1597	Molded Electronic Box	1
14	QPA27-1576-W	Molded Foot Litter End	1
15	VB15A1O32-S	Scotch Grip Bolt 5/16"-18 x 1"	2
16	VB15A1O54	"Full Thread" Bolt 5/16-18 x 2 3/4"	4
17	VE30A0G	Nylon Locknut #10-32	9
18	VE30A1O	Nylon Locknut 5/16"-18	4
19	VE80A0G	Locknut #10-32	1
20	VV33A0G28	Phillips Machine Screw 10-32 x 7/8"	5
21	VV83A9E16	Phillips Screw #8 x 3/8"	4
22	VV83A9G16	Phillips Screw #10 x 1/2"	11
23	VV87A9A24	Phillips Tapping Screw #4 x 3/4"	4
24	VVB4A1024	Thread Rolling Bolt 5/16-18 x 3/4"	4
25	VV83A9G24	Phillips Tapping Screw #10 x 3/4"	4
26	QDF2089	Battery Switch	1
27	27-1972Z	Switch Support Plate	1
28	QDF75-0440	DC Control Board	1
29	QDF2091	Wiring Clip	1
30	27-2058Z	Spacer	2
31	27-1858W	Electronic Box Reinforcement	1
32	VV37A0G16	Phillips Machine Screw 10-32 x 1/2"	2
33	QE71-1061	Battery Protection Sticker	1
34	VW10C081802	Nylon Washer, 9/16" x 1/16"	4
35	VV31A0G32	Phillips Machine Screw 10-32 x 1"	2

Litter Assembly, Standard Cabling

(Applies to beds with Serial Numbers U01001 - U03318)

(Excluding U03258 and U03259)

L27-037 Rev-00 (Reference Only)

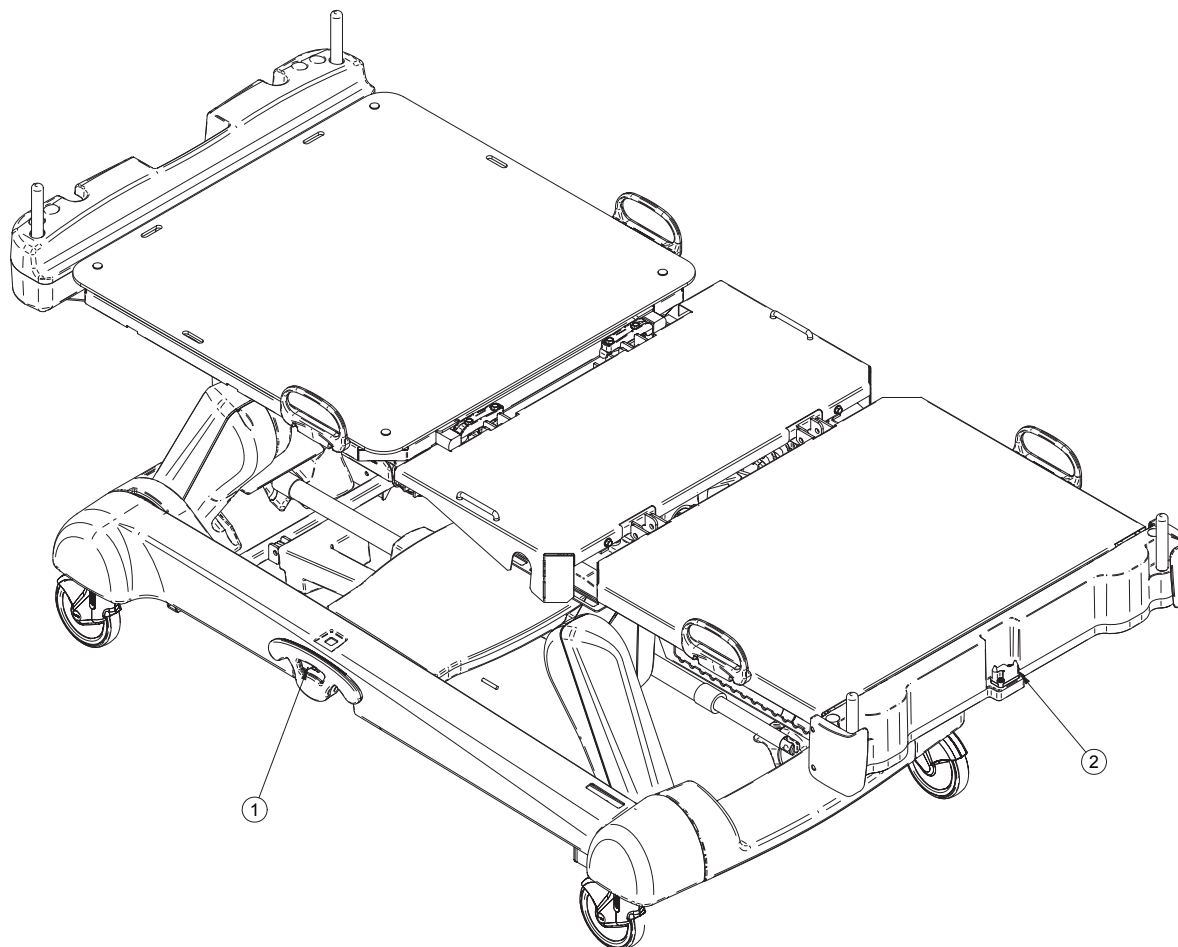


Item	Part No.	Part Name	Qty.
1	27-1660	Base and Lever Cabling	1
2	27-2256	Litter Cabling	1

Litter Assembly, Standard Cabling

(Applies to beds with Serial Numbers U03319 - U04982)
(Including U03258 and U03259)

L27-053 Rev-00 (Reference Only)

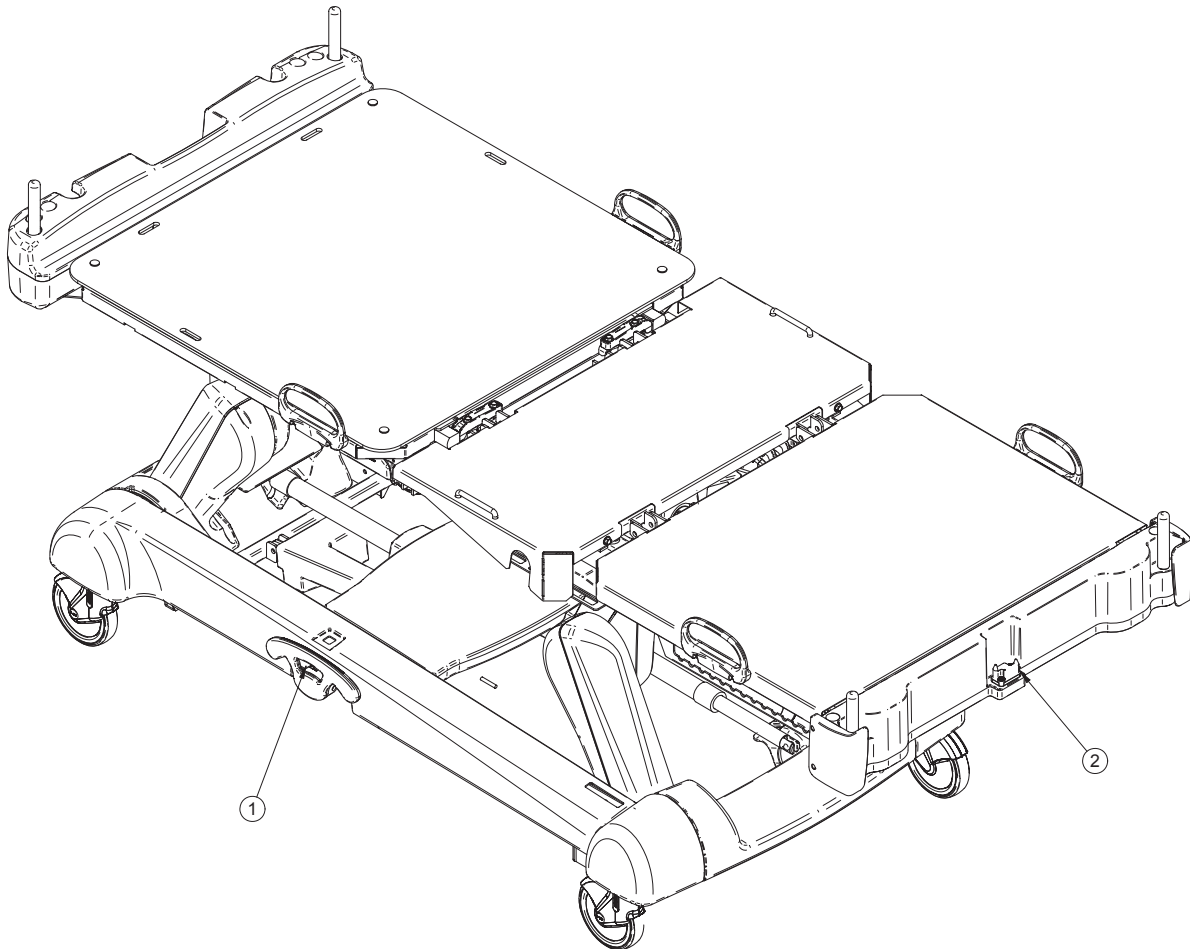


Item	Part No.	Part Name	Qty.
1	27-1660	Base and Lever Cabling	1
2	27-2559	Litter Cabling	1

Litter Assembly, Standard Cabling

(Applies to beds with Serial Numbers U04983 - Current)

L27-059 Rev B (Reference Only)

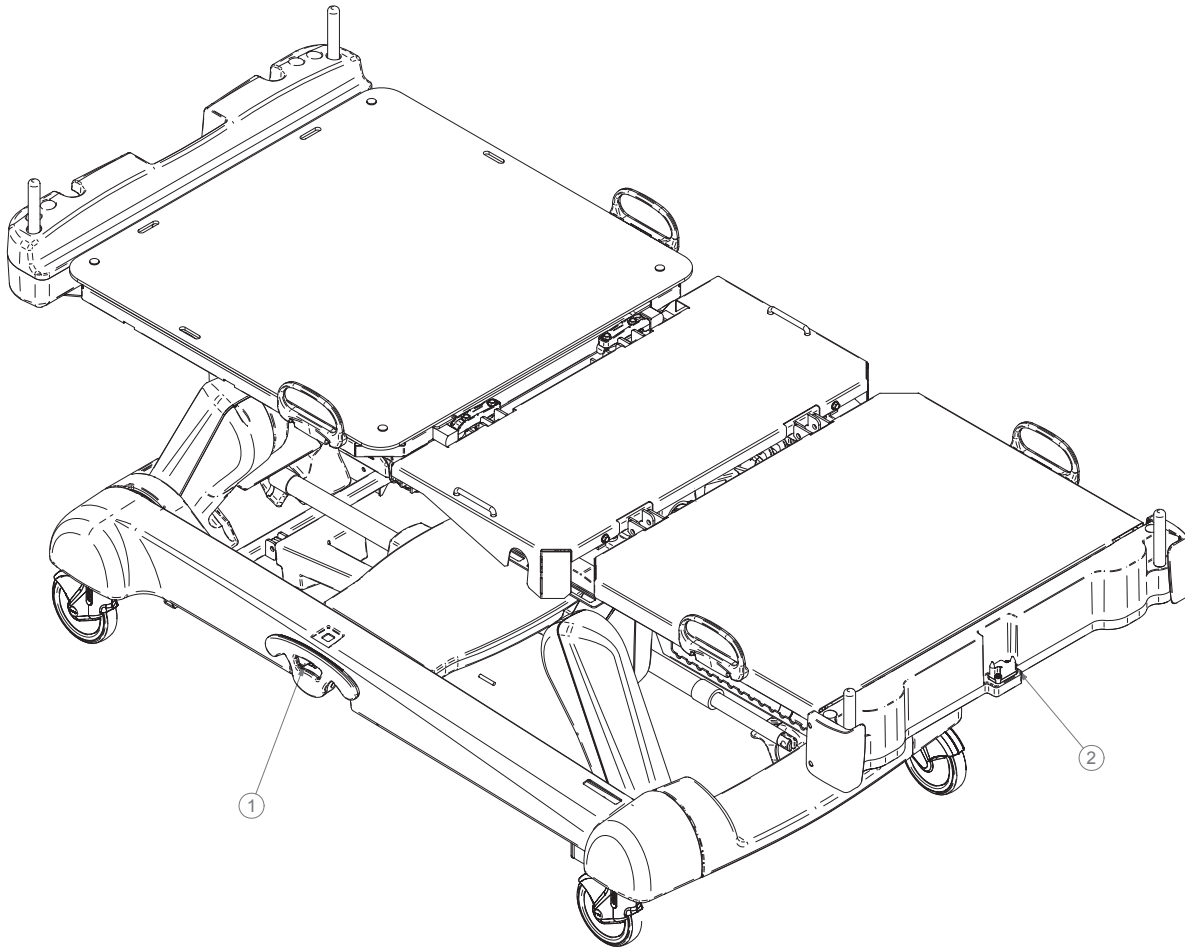


Item	Part No.	Part Name	Qty.
1	27-2687	Base and Lever Wiring	1
2	27-2695	Litter Wiring	1

***(Applies to beds with Serial Numbers U01001 - U03318)
(Excluding U03258 and U03259)***

Note: To avoid any binding risk when assembling these cables, the bed must be in high position.

- Fowler at 70 degrees
Knee Gatch at 15 degrees
Foot Litter at 45 degrees

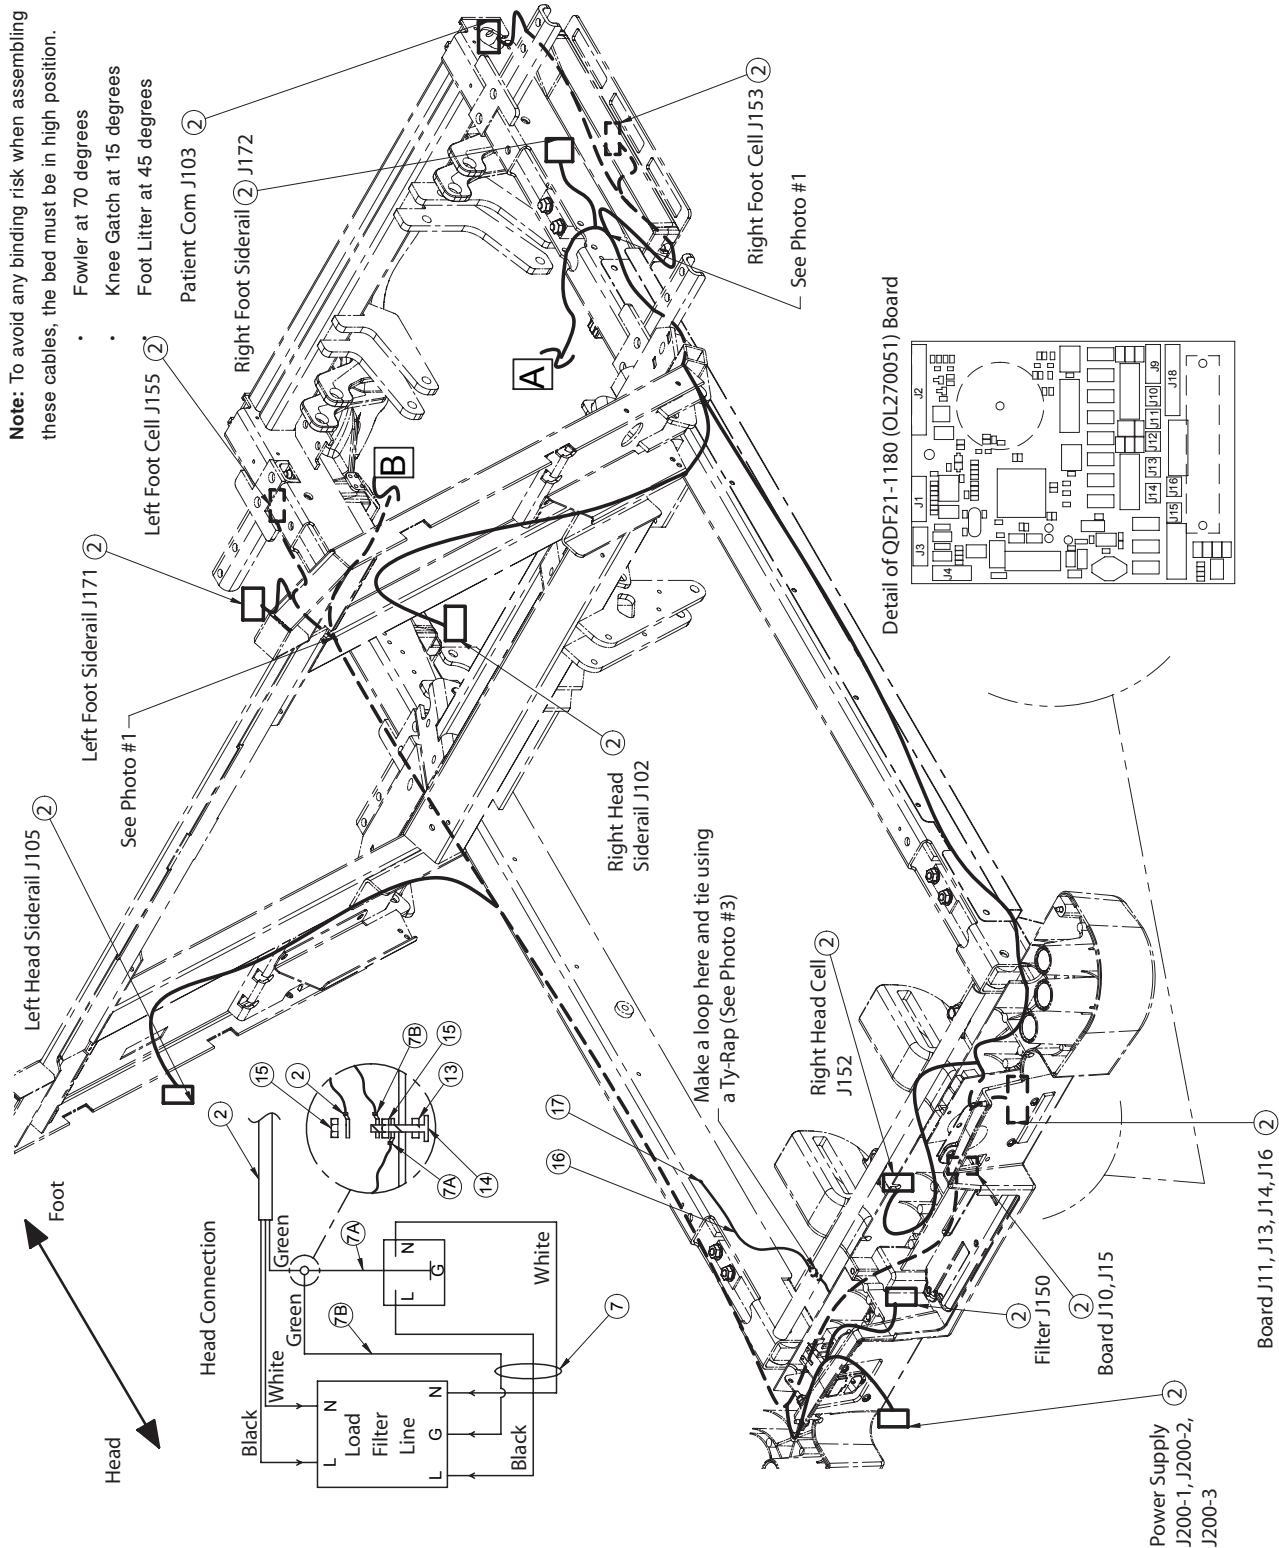

**(Applies to beds with Serial Numbers U01001 - U03318)
(Excluding U03258 and U03259)**



Litter Assembly, Electrical

*(Applies to beds with Serial Numbers U01001 - U03318)
(Excluding U03258 and U03259)*

Photo #1

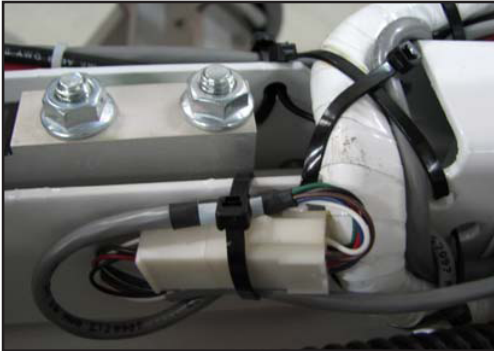



Photo #2



Photo #3



Photo #4

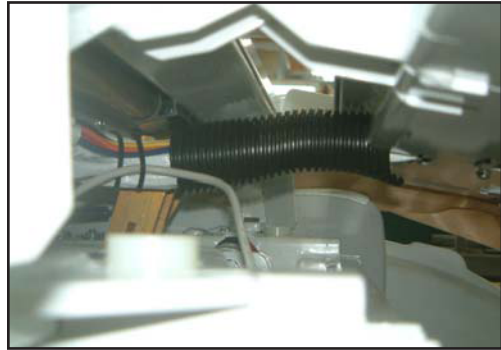

QDF27-1381 CABLES #1 CONNECTION TABLE

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1381	Red Grommet	To	QDF9188	Battery A Pole + (27-2260)
QDF27-1381	Terminal	To	QDF9188	Switch (27-2260)
QDF27-1381	Terminal	To	QDF9188	Switch (27-2260)

QDF27-2213 CABLES #2 CONNECTION TABLE

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2213	J22	To	QDF75-0440	J22 DC Board
QDF27-2213	J21	To	QDF75-0440	J21 DC Board
QDF27-2213	J20A	To	QDF75-0440	J20A DC Board
QDF27-2213	J20B	To	QDF75-0440	J20B DC Board
QDF27-2213	J20C	To	QDF75-0440	J20C DC Board

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U01001 - U03318)

(Excluding U03258 and U03259)

QDF27-2213 CABLES #2 CONNECTION TABLE				
QDF27-2213	J19	To	QDF75-0440	J19 DC Board
QDF27-2213	J29	To	QDF75-0440	J29 DC Board
QDF27-2213	J15A	To	QDF75-0440	J15A DC Board
QDF27-2213	J15B	To	QDF75-0440	J15B DC Board
QDF27-2213	J15C	To	QDF75-0440	J15C DC Board
QDF27-2213	J15D	To	QDF75-0440	J15D DC Board
QDF27-2213	J204	To	QDF27-2038	Transfo J204
QDF27-2213	J27	To	QDF75-0440	J27 DC Board
QDF27-2213	J3	To	QDF75-0440	J3 DC Board
QDF27-2213	J5	To	QDF75-0440	J5 DC Board
QDF27-2213	J113	To	QDF27-1209	Foot Sensor (27-2260)
QDF27-2213	J202	To	QDF75-0440	Gatch Ground
QDF27-2213	J114	To	QDF27-1209	Trend Sensor (L27-041)
QDF27-2213	J153	To	QDF27-1372	Right Foot Cell
QDF27-2213	J103	To	27-0264	Removable Control
(L27-041)	J103		27-0264	Removable Pendant (L27-041)
QDF27-2213	J172	To	QDF27-1208	Right Foot Siderail
QDF27-2213	J102	To	QDF27-2212	Right Head Siderail
QDF27-2213	J152	To	QDF27-1372	Right Head Cell
QDF27-2213	J202A	To	---	
QDF27-2213	J16	To	QDF75-0270	J16
QDF27-2213	J15	To	QDF75-0270	J15
QDF27-2213	J14	To	QDF75-0270	J14
QDF27-2213	J13	To	QDF75-0270	J13
QDF27-2213	J10	To	QDF75-0270	J10
QDF27-2213	J11	To	QDF75-0270	J11
QDF27-2213	J144	To	QDF27-1215	Gatch Motor (L27-038)
QDF27-2213	J142	To	QDF27-1214	Fowler Motor (L27-038)
QDF27-2213	J112	To	QDF27-1209	Fowler Sensor (L27-038)
QDF27-2213	J118	To	QDF27-1209	Gatch Sensor (L27-038)
QDF27-2213	J155	To	QDF27-1372	Left Foot Cell
QDF27-2213	J171	To	QDF27-1208	Left Foot Siderail
QDF27-2213	J105	To	QDF27-2212	Left Head Siderail
QDF27-2213	J150	To	QDF27-1372	Left Head Cell
QDF27-2213	J23	To	QDF75-0440	J23 DC Board
QDF27-2213	J26	To	QDF75-0440	J26 DC Board
QDF27-2213	J200A Black	To	Line "L" (Filter L27-014)	
QDF27-2213	J200B White	To	Line "N" (Filter L27-014)	
QDF27-2213	J200C Green	To		Head Screw (L27-014)

Litter Assembly, Electrical

***(Applies to beds with Serial Numbers U01001 - U03318)
(Excluding U03258 and U03259)***

QDF27-1607 CABLES #3 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1607	Con. MTA 5 Pos.	To	QDF75-0440	J25 DC Board
QDF27-1607	Contact	To	QDF27-2214	Contact 7 or 8
QDF27-1607	Contact	To	QDF27-2214	Contact 7 or 8
QDF27-1607	Terminal	To	QDF9535	Right Limit Switch (27-2260) No/Com
QDF27-1607	Terminal	To	QDF9535	Right Limit Switch (27-2260) Com/No
QDF27-1607	Terminal	To	QDF9535	Left Limit Switch (27-2260) No/Com
QDF27-1607	Terminal	To	QDF9535	Left Limit Switch (27-2260) Com/No

QDF27-1646 CABLES #4 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1646	Mini Fit	To	QDF75-0440	J12 DC Board
QDF27-1646	Black Grommet	To	QDF9188	Battery B Pole + (27-2260)
QDF27-1646	White Grommet	To	QDF9188	Battery A Pole – (27-2260)

QDF5095 CABLES #5 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF5095	Con. MTA	To	QDF75-0440	J13 DC Board
QDF5095	Buzzer	To	Electrical Box	See Position on Drawing

QDF27-1524 CABLES #7 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1524	Black 90° Terminal	To	QDF9571	Line “L” (Filter L27-014)
QDF27-1524	White 90° Terminal	To	QDF9571	Line “N” (Filter L27-014)
QDF27-1524	Green 90° Terminal	To	QDF9571	Line “E” (Filter L27-014)
QDF27-1524	Black Right Terminal	To	QDF9574	“L” (Power Supply L27-014)
QDF27-1524	White Right Terminal	To	QDF9574	“N” (Power Supply L27-014)
QDF27-1524	Green Right Terminal	To	QDF9574	“E” (Power Supply L27-014)
QDF27-1524	Cross Grommet	To	Head Ground	Screw (L27-014)
QDF27-1524	Cross Grommet	To	Head Ground	Screw (L27-014)

QDF27-1214 CABLES #10 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2214	Con. MTA 6 Pos.	To	QDF75-0440	J18 DC Board
QDF27-2214	Con. Metrimate	To	27-1547	Panel (27-1547)

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U01001 - U03318)
(Excluding U03258 and U03259)

QDF27-2228 CABLES #11 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2228	J205	To	QDF27-2038	Transfo (L27-038)
QDF27-2228	J202 Grommet	To	---	Foot Litter Ground
QDF27-2228	J208AL (Black)	To	QDF9573	Single Outlet (27-2260)
QDF27-2228	J207 Terminal	To	QDF9025	Breaker (27-2260)
QDF27-2228	J206 Terminal	To	QDF9025	Breaker (27-2260)
QDF27-2228	J208AN (White)	To	QDF9573	Outlet (27-2260) White
QDF27-2228	J208AG (Green/Yellow)	To	QDF9573	Outlet (27-2260) Ground

QDF27-2025 CABLES #12 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2025	Light	To	QDF75-0440	J20 DC Board


Litter Assembly, Cabling - Common Components - 27-2256 Rev-00 (Reference Only)

Item	Part No.	Part Name	Qty.
1*	QDF27-1381	Battery Switch Wire	2
2*	QDF27-2213	#1 Wire Harness	1
3*	QDF27-1607	I.V. Pole and Bed Extender Cable	1
4*	QDF27-1646	Battery Wires	1
5*	QDF5095	Buzzer	1
6*	QDF9518	Cable Tie	51
7*	QDF27-1524	Filter and Receiver Connector	1
10*	QDF27-2214	Panel – Control Board Cable	1
11*	QDF27-2228	Auxiliary 120V Outlet Cable without Mattress Connector	1
12*	QDF27-2025	12V Night Light	1
13*	VW20A76	Locking Washer	3
14*	VV33A0G28	Phillips Machine Screw #10-32 x 7/8"	3
15*	VE30A0G	Nylon Locknut #10-32	6
16*	QDF17-0138	Electronic Board Ground Wire	1
17*	VV83A9G12	Phillips Screw 10 x 3/8"	1
18	QDF2115	1.25 Split Loom Polyethylene	1

**(Applies to beds with Serial Numbers U03319 - U04982)
(Including U03258 and U03259)**

Note: To avoid any binding risk when assembling these cables, the bed must be in high position.

- Fowler at 70 degrees
- Knee Gatch at 15 degrees
- Foot Litter at 45 degrees

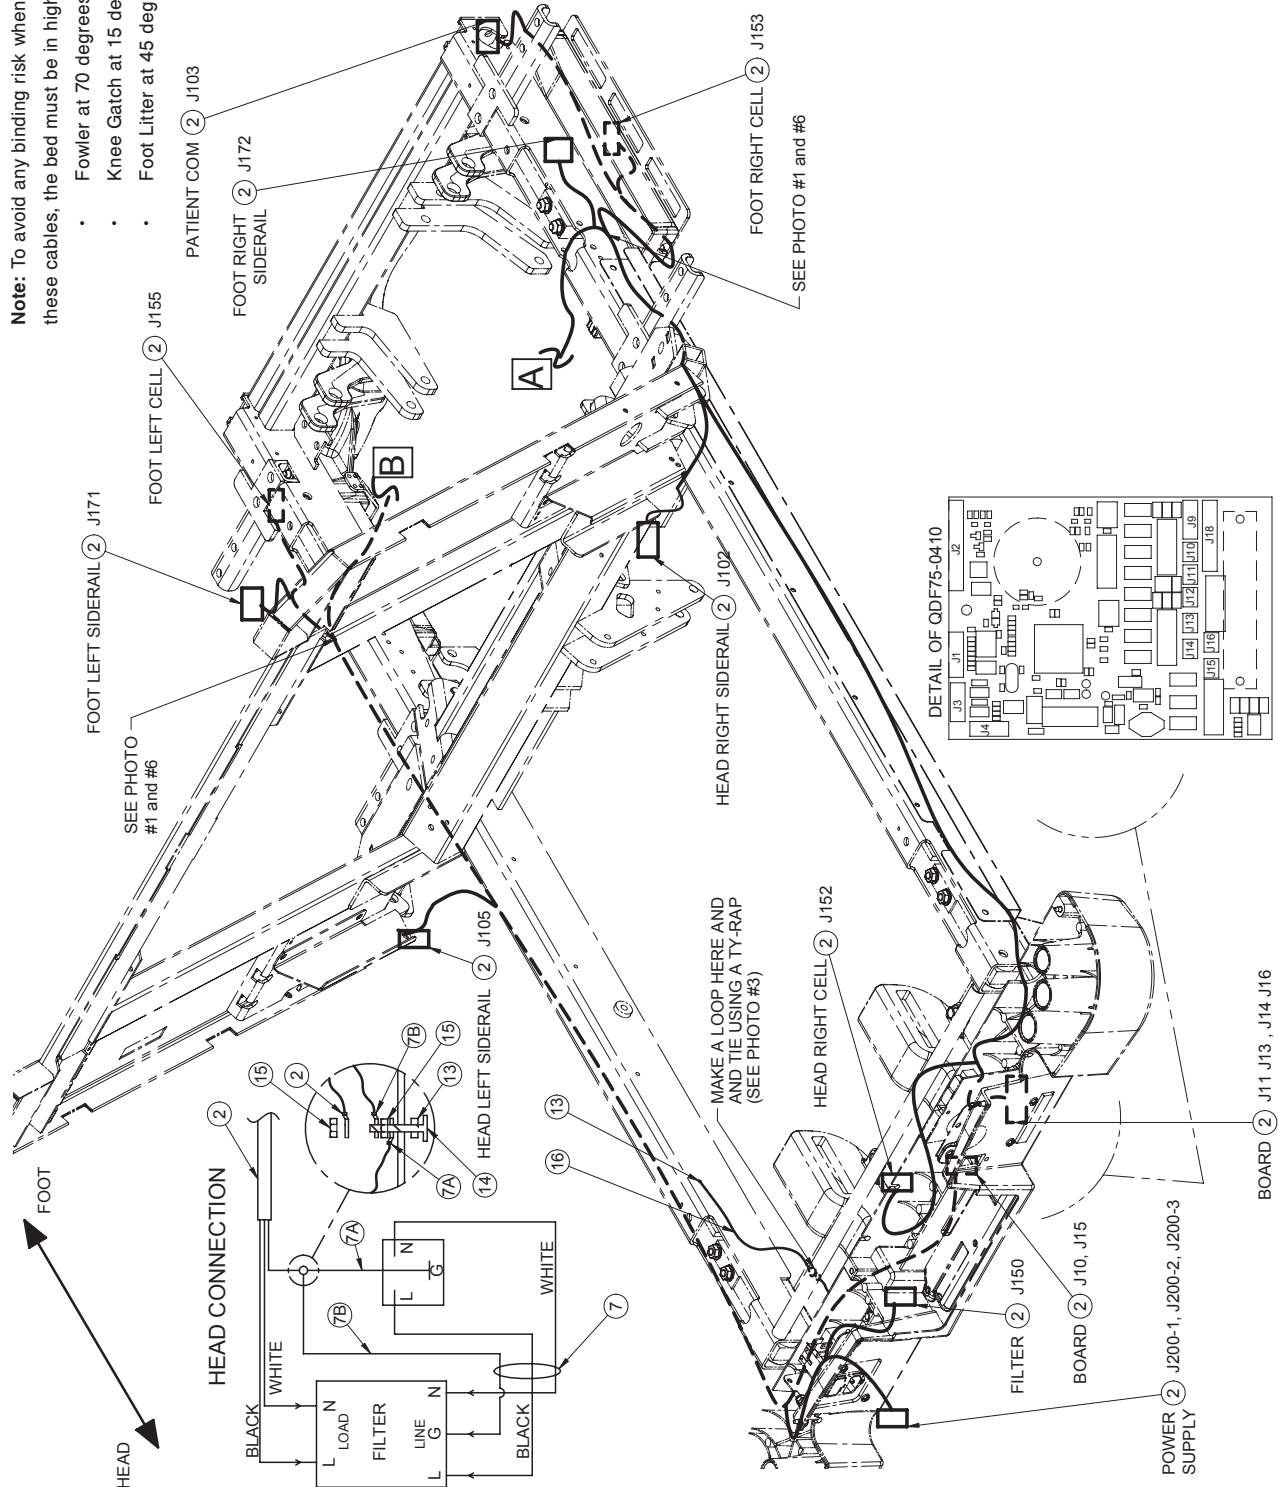

***(Applies to beds with Serial Numbers U03319 - U04982)
(Including U03258 and U03259)***



Litter Assembly, Electrical

(Applies to beds with Serial Numbers U03319 - U04982)
(Including U03258 and U03259)

Photo #1

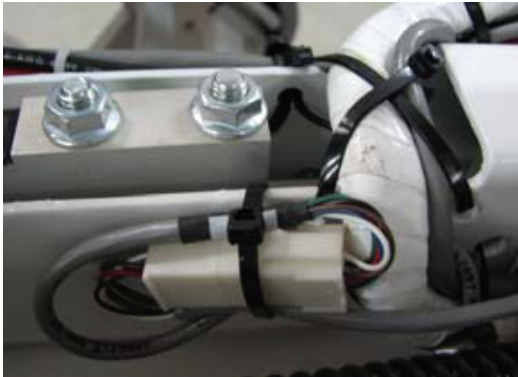


Photo #2



Photo #3

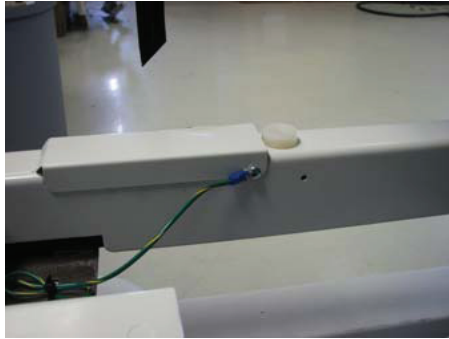


Photo #4

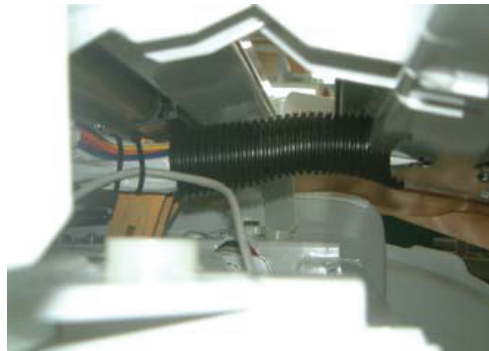


Photo #5



QDF27-1381 CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1381	Red Grommet	To	QDF9188	Battery A Pole + (27-2478)
QDF27-1381	Terminal	To	QDF9188	Switch (27-2478)
QDF27-1381	Terminal	To	QDF9188	Switch (27-2478)

QDF27-1646 CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1646	Mini Fit	To	QDF75-0440	J12 DC Board
QDF27-1646	Black Grommet	To	QDF9188	Battery B Pole + (27-2478)
QDF27-1646	White Grommet	To	QDF9188	Battery A Pole - (27-2478)

[Return To Table of Contents](#)

Litter Assembly, Electrical

**(Applies to beds with Serial Numbers U03319 - U04982)
(Including U03258 and U03259)**

QDF27-2213 CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2213	J22	To	QDF75-0440	J22 DC Board
QDF27-2213	J21	To	QDF75-0440	J21 DC Board
QDF27-2213	J20A	To	QDF75-0440	J20A DC Board
QDF27-2213	J20B	To	QDF75-0440	J20B DC Board
QDF27-2213	J20C	To	QDF75-0440	J20C DC Board
QDF27-2213	J19	To	QDF75-0440	J19 DC Board
QDF27-2213	J29	To	QDF75-0440	J29 DC Board
QDF27-2213	J15A	To	QDF75-0440	J15A DC Board
QDF27-2213	J15B	To	QDF75-0440	J15B DC Board
QDF27-2213	J15C	To	QDF75-0440	J15C DC Board
QDF27-2213	J15D	To	QDF75-0440	J15D DC Board
QDF27-2213	J204	To	QDF27-2038	Transformer J204
QDF27-2213	J27	To	QDF75-0440	J27 DC Board
QDF27-2213	J3	To	QDF75-0440	J3 DC Board
QDF27-2213	J5	To	QDF75-0440	J5 DC Board
QDF27-2213	J113	To	QDF75-0140	Foot Sensor (27-2478)
QDF27-2213	J202	To	---	Gatch Ground
QDF27-2213	J114	To	QDF75-0140	Trend Sensor
QDF27-2213	J153	To	QDF27-1372	Right Foot Cell
QDF27-2213	J103	To	27-0264	Removable Control
QDF27-2213	J172	To	QDF27-1208	Right Foot Siderail
QDF27-2213	J102	To	QDF27-2212	Right Head Siderail
QDF27-2213	J152	To	QDF27-1372	Right Head Cell
QDF27-2213	J202A	To	---	Foot Ground
QDF27-2213	J16	To	QDF75-0270	J16
QDF27-2213	J15	To	QDF75-0270	J15
QDF27-2213	J14	To	QDF75-0270	J14
QDF27-2213	J13	To	QDF75-0270	J13
QDF27-2213	J10	To	QDF75-0270	J10
QDF27-2213	J11	To	QDF75-0270	J11
QDF27-2213	J144	To	QDF27-1215	Gatch Motor
QDF27-2213	J142	To	QDF27-1214	Fowler Motor
QDF27-2213	J112	To	QDF75-0140	Fowler Sensor
QDF27-2213	J118	To	QDF75-0140	Gatch Sensor
QDF27-2213	J155	To	QDF27-1372	Left Foot Cell
QDF27-2213	J171	To	QDF27-1208	Left Foot Siderail
QDF27-2213	J105	To	QDF27-2212	Left Head Siderail
QDF27-2213	J150	To	QDF27-1372	Left Head Cell
QDF27-2213	J23	To	QDF75-0440	J23 DC Board
QDF27-2213	J26	To	QDF75-0440	J26 DC Board
QDF27-2213	J200A Black	To	QDF9571	Line "L"
QDF27-2213	J200B White	To	QDF9571	Line "N"
QDF27-2213	J200C Green	To	Ground	Head Screw

[Return To Table of Contents](#)

Litter Assembly, Electrical

*(Applies to beds with Serial Numbers U03319 - U04982)
(Including U03258 and U03259)*

QDF27-1607 CABLES #3 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1607	Con. MTA 5 Pos.	To	QDF75-0440	J25 DC Board
QDF27-1607	Contact	To	QDF27-1213	Contact 7 or 8
QDF27-1607	Contact	To	QDF27-1213	Contact 7 or 8
QDF27-1607	Terminal	To	QDF9535	Right Limit Switch (27-2478) No/Com
QDF27-1607	Terminal	To	QDF9535	Right Limit Switch (27-2478) Com/No
QDF27-1607	Terminal	To	QDF9535	Left Limit Switch (27-2478) No/Com
QDF27-1607	Terminal	To	QDF9535	Left Limit Switch (27-2478) Com/No

QDF5095 CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF5095	Con. MTA	To	QDF75-0440	J13 DC Board
QDF5095	Buzzer	To	Electrical Box	See Position on Drawing

QDF27-1524 CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1524	Black 90° Terminal	To	QDF9571	Line "L"
QDF27-1524	White 90° Terminal	To	QDF9571	Line "N"
QDF27-1524	Green 90° Terminal	To	QDF9571	Line "E"
QDF27-1524	Black Right Terminal	To	QDF9574	"L" (Power Supply
QDF27-1524	White Right Terminal	To	QDF9574	"N" (Power Supply
QDF27-1524	Green Right Terminal	To	QDF9574	"E" (Power Supply
QDF27-1524	Cross Grommet	To	Head Ground	Screw
QDF27-1524	Cross Grommet	To	Head Ground	Screw

QDF27-1214 CABLES #10 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2214	Con. MTA 6 Pos.	To	QDF75-0440	J18 DC Board
QDF27-2214	Con. Metrimate	To	27-1547	Panel (27-1547)

QDF27-2025 CABLES #12 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2025	Light	To	QDF75-0440	J20 DC Board

Litter Assembly, Electrical

***(Applies to beds with Serial Numbers U03319 - U04982)
(Including U03258 and U03259)***

QDF27-2228 CABLES #11 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2228	J205	To	QDF27-2038	Transformer
QDF27-2228	J202 Grommet	To	---	Foot Litter Ground
QDF27-2228	J208AL (Black)	To	QDF9573	Single Outlet (27-2478)
QDF27-2228	J207 Terminal	To	QDF9025	Breaker (27-2478)
QDF27-2228	J206 Terminal	To	QDF9025	Breaker (27-2478)
QDF27-2228	J208AN (White)	To	QDF9573	Outlet (27-2478) White
QDF27-2228	J208AG (Green/Yellow)	To	QDF9573	Outlet (27-2478) Ground

Litter Assembly, Cabling - Common Components - 27-2559 Rev-00 (Reference only)

Item	Part No.	Part Name	Qty.
1*	QDF27-1381	Battery Switch Wire	2
2*	QDF27-2213	#1 Wire Harness	1
3*	QDF27-1607	I.V. Pole and Bed Extender Cable	1
4*	QDF27-1646	Battery Wires	1
5*	QDF5095	Buzzer	1
6*	QDF9518	Cable Tie	51
7*	QDF27-1524	Filter and Receiver Connector	1
10*	QDF27-2214	Panel – Control Board Cable	1
11*	QDF27-2228	Auxiliary 120V Outlet Cable without Mattress Connector	1
12*	QDF27-2025	12V Night Light	1
13*	VW20A76	Locking Washer	4
14*	VV33A0G28	Phillips Machine Screw #10-32 x 7/8"	3
15*	VE30A0G	Nylon Locknut #10-32	6
16*	QDF27-2284	Electronic Board Ground Wire	1
18	QDF2115	1.25 Split Loom Polyethylene	1


Litter Assembly, Electrical

(Applies to beds with Serial Numbers U04983 - U50240)

27-2643 Rev-00 (Reference Only)


Note: To avoid any binding risk when assembling these cables, the bed must be in high position.

- Fowler at 70 degrees
- Knee Gatch at 15 degrees
- Foot Litter at 45 degrees

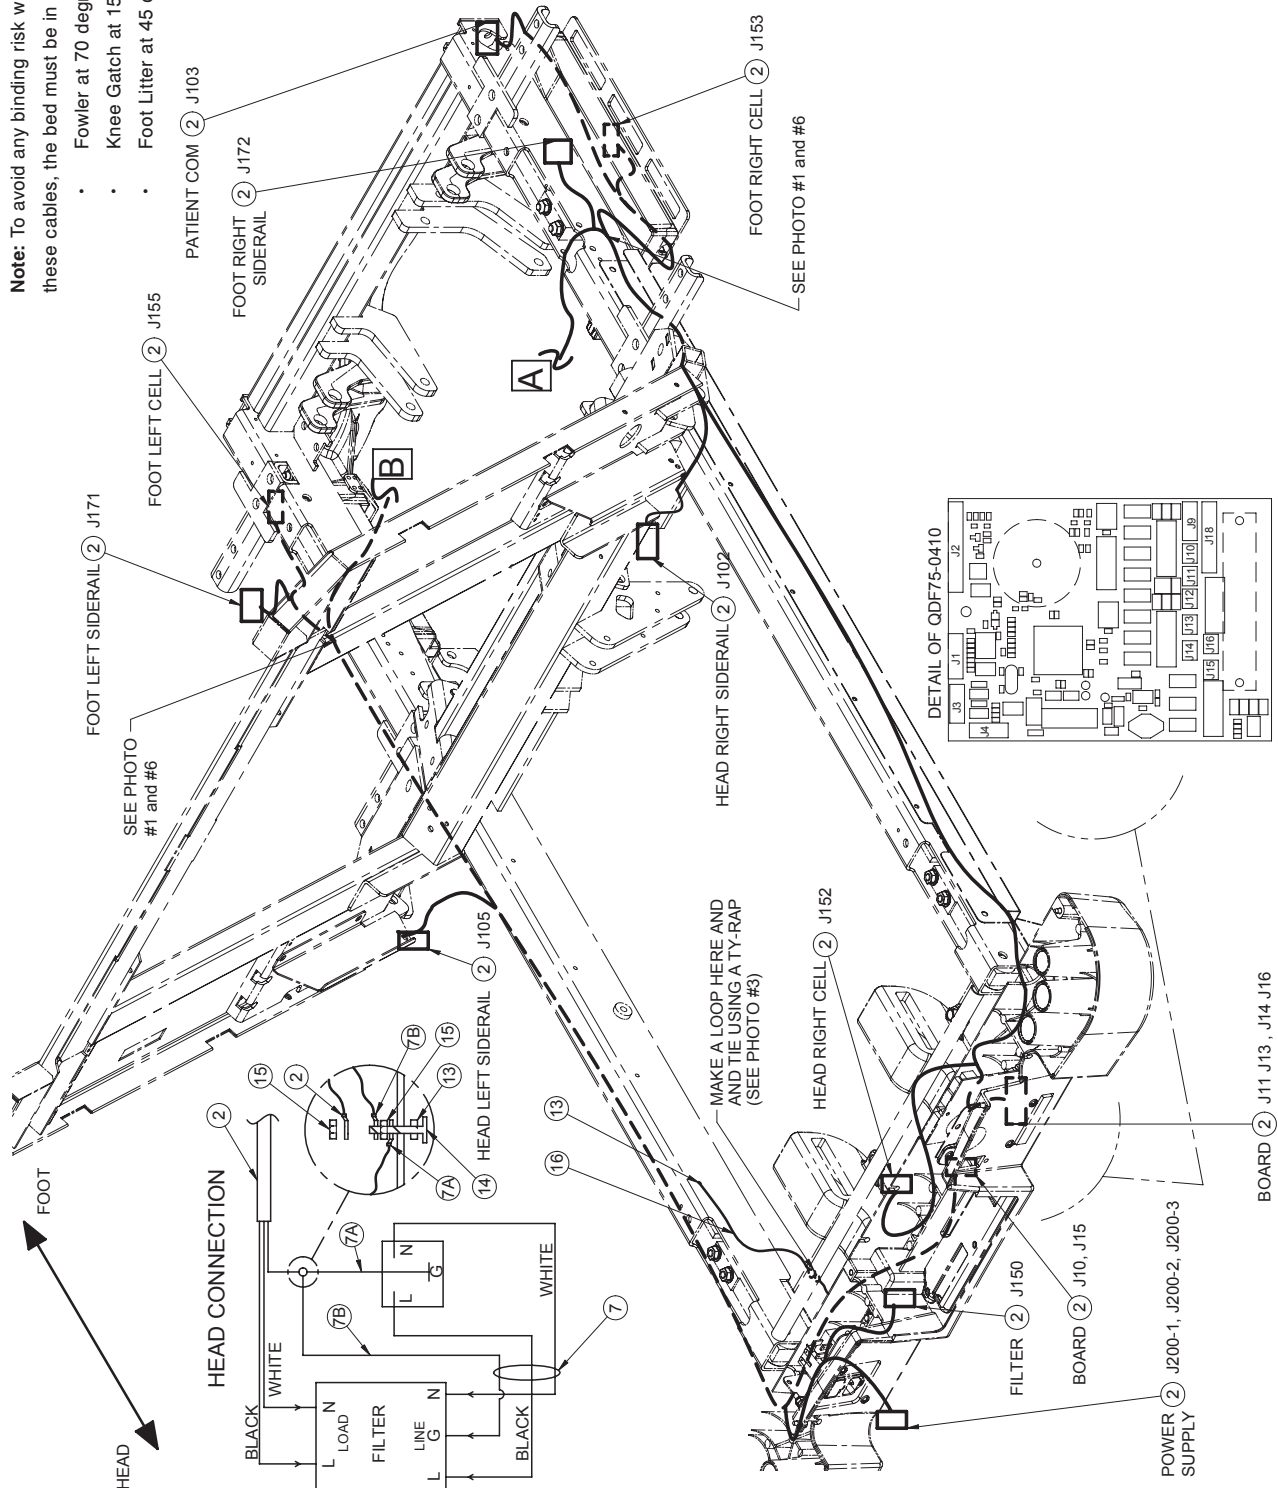

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U04983 - U50240)

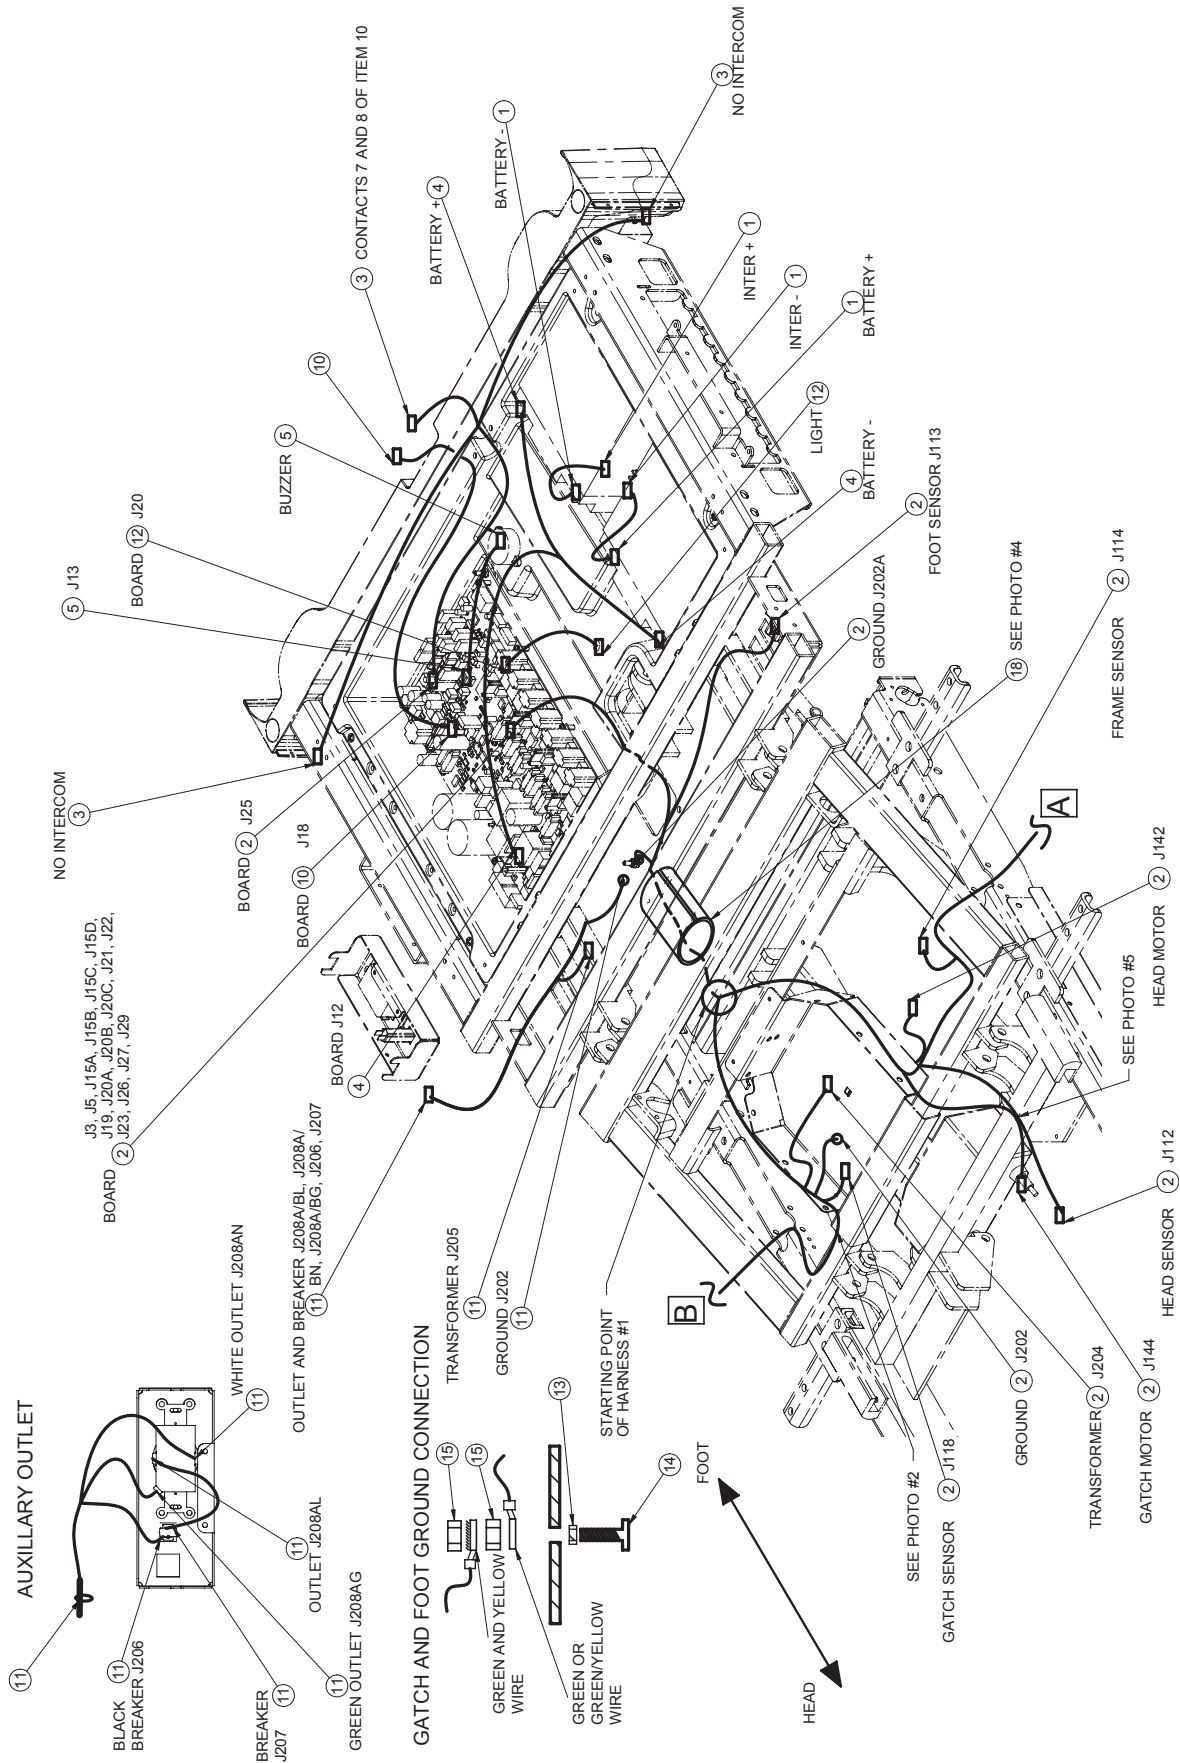

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U04983 - U50240)

Photo #1

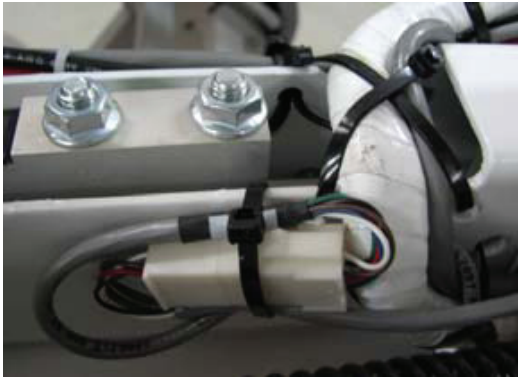


Photo #2



Photo #3

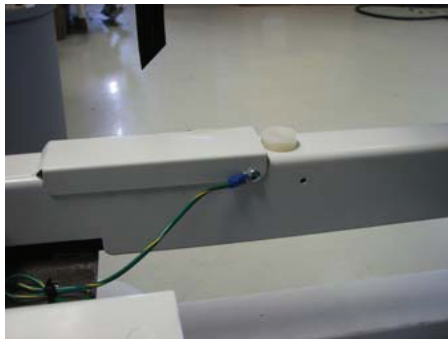


Photo #4



Photo #5



QDF27-1381 CABLES CONNECTION TABLE

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1381	Red Grommet	To	QDF9188	Battery A Pole + (27-2478)
QDF27-1381	Terminal	To	QDF9188	Switch (27-2478)
QDF27-1381	Terminal	To	QDF9188	Switch (27-2478)

QDF27-1646 CABLES CONNECTION TABLE

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1646	Mini Fit	To	QDF75-0440	J12 DC Board
QDF27-1646	Black Grommet	To	QDF9188	Battery B Pole + (27-2478)
QDF27-1646	White Grommet	To	QDF9188	Battery A Pole - (27-2478)

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U04983 - U50240)

QDF27-2213 CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2213	J22	To	QDF75-0440	J22 DC Board
QDF27-2213	J21	To	QDF75-0440	J21 DC Board
QDF27-2213	J20A	To	QDF75-0440	J20A DC Board
QDF27-2213	J20B	To	QDF75-0440	J20B DC Board
QDF27-2213	J20C	To	QDF75-0440	J20C DC Board
QDF27-2213	J19	To	QDF75-0440	J19 DC Board
QDF27-2213	J29	To	QDF75-0440	J29 DC Board
QDF27-2213	J15A	To	QDF75-0440	J15A DC Board
QDF27-2213	J15B	To	QDF75-0440	J15B DC Board
QDF27-2213	J15C	To	QDF75-0440	J15C DC Board
QDF27-2213	J15D	To	QDF75-0440	J15D DC Board
QDF27-2213	J204	To	QDF27-2038	Transformer J204
QDF27-2213	J27	To	QDF75-0440	J27 DC Board
QDF27-2213	J3	To	QDF75-0440	J3 DC Board
QDF27-2213	J5	To	QDF75-0440	J5 DC Board
QDF27-2213	J113	To	QDF75-0140	Foot Sensor (27-2478)
QDF27-2213	J202	To	---	Gatch Ground
QDF27-2213	J114	To	QDF75-0140	Trend Sensor
QDF27-2213	J153	To	QDF27-1372	Right Foot Cell
QDF27-2213	J103	To	27-0264	Removable Control
QDF27-2213	J172	To	QDF27-1208	Right Foot Siderail
QDF27-2213	J102	To	QDF27-2212	Right Head Siderail
QDF27-2213	J152	To	QDF27-1372	Right Head Cell
QDF27-2213	J202A	To	---	Foot Ground
QDF27-2213	J16	To	QDF75-0270	J16
QDF27-2213	J15	To	QDF75-0270	J15
QDF27-2213	J14	To	QDF75-0270	J14
QDF27-2213	J13	To	QDF75-0270	J13
QDF27-2213	J10	To	QDF75-0270	J10
QDF27-2213	J11	To	QDF75-0270	J11
QDF27-2213	J144	To	QDF27-1215	Gatch Motor
QDF27-2213	J142	To	QDF27-1214	Fowler Motor
QDF27-2213	J112	To	QDF75-0140	Fowler Sensor
QDF27-2213	J118	To	QDF75-0140	Gatch Sensor
QDF27-2213	J155	To	QDF27-1372	Left Foot Cell
QDF27-2213	J171	To	QDF27-1208	Left Foot Siderail
QDF27-2213	J105	To	QDF27-2212	Left Head Siderail
QDF27-2213	J150	To	QDF27-1372	Left Head Cell
QDF27-2213	J23	To	QDF75-0440	J23 DC Board
QDF27-2213	J26	To	QDF75-0440	J26 DC Board
QDF27-2213	J200A Black	To	QDF9571	Line "L"
QDF27-2213	J200B White	To	QDF9571	Line "N"
QDF27-2213	J200C Green	To	Ground	Head Screw

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U04983 - U50240)

QDF27-1607 CABLES #3 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1607	Con. MTA 5 Pos.	To	QDF75-0440	J25 DC Board
QDF27-1607	Contact	To	QDF27-1213	Contact 7 or 8
QDF27-1607	Contact	To	QDF27-1213	Contact 7 or 8
QDF27-1607	Terminal	To	QDF9535	Right Limit Switch (27-2478) No/Com
QDF27-1607	Terminal	To	QDF9535	Right Limit Switch (27-2478) Com/No
QDF27-1607	Terminal	To	QDF9535	Left Limit Switch (27-2478) No/Com
QDF27-1607	Terminal	To	QDF9535	Left Limit Switch (27-2478) Com/No

QDF5095 CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF5095	Con. MTA	To	QDF75-0440	J13 DC Board
QDF5095	Buzzer	To	Electrical Box	See Position on Drawing

QDF27-1524 CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1524	Black 90° Terminal	To	QDF9571	Line "L"
QDF27-1524	White 90° Terminal	To	QDF9571	Line "N"
QDF27-1524	Green 90° Terminal	To	QDF9571	Line "E"
QDF27-1524	Black Right Terminal	To	QDF9574	"L" (Power Supply
QDF27-1524	White Right Terminal	To	QDF9574	"N" (Power Supply
QDF27-1524	Green Right Terminal	To	QDF9574	"E" (Power Supply
QDF27-1524	Cross Grommet	To	Head Ground	Screw
QDF27-1524	Cross Grommet	To	Head Ground	Screw

QDF27-1214 CABLES #10 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2214	Con. MTA 6 Pos.	To	QDF75-0440	J18 DC Board
QDF27-2214	Con. Metrimate	To	27-1547	Panel (27-1547)

QDF27-2025 CABLES #12 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2025	Light	To	QDF75-0440	J20 DC Board

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U04983 - U50240)


QDF27-2228 CABLES #11 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2228	J205	To	QDF27-2038	Transformer
QDF27-2228	J202 Grommet	To	---	Foot Litter Ground
QDF27-2228	J208AL (Black)	To	QDF9573	Single Outlet (27-2478)
QDF27-2228	J207 Terminal	To	QDF9025	Breaker (27-2478)
QDF27-2228	J206 Terminal	To	QDF9025	Breaker (27-2478)
QDF27-2228	J208AN (White)	To	QDF9573	Outlet (27-2478) White
QDF27-2228	J208AG (Green/Yellow)	To	QDF9573	Outlet (27-2478) Ground

Litter Assembly, Cabling - Common Components - 27-2643 Rev-00 (Reference Only)

Item	Part No.	Part Name	Qty.
1*	QDF27-1381	Battery Switch Wire	2
2*	QDF27-2213	#1 Wire Harness	1
3*	QDF27-1607	I.V. Pole and Bed Extender Cable	1
4*	QDF27-1646	Battery Wires	1
5*	QDF5095	Buzzer	1
6*	QDF9518	Cable Tie	51
7*	QDF27-1524	Filter and Receiver Connector	1
10*	QDF27-2214	Panel – Control Board Cable	1
11*	QDF27-2228	Auxiliary 120V Outlet Cable without Mattress Connector	1
12*	QDF27-2025	12V Night Light	1
13*	VW20A76	Locking Washer	4
14*	VV33A0G28	Phillips Machine Screw #10-32 x 7/8"	3
15*	VE30A0G	Nylon Locknut #10-32	6
16*	QDF27-2284	Electronic Board Ground Wire	1
18	QDF2115	1.25 Split Loom Polyethylene	1

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U50241 - Current)

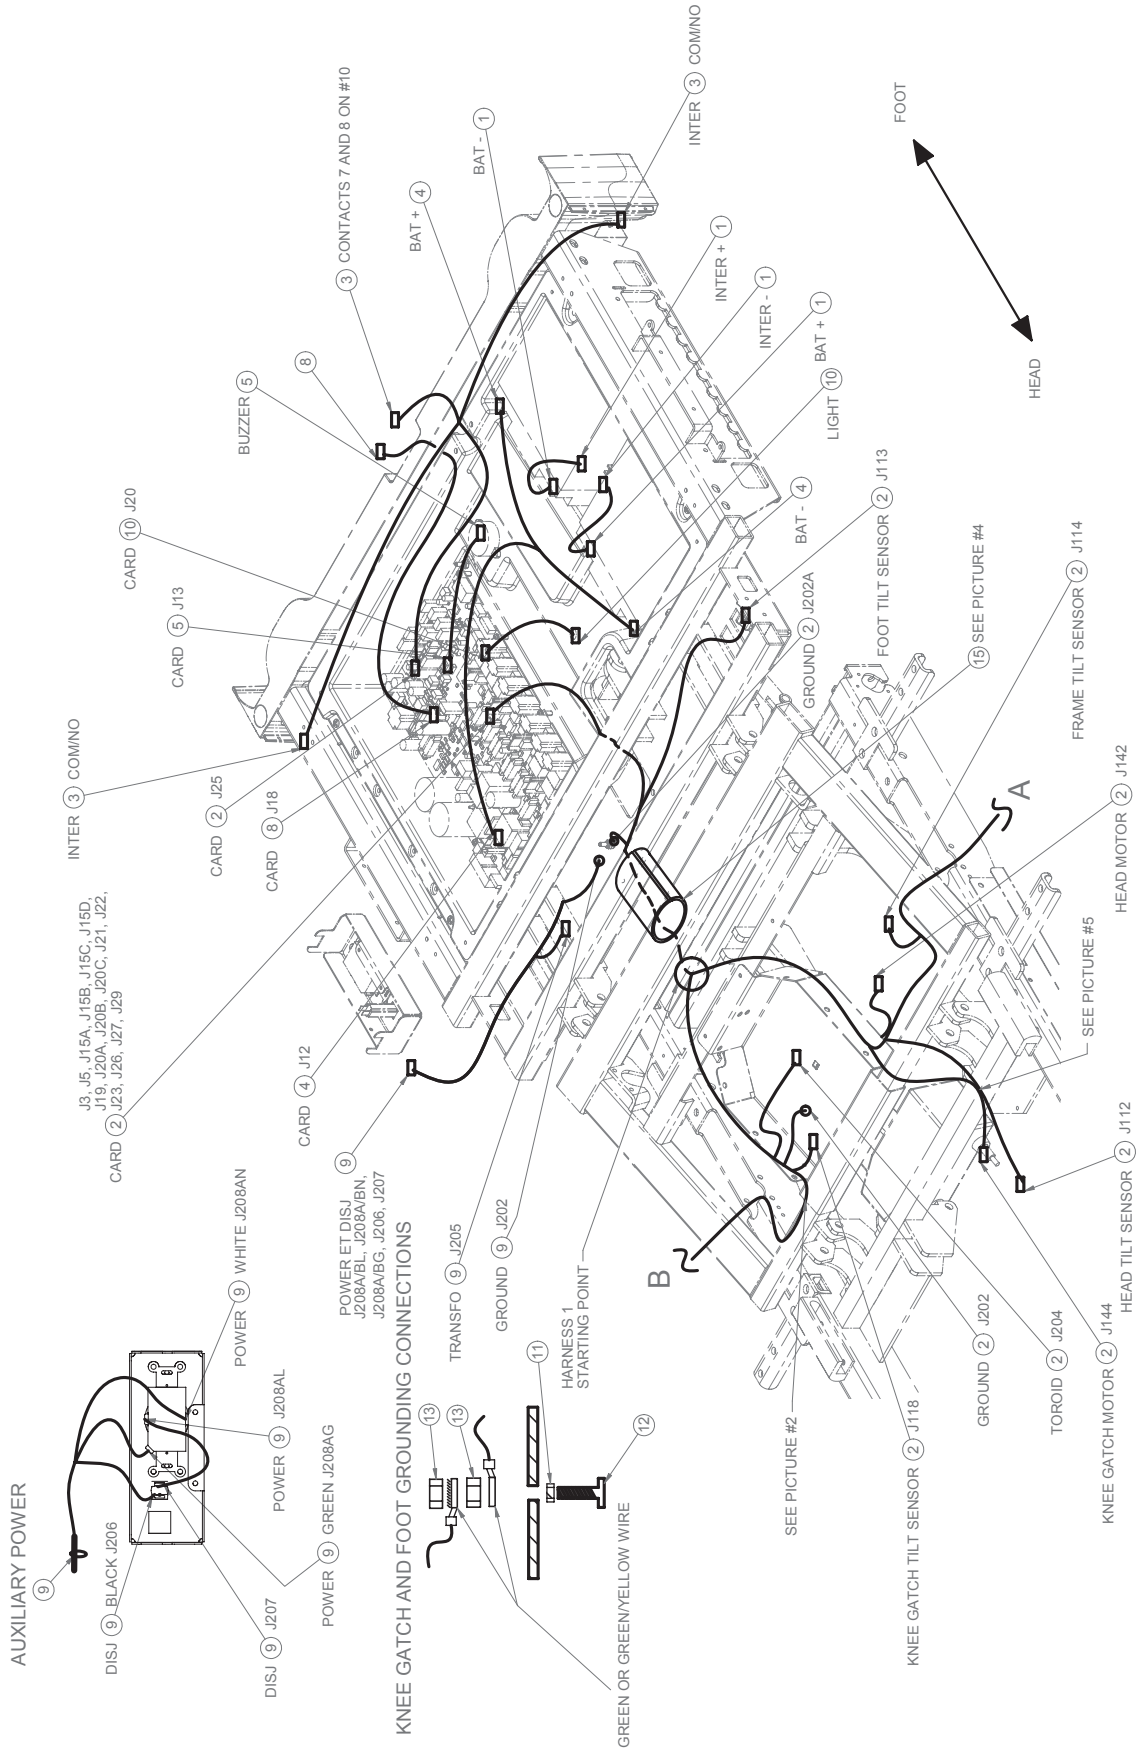

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U50241 - Current)

Photo #1



Photo #2



Photo #3

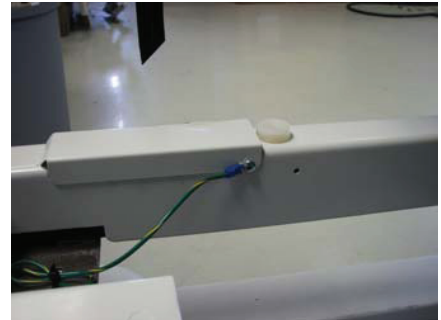


Photo #4



Photo #5



Photo #5



19

QDF27-1381 CABLES #1 CONNECTION TABLE

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1381	Grommet	To	QDF9188	Battery
QDF27-1381	Terminal	To	QDF2089	Interrupter
QDF27-1381	Terminal	To	QDF2089	Interrupter

QDF27-1646 CABLES #4 CONNECTION TABLE

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1646	Mini Fit	To	QDF75-0440	J12 DC Board
QDF27-1646	Black Grommet	To	QDF9188	Battery #2 Pole -
QDF27-1646	White Grommet	To	QDF9188	Battery #1 Pole +

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U50241 - Current)

QDF27-2213 CABLES #2 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2213	J22	To	QDF75-0440	J22 DC Board
QDF27-2213	J21	To	QDF75-0440	J21 DC Board
QDF27-2213	J20A	To	QDF75-0440	J20A DC Board
QDF27-2213	J20B	To	QDF75-0440	J20B DC Board
QDF27-2213	J20C	To	QDF75-0440	J20C DC Board
QDF27-2213	J19	To	QDF75-0440	J19 DC Board
QDF27-2213	J29	To	QDF75-0440	J29 DC Board
QDF27-2213	J15A	To	QDF75-0440	J15A DC Board
QDF27-2213	J15B	To	QDF75-0440	J15B DC Board
QDF27-2213	J15C	To	QDF75-0440	J15C DC Board
QDF27-2213	J15D	To	QDF75-0440	J15D DC Board
QDF27-2213	J204	To	QDF27-2038	Transformer J204
QDF27-2213	J27	To	QDF75-0440	J27 DC Board
QDF27-2213	J3	To	QDF75-0440	J3 DC Board
QDF27-2213	J5	To	QDF75-0440	J5 DC Board
QDF27-2213	J113	To	QDF75-0140	Foot Sensor (27-2708)
QDF27-2213	J202	To	–	Gatch Ground
QDF27-2213	J114	To	QDF75-0140	Trend Sensor
QDF27-2213	J153	To	QDF27-1372	Right Foot Cell
QDF27-2213	J103	To	27-2598	Removable Control
QDF27-2213	J172	To	QDF27-1208	Right Foot Siderail
QDF27-2213	J102	To	QDF27-2212	Right Head Siderail
QDF27-2213	J152	To	QDF27-1372	Right Head Cell
QDF27-2213	J202A	To	–	Foot Ground
QDF27-2213	J16	To	QDF75-0270	J16
QDF27-2213	J15	To	QDF75-0270	J15
QDF27-2213	J14	To	QDF75-0270	J14
QDF27-2213	J13	To	QDF75-0270	J13
QDF27-2213	J10	To	QDF75-0270	J10
QDF27-2213	J11	To	QDF75-0270	J11
QDF27-2213	J144	To	QDF27-1215	Gatch Motor
QDF27-2213	J142	To	QDF27-1214	Fowler Motor
QDF27-2213	J112	To	QDF75-0140	Fowler Sensor
QDF27-2213	J118	To	QDF75-0140	Gatch Sensor
QDF27-2213	J155	To	QDF27-1372	Left Foot Cell
QDF27-2213	J171	To	QDF27-1208	Left Foot Siderail
QDF27-2213	J105	To	QDF27-2212	Left Head Siderail
QDF27-2213	J150	To	QDF27-1372	Left Head Cell
QDF27-2213	J23	To	QDF75-0440	J23 DC Board
QDF27-2213	J26	To	QDF75-0440	J26 DC Board
QDF27-2213	J200A Black	To	QDF9571	Line “L”
QDF27-2213	J200B White	To	QDF9571	Line “N”
QDF27-2213	J200C Green/Yellow	To	Ground	Head Screw

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U50241 - Current)

QDF27-1607 CABLES #3 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1607	Con. MTA 5 Pos.	To	QDF75-0440	J25 DC Board
QDF27-1607	Contact	To	QDF27-1213	Contact 7 or 8
QDF27-1607	Contact	To	QDF27-1213	Contact 7 or 8
QDF27-1607	Terminal	To	QDF9535	Right Limit Switch No/Com
QDF27-1607	Terminal	To	QDF9535	Right Limit Switch Com/No
QDF27-1607	Terminal	To	QDF9535	Left Limit Switch No/Com
QDF27-1607	Terminal	To	QDF9535	Left Limit Switch Com/No

QDF5095 CABLES #5 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF5095	Con. MTA	To	QDF75-0440	J13 DC Board
QDF5095	Buzzer	To	Electrical Box	See Position on Drawing

QDF27-1524 CABLES #7 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1524	Black 90° Terminal	To	QDF9571	Line "L"
QDF27-1524	White 90° Terminal	To	QDF9571	Line "L"
QDF27-1524	Green 90° Terminal	To	QDF9571	Line "L"
QDF27-1524	Black Right Terminal	To	QDF9574	"L" (Power Supply
QDF27-1524	White Right Terminal	To	QDF9574	"N" (Power Supply
QDF27-1524	Green Right Terminal	To	QDF9574	"E" (Power Supply
QDF27-1524	Cross Grommet	To	Head Ground	Screw
QDF27-1524	Cross Grommet	To	Head Ground	Screw

QDF27-2214 CABLES #10 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2214	Con. MTA 6 Pos.	To	QDF75-0440	J18 DC Board
QDF27-2214	Con. Metrimate	To	27-1547	Panel (27-1547)

QDF27-2025 CABLES #12 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2025	Light	To	QDF75-0440	J20 DC Board

Litter Assembly, Electrical

(Applies to beds with Serial Numbers U50241 - Current)

QDF27-2228 CABLES #11 CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2228	J205	To	QDF27-2038	Transformer
QDF27-2228	J202 Grommet	To	–	Foot Litter Ground
QDF27-2228	J208AL (Black)	To	QDF9573	Single Outlet
QDF27-2228	J207 Terminal	To	QDF9025	Breaker
QDF27-2228	J206 Terminal	To	QDF9025	Breaker
QDF27-2228	J208AN (White)	To	QDF9573	Right Limit Switch No/Com
QDF27-2228	J208AG (Green/Yellow)	To	QDF9573	Ground


Litter Assembly, Electrical - 27-2695 Rev B (Reference Only)

Item	Part No.	Part Name	Qty.
1*	QDF27-1381	Battery Switch Wire	2
2*	QDF27-2213	#1 Wire Harness	1
3*	QDF27-1607	I.V. Pole and Bed Extender Cable	1
4*	QDF27-1646	Battery Wires	1
5*	QDF5095	Buzzer	1
6*	QDF9518	Cable Tie	51
7*	QDF27-1524	Filter and Receiver Connector	1
8*	QDF27-2214	Panel – Control Board Cable	1
9*	QDF27-2228	Auxiliary 120V Outlet Cable without Mattress Connector	1
10*	QDF27-2025	12V Night Light	1
11*	VW20A76	Locking Washer	4
12*	VV33A0G28	Phillips Machine Screw #10-32 x 7/8"	3
13*	VE30A0G	Nylon Locknut #10-32	6
14*	QDF27-2284	Electronic Board Ground Wire	1
15	QDF2115	1.25 Split Loom Polyethylene	1
16	QDF9523	Wire Tie	2

120V Electric System

OL270206-XXX Rev E (Model 2131 Only) (For Reference Only)

OL270211-XXX Rev E (Model 2141 Only)

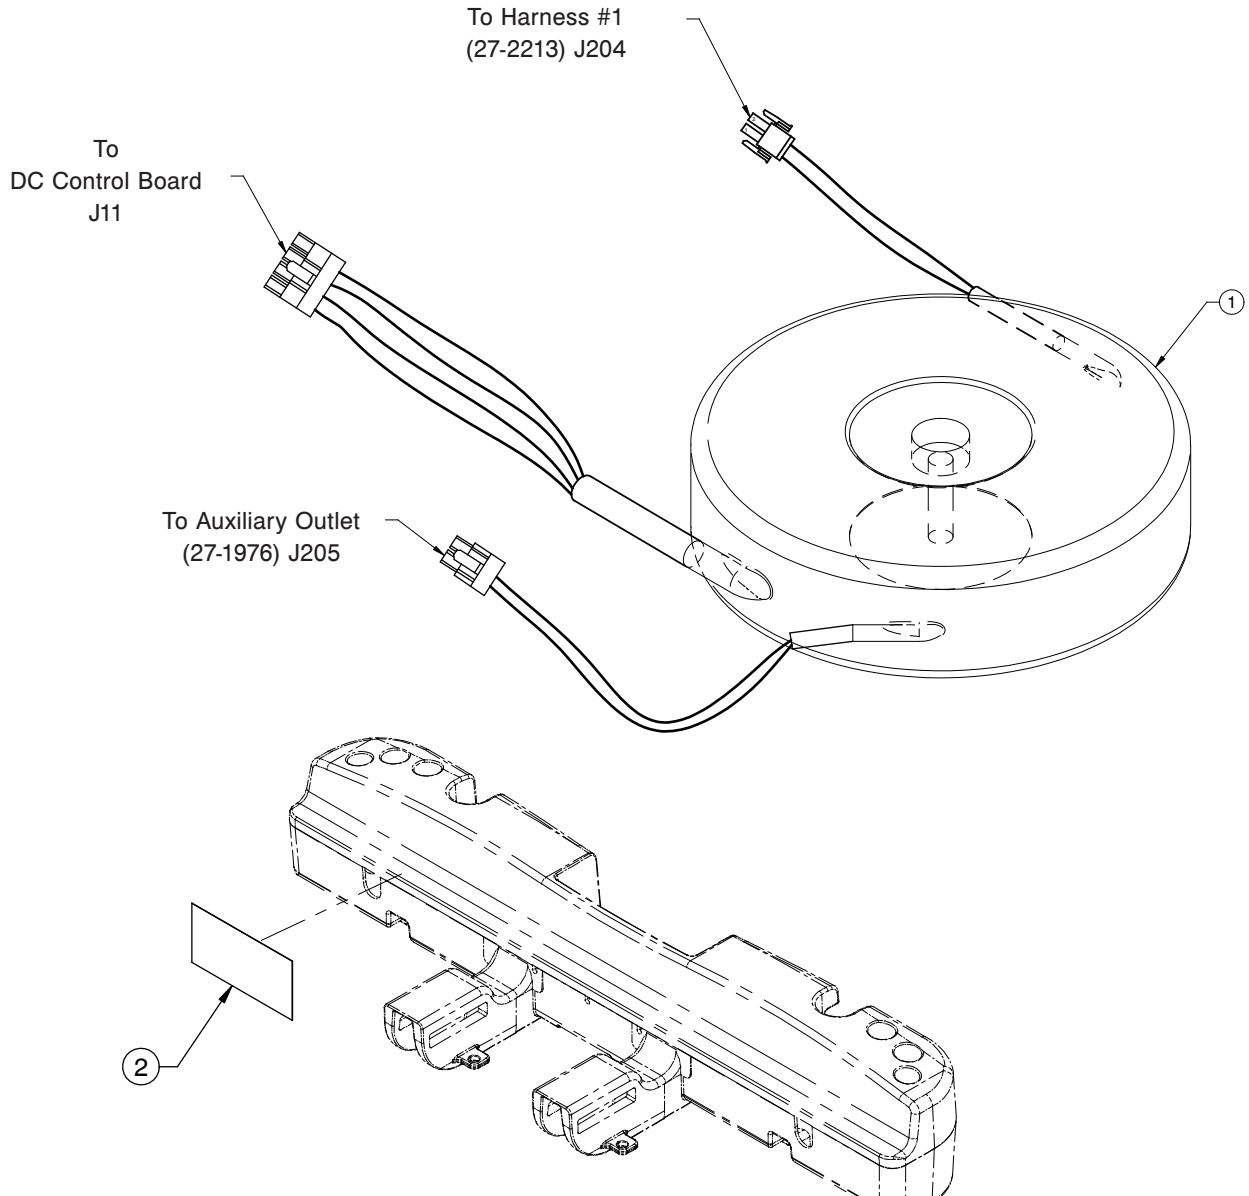


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF27-2038	Medical Toroidal Transformer	1
2	QE71-1183-XXX	120V CSA Label (2131 Models Only)	1 or
	QE71-1188-XXX	120V CSA Label (2141 Models Only)	1

Coiled Power Cord

(Applies to beds with Serial Numbers U51438 - Current)


27-2782 Rev A (Reference Only)

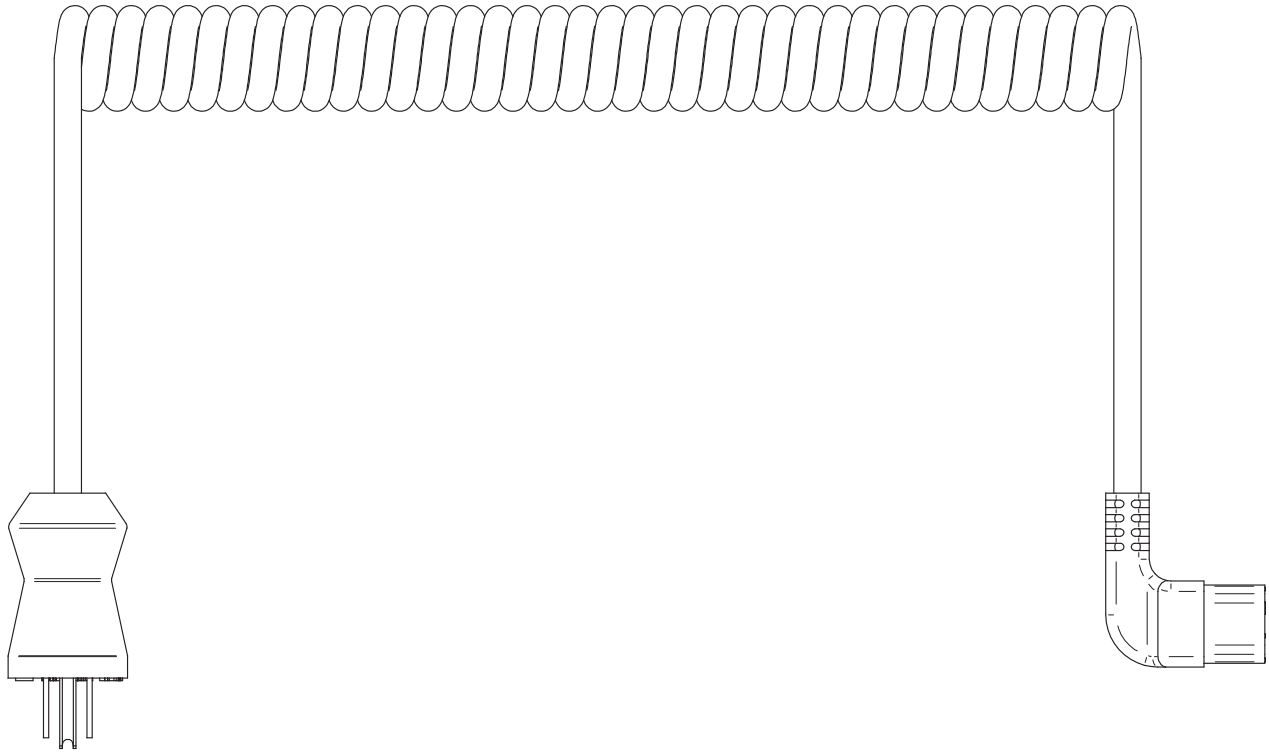

120V Straight Plug

(Applies to beds with Serial Numbers U01001 - U51437)


OL250053 Rev B (Reference Only)

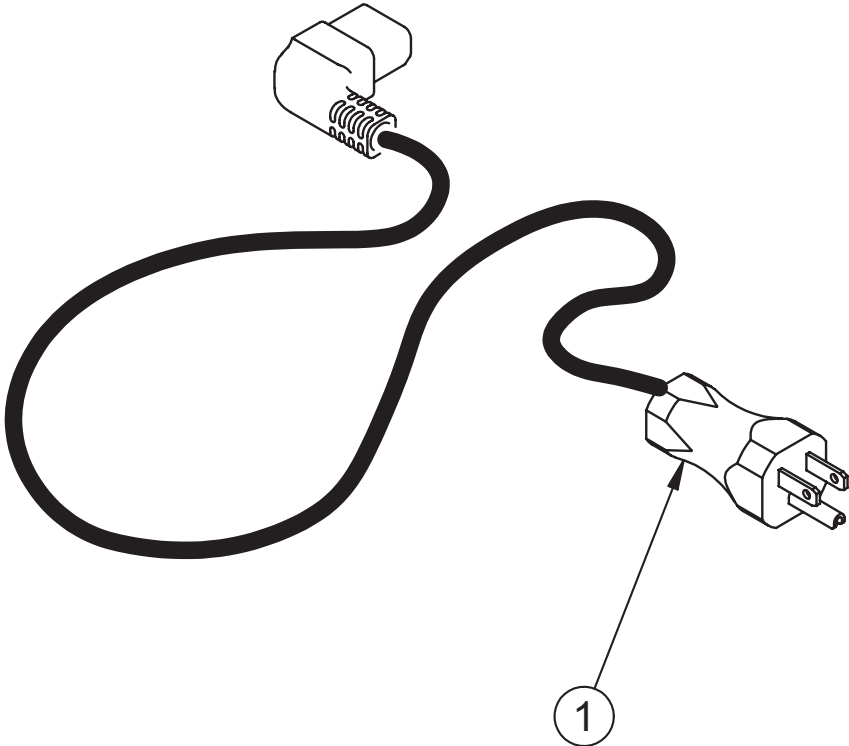

Item	Part No.	Part Name	Qty.
1	QDF8066	North American Straight Plug	1

Optional 120V 90 Degree Plug


OL250055 Rev B (Reference Only)

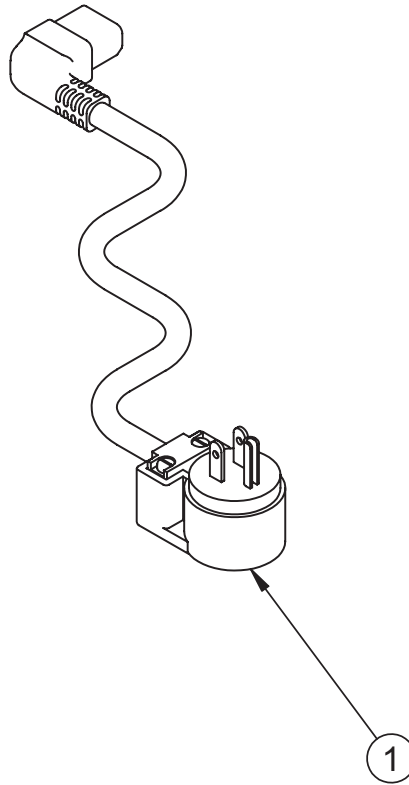

Item	Part No.	Part Name	Qty.
1	QDF8066-90D	North American 90 Degree Plug	1

Litter Assembly, Foot End, without Mattress Connector


OL270165 Rev 1 (Reference Only)

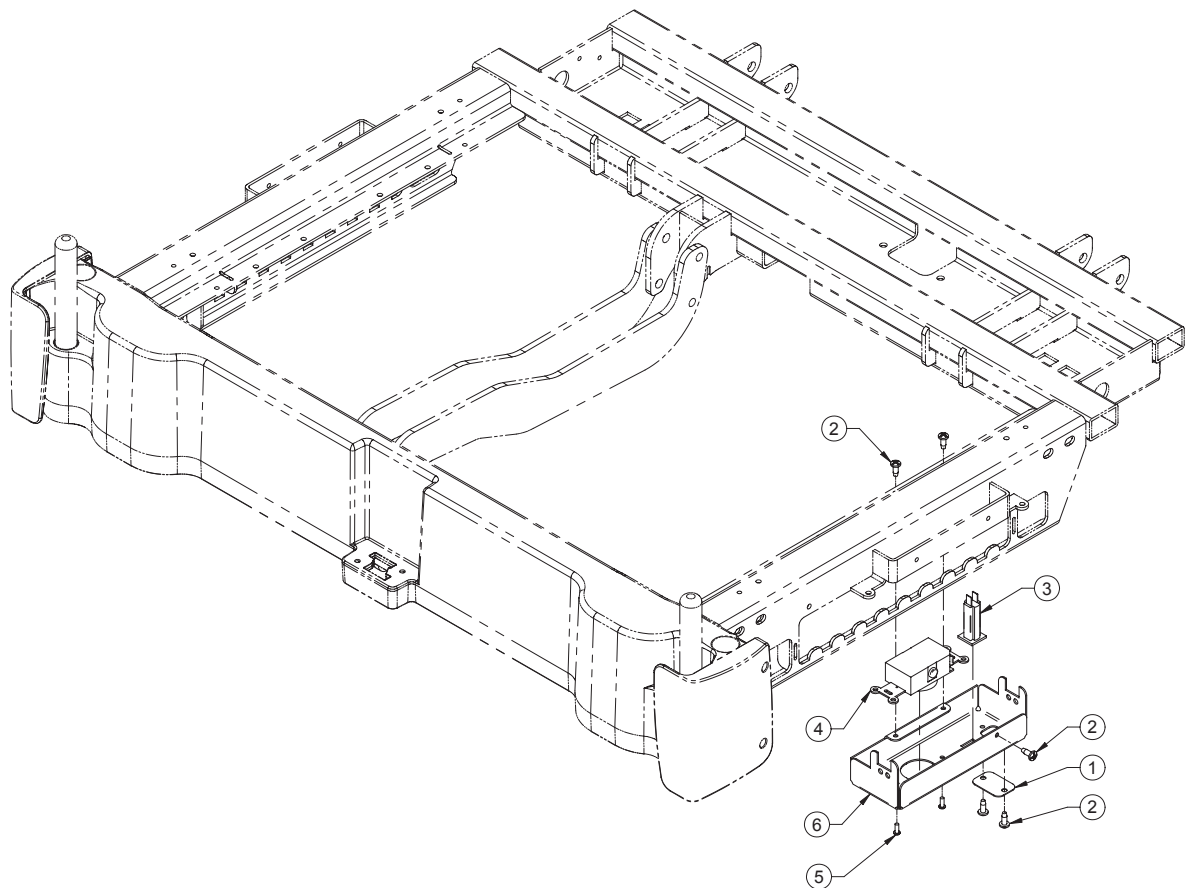

Item	Part No.	Part Name	Qty.
1	27-2250P	Plate without Connector	1
2	VV83A9G16	Tapping Screw	5
3	QDF9025	5A Breaker	1
4	QDF9573	Single Leviton 8310-G Outlet	1
5	VV37A1C12	Machine Screw	2
6	27-1967P	Auxiliary Outlet Box	1


Litter Assembly, Foot End, with Mattress Connector

OL270166 Rev 2 (Reference Only)

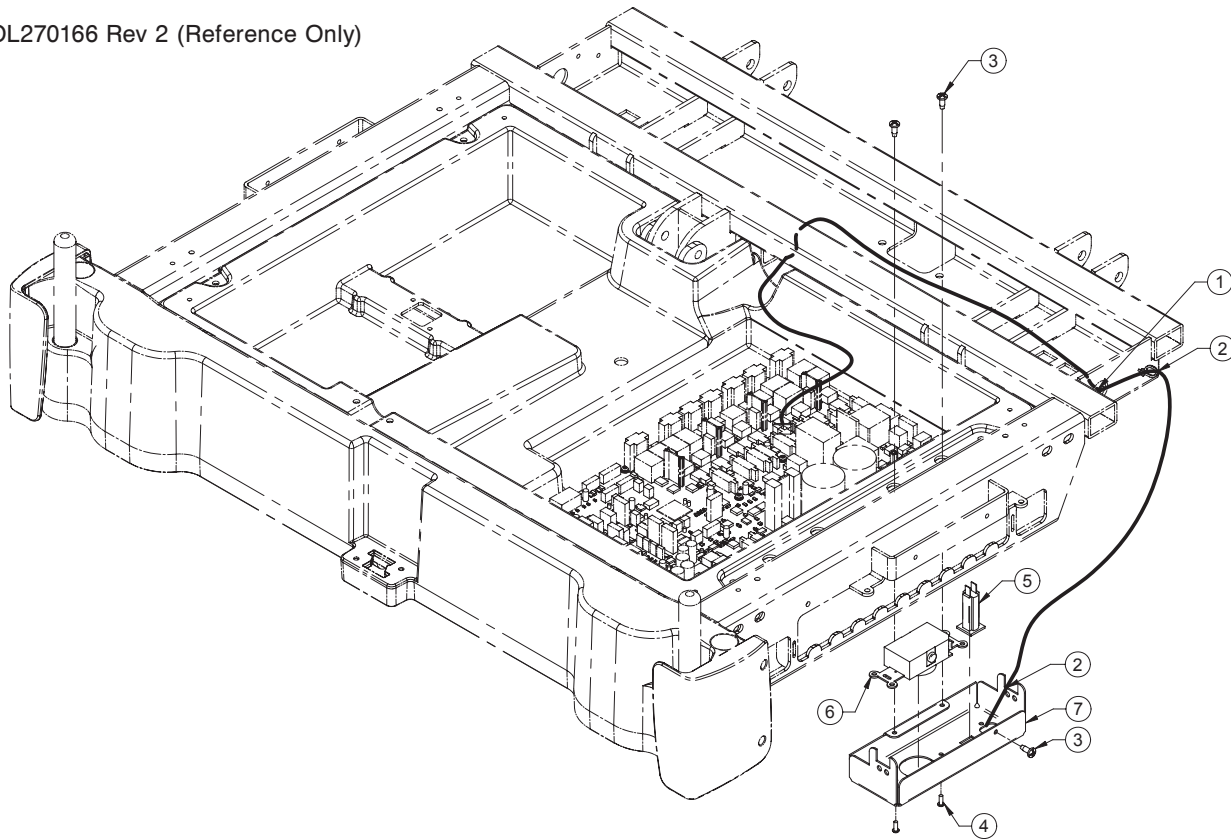


QDF27-2248 CABLES #1 CONNECTION TABLE

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2248	J17	To	QDF27-1960	J17 DC Board
QDF27-2248	J17A	To	Hole	(27-1200)

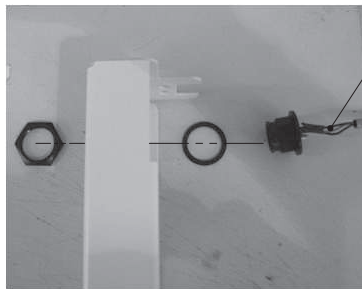

MATTRESS CONNECTOR ASSEMBLY

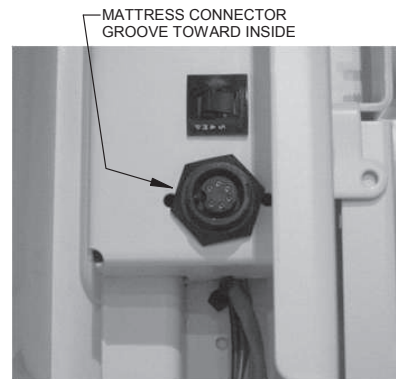


BOTTOM VIEW

Item	Part No.	Part Name	Qty.
1	QDF27-2248	Mattress Connector Cable	1
2	QDF9518	Cable Tie	2
3	VV83A9G16	Tapping Screw	3
4	VV37A1C12	Machine Screw	2
5	QDF9025	5A Breaker	1
6	QDF9573	Single Leviton 8310-G Outlet	1
7	27-1967P	Auxiliary Outlet Box	1

Standard Outlet


OL270247 Rev C (Reference Only)

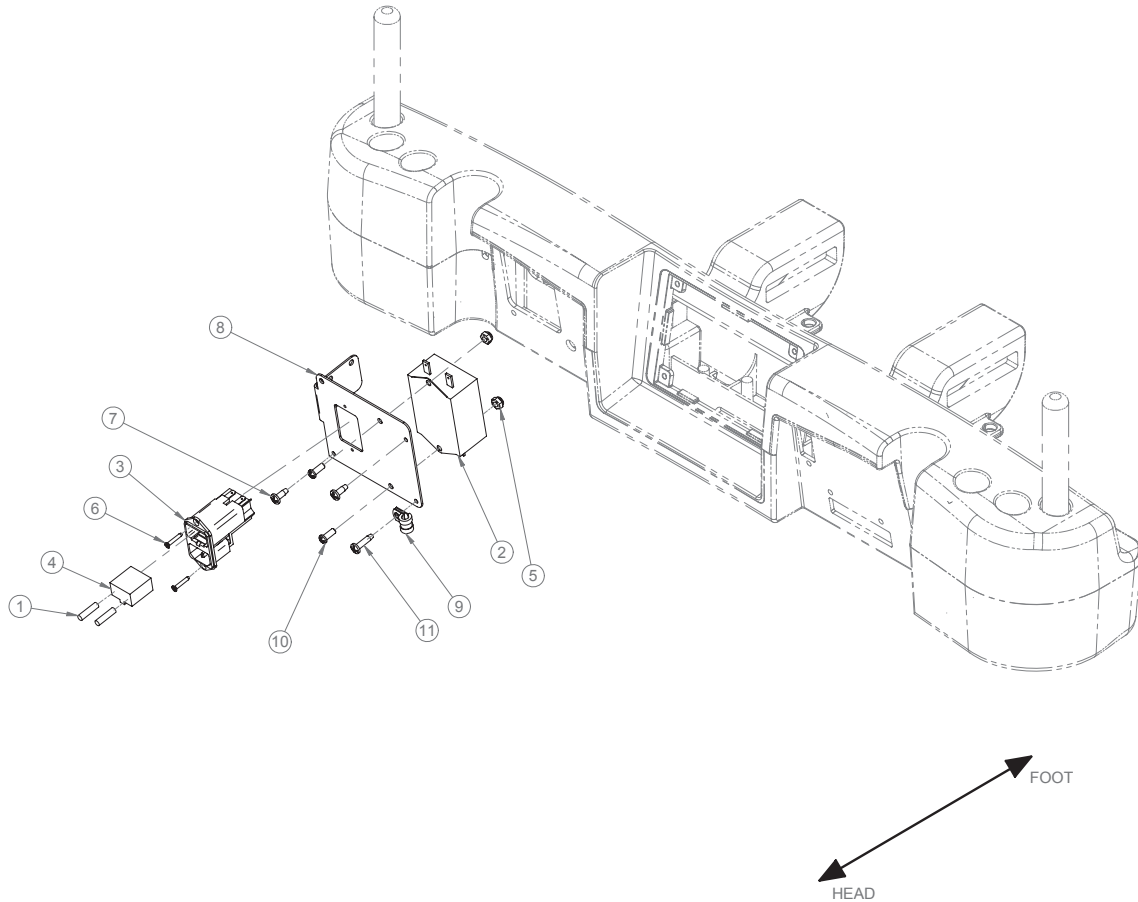

Item	Part No.	Part Name	Qty.
1	QDF8078	10A 250V Fuse	2
2	QDF9571	Medical Filer	1
3	QDF9574	Main Power Supply	1
4	QDF9575	Fuse Holder	1
5	VE30A0G	Nylon Hex. Locknut	2
6	VV41A1A20	Tapping Screw Flat Head Phillips	2
7	VV83A9G16	Tapping Screw Pan Head Phillips	2
8	27-1723P	Head Plate without Auxiliary Outlet	1
9	QDF2155	Steel Cable Clamp	1
10	VV33A0G16	Machine Screw Pan Head Phillips	2
11	VV83A9G24	Pan Head Tapping Screw	1

Litter Assembly, Optional Dual 120V Outlet

OL270013-XXX Rev-04 (Reference Only)

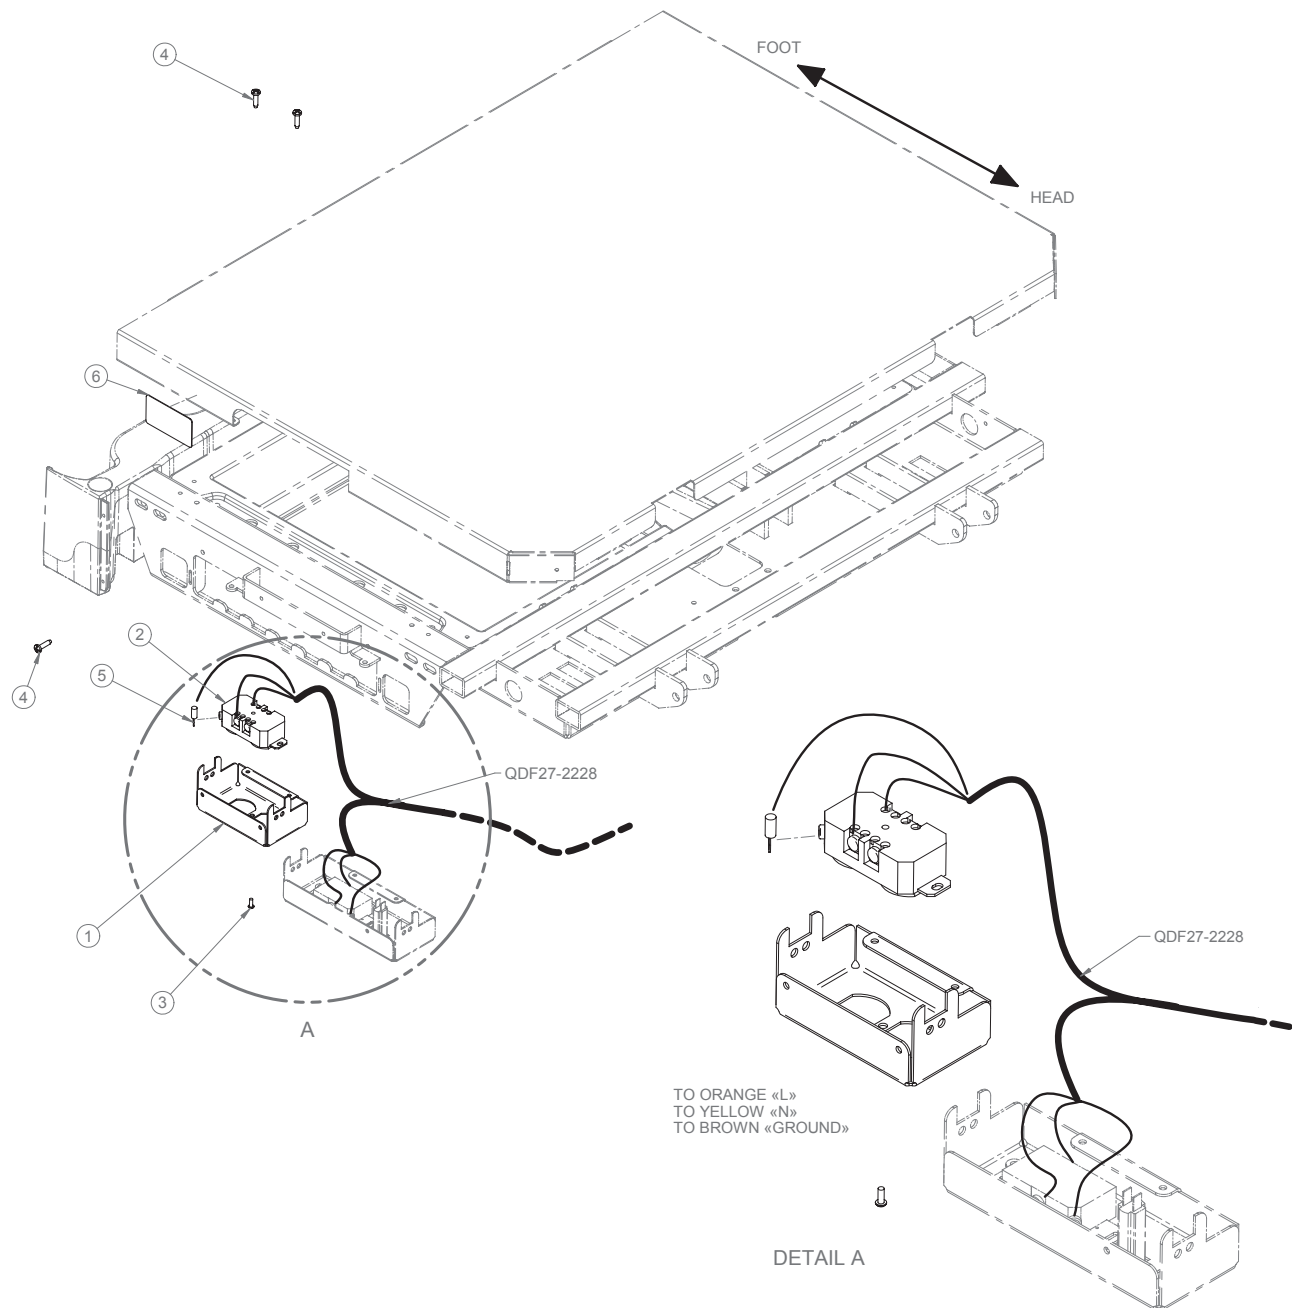

QDF27-2228 CABLE CONNECTION TABLE

Cable No	Connector No.	Cable No	Connector No.
QDF27-2228	J108A-L (Black)	QDF9573	"L"
QDF27-2228	J108A-N (White)	QDF9573	"N"
QDF27-2228	J108A-G (Green)	QDF9573	"GROUND"
QDF27-2228	J108B-L (Orange)	QDF8024	"L"
QDF27-2228	J108B-N (Yellow)	QDF8024	"N"
QDF27-2228	J108B-G (Brown)	QDF8024	"GROUND"

Litter Assembly, Optional Dual 120V Outlet

Litter Assembly, Optional Dual 120V Outlet - 270013-XXX Rev-04 (Reference Only)


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	27-1978P	Optional Auxiliary Outlet Box	1
2	QDF8024	Leviton 8200-w Double Outlet	1
3	VV37A1C12	Truss Head Machine Screw	1
4	VV83A9G24	Tapping Screw	3
5	QDF2124	Terminal #10 for 16-14 AWG	1
6	QE71-0964-XXX	Auxiliary Plug Label-XXX	1

Optional 100V Electric System

OL270205-XXX Rev E (Model 2131 Only) (For Reference Only)

OL270210-XXX Rev E (Model 2141 Only)

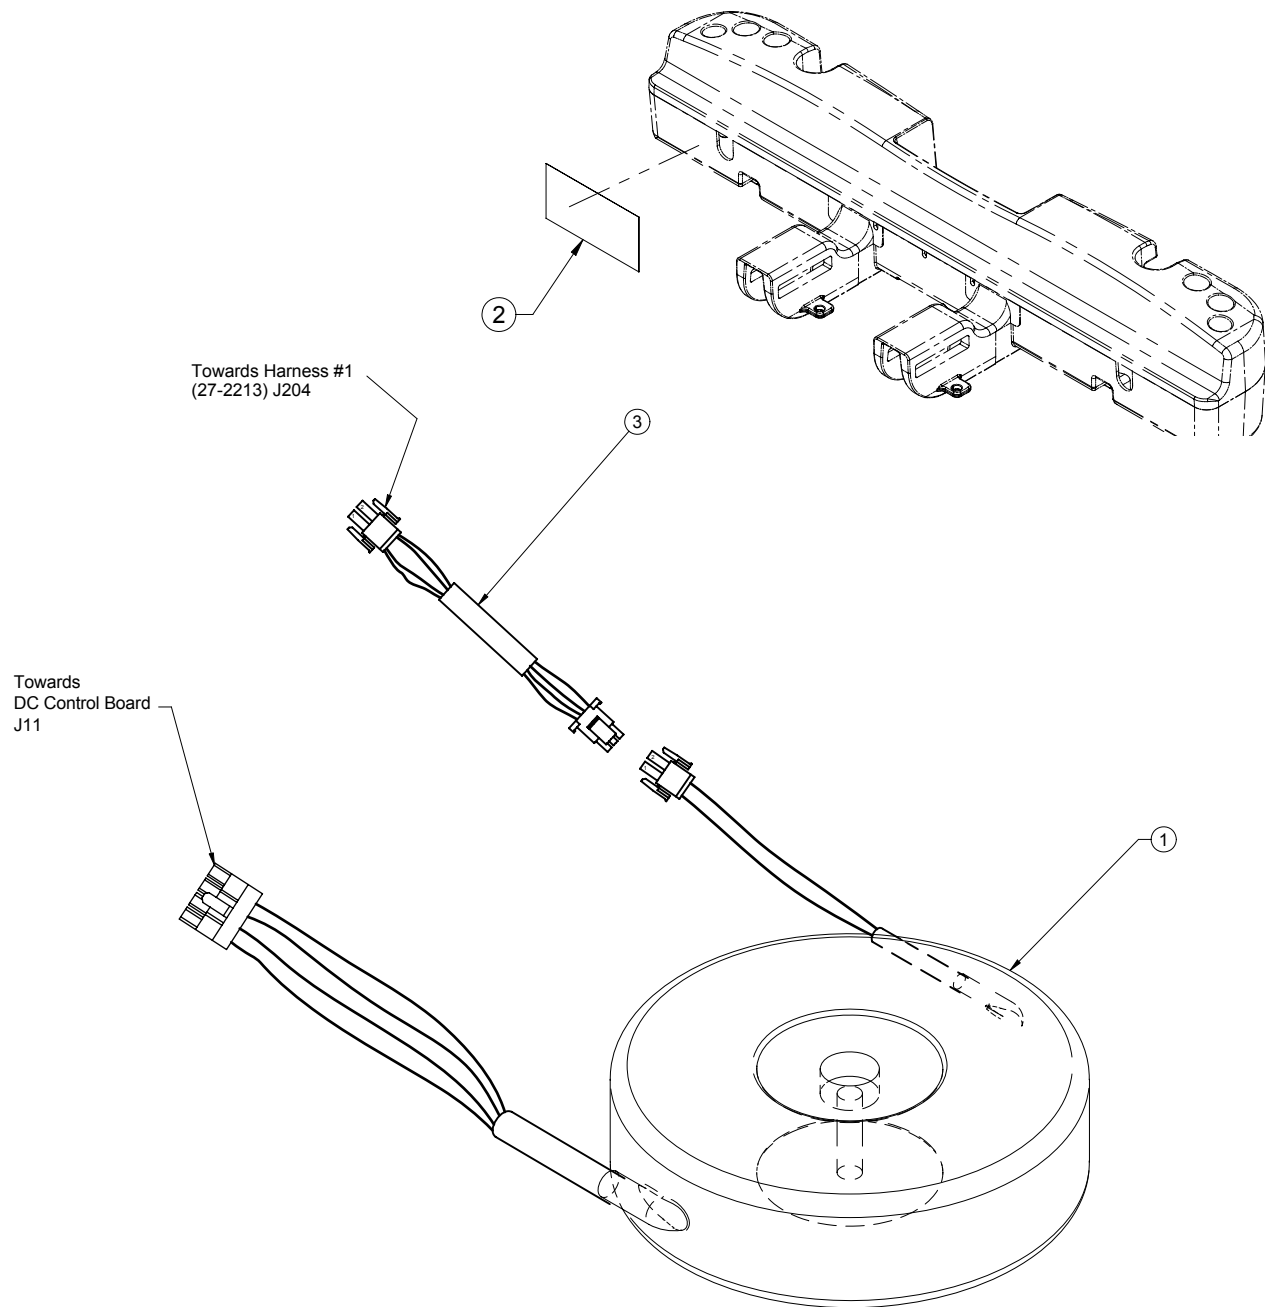


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF27-2049	International Medical Toroidal Transformer	1
2	QE71-1182-XXX	100V CSA Label (2131 Models Only)	1 or
	QE71-1187-XXX	100V CSA Label (2141 Models Only)	
3	QDF27-1841	100V Adapter	1

Optional 110V Electric System

OL270296-XXX Rev A (Model 2131 Only) (For Reference Only)

OL270297-XXX Rev A (Model 2141 Only)

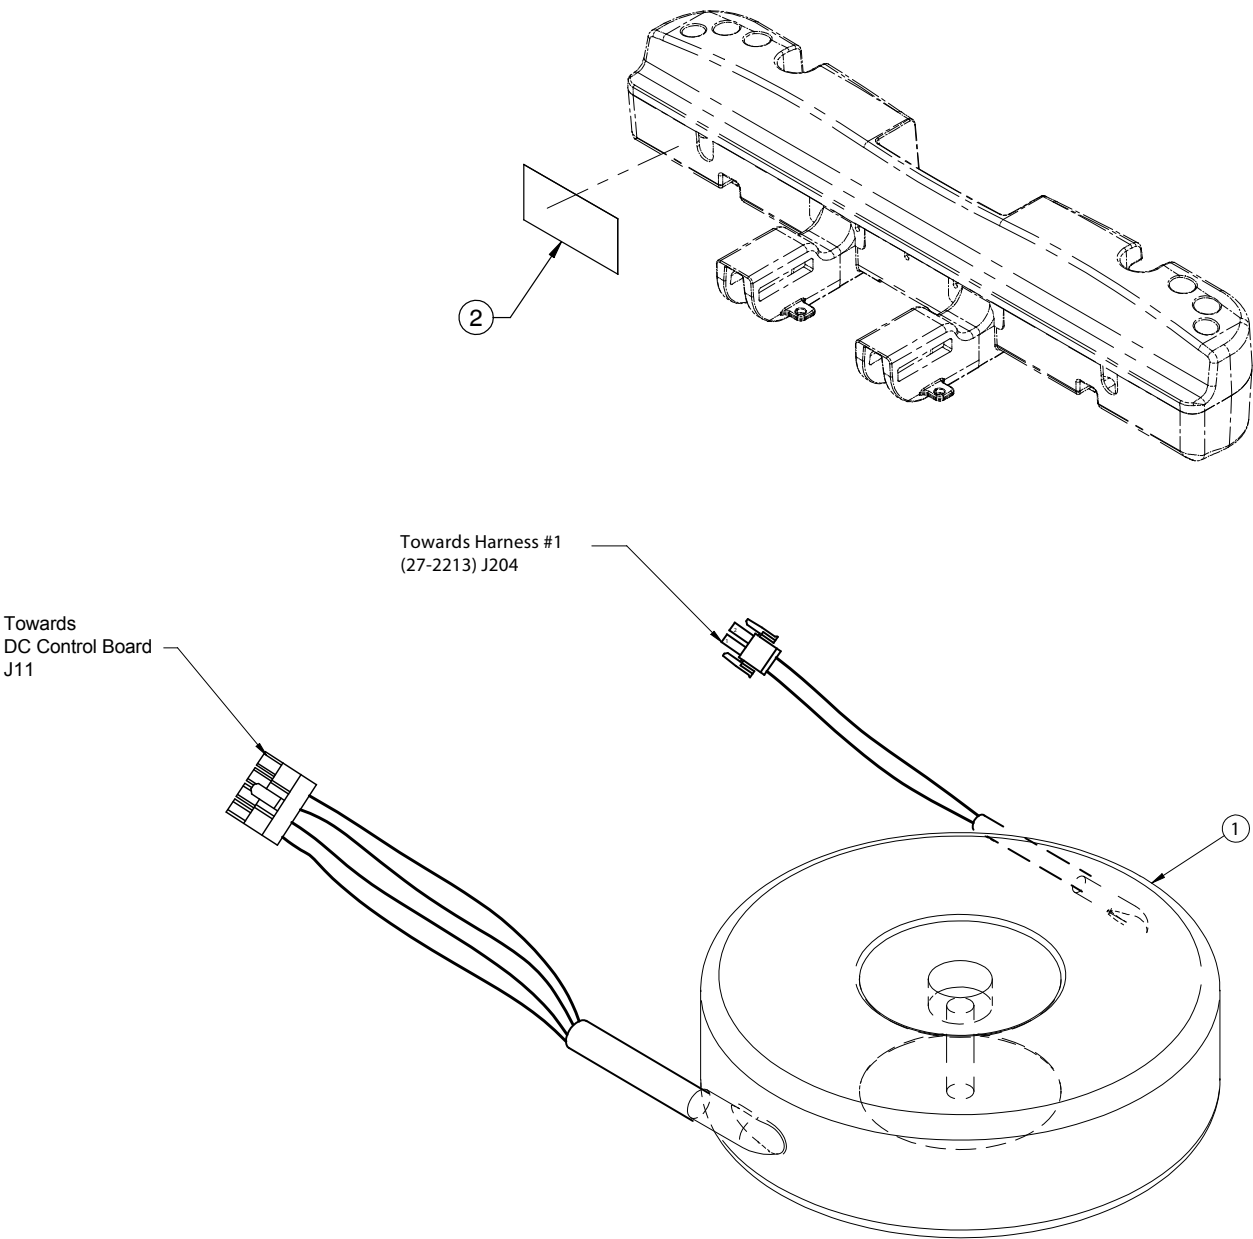


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF27-2659	International Medical Toroidal Transformer	1
2	QE71-1353-XXX	110V CSA Label (2131 Models Only)	1 or
	QE71-1352-XXX	110V CSA Label (2141 Models Only)	

Optional 200V Electric System

OL270207-XXX Rev E (Model 2131 Only) (For Reference Only)

OL270212-XXX Rev E (Model 2141 Only)

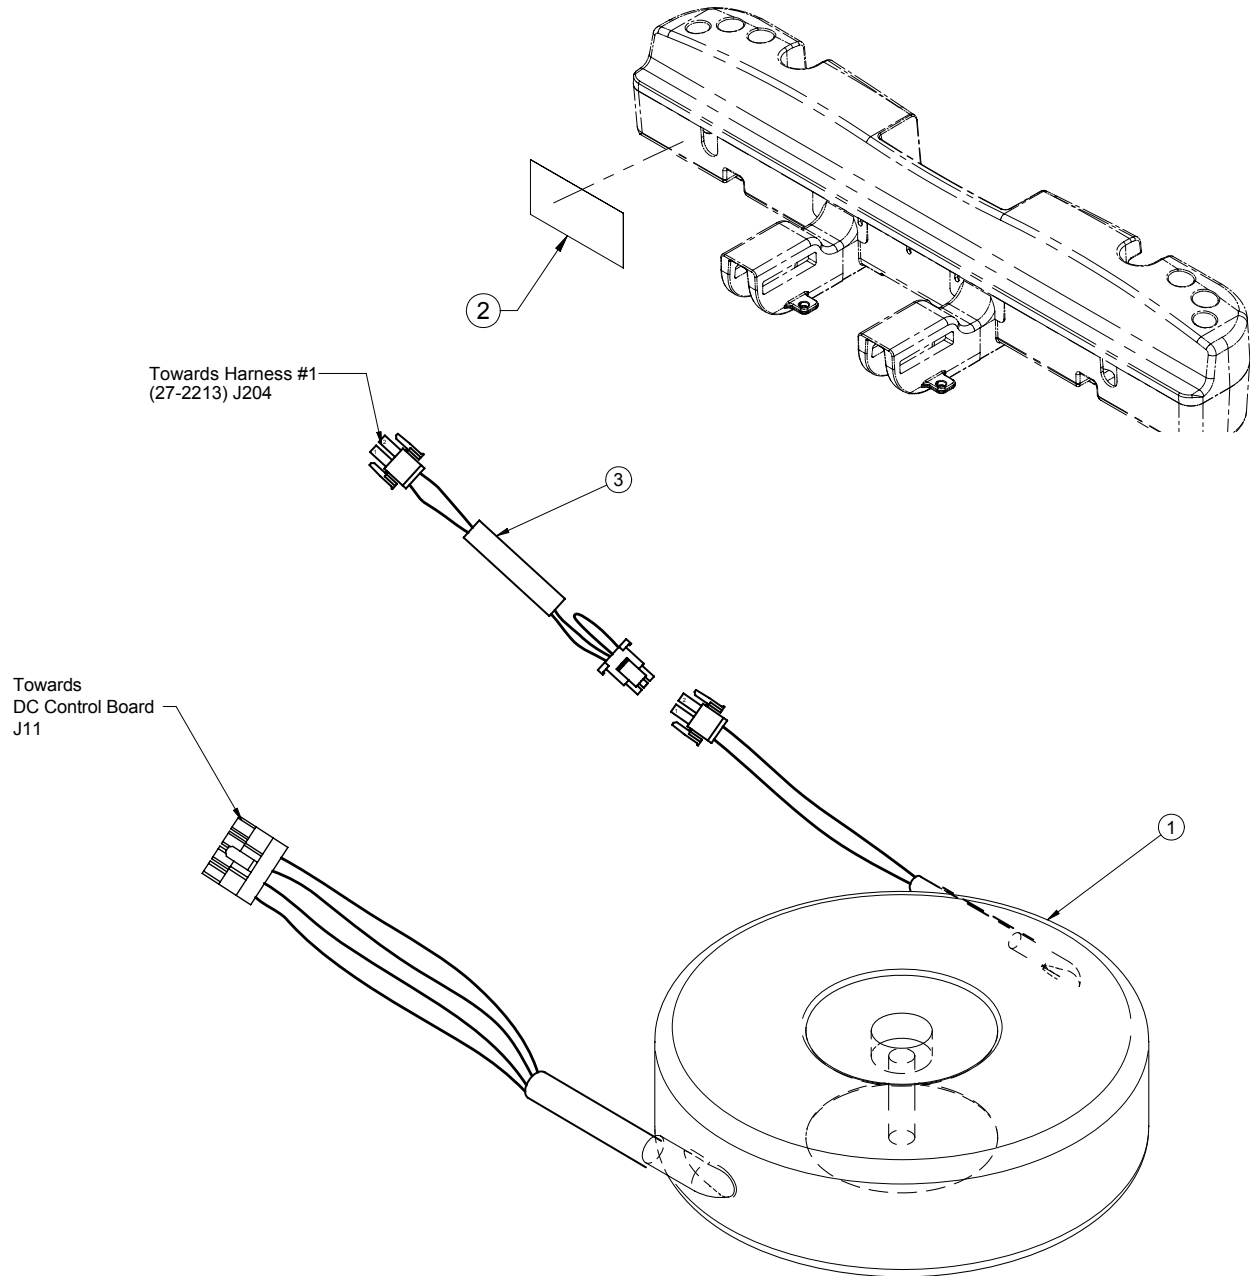


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF27-2049	International Medical Toroidal Transformer	1
2	QE71-1184-XXX	200V CSA Label (2131 Models Only)	1 or
	QE71-1189-XXX	200V CSA Label (2141 Models Only)	
3	QDF27-1842	200V Adapter	1

Optional 220V Electric System

OL270208-XXX Rev E (Model 2131 Only) (For Reference Only)
OL270213-XXX Rev E (Model 2141 Only)

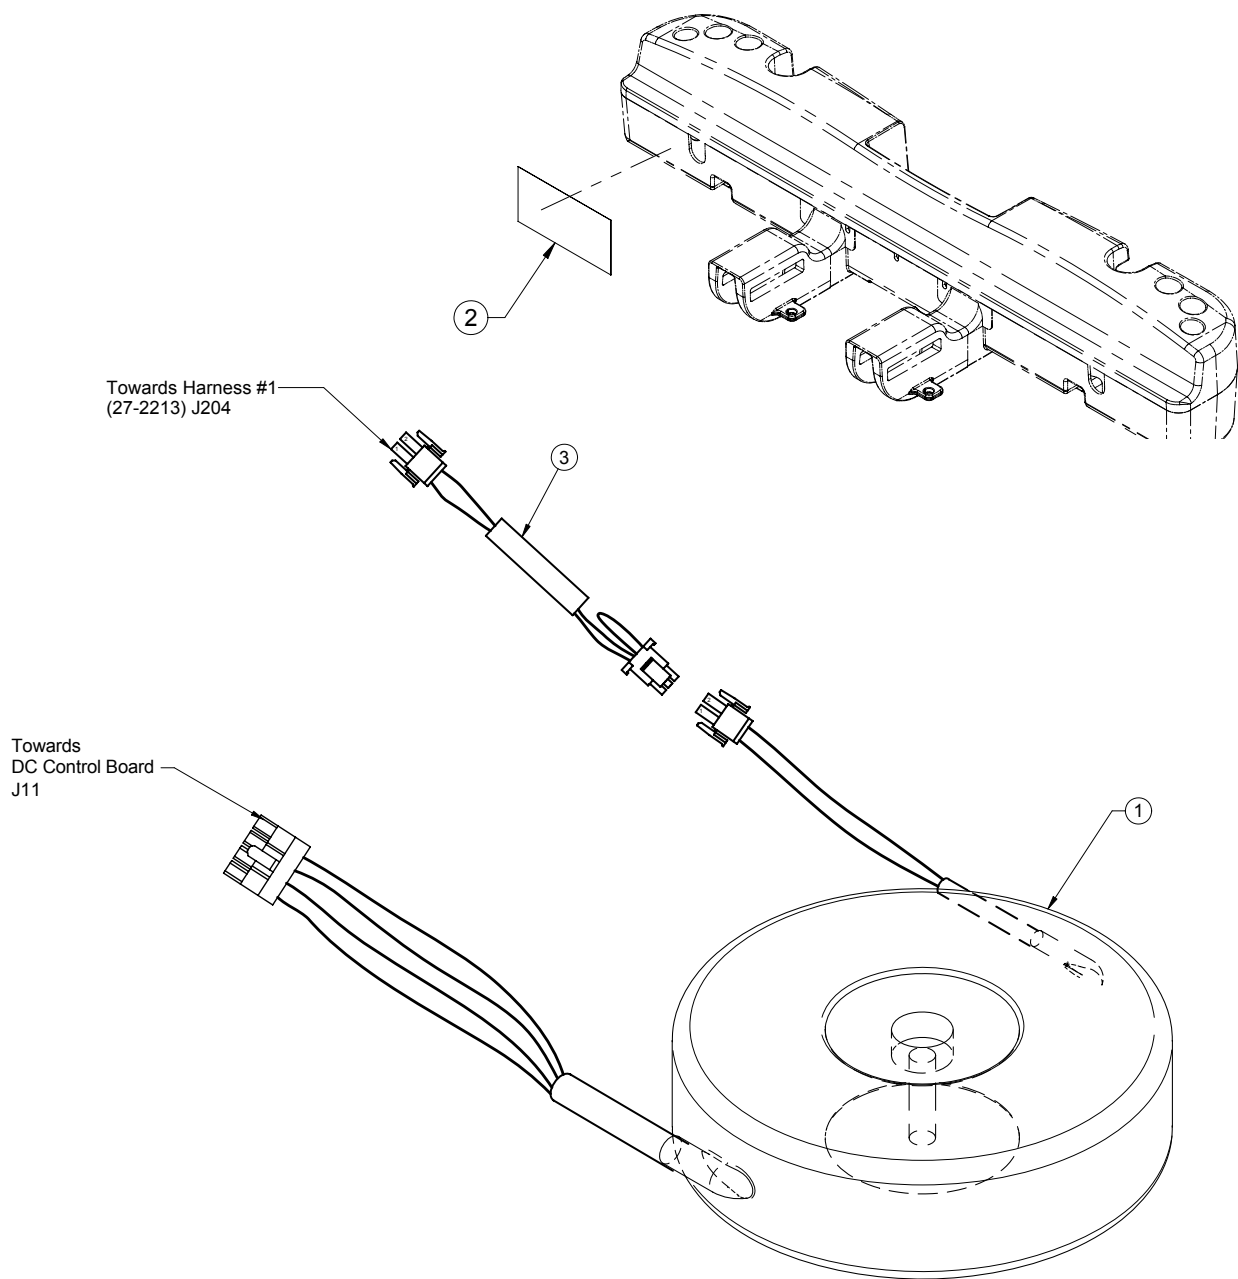


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF27-2049	International Medical Toroidal Transformer	1
2	QE71-1185-XXX	220V CSA Label (2131 Models Only)	1 or
	QE71-1190-XXX	220V CSA Label (2141 Models Only)	
3	QDF27-1843	220V Adapter	1

Optional 240V Electric System

OL270209-XXX Rev E (Model 2131 Only) (For Reference Only)
OL270214-XXX Rev E (Model 2141 Only)

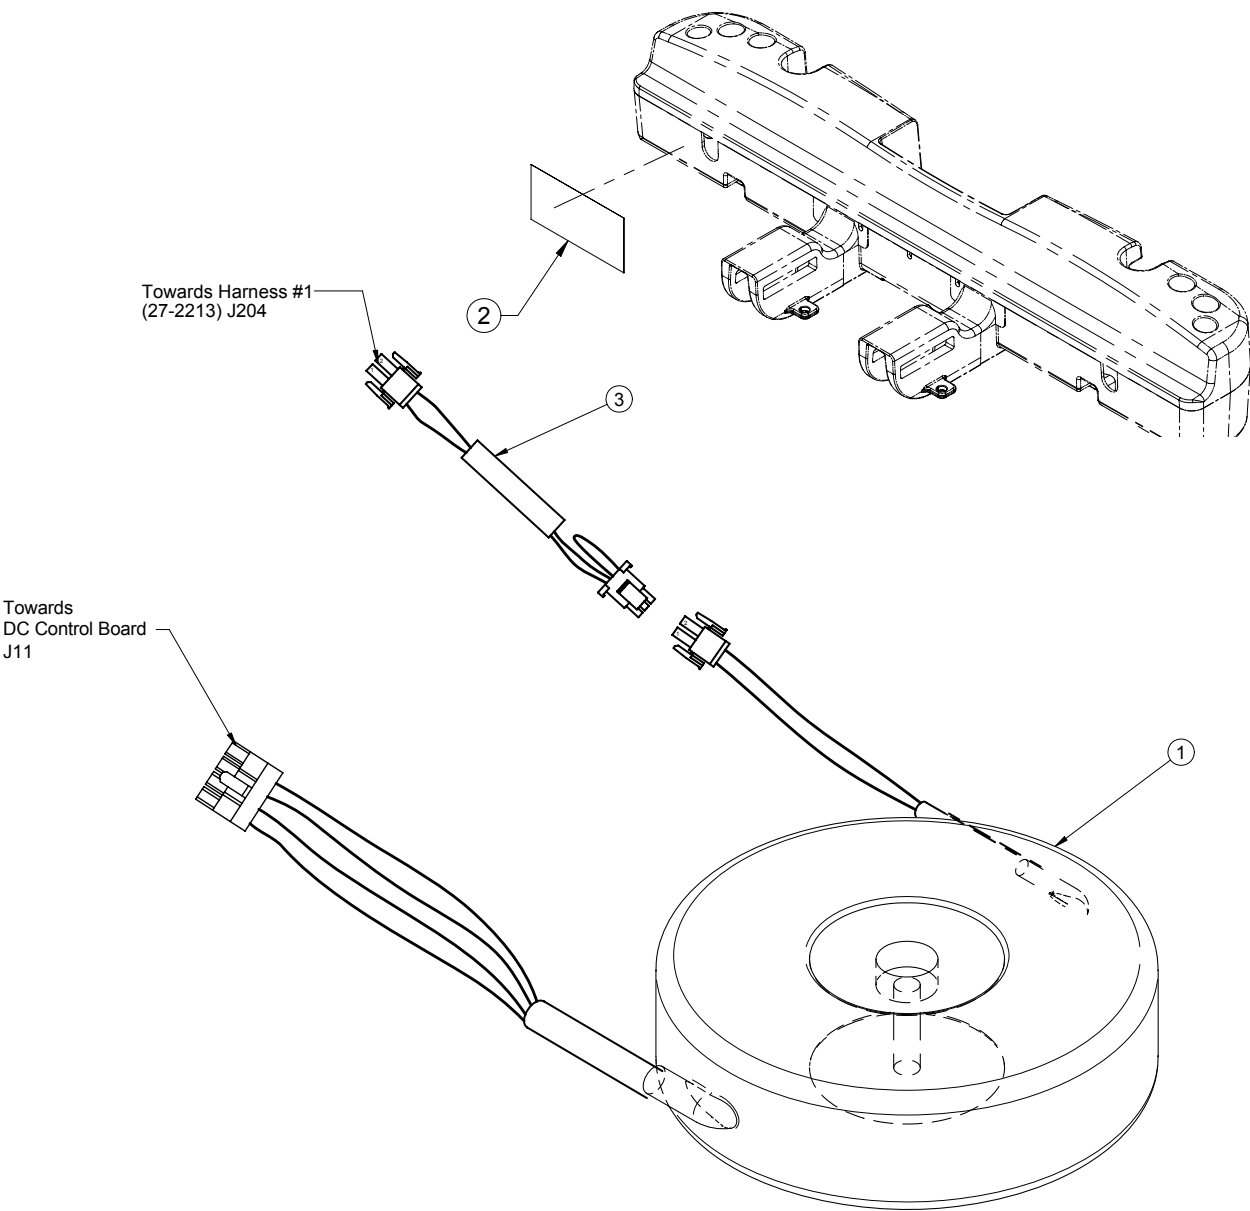


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF27-2049	International Medical Toroidal Transformer	1
2	QE71-1186-XXX	240V CSA Label (2131 Models Only)	1 or
	QE71-1191-XXX	240V CSA Label (2141 Models Only)	
3	QDF27-1840	240V Adapter	1

CPR Assembly, Mechanical


L27-033 Rev-09 (Reference Only)

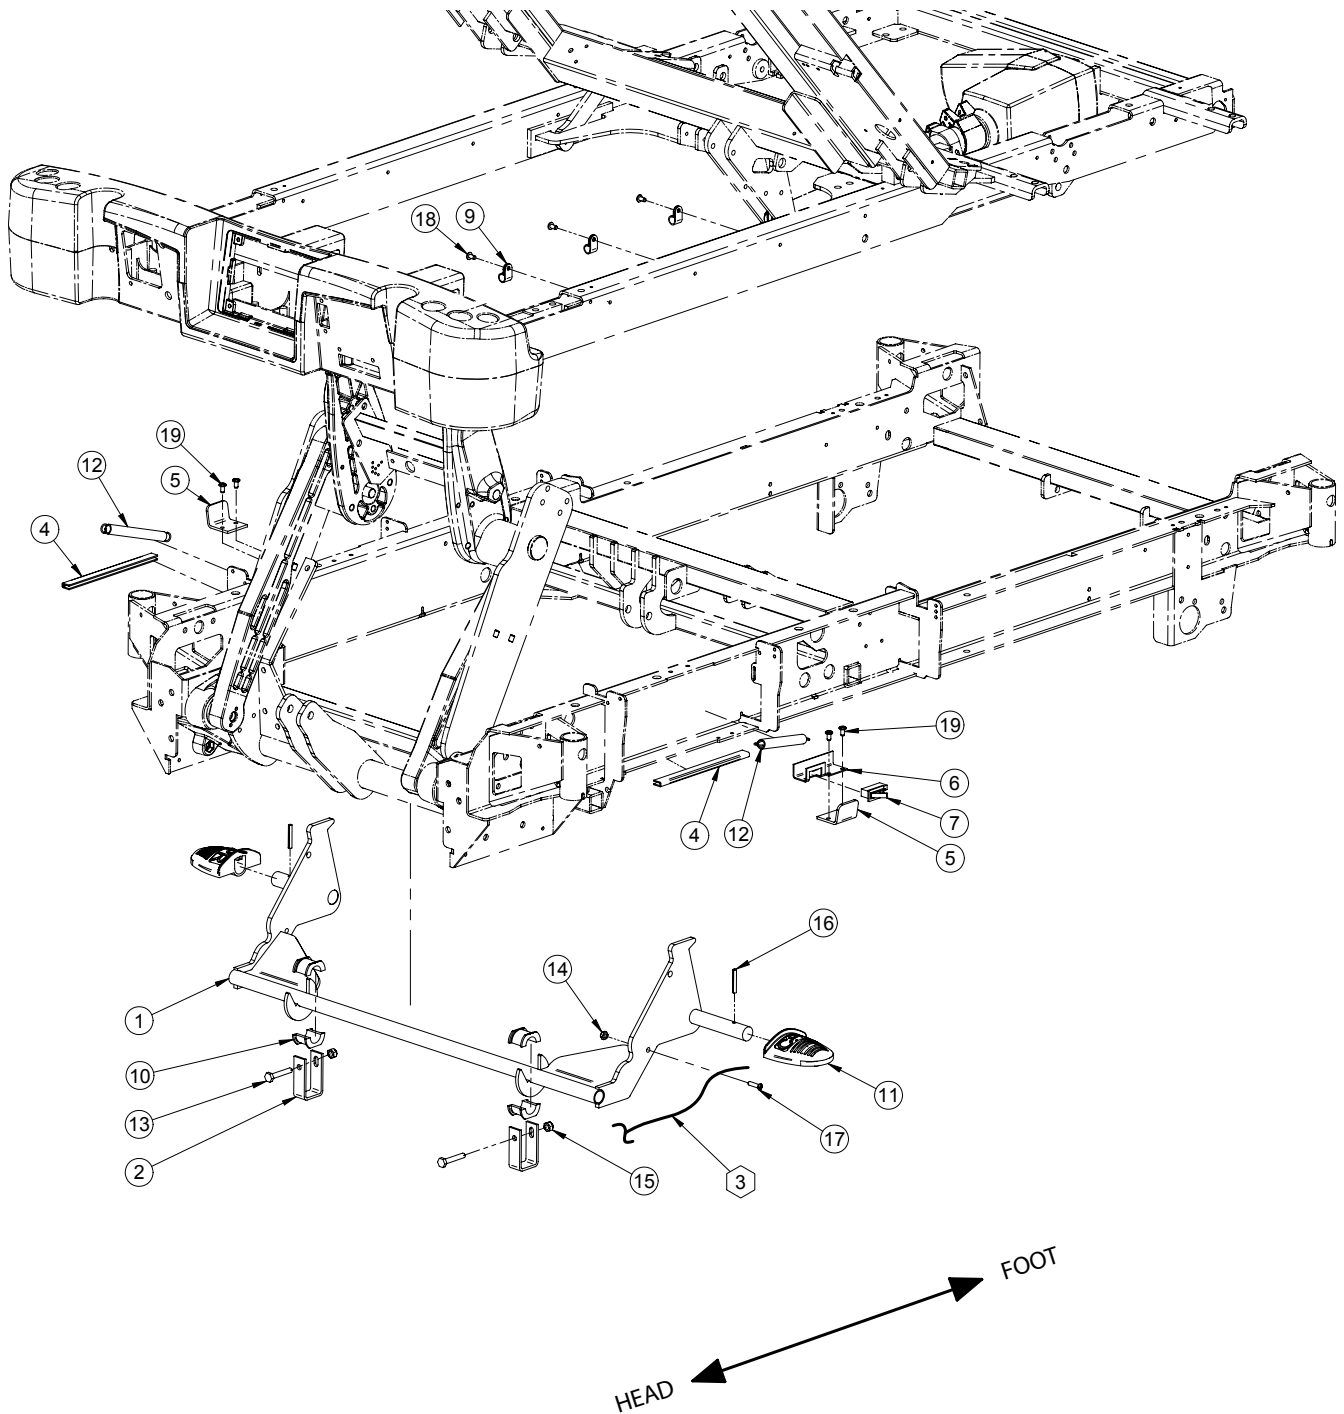

CPR Assembly, Mechanical

NOTE: For Cable Routing

- The Fowler must at 30° when installing the cable.
- There must be no tie installed on the actuator

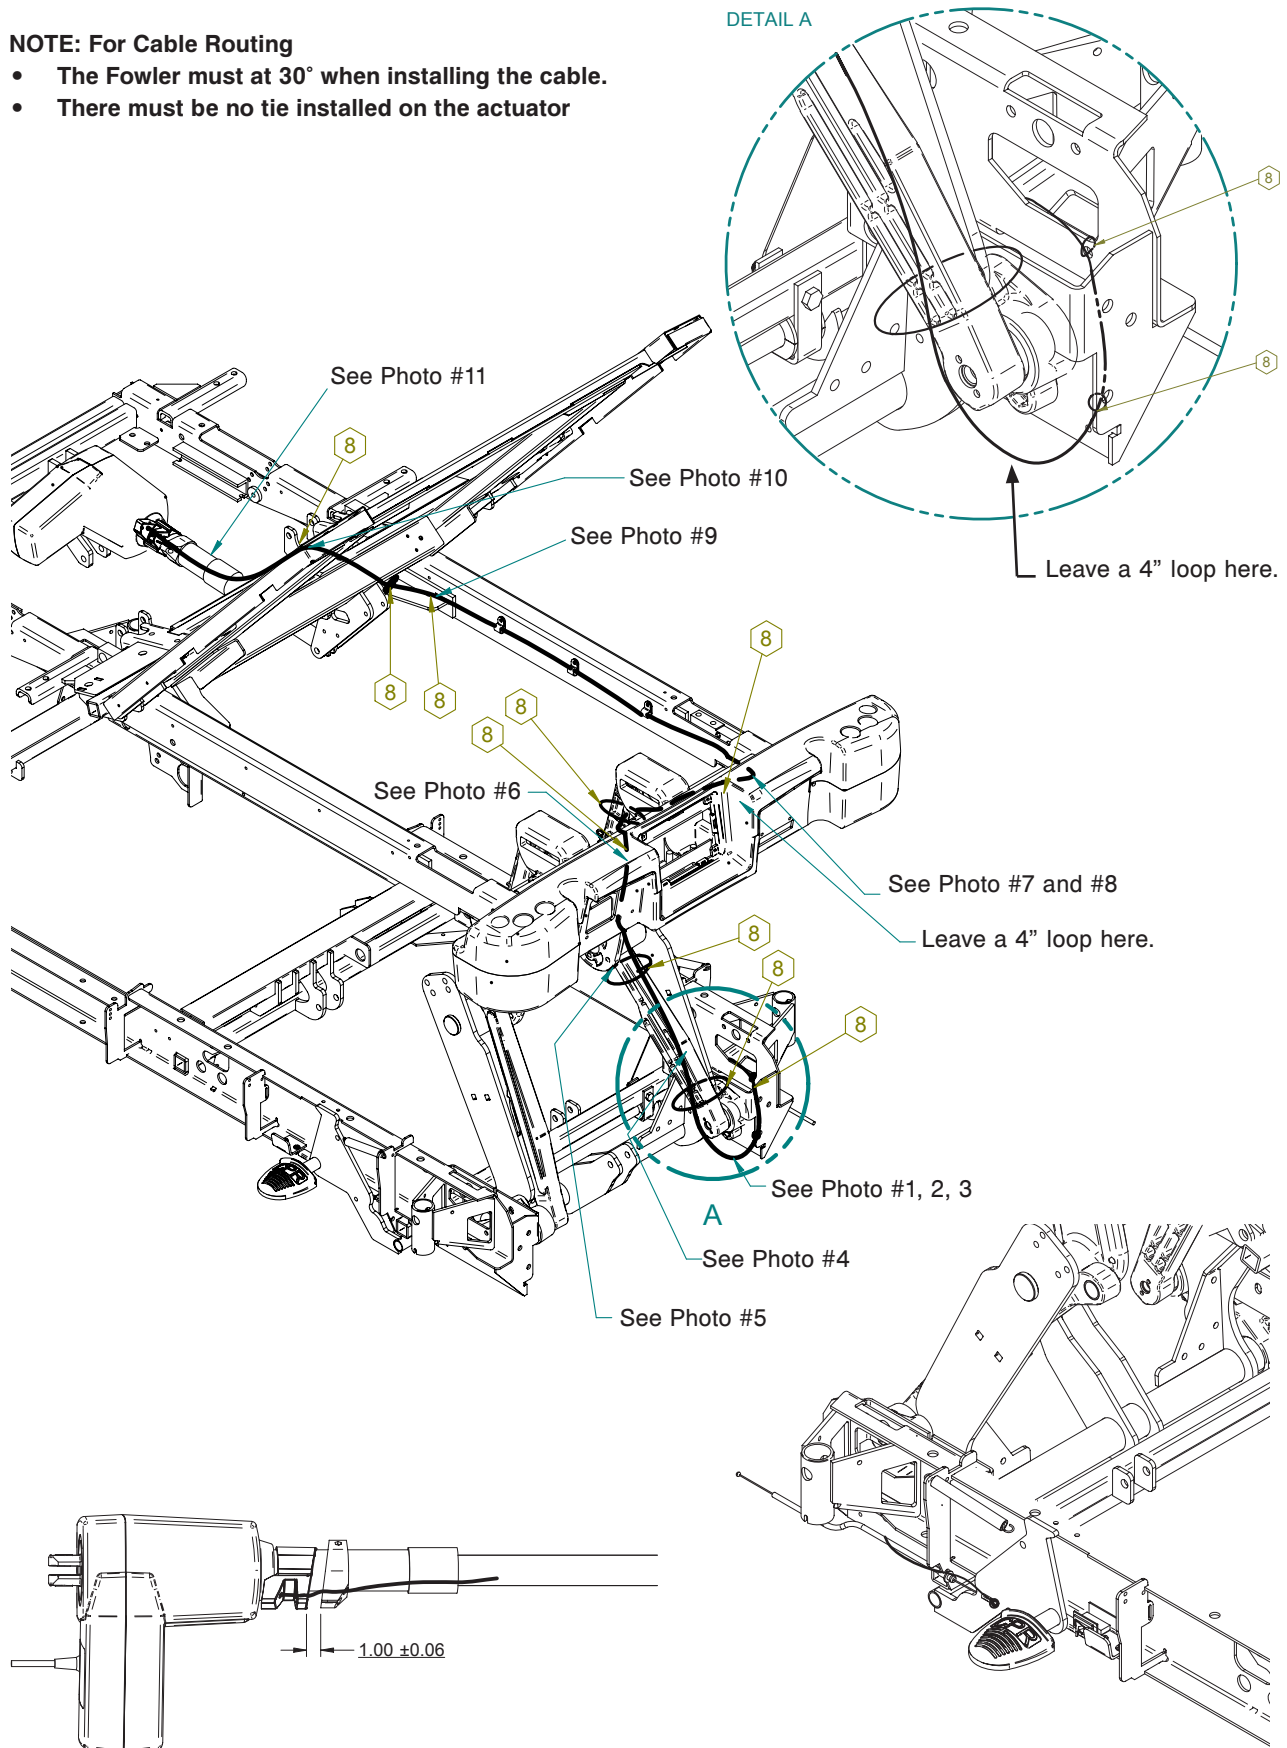

CPR Assembly, Mechanical

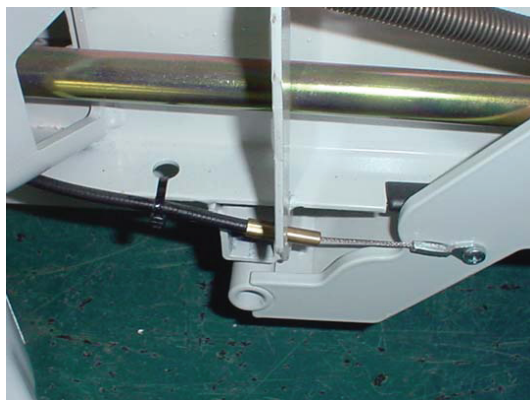


Photo #1



Photo #2



Photo #3



Photo #4

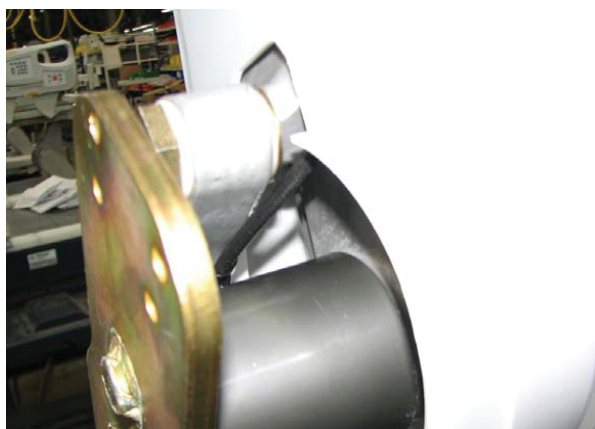


Photo #5



Photo #6

CPR Assembly, Mechanical



Photo #7



Photo #8



Photo #9

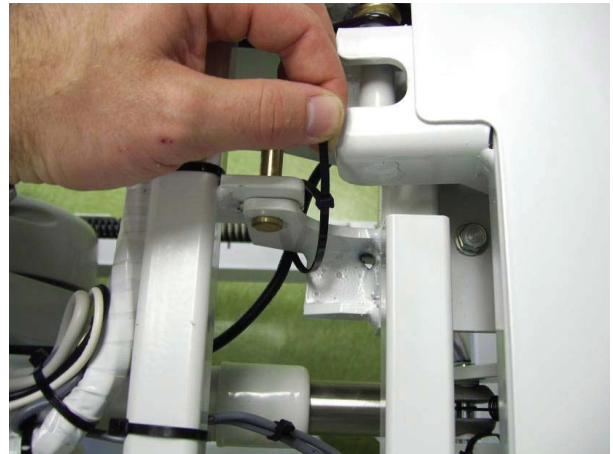


Photo #10



Photo #11

CPR Assembly, Mechanical

CABLE CONNECTION TABLE			
Cable No.	Connector No.	Cable No.	Connector No.
QDF2083	CPR Switch	QDF27-1204	J127


CPR Assembly, Mechanical - L27-033 Rev-09 (Reference Only)

Item	Part No.	Part Name	Qty.
1	27-1897P	CPR Pedal	1
2	27-1917Z	CPR Support	2
3	27-1966	CPR Cable	1
4	27-2036	CPR Lateral Stop	2
5	27-2062Z	CPR Pedal Stopper	2
6	27-2086Z	CPR Switch Support	1
7	QDF2083	Lever Switch	1
8	QDF9518	Cable Tie	12
9	QDF2155	Steel Cable Clamp	3
10	QP19-0270	Shaft Support Bearing	4
11	QP27-2065	CPR Pedal	2
12	QRE23-0438	Siderail Spring	2
13	VB15A1N44	Bolt	2
14	VE30A0G	Nylon Locknut	1
15	VE30A1N	Nylon Locknut	2
16	VG10B0636	Spring Pin	2
17	VV33A0G24	Pan Head Machine Screw	1
18	VV83A9G12	Pan Head Tapping Screw	3
19	VV83A9G16	Pan Head	4

Handle Assembly (Model 2131 Only)

(Applies to beds with Serial Numbers U01001 - U51437)

OL270058-XXX Rev-05 (Reference Only)

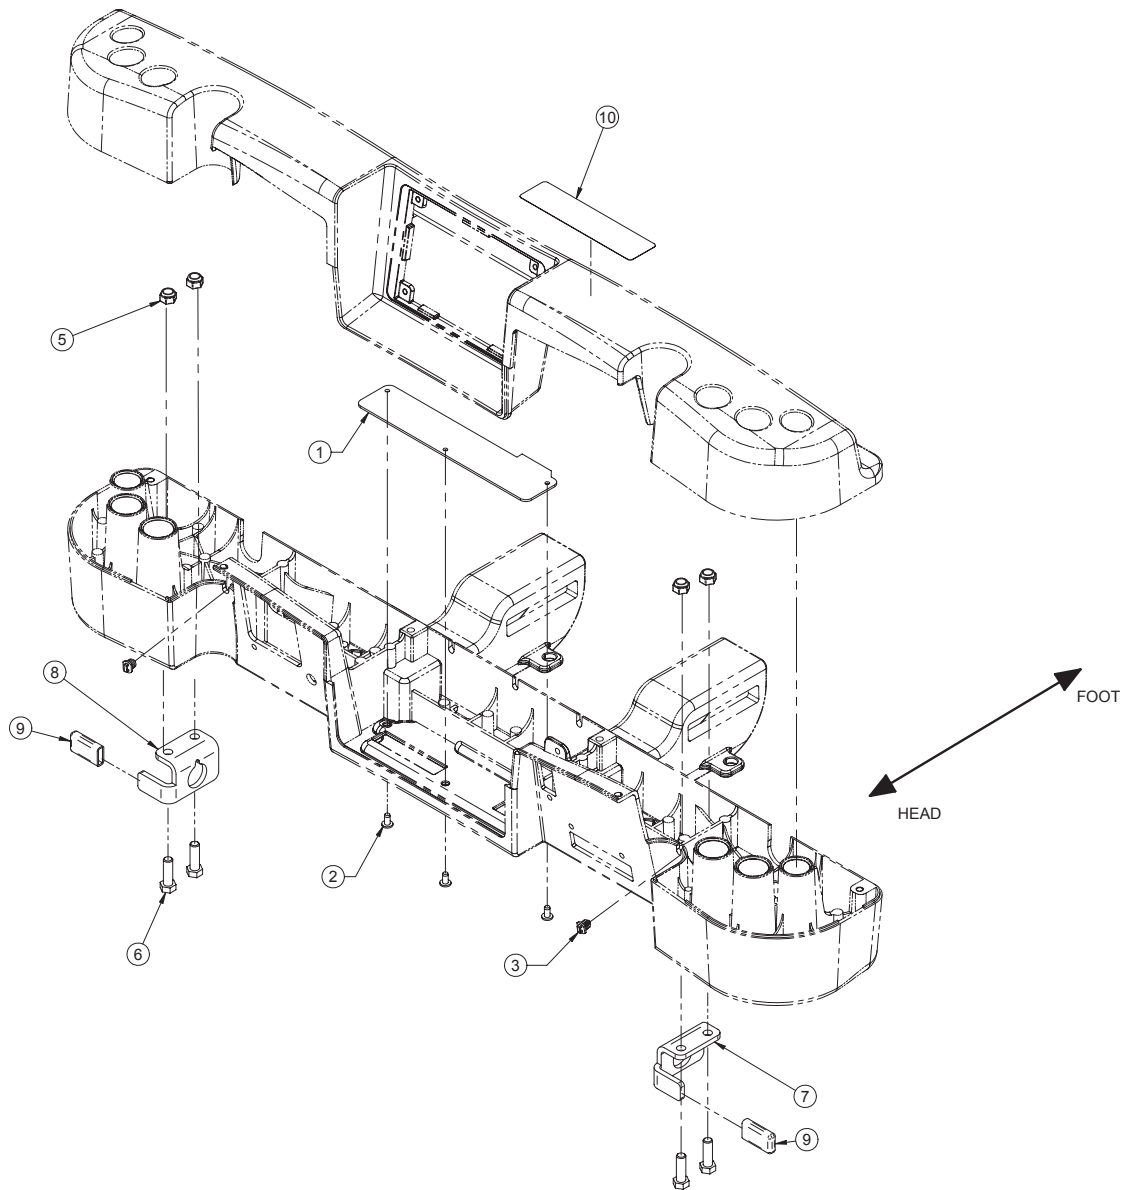


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	27-1651P	Without 5th Wheel Plate	1
2	VV83A9G12	Tapping Screw	3
3	QDF5096	Plastic Tie	2
5	VE30A1O	Nylon Self-Locking Nut	4
6	VB15A1O32	Hex Bolt	4
7	27-2272Z	Zoom® Handle Bracket, Right	1
8	27-2273Z	Zoom® Handle Bracket, Left	1
9	QDF2131	Yellow Flat Vinyl Cap	2
10	QE71-1176-XXX	Sticker, Electric Cable Rolling Up	1

Handle Assembly (Model 2131 Only)

(Applies to beds with Serial Numbers U51438 - Current)

OL270058-XXX Rev G (Reference Only)

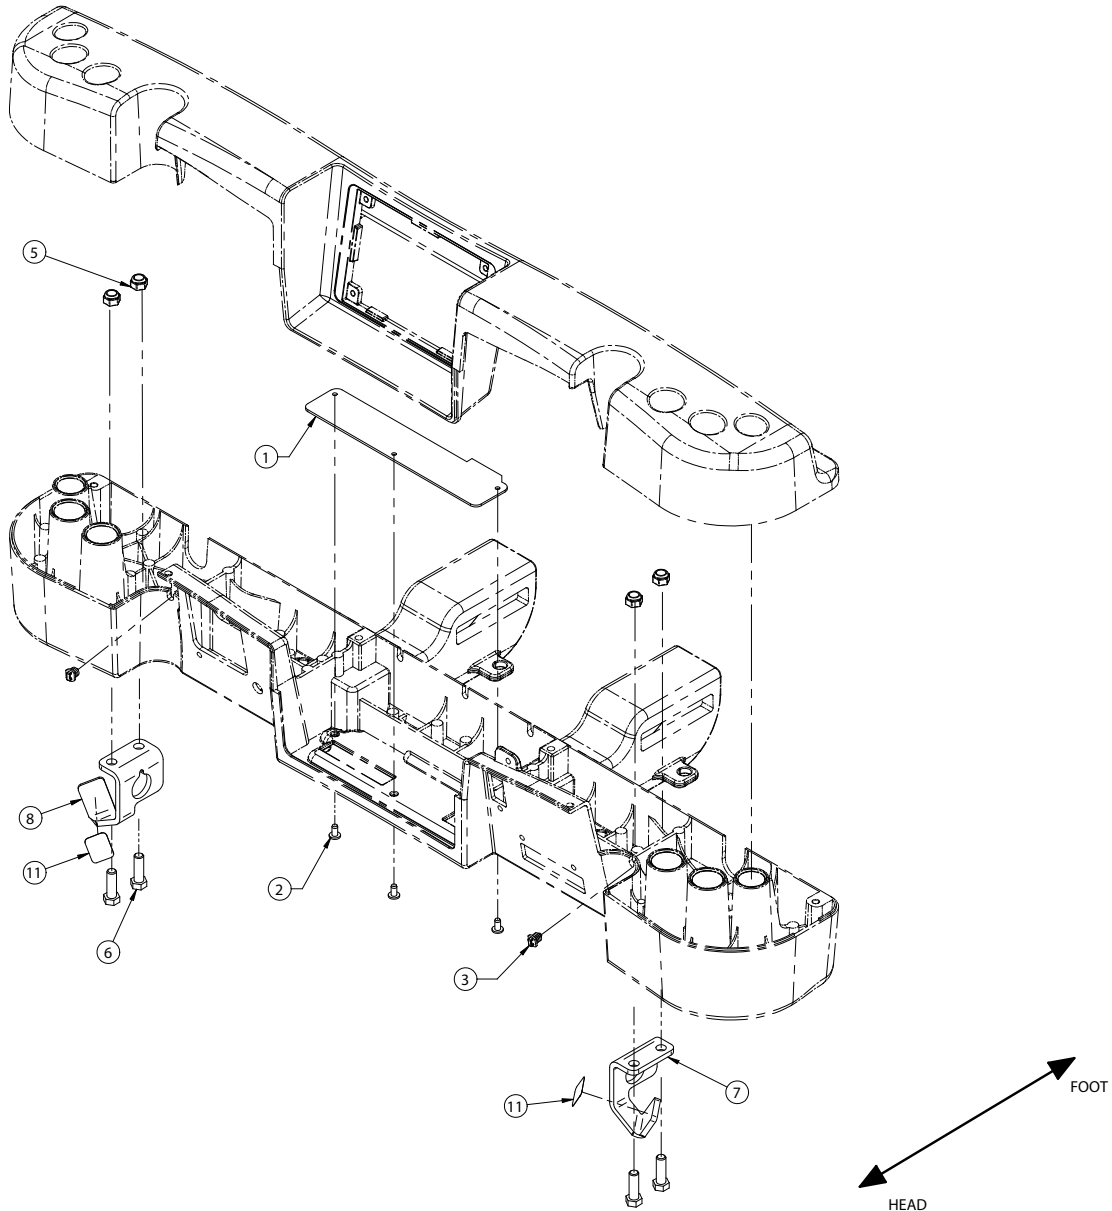

NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)


Item	Part No.	Part Name	Qty.
1	27-1651P	Without 5th Wheel Plate	1
2	VV83A9G12	Pan Head Tapping Screw	3
3	QDF5096	Plastic Tie	2
5	VE30A1O	Nylon Hex Locknut	4
6	VB15A1O32	Bolt	4
7	27-2790P	Zoom® Handle Bracket, Right	1
8	27-2789P	Zoom® Handle Bracket, Left	1
11	QE71-1373	Coiled Power Cord Label	2

Zoom® Handle Assembly (Model 2141 Only)

(Applies to beds with Serial Numbers U01001 - U04982)

(Excluding U03258 and U03259)

27-0900 Rev-10 (Reference Only)

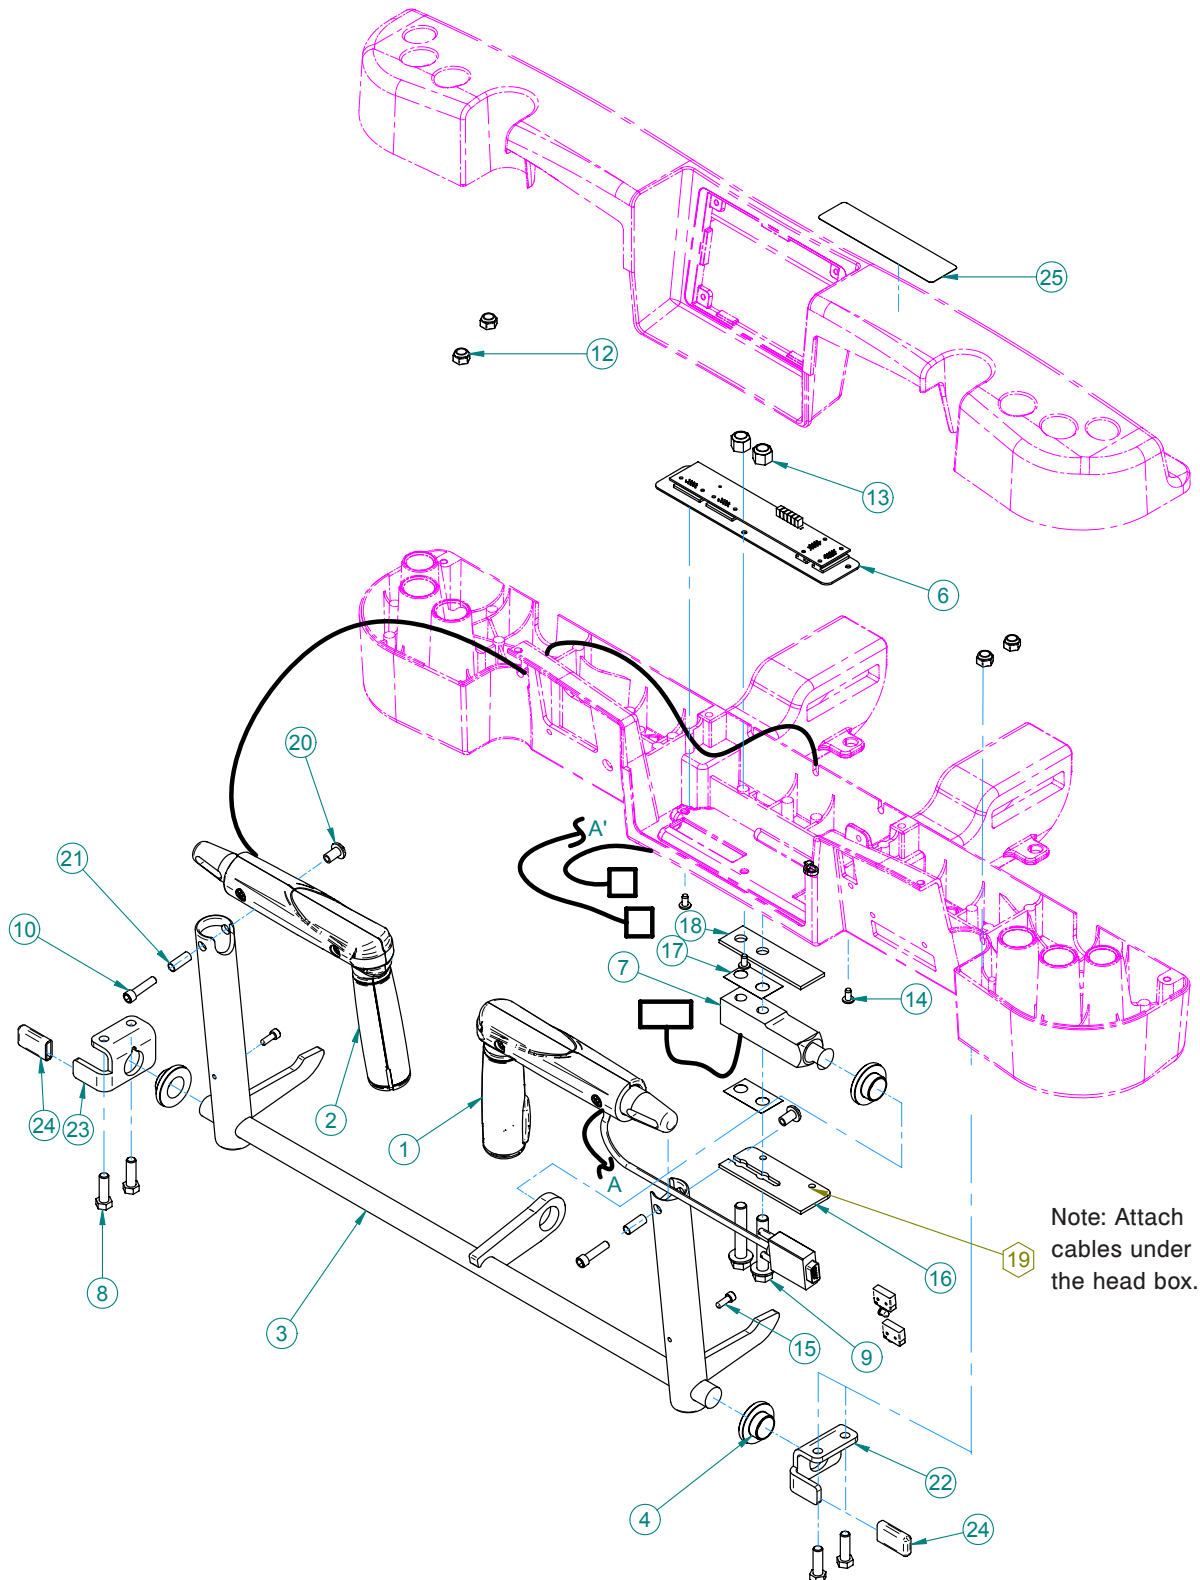


Note: Attach
cables under
the head box.

Zoom® Handle Assembly (Model 2141 Only)

*(Applies to beds with Serial Numbers U01001 - U04982)
(Excluding U03258 and U03259)*

Board CSI 1157 Connection

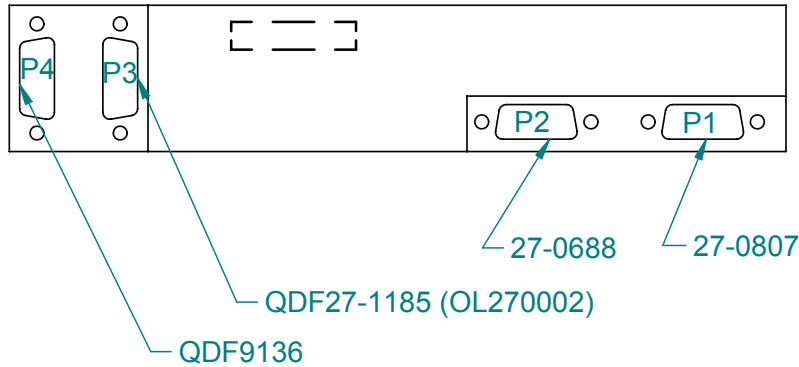

Zoom® Handle Assembly - Common Components - 27-0900 Rev-10 (Reference Only)


Item	Part No.	Part Name	Qty.
1	27-0688	Right Zoom® Handle	1
2	27-0807	Left Zoom® Handle	1
3	27-0880C	Tie Bus	1
4	27-1181	Zoom® Handle Sleeve	3
6	27-1371	Board CSI 1157	1
7	QDF9136	250 lbs Load Cell	1
8	VB15A1O32	Bolt	4
9	VB95A1P48	Hexagon Neck Bolt	2
10	VD60B1N32-S	Shoulder Screw	2
12	VE30A1O	Nylon Locknut	4
13	VE30A1P	Nylon Locknut	2
14	VV83A9G12	Phillips Head Tapping Screw	3
15	VV10A0G16-S	Hex Head Screw	2
16	27-1857Z	Bottom Zoom® Load Cell Stopper	1
17	QDF27-1780	Load Cell Spacer	2
18	27-1775Z	Zoom® Load Cell Stopper	1
19	QDF9518	Nylon Tie-Wrap	1
20	QDF2121	Barrel Nut	2
21	27-2249Z	Zoom® Handle Spacer	2
22	27-2272Z	Right Zoom® Handle Bracket	1
23	27-2273Z	Left Zoom® Handle Bracket	1
24	QDF2131	Flat Vinyl Cap	2
25	QE71-1176-T	Sticker, Electric Cable Rolling Up	1

Zoom® Handle Assembly (Model 2141 Only)

(Applies to beds with Serial Numbers U04983 - U51437)

(Including U03258 and U03259)


27-2547-XXX Rev-00 (Reference Only)

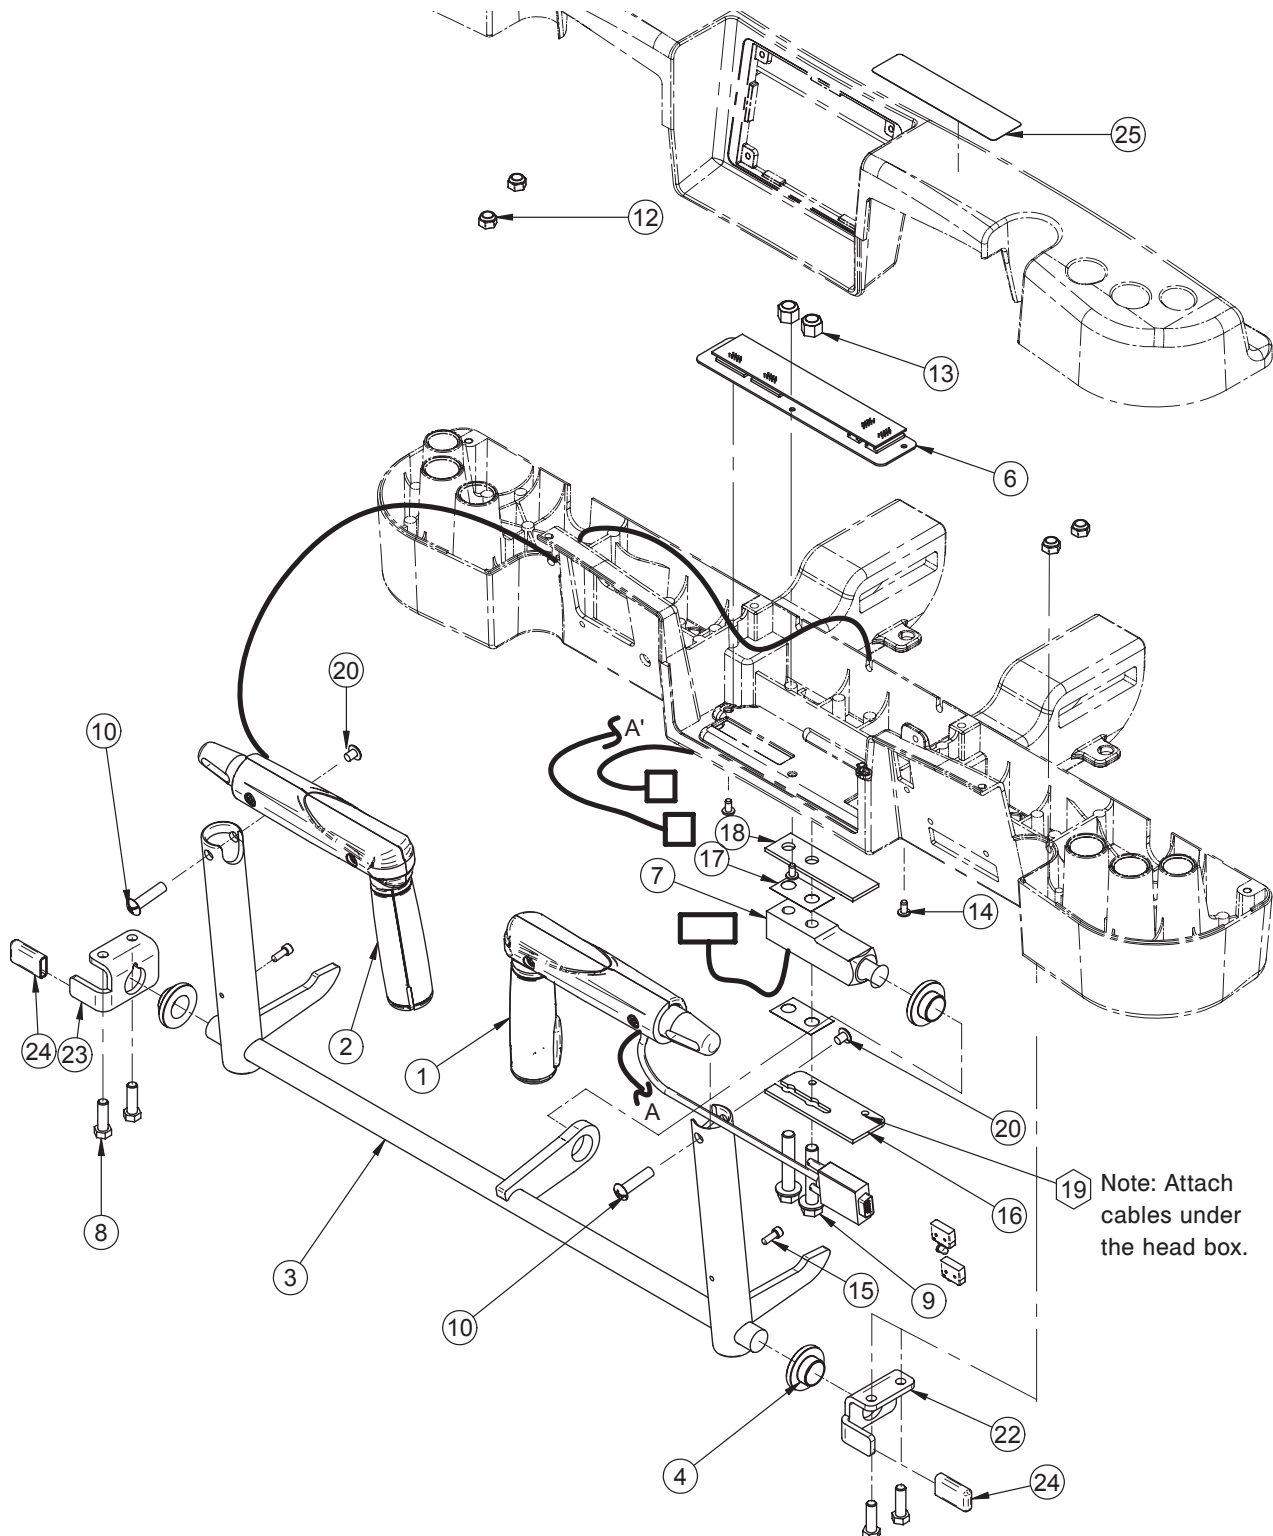

Zoom® Handle Assembly (Model 2141 Only)

(Applies to beds with Serial Numbers U04983 - U51437)
(Including U03258 and U03259)

27-2548 BOARD CONNECTION

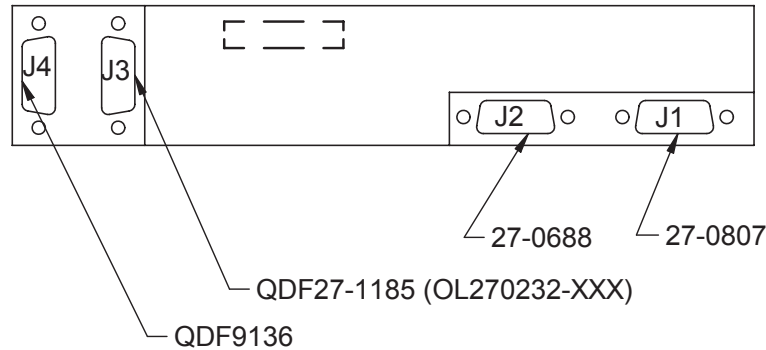

Zoom® Handle Assembly - 27-2547-XXX Rev-00 (Reference Only)


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	27-0688	Right Zoom® Handle	1
2	27-0807	Left Zoom® Handle	1
3	27-0880C	Tie Bus	1
4	27-1181	Zoom® Handle Sleeve	3
6	27-2548	Zoom® Control Board Assembly	1
7	QDF9136	250 lbs Load Cell	1
8	VB15A1O32	Bolt	4
9	VB95A1P48	Hex Neck Bolt	2
10	VE42A9036	Combination Barrel Nut	2
12	VE30A1O	Nylon Locknut	4
13	VE30A1P	Nylon Locknut	2
14	VV83A9G12	Phillips Head Tapping Screw	3
15	VV10A0G16-S	Hex Head Screw	2
16	27-1857Z	Bottom Zoom® Load Cell Stopper	1
17	QDF27-1780	Load Cell Spacer	2
18	27-1775Z	Zoom® Load Cell Stopper	1
19	QDF9518	Nylon Tie-Wrap	1
20	VV33A1N10-S	Machine Screw	2
22	27-2272Z	Right Zoom® Handle Bracket	1
23	27-2273Z	Left Zoom® Handle Bracket	1
24	QDF2131	Flat Vinyl Cap	2
25	QE71-1176-XXX	Electric Cable Rolling Up Label	1

Zoom® Handle Assembly (Model 2141 Only)

(Applies to beds with Serial Numbers U51438 - Current)


27-2547-XXX Rev B (Reference Only)

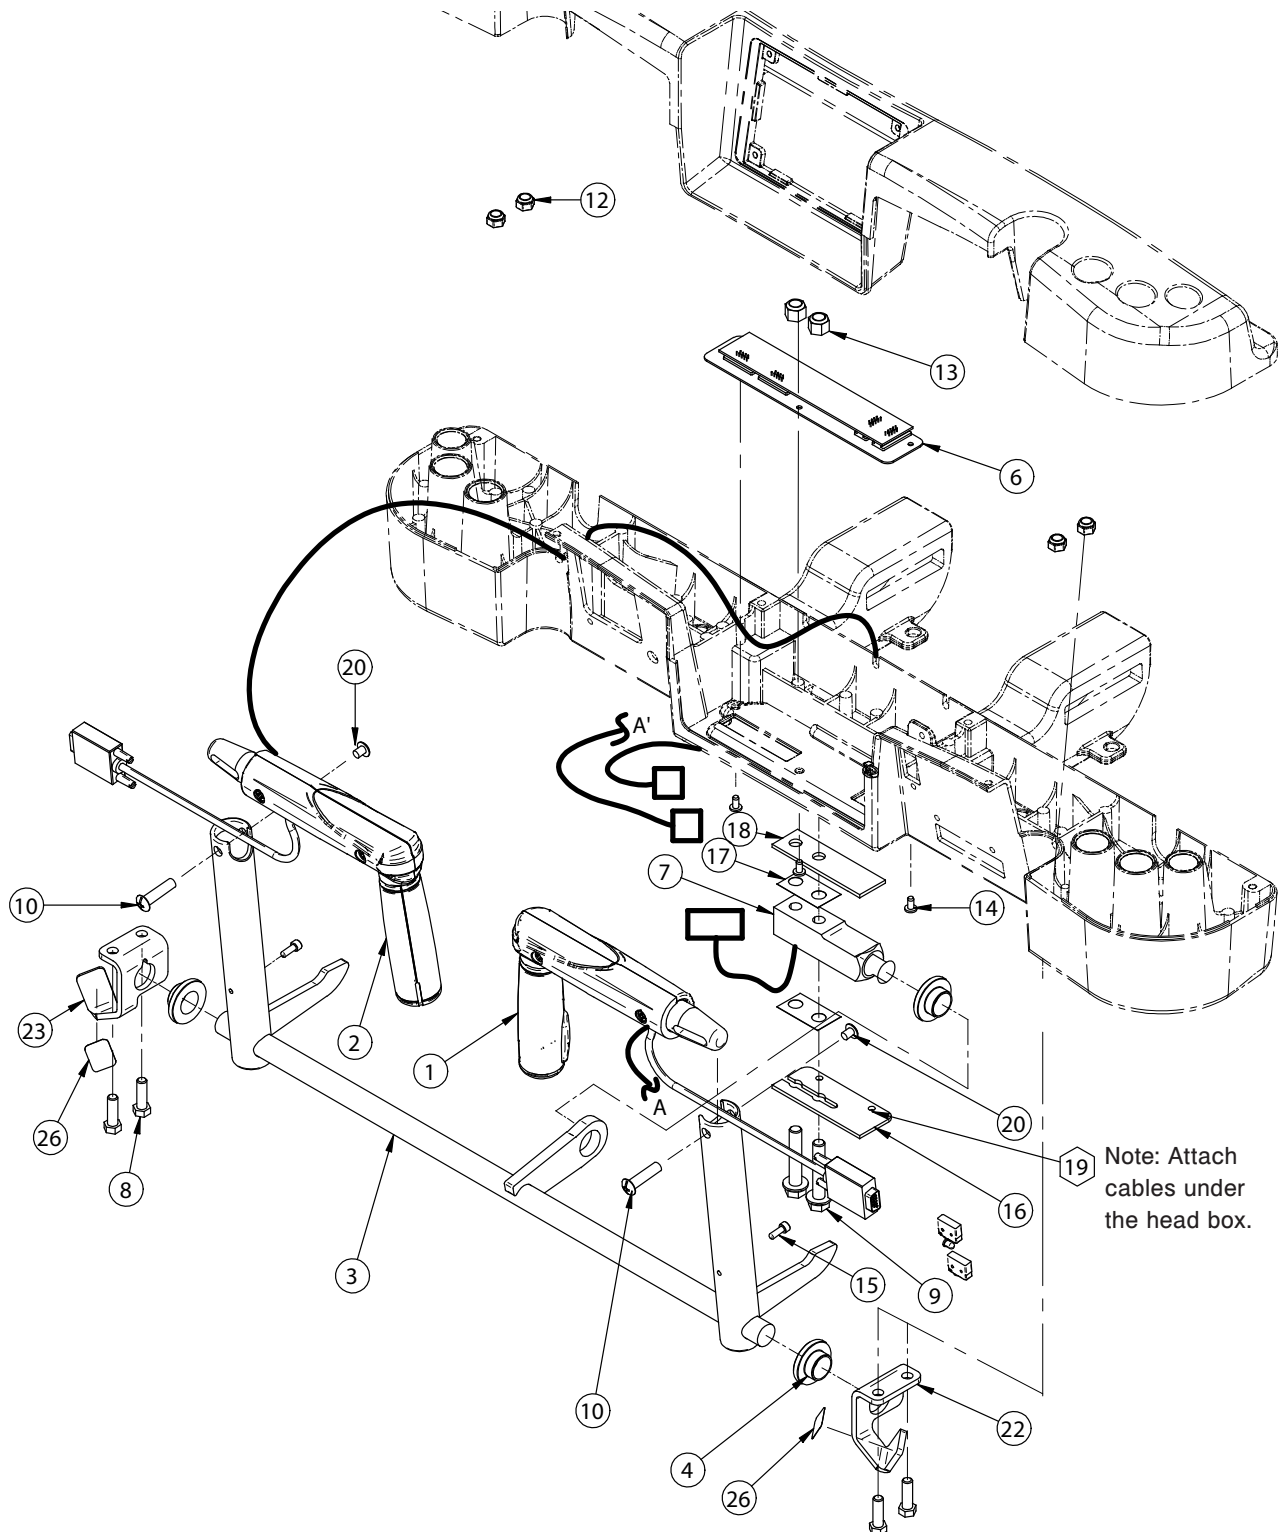

Zoom® Handle Assembly (Model 2141 Only)

(Applies to beds with Serial Numbers U51438 - Current)

27-2548 BOARD CONNECTION

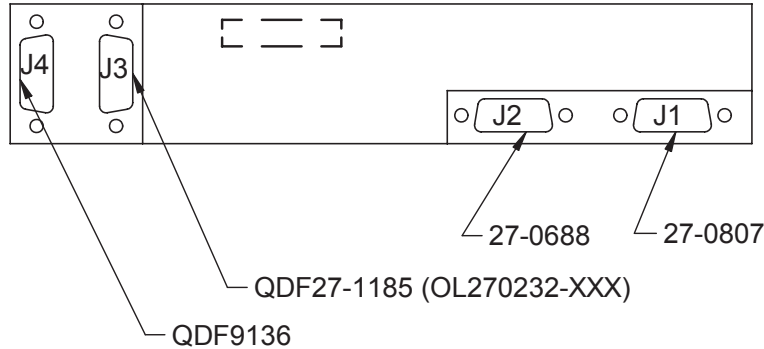

Zoom® Handle Assembly - 27-2547-XXX Rev B (Reference Only)


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	27-0688	Right Zoom® Handle	1
2	27-0807	Left Zoom® Handle	1
3	27-0880C	Tie Bus	1
4	27-1181	Zoom® Handle Sleeve	3
6	27-2548	Zoom® Control Board Assembly	1
7	QDF9136	250 lbs Load Cell	1
8	VB15A1O32	Bolt	4
9	VB95A1P48	Hex Neck Bolt	2
10	VE42A9036	Combination Barrel Nut	2
12	VE30A1O	Nylon Locknut	4
13	VE30A1P	Nylon Locknut	2
14	VV83A9G12	Phillips Head Tapping Screw	3
15	VV10A0G16-S	Hex Head Screw	2
16	27-1857Z	Bottom Zoom® Load Cell Stopper	1
17	QDF27-1780	Load Cell Spacer	2
18	27-1775Z	Zoom® Load Cell Stopper	1
19	QDF9518	Nylon Tie-Wrap	1
20	VV33A1N10-S	Machine Screw	2
22	27-2790P	Zoom® Handle Bracket, Right	1
23	27-2789P	Zoom® Handle Bracket, Left	1
26	QE71-1373	Coiled Power Cord Label	2

Zoom® Assembly

(Applies to beds with Serial Numbers U01001 - U51437)

OL270077-XXX Rev-02 (Reference Only)

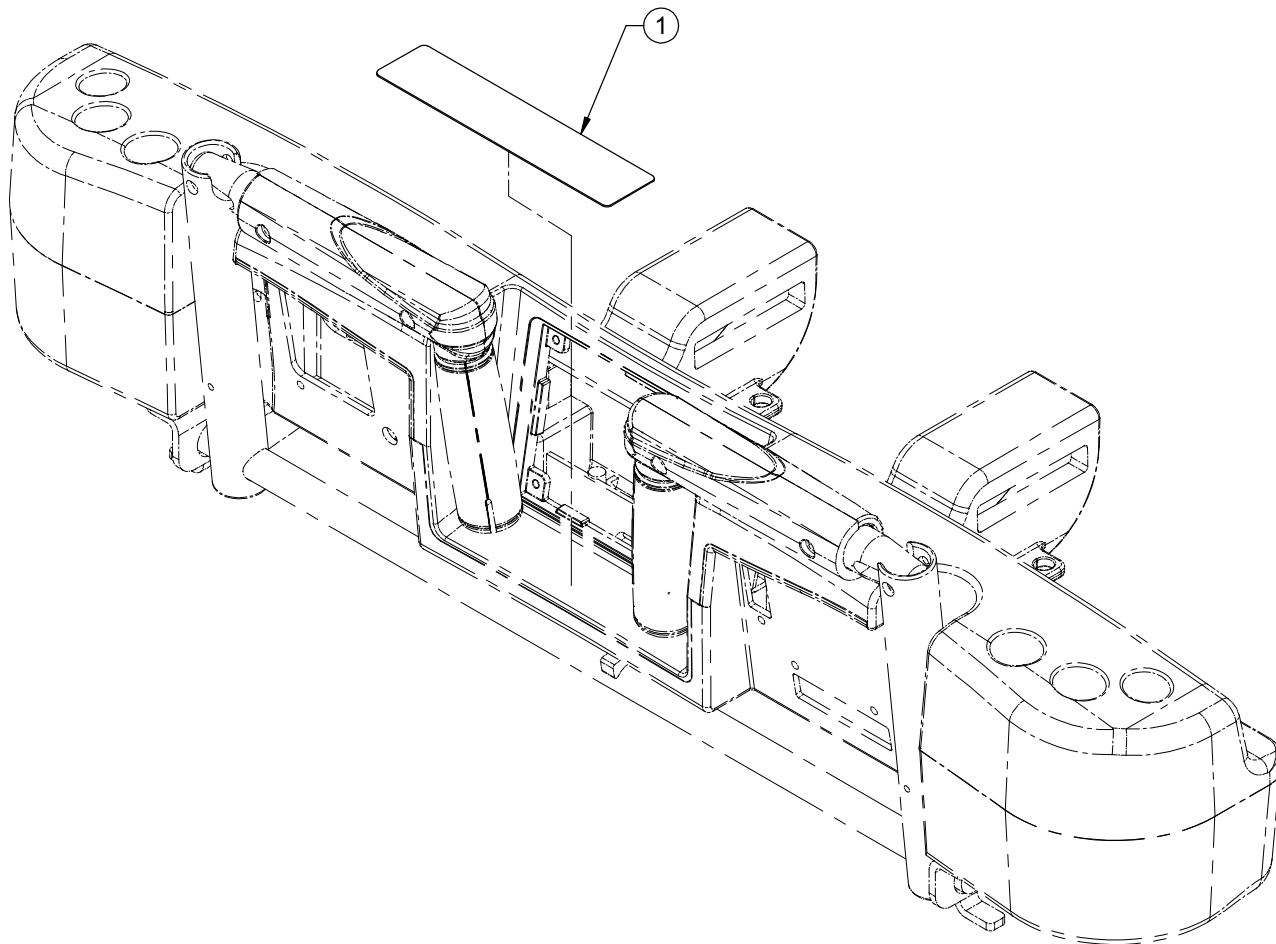


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QE71-0946-XXX	Zoom® Label	1

Zoom® Assembly

(Applies to beds with Serial Numbers U51438 - Current)

OL270077-XXX Rev D (Reference Only)

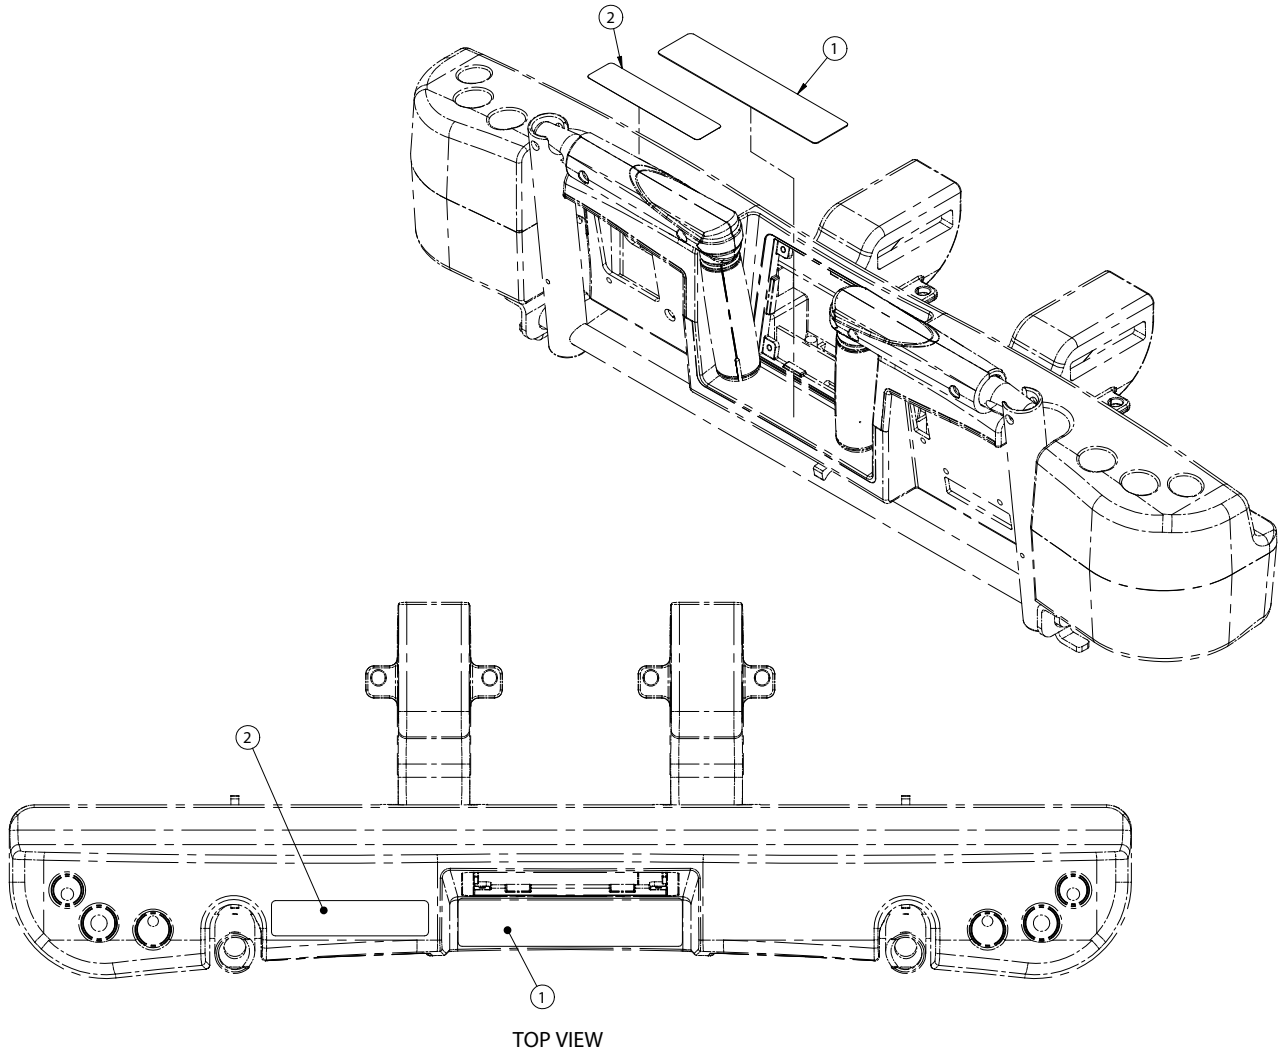


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QE71-0946-XXX	Zoom® Label	1
2	QE71-1372	Zoom® Handle Label	1

Optional No Head End Control Panel

OL270019 Rev-01 (Reference Only)

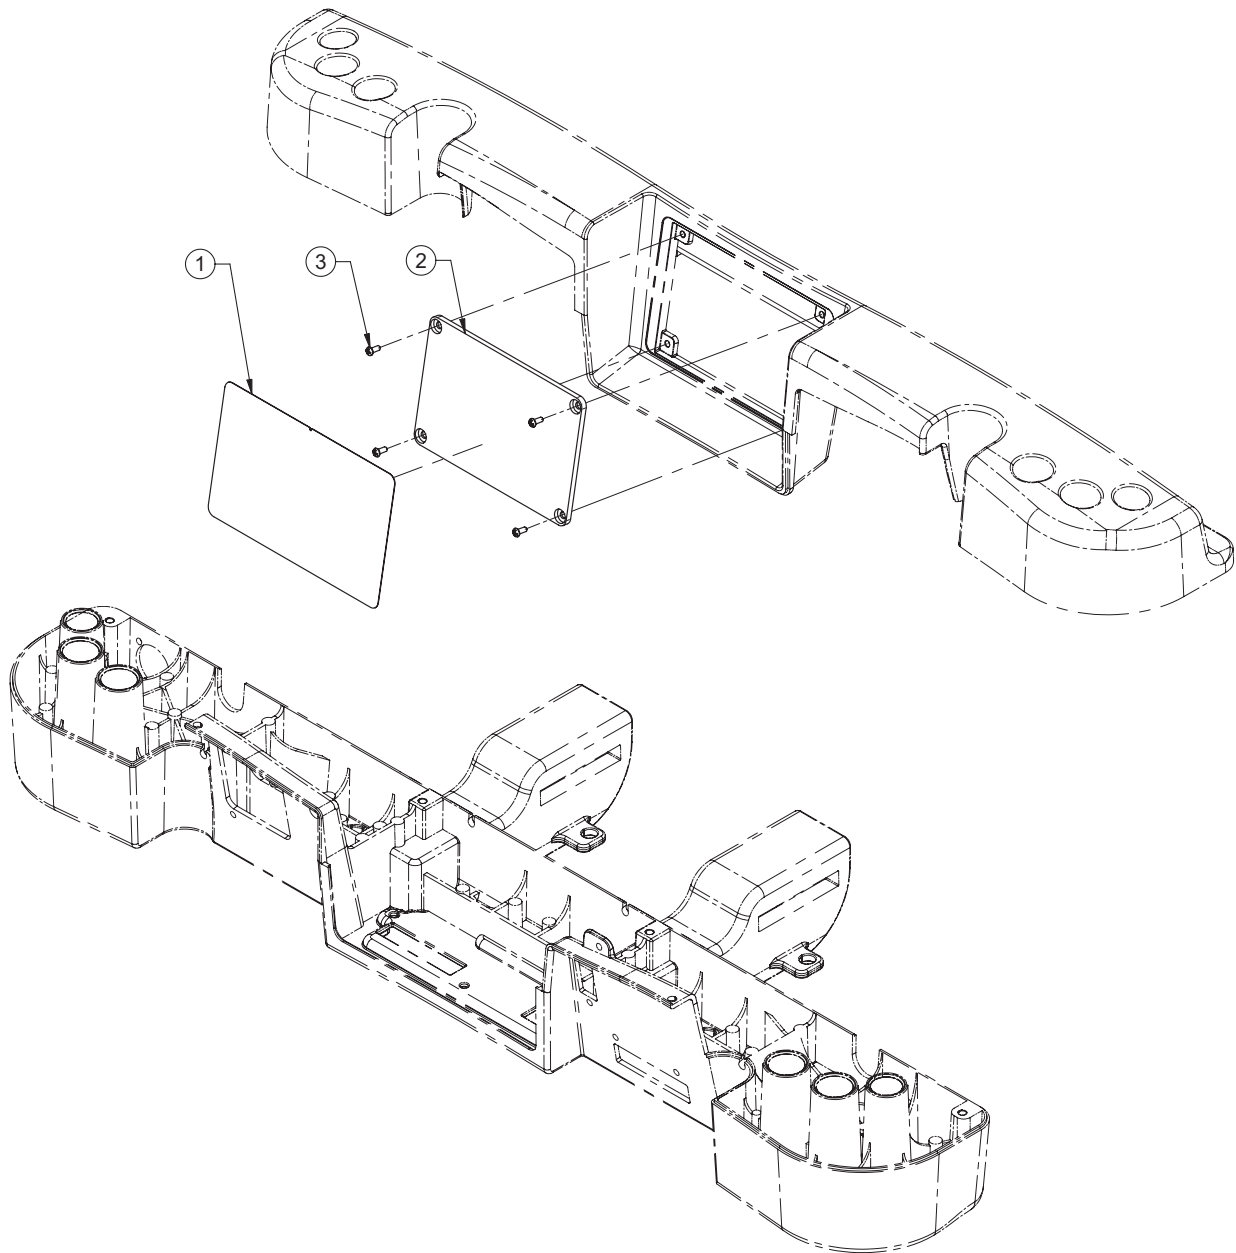

No Head End Control Panel Assembly - OL270019 Rev-01 (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF27-1649	Head End Control Fascia without Motorized Zoom® Drive	1
2	QP27-1650	Head Frame Plate	1
3	VV23A9C12HL	Pan Head Screw	4

Optional Head End Control Panel Assembly


OL270181 Rev-00 (Reference Only) (U01001 - U03318, excluding U03258 and U03259)

OL270245 Rev-00 (Reference Only) (U03319 - U04982, including U03258 and U03259)

OL270263-XXX Rev-00 (Reference Only) (U04983 - U50240)

OL270279-XXX Rev A (Reference Only) (U50241 - 2.5)

OL270263-XXX Rev C (Reference Only) (3.0 - Current)

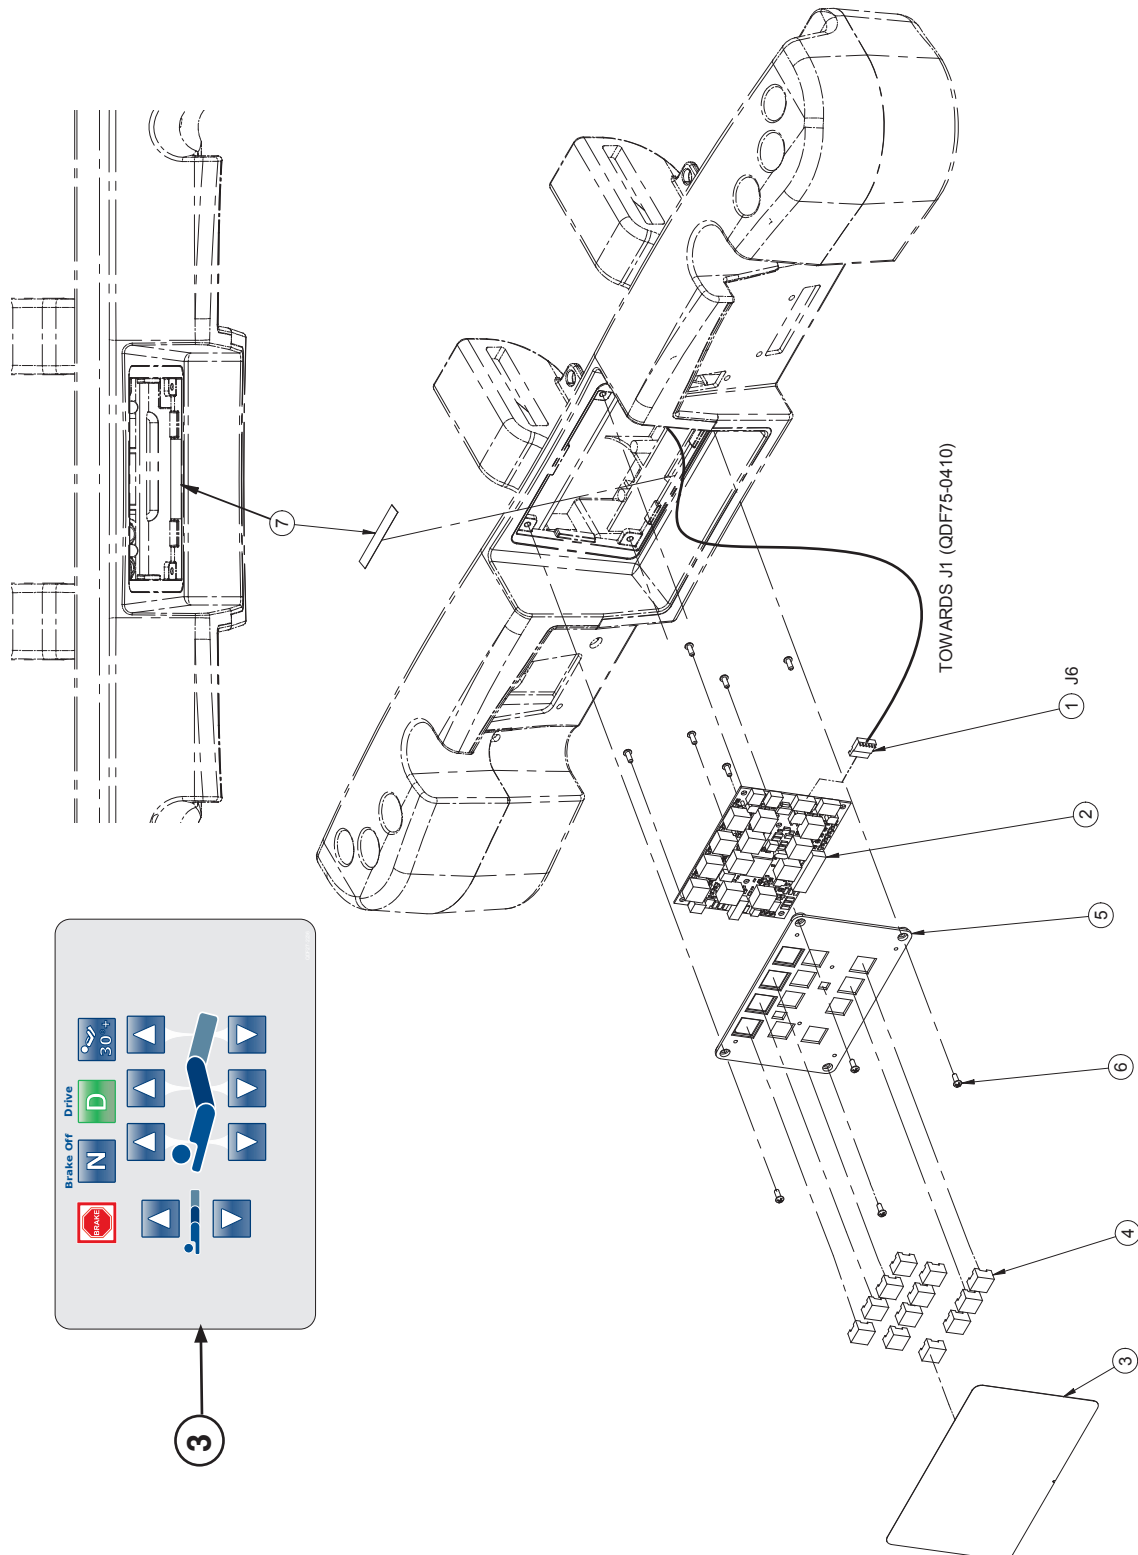

Optional Head End Control Panel Assembly

QDF21-2895 CONNECTION TABLE			
Cable No	Connector No.	Cable No	Connector No.
QDF21-2895	MTA6	QDF27-1099	J6
QDF21-2895	MTA6	QDF75-0270	J1

DIP SWITCH CONFIGURATION ON QDF27-1099			
SW13	ON	OFF	ON
SW14	OFF	OFF	-

Optional Head End Control Panel Assembly
OL270181 Rev-00 (Reference Only) (U01001 - U03318, excluding U03258 and U03259)
OL270245 Rev-00 (Reference Only) (U03319 - U04982, including U03258 and U03259)
OL270263-XXX Rev-00 (Reference Only) (U04983 - U50240)
OL270279-XXX Rev A (Reference Only) (U50241 - 2.5)
OL270263-XXX Rev C (Reference Only) (3.0 - Current)


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF21-2895	12" Network Cable	1
2	QDF27-1099	Siderail Nurse Control Board	1
3	QF27-2236-XXX	Fascia, Head of Bed Control	1
4	QDF9183	Electronic Board Button	12
5	QP27-1111	Nurse Control Board Support	1
6	VV23A9C12HL	Pan Head Screw	10
7	QE71-1340	Connection Isolation Sticker	1

Siderail Mounting Assembly, Head End

(Applies to beds with Serial Numbers U01001 - U02817)

L27-039 Rev-00 (Reference Only)

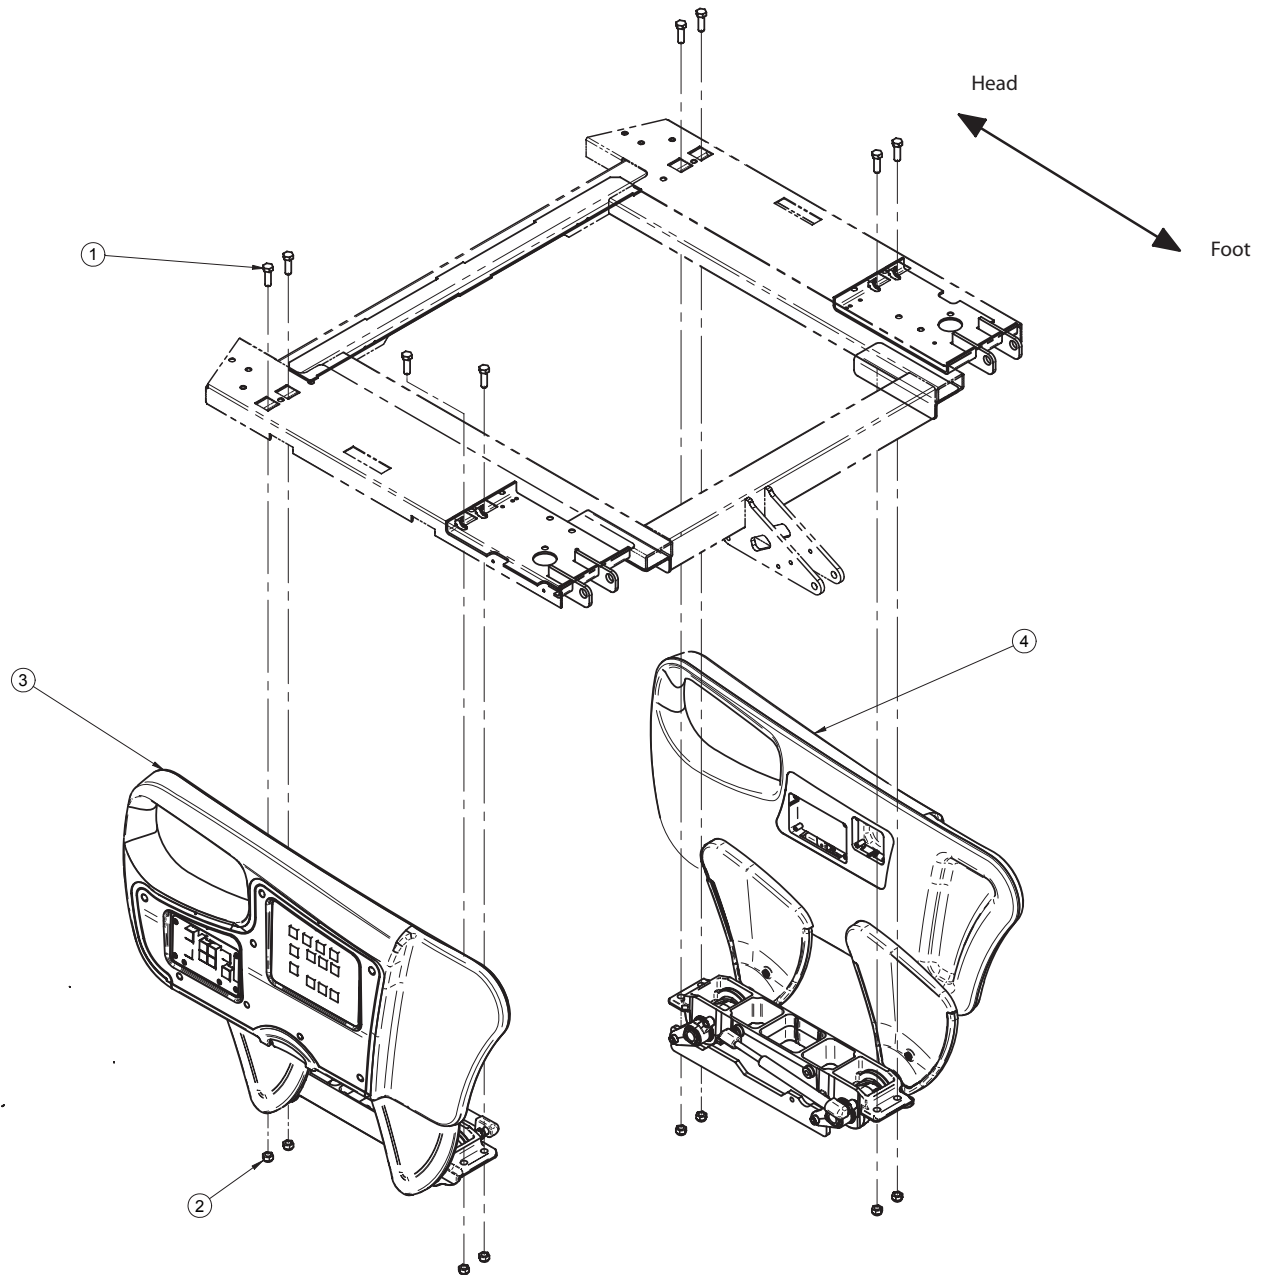


Item	Part No.	Part Name	Qty.
1	VB18A1O32	Bolt	8
2	VE30A1O	Nylon Locknut	8
3	27-2257W	Right Head Siderail	1
4	27-2258W	Left Head Siderail	1

Siderail Mounting Assembly, Head End

(Applies to beds with Serial Numbers U02818 - Current)

L27-039 Rev-01 (Reference Only)

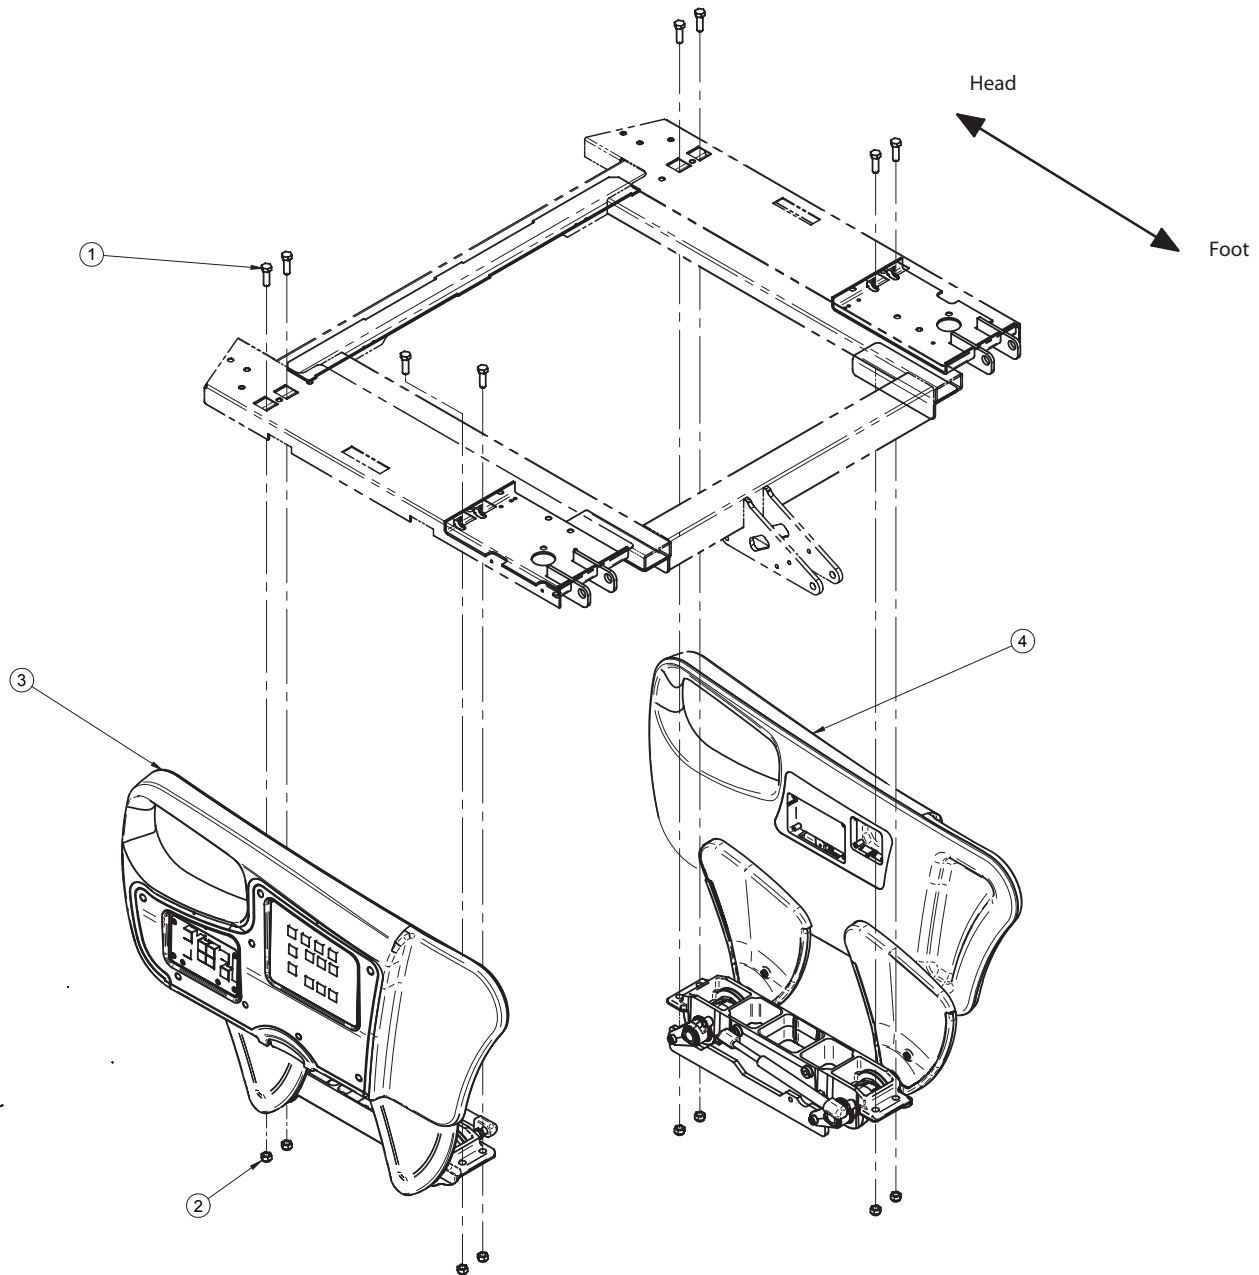


Item	Part No.	Part Name	Qty.
1	VB18A1O32	Bolt	8
2	VE30A1O	Nylon Locknut	8
3	27-2287	Head End Siderail, Right	1
4	27-2288	Head End Siderail, Left	1

Standard Siderail Assembly, Head End, Right

(Applies to beds with Serial Numbers U01001 - U02817)

27-2257 Rev-00 (Reference Only)

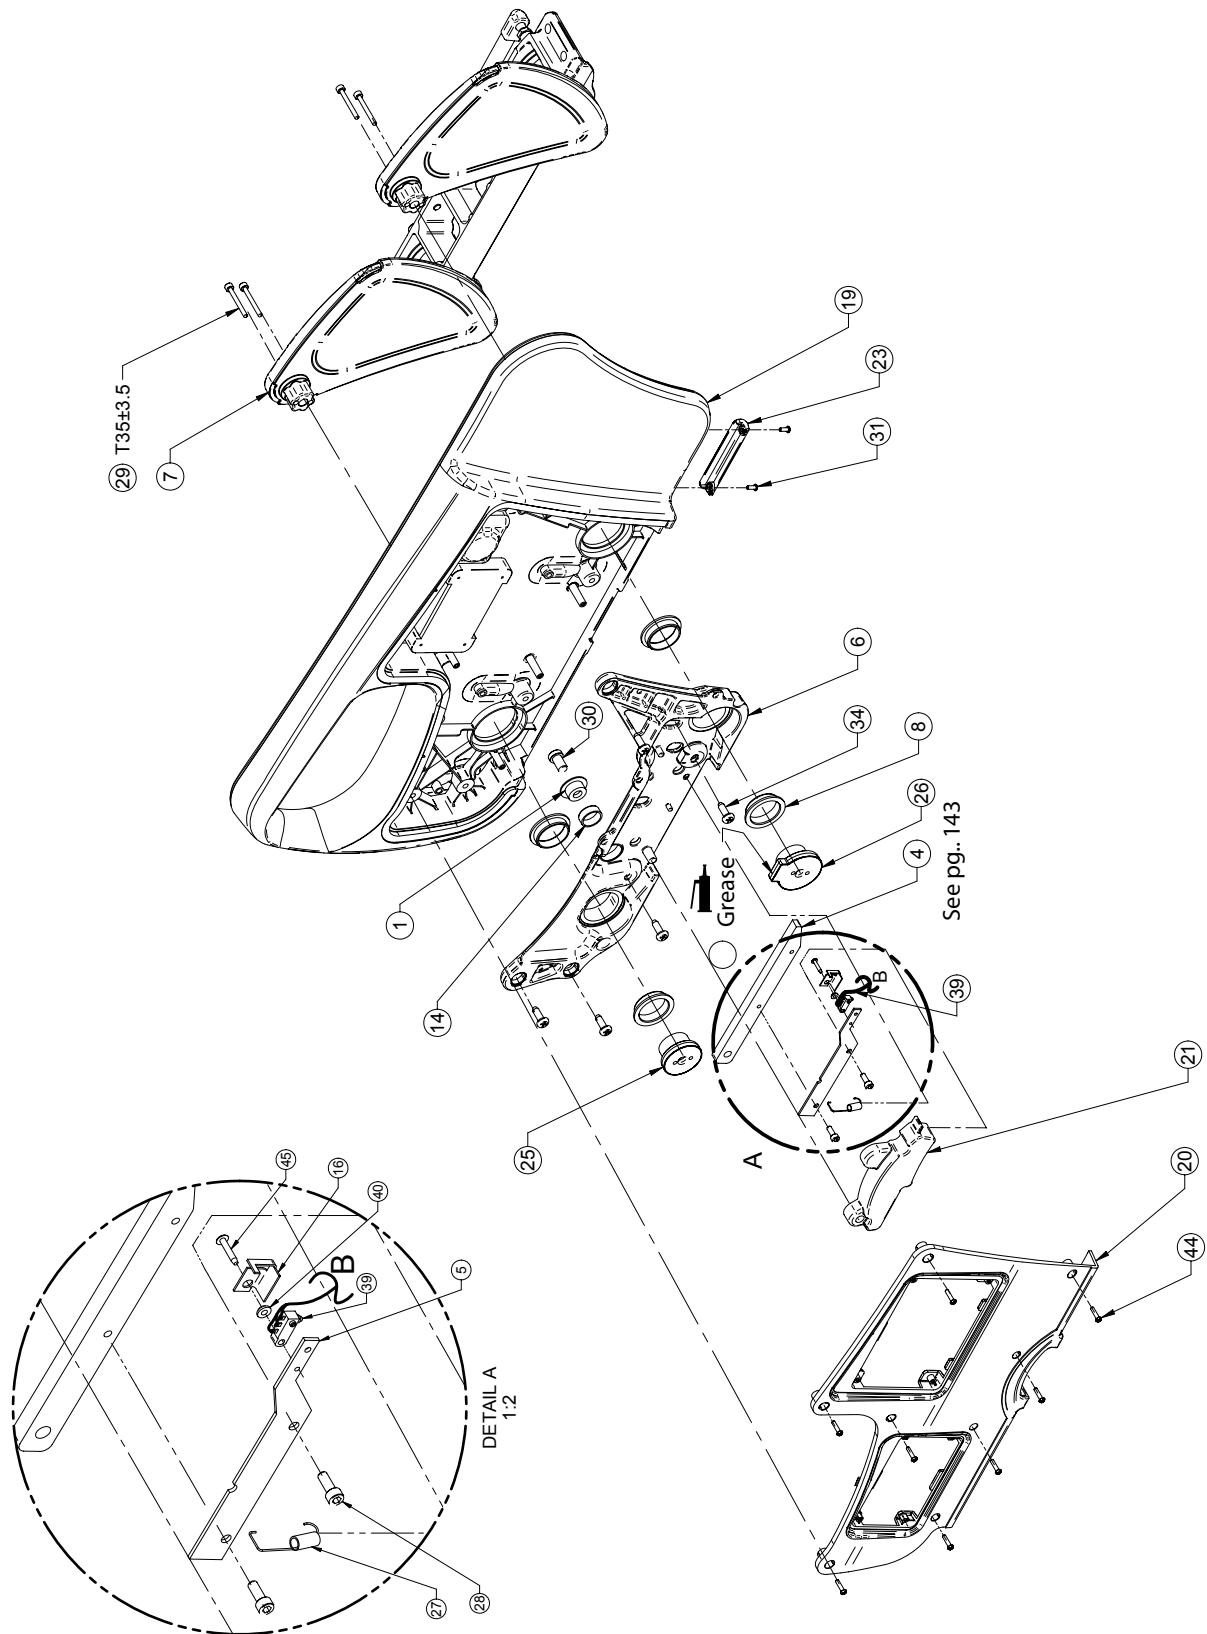

(Applies to beds with Serial Numbers U01001 - U02817)



Standard Siderail Assembly, Head End, Right

(Applies to beds with Serial Numbers U01001 - U02817)

POSITION ON CONNECTOR					
Cable 35	Position on Connector 41	Position on Connector 43	Position on Connector 42	Signal	Color
1	1	-	-	"CAN H"	Black / Red
2	2	-	-	"CAN L"	Red
3	3	-	-	+12V	Black / White
4	4	-	-	"GND"	White
5	5	-	-	"SAFE"	Black / Green
6	6	-	-	+24V	Green
-	-	-	-	Audioshield	-
1	-	1	-	"SPK HIGH"	Black
2	-	2	-	"SPK COM"	White
1	-	-	1	N.O.	Red
2	-	-	2	COM	Green
3	-	-	3	N.C.	Brown

DIPSWITCH SETUP ON QDF27-1099			
SW13	ON	ON	ON
SW14	ON	ON	-

CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1681	MTA – 3 Positions	To	QDF27-1099	
QDF27-1156	MTA – 6 Positions	To	QDF27-1099	
QDF27-1156	MTA – 6 Positions	To	QDF27-1097	
QDF27-1784	MTA – 3 Positions	To	QDF27-2212	
QDF27-2212	Mate N Lock 12 Pos.	To	QDF27-2213	
QDF27-2212	MTA – 6 Positions	To	QDF27-1099	
QDF27-2212	MTA – 3 Positions	To	See OL270162, OL270163, OL270164, OL270173, OL270174, OL270175	
QDF27-2212	MTA – 2 Positions	To		

Standard Siderail Assembly, Head End, Right


(Applies to beds with Serial Numbers U01001 - U02817)

Standard Siderail Assembly, Head End, Right - Common Components - 27-2257 Rev-00 (Reference Only)

Item	Part No.	Part Name	Qty.
1	QPA28-0493	Siderail Sleeve	1
3	QDF27-1099	Siderail Nurse Control Board	1
4	QDB27-1141	Siderail Lock	1
5	27-1142Z	Siderail Switch Support	1
6	27-1269	Right Head Siderail Structure	1
7	27-2061W	Reversed Siderail Mechanism S.A.	1
8	QDF2049	Shoulder Spacer	4
9	QDF27-1097	Brake Control Board	1
10	QDF27-2237	Right Head Nurse Control Fascia	1
14	QDF28-0491	Machined Spacer QDF9191	1
15	QDF9183	Electronic Board Button	20
16	27-1739Z	Switch Guide 2	1
17	QP27-1109-10	Brake Board Support	1
18	QP27-1111	Nurse Control Board Support	1
19	QP27-2225-05	Right Head Siderail	1
20	QP27-1265-05	Right Head Siderail Cover	1
21	QP27-1273-08	Right Siderail Handle	1
23	QP27-1496-05	Head Siderail Cap	1
24	QP28-0040-10	Reversed Siderail Arm Cover	2
25	QPA28-0015	Siderail Sleeve	1
26	QPA28-0016	Sleeve with Lock	1
27	QRE27-1736	Return Spring	1
28	VV10A0G16-S	Cylinder Head Screw	2
29	VV10A0G40-S	Cylinder Head Screw	4
30	VV10A1P20-S	Cylinder Head Screw	1
31	VV23A9C12HL	Phillips Screw	22
32	VV31A0G16	Phillips Machine Screw	2
34	VVB3A9N24PF	Bosscrew Screw	5
35*	QDF27-2212	Head Siderail Wire	1
36*	QDF9518	Cable Tie	1
38*	QDF27-1156	Brake Board Cable	1
39*	QDF27-1521	Siderail Limit Switch	1
40	27-1839	Spacer Washer	1
41*	QDF2088	6 Positions Polarized Connector	1
42*	QDF9028	3 Positions Connector	1
43*	QDF2087	2 Positions Connector	1
44	VV23A9C20HI	Phillips Screw	8
45	VV87A9A20	Phillips Screw	1
46*	M0019	OG 2 Grade Grease	1
47*	QDF2127	2 Pins Connector	1

(Applies to beds with Serial Numbers U02818 - Current)


27-2287 Rev-04 (Reference Only)

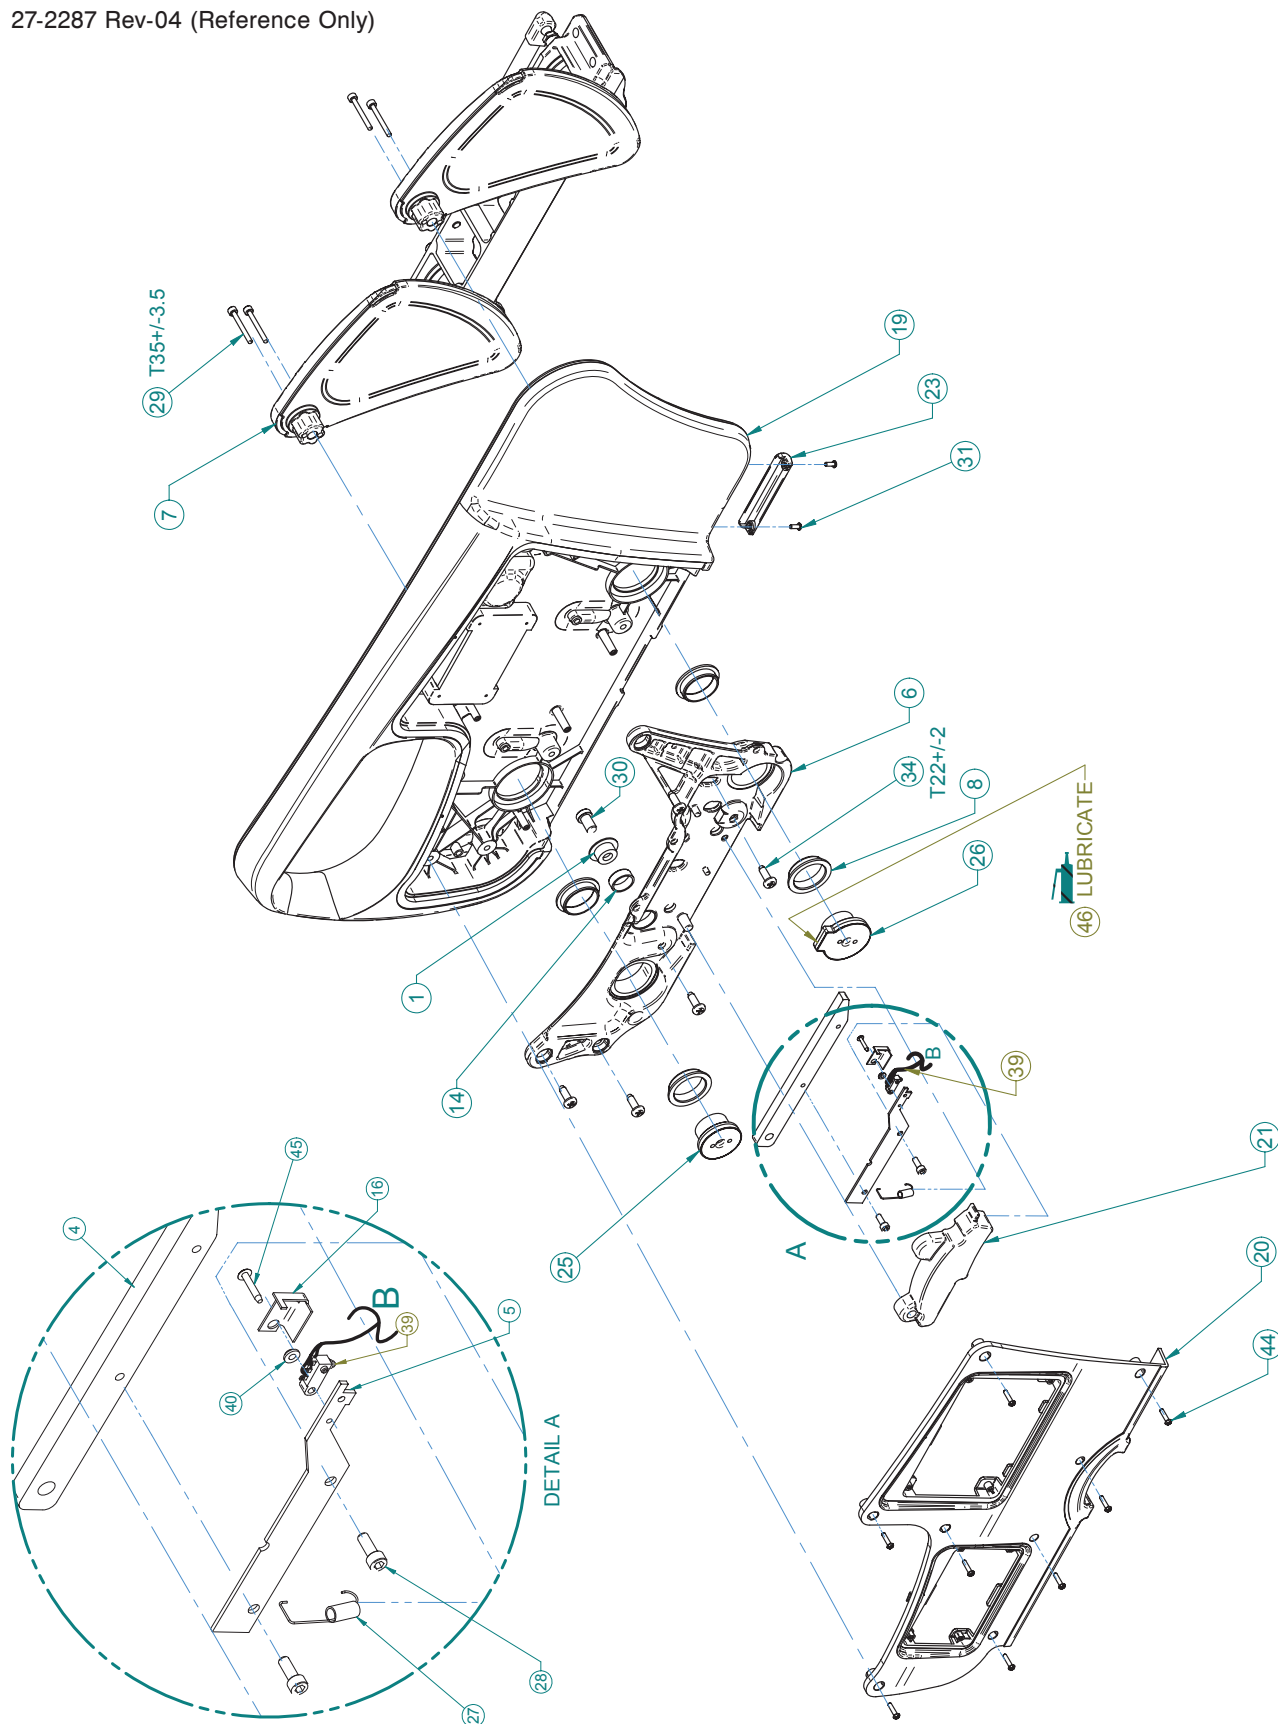

[Return To Table of Contents](#)

Standard Siderail Assembly, Head End, Right

(Applies to beds with Serial Numbers U02818 - Current)

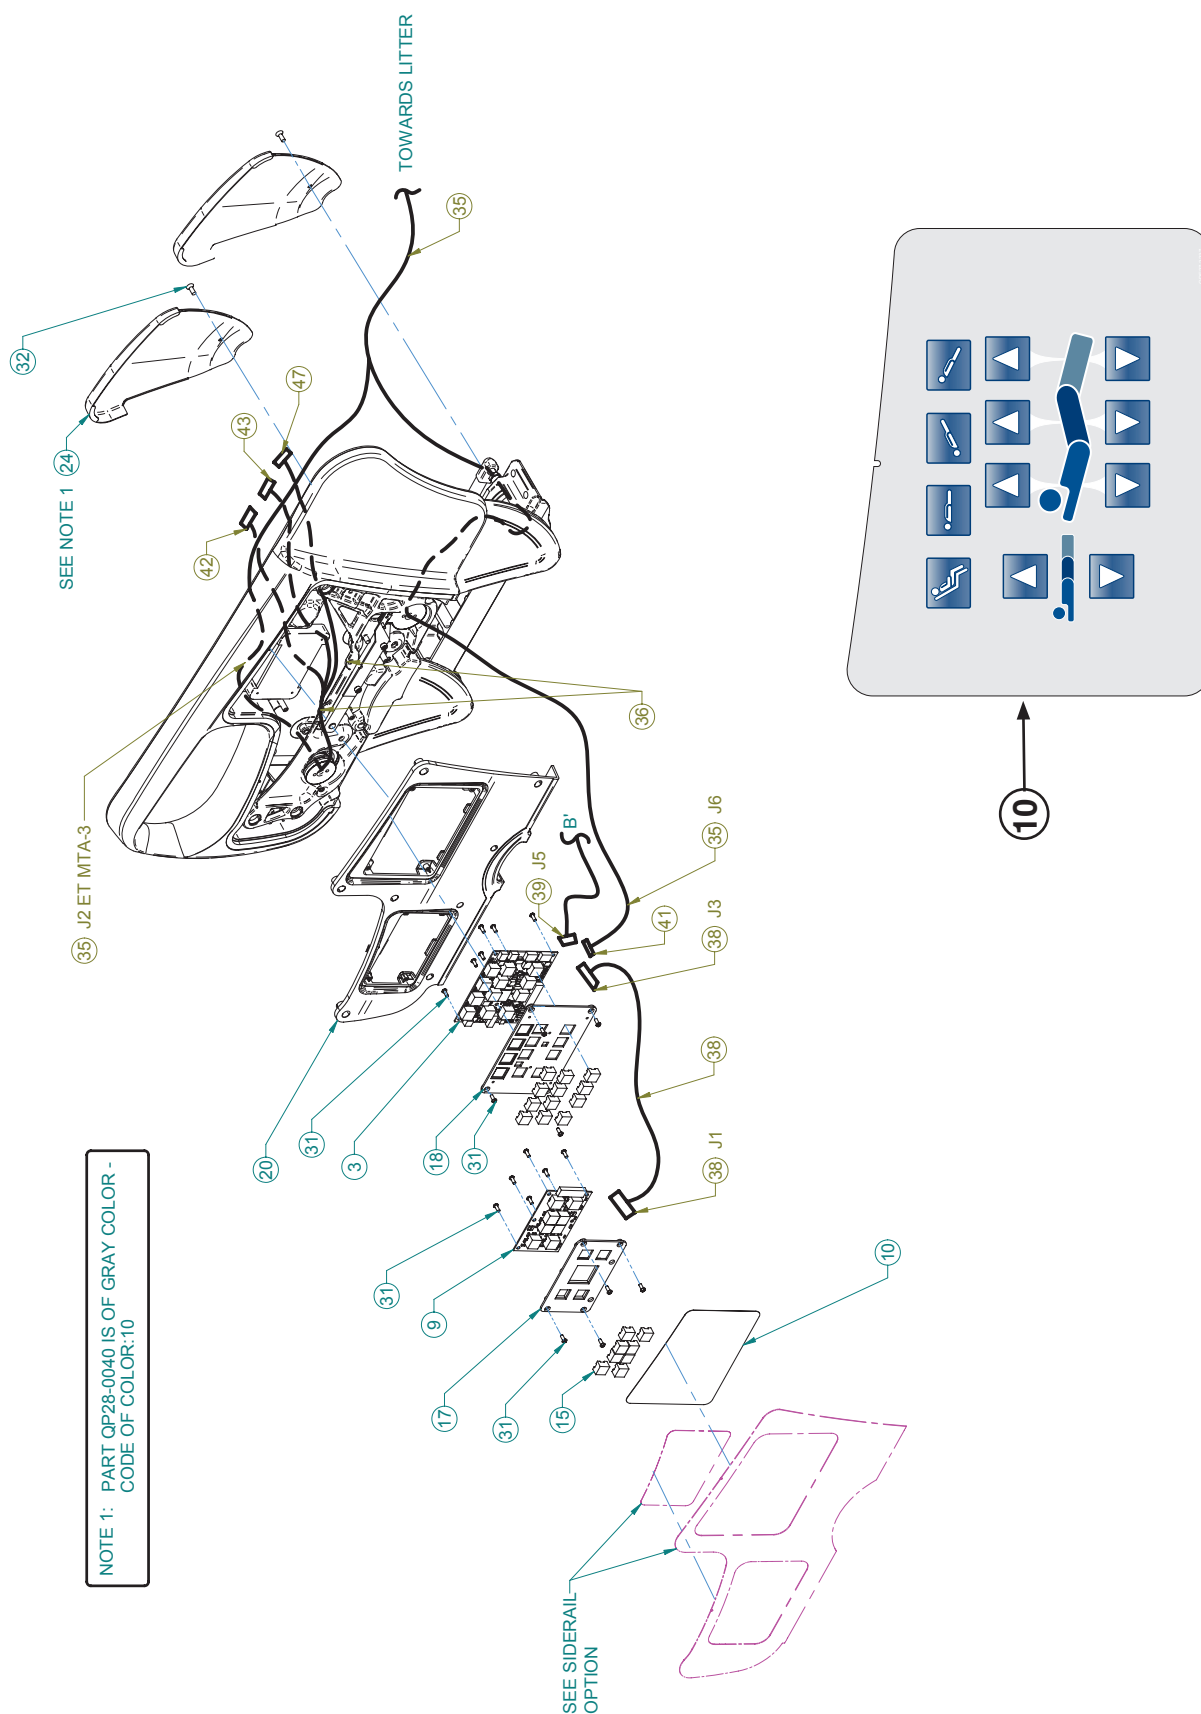

Standard Siderail Assembly, Head End, Right

(Applies to beds with Serial Numbers U02818 - Current)

POSITION ON CONNECTOR						
Cable 36	Position on Connector 47	Position on Connector 41	Position on Connector 43	Position on Connector 42	Signal	Color
1	-	1	-	-	"CAN H"	Black / Red
2	-	2	-	-	"CAN L"	Red
3	-	3	-	-	+12V	Black / White
4	-	4	-	-	"GND"	White
5	-	5	-	-	"SAFE"	Black / Green
6	-	6	-	-	+24V	Green
-	-	-	-	-	Audioshield	-
1	-	-	1	-	"SPK HIGH"	Black
2	-	-	2	-	"SPK COM"	White
1	-	-	-	1	N.O.	Red
2	-	-	-	2	COM	Green
3	-	-	-	3	N.C.	Brown
1	1	-	-	-	Speaker	Blue
2	2	-	-	-	Speaker	Orange

DIP SWITCH SETUP ON QDF27-1099			
SW13	ON	ON	ON
SW14	ON	ON	-

CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1681	MTA – 3 Positions	To	QDF27-1099	J5
QDF27-1156	MTA – 6 Positions	To	QDF27-1099	J3
QDF27-1156	MTA – 6 Positions	To	QDF27-1097	J1
QDF27-1784	MTA – 3 Positions	To	QDF27-2212	MTA-2 Positions
QDF27-2212	Mate N Lock 12 Positions	To	QDF27-2213	J105 (L27-038)
QDF27-2212	MTA – 6 Positions	To	QDF27-1099	J6
QDF27-2212	MTA – 3 Positions	To	See OL270162, OL270163, OL270164, OL270173, OL270174, OL270175	
QDF27-2212	MTA – 2 Positions	To		
QDF27-2212	Connector 2 Pins	To		

Standard Siderail Assembly, Head End, Right

(Applies to beds with Serial Numbers U02818 - Current)


Standard Siderail Assembly, Head End, Right - 27-2287 Rev-04 (Reference Only)

Item	Part No.	Part Name	Qty.
1	QPA28-0493	Siderail Sleeve	1
3	QDF27-1099	Siderail Nurse Control Board	1
4	QDF27-2574Z	Siderail Lock	1
5	27-2575Z	Siderail Switch Support	1
6	QPA27-2295	Right Head Siderail Structure	1
7	27-2061W	Reversed Siderail Mechanism S.A.	1
8	QDF2049	Shoulder Spacer	4
9	QDF27-1097	Brake Control Board	1
10	QDF27-2237	Right Head Nurse Control Fascia	1
14	QDF28-0491	Machined Spacer QDF9191	1
15	QDF9183	Electronic Board Button	20
16	27-2292Z	Switch Guide 2	1
17	QP27-1109-10	Brake Board Support	1
18	QP27-1111	Nurse Control Board Support	1
19	QP27-2225-05	Right Head Siderail	1
20	QP27-1265-05	Right Head Siderail Cover	1
21	QP27-1273-08	Right Siderail Handle	1
23	QP27-1496-05	Head Siderail Cap	1
24	QP28-0040-10	Reversed Siderail Arm Cover	2
25	QPA28-0015	Siderail Sleeve	1
26	QPA28-0016	Sleeve with Lock	1
27	QRE27-1736	Return Spring	1
28	VV10A0G16-S	Cylinder Head Screw	2
29	VV10B0G40-S	Cylinder Head Screw	4
30	VV10A1P20-S	Cylinder Head Screw	1
31	VV23A9C12HL	Phillips Screw	22
32	VV31A0G16	Phillips Machine Screw	2
34	VVB3A9N24PF	Bosscrew Screw	5
35*	QDF27-2212	Head Siderail Wire	1
36*	QDF9518	Cable Tie	2
38*	QDF27-1156	Brake Board Cable	1
39*	QDF27-1521	Siderail Limit Switch	1
40	27-1839	Spacer Washer	1
41*	QDF2088	6 Positions Polarized Connector	1
42*	QDF9028	3 Positions Connector	1
43*	QDF2087	2 Positions Connector	1
44	VV23A9C20HL	Phillips Screw	8
45	VV87A9A20	Phillips Screw	1
46*	M0019	OG 2 Grade Grease	1
47*	QDF2127	2 Pins Connector	1

Standard Siderail Assembly, Head End, Left


(Applies to beds with Serial Numbers U01001 - U02817)

27-2258 Rev-00 (Reference Only)

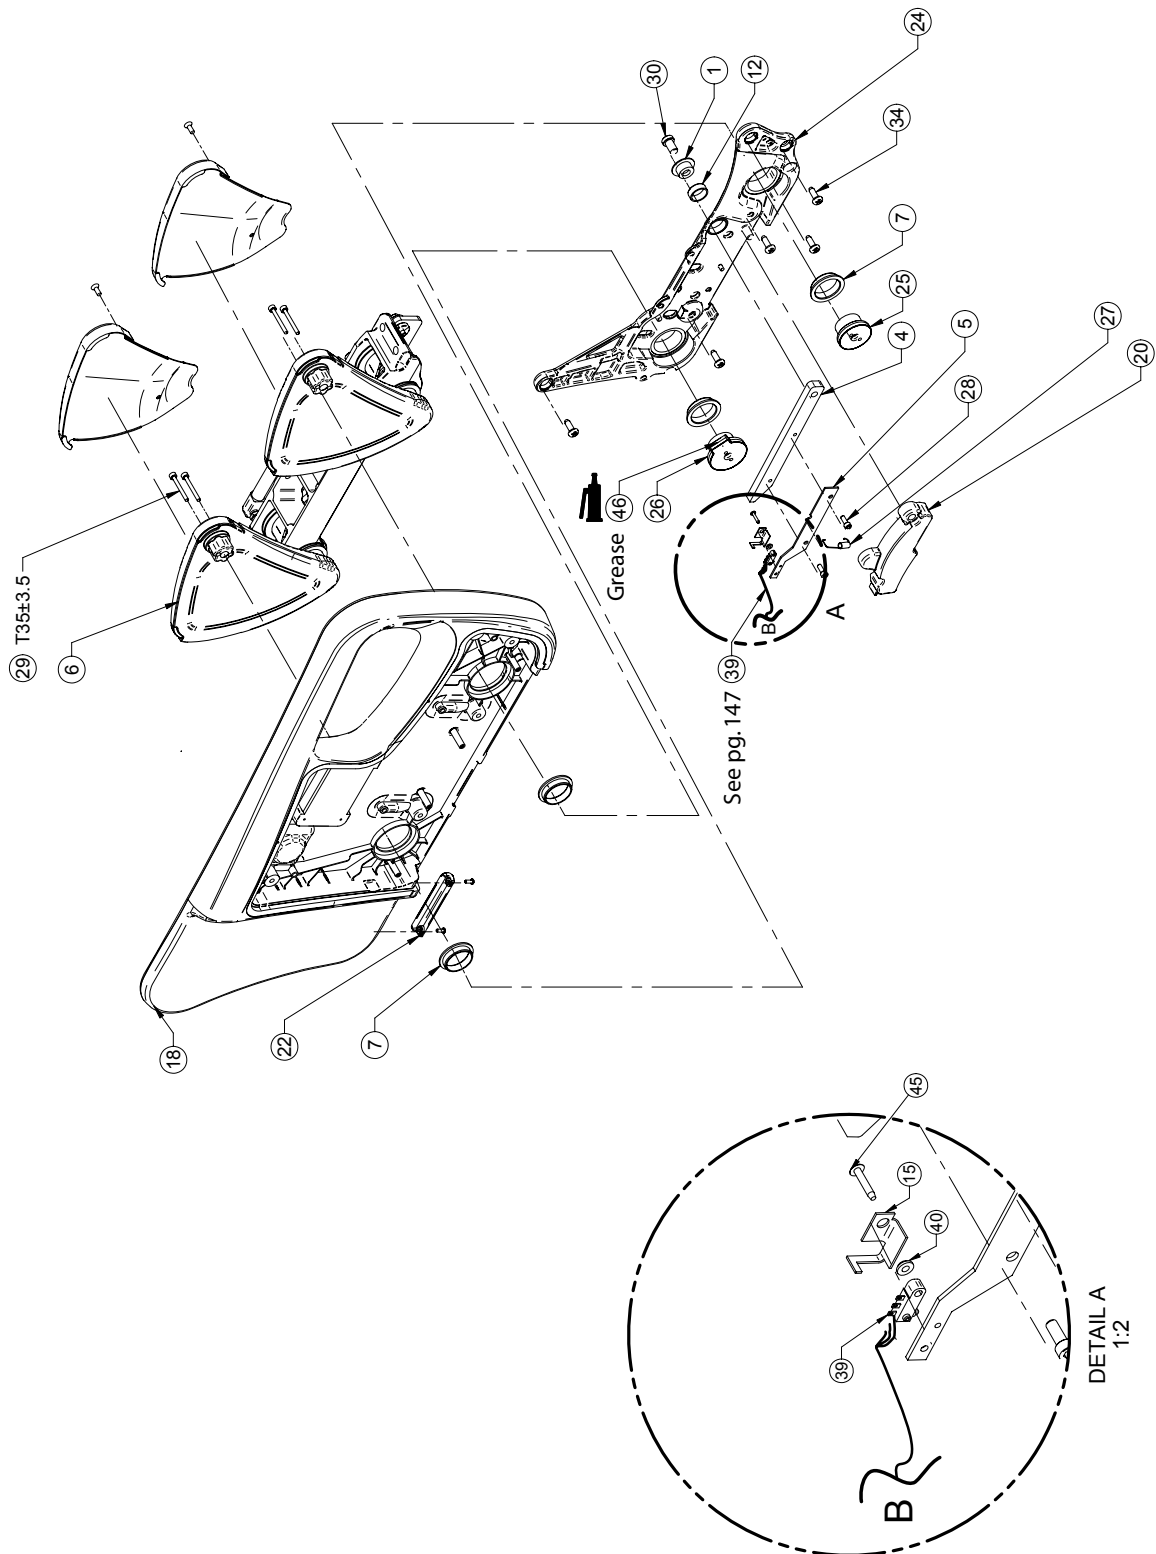

Standard Siderail Assembly, Head End, Left

(Applies to beds with Serial Numbers U01001 - U02817)

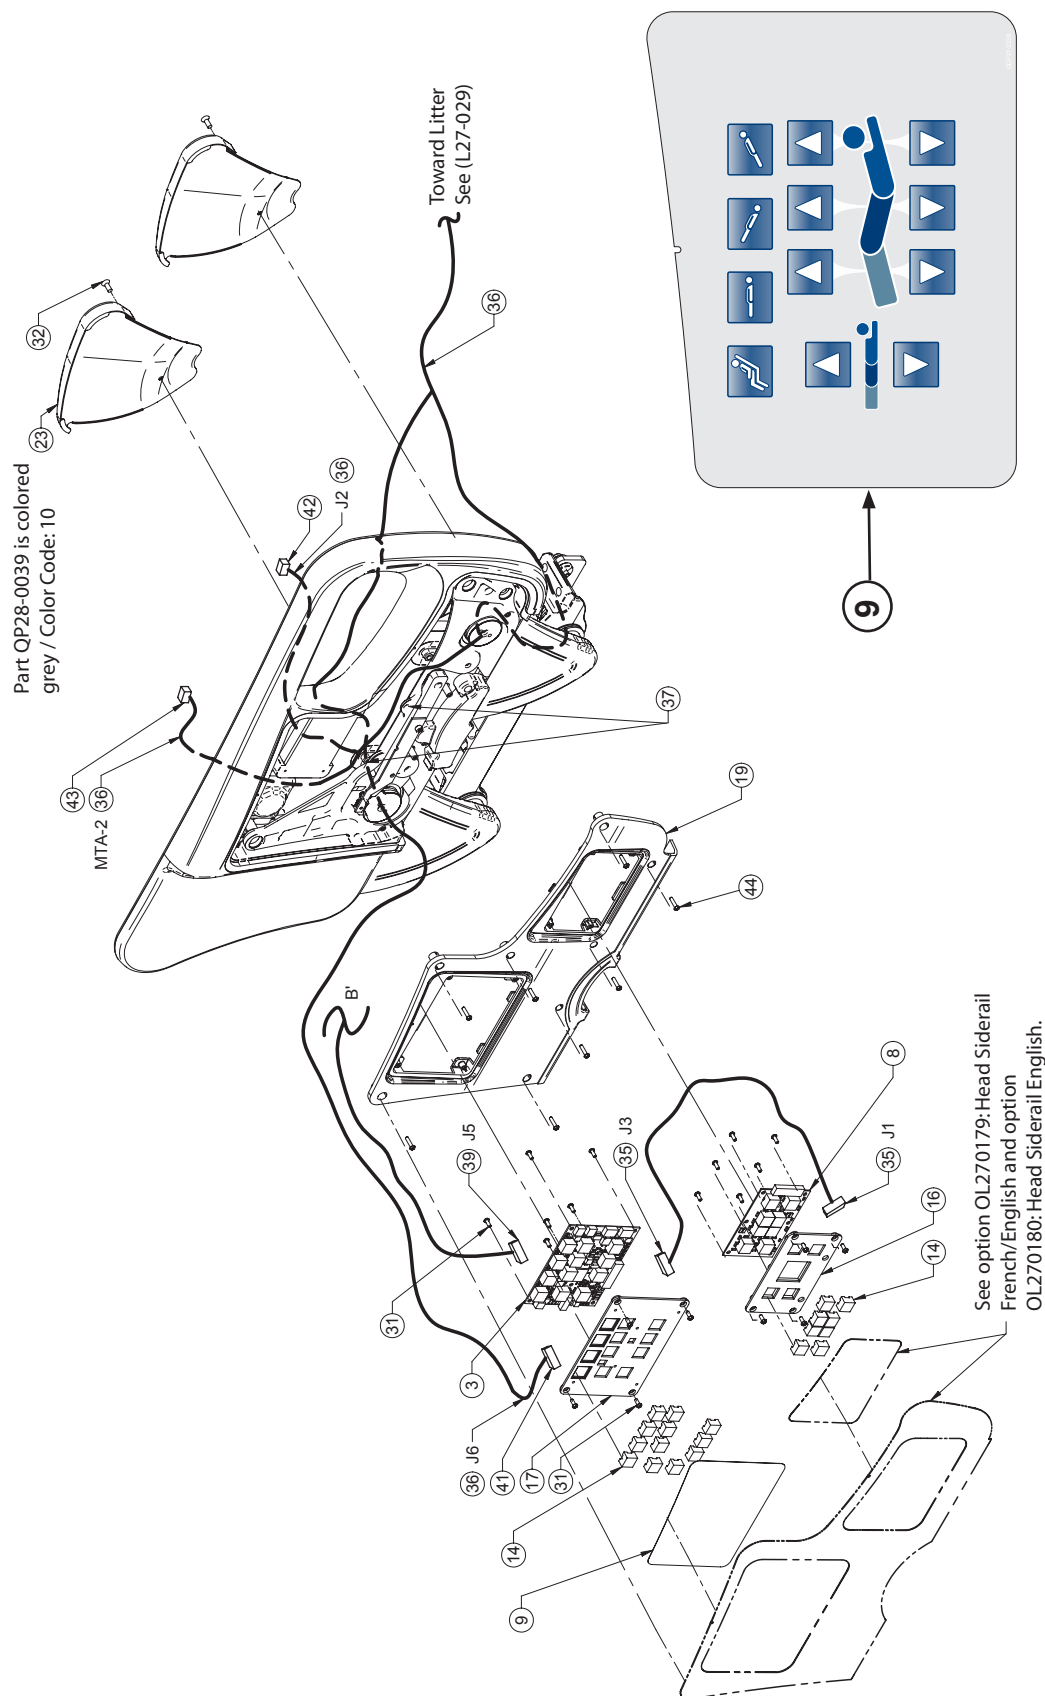

Standard Siderail Assembly, Head End, Left

(Applies to beds with Serial Numbers U01001 - U02817)

POSITION ON CONNECTOR					
Cable 36	Position on Connector 41	Position on Connector 43	Position on Connector 42	Signal	Color
1	1	-	-	"CAN H"	Black
2	2	-	-	"CAN L"	Red
3	3	-	-	+12V	Black
4	4	-	-	"GND"	White
5	5	-	-	"SAFE"	Black
6	6	-	-	+24V	Green
-	-	-	-	Audioshield	-
1	-	1	-	"SPK HIGH"	Black
2	-	2	-	"SPK COM"	White
1	-	-	1	N.O.	Red
2	-	-	2	COM	Green
3	-	-	3	N.C.	Brown

DIPSWITCH SETUP ON QDF27-1099			
SW13	OFF	ON	ON
SW14	OFF	OFF	-

CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1681	MTA – 3 Positions	To	QDF27-1099	
QDF27-1156	MTA – 6 Positions	To	QDF27-1099	
QDF27-1156	MTA – 6 Positions	To	QDF27-1097	
QDF27-1784	MTA – 3 Positions	To	QDF27-2212	
QDF27-2212	Mate N Lock 12 Pos.	To	QDF27-2213	
QDF27-2212	MTA – 6 Positions	To	QDF27-1099	
QDF27-2212	MTA – 3 Positions	To	See OL270162, OL270163, OL270164, OL270173, OL270174, OL270175	
QDF27-2212	MTA – 2 Positions	To		

Standard Siderail Assembly, Head End, Left

(Applies to beds with Serial Numbers U01001 - U02817)


Standard Siderail Assembly, Head End, Left - Common Components - 27-2288 Rev-00 (Reference Only)

Item	Part No.	Part Name	Qty.
1	QPA28-0493	Siderail Sleeve	1
3	QDF27-1099	Siderail Nurse Control Board	1
4	QDB27-1141	Siderail Lock	1
5	27-1142Z	Switch Support	1
6	27-2060W	Siderail Mechanics S.A.	1
7	QDF2049	Spacer ID 1.25 OD 1.406 WI 3/8	4
8	QDF27-1097	Brake Control Board	1
9	QDF27-2238	Left Head Nurse Control Fascia	1
12	QDF28-0491	Machining Spacer QDF9191	1
14	QDF9183	Electronic Board Button	20
15	27-1740Z	Switch Guide 1	1
16	QP27-1109-10	Brake Board Support	1
17	QP27-1111	Nurse Control Board Support	1
18	QP27-2226-05	Left Head Siderail	1
19	QP27-1266 -05	Left Head Siderail Cover	1
20	QP27-1274-08	Left Siderail Handle	1
22	QP27-1496-05	Head Siderail Cap	1
23	QP28-0039-10	Siderail Rotation Lever Cover	2
24	QPA27-1270	Left Head Siderail Structure	1
25	QPA28-0015	Siderail Sleeve	1
26	QPA28-0016	Sleeve with Lock	1
27	QRE27-1736	Spring Balance	1
28	VV10A0G16-S	Hexagon Socket Hd. Screw	2
29	VV10A0G40-S	Hexagon Socket Hd. Screw	4
30	VV10A1P20-S	Hexagon Socket Hd. Screw	1
31	VV23A9C12HL	Pan Hd. Screw Type Hi-Lo	22
32	VV31A0G16	Flat Hd. Machine Screw	2
34	VVB3A9N24PF	Bosscrew Screw	5
35*	QDF27-1156	Brake Board Cable	1
36*	QDF27-2212	Head Siderail Wire	1
37*	QDF9518	Cable Tie	1
39*	QDF27-1521	Siderail Limit Switch S.A.	1
40	27-1839	Side Ring	1
41*	QDF2088	Polarized 6-Position Connector	1
42*	QDF9028	3-Position Connector	1
43*	QDF2087	2-Position Connector	1
44	VV23A9C20HL	Pan Head hi-Low Screw	8
45	VV87A9A20	Truss Head Tapping Screw	1
46*	M0019	OG2 Grade Grease	1
47*	QDF2127	2 Pins Connector	1

Standard Siderail Assembly, Head End, Left

(Applies to beds with Serial Numbers U02818 - Current)


27-2288 Rev-04 (Reference Only)

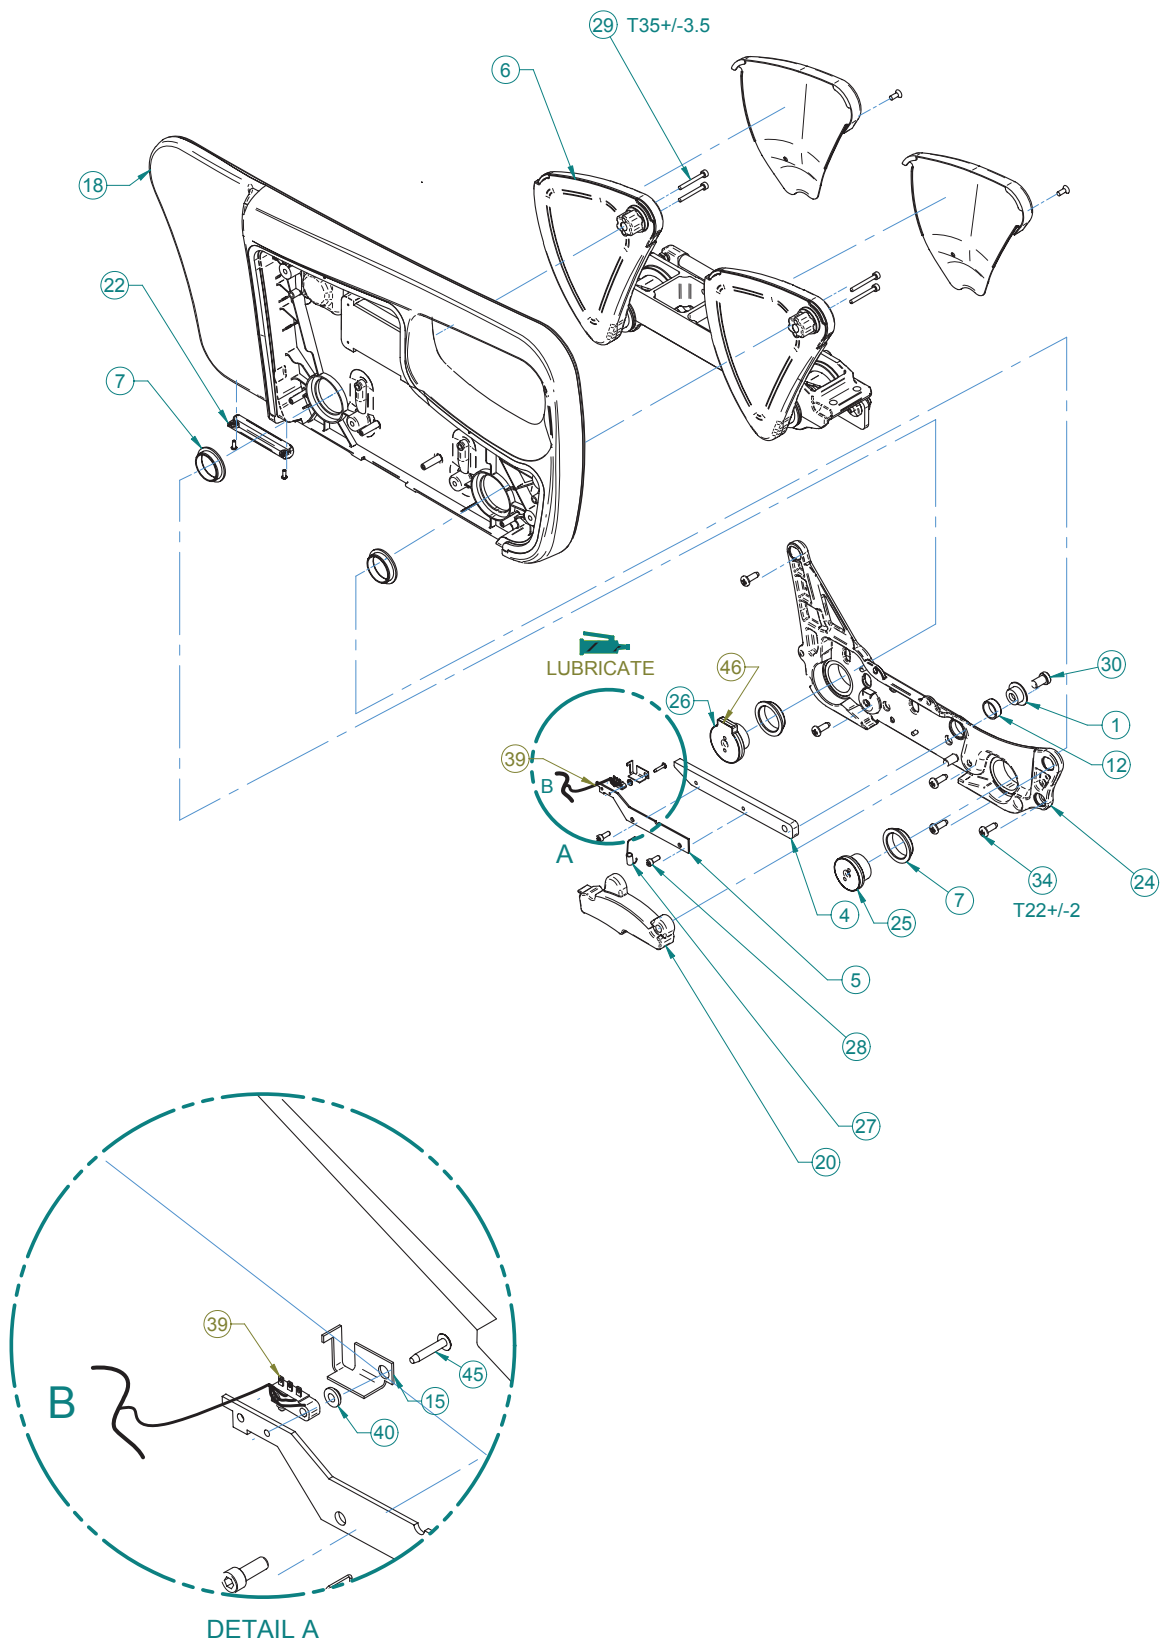

[Return To Table of Contents](#)

Standard Siderail Assembly, Head End, Left

(Applies to beds with Serial Numbers U02818 - Current)

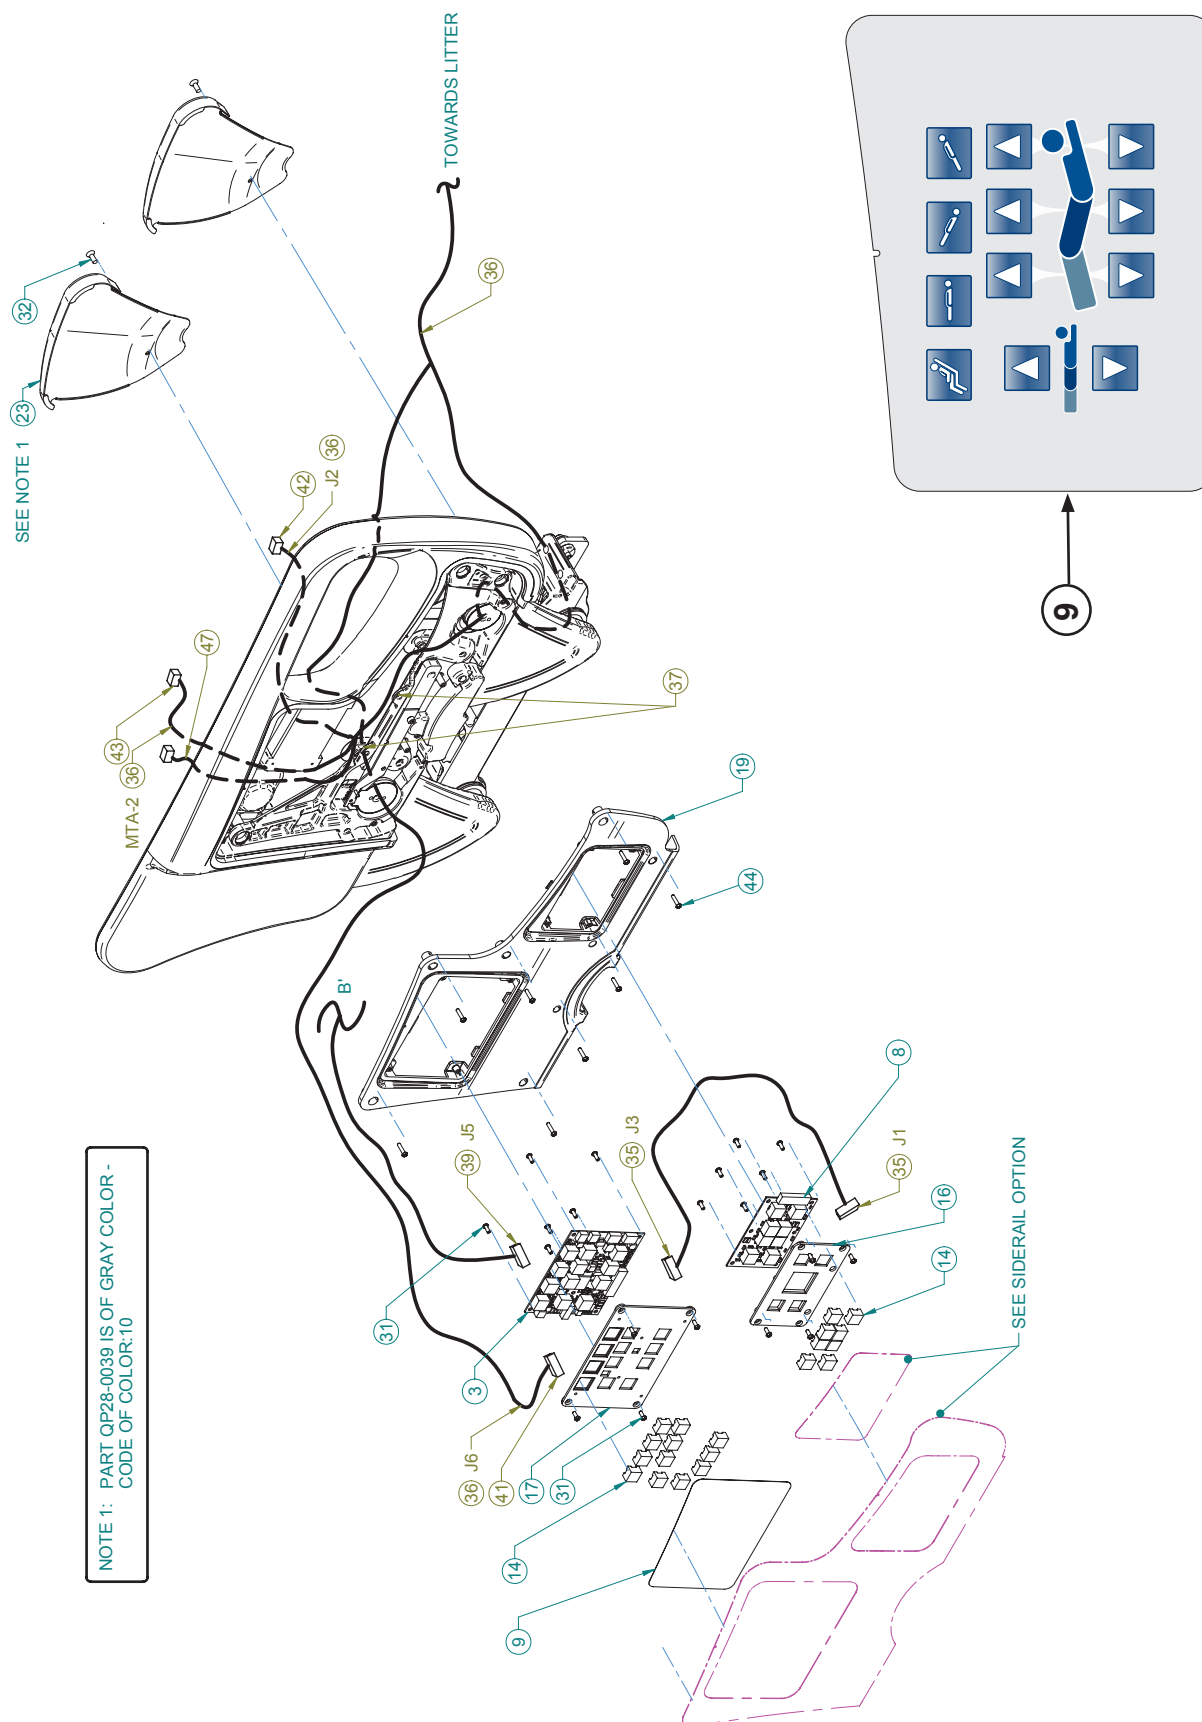

Standard Siderail Assembly, Head End, Left

(Applies to beds with Serial Numbers U02818 - Current)

POSITION ON CONNECTOR						
Cable 36	Position on Connector 47	Position on Connector 41	Position on Connector 43	Position on Connector 42	Signal	Color
1	-	1	-	-	"CAN H"	Black / Red
2	-	2	-	-	"CAN L"	Red
3	-	3	-	-	+12V	Black / White
4	-	4	-	-	"GND"	White
5	-	5	-	-	"SAFE"	Black / Green
6	-	6	-	-	+24V	Green
-	-	-	-	-	Audioshield	-
1	-	-	1	-	"SPK HIGH"	Black
2	-	-	2	-	"SPK COM"	White
1	-	-	-	1	N.O.	Red
2	-	-	-	2	COM	Green
3	-	-	-	3	N.C.	Brown
1	1	-	-	-	Speaker	Blue
2	2	-	-	-	Speaker	Orange

DIP SWITCH SETUP ON QDF27-1099			
SW13	OFF	ON	ON
SW14	OFF	OFF	-

CABLES CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-1681	MTA – 3 Positions	To	QDF27-1099	J5
QDF27-1156	MTA – 6 Positions	To	QDF27-1099	J3
QDF27-1156	MTA – 6 Positions	To	QDF27-1097	J1
QDF27-1784	MTA – 3 Positions	To	QDF27-2212	MTA-2 Positions
QDF27-2212	Mate N Lock 12 Positions	To	QDF27-2213	J105 (L27-038)
QDF27-2212	MTA – 6 Positions	To	QDF27-1099	J6
QDF27-2212	MTA – 3 Positions	To	See OL270162 OL270163, OL270164, OL270173, OL270174, OL270175	
QDF27-2212	MTA – 2 Positions	To		
QDF27-2212	Connector 2 Pins	To		

Standard Siderail Assembly, Head End, Left

(Applies to beds with Serial Numbers U02818 - Current)


Standard Siderail Assembly, Head End, Left - 27-2288 Rev-04 (Reference Only)

Item	Part No.	Part Name	Qty.
1	QPA28-0493	Siderail Sleeve	1
3	QDF27-1099	Siderail Nurse Control Board	1
4	QDF27-2574Z	Siderail Lock	1
5	27-2575Z	Switch Support	1
6	27-2060W	Siderail Mechanics S.A.	1
7	QDF2049	Spacer	4
8	QDF27-1097	Brake Control Board	1
9	QDF27-2238	Left Head Nurse Control Fascia	1
12	QDF28-0491	Machining Spacer QDF9191	1
14	QDF9183	Electronic Board Button	20
15	27-2293Z	Switch Guide 1	1
16	QP27-1109-10	Brake Board Support	1
17	QP27-1111	Nurse Control Board Support	1
18	QP27-2226-05	Left Head Siderail	1
19	QP27-1266 -05	Left Head Siderail Cover	1
20	QP27-1274-08	Left Siderail Handle	1
22	QP27-1496-05	Head Siderail Cap	1
23	QP28-0039-10	Siderail Rotation Lever Cover	2
24	QPA27-2296	Left Head Siderail Structure	1
25	QPA28-0015	Siderail Sleeve	1
26	QPA28-0016	Sleeve with Lock	1
27	QRE27-1736	Spring Balance	1
28	VV10A0G16-S	Hexagon Socket Head Screw	2
29	VV10B0G40-S	Hexagon Socket Head Screw	4
30	VV10A1P20-S	Hexagon Socket Head Screw	1
31	VV23A9C12HL	Pan Hd. Screw Type Hi-Lo	22
32	VV31A0G16	Flat Hd. Machine Screw	2
34	VVB3A9N24PF	Bosscrew Screw	5
35*	QDF27-1156	Brake Board Cable	1
36*	QDF27-2212	Head Siderail Wire	1
37*	QDF9518	Cable Tie	1
39*	QDF27-1521	Siderail Limit Switch S.A.	1
40	27-1839	Side Ring	1
41*	QDF2088	Polarized 6-Position Connector	1
42*	QDF9028	3-Position Connector	1
43*	QDF2087	2-Position Connector	1
44	VV23A9C20HL	Pan Head hi-Low Screw	8
45	VV87A9A20	Truss Head Tapping Screw	1
46*	M0019	OG2 Grade Grease	1
47*	QDF2127	2 Pins Connector	1



Standard Siderail Assembly, Labeling

OL270180-XXX Rev-02 (Reference Only)


Head End Right

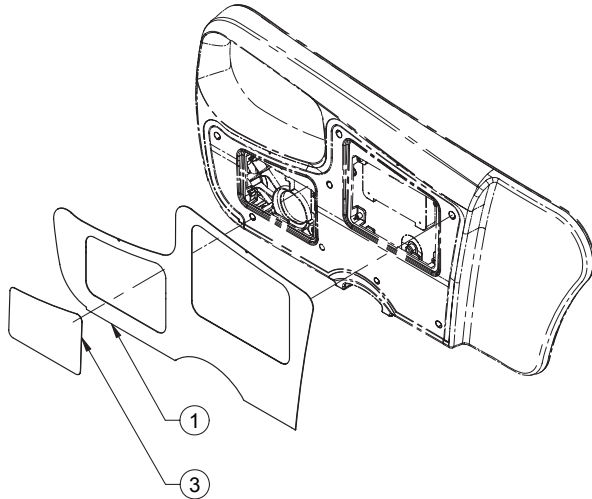

Head End Left

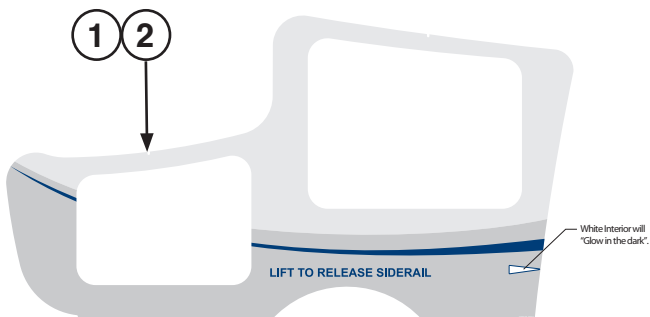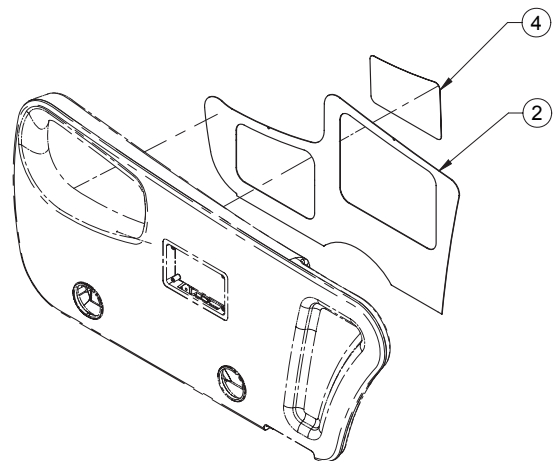

Right label shown (QDF27-0906)

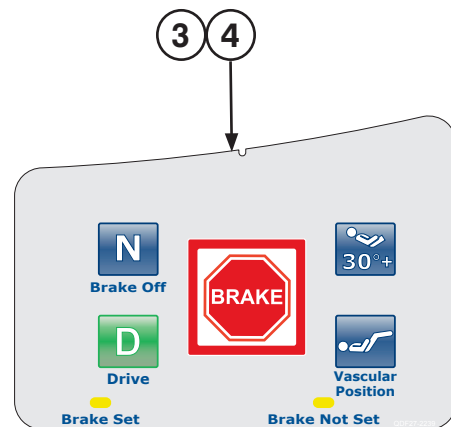


Right label shown (QDF27-2239)

NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF27-0906-XXX	Nurse Control Label, HE, Right	1
2	QDF27-0907-XXX	Nurse Control Label, HE, Left	1
3	QDF27-2239-XXX	Brake Control Label, HE, Right	1
4	QDF27-2240-XXX	Brake Control Label, HE, Left	1

Optional Siderail Assembly, Head End, without Speaker/without NC


OL270175 Rev-00 (Reference Only)

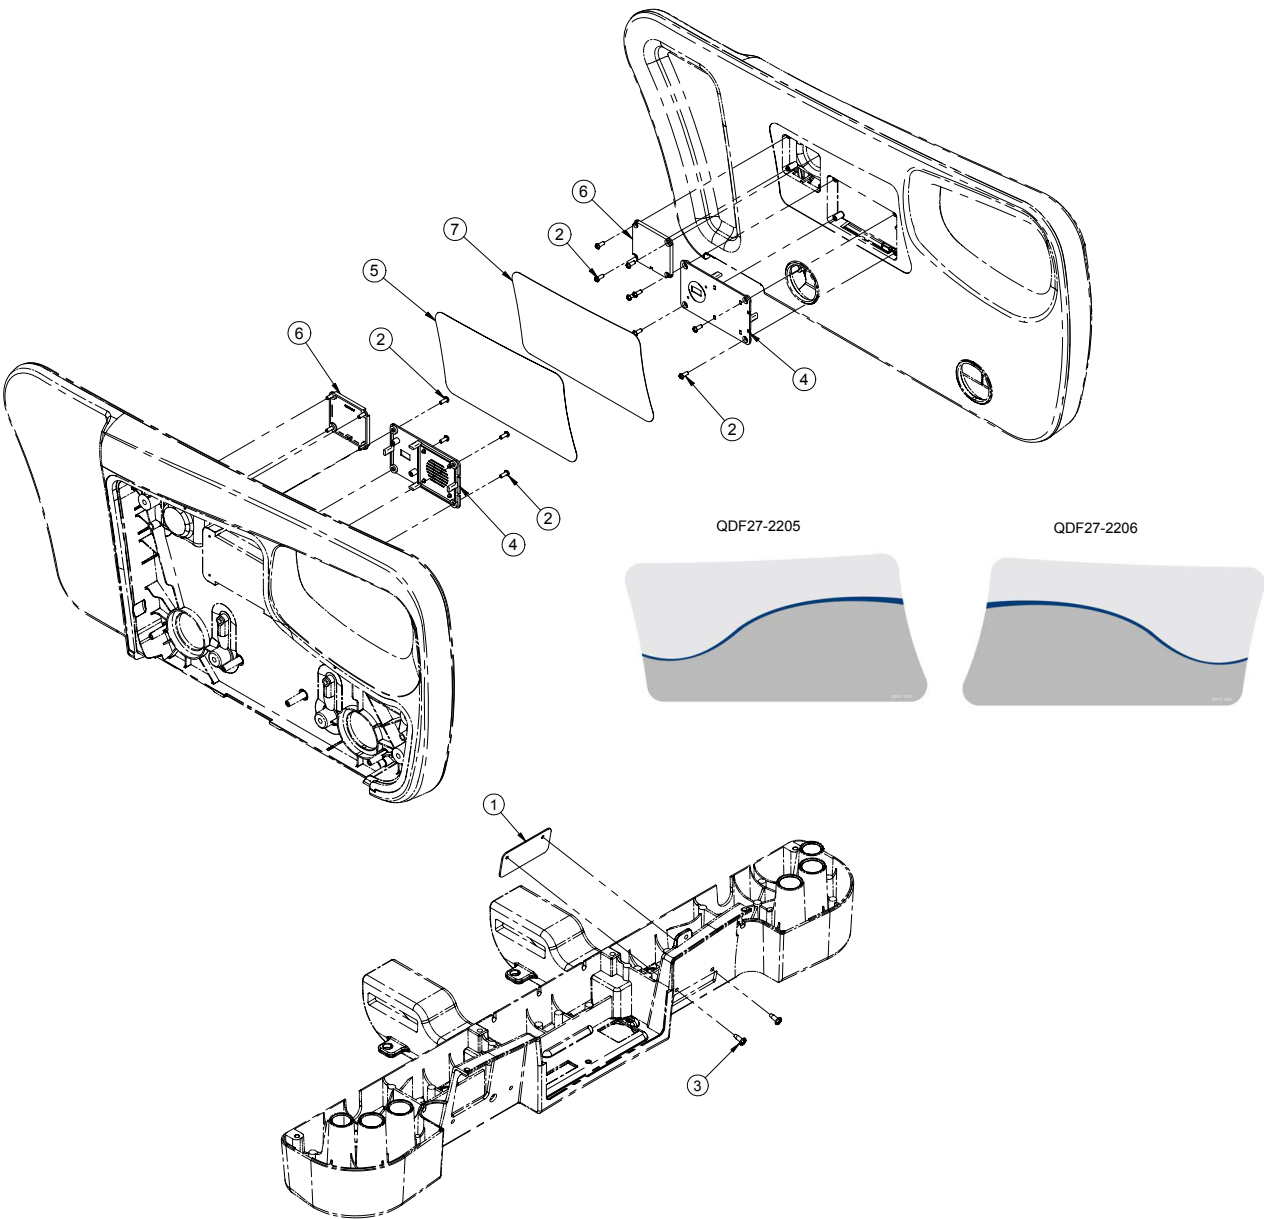

Item	Part No.	Part Name	Qty.
1	27-2137P	Plate without Nurse Call	1
2	VV23A9C12HL	Pan Head Tapping Screw	16
3	VV83A9G16	Pan Head Tapping Screw	2
4	QP27-2136	Nurse Call Support	2
5	QDF27-2206	Left Patient Control	1
6	QP27-2197	Head Speaker Cover	2
7	QDF27-2205	Right Patient Control	1

Optional Siderail Assembly, Head End, with Speaker/without NC

OL270310 Rev A (Reference Only)

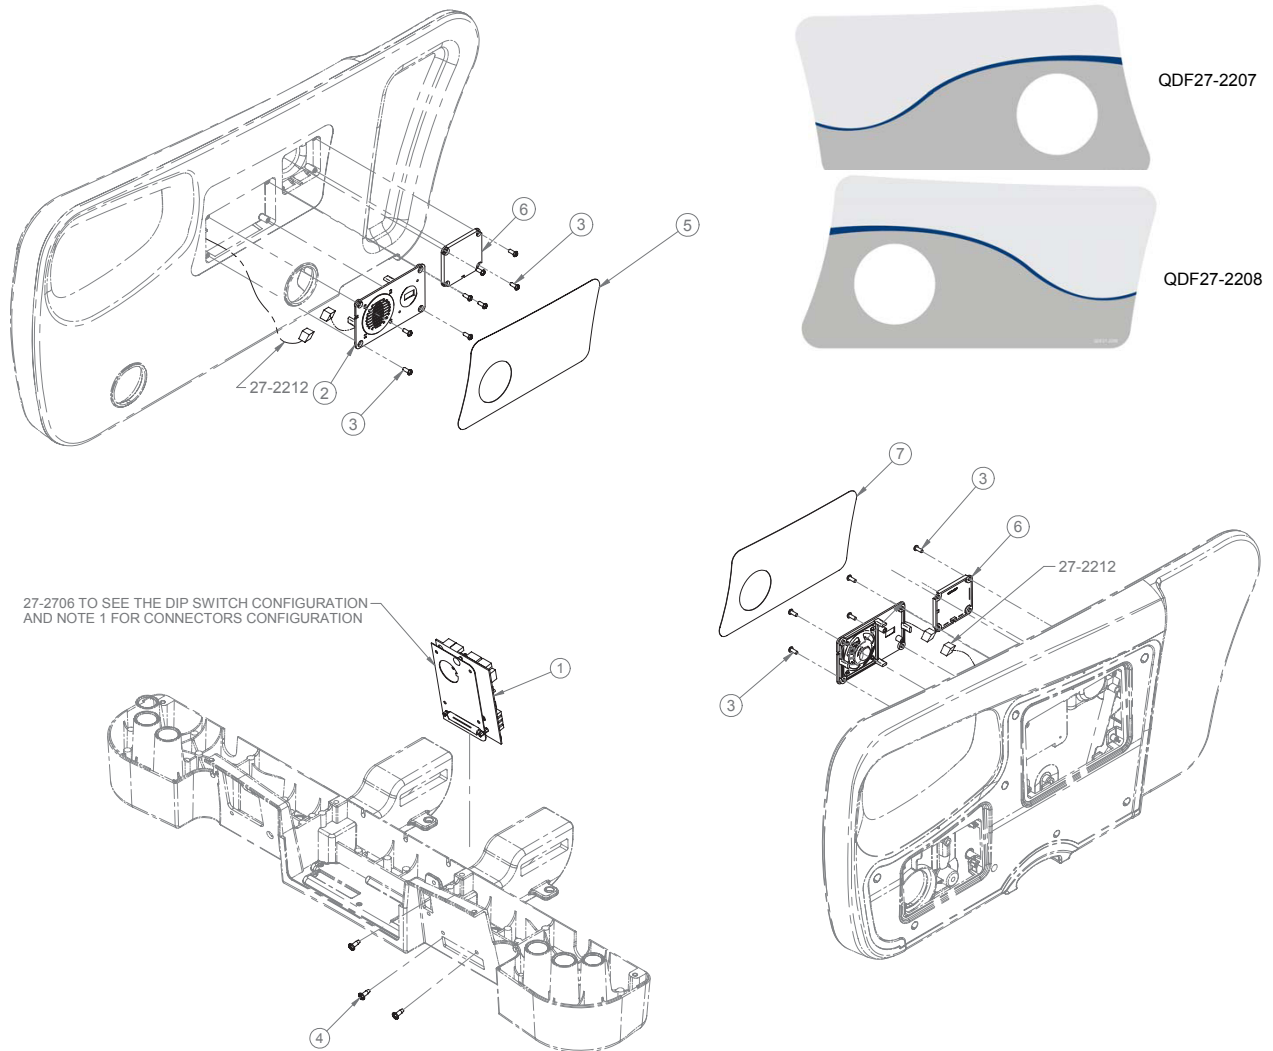

Cable No.	Cable Connection	To	Cable No.	Cable Connection
QDF27-2175	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Left)
QDF27-2216	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Right)


Optional Siderail Assembly, Head End, with Speaker/without NC - OL270310 Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF75-0270	Room Interface Board	1
2	QDF27-2175	Siderail Speaker, Left	1
3	VV23A9C12HL	Pan Head Tapping Screw	13
4	VV83A9G16	Pan Head Tapping Screw	3
5	QDF27-2208	Left Communications Label	1
6	QP27-2197	Head Speaker Cover	2
7	QDF27-2207	Right Communications Label	1
8	QDF27-2216	Right Siderail Speaker, Right	1

[Return To Table of Contents](#)

Optional Siderail Assembly, Head End, with Speaker/iAudio

OL270308 Rev A (Reference Only)

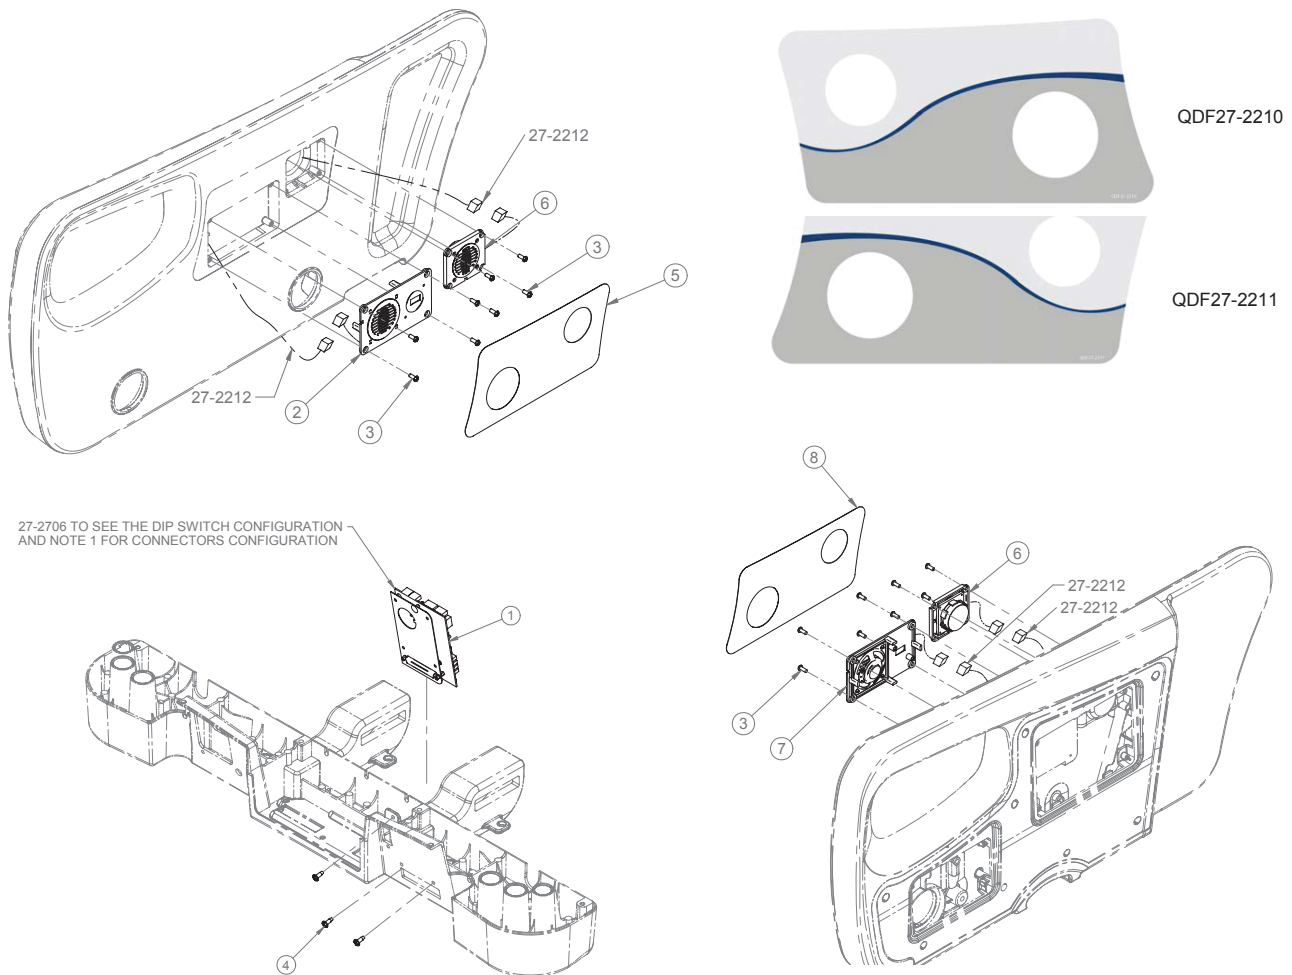


Cable No.	Cable Connection	To	Cable No.	Cable Connection
QDF27-2175	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Left)
QDF27-2216	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Right)
QDF27-2196	2 Position Conn.	To	QDF27-2212	(Standard Siderail Assembly, Head End, Left) and (Standard Siderail Assembly, Head End, Right)

Optional Siderail Assembly, Head End, with Speaker/iAudio - OL270308 Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF75-0270	Room Interface Board	1
2	QDF27-2175	Siderail Speaker, Left	1
3	VV23A9C12HL	Pan Head Tapping Screw	16
4	VV83A9G16	Pan Head Tapping Screw	3
5	QDF27-2211	Left Communications Label	2
6	QDF27-2196	Head Speaker	2
7	QDF27-2216	Siderail Speaker, Right	1

Optional Siderail Assembly, Head End, with Speaker/with NC

OL270309 Rev A (Reference Only)

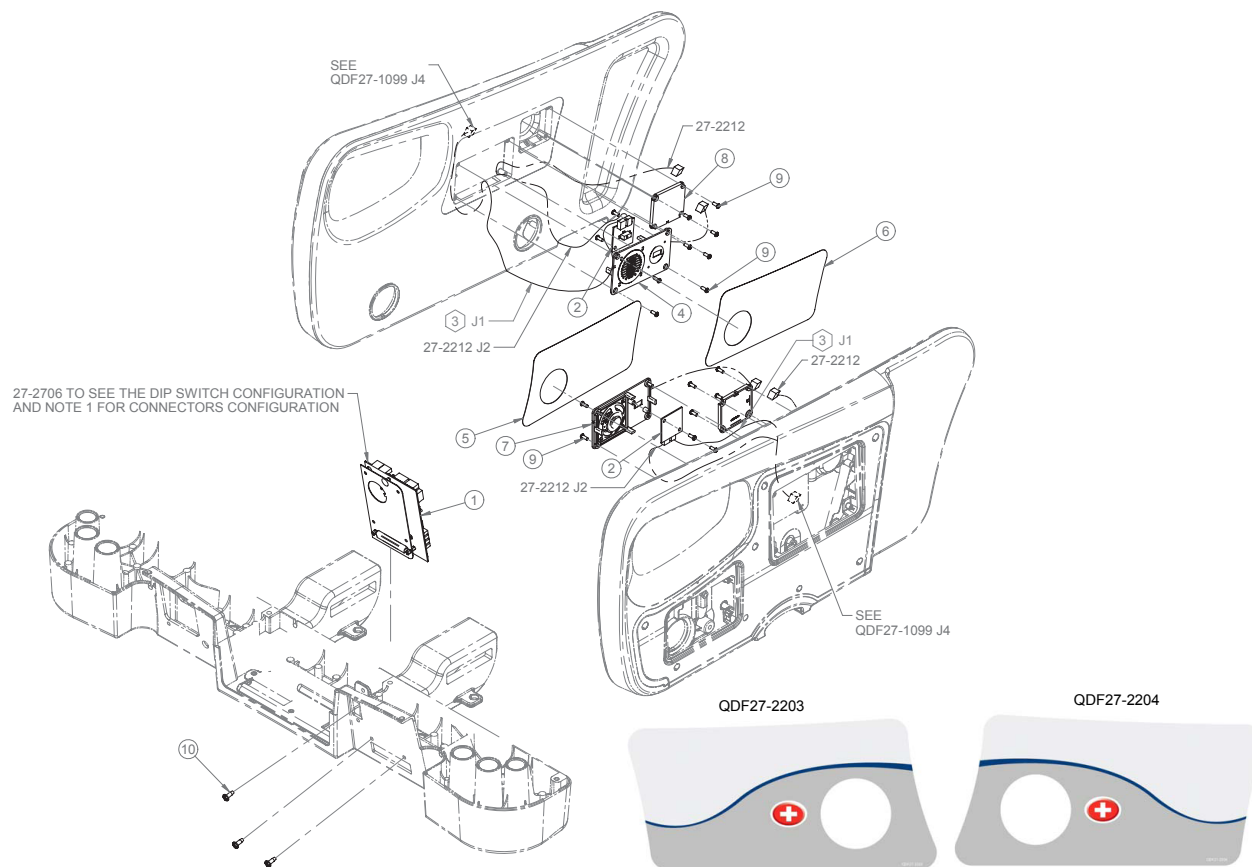

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2175	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Left)
QDF27-1429	J1	To	QDF27-1682	MTA-3 Positions
QDF27-1429	J2	To	QDF27-1206	MTA-3 Positions (Standard Siderail Assembly, Head End, Right)
QDF27-1682	MTA-3 Positions	To	QDF27-1429	J1
QDF27-1682	MTA-3 Positions	To	QDF27-1099	J4 (Standard Siderail Assembly, Head End, Left) and (Standard Siderail Assembly, Head End, Right)
QDF27-2216	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Right)


Optional Siderail Assembly, Head End, with Speaker/with NC - OL270309 Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF75-0270	Room Interface Board	1
2	QDF27-1429	Nurse Call Board	2
3*	QDF27-1682	Siderail Nurse Call Wires	2
4	QDF27-2175	Left Siderail Speaker	1
5	QDF27-2203	Right Nurse Call Fascia	1
6	QDF27-2204	Left Nurse Call Fascia	1
7	QDF27-2216	Right Siderail Speaker	1
8	QP27-2197	Head Speaker Cover	2
9	VV23A9C12HL	Pan Head Tapping Screw	20
10	VV83A9G16	Pan Head Tapping Screw	3

[Return To Table of Contents](#)

Optional Siderail Assembly, Head End, with iAudio - OL270164

OL270164 Rev-02 (Reference Only)


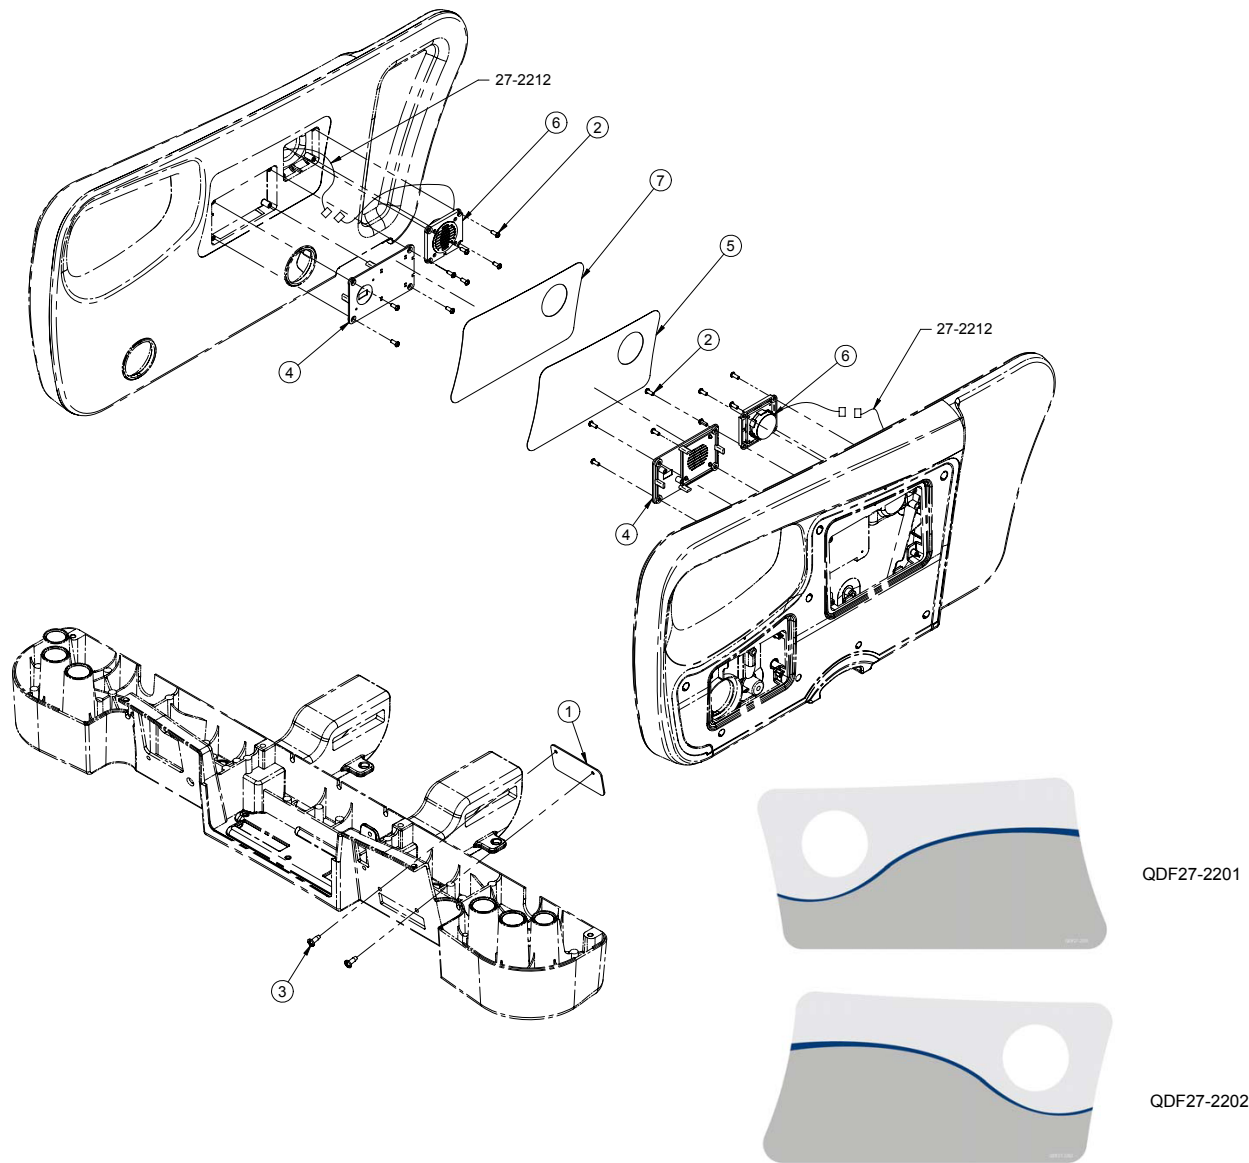


Cable No.	Cable Connection	To	Cable No.	Cable Connection
QDF27-2196	2 Position Conn.	To	QDF27-2212	(27-2257, 27-2258)


Item	Part No.	Part Name	Qty.
1	27-2137P	Plate without Nurse Call	1
2	VV23A9C12HL	Pan Head Tapping Screw	16
3	VV83A9G16	Pan Head Tapping Screw	2
4	QP27-2136	Nurse Call Support	2
5	QDF27-2201	Right iAudio Speaker Fascia	1
6	QDF27-2196	Head Speaker	2
7	QDF27-2202	Left iAudio Speaker Fascia	1

Optional Siderail Assembly, Head End, with Speaker/with NC/with *i*Audio

OL270311 Rev A (Reference Only)

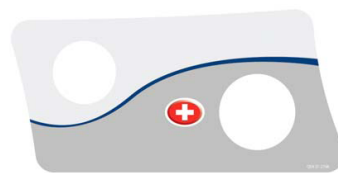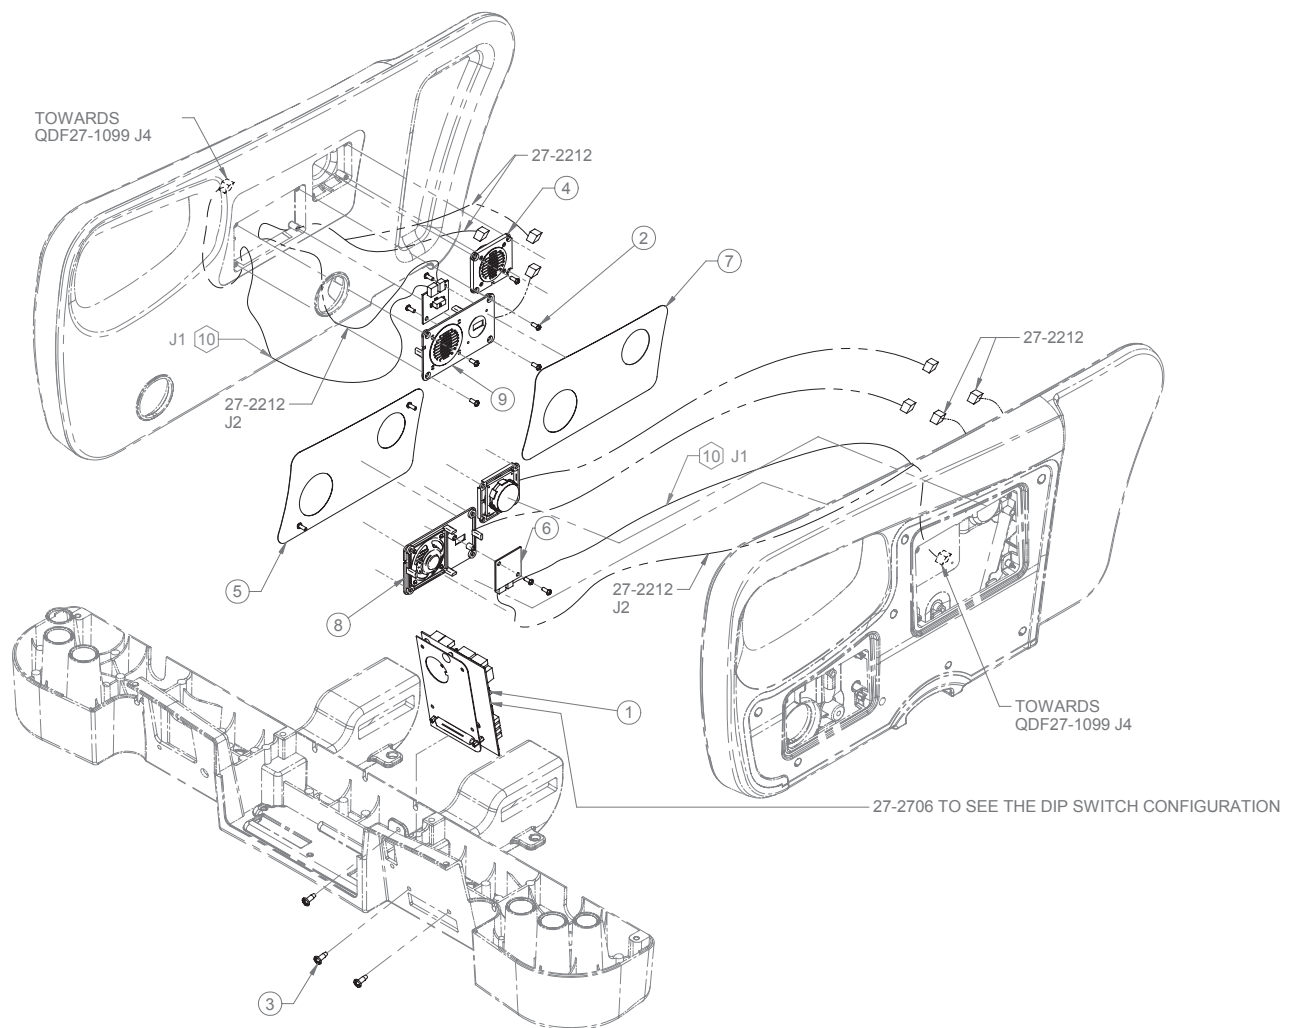

QFD27-2198

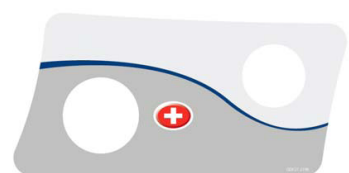

QFD27-2199

Optional Siderail Assembly, Head End, with Speaker/with NC/with iAudio


Optional Siderail Assembly, HE, with Speaker/with NC/with iAudio - OL270311 Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF75-0270	Room Interface Board	1
2	VV23A9C12HL	Pan Head Tapping Screw	20
3	VV83A9G16	Pan Head Tapping Screw	3
4	QDF27-2196	Head Speaker	2
5	QDF27-2198	Nurse Call and Speaker Fascia, Right	1
6	QDF27-1429	Nurse Call Board	2
7	QDF27-2199	Nurse Call and Speaker Fascia, Left	1
8	QDF27-2216	Siderail Speaker, Right	1
9	QDF27-2175	Siderail Speaker, Left	1
10*	QDF27-1682	Siderail Nurse Call Wires	2

Cable No.	Cable Connection	To	Cable No.	Cable Connection
QDF27-2175	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Left)
QDF27-1429	J1	To	QDF27-1682	MTA-3 Positions
QDF27-1429	J2	To	QDF27-1206	MTA-3 Positions (Standard Siderail Assembly, Head End, Left) and (Standard Siderail Assembly, Head End, Right)
QDF27-1682	MTA-3 Positions	To	QDF27-1429	J1
QDF27-1682	MTA-3 Positions	To	QDF27-1099	J4 (Standard Siderail Assembly, Head End, Left) and (Standard Siderail Assembly, Head End, Right)
QDF27-2216	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Right)
QDF27-2196	2 Positions Conn.	To	QDF27-2212	(Standard Siderail Assembly, Head End, Left) and (Standard Siderail Assembly, Head End, Right)



Optional Siderail Assembly, Head End, with Speaker/with NC/ with *i*Audio/with *i*Bed® Wireless

OL270302 Rev B (Reference Only)

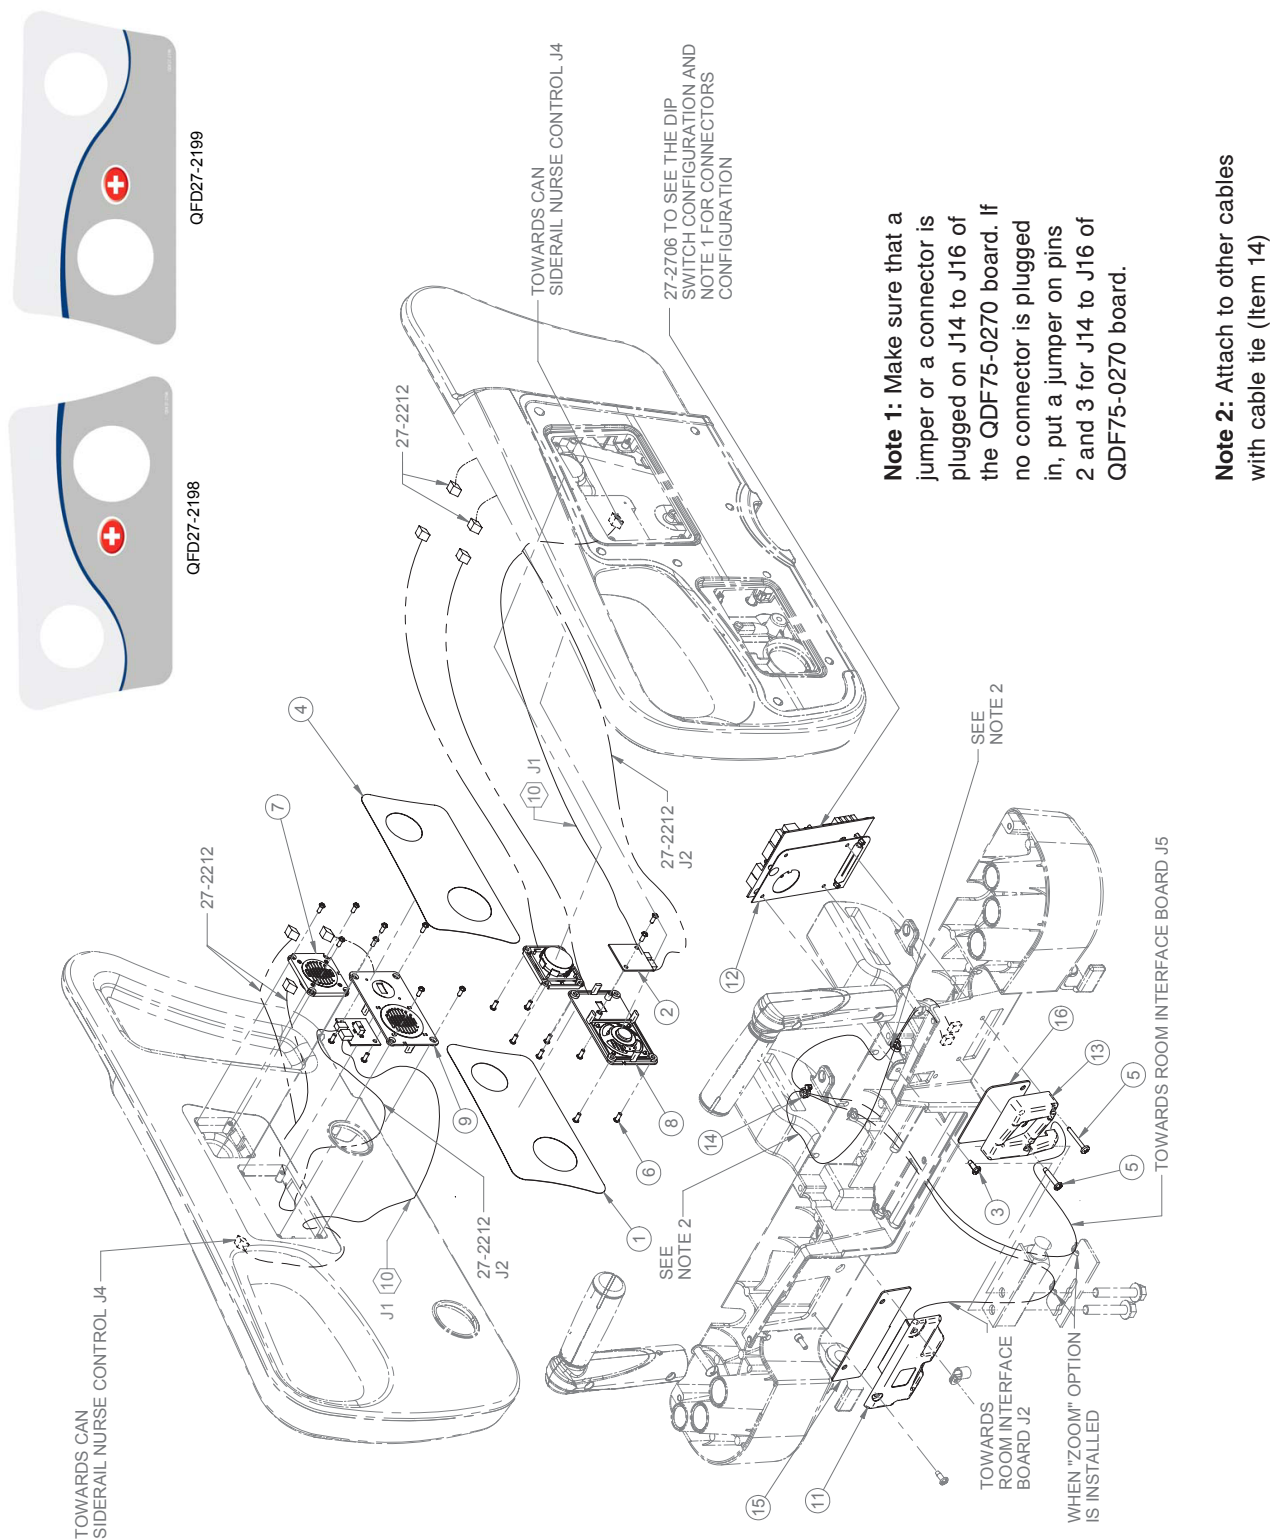

Optional Siderail Assembly, Head End, with Speaker/with NC/ with *i*Audio/with *i*Bed® Wireless

Path of IR Module Cables to the Room Interface Board

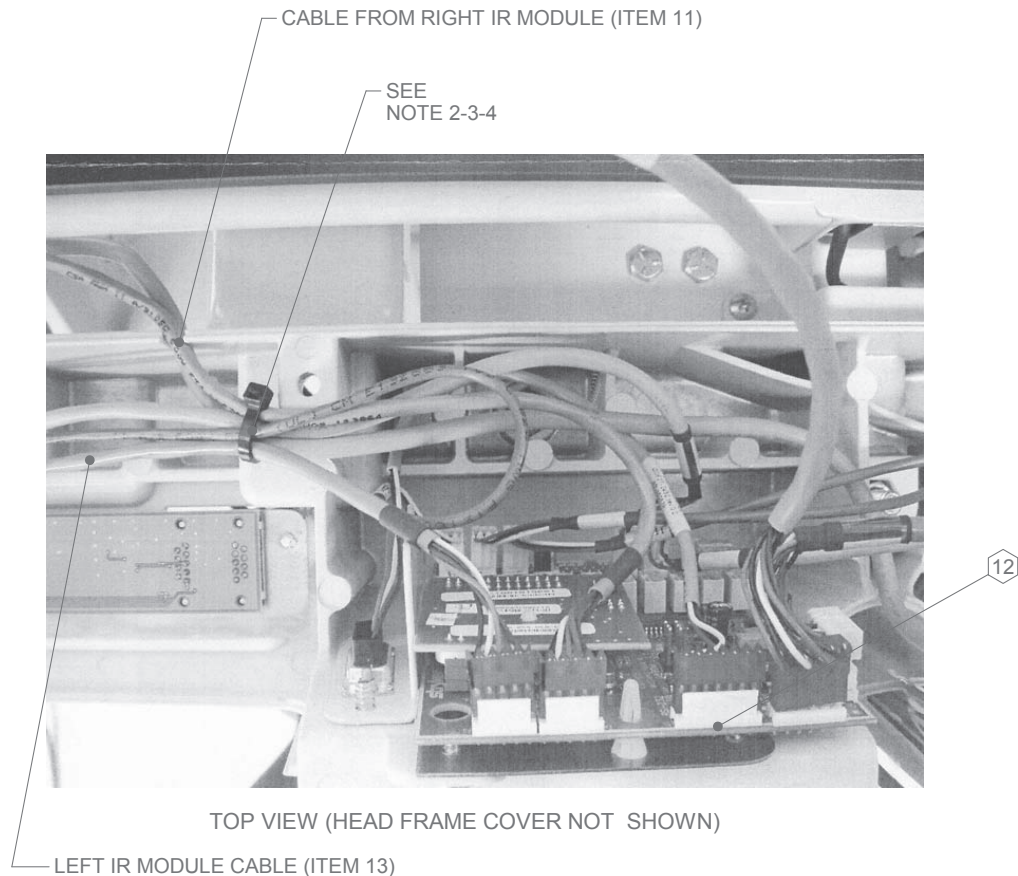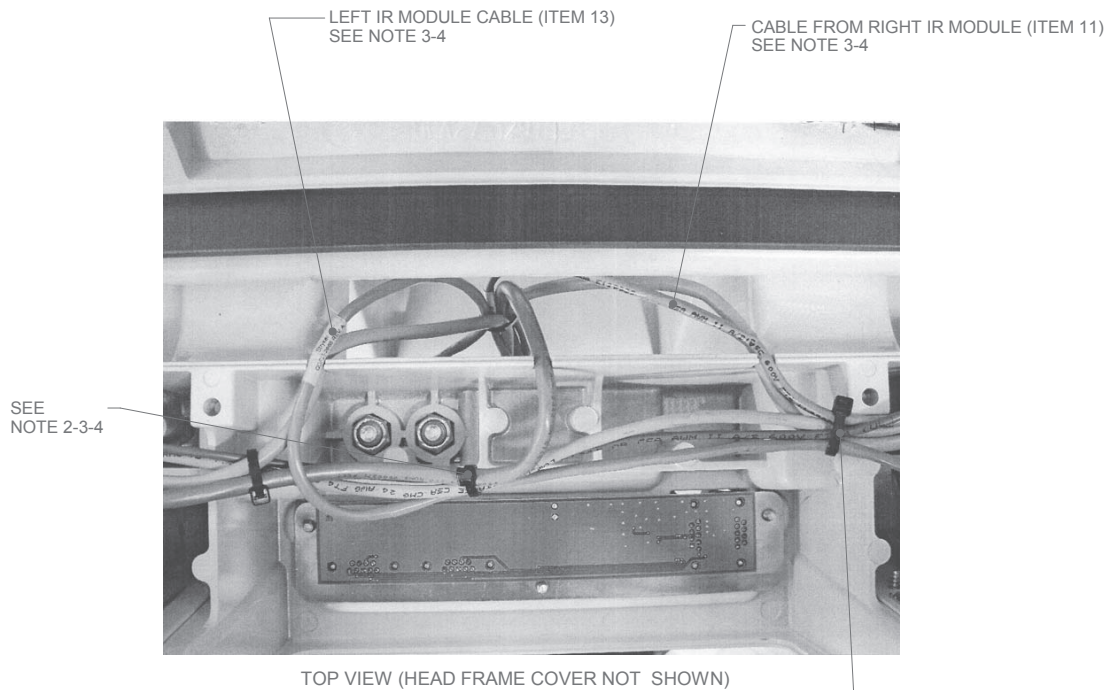

Optional Siderail Assembly, Head End, with Speaker/with NC/ with *i*Audio/with *i*Bed® Wireless

Path of IR Module Cables to the Room Interface Board



[Return To Table of Contents](#)

Optional Siderail Assembly, Head End, with Speaker/with NC/ with *i*Audio/with *i*Bed® Wireless

Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2175	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Left)
QDF27-1429	J1	To	QDF27-1682	MTA-3 Positions
QDF27-1429	J2	To	QDF27-1206	MTA-3 Positions (Standard Siderail Assembly, Head End, Left) and (Standard Siderail Assembly, Head End, Right)
QDF27-1682	MTA-3 Positions	To	QDF27-1429	J1
QDF27-1682	MTA-3 Positions	To	QDF27-1099	J4 (Standard Siderail Assembly, Head End, Left) and (Standard Siderail Assembly, Head End, Right)
QDF27-2216	MTA-2 Positions	To	QDF27-2212	MTA-2 Positions (Standard Siderail Assembly, Head End, Right)
QDF27-2196	2 Positions Conn.	To	QDF27-2212	(Standard Siderail Assembly, Head End, Left) and (Standard Siderail Assembly, Head End, Right)


Optional Siderail Assembly, Head End, with Speaker/with NC /with *i*Audio/with *i*Bed® Wireless - OL270302 Rev B (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF27-2198	<i>i</i> Audio Speaker and Nurse Call Overlay, Right	1
2	QDF27-1429	Nurse Call Board	2
3	VV83A9G16	Pan Head Tapping Screw	1
4	QDF27-2199	<i>i</i> Audio Speaker and Nurse Call Overlay, Left	1
5	VV83A9G36	Round Head Tapping Screw	2
6	VV23A9C12HL	Pan Head Tapping Screw	20
7	QDF27-2196	Head Speaker Cover	2
8	QDF27-2216	Right Siderail Speaker	1
9	QDF27-2175	Left Siderail Speaker	1
10	QDF27-1682	Siderail Nurse Call Wires	2
11	27-2661	IR Module, Left	1
12	QDF75-0270	Room Interface Board	1
13	27-2662	IR Module, Right	1
14	QDF9518	Cable Tie	3
15	QP27-2735	IR Support Gasket, Left	1
16	QP27-2734	IR Support Gasket, Right	1

Siderail Mounting Assembly, Foot End

(Applies to beds with Serial Numbers U01001 - U02817)

L27-032 Rev-01 (Reference Only)

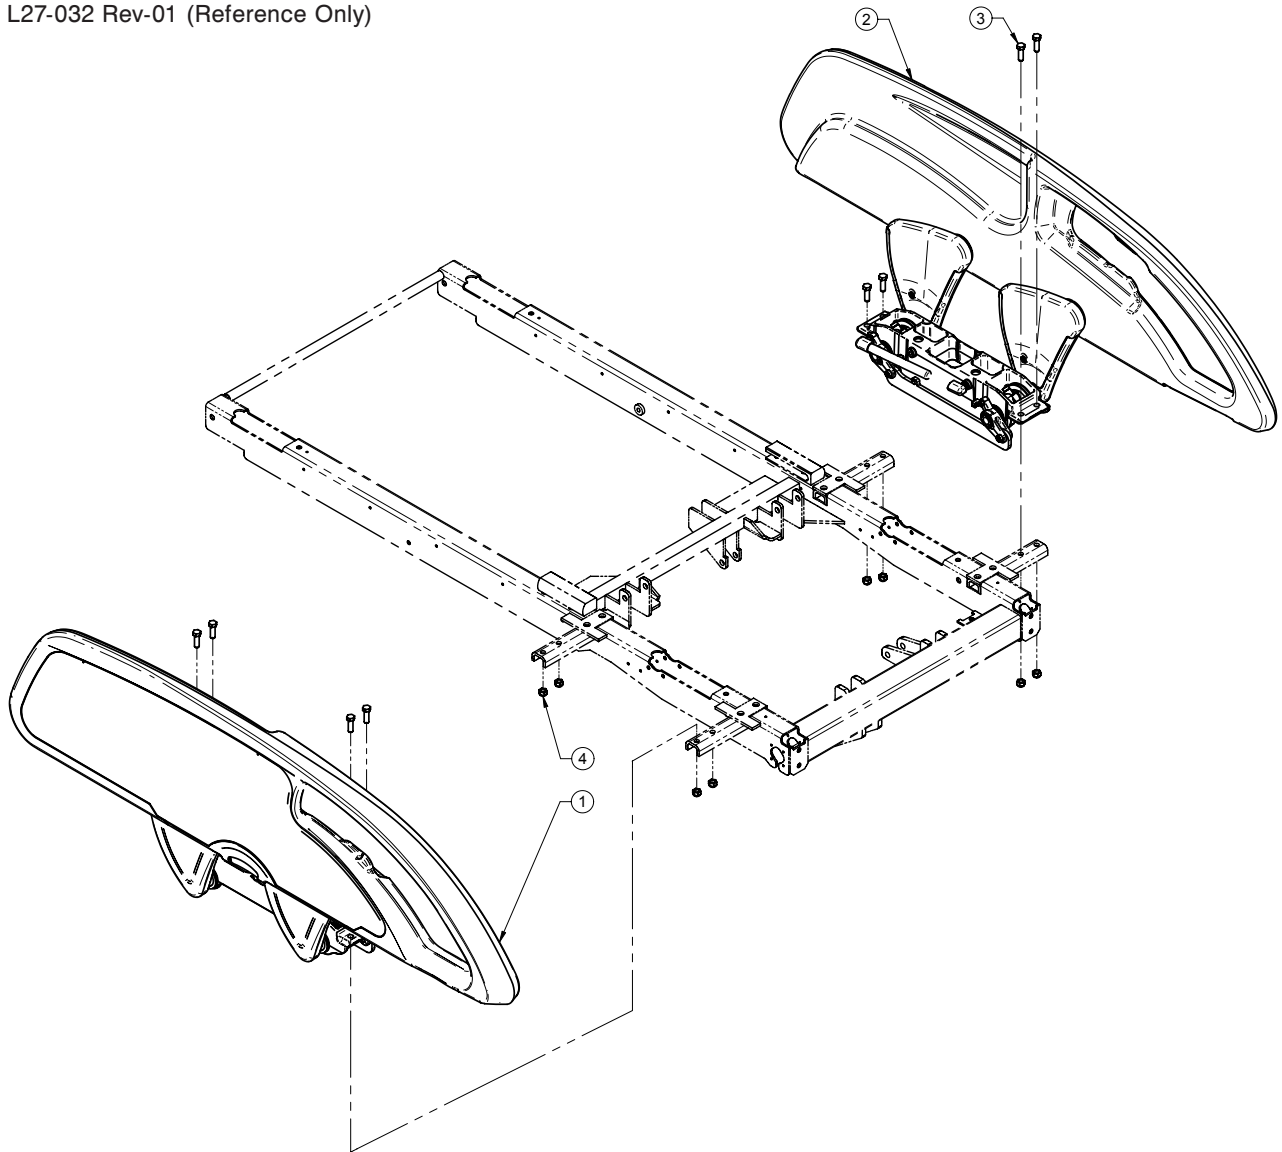


Item	Part No.	Part Name	Qty.
1	27-0389W	Right Foot Siderail Assembly	1
2	27-0390W	Left Foot Siderail Assembly	1
3	VB18A1032	Bolt	8
4	VE30A10	Nylon Locknut	8

Siderail Mounting Assembly, Foot End

(Applies to beds with Serial Numbers U02818 - Current)

L27-032 Rev-02 (Reference Only)


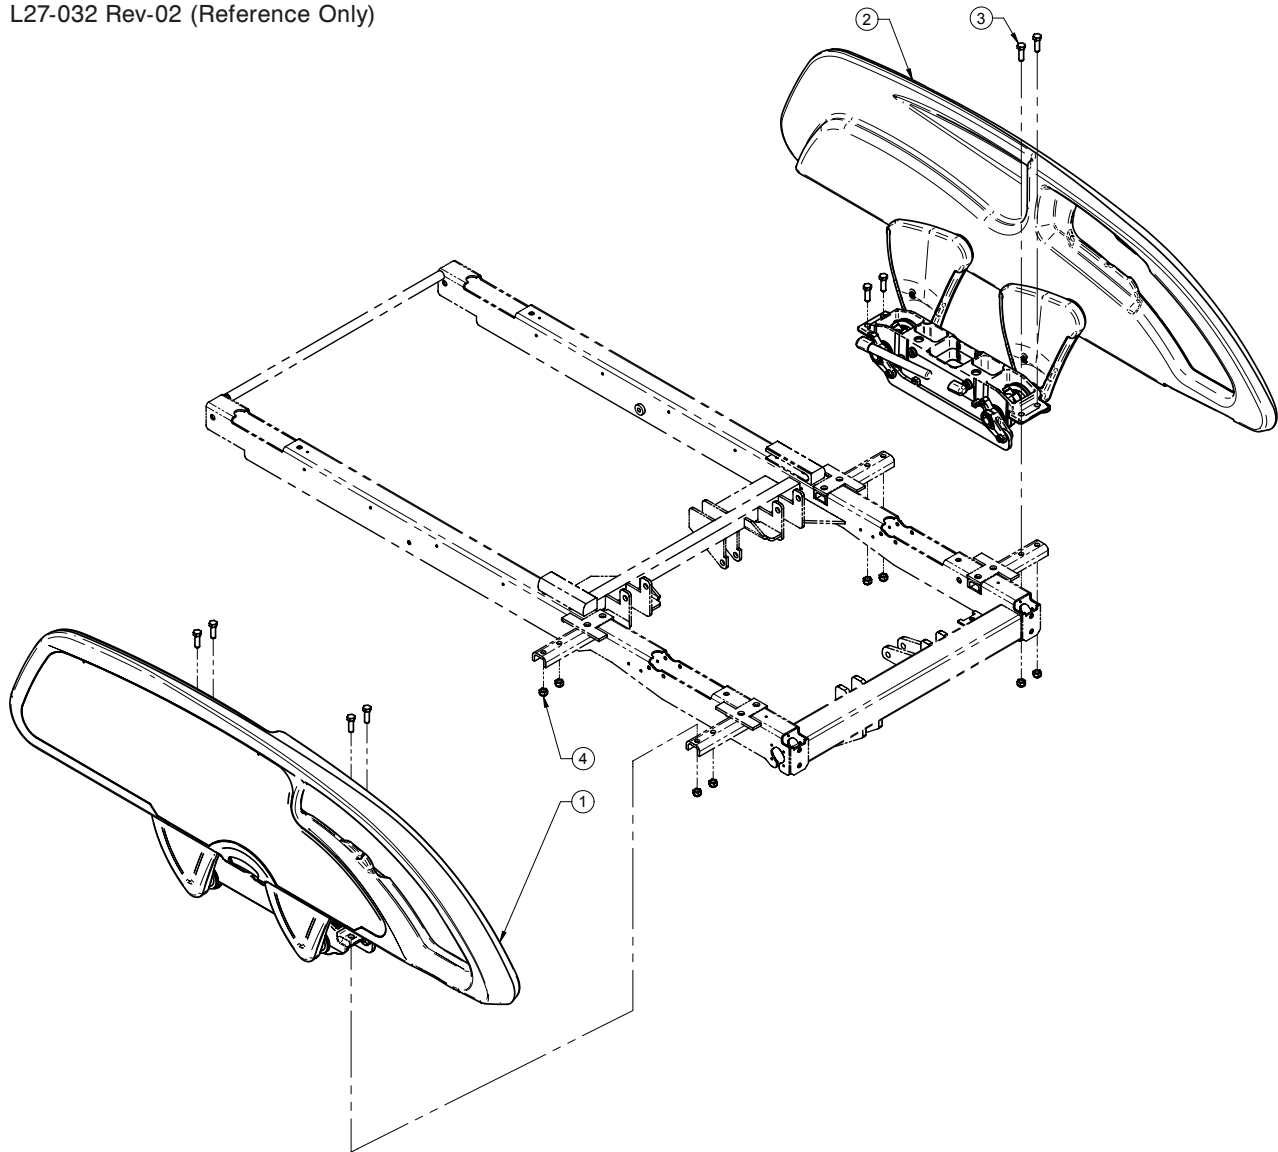


Item	Part No.	Part Name	Qty.
1	27-2289	Right Foot Siderail Assembly	1
2	27-2290	Left Foot Siderail Assembly	1
3	VB18A1O32	Bolt	8
4	VE30A1O	Nylon Locknut	8

Standard Siderail Assembly, Foot End, Right

(Applies to beds with Serial Numbers U01001 - U02817)

27-0389 Rev-19 (Reference Only)

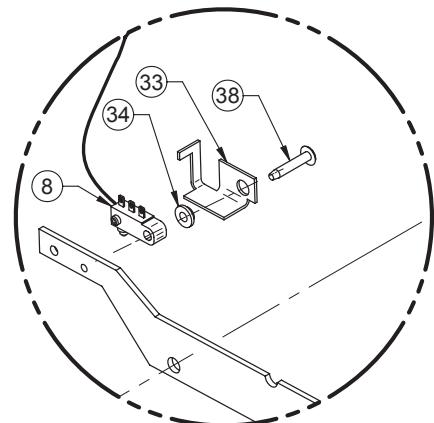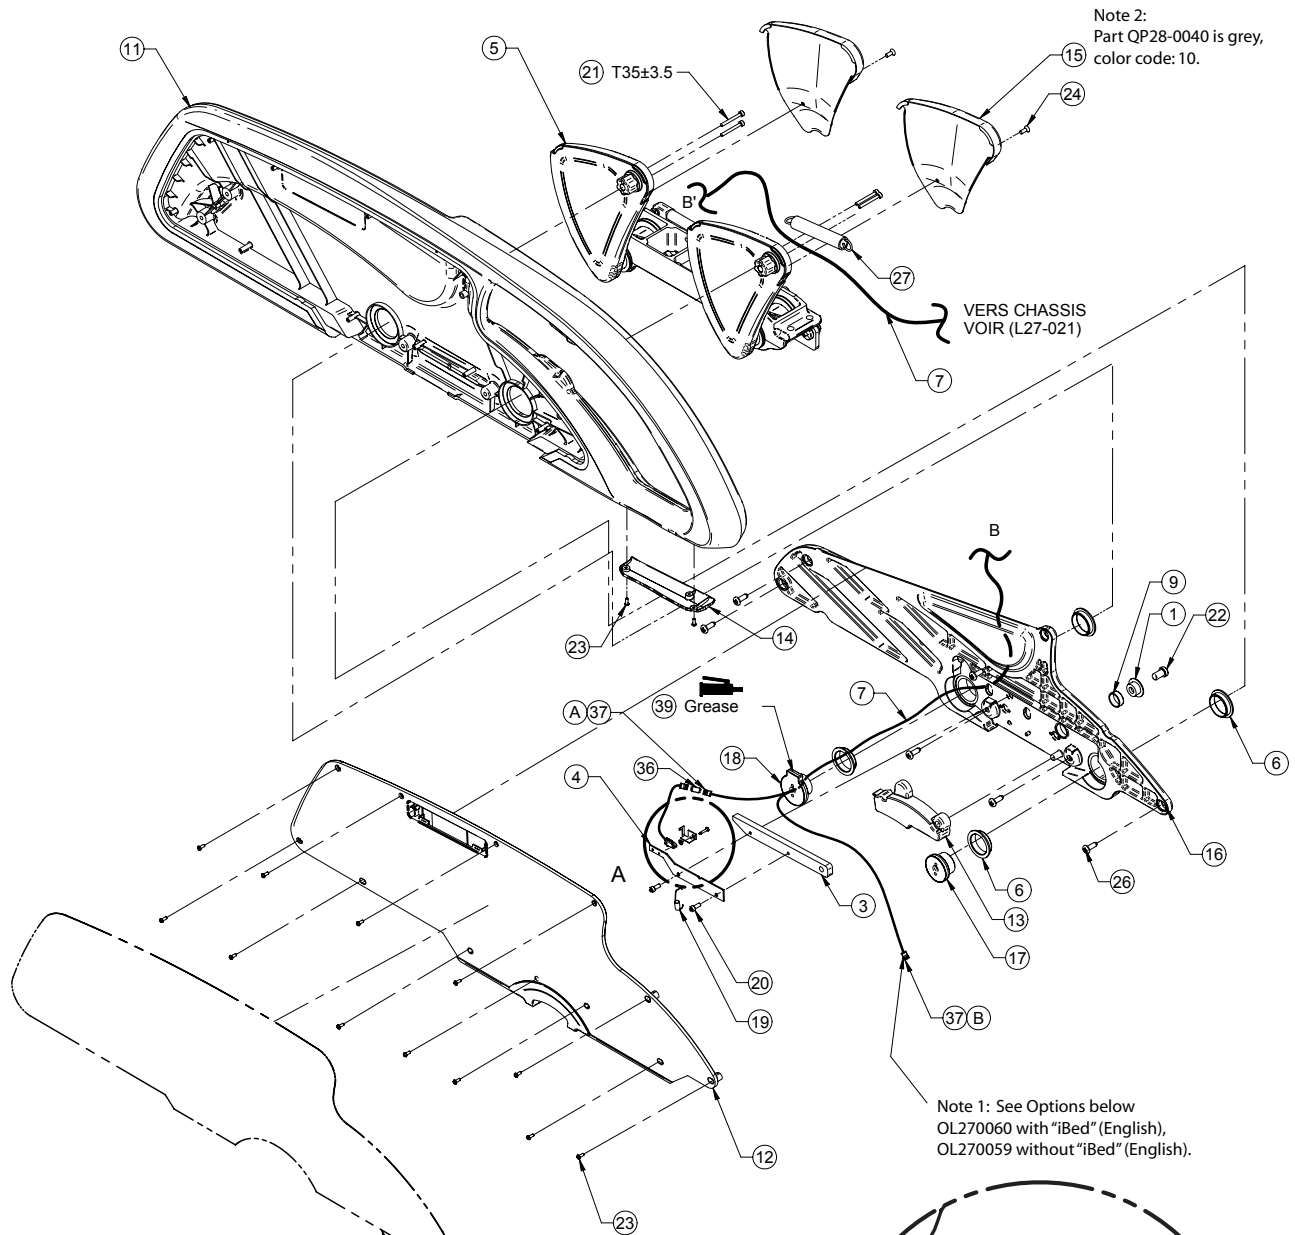

DETAIL A

[Return To Table of Contents](#)

Standard Siderail Assembly, Foot End, Right

(Applies to beds with Serial Numbers U01001 - U02817)

POSITION ON CONNECTOR			
Cable No.	Connector No.	Cable No.	Connector No.
QDF27-1521	MTA-100 3 Positions	QDF27-1208	MTA-100 3 Positions
QDF27-1208	MTA-100 3 Positions	QDF27-1521	MTA-100 3 Positions
QDF27-1208	Mate N Lock 3 Positions	QDF27-2213	J172 (L27-037)

POSITION ON CONNECTOR				
Cable QDF27-1208 ⑦	Signal	Color	Position on Connector ③⑦ A	Position on Connector ③⑦ B
1	NO SWITCH	White	1	-
2	COM SWITCH	Black	2	-
3	NC SWITCH	Green	3	-
4	LED1 LBS	Orange	-	1
5	+12V	Red	-	2
6	LED2 LBS	Blue	-	3

Note 1:

Siderail **without iBed** option - See OL270059-XXX ([page 283](#)).

Siderail **with iBed** option - See OL270060-XXX ([page 284](#)).

Standard Siderail Assembly, Foot End, Right

(Applies to beds with Serial Numbers U01001 - U02817)


Standard Siderail Assembly, Foot End, Right - Common Components - 27-0389 Rev-19 (Reference only)

Item	Part No.	Part Name	Qty.
1	QPA28-0493	Siderail Sleeve	1
3	QDB27-1141Z	Siderail Lock	1
4	27-1142Z	Siderail Switch Support	1
5	27-2060W	Siderail Mechanics	1
6	QDF2049	Spacer	4
7	QDF27-1208	Foot Limit Switch Siderail Cable	1
8	QDF27-1521	Siderail Switch	1
9	28-0491	QDF9191 Spacer Tooling	1
10	QDF7826	Tape	1
11	QP27-1263-05	Right Foot Siderail	1
12	QP27-1267-05	Left Foot Siderail Cover	1
13	QP27-1274-08	Left Siderail Trigger	1
14	QP27-1508-05	Right Foot Siderail Cap	1
15	QP28-0039-10	Siderail Rotation Arm Cover	2
16	QPA27-1271	Right Foot Siderail Structure	1
17	QPA29-0015	Siderail Sleeve	1
18	QPA28-0016	Sleeve with Lock	1
19	QRE27-1736	Spring Return	1
20	VV10A0G16-S	Hexagon Cylinder Head Screw	2
21	VV10A0G40-S	Hexagon Cylinder Head Screw	4
22	VV10A1P20-S	Hexagon Cylinder Head Screw	1
23	VV23A9C12HL	Pan Head Screw	15
24	VV31A0G16	Flat Head Machine Screw	2
26	VVB3A9N24PF	Screw Bosscrew	6
27	QRE28-0293	Siderail Tension Spring, K11	1
33	27-1740Z	Siderail Plate 1	1
34	27-1839	Spacer Washer	1
36	QDF2080	Inline Splice (ITW MWTZ 100-3-D)	1
37	QDF2099	Female Connector MTA-100 3 Pos.	2
38	VV87A9A20	Phillips Truss Head Tapping Screw	1
39	M0019	Grease	1


Standard Siderail Assembly, Foot End, Right

(Applies to beds with Serial Numbers U02818 - Current)

27-2289 Rev-03 (Reference Only)

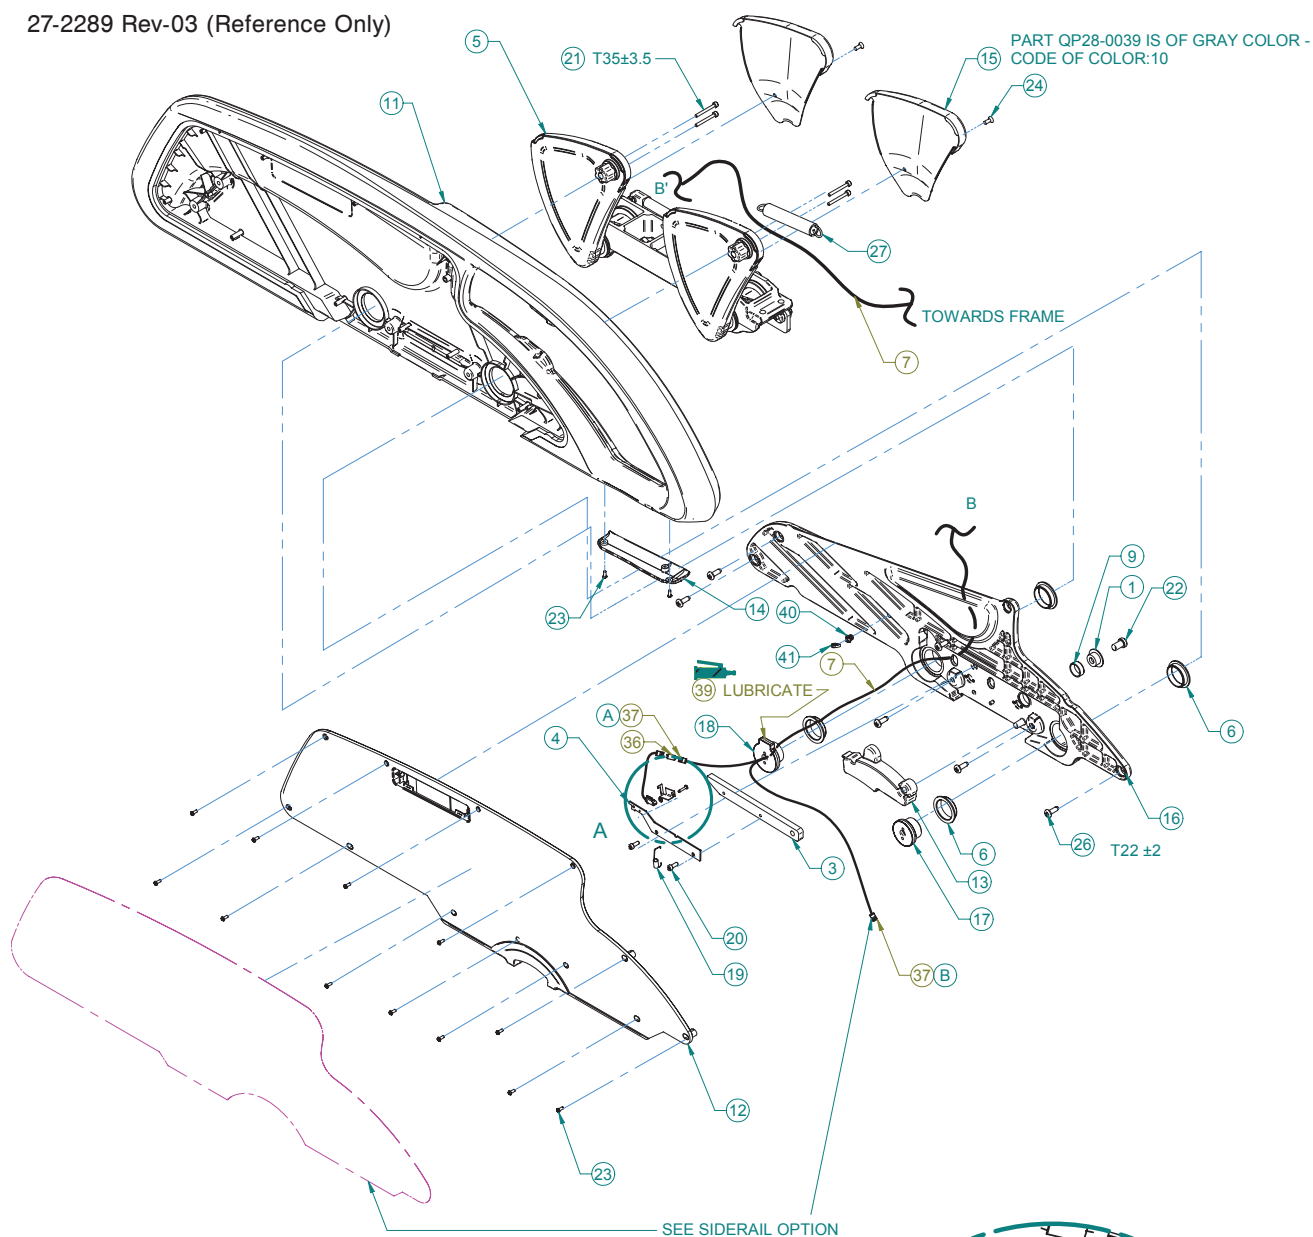

RACEWAY

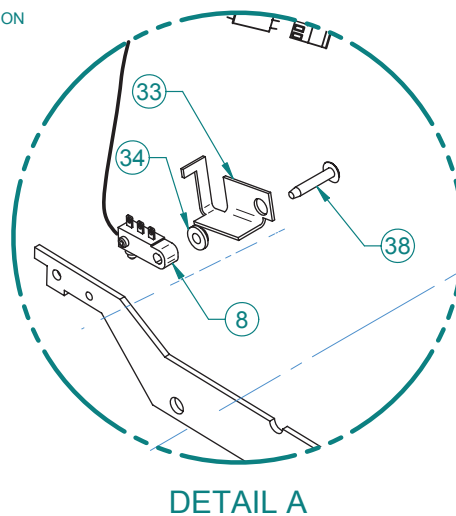

Standard Siderail Assembly, Foot End, Right

(Applies to beds with Serial Numbers U02818 - Current)

POSITION ON CONNECTOR			
Cable No.	Connector No.	Cable No.	Connector No.
QDF27-1521	MTA-100 3 Positions	QDF27-1208	MTA-100 3 Positions
QDF27-1208	MTA-100 3 Positions	QDF27-1521	MTA-100 3 Positions
QDF27-1208	Mate N Lock 3 Positions	QDF27-1481	J172 (L27-029)

POSITION ON CONNECTOR				
Cable QDF27-1208 ⑦	Signal	Color	Position on Connector ③⑦ A	Position on Connector ③⑦ B
1	NO SWITCH	White	1	-
2	COM SWITCH	Black	2	-
3	NC SWITCH	Green	3	-
4	LED1 LBS	Orange	-	1
5	+12V	Red	-	3
6	LED2 LBS	Blue	-	2

Note 1:

Siderail **without iBed** option - See OL270059-XXX ([page 283](#)).

Siderail **with iBed** option - See OL270060-XXX ([page 284](#)).

Standard Siderail Assembly, Foot End, Right



(Applies to beds with Serial Numbers U02818 - Current)

Standard Siderail Assembly, Foot End, Right - 27-2289 Rev-03 (Reference Only)

Item	Part No.	Part Name	Qty.
1	QPA28-0493	Siderail Sleeve	1
3	QDF27-2574Z	Siderail Lock	1
4	27-2575Z	Switch Support	1
5	27-2060	S.A. Siderail Mechanism	1
6	QDF2049	Shoulder Spacing	4
7	QDF27-1208	Foot Siderail Limit Switch Cable	1
8	QDF27-1521	S.A. Siderail Switch	1
9	28-0491	Machined Spacer QDF9191	1
11	QP27-1263	Right Foot Siderail	1
12	QP27-1267	Right Foot Siderail Cover	1
13	QP27-1274	Left Siderail Handle	1
14	QP27-1508	Right Foot Siderail Cap	1
15	QP28-0039	Siderail Rotation Arm Cover	2
16	QPA27-2297	Right Foot Siderail Structure	1
17	QPA28-0015	Siderail Sleeve	1
18	QPA28-0016	Sleeve with Lock	1
19	QRE27-1736	Return Spring	1
20	VV10A0G16-S	Hexagon Cylindric Head Screw	2
21	VV10B0G40-S	Hexagon Cylindric Head Screw	4
22	VV10A1P20-S	Hexagon Cylindric Head Screw	1
23	VV23A9C12HL	Phillips Pan Head Screw	15
24	VV31A0G16	Phillips Flat Head Screw	2
26	VVB3A9N24PF	Bosscrew Screw	6
27	QRE28-0293	Siderail Tension Spring,	1
33	27-2293Z	Switch Guide 1	1
34	27-1839	Shoulder Washer	1
36	QDF2080	Inline Splice	1
37	QDF2099	Female Connector MTA-100	1
		3 Positions	2
38	VV87A9A20	Phillips Truss Head Tapping Screw	1
39	M0019	Grease	1
40	QDF5096	Plastic Tie Support	1
41	QDF9518	Cable Tie	1

(Applies to beds with Serial Numbers U01001 - U02817)

27-0390 Rev-19 (Reference Only)

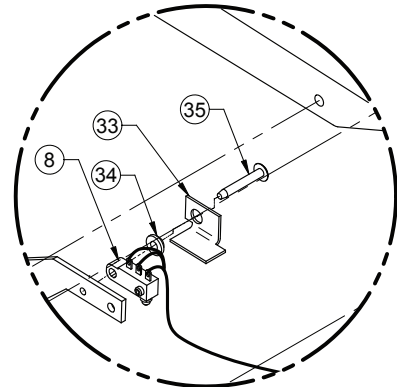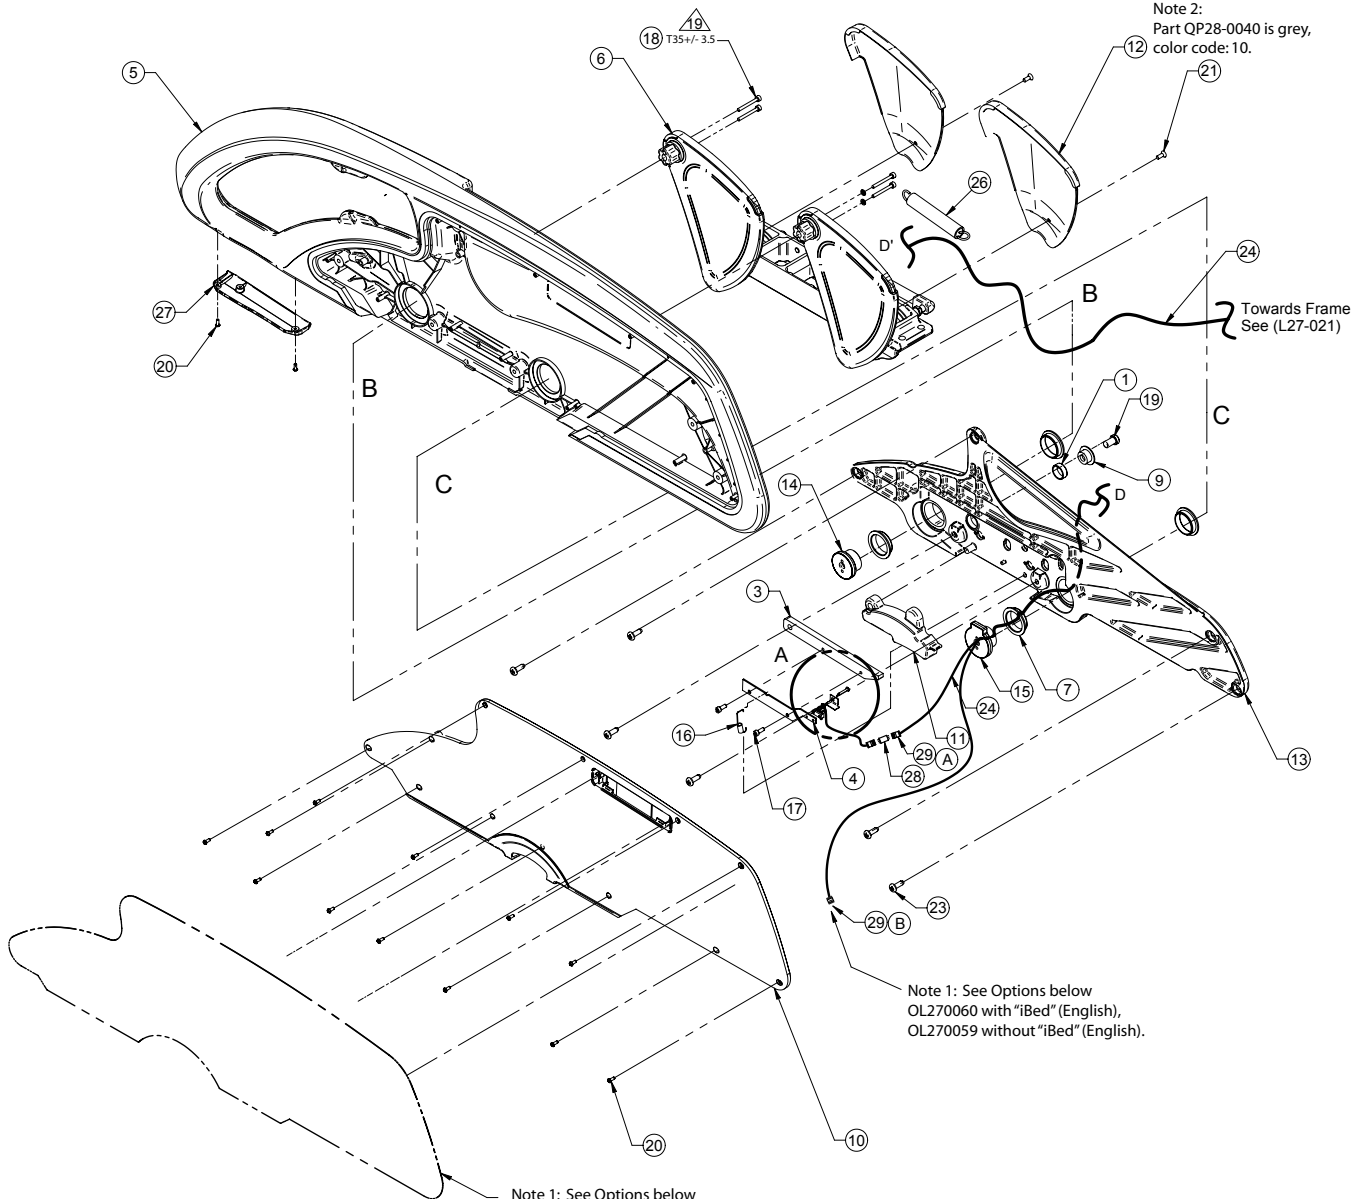

DETAIL A

Standard Siderail Assembly, Foot End, Left

(Applies to beds with Serial Numbers U01001 - U02817)

POSITION ON CONNECTOR			
Cable No.	Connector No.	Cable No.	Connector No.
QDF27-1521	MTA-100 3 Positions	QDF27-1208	MTA-100 3 Positions
QDF27-1208	MTA-100 3 Positions	QDF27-1521	MTA-100 3 Positions
QDF27-1208	Mate N Lock 3 Positions	QDF27-2213	J171 (L27-037)

POSITION ON CONNECTOR				
Cable QDF27-1208 (24)	Signal	Color	Position on Connector (29) (A)	Position on Connector (29) (B)
1	NO SWITCH	White	1	-
2	COM SWITCH	Black	2	-
3	NC SWITCH	Green	3	-
4	LED1 LBS	Orange	-	1
5	+12V	Red	-	2
6	LED2 LBS	Blue	-	3

Note 1:

Siderail **without iBed** option - See OL270059-XXX ([page 283](#)).

Siderail **with iBed** option - See OL270060-XXX ([page 284](#)).

Standard Siderail Assembly, Foot End, Left


(Applies to beds with Serial Numbers U01001 - U02817)

Standard Siderail Assembly, Foot End, Left - Common Components - 27-0390 Rev-19 (Reference only)


Item	Part No.	Part Name	Qty.
1	QDF28-0491	Machining Spacer	1
3	QDF27-1141Z	Siderail Lock	1
4	27-1142Z	Siderail Switch Support	1
5	QP27-1264-05	Left Foot Siderail	1
6	27-2061W	Inverted Siderail Mechanics	1
7	QDF2049	Spacer	4
8	QDF27-1521	Siderail Switch	1
9	QPA28-0493	Siderail Sleeve	1
10	QP27-1268-05	Left Foot Siderail Cover	1
11	QP27-1273-08	Right Siderail Handle	1
12	QP28-0040-10	Inverted Siderail Arm Cover	2
13	QPA27-1272	Left Foot Siderail Structure	1
14	QPA28-0015	Siderail Sleeve	1
15	QPA28-0016	Sleeve with Lock	1
16	QRE27-1736	Spring Balance	1
17	VV10A0G16-S	Hex Socket Head Screw	2
18	VV10A0G40-S	Hex Socket Head Screw	4
19	VV10A1P20-S	Hex Socket Head Screw	1
20	VV23A9C12HL	Hi-Lo Screw	15
21	VV31A0G16	Machine Screw	2
23	VVB3A9N24PF	Bosscrew Screw	6
24*	QDF27-1208	Foot Limit Switch Siderail Cable	1
25*	QDF7826	Tape	1
26	QRE28-0293	Siderail Tension Spring, K11	1
27	QP27-1509-05	Left Foot Siderail Cap	1
28*	QDF2080	Inline Splice (ITW MWTZ 100-3-D)	1
29*	QDF2099	Female Connector mta-100 3 Pos.	2
33	27-1739Z	Siderail Plate 2	1
34	27-1839	Side Ring	1
35	VW879A20	Tapping Screw	1

(Applies to beds with Serial Numbers U02818 - Current)

27-2290 Rev-03 (Reference Only)

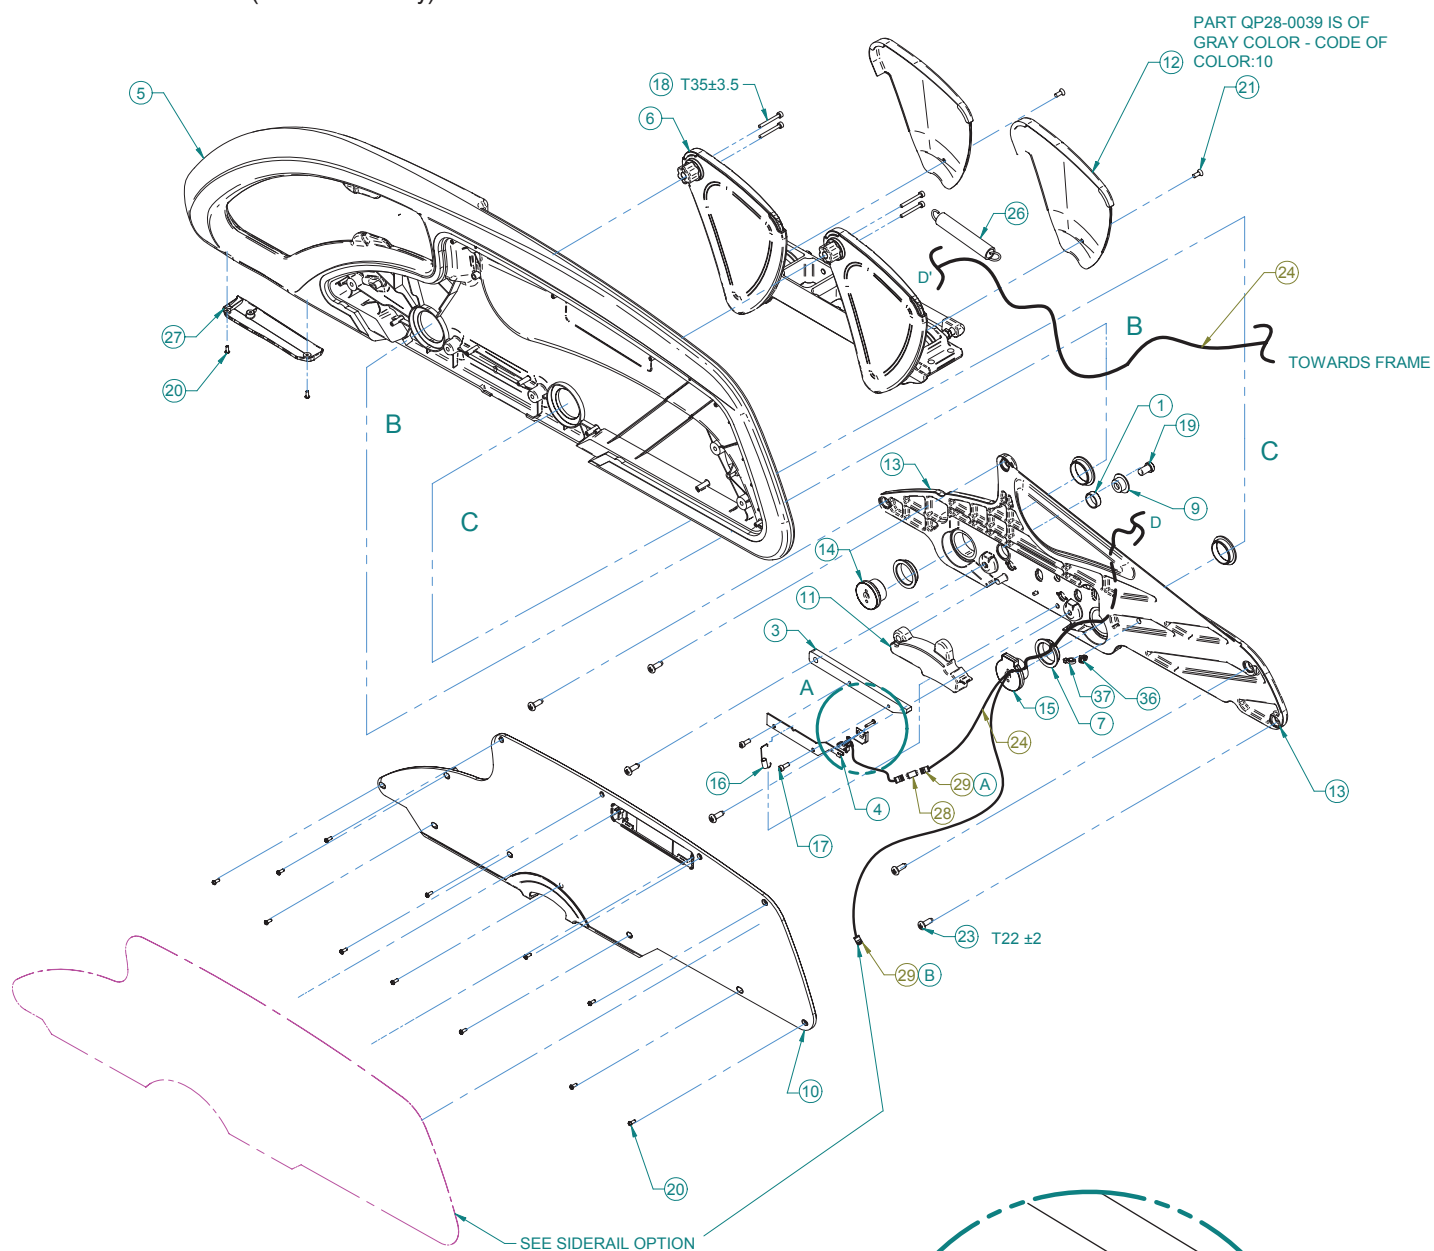

RACEWAY

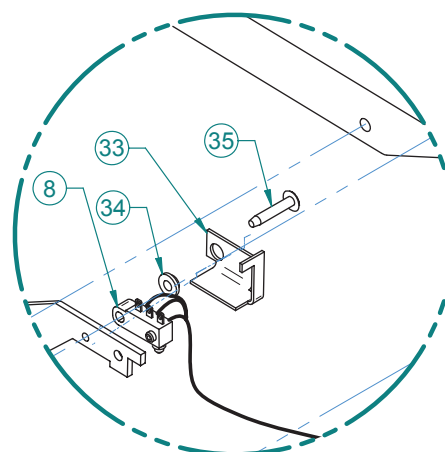

DETAIL A

Standard Siderail Assembly, Foot End, Left

(Applies to beds with Serial Numbers U02818 - Current)

POSITION ON CONNECTOR			
Cable No.	Connector No.	Cable No.	Connector No.
QDF27-1521	MTA-100 3 Positions	QDF27-1208	MTA-100 3 Positions
QDF27-1208	MTA-100 3 Positions	QDF27-1521	MTA-100 3 Positions
QDF27-1208	Mate N Lock 3 Positions	QDF27-1481	J171 (L27-029)

POSITION ON CONNECTOR				
Cable QDF27-1208 (24)	Signal	Color	Position on Connector (29) (A)	Position on Connector (29) (B)
1	NO SWITCH	White	1	-
2	COM SWITCH	Black	2	-
3	NC SWITCH	Green	3	-
4	LED1 LBS	Orange	-	1
5	+12V	Red	-	3
6	LED2 LBS	Blue	-	2

Note 1:

Siderail **without iBed** option - See OL270059-XXX ([page 283](#)).

Siderail **with iBed** option - See OL270060-XXX ([page 284](#)).

Standard Siderail Assembly, Foot End, Left


(Applies to beds with Serial Numbers U02818 - Current)

Standard Siderail Assembly, Foot End, Left - 27-2290 Rev-03 (Reference Only)


Item	Part No.	Part Name	Qty.
1	QDF28-0491	Machined Spacer QDF9191	1
3	QDF27-2574Z	Siderail Lock	1
4	27-2575Z	Switch Support	1
5	QP27-1264	Left Foot Siderail	1
6	27-2061	S.A. Reversed Siderail Mechanism	1
7	QDF2049	Shoulder Spacer	4
8	QDF27-1521	S.A. Siderail Switch	1
9	QPA28-0493	Siderail Sleeve	1
10	QP27-1268	Left Foot Siderail Cover	1
11	QP27-1273	Right Siderail Handle	1
12	QP28-0040	Reversed Siderail Arm Cover	2
13	QPA27-2298	Foot Left Siderail Casting	1
14	QPA28-0015	Siderail Sleeve	1
15	QPA28-0016	Sleeve with Lock	1
16	QRE27-1736	Return Spring	1
17	VV10A0G16-S	Hexagon Cylindric Head Screw	2
18	VV10B0G40-S	Hexagon Cylindric Head Screw	4
19	VV10A1P20-S	Hexagon Cylindric Head Screw	1
20	VV23A9C12HL	Phillips Pan Head Screw	15
21	VV31A0G16	Phillips Flat Head Screw	2
23	VVB3A9N24PF	Bosscrew Screw	6
24	QDF27-1208	Foot Siderail Limit Switch Cable	1
26	QRE28-0293	Siderail Tension Spring, K11	1
27	QP27-1509-05	Left Foot Siderail Cap	1
28	QDF2080	Inline Splice	1
29	QDF2099	Female Connector MTA-100	
		3 Positions	2
33	27-2292Z	Switch Guide 2	1
34	27-1839	Shoulder Washer	1
35	VV87A9A20	Phillips Tapping Screw	1
36	QDF5096	Plastic Tie Support	1
37	QDF9518	Cable Tie	1

Standard Siderail Assembly without iBed

OL270059-XXX Rev-05 (Reference Only)

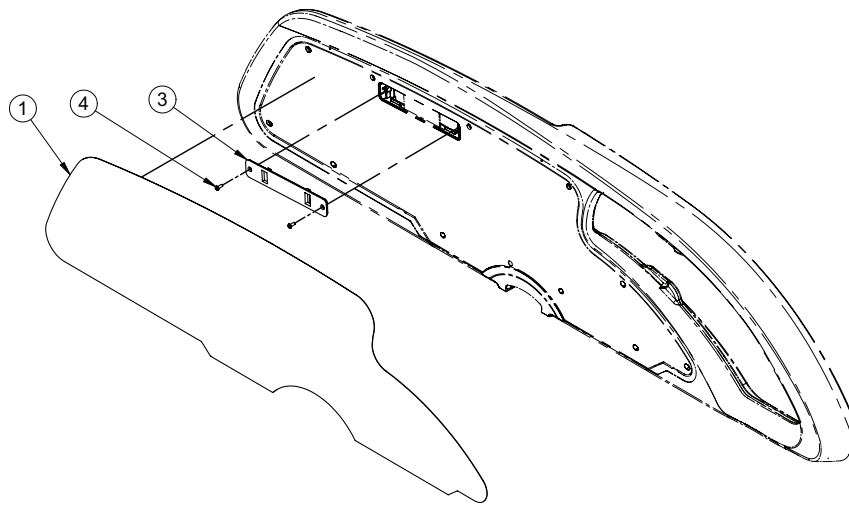

Right Siderail Shown

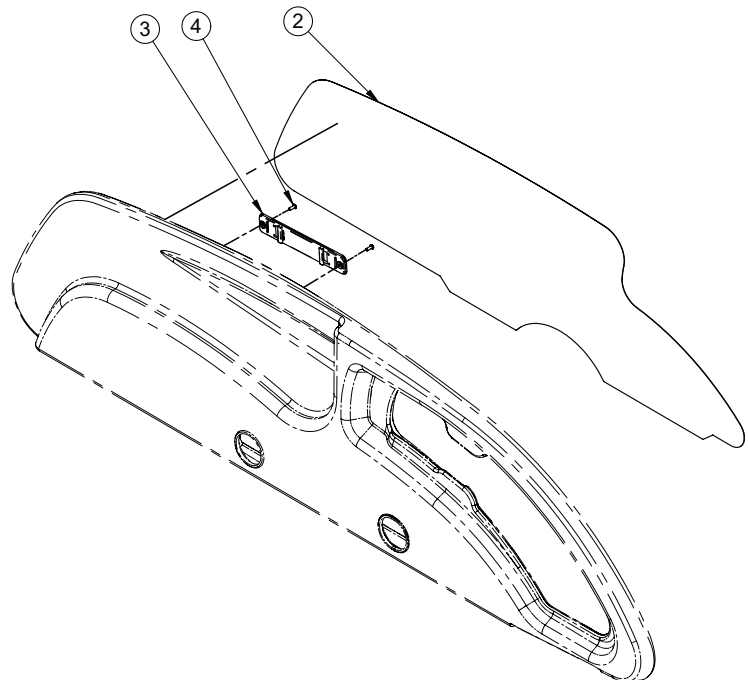

Left Siderail Shown


NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Item	Part No.	Part Name	Qty.
1	QDF27-0909-XXX	Right Foot Siderail Cover Fascia	1
2	QDF27-0910-XXX	Left Foot Siderail Cover Fascia	1
3	QP27-1831	LBS Lens Foot Siderail	2
4	VV23A9C12HL	Pan Head Tapping Screw	4

Optional Siderail Assembly with iBed

OL270060-XXX Rev-04 (Reference Only)

Left Siderail Shown

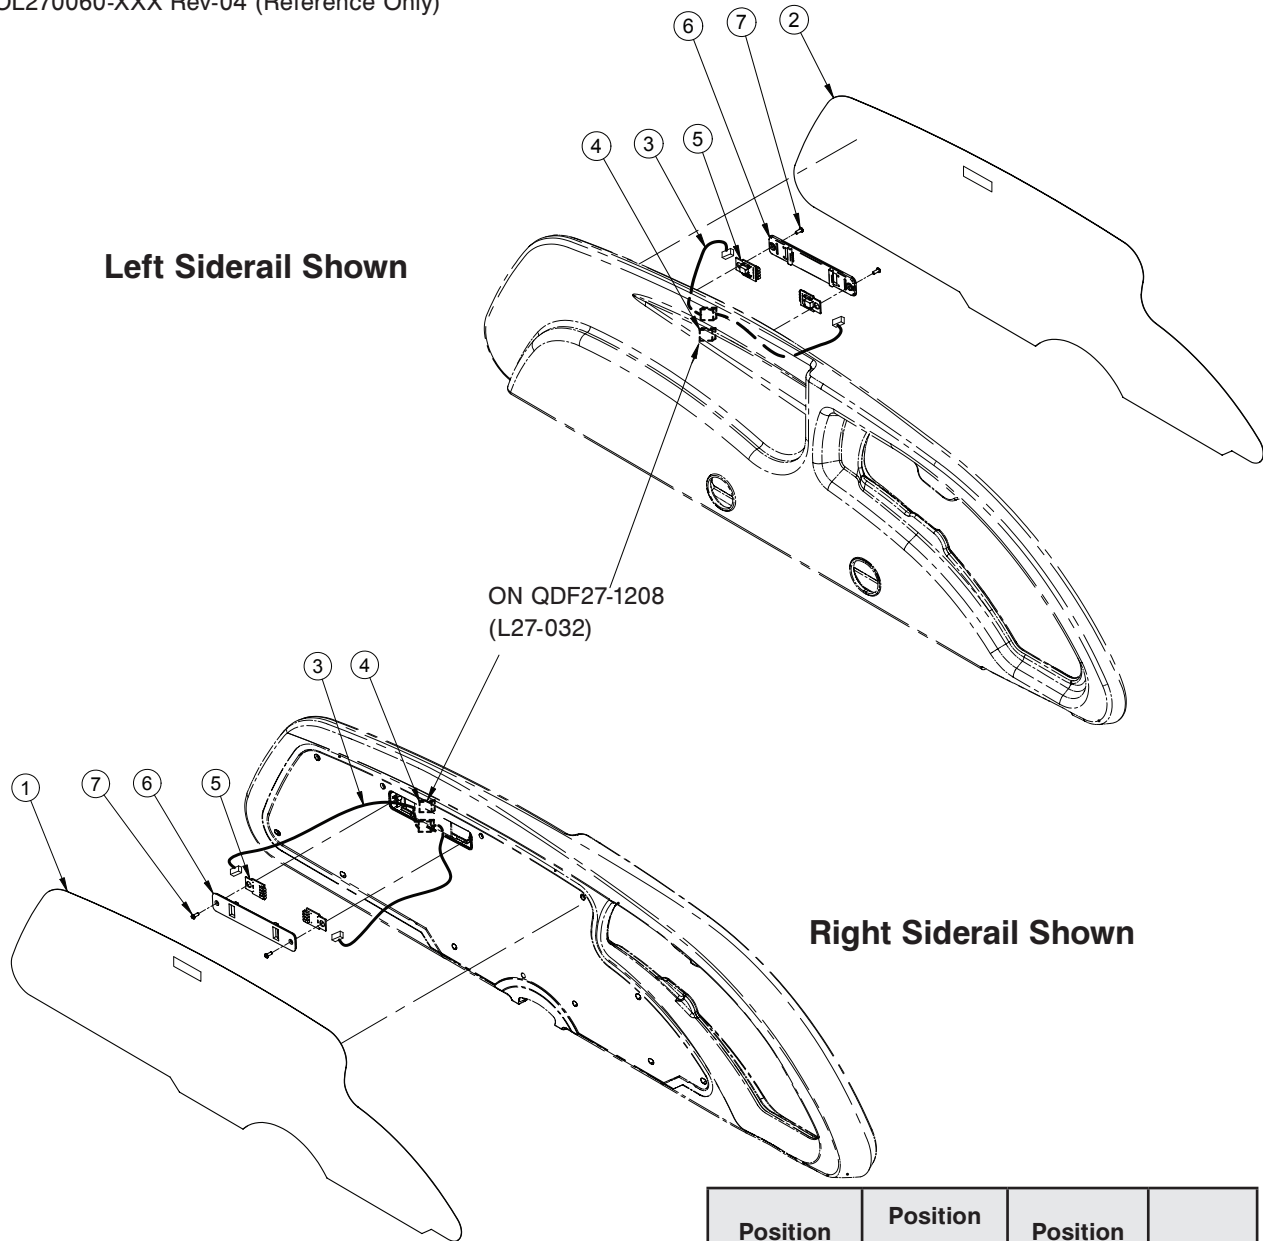


NOTE: XXX - indicates language choice
(tri = English/French/Spanish; bil = English/French)

Position on Wire 27-1834	Position on Connector 4	Position on Wire 27-1208	Signal
1	1	1	LED 1
2	2	2	LED 2
3	3	3	+12V

Item	Part No.	Part Name	Qty.
1	QDF27-2030-XXX	Right Foot Siderail Fascia with iBed	1
2	QDF27-2031-XXX	Left Foot Siderail Fascia with iBed	1
3	QDF27-1834	LBS Cable Foot Siderail	2
4	QDF2080	Inline Splice	2
5	QDF27-1562	iBED Electronic Board Lens	4
6	QP27-1831	LBS Foot Siderail Lens	2
7	VV23A9C12HL	Pan Head Tapping Screw	4

Headboard and Footboard Assembly


L27-028 Rev E (Reference Only)

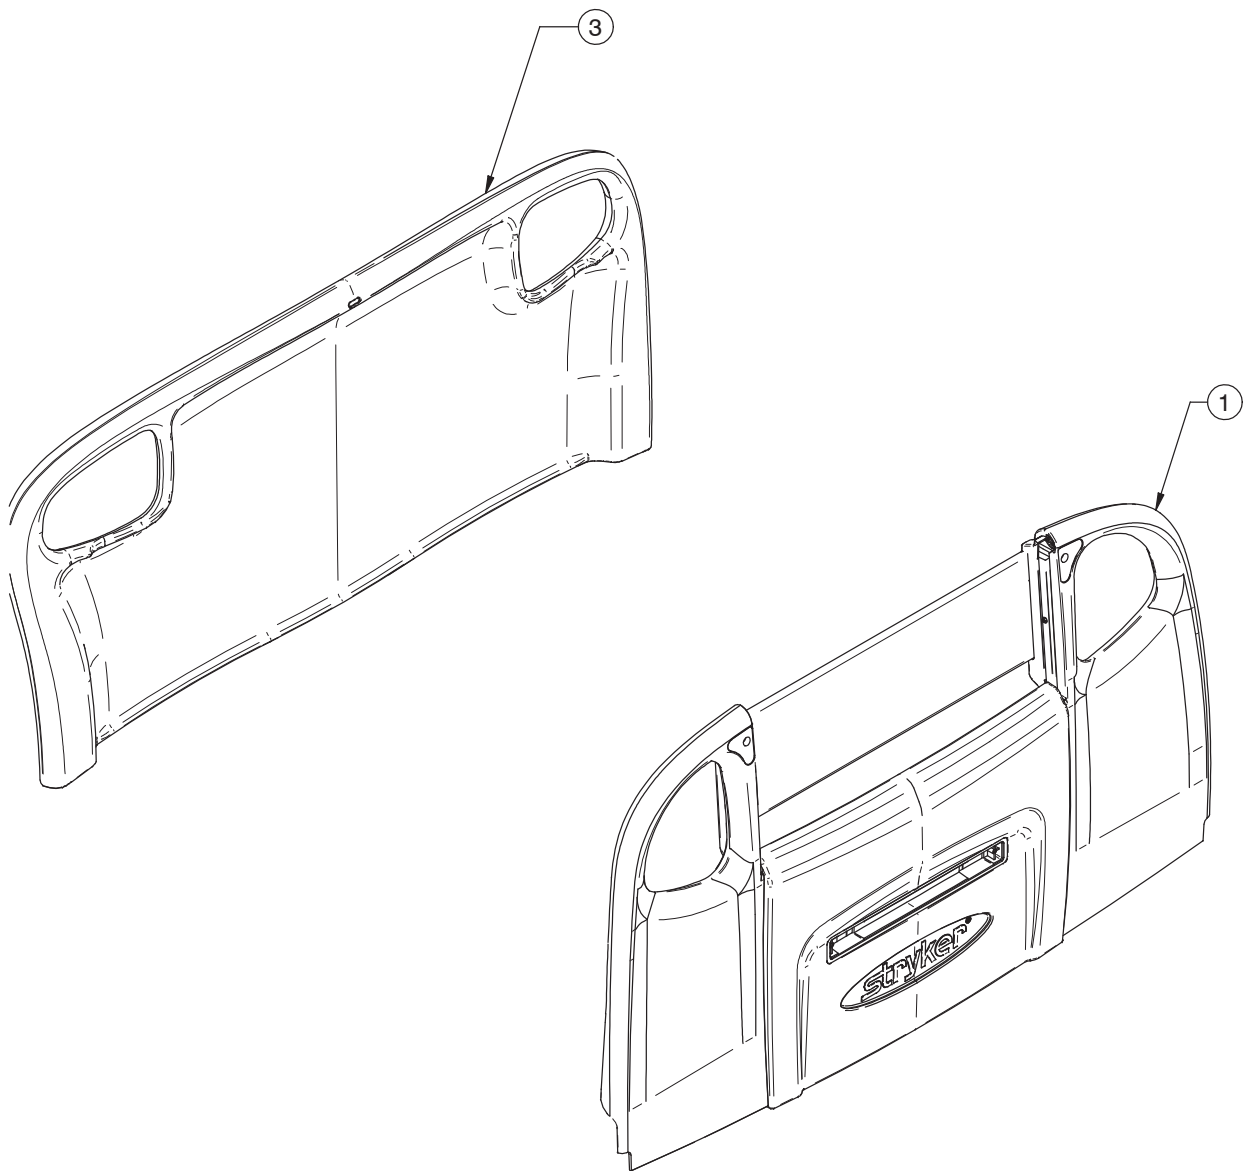

Item	Part No.	Part Name	Qty.
1	27-1547	Footboard Assembly	1
3	QP27-1077	Head Panel	1

Standard Footboard Assembly

27-1547 Rev P (Reference Only)

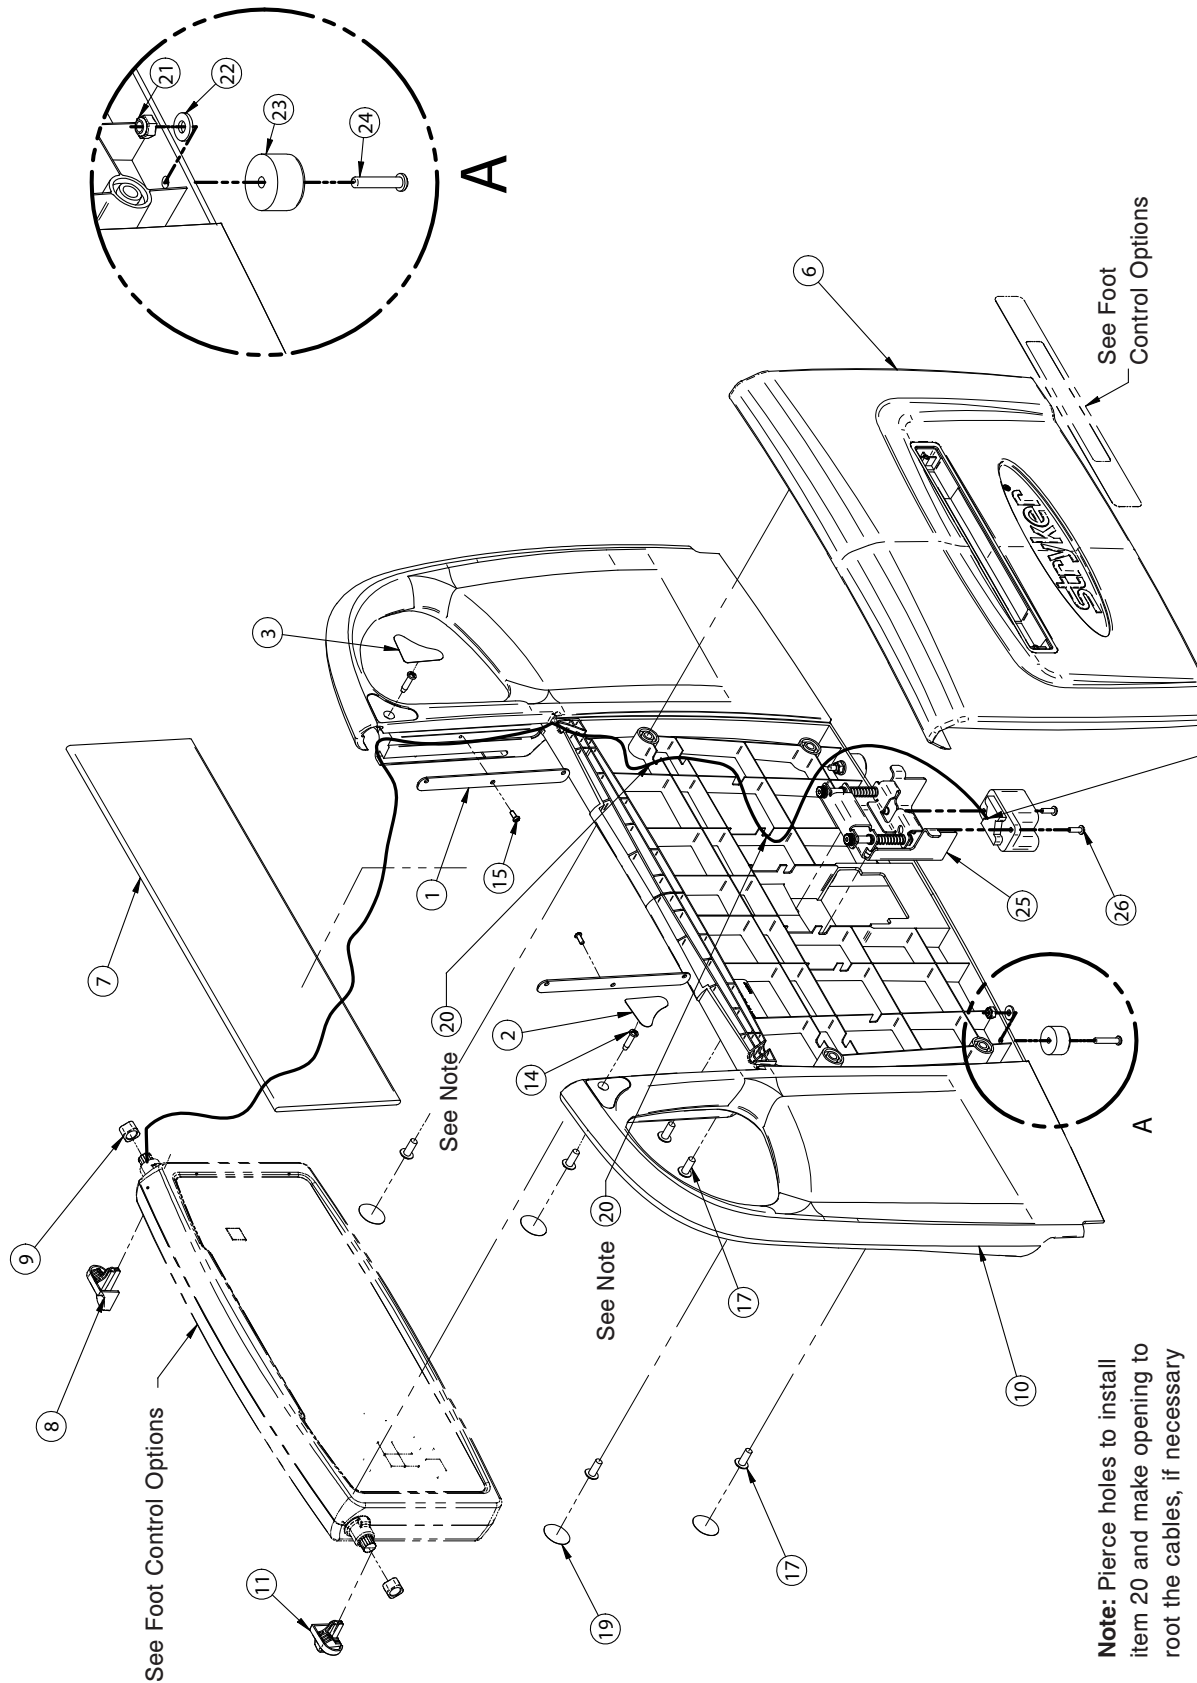

Standard Footboard Assembly

Footboard Assembly - 27-1547 Rev P (Reference Only)



Item	Part No.	Part Name	Qty.
1	27-2274P	Board Wire Cover	2
2	QDF27-1601	Footboard Screw Cover Sticker, Right	1
3	QDF27-1602	Footboard Screw Cover Sticker, Left	1
6	QP27-1026	Footboard Cover	1
7	QP27-1359	Foot Support	1
8	QP27-1493	Right Foot Control Support	1
9	QP27-1511	Foot Control Pivot Bushing	2
10	27-2785	Main Footboard	1
11	QP27-1569	Left Foot Control Support	1
14	VV23A1G24HL	Phillips Screw	2
15	VV23A9C12HL	Pan Head Tapping Screw	2
17	VV37A1N20-S	Truss Head Machine Screw	4
19	QDF21-3943	Screw Cover	4
20	QDF9518	Cable Tie	2
21	VE30A1G	Nylon Hex Locknut	2
22	VW10A06	Flat Washer	2
23	0056-028-000	Black TPR Bumper	2
24	VV33A1G32	Pan Head Machine Screw	2
25	27-2770	Spring Load Connector	1
26	VV33A1E16	Pan Head Machine Screw	2

OL270268-XXX Rev B (Reference Only)



Footboard Assembly with iBed and Wi-Fi


NOTE 1: PAY ATTENTION NOT TO WEDGE WIRE LBS BY CLOSING THE PANEL

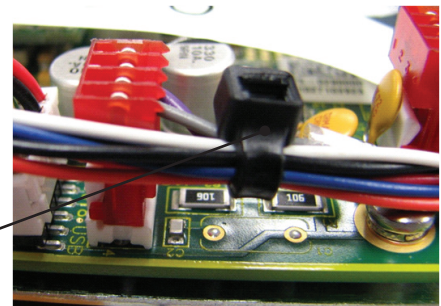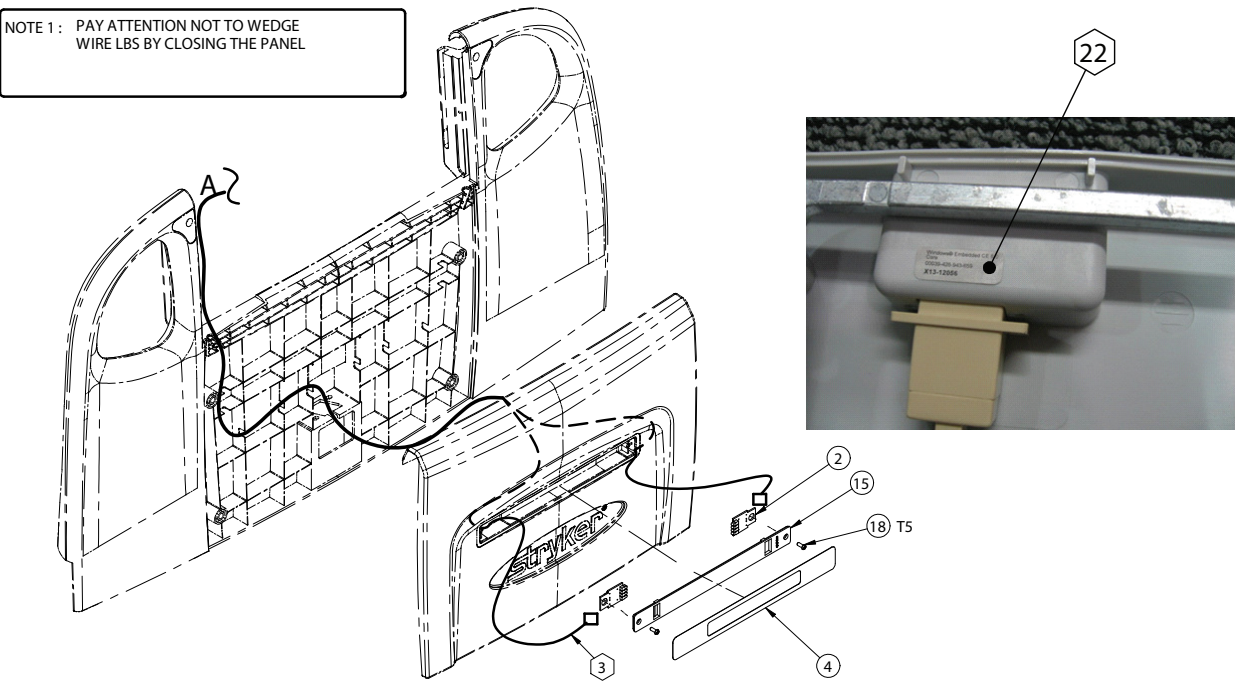

CONNECTION OF THE TOUCHSCREEN ON J3 BOARD

QDF75-0290 BOARD ASSEMBLY

POSITION THE SCREEN TO HAVE THE YELLOW CABLES UPWARD

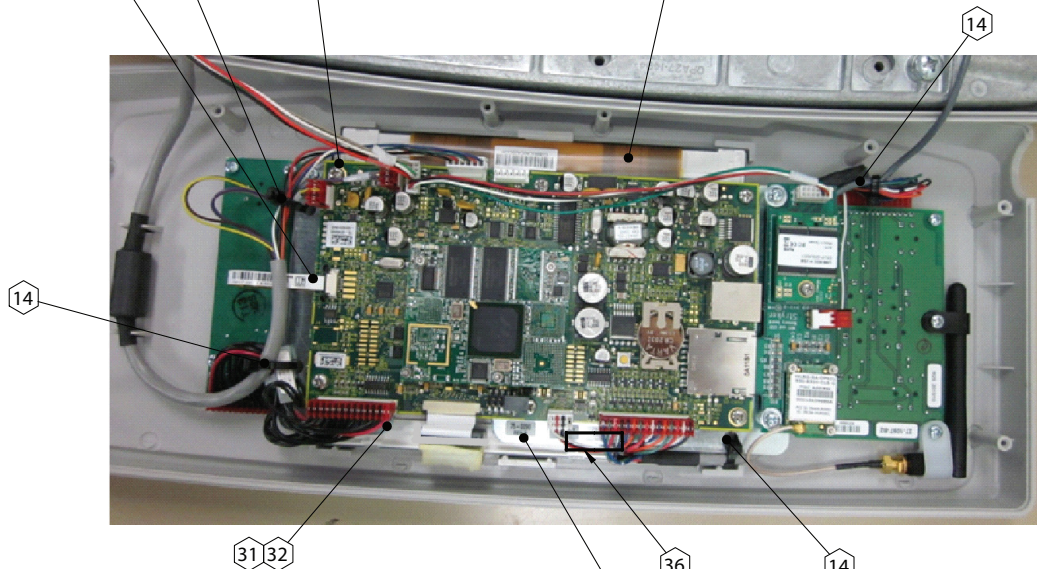

BOARD ORIENTED TO HAVE THE WRITING ON THE RIGHT SIDE VISIBLE

[Return To Table of Contents](#)

Footboard Assembly with iBed and Wi-Fi

CABLE CONNECTION TABLE				
Cable No.	Connector No.	To	Cable No.	Connector No.
QDF27-2253	Connector MTA	To	QDF27-1562	Left Side
QDF27-2253	Connector MTA	To	QDF27-1562	Right Side
QDF27-2253	Connector MTA 4 Positions	To	QDF75-0290	J9 (Interface Board)
QDF27-2594	Connector MTA 15 Positions	To	QDF75-0290	J12 (Interface Board)
QDF27-2594	Connector MTA 15 Positions	To	QDF27-1097	J1 (Brake Board)
QDF27-2594	Connector MTA 3 Positions	To	QDF75-0630	J5 (USB WI-FI Board)
QDF27-2230	Connector MTA 13 Positions	To	QDF75-0290	J6 (Interface Board)
QDF27-2230	Connector MTA 13 Positions	To	QDF75-0010	J1 (Menu Board)
QDF27-2232	Connector Metrimate 19 Pos.	To	QDF27-1213	Con. Metrimate (27-1661)
QDF27-2232	Connector MTA 4 Positions J1	To	QDF75-0290	J1 (Brake Board)
QDF27-2232	Connector MTA 4 Positions J19	To	QDF75-0290	J19 (Interface Board)
QDF27-2232	Connector MTA 6 Positions	To	QDF75-0290	J17 (Interface Board)
QDF27-2193	Touch Screen	To	QDF75-0290	J3 (Interface Board)
QDF27-2741	PCB Flex	To	QDF75-0290	J7 (Interface Board)
QDF27-2573	Connector 12 Positions	To	QDF75-0290	J18 (Touch Board)
QDF27-2573	Connector 12 Positions	To	QDF75-0630	J4 (USB WI-FI Board)

NOTE: XXX - indicates language choice (tri = English/French/Spanish; bil = English/French)

Footboard Assembly with iBed and Wi-Fi - OL270268-XXX Rev B (Reference Only)


Item	Part No.	Part Name	Qty.	Item	Part No.	Part Name	Qty.
1	QDF27-1097	Brake Control Board	1	19	VV23A9C20HL	Pan Head Tapping Screw	10
2	QDF27-1562	Local Bed Status Board	2	20	VVB3A9N24PF	Bosscrew Screw	4
3	QDF27-2253	LBS Cable Foot Panel	1	21	27-2757	LCD Screen	1
4	QDF27-1610	iBed Lens Label	1	22	QDF27-2279	Windows License CE Label	1
5	QDF27-2756	Back Foot Control Fascia	1	23*	QDF2053	Red Electric Tape	1
6	QDF27-2188-XXX	Foot Control Overlay	1	24*	75-0434	Software InTouch 3.0 Board	1
7	QDF27-2193	8" Touch Screen	1	25	QDF2157	Collar Spacer	2
8*	QDF27-2594	Brake to Interface Cable	1	26	QDF75-0630	USB WI-FI Board	1
9*	QDF27-2230	Menu to Interface Cable	1	27	VV33A0A16	Pan Head Machine Screw	2
10*	QDF27-2232	Foot Panel Cable	1	28	VE39A0A	Nylon Hex Locknut	2
11	QDF75-0290	Touch Board Assembly	1	29	QDF9520	Wire Clip	1
12	QDF75-0010	Main Menu Board	1	30	QDF27-2573	Interface Board	
13	QDF9183	Control Board Button	9			"Y" USB Cable	1
14*	QDF9518	Cable Tie	5	34	27-2682Z	Shim	2
15	QP27-1609	iBed Lens	1	35	QP27-2185	Nurse Control Panel,	
16	QP27-2186	Rear Footboard Control	1			Foot End	1
17	QPA27-1494	Foot Control Frame	1	36	QE71-1362-E	InTouch 3.0 Software Label	1
18	VV23A9C12HL	Pan Head Tapping Screw	14	37	QDF1054	Wire Clip	1
				38	27-2698	Protection Tape	1

Optional Bed Accessories

Accessory	Part Number	Page Reference
Bed Extender	FA64234-XXX	See page 292
Bed Extender Mattress (2920 PositionPRO only)	DM64196	See page 293
Bed Extender Mattress (2950 XPRT™ only)	DM64197	See page 293
Line Management System	FA64210-XXX	See page 294
I.V. Pole, Permanent - Left	FA64221-XXX	See page 295
I.V. Pole, Permanent - Right	FA64238-XXX	See page 295
I.V. Pole, Dual Head End Permanently Attached	FA64202-XXX	See page 296
Monitor Tray	FA64214-XXX	See page 298
Oxygen Bottle Holder, Upright	FA64187-XXX	See page 299
Oxygen Bottle Holder, Right Fit	FA64203	See page 300
Pendant with Motion Control Only	FA64228-XXX	See page 301
Pendant with Motion Control & Nurse Call	FA64226	See page 302
Pendant with Motion Control & Smart TV	FA64227	See page 303
Pendant with Motion Control, Nurse Call & Smart TV	FA64225	See page 304
Pendant Clip	FA64186-XXX	See page 304
Roller Bumpers	OL270050	See page 305
Traction Sleeve 4" x 1/2"	FA64215-XXX	See page 306
Traction Sleeve 4" x 3/4"	FA64216-XXX	See page 307
Traction Sleeve 8" x 1/2"	FA64217-XXX	See page 308
Traction Sleeve 8" x 3/4"	FA64218-XXX	See page 309
Traction Sleeve 6-1/2" x 3/4"	FA64219-XXX	See page 310
Wall Saver Cable	FA64208	See page 311
X-Ray Cassette Holder	FA64205-XXX	See page 312
Standard Mattress Retainer	OL270223	See page 314
Tube Support	OL270224-XXX	See page 315


Bed Extender - FA64234-XXX

L64-150-XXX Rev A (Reference Only)

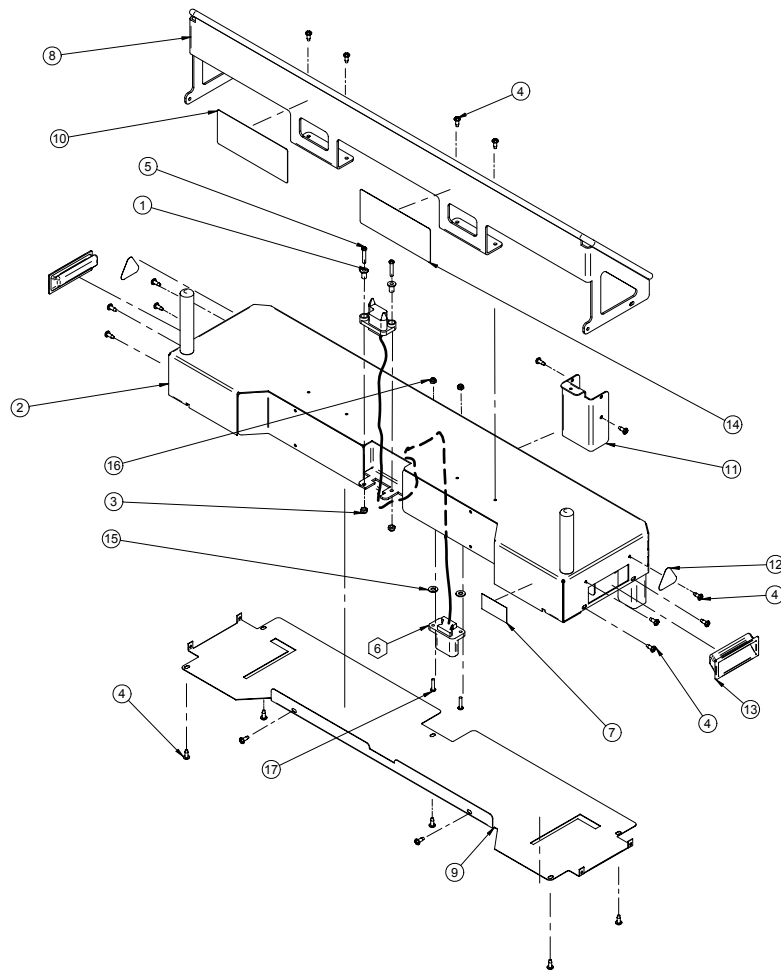


Item	Part No.	Part Name	Qty.
1	25-0527Z	Connector Sleeve	2
2	64-1158W	Bed Extender	1
3	VE30A0G	Nylon Locknut	2
4	VV83A9G16	Phillips Head Tapping Screw	21
5	VV31A0G32	Phillips Head Machine Screw	2
6	QDF64-1358	Bed Extender Cable	1
7	QE14399-T	Manufacturer Nameplate	1
8	64-1271W	Bed Extender Protective Device	1
9	64-1278W	Bed Extender Cover	1
10	QE71-1112-XXX	Bed Extender Warning Label	1
11	64-1284W	Bed Extender Connector	1
12	QE71-0533	Protective Top Sticker	2
13	QDF6029	ABS Plastic Snap-in Flush Mount	2
14	QE71-1132-XXX	Appropriate Cushion Label	1
15	VW10C081802	Nylon Washer	2
16	VE30A1E	Nylon Hex Locknut	2
17	VV33A1E24	Phillips Pan Machine Screw	2

Bed Extender Pad with Position Pro Mattress - DM64196

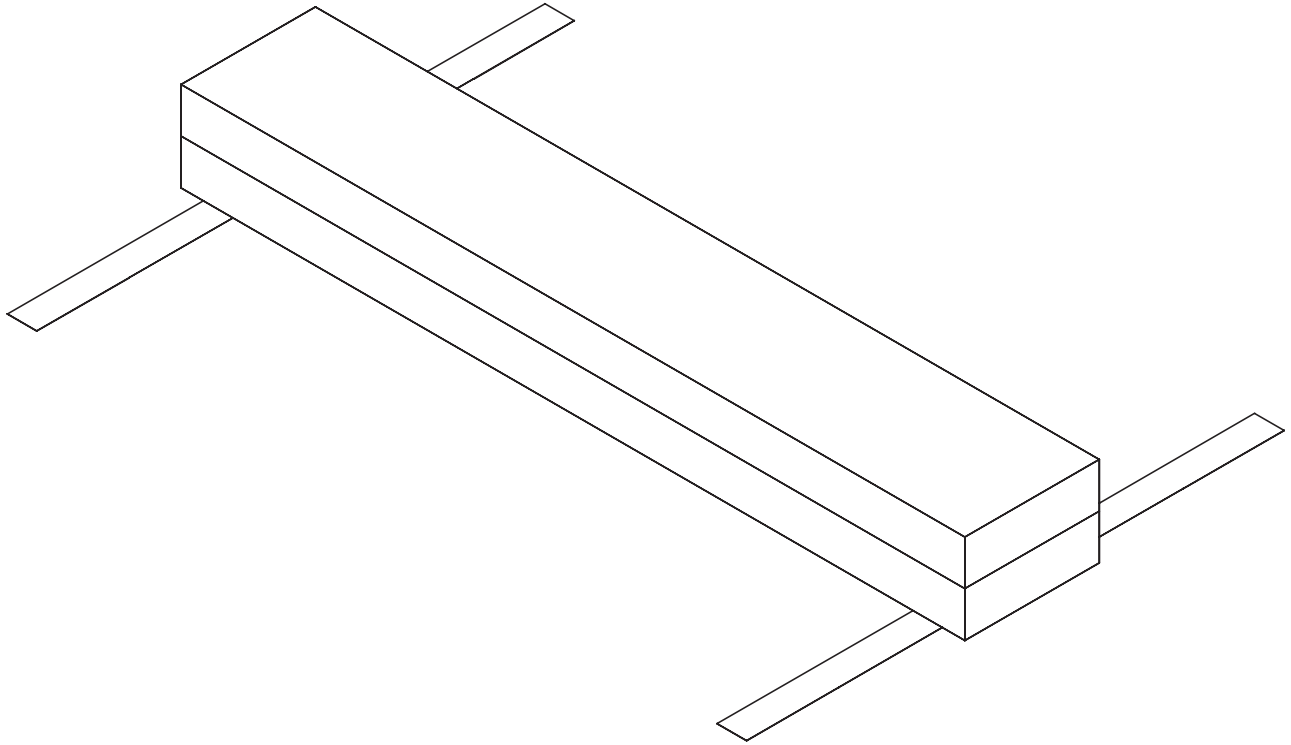


Bed Extender Pad with XPRT™ Mattress - DM64197

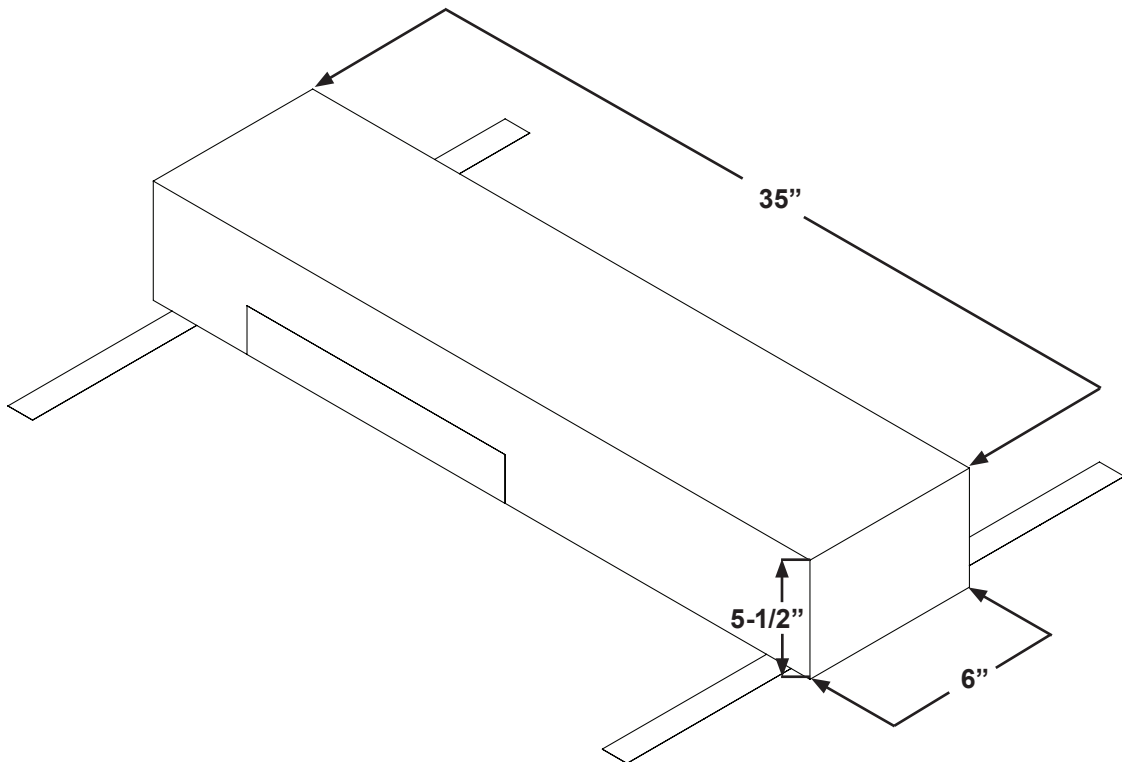


Line Management System Assembly - FA64210-XXX

L64-130-XXX Rev A (Reference Only)

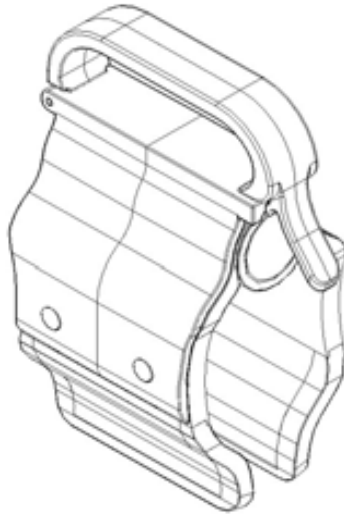


I.V. Pole Assembly, Permanent - FA64221-XXX/FA64238-XXX

L64-139-XXX Rev A (Reference Only)

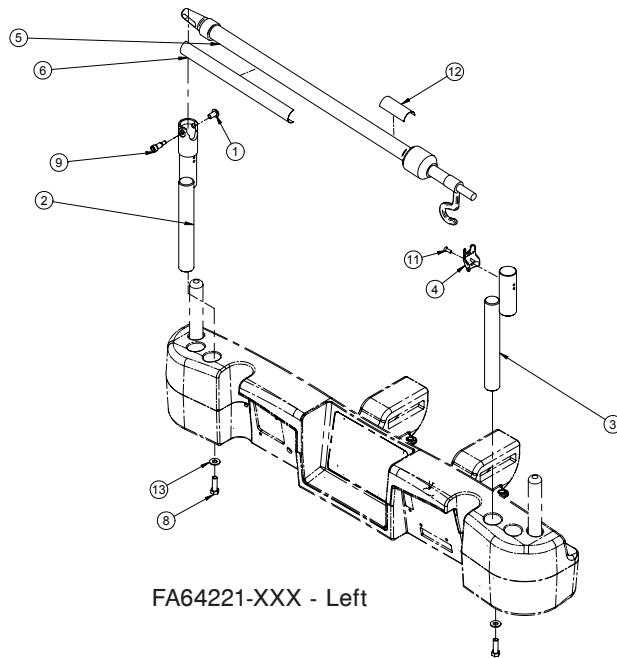

L64-153-XXX Rev A (Reference Only)

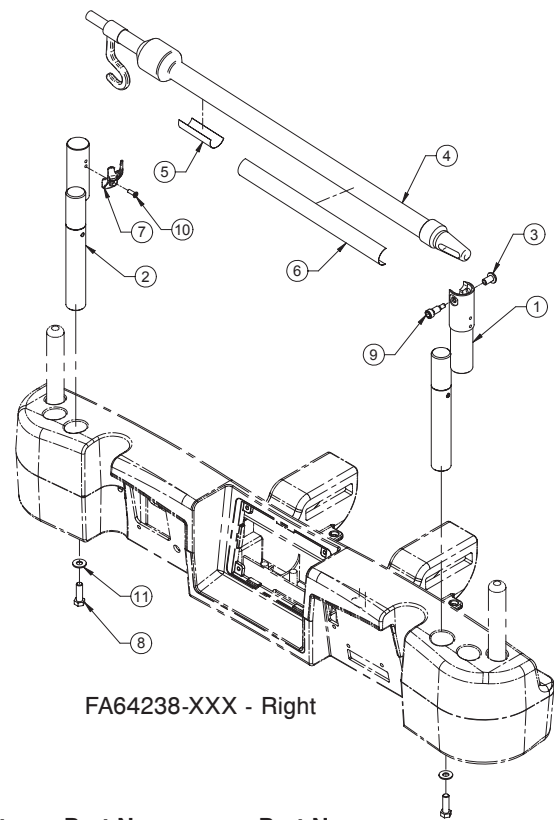


Item	Part No.	Part Name	Qty.	Item	Part No.	Part Name	Qty.
1	QDF2121	Barrel Nut	1	1	QDF64-1366	Ass. Right Support IV Pole	1
2	QDF64-1362	I.V. Pole Assembly, Left	1	2	QDF64-1367	Ass. Left Simple Stop IV Pole	1
3	QDF64-1365	I.V. Pole Assembly, Single	1	3	QDF2121	Fillets Mantle	1
4	QP64-1225-10	I,V, Pole Plastics Support	1	4	QDF5073	2 Stage IV Pole	1
5	QDF5073	2-Stage I.V. Pole	1	5	QE14399-T	Label, Manufacturing	1
6	QE71-1306-XXX	Label, "Warning"	1	6	QE71-1306-XXX	Label, "Warning"	1
8	VB15A1O32-S	Hex Bolt	2	7	QP64-1225-10	Plastic Support for IV Pole	1
9	VD60A1N1016-S	Bolt	1	8	VB15A1O32-S	Bolt 5/16x1 Gr.5 Scotch Grip	2
11	VV81A9E16-10	Tapping Screw	1	9	VD60A1N1016-S	Screw	1
12	QE14399-T	Manufacturer's Nameplate	1	10	VV81A9E16-10	Tapping Screw - Flathead	1
13	VW10A10	Flat Washer	2	11	VW10A10	Flat Washer	2

[Return To Table of Contents](#)

I.V. Pole Ass'y, Dual Head End, Permanent - FA64202-XXX

L64-107-XXX Rev A (Reference Only)

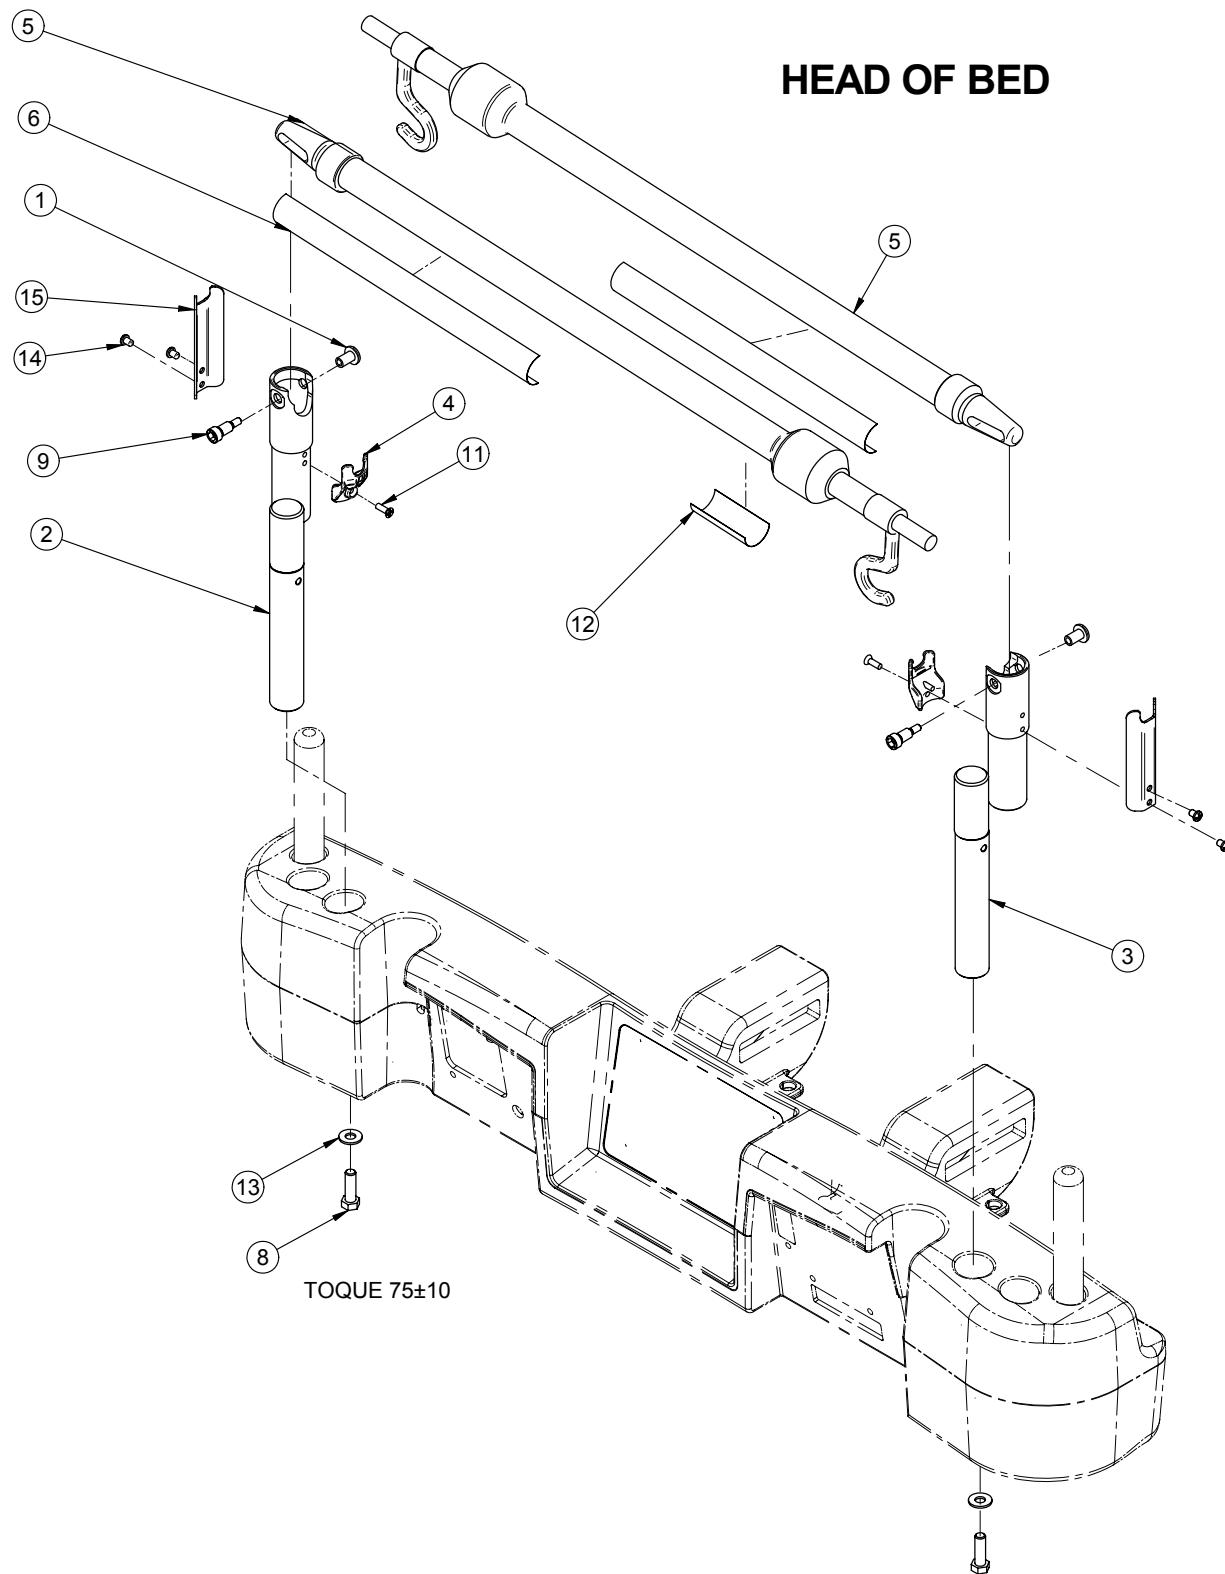


I.V. Pole Ass'y, Dual Head End, Permanent (Continued) - FA64202-XXX

I.V. Pole Assembly, Dual Head End, Permanent - L64-107-XXX Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	QDF2121	Tapped Sleeve	2
2	QDF64-1362	Left I.V. Pole Support	1
3	QDF64-1366	Right I.V. Pole Support	1
4	QP64-1225-10	I.V. Pole Plastic Support	2
5	QDF5073	2-Stage I.V. Pole	2
6	QE71-1306-XXX	Warning Sticker	2
8	VB15A1O32-S	Bolt	2
9	VD60A1N1016-S	Shoulder Bolt	2
11	VV81A9E16-10	Phillips Head Tapping Screw	2
12	QE14399-T	Manufacturer Sticker	1
13	VW10A10	Flat Washer	2
14	VV33A1G08-S	Phillips Head Tapping Screw	4
15	64-1269C	Double I.V. Pole Support	2


Monitor Tray Assembly - FA64214-XXX

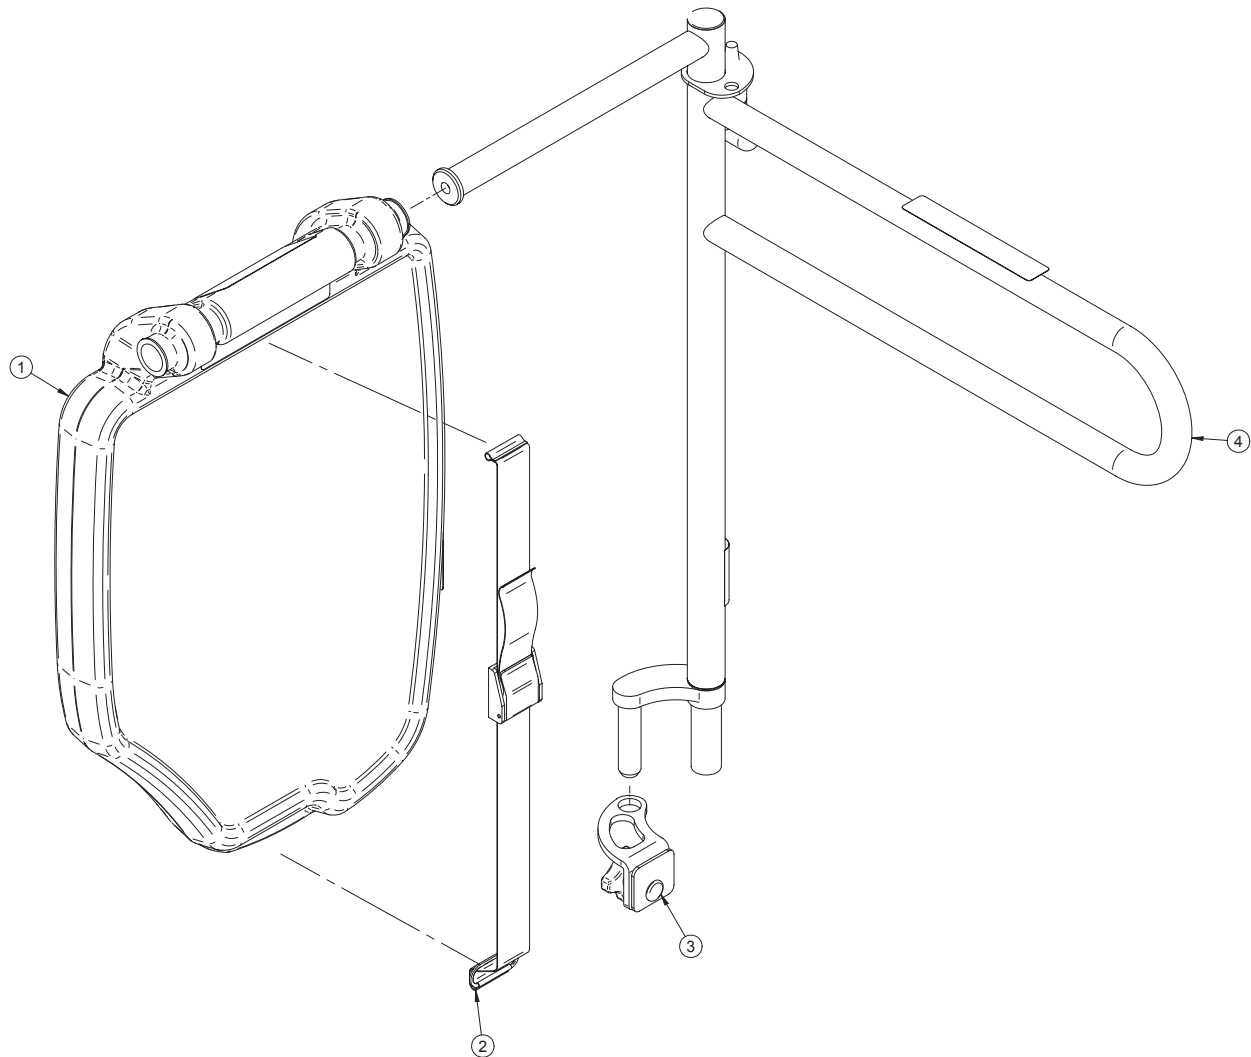

Item	Part No.	Part Name	Qty.
1	QDF64-1300	Tray	1
2	QDF64-1301	Transport Strap	1
3	QDF64-1302	Fastener Sleeve	1
4	QDF64-1303T	Tray Support Pole	1

Upright Oxygen Bottle Holder Assembly - FA64187-XXX


L64-112-XXX Rev A (Reference Only)

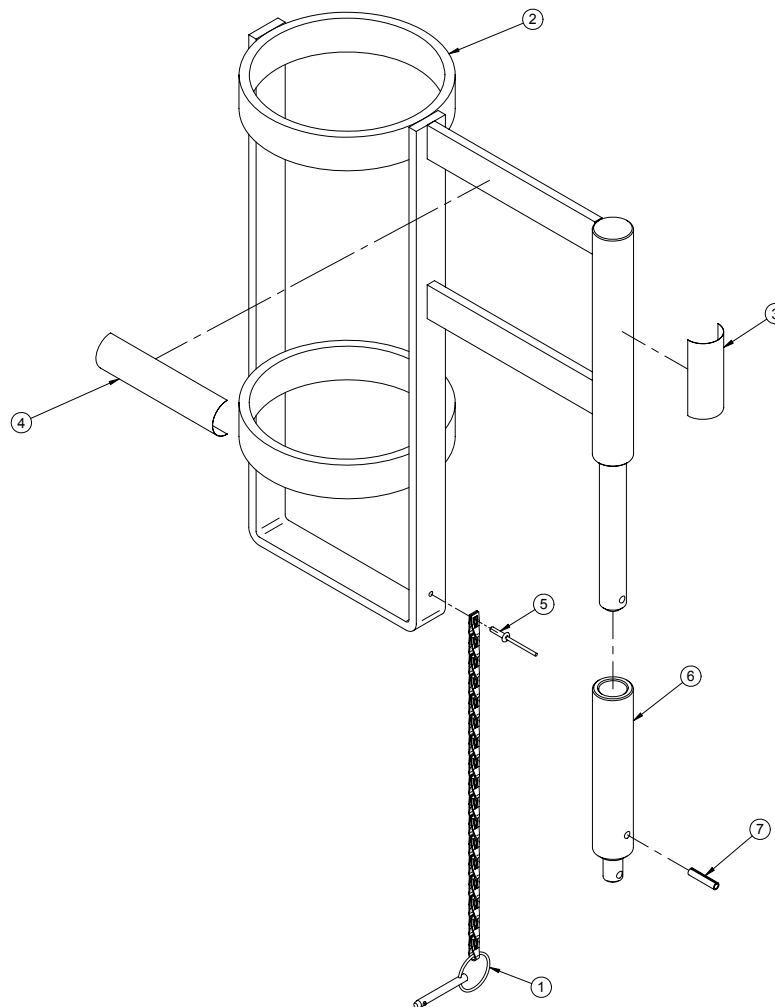

Item	Part No.	Part Name	Qty.
1	64-0647	Security Chain	1
2	QDF64-1059	Bottle Holder	1
3	QE14399-T	Manufacturer Sticker	1
4	QE71-0601	Maximum Load Sticker	1
5	VR11H46	POP Rivet, Dome Head	1
6	64-1285	Oxygen Bottle Holder Socket	1
7	VG10B0628	Spring Pin	1


Right-Fit Oxygen Bottle Holder Assembly - FA64203

L64-124 Rev-00 (Reference Only)

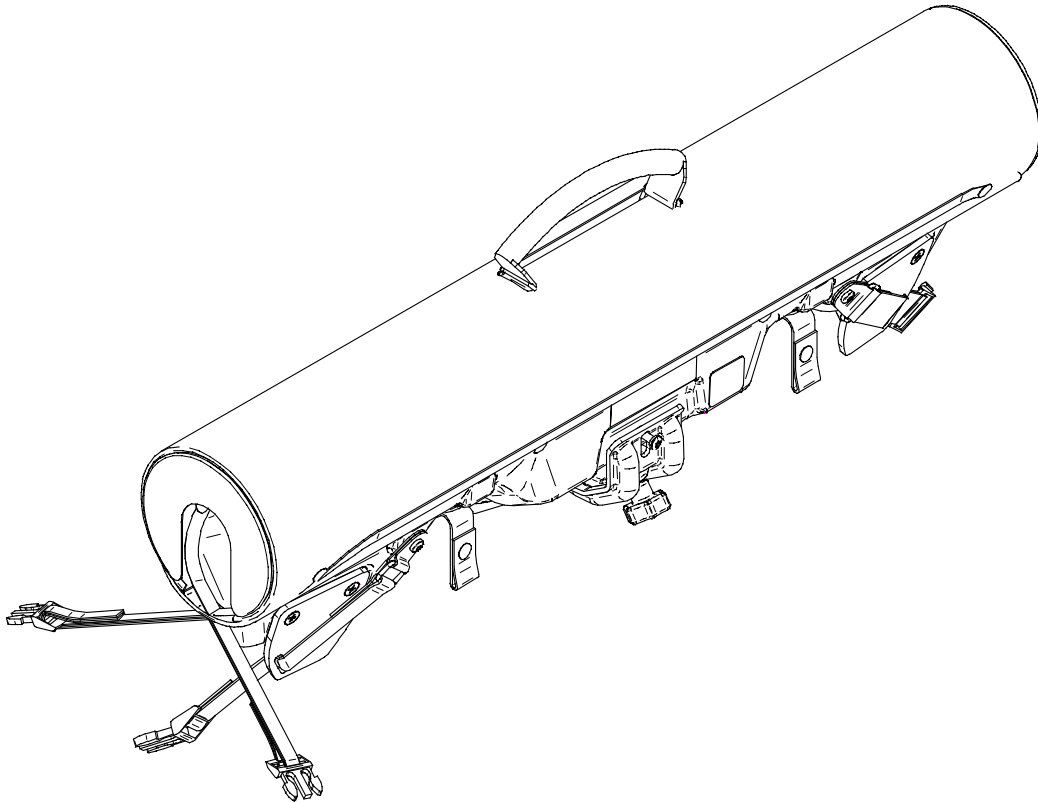

Pendant Assembly with Motion Control - FA64228-XXX


L64-146-XXX Rev A (Reference Only)

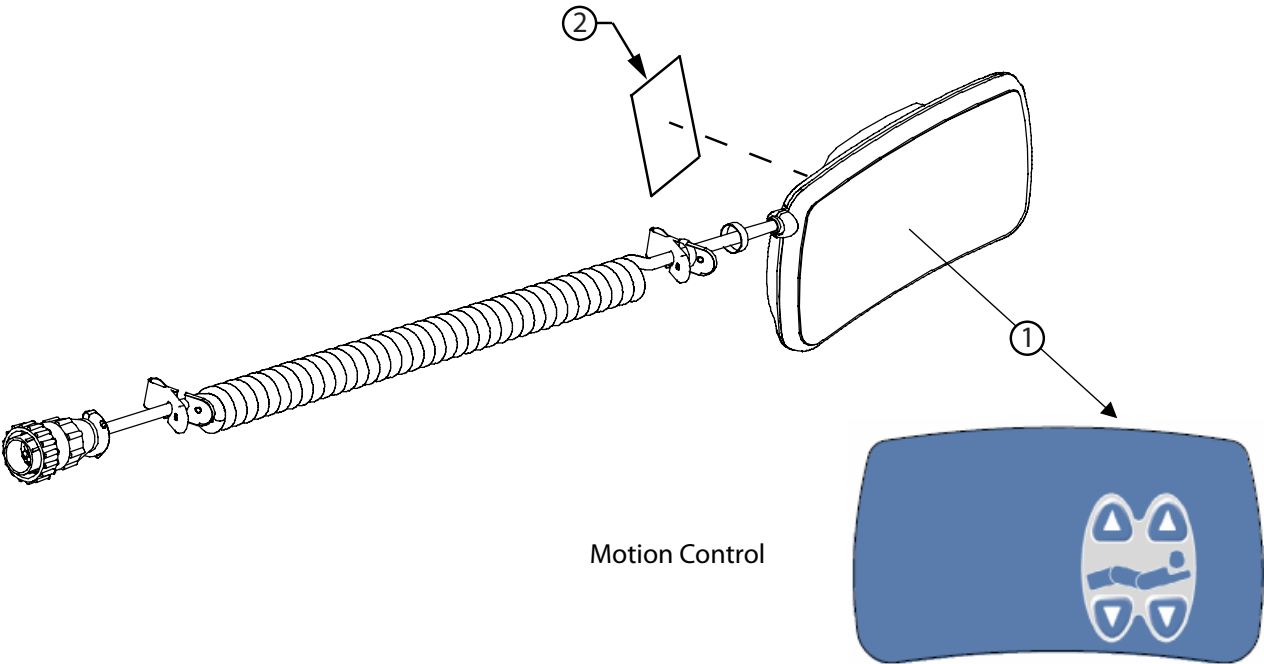

Item	Part No.	Part Name	Qty.
1	QDF64-1240	Removable Pendant with Motion Control	1
2	QE14399-T	Manufacturer Sticker	1

Pendant Assembly with Motion Control/NC - FA64226


L64-118 (Reference Only)

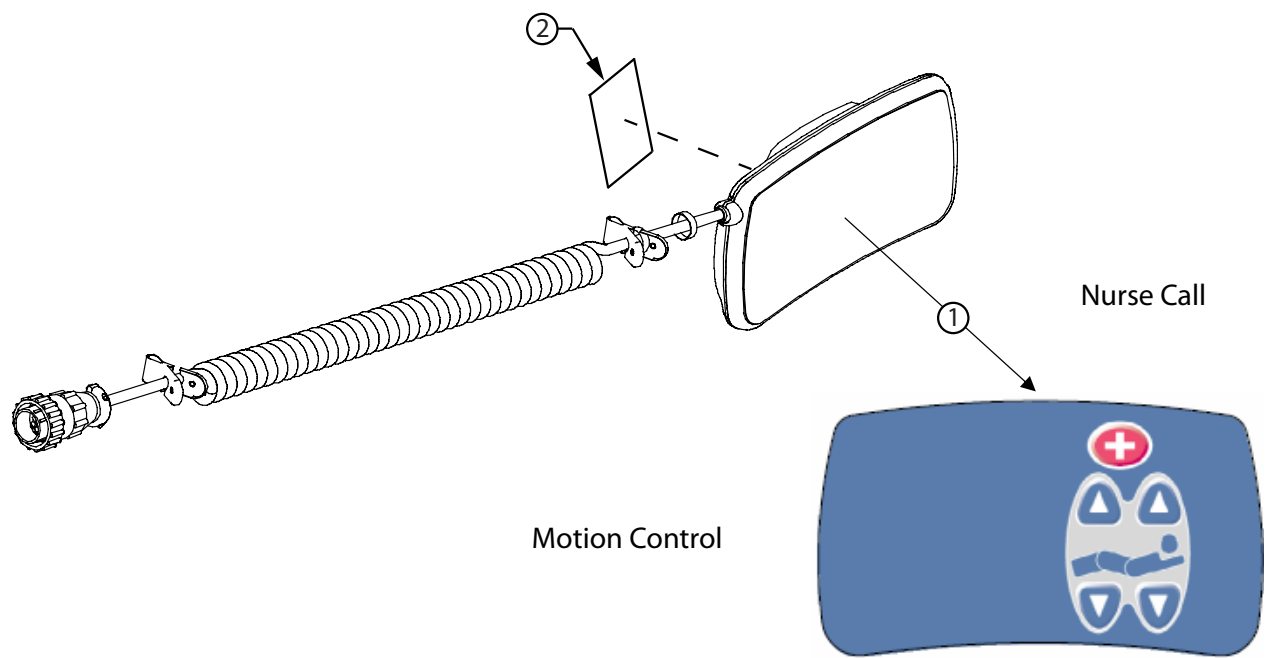

Item	Part No.	Part Name	Qty.
1	QDF64-1238	Removable Pendant with Nurse Call and Motion Control	1
2	QE14399-T	Manufacturer Sticker	1

Pendant Assembly with Motion Control/Smart TV - FA64227


L64-119 (Reference Only)

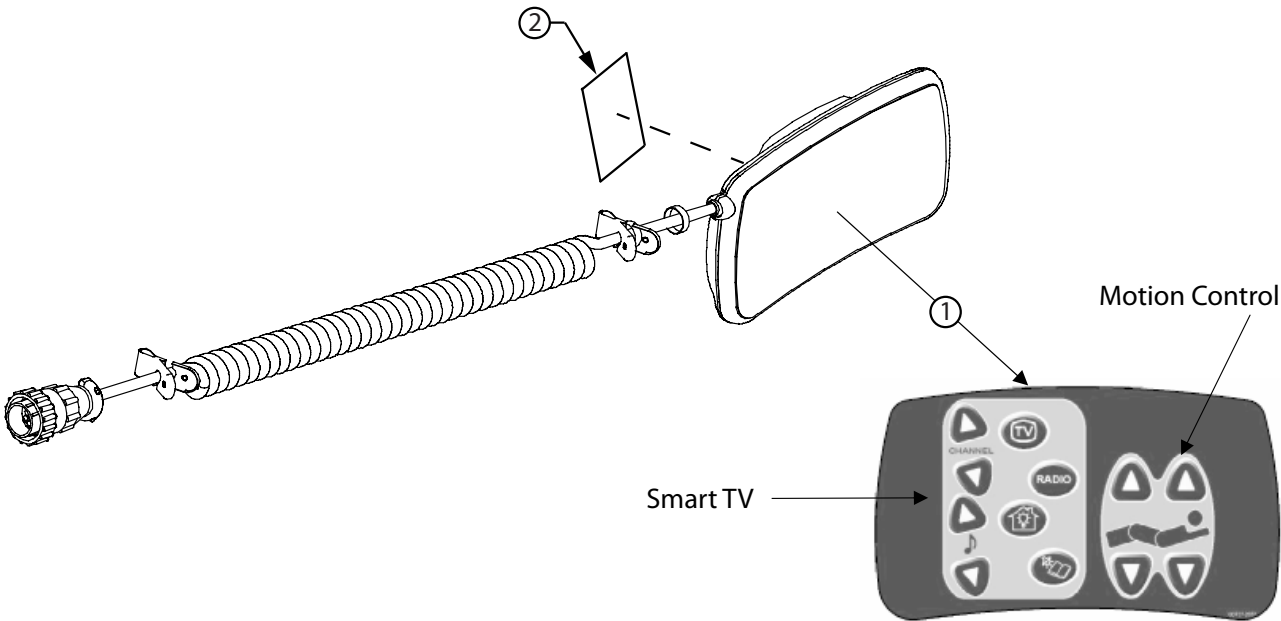

Item	Part No.	Part Name	Qty.
1	QDF64-1239	Removable Pendant with Motion Control and Smart TV	1
2	QE14399-T	Manufacturer Sticker	1

Pendant Assembly with Motion Control/NC/Smart TV - FA64225


L64-117 (Reference Only)

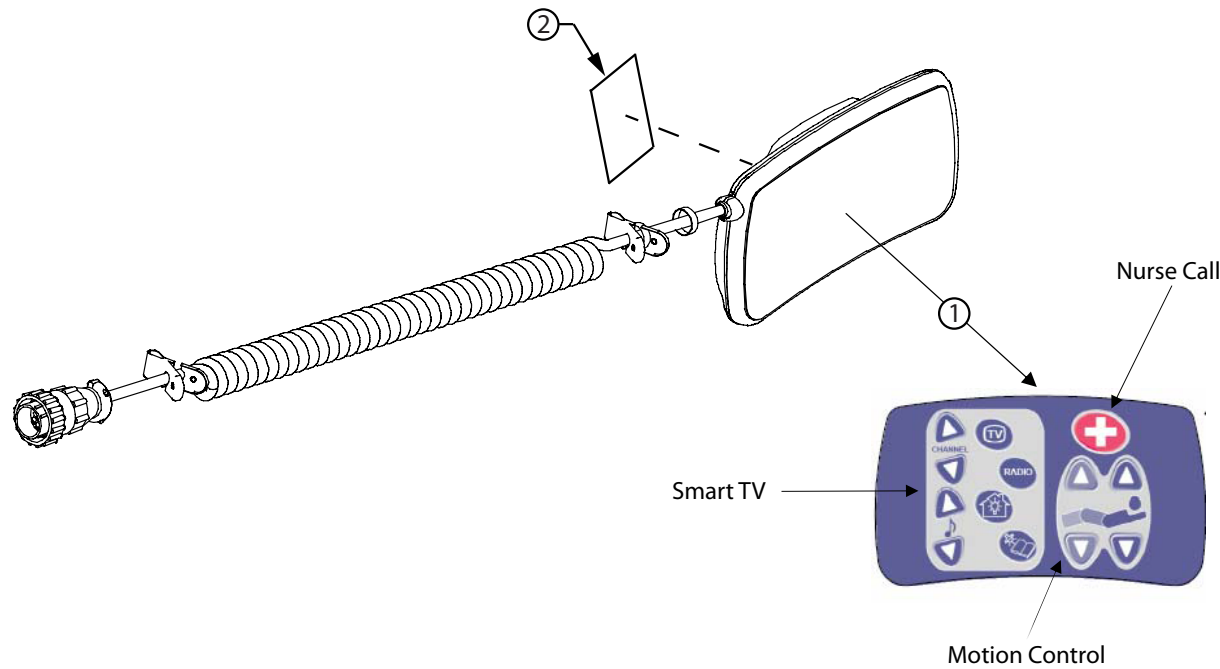

Item	Part No.	Part Name	Qty.
1	QDF64-1237	Removable Pendant with Nurse Call, Motion Control and Smart TV	1
2	QE14399-T	Manufacturer Sticker	1

Pendant Clip Assembly - FA64186-XXX


L64-111 Rev-01 (Reference Only)

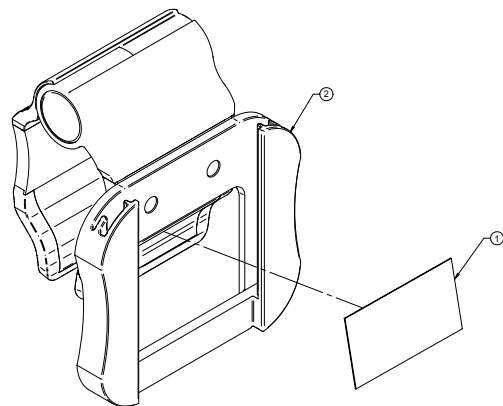

Item	Part No.	Part Name	Qty.
1	QE14399-T	Manufacturer Sticker	1
2	QDF64-1282	Additional Removable Grip	1

Roller Bumpers


OL270050 Rev 04 (Reference Only)

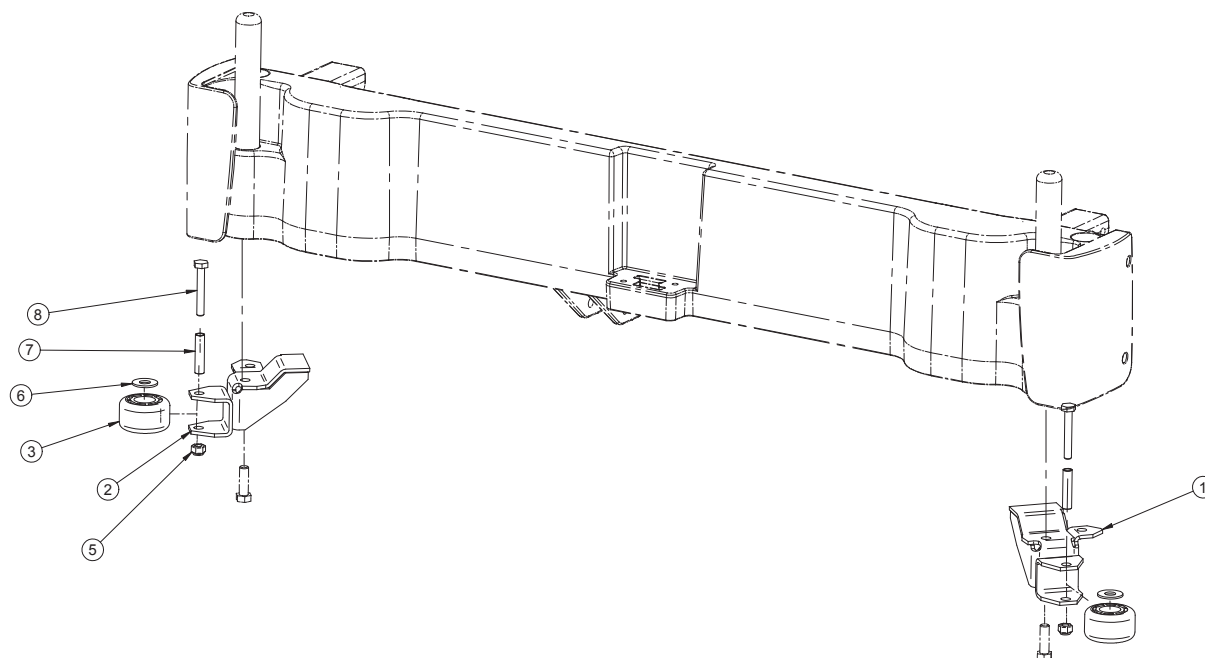

Item	Part No.	Part Name	Qty.
1	27-2046P	Left Bumper Support	1
2	27-2056P	Right Bumper Support	1
3	QPC27-2059	Wheel, 1 3/4" Diameter	2
5	VE30A1N	Nylon Locknut	2
6	VW10C122802	Nylon Washer	2
7	27-2235Z	Bumper Spacer	2
8	VB15A1N44	Bolt	2

Traction Sleeve Assembly, 4" x 1/2" - FA64215-XXX


L64-134-XXX Rev A (Reference Only)

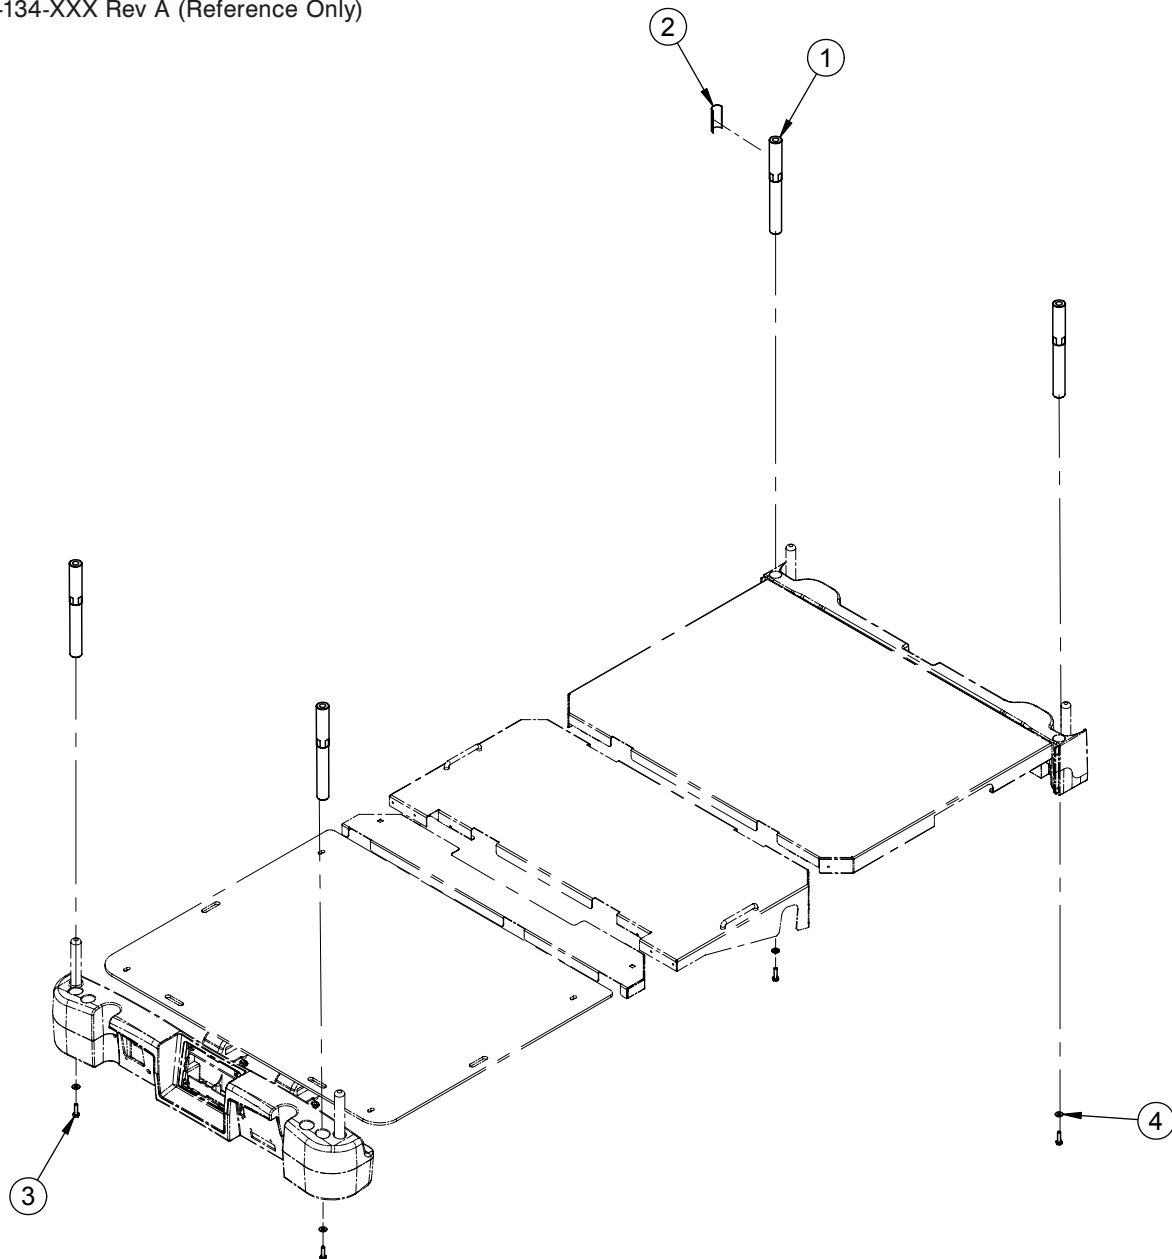

Item	Part No.	Part Name	Qty.
1	64-1262C	Traction Sleeve 4" x 1/2"	4
2	QE14399-T	Manufacturer's Nameplate	1
3	VB15A1N32-S	Hex Bolt	4
4	VW10A08	Flat Washer	4

Traction Sleeve Assembly, 4" x 3/4" - FA64216-XXX


L64-135-XXX Rev A (Reference Only)

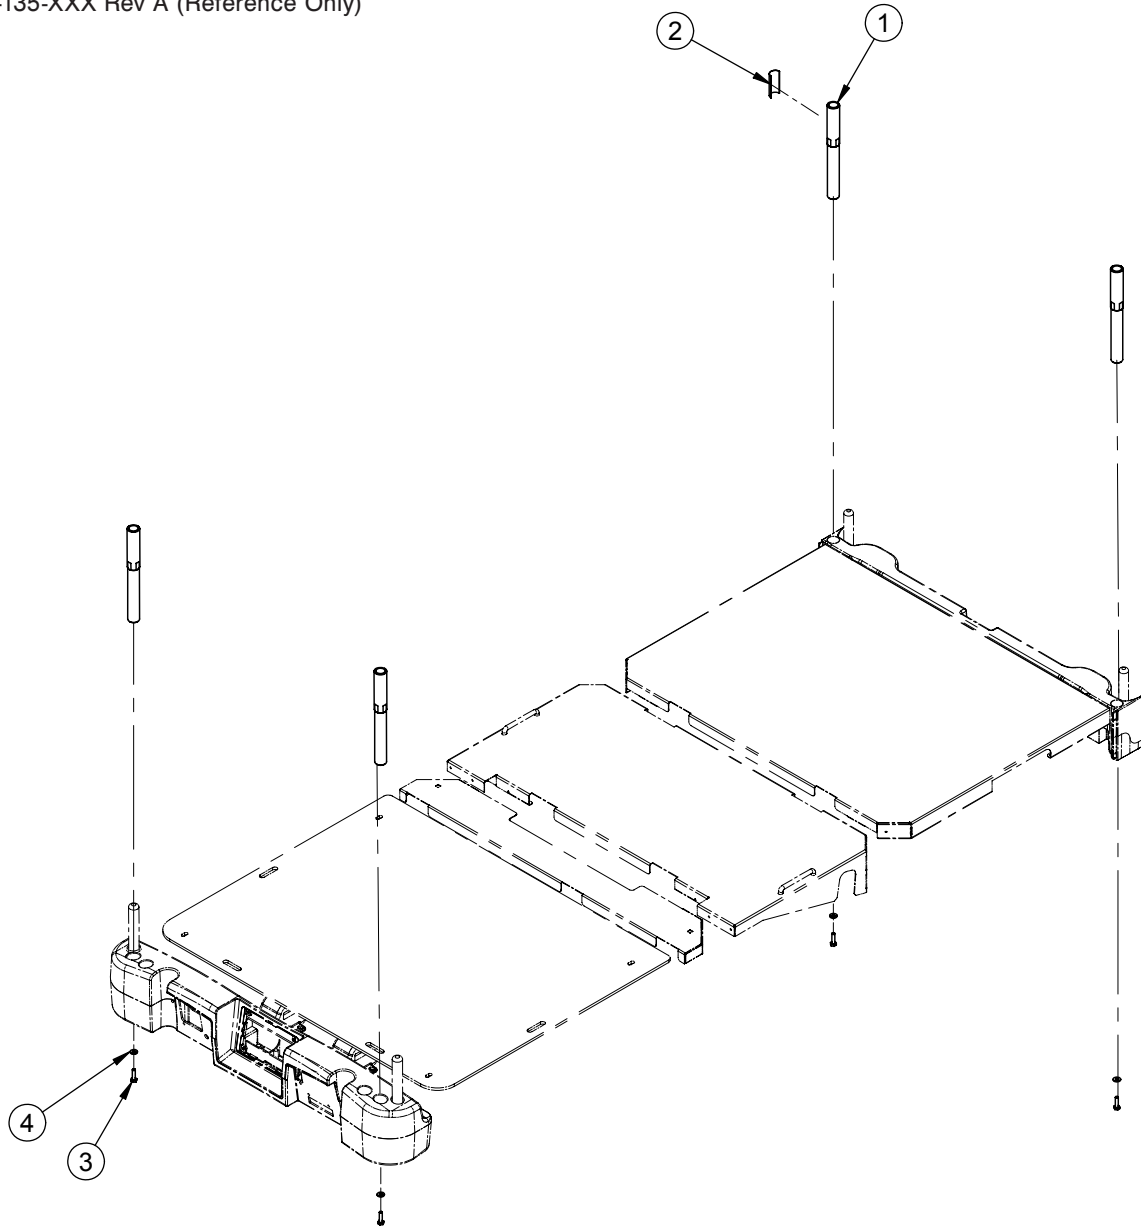

Item	Part No.	Part Name	Qty.
1	64-1263C	Traction Sleeve 4" x 3/4"	4
2	QE14399-T	Manufacturer's Nameplate	1
3	VB15A1N32-S	Hex Bolt	4
4	VW10A08	Flat Washer	4

Traction Sleeve Assembly, 8" x 1/2" - FA64217-XXX


L64-136-XXX Rev A (Reference Only)

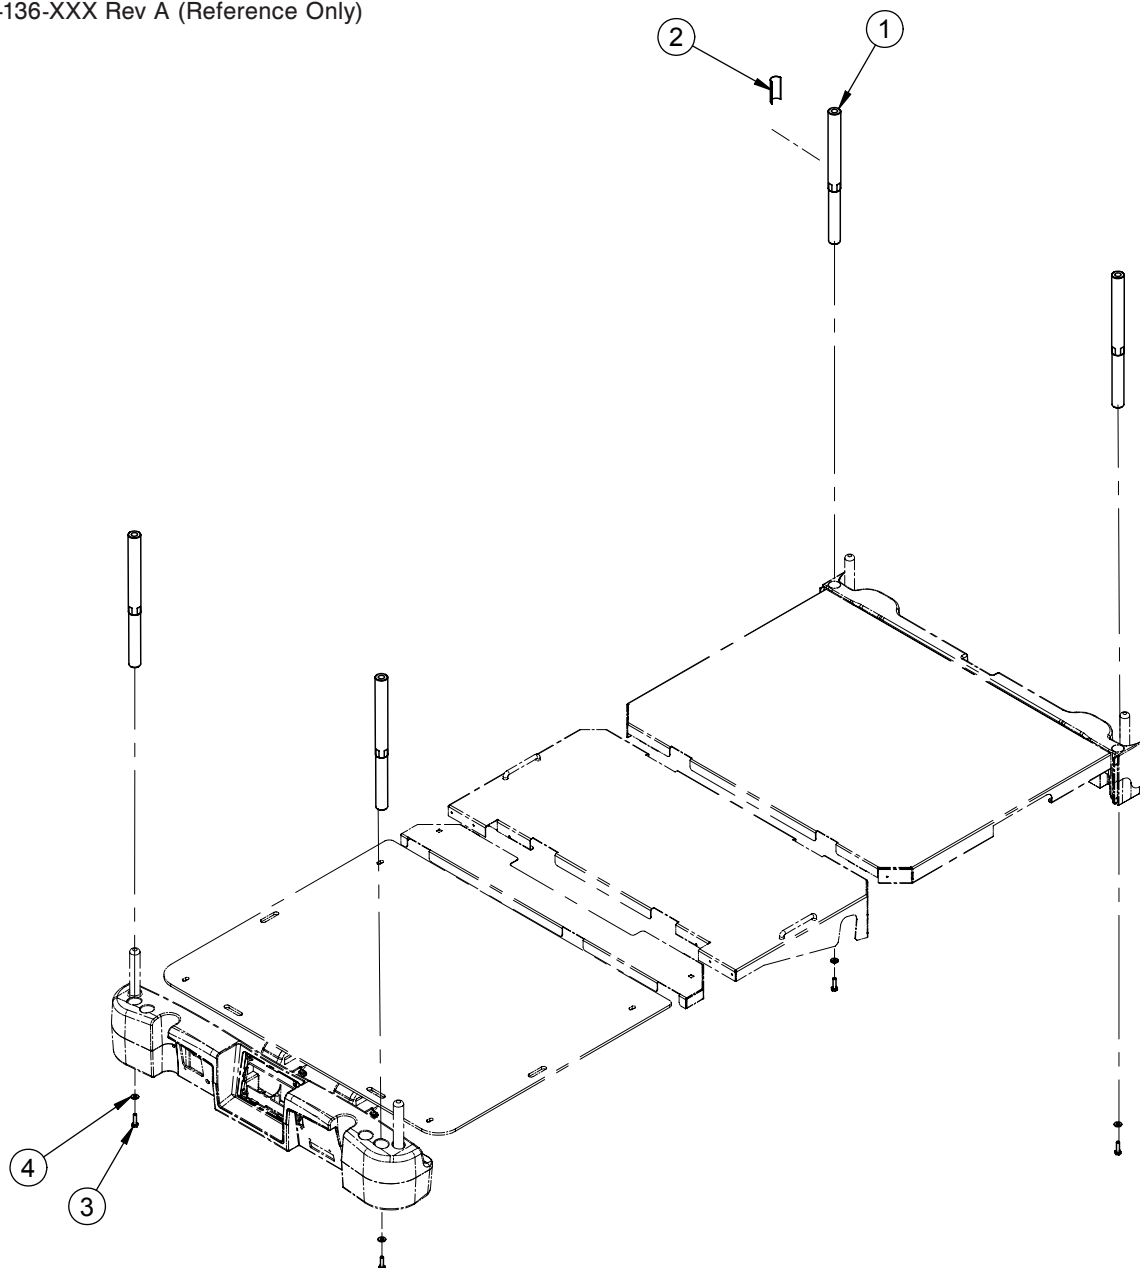

Item	Part No.	Part Name	Qty.
1	64-1264C	Traction Sleeve 8" x 1/2"	4
2	QE14399-T	Manufacturer's Nameplate	1
3	VB15A1N32-S	Hex Bolt	4
4	VW10A08	Flat Washer	4

Traction Sleeve Assembly, 8" x 3/4" - FA64218-XXX


L64-137-XXX Rev A (Reference Only)

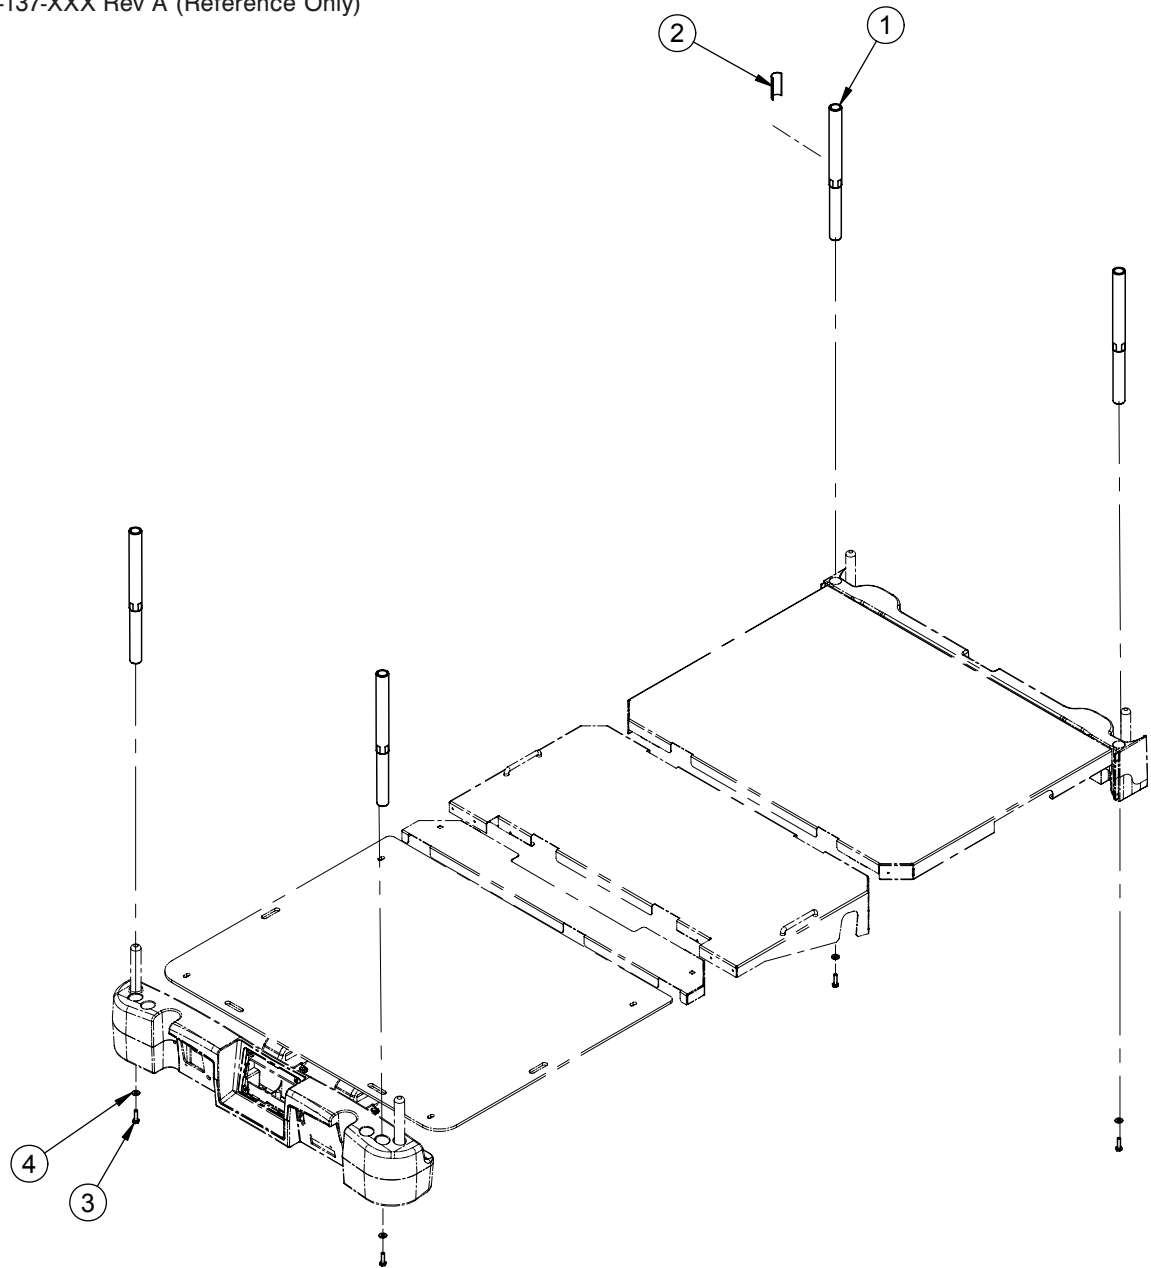

Item	Part No.	Part Name	Qty.
1	64-1265C	Traction Sleeve 8" x 3/4"	4
2	QE14399-T	Manufacturer's Nameplate	1
3	VB15A1N32-S	Hex Bolt	4
4	VW10A08	Flat Washer	4

Traction Sleeve Assembly, 6-1/2" x 3/4" - FA64219-XXX


L64-138-XXX Rev A (Reference Only)

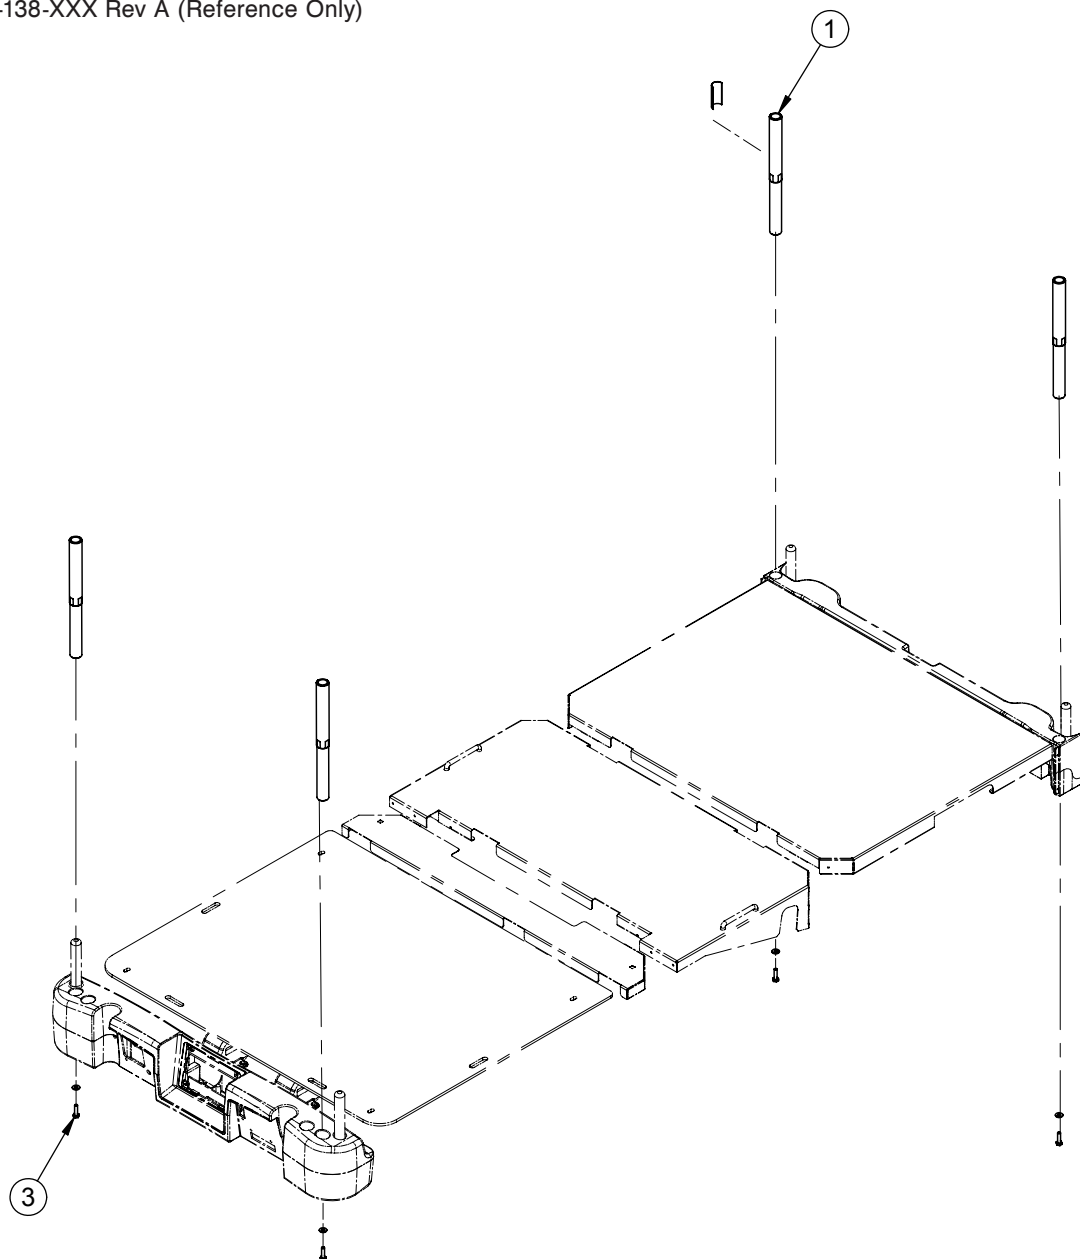

Item	Part No.	Part Name	Qty.
1	64-1266C	Traction Sleeve 6-1/2" x 3/4"	4
2	QE14399-T	Manufacturer's Nameplate	1
3	VB15A1N32-S	Hex Bolt	4
4	VW10A08	Flat Washer	4

Wall Saver Cable Assembly - FA64208


L64-129 Rev-03 (Reference Only)

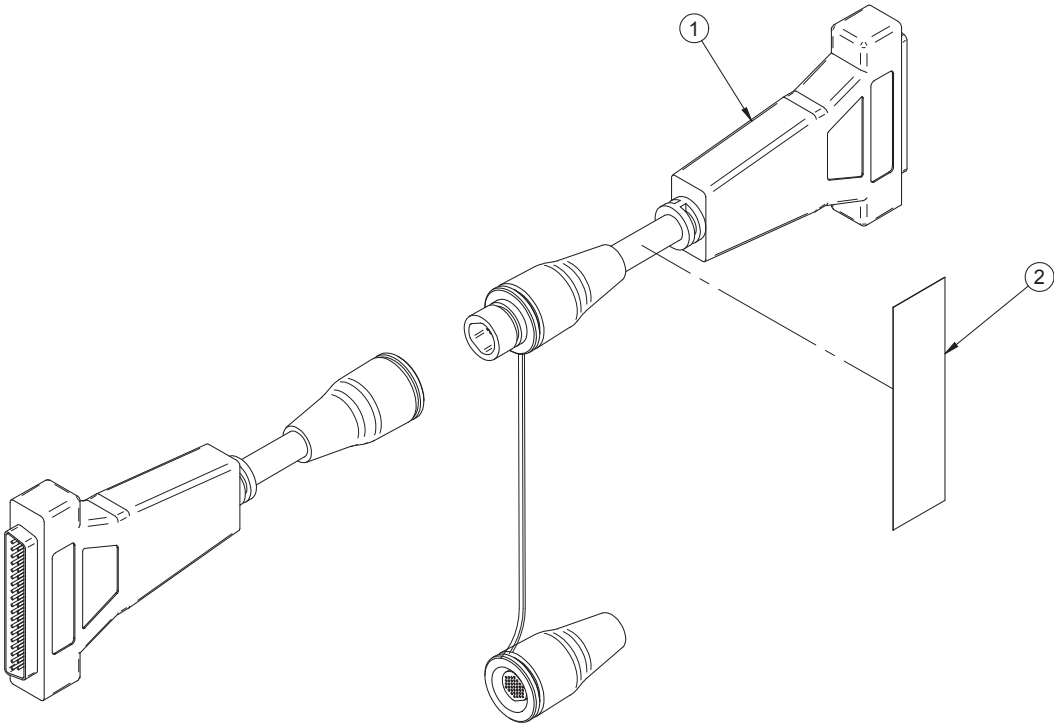

Item	Part No.	Part Name	Qty.
1	QDF64-1371	Wall Saver	1
2	QE71-1313-T	Sticker Manufacturing	1

X-Ray Cassette Holder Assembly - FA64205-XXX

L64-123-XXX Rev A (Reference Only)

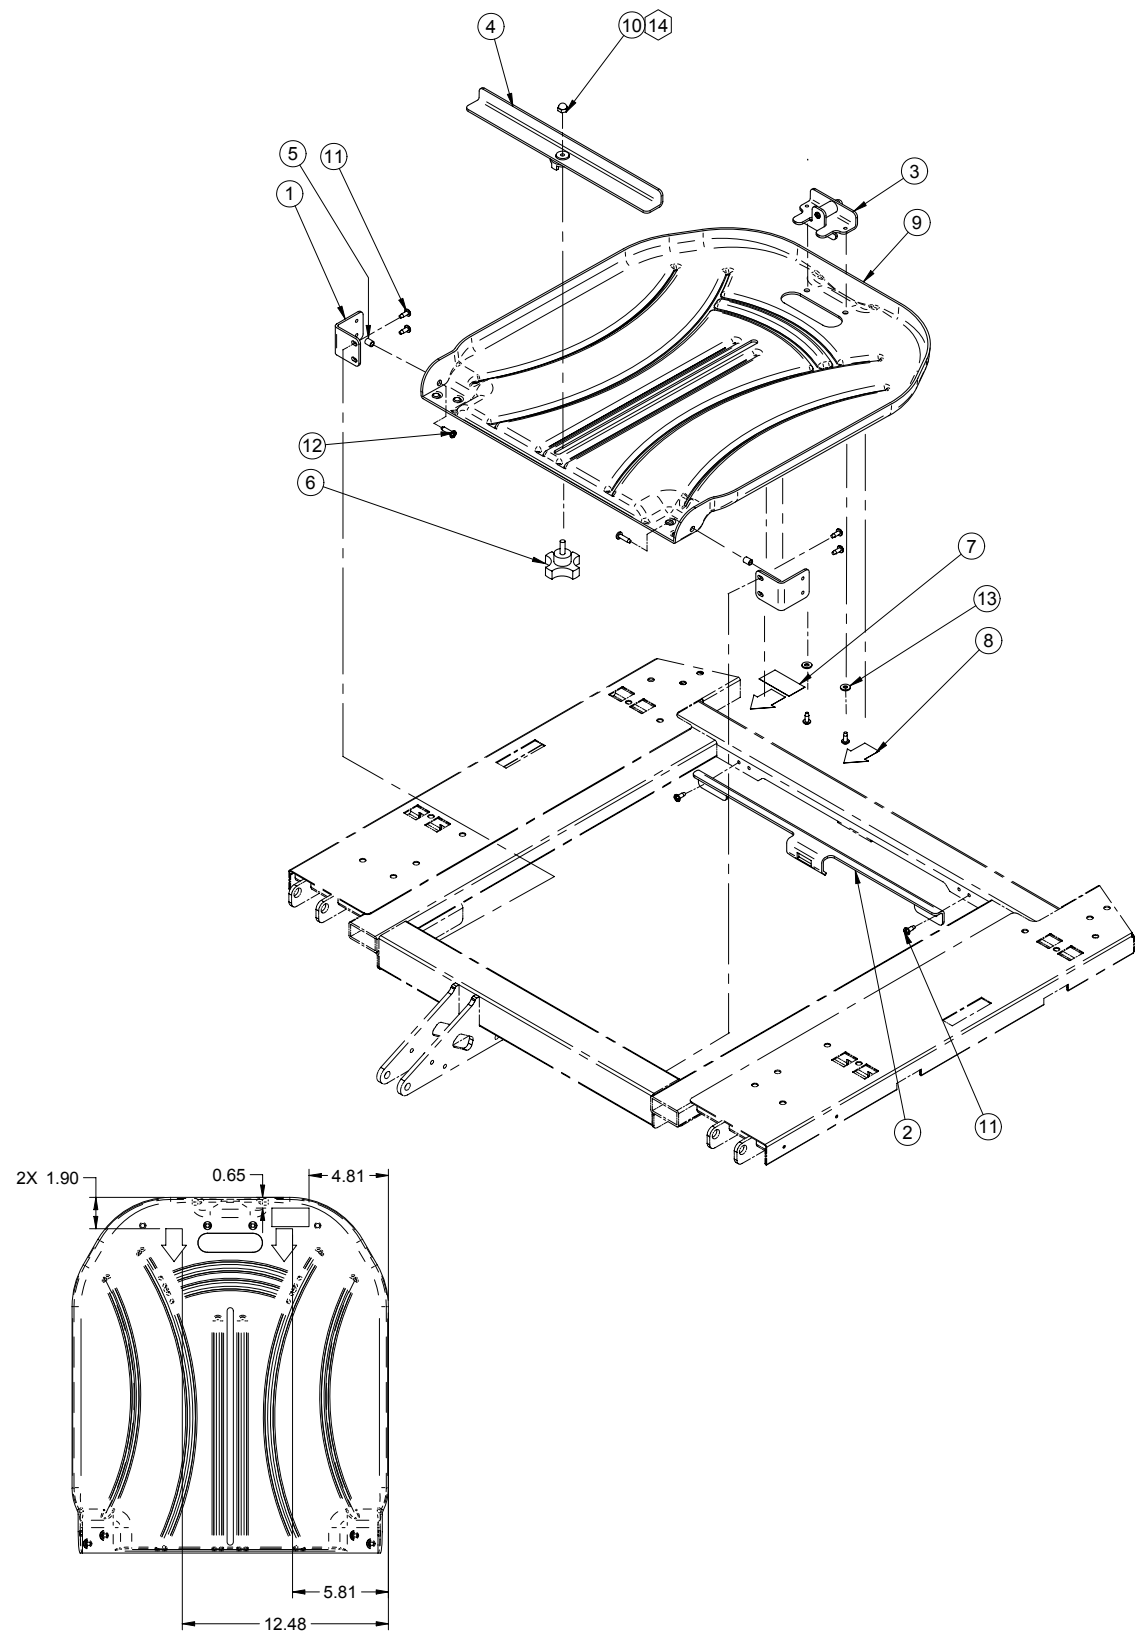


X-Ray Cassette Holder Assembly - FA64205-XXX

X-Ray Cassette Holder Assembly - L64-123-XXX Rev A (Reference Only)

Item	Part No.	Part Name	Qty.
1	64-1199Z	Right Cassette Holder Pivot Point	2
2	64-1372P	Fastener	1
3	64-1255	Plunger	1
4	64-1260Z	Cassette Support	1
5	64-1276	X-Ray Cassette Support Spacer	2
6	QDF2093	X-Ray Cassette	
		Manual Tightening Screw	1
7	QE14399-T	Manufacturer Sticker	1
8	QE71-1080	X-Ray Cassette Handle Sticker	2
9	QP64-1185	X-Ray Cassette for Plate	1
10	VE40A1N	Cap Nut	1
11	VV83A9G16	Phillips Head Tapping Screw	8
12	VV83A9G24	Phillips Head Tapping Screw	2
13	VW10A06	Flat Washer	2
14	M0008	Threadlocker	—
		Medium Strength (Blue)	—

Standard Mattress Retainer


OL270223 Rev 01 (Reference Only)

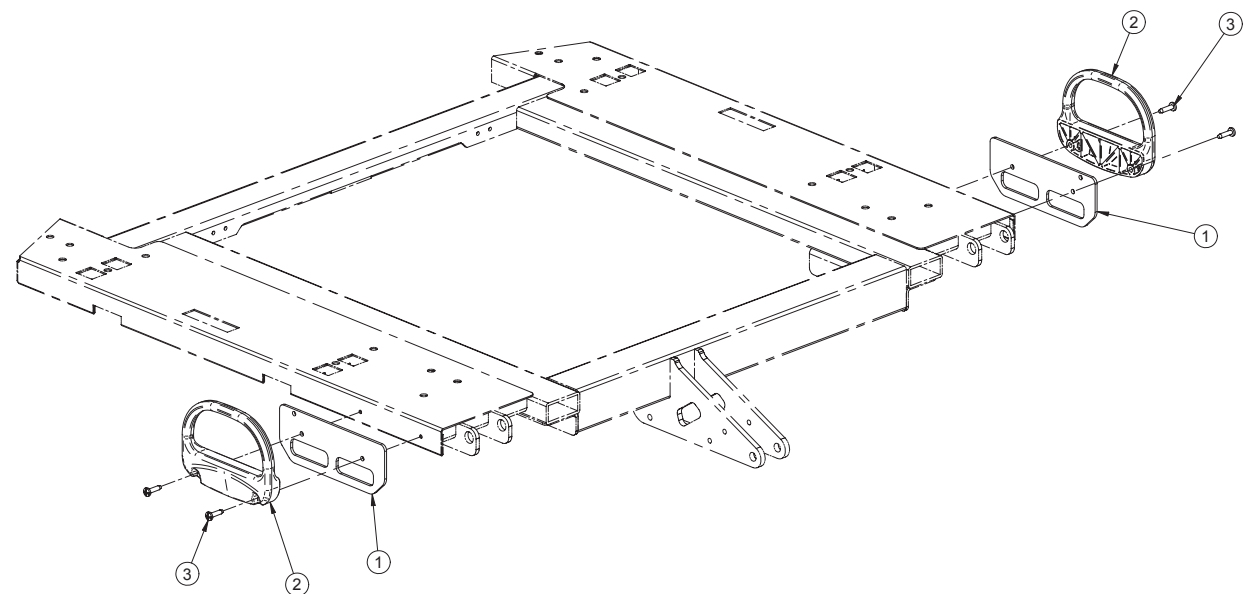

Item	Part No.	Part Name	Qty.
1	27-2015P	Application Support Head	2
2	QP27-1435	Mattress End	2
3	VV83A9G24	Std. Phillips Head Screw	4

Tube Support


OL270224-XXX (Reference Only)

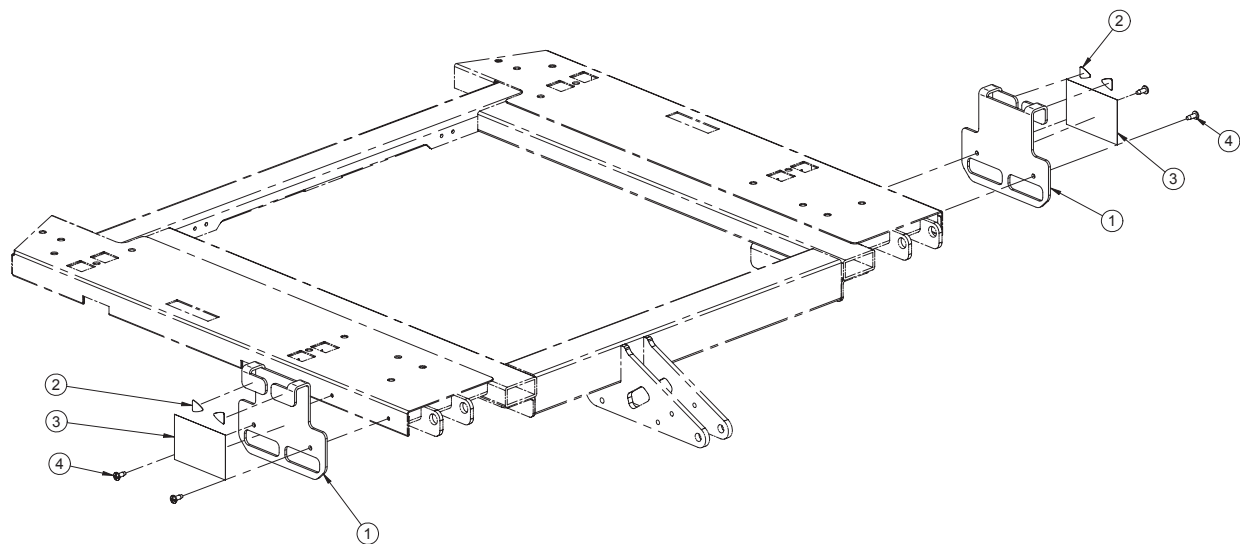

Item	Part No.	Part Name	Qty.
1	27-2518P	Tube Support	2
2	QE71-0498	Triangular Sticker	4
3	QE71-1248-XXX	Sticker to Drainage Tube	2
4	VV83A9G24	Pan Phillips Head Screw	4

Recycling Passports


Assembly Part number: 27-2257/27-2258 (Reference Only)
27-2287/27-2288 (Reference Only)

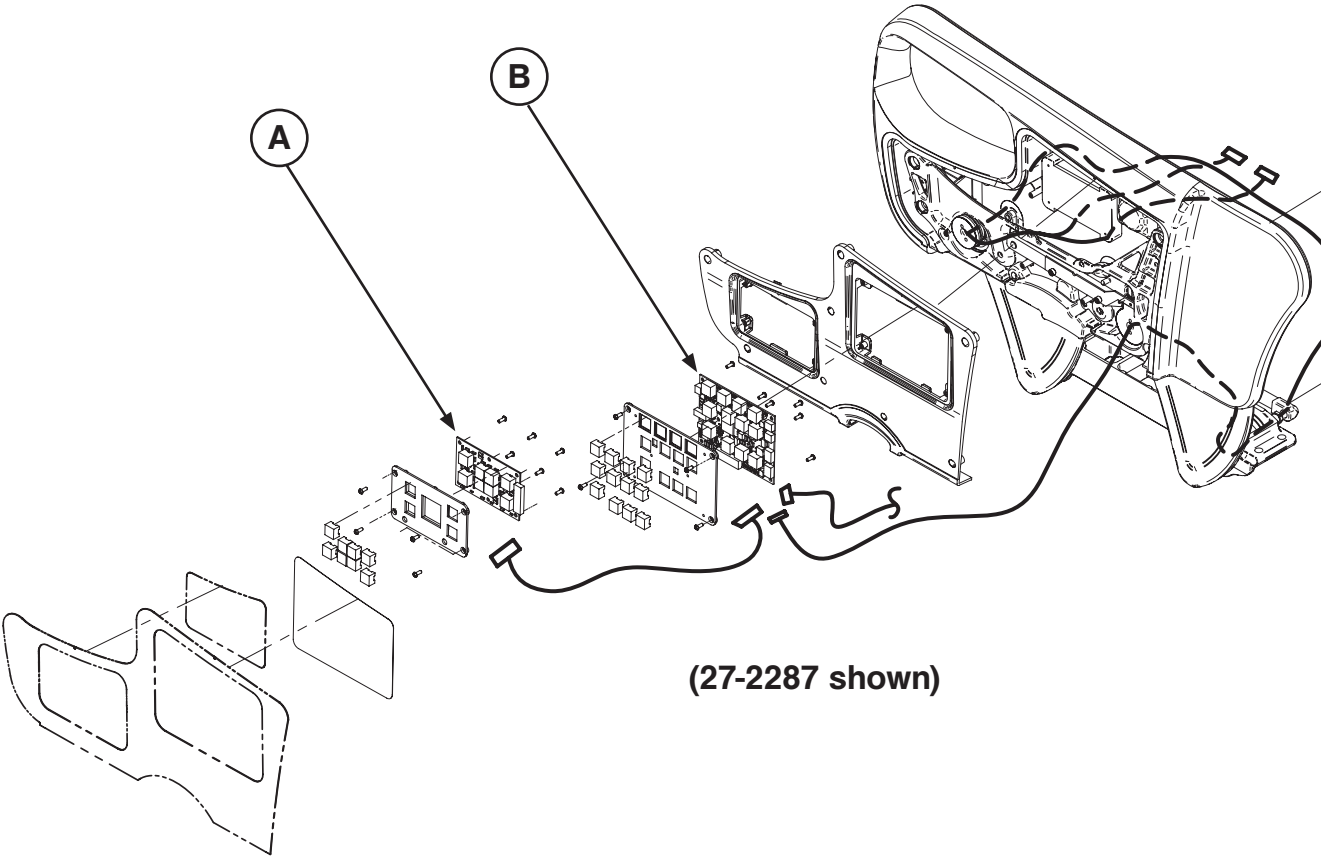

Item	Recycling/Material Code	Important Information	Qty
A	(QDF27-1097) Brake Control Board		2
B	(QDF27-1099) Siderail Nurse Control Board		2

Recycling Passports


Assembly Part number: OL270309 (Reference Only)
 OL270311 (Reference Only)

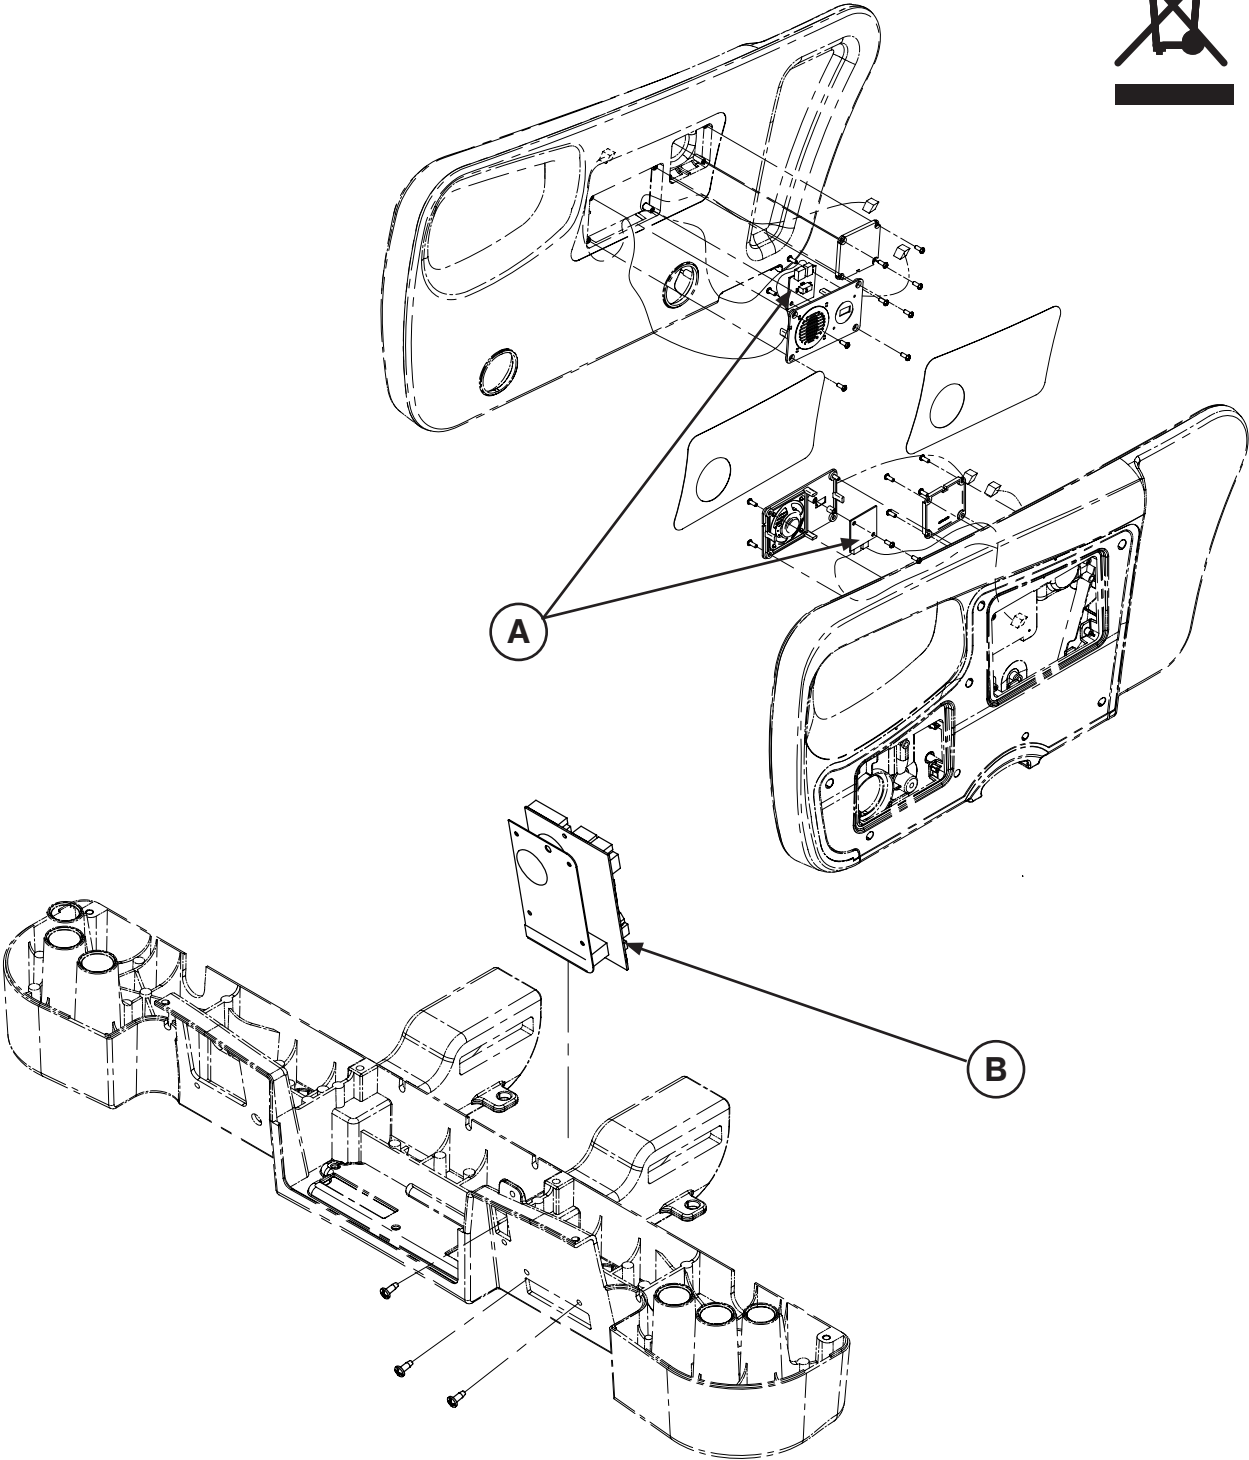

Item	Recycling/Material Code	Important Information	Qty
A	(QDF27-1429) Nurse Call Board		2
B	(QDF75-0270) Room Interface Board		1

Recycling Passports


Assembly Part number: OL270302 (Reference Only)

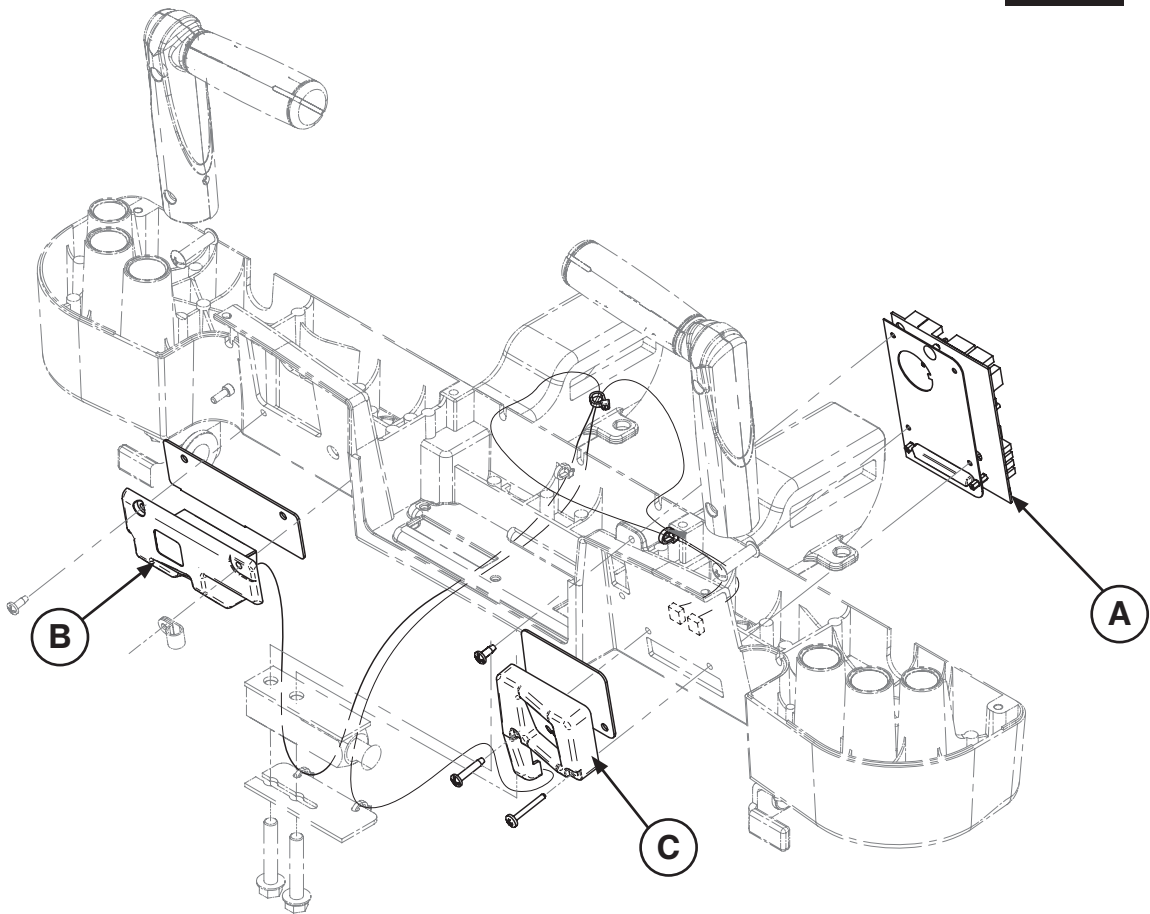

Item	Recycling/Material Code	Important Information	Qty
A	(QDF75-0270) Room Interface Board		1
B	(27-2661) Left IR Module		1
C	(27-2662) Right IR Module		1

Recycling Passports


Assembly Part number: OL270032 (Reference Only)

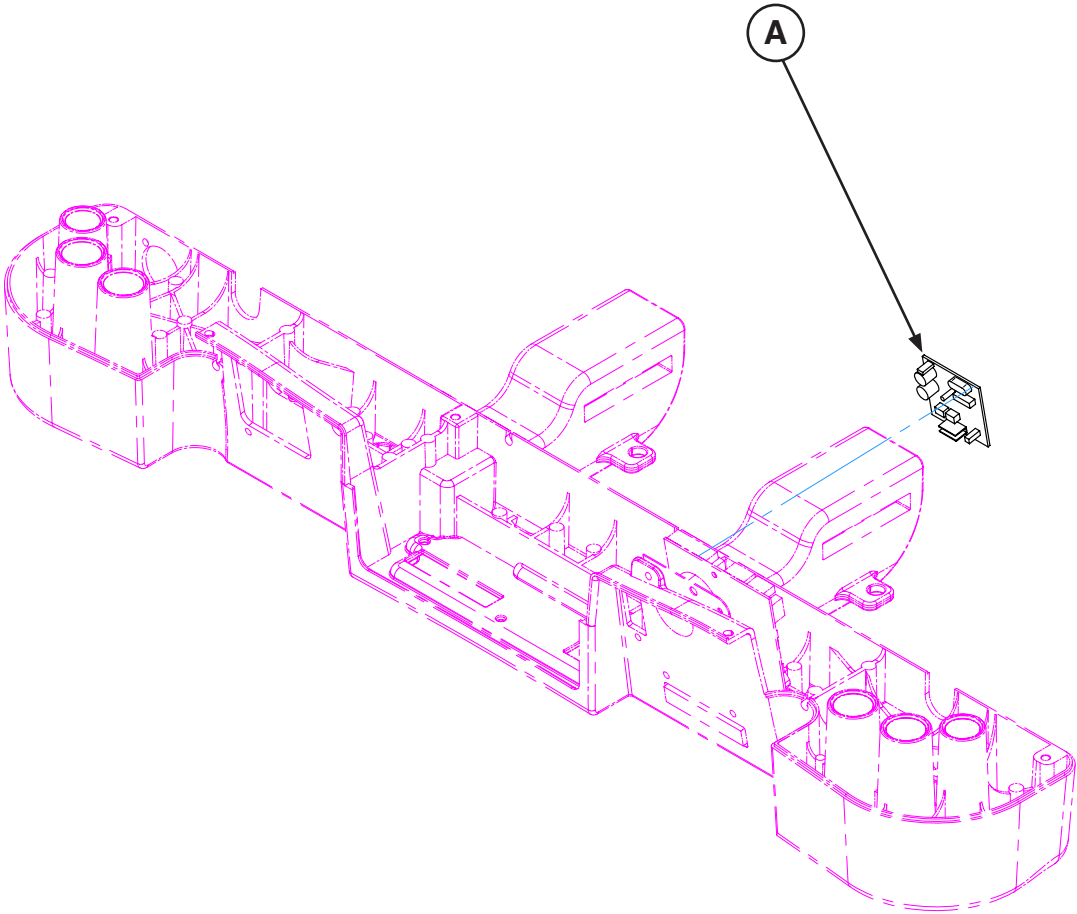

Item	Recycling/Material Code	Important Information	Qty
A	(QDF2060) Smart TV Board		1

Recycling Passports


Assembly Part number: OL270060-XXX (Reference Only)

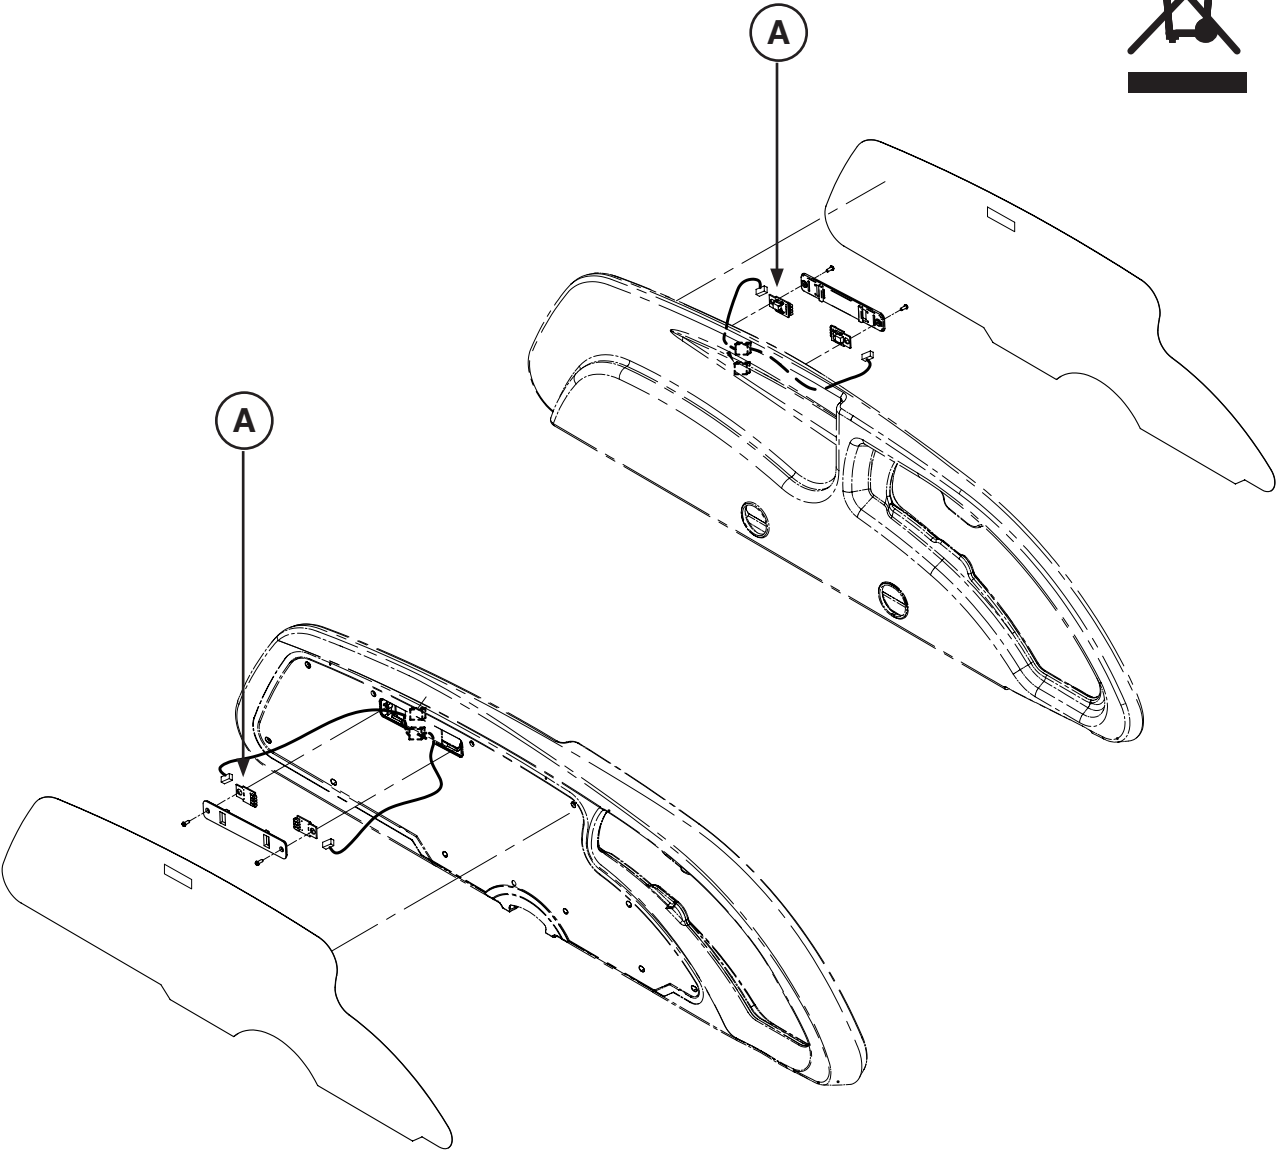

Item	Recycling/Material Code	Important Information	Qty
A	(QDF27-1562) iBed Electronic Board Lens		4

Recycling Passports


Assembly Part number: OL270181 Rev-00 (Reference Only)
(U01001 - U03318, excluding U03258 and U03259)
OL270245 Rev-00 (Reference Only)
(U03319 - U04982, including U03258 and U03259)
OL270263-XXX Rev-00 (Reference Only) (U04983 - U50240)
OL270279-XXX Rev A (Reference Only) (U50241 - 2.5)
OL270263-XXX Rev C (Reference Only) (3.0 - Current)

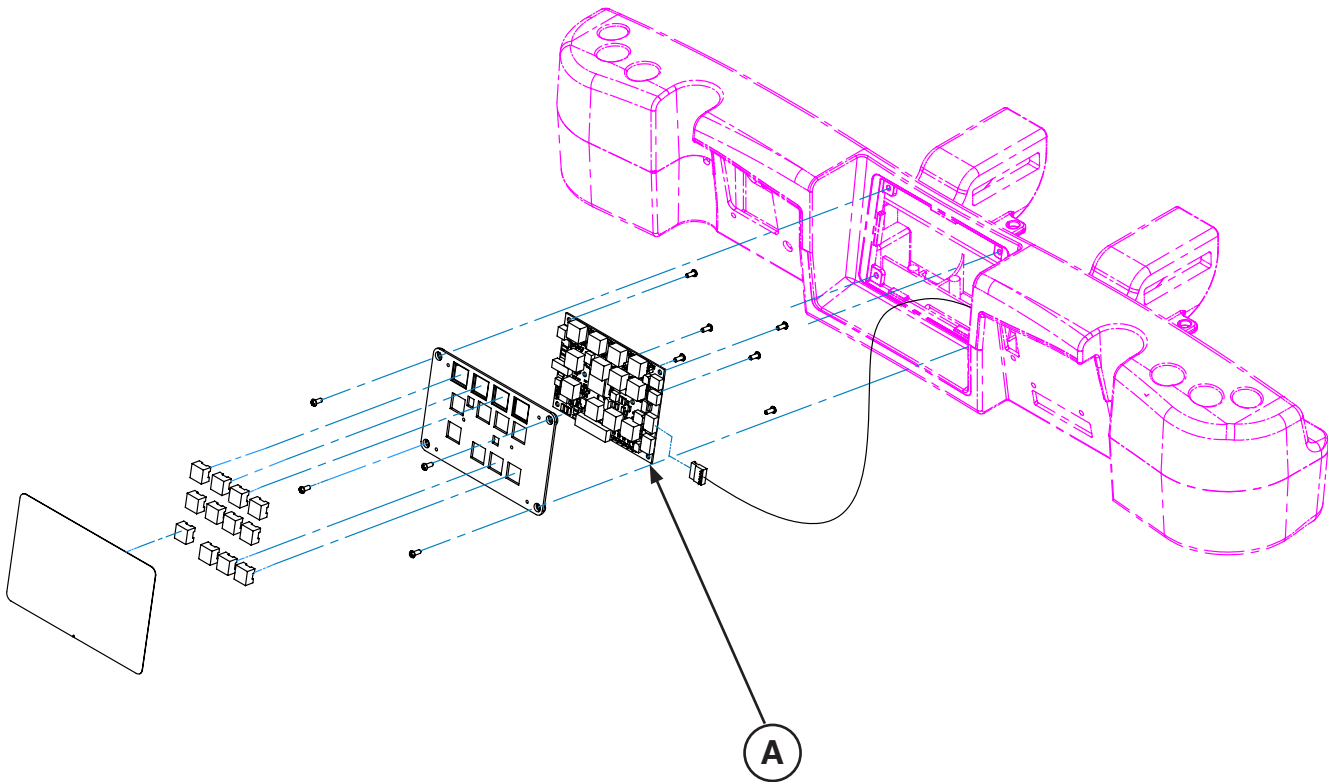

Item	Recycling/Material Code	Important Information	Qty
A	(QDF27-1099) Siderail Nurse Control Board		3

Recycling Passports


Assembly Part number: 27-0900 (Reference Only)
27-2547-XXX (Reference Only)

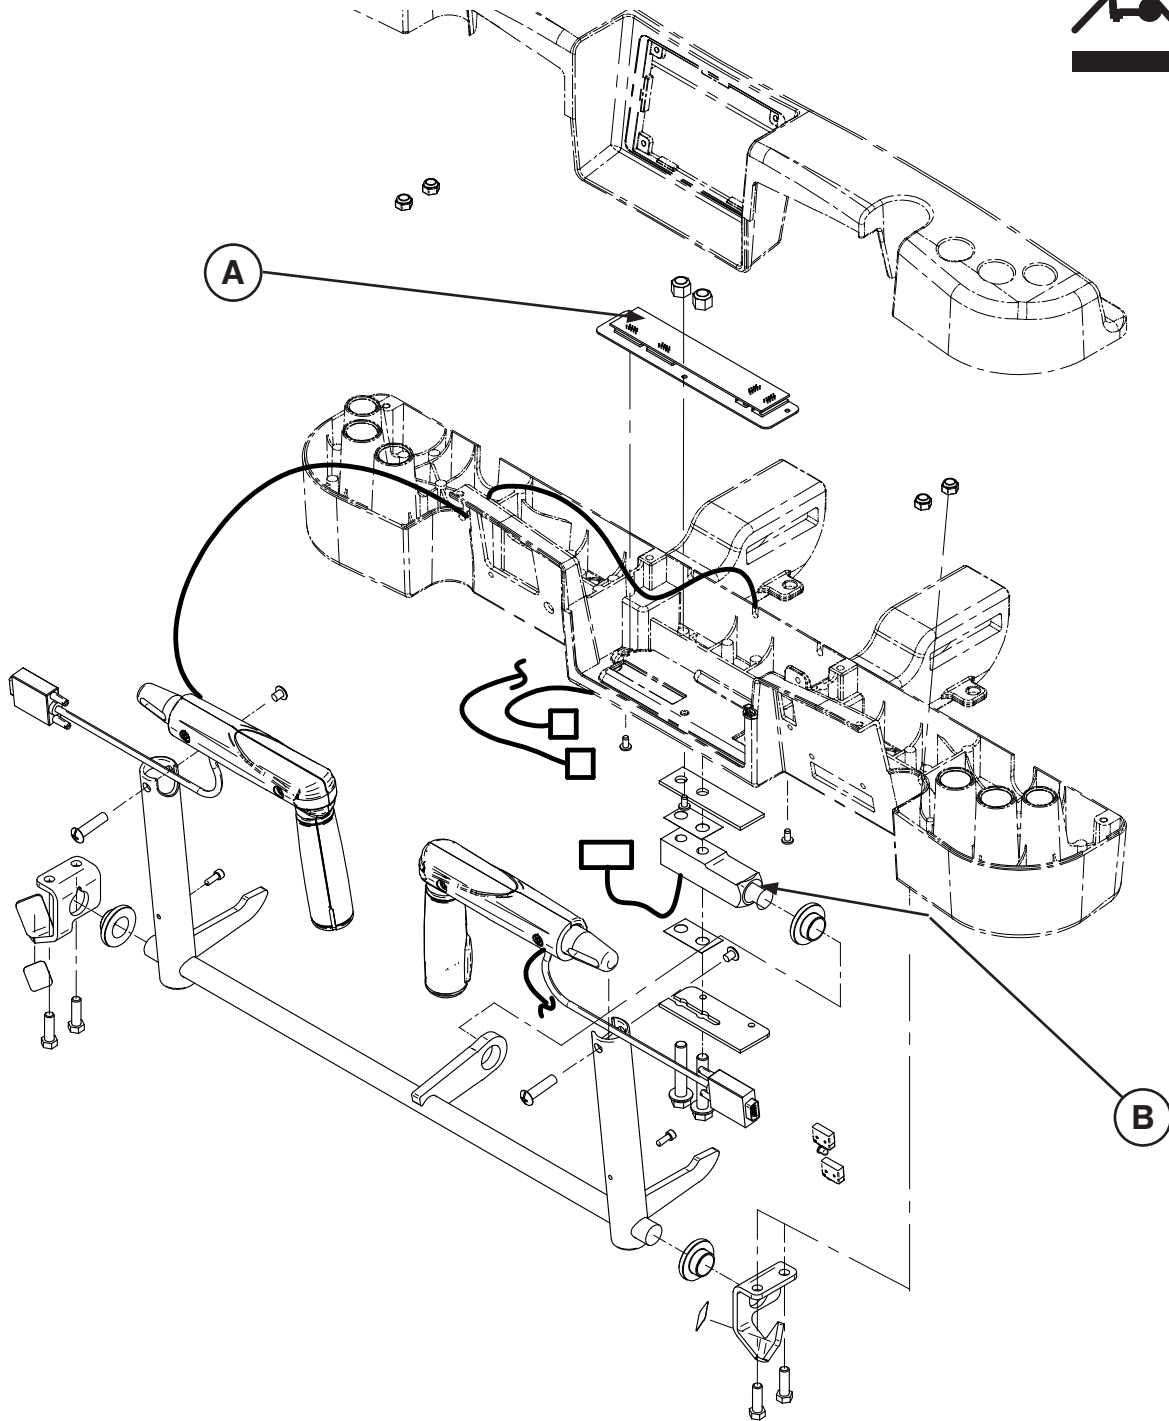

Item	Recycling/Material Code	Important Information	Qty
A	(27-1371) Board CSI 1157	For 27-0900	1
A	(27-2548) Zoom® Control Board	For 27-2547-XXX	1
B	(QDF9136) Zoom® Load Cell		1

Recycling Passports


Assembly Part number: OL270268-XXX (Reference Only)

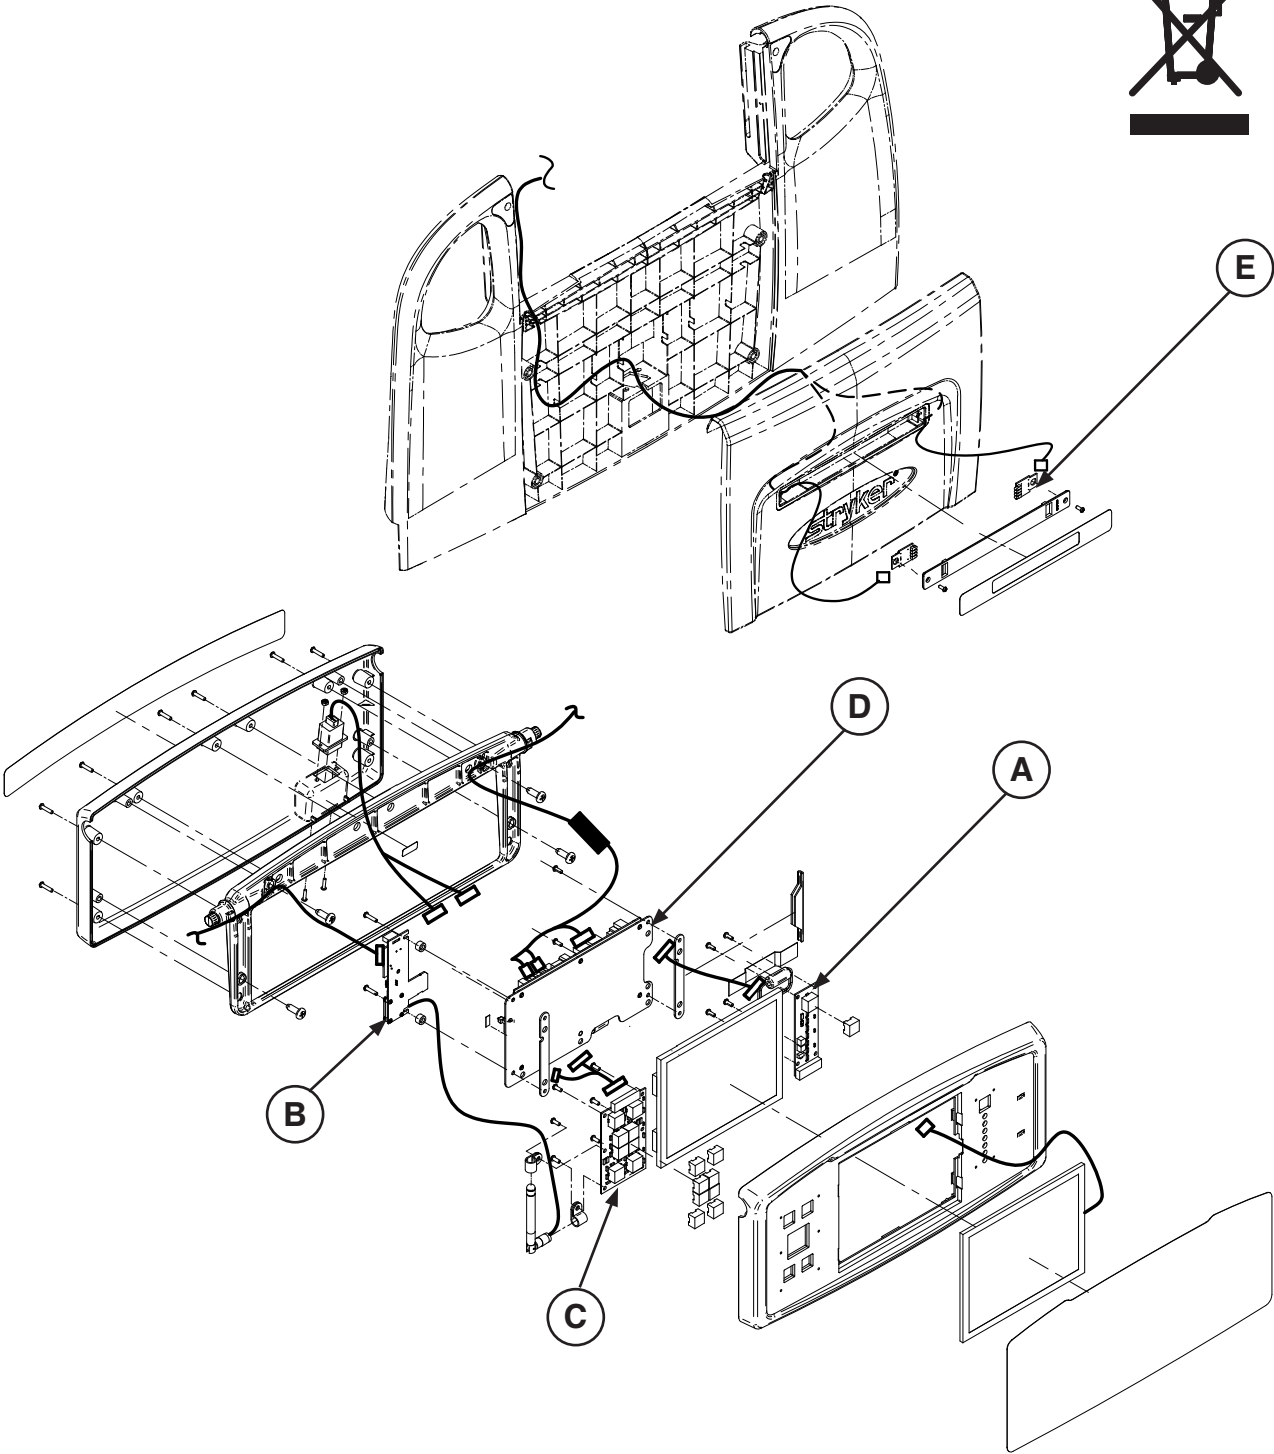

Item	Recycling/Material Code	Important Information	Qty
A	(QDF75-0010) Main Menu Board		1
B	(QDF75-0630) USB Wi-Fi Board		1
C	(QDF27-1097) Brake Control Board		1
D	(QDF75-0290) Touch Board Assembly		1
E	(QDF27-1562) iBed Electronic Board Lens		4

Recycling Passports


Assembly Part number: L27-065 (Reference Only)

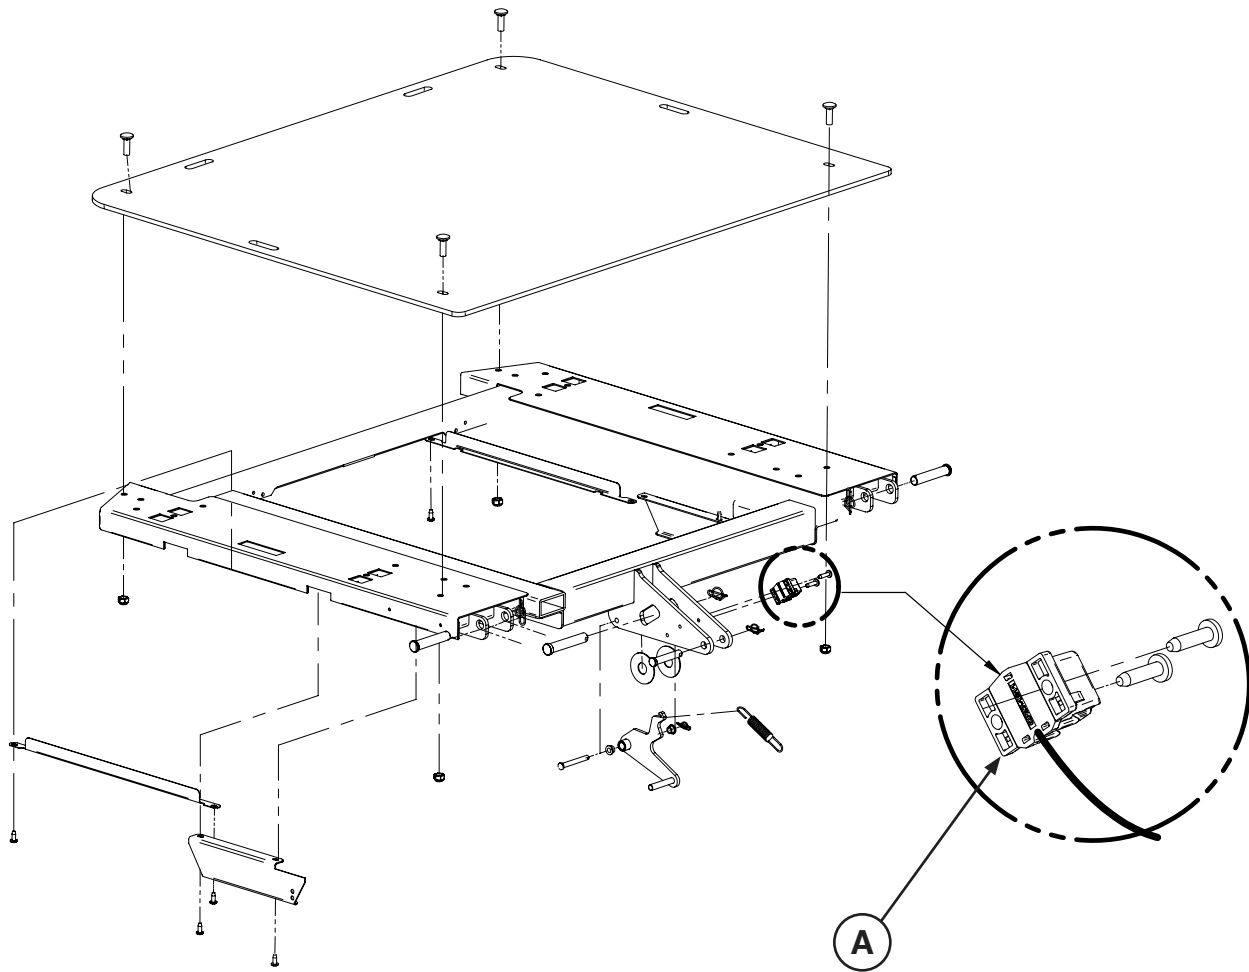

Item	Recycling/Material Code	Important Information	Qty
A	(27-1209) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U01001 - U02817	1
A	(27-2477) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U02818 - Current	1

Recycling Passports


Assembly Part number: L27-065 (Reference Only)

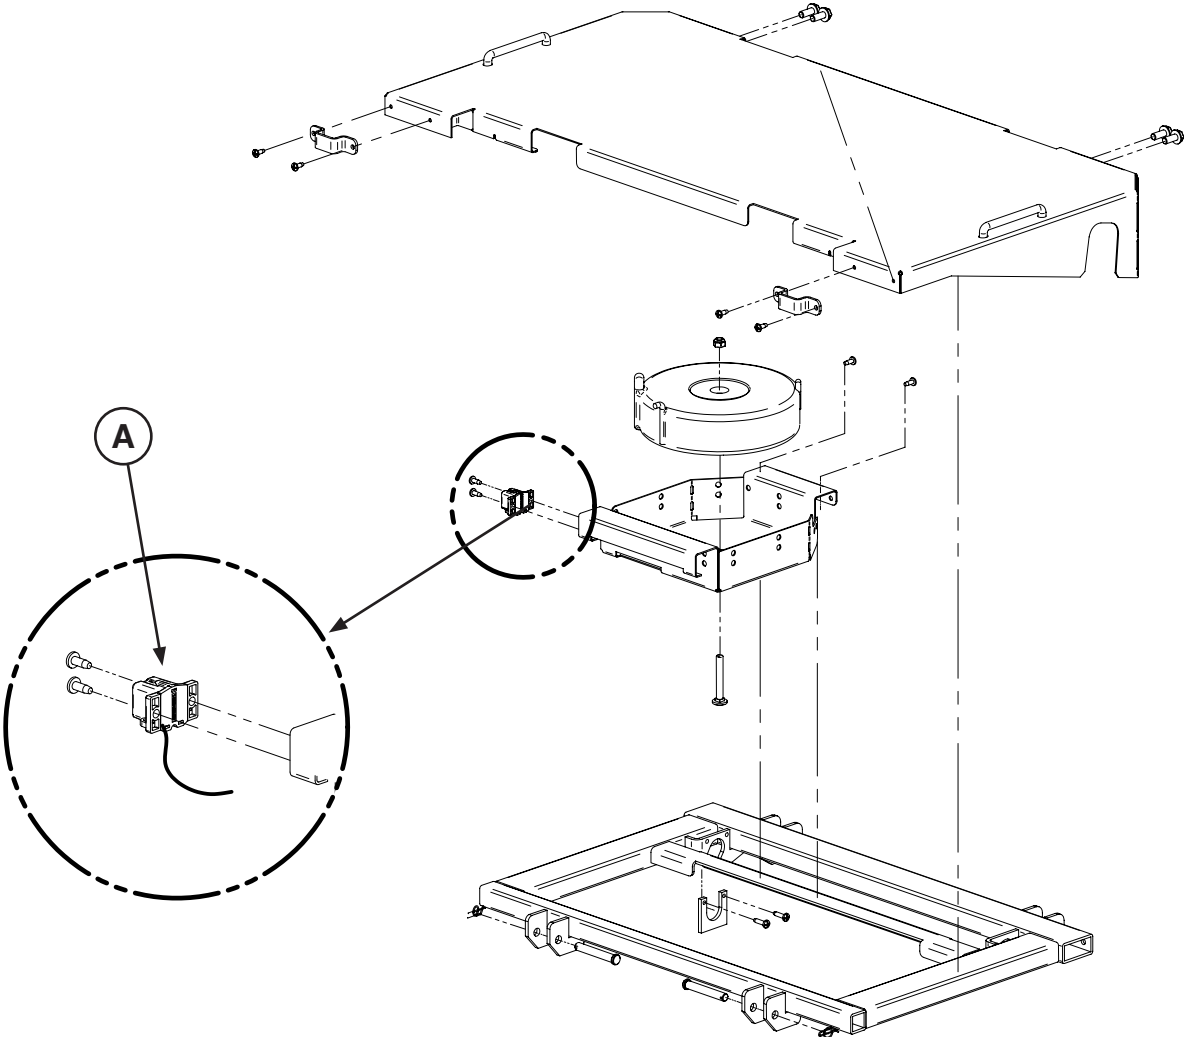

Item	Recycling/Material Code	Important Information	Qty
A	(27-1209) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U01001 - U02817	1
A	(27-2477) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U02818 - Current	1

Recycling Passports


Assembly Part number: 27-2708 (Reference Only)

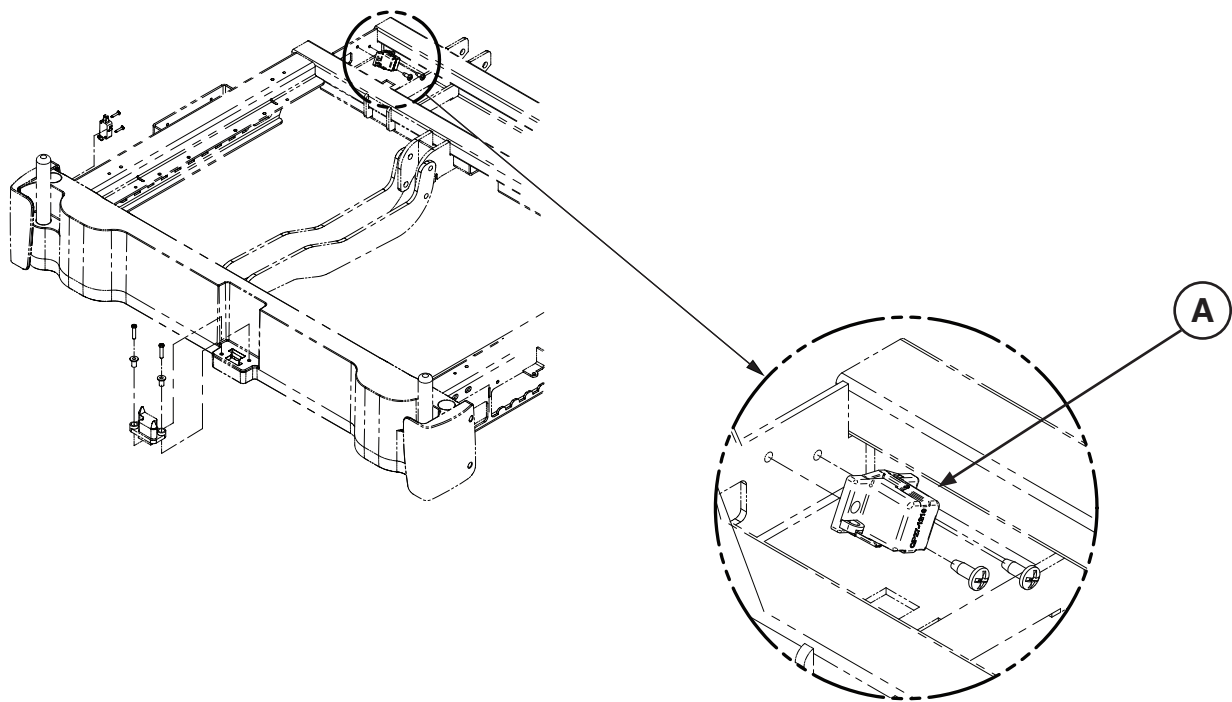

Item	Recycling/Material Code	Important Information	Qty
A	(27-1209) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U01001 - U02817	1
A	(27-2477) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U02818 - Current	1

Recycling Passports


Assembly Part number: L27-043 (Reference Only)

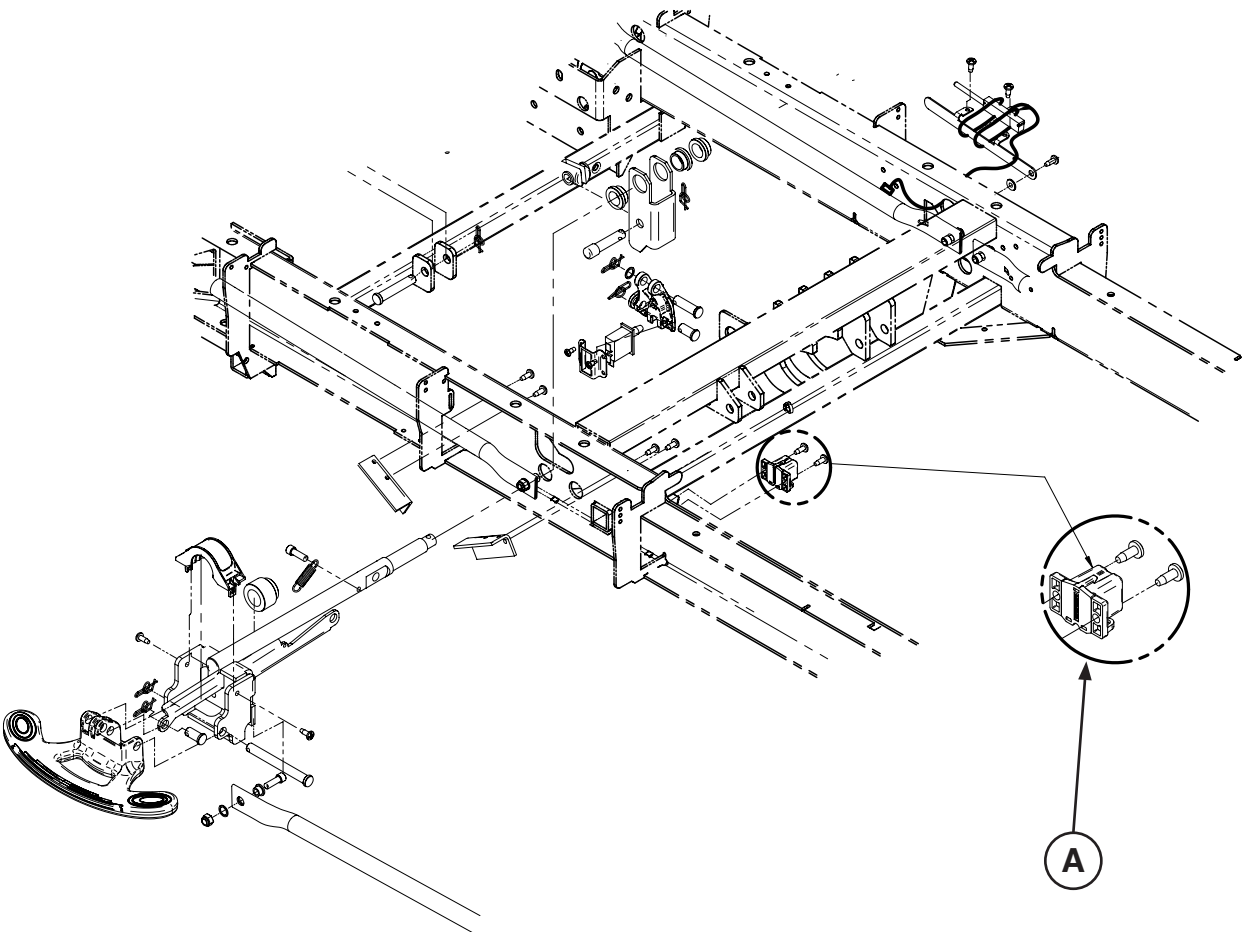

Item	Recycling/Material Code	Important Information	Qty
A	(27-1209) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U01001 - U02817	1
A	(27-2477) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U02818 - Current	1

Recycling Passports


Assembly Part number: L27-046 (Reference Only)

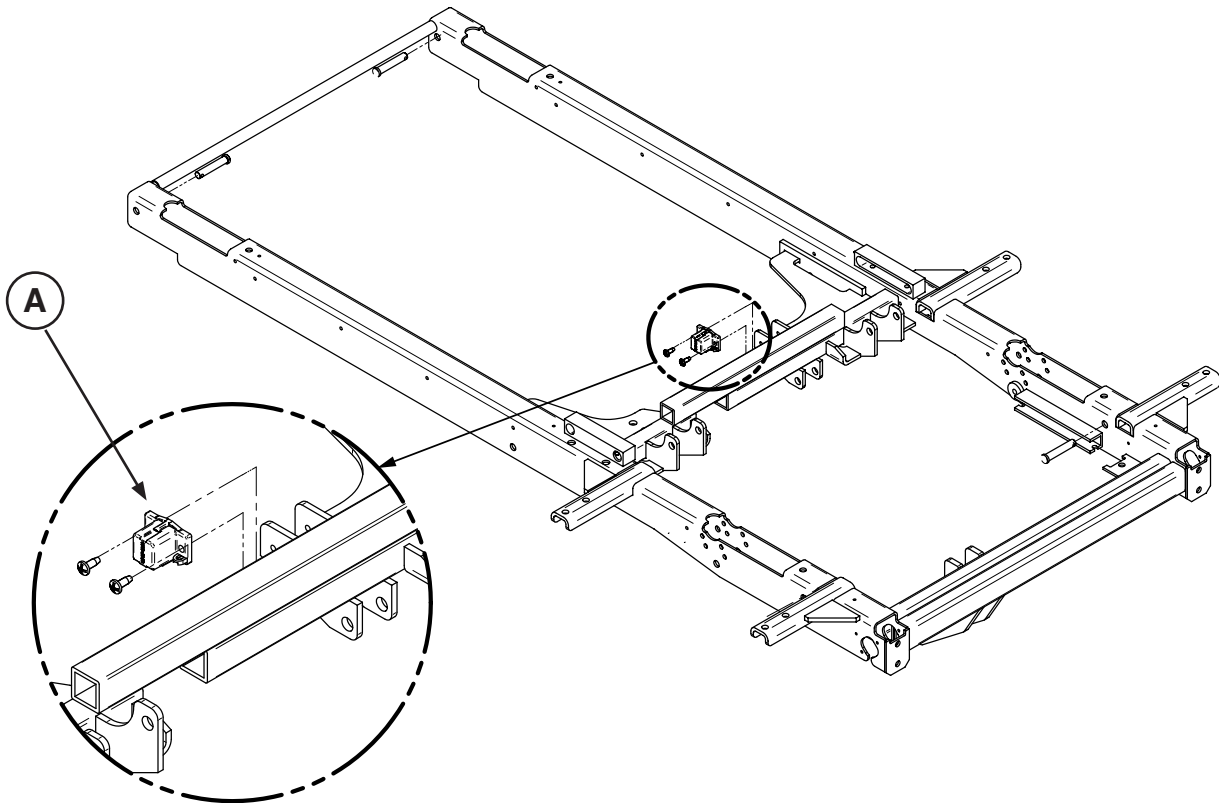

Item	Recycling/Material Code	Important Information	Qty
A	(27-1209) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U01001 - U02817	1
A	(27-2477) Fowler Angle Sensor Assembly	Applies to beds with serial numbers U02818 - Current	1

Recycling Passports


Assembly Part Number: 27-2708 (Reference Only)

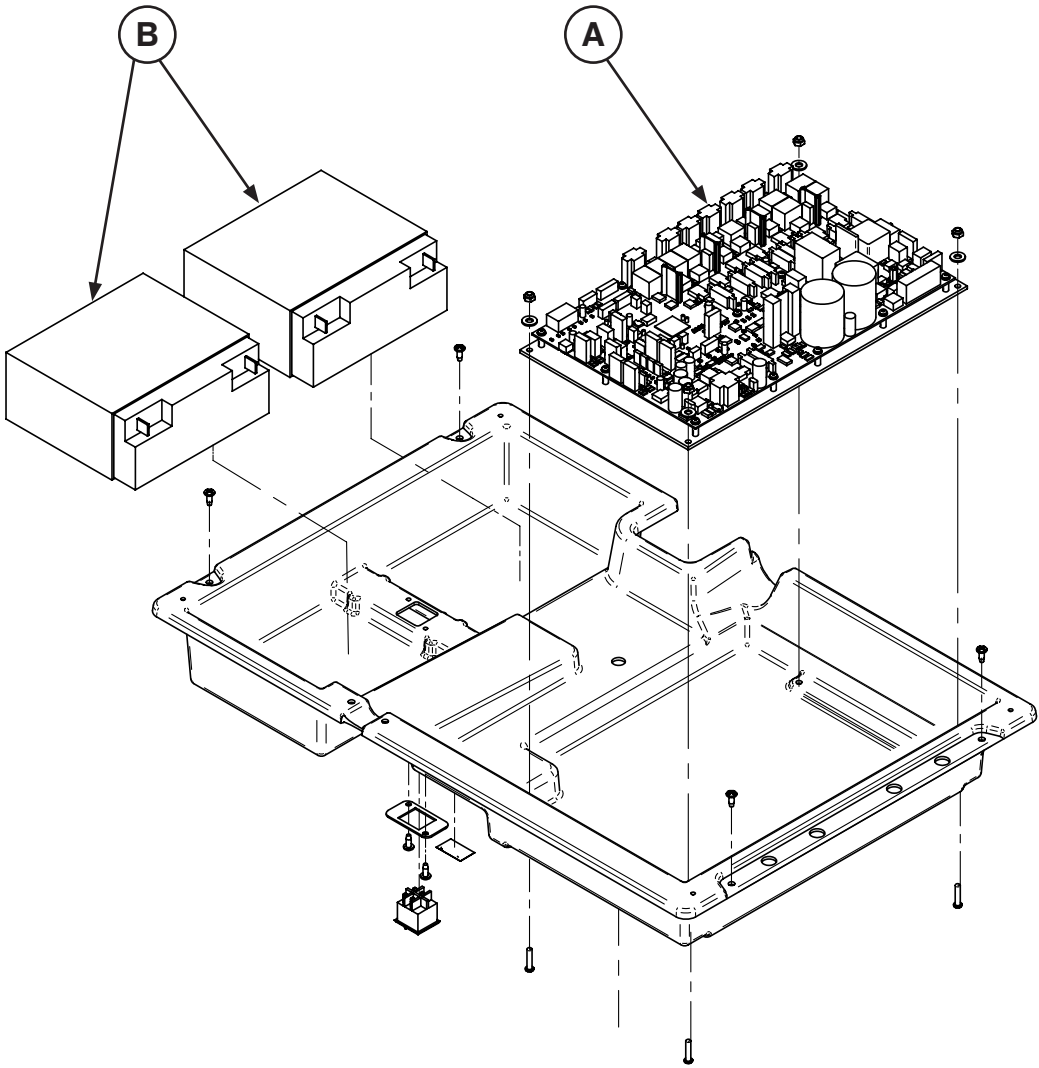

Item	Recycling/Material Code	Important Information	Qty
A	(QDF75-0440) DC Power Control Board		1
B	(QDF9188) 12V 18Ah Battery		2

Recycling Passports


Assembly Part number: 27-2546 (Reference Only)

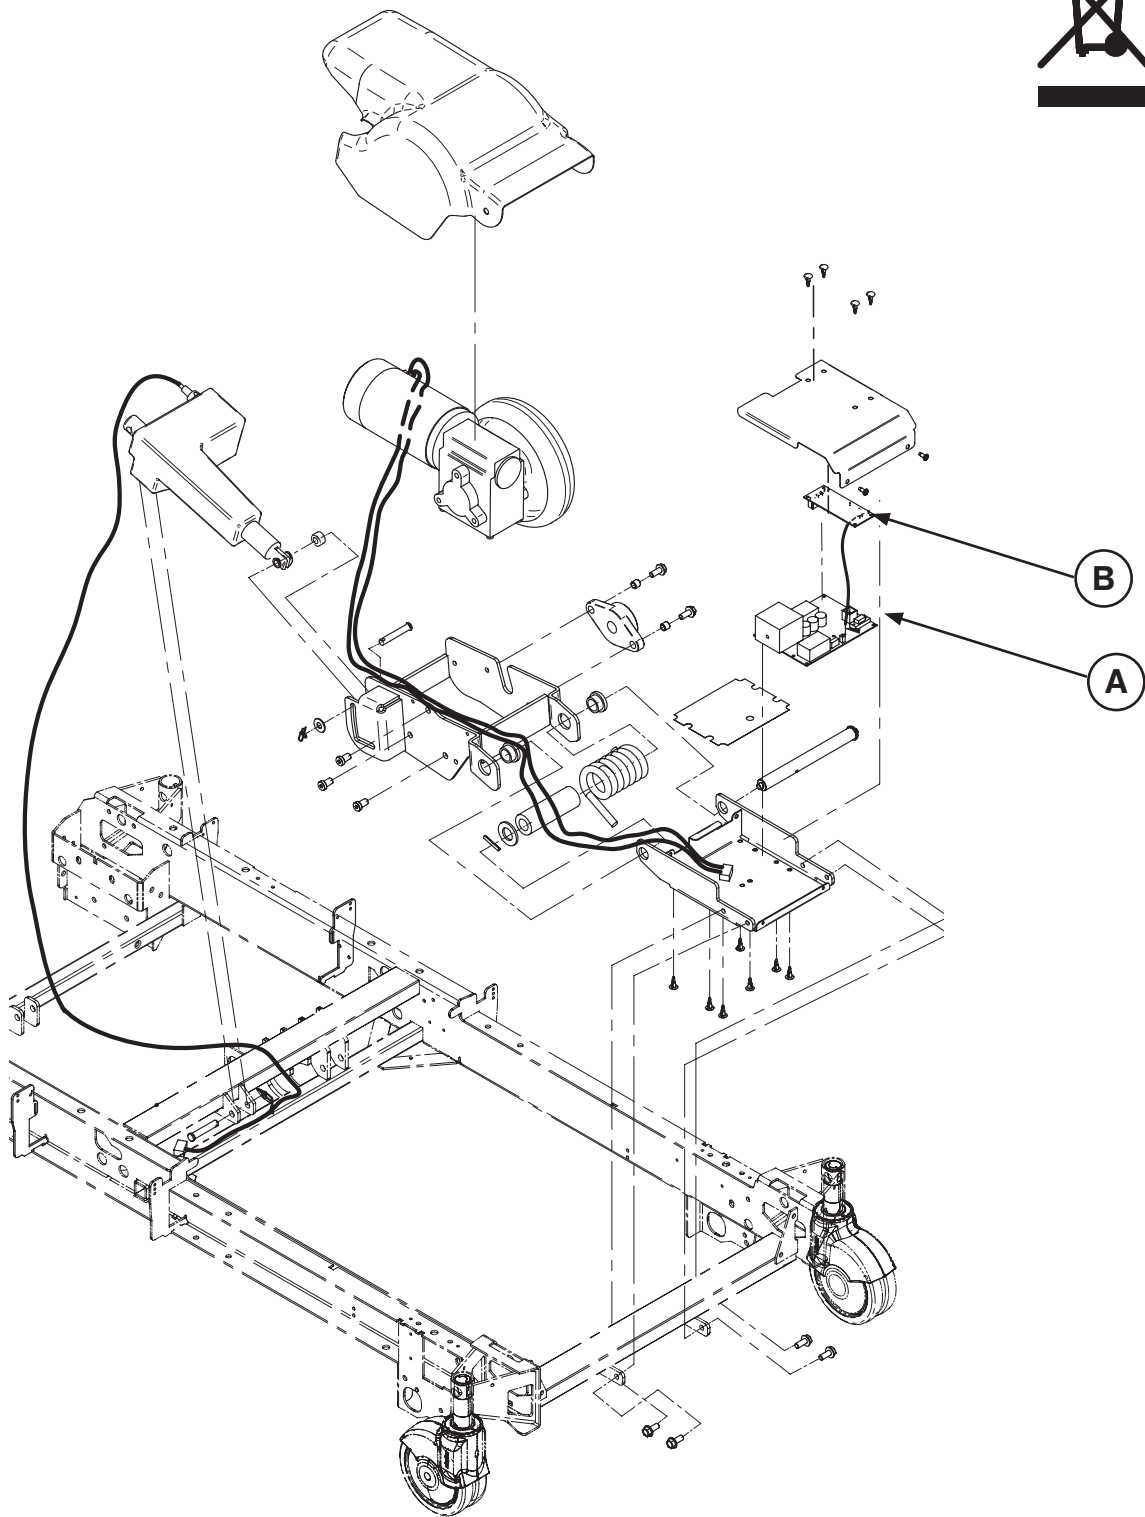

Item	Recycling/Material Code	Important Information	Qty
A	(QDF27-1430) Zoom® Board	Applies to beds with serial numbers U01001 - U03318	1
A	(QDF27-1430) Zoom® Board	Applies to beds with serial numbers U03319 - Current	1
B	(QDF75-0240) Zoom® Interface Board		1

Recycling Passports

Assembly Part number: L27-055 (Reference Only)

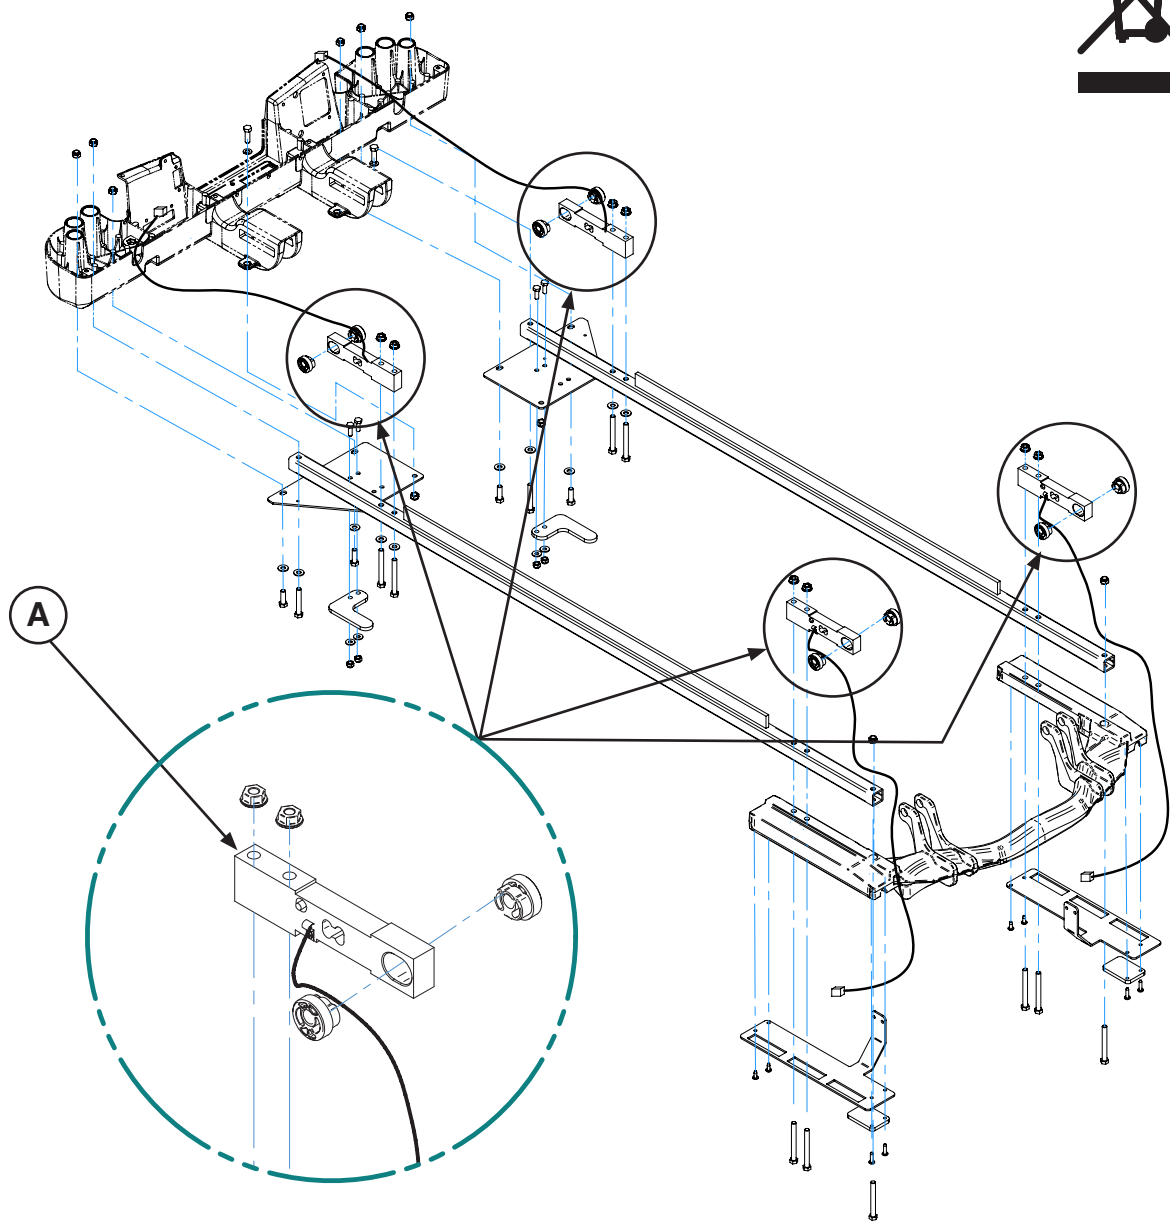

Item	Recycling/Material Code	Important Information	Qty
A	(QDF27-1372) Litter Load Cell		4

Warranty

LIMITED WARRANTY

Stryker Medical Division, a division of Stryker Corporation, warrants to the original purchaser the *InTouch®* Critical Care Bed, Model FL27 (2131/2141) be free from defects in material and workmanship for a period of one (1) years after date of delivery. Stryker's obligation under this warranty is expressly limited to supplying replacement parts and labor for, or replacing, at its option, any product which is, in the sole discretion of Stryker, found to be defective. If requested by Stryker, products or parts for which a warranty claim is made shall be returned prepaid to the factory. Any improper use or any alteration or repair by others in such manner as in Stryker's judgment affects the product materially and adversely shall void this warranty. Any repair of Stryker products using parts not provided or authorized by Stryker shall void this warranty. No employee or representative of Stryker is authorized to change this warranty in any way.

Stryker Medical bed products are designed for a 10 year expected service life under normal use, conditions, and with appropriate periodic maintenance as described in the maintenance manual for each device. Stryker warrants to the original purchaser that the welds on its bed products will be free from structural defects for the expected 10 year life of the bed product as long as the original purchaser owns the product.

This statement constitutes Stryker's entire warranty with respect to the aforesaid equipment. **Stryker makes no other warranty or representation, either expressed or implied, except as set forth herein. There is no warranty of merchantability and there are no warranties of fitness for any particular purpose. In no event shall Stryker be liable here under for incidental or consequential damages arising from or in any manner related to sales or use of any such equipment.**

TO OBTAIN PARTS AND SERVICE

Stryker products are supported by a nationwide network of dedicated Stryker Field Service Representatives. These representatives are factory trained, available locally, and carry a substantial spare parts inventory to minimize repair time. Simply call your local representative, or call Stryker Customer Service USA at 1-800-327-0770, Canada 1-888-233-6888.

SERVICE CONTRACT COVERAGE

Stryker has developed a comprehensive program of service contract options designed to keep your equipment operating at peak performance at the same time it eliminates unexpected costs. We recommend that these programs be activated before the expiration of the new product warranty to eliminate the potential of additional equipment upgrade charges.

A Service Contract helps to:

- Ensure equipment reliability
- Stabilize maintenance budgets
- Diminish downtime
- Establish documentation for JCAHO
- Increase product life
- Enhance trade-in value
- Address risk management and safety

Stryker Medical also offers personalized service contracts.
Pricing is determined by age, location, model and condition of product.

**For more information on our service contracts,
please call your local representative.**

Warranty

RETURN AUTHORIZATION

Merchandise cannot be returned without approval from the Stryker Customer Service Department. An authorization number will be provided which must be printed on the returned merchandise. Stryker reserves the right to charge shipping and restocking fees on returned items. **Special, modified, or discontinued items not subject to return.**

DAMAGED MERCHANDISE

ICC Regulations require that claims for damaged merchandise must be made with the carrier within fifteen (15) days of receipt of merchandise. **Do not accept damaged shipments unless such damage is noted on the delivery receipt at the time of receipt.** Upon prompt notification, Stryker will file a freight claim with the appropriate carrier for damages incurred. Claim will be limited in amount to the actual replacement cost. In the event that this information is not received by Stryker within the fifteen (15) day period following the delivery of the merchandise, or the damage was not noted on the delivery receipt at the time of receipt, the customer will be responsible for payment of the original invoice in full. Claims for any short shipment must be made within thirty (30) days of invoice.

INTERNATIONAL WARRANTY CLAUSE

This warranty reflects U.S. domestic policy. Warranty outside the U.S. may vary by country. Please contact your local Stryker Medical representative for additional information.



Manufactured For
Stryker Medical
3800 E. Centre Ave.
Portage, Michigan 49002
USA

stryker[®]